


BM70659 installation manual

Jun 17, 2011

CANON INC.

Medical Equipment Design Group

The Image for installation of BM70659 Module

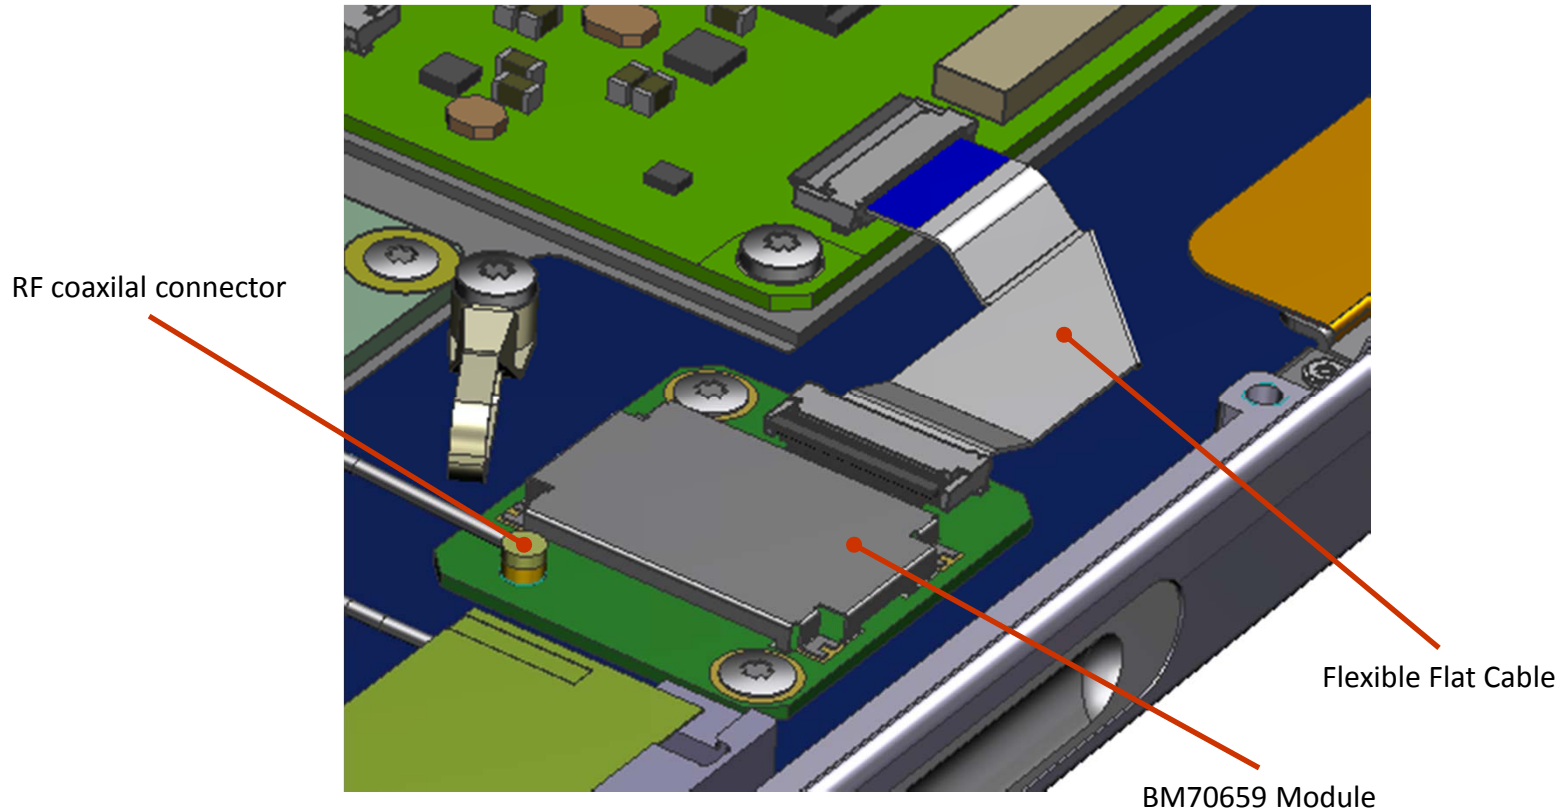

Installed inside Digital Radiography

■ Power Supply Voltage

Power supply voltage of BM70659 Module is $3.5V \pm 10\%$.

The end product must supply the power supply mentioned above.

■ **For U.S.A. and Canada**

The following sentences are added to the label of end product.

“Contains FCC ID: AZDBM70659, IC: 498J-BM70659 “

The following sentences are added to the users manual of end product in English and French.

- (1) This transmitter must not be co-located or operated in conjunction with any other antenna or transmitter.
- (2) The available scientific evidence does not show that any health problems are associated with using low power wireless devices. There is no proof, however, that these low power wireless devices are absolutely safe. Low power Wireless devices emit low levels of radio frequency energy (RF) in the microwave range while being used. Whereas high levels of RF can produce health effects (by heating tissue), exposure of low-level RF that does not produce heating effects causes no known adverse health effects. Many studies of low-level RF exposures have not found any biological effects. Some studies have suggested that some biological effects might occur, but such findings have not been confirmed by additional research.

XXXXX* has been tested and found to comply with FCC/IC radiation exposure limits set forth for an uncontrolled environment and meets the FCC radio frequency (RF) Exposure Guidelines in Supplement C to OET65 and RSS-102 of the IC radio frequency (RF) Exposure rules.

*XXXXX is the model name of the end product.

- (3) 5.15-5.25GHz band is restricted to indoor operations only.