LEPU MEDICAL

AlView Series Patient Monitor

Operator's Manual

I Preface

Copyright

This manual contains proprietary information protected by copyright law. All rights reserved. Without the prior written consent of the manufacturer, no part of this manual shall be copied or reproduced in any form or by any means.

Manual Purpose

The instructions for safe operation of the product in keeping with its function and intended use are contained in this manual. In order to operate the product properly, and protect patient and operator from injury, compliance with this manual is first priority.

This manual is based on the maximum configuration and therefore some contents may not apply to your product. Please keep in touch with the manufacturer or your local distributor if you have any questions.

As an indispensable portion of the product, this manual should always be placed near the device so that it can be got easily when needed.

Intended Audience

This manual applies to clinical professionals with knowledge of medical procedures, practices and terminology as required for monitoring of critically ill patients.

Only clinical professionals, anyone who are under their guidance or people who have been trained adequately can use this monitor. The unauthorized or the untrained are forbidden to operate the product.

About this Manual

P/N: 3502-2530019

Release Date: October 2021

Revision: V1.2

Software Version: V1
Contact Information

Manufacturer: Shenzhen Creative Industry Co., Ltd.

Address: Floor 5, BLD 9, BaiWangXin High-Tech Industrial

Park, Songbai Road, Xili Street, Nanshan District,

518110 Shenzhen, PEOPLE'S REPUBLIC OF

CHINA

Website: www.creative-sz.com F-mail· info@creative-sz.com Tel: +86 755 26431658 Fax: +86 755 26430930

EC Shanghai International Holding Corp. GmbH

Representative: (Europe)

Address: Eiffestrasse 80, 20537 Hamburg Germany

UK Responsible

Etheria Medical Ltd Person

The Old Brush Factory Unit 2d Whickham

Address: Industrial Estate, Swalwell, Newcastle Upon Tyne,

United Kingdom, NE16 3DA

Tel: +44-191-4889922 Fax: +44-191-4889922

E-mail: EtheriaMedicalLtd@outlook.com

Manual Conventions Ш

Illustrations

Setup or data displayed on your monitor may not be necessarily showed in all illustrations in this manual, because they are used only as examples.

All names mentioned in this manual and illustrations are fictitious. Any similarity is purely coincidental.

General Notes

- Italic text is used to indicate prompt information or quote the referenced chapters or sections.
- [XX] is used to indicate the character string in the software.
- → is used to indicate operational procedures.

Special Notes

The warnings, cautions and notes in this manual are used to remind readers of some specific information.



Indicates a potential hazard or unsafe practice that, if not avoided, could result in death or serious injury.



① Caution

Indicates a potential hazard or unsafe practice that, if not avoided, could result in minor personal injury or product/property damage.



Provides application tips or other useful information to ensure that you get the most from your product.

This page intentionally left blank.

Table of Contents

Chapter 1 Safety	1-1
1.1 Safety Information	1-1
1.1.1 Warnings	1-1
1.1.2 Cautions	1-4
1.1.3 Notes	1-4
1.2 Device Symbols	1-5
Chapter 2 Product Introduction	2-1
2.1 Product Name and Model	2-1
2.2 Intended Use	2-3
2.3 Contraindication	2-3
2.4 Date of Manufacture and Service Life	2-3
2.5 Function Features	2-3
2.6 Product View	2-4
2.6.1 Front View	2-5
2.6.2 Rear View	2-7
2.6.3 Left View	2-8
2.6.4 Right View	2-9
2.6.5 Bottom View	2-10
Chapter 3 Getting Started	3-1
3.1 Unpacking and Checking	3-1
3.2 Installation Precautions	3-1
3.3 Environment Requirements	3-2
3.4 Connecting to Power Source	3-3
3.4.1 Using AC Power Source	3-3
3.4.2 Using the Battery	3-3
3.5 Turning on the Monitor	3-4
3.6 Checking the Recorder/Printer	3-4
3.7 Operating and Navigating	3-4
3.7.1 Using the Touchscreen	
3.7.2 Using the On-Screen Keyboard	3-5
3.7.3 Using Keys	3-5
3.8 Screen Views	3-8
3.8.1 Screen Types	3-8
3.8.2 Screen Display	3-8
3.9 Operating Modes	3-10
3.9.1 Monitoring Mode	3-10
3.9.2 Demo Mode	3-10

3.9.3 Night Mode	3-11
3.9.4 Intubation Mode	3-12
3.9.5 Private Mode	3-12
3.9.6 Suspend Monitoring Mode	3-13
3.9.7 Standby Mode	3-14
3.10 Changing Monitor Settings	3-14
3.10.1 Selecting the Language	3-14
3.10.2 Setting the Date and Time	3-15
3.10.3 Enabling Daylight Saving Time	3-15
3.10.4 Adjusting the Screen Brightness	3-15
3.10.5 Adjusting the Volume	3-15
3.11 General Operations	3-16
3.11.1 Configuring the Displayed Quick Keys	3-16
3.11.2 Switching On or Off a Parameter	3-16
3.11.3 Configuring the Normal Screen Layout	3-17
3.11.4 Setting Monitoring Parameters	3-17
3.11.5 Setting the Beat Mode	3-17
3.11.6 Selecting a Screen	3-18
3.11.7 Configuring the Big Numerics Screen	3-18
3.11.8 Changing Parameter Colors	3-18
3.11.9 Setting Password Protection	3-19
3.12 Turning off the Monitor	3-19
Chapter 4 Networked Monitoring	4-1
4.1 Safety Information	4-1
4.2 Remote View	4-1
4.2.1 Opening the Remote View Window	4-2
4.2.2 Setting the Remote View Window	
4.3 Setting the Wired Network	4-2
4.4 Setting the Wireless Network	4-3
4.5 Connecting the CMS	4-3
4.6 Connecting the AI-ECG Server	
Chapter 5 Alarms	5-1
5.1 Safety Information	5-1
5.2 Alarm Categories	
5.3 Alarm Priorities	
5.4 Alarm Mode	
5.5 Alarm Status Symbols	
5 6 Changing Alarm Settings	

5.6.1 Setting Parameter Alarm Properties	5-4
5.6.2 Changing the Alarm Volume	5-5
5.6.3 Setting the Alarm Audio Interval	5-5
5.6.4 Setting the Alarm Audio Pause Time	5-6
5.6.5 Setting the Switch of the Apnea Alarm Off	5-6
5.7 Pausing Alarm Sound	5-6
5.8 Switching Off Alarm Sound	5-7
5.9 Latching Alarms	5-7
5.10 Viewing Alarms	5-8
5.11 Confirming Alarms	5-8
5.12 Reviewing Alarms	5-8
5.13 Resetting Alarms	5-9
5.14 Testing Alarms	5-9
5.15 Processing Alarms	5-9
Chapter 6 Managing Patients	6-1
6.1 Admitting a Patient	6-1
6.2 Quickly Admitting a Patient	6-2
6.3 Editing Patient Information	6-2
6.4 Starting Monitoring a Patient	6-3
6.5 Stopping a Parameter Measurement	
6.6 Discharging a Patient	6-3
6.7 Managing Patient Data	6-4
6.7.1 Querying Patient Data	6-4
6.7.2 Viewing Historical Patient Data	6-4
6.7.3 Importing / Exporting Patient Data	6-4
6.7.4 Deleting Patient Data	6-4
6.8 Configuring Patient Information	6-5
6.9 Managing Operators	6-5
Chapter 7 Monitoring ECG, Arrhythmia, ST, QT/QTc Analysis	7-1
7.1 Introduction	7-1
7.2 Safety Information	7-1
7.3 ECG Monitoring Preparation	7-3
7.3.1 Preparing the Patient Skin	7-3
7.3.2 Connecting ECG Cable and Applying Electrodes.	
7.3.3 ECG Electrode Placement	
7.4 ECG Display	7-9
7.5 Changing ECG Settings	7-10
7.5.1 Setting FCG Menu	7-10

7.5.2 Setting ECG Alarm Properties	. 7-12
7.5.3 Setting ECG Lead Off Alarm Priority	7-12
7.5.4 Setting the ECG Standard	7-12
7.6 About Arrhythmia Monitoring	7-13
7.6.1 Safety Information	7-13
7.6.2 Changing Arrhythmia Alarm Settings	7-14
7.6.3 Setting the Lethal Arrhythmia Alarms Switch	7-14
7.6.4 Changing Arrhythmia Alarm Threshold Settings	7-14
7.6.5 Arrhythmia Analysis Classifications	
7.7 About ST Monitoring	7-17
7.7.1 Safety Information	7-17
7.7.2 Enabling ST Analysis/Display ST Parameters	7-18
7.7.3 Displaying ST Segments in the Waveform Area	
7.7.4 Displaying ISO Point, J Point and ST Point Markers	
7.7.5 Displaying Baseline ST Segments	
7.7.6 Setting ST Alarm Properties	
7.8 About QT/QTc Interval Monitoring	
7.8.1 Enabling QT/QTc Monitoring	
7.8.2 Selecting Leads for QT Calculation	
7.8.3 Selecting the QTc Formula	
7.8.4 Setting QT Alarm Properties	
7.9 Factors Affecting ECG Signal	
Chapter 8 Resting 12-Lead ECG Analysis	8-1
8.1 Entering the 12-Lead Screen	
8.2 Setting the 12-Lead ECG Acquisition	
8.3 Connecting to the AI-ECG Server	
8.4 Initiating 12-Lead ECG Acquisition	
8.5 Reports Management	
Chapter 9 Ambulatory ECG Analysis	
9.1 Connecting to the AI-ECG Server	
9.2 Electrode Placement	
9.3 Initiating Ambulatory ECG Acquisition	
9.4 Reports Management	
Chapter 10 Monitoring Respiration (Resp)	
10.1 Introduction	10-1
10.2 Safety Information	. 10-1
10.3 Resp Monitoring Preparation	10-2
10.3.1 Preparing the Patient Skin	10-2

10.3.2 Placing the Electrodes	10-2
10.4 Resp Display	10-4
10.5 Changing Resp Settings	10-5
10.5.1 Setting Resp Menu	10-5
10.5.2 Setting Resp Alarms	
Chapter 11 Monitoring Pulse Oxygen Saturation (SpO ₂)	
11.1 Introduction	11-1
11.2 Safety Information	11-1
11.3 Measurement Interferences	11-3
11.4 SpO ₂ Display	11-4
11.5 SpO ₂ Monitoring Preparation	11-5
11.6 Changing SpO ₂ Settings	
11.6.1 Setting SpO ₂ Menu	11-8
11.6.2 Changing the SpO ₂ Alarm Settings	11-9
11.6.3 Setting the Priority of the SpO ₂ Sensor Off Alarm.	
11.7 Changing PR Settings	11-9
11.7.1 Changing the PR Alarm Settings	11-9
11.7.2 Setting the PR Source	11-9
Chapter 12 Monitoring Temperature (Temp)	12-1
12.1 Introduction	12-1
12.2 Safety Information	12-1
12.3 Temp Display	12-1
12.4 Temp Monitoring Preparation	12-2
12.5 Changing Temp Settings	12-2
12.5.1 Setting Temp Menu	12-2
12.5.2 Setting Temp Alarms	12-3
Chapter 13 Monitoring Non-Invasive Blood Pressure (NIBP)	13-1
13.1 Introduction	13-1
13.2 Safety Information	
13.3 Measurement Interferences	13-3
13.4 Measurement Modes	13-4
13.5 NIBP Display	13-5
13.6 NIBP Monitoring Preparation	
13.7 Starting and Stopping NIBP Measurements	
13.8 Correcting the NIBP Measurements	
13.9 Changing NIBP Settings	
13.9.1 Setting NIBP Menu	
13.9.2 Setting NIBP Alarm Properties	

13.9.3 Setting NIBP Measurement Timeout	13-10
13.9.4 Displaying NIBP List	13-10
13.10 NIBP Analysis	13-10
13.10.1 Entering the NIBP Analysis Screen	13-10
13.10.2 Setting the NIBP Analysis	13-11
13.10.3 Viewing NIBP Analysis Results	13-11
13.11 Assisting Venous Puncture	13-12
13.12 Factors Affecting NIBP Measurement	13-13
Chapter 14 Monitoring Invasive Blood Pressure (IBP)	14-1
14.1 Introduction	14-1
14.2 Safety Information	14-1
14.3 IBP Display	14-4
14.4 IBP Monitoring Preparation	14-4
14.5 Changing IBP Settings	14-5
14.5.1 Setting IBP Menu	14-5
14.5.2 Setting IBP Alarm Properties	14-7
14.5.3 Setting the Priority of the IBP No Transducer	Alarm14-7
Chapter 15 Monitoring Carbon Dioxide (CO ₂)	15-1
15.1 Introduction	15-1
15.2 Safety Information	15-1
15.3 CO ₂ Display	15-5
15.4 Zeroing the CO ₂ Sensor	15-5
15.5 Connecting CO ₂ Sensor	15-6
15.5.1 Connecting the Sidestream CO ₂ Sensor	15-6
15.5.2 Sidestream Tubing Types	15-7
15.5.3 Connecting the Mainstream CO ₂ Sensor	15-8
15.6 Changing CO ₂ Parameter Settings	15-10
15.6.1 Setting CO ₂ Menu	15-10
15.6.2 Setting CO ₂ Alarm Properties	15-11
15.7 Measurement Limitations	15-11
Chapter 16 Review	16-1
16.1 Review Overview	16-1
16.2 Tabular Trends Review	16-1
16.3 Graphic Trends Review	16-2
16.4 NIBP List Review	
16.5 Events Review	
16.6 Full Disclosure Review	
16.7 ST Review	

	16.8 OxyCRG Review	. 16-5
	16.8.1 Entering the OxyCRG Screen	. 16-5
	16.8.2 Exiting the OxyCRG Screen	. 16-6
	16.8.3 Entering the OxyCRG Review Screen	. 16-6
	16.9 Minitrends Screen	. 16-6
	16.9.1 Entering the Minitrends Screen	. 16-6
	16.9.2 Exiting the Minitrends Screen	. 16-7
	16.10 Screenshot Review	. 16-7
Cha	pter 17 Calculations	. 17-1
	17.1 Introduction	. 17-1
	17.2 Drug Calculations	. 17-1
	17.2.1 Calculation Procedure	
	17.2.2 Checking the Titration Table	
	17.2.3 Drug Calculation Formula	
	17.2.4 Titration Table Calculation Formula	
	17.3 Hemodynamic Calculations	
	17.3.1 Calculation Procedure	
	17.3.2 Input Parameters for Hemodynamic Calculations.	
	17.3.3 Output Parameters and Formulas for Hemodynam	
	Calculations	
	17.4 Oxygenation Calculations	. 17-7
	17.4.1 Calculation Procedure	. 17-7
	17.4.2 Input Parameters for Oxygenation Calculations	. 17-9
	17.4.3 Output Parameters and Formulas for Oxygenation	1
	Calculations	17-10
	17.5 Ventilation Calculations	17-11
	17.5.1 Calculation Procedure	17-11
	17.5.2 Input Parameters for Ventilation Calculations	17-13
	17.5.3 Output Parameters and Formulas for Ventilation	
	Calculations	
	17.6 Renal Function Calculations	
	17.6.1 Calculation Procedure	
	17.6.2 Input Parameters for Renal Function Calculations	
	17.6.3 Output Parameters and Formulas for Renal Funct	
	Calculations	
	17.7 Early Warning Score (EWS)	
	17.7.1 Scoring Parameters	
	17.7.2 Displaying the EWS Parameter Area	
	17.7.3 Entering the FWS Screen	17-18

17.7.4 Performing EWS Scoring	17-18
17.7.5 Auto Scoring	17-19
17.7.6 EWS Settings	17-19
Chapter 18 Other Functions	18-1
18.1 Freezing Waveforms	18-1
18.1.1 Entering Freeze Screen	18-1
18.1.2 Exiting Freeze Screen	18-1
18.1.3 Reviewing Frozen Waveforms	18-1
18.2 Using the On-Screen Timer	18-1
18.2.1 Displaying the Timer	18-1
18.2.2 Using the Timer	18-2
18.3 Nurse Call	18-2
18.4 Managing Configurations	18-3
18.4.1 Restoring Default Configuration	18-3
18.4.2 Saving Current Settings	18-3
18.4.3 Deleting a Configuration	18-4
18.4.4 Loading a Configuration	18-4
18.4.5 Exporting a Configuration	18-4
18.4.6 Importing a Configuration	18-4
Chapter 19 Recording	19-1
19.1 Recorder	19-1
19.2 Setting up the Recorder	19-1
19.3 Starting Recordings	19-2
19.3.1 Manually Starting Recordings	19-2
19.3.2 Automatic Recordings	19-2
19.4 Stopping Recordings	19-3
19.5 Loading Paper	19-3
19.6 Removing Paper Jam	19-3
19.7 Precautions	19-4
Chapter 20 Printing	20-1
20.1 Supported Printer	20-1
20.2 Setting the Network Printer	20-1
20.3 Starting a Printing Task	20-2
20.3.1 Manual Printing	20-2
20.3.2 Automatic Printing	20-2
20.4 Stopping a Printing Task	20-2
20.5 Configuring Reports	20-2
20.5.1 Configuring ECG Reports	20-2

20.5.2 Configuring Real-time Reports	. 20-3
20.5.3 Configuring Tabular Trends Reports	. 20-4
20.5.4 Configuring Graphic Trends Reports	. 20-4
20.5.5 Configuring Event Reports	. 20-5
20.6 Viewing Printing Status	20-5
Chapter 21 Battery	. 21-1
21.1 Introduction	21-1
21.2 Safety Information	. 21-1
21.3 Installing the Battery	. 21-2
21.4 Battery Indication	. 21-3
21.4.1 Battery Status Indicators	. 21-3
21.4.2 Battery Icons	. 21-3
21.4.3 Battery-related Alarms	. 21-4
21.5 Charging the Battery	. 21-4
21.6 Maintaining the Battery	. 21-4
21.6.1 Battery Optimization	. 21-4
21.6.2 Checking Battery Performance	. 21-5
21.7 Storing the Battery	. 21-5
21.8 Replacing and Recycling the Battery	. 21-6
Chapter 22 Cleaning and Disinfection	. 22-1
22.1 Safety Information	. 22-1
22.2 Recommended Cleaning Agents	. 22-1
22.3 Cleaning	. 22-1
22.4 Disinfection	. 22-2
22.5 Sterilization	. 22-3
22.6 Cleaning the Print Head	. 22-3
22.7 Cleaning, Disinfection and Sterilization of Accessories	. 22-3
Chapter 23 Care and Maintenance	. 23-1
23.1 Safety Information	. 23-1
23.2 Daily Inspection	. 23-2
23.3 Routine Maintenance	23-3
23.4 Battery Maintenance	. 23-4
23.5 ECG Calibration	
23.6 NIBP Maintenance	23-5
23.6.1 NIBP Leakage Test	. 23-5
23.6.2 NIBP Pressure Accuracy Verification	
23.7 CO ₂ Calibration	
23 8 IBP Calibration	23-7

23.9 Storage, Packaging and Transportation	23-8
23.10 Viewing Version Information	23-8
Chapter 24 Troubleshooting	24-1
24.1 Prompt Messages	24-1
24.2 Common Faults	24-7
24.2.1 Display Troubleshooting	24-7
24.2.2 Power Supply Troubleshooting	24-8
24.2.3 Alarm Troubleshooting	24-8
24.2.4 ECG Troubleshooting	24-9
24.2.5 SpO ₂ and NIBP Troubleshooting	24-9
24.2.6 IBP Troubleshooting	24-9
24.2.7 CO ₂ Troubleshooting	24-10
Chapter 25 Accessories	25-1
25.1 ECG Accessories	25-3
25.2 Temp Accessories	25-3
25.3 SpO ₂ Accessories	25-4
25.4 NIBP Accessories	25-4
25.5 CO ₂ Accessories	25-6
25.6 IBP Accessories	25-7
25.7 Other Accessories	25-7
Appendix A Technical Specifications	A-1
A.1 Safety Specifications	A-1
A.2 Environmental Specifications	
A.3 Power Supply Specifications	
A.4 Physical Specifications	
A.5 Signal Outputs Specifications	
A.6 Data Storage	
A.7 Wi-Fi Specifications	
A.8 ECG Specifications	
A.9 Resp Specifications	
A.10 Temp Specifications	
A.11 NIBP Specifications	
A.12 SpO ₂ Specifications	
A.13 PR Specifications	
A.14 CO ₂ Specifications	
A.15 IBP Specifications	
Appendix B Alarm Messages	
B.1 Physiological Alarm Messages	

B.2 Technical Alarm Messages	…B-ઉ
B.3 Nellcor SpO ₂ Alarm Messages	B-3
Appendix C Default Settings	C-1
C.1 Alarm Default Settings	C-1
C.2 System Default Settings	C-6
Appendix D Typical Pressures and CO ₂ Readings at Altitudes	D-1
Appendix E EMC Compliance	E-1

Chapter 1 Safety

1.1 Safety Information

1.1.1 Warnings



⚠ Warning

WARNING for PACEMAKER PATIENTS: Although the pacemaker pulse inhibition function is available in this device, the heart rate meter may continue to count the pacemaker rate during occurrences of cardiac arrest or some arrhythmias. Do not rely entirely upon rate meter ALARMS. Keep pacemaker patients under close surveillance. See this manual for disclosure of the pacemaker pulse rejection capability of this device.



⚠ Warning

Each time the monitor is used, check the alarm limits to ensure that they are appropriate for the patient being monitored.



⚠ Warning

Before putting the system into operation, the operator must verify that the device, connecting cables, and accessories are in correct working order and operating condition.



⚠ Warning

The alarm limit shall be within the measuring range, or it may disable the alarm system. Please refer to the related chapter for alarm limit range.



⚠ Warning

A HAZARD can exist if different alarm presets are used for the same or similar device in a single area.



4 Warning

Do not silence the audible alarm if patient safety may be compromised.



⚠ Warning

The monitor is prohibited from applying to those who have severe hemorrhagic tendency or who are with sickle cell disease for they may develop partial bleeding when this monitor is used to take the blood pressure measurement.

⚠ Warning

Connect only approved equipments to this device. Equipments connected to the device must meet the requirements of the applicable IEC standards (e.g. IEC 60950 safety standards for information technology equipment and IEC 60601-1 safety standards for medical electrical equipment). The system configuration must meet the requirements of the IEC 60601-1 medical electrical systems standard. Any personnel who connect equipments to the device's signal input/output port are responsible for providing evidence that the safety certification of the devices has been performed in accordance to the IEC 60601-1.

⚠ Warning

The device should not be used adjacent to or stacked with other equipment. If adjacent or stacked use is necessary, the device should be observed to verify that it can run normally in the configuration in which it is used.

⚠ Warning

Do not touch the patient or metal parts in contact with the patient during defibrillation. Otherwise serious injury or death could result.

⚠ Warning

This device is used for a single patient at a time.

⚠ Warning

To avoid explosion hazards, do not use the equipment in the presence of oxygen-rich atmospheres, flammable anesthetics, or other flammable agents.

⚠ Warning

Using the device in the environment of flammable anaesthetic agents may be at risk of explosion.

⚠ Warning

Disconnect the monitor and sensors from the patient before MRI scanning. Using them during MRI could cause burns or adversely affect the MRI image or the monitor's accuracy.

⚠ Warning

If you are in doubt about the accuracy of any measurement, firstly check the patient's vital signs by any alternative means, and then make sure the monitor is functioning properly.



The monitor is intended only as an adjunct in patient assessment. It must be used in conjunction with clinical signs and symptoms.



The monitor is defibrillation-proof. Verify that the accessories can function safely and normally, and the monitor is grounded correctly before conducting defibrillation. Operate the device on battery power if the integrity of the protective earth conductor or the protective earthing system in the installation is in doubt.

⚠ Warning

Do not place the device or accessories in any position that might cause it to fall on the patient.

⚠ Warning

All the connecting cables and tubes of the applying parts should be kept away from the patient's neck to prevent any possible suffocation of the patient.

⚠ Warning

Do not allow service or maintenance on the device while being used on a patient.

⚠ Warning

Do not open the device housings. All servicing and future upgrades must be carried out by trained and authorized personnel.

⚠ Warning

To prevent the risk of the short circuit and to ensure the ECG signal quality, the device must be properly grounded.

⚠ Warning

Although biocompatibility tests have been performed on all the applied parts, some exceptional allergic patients may still have anaphylaxis. Do NOT apply to those who have anaphylaxis.

⚠ Warning

Please peruse the relative content about the clinical restrictions and contraindication.



It is recommended that the clinical operator regularly test the device and accessories. The visual and auditory alarm signal can be checked by disconnecting the accessories or by setting it at Demo mode to simulate alarm event.

1.1.2 Cautions



(I) Caution

All the parts of the monitor should NOT be replaced at will, substitution of a component different from that supplied by the manufacturer might result in measurement error. If necessary, please use the components provided by the manufacturer or those that are of the same model and standards as the accessories along with the monitor which are provided by the same factory, otherwise, negative effects concerning safety and biocompatibility etc. may be caused. No modification of this device is allowed.



(I) Caution

The accessories which can be used repeatedly should be cleaned thoroughly before use on another patient. Please refer to the related chapter for maintenance method.



Caution

Do not immerse the monitor or its accessories in liquid to clean.



Caution

Store and use the device in specified environmental condition. The monitor and accessories may not meet the performance specification due to aging, stored or used outside the specified temperature and humidity range.



Caution

If the monitor falls down accidentally or has other functional failures, it cannot be used any more. The safety performance and technical indicators must be tested in detail, and it can be used only after the test results are qualified.

1.1.3 Notes



Note

All combinations of equipment must be in compliance with the standard IEC 60601-1.

Note

The device and accessories must be disposed of in compliance with local regulations at the end of their service lives.

Note

Put the device in a location where it can be easily viewed and operated. Do not locate the device in a place difficult to access the mains plug.

Note

Upon request, the manufacturer may provide necessary circuit diagrams, component part lists, and other technical information to assist qualified service personnel in parts repair.

1.2 Device Symbols

Symbol	Description	Symbol	Description			
4 *	Device or part of CF type with defibrillation proof		VGA connector			
)	VGA output	ψ	USB connector			
\hookrightarrow	Nurse call port	몶	Network port			
业	Synchronous defibrillation analog output port	-₩	Equipotential grounding terminal			
	Manufacturer	3	Date of manufacture			
SN	Serial number	((·•))	Non-ionizing electromagnetic radiation			
\triangle	Caution! Consult accompanying documents	X	Follow WEEE regulations for disposal			
\triangle	General warning sign (Background: yellow; Symbol and line: black)	(3)	Refer to Operator's Manual (Background: blue; Symbol: white)			

Symbol	Description	Symbol	Description
CE 0123	The symbol indicates that the device complies with the European Council Directive 93/42/EEC concerning medical devices.	EC REP	Authorised representative in the European Community
UK RP	UK Responsible Person		

Note

Your device does not necessarily have all of the above symbols.

Note

This manual is printed in Black and White.

This page intentionally left blank.

Chapter 2 Product Introduction

2.1 Product Name and Model

Product Name: Patient Monitor Product Model: See label on device

See the table below for the model differences:

Model	Screen size	ECG 3/5-Lead	ECG 6/10-Lead	HR/ARR Analysis	Resp	NIBP (KRK)	NIBP (SunTech)	Temp	CO ₂	SpO₂/PR (KRK)	SpO ₂ /PR (Nellcor)	IBP	Nurse Call
AIView V10	11.6"	•	0	•	•	•	-	•	•	•	-	•	•
AIView V10	11.6"	•	0	•	•	•	-	•	•	-	•	•	•
AIView V10	11.6"	•	0	•	•	•	-	•	•	•	-	•	•
AIView V10	11.6"	•	0	•	•	-	•	•	•	-	•	•	•
AIView V12	13.3"	•	0	•	•	•	-	•	•	•	-	•	•
AIView V12	13.3"	•	0	•	•	•	-	•	•	-	•	•	•
AIView V12	13.3"	•	0	•	•	•	-	•	•	•	-	•	•
AIView V12	13.3"	•	0	•	•	-	•	•	•	-	•	•	•
AIView PH10	11.6"	•	0	•	•	•	-	•	0	•	-	0	-
AIView PH12	13.3"	•	0	•	•	•	-	•	0	•	-	0	-

2.2 Intended Use

The AlView series patient monitor, hereafter called the monitor, is intended to be used for monitoring, displaying, reviewing, storing, alarming and transferring of multiple physiological parameters including ECG (3-lead, 5-lead, 6-lead and 12-lead (optional), arrhythmia detection, ST segment analysis, QT analysis, HRV analysis, and heart rate (HR)), respiration (Resp), body temperature (Temp), pulse oxygen saturation (SpO₂), pulse rate (PR), non-invasive blood pressure (NIBP), invasive blood pressure (IBP) and end-tidal carbon dioxide (EtCO₂). The monitor also provides acquisition, display, storage and transmission of 12-lead resting ECG signals, as well as the acquisition, storage and transmission of ambulatory ECG signals, and receive analysis results for clinical diagnosis.

The monitor is to be used in medical institutions by qualified clinical professionals or under their guidance. The operators must have received adequate training and be fully competent in the use of the monitor.



The monitor can be configured with different parameters. This manual describes all features and options. The monitor you purchase may not cover all functions described below.

2.3 Contraindication

No contraindication.

2.4 Date of Manufacture and Service Life

The service life of the device is 10 years. Please refer to the label on the device for the date of manufacture.

2.5 Function Features

The monitor has the following features:

- Touchscreen and quick keys operation, easy to operate.
- Convenient patient archive management, able to be connected with hospital management system.
- Multiple display views are available, which can be easily shifted for different monitoring purpose.
- The view can be flexibly configured and the display area is adaptive.

- Lead off detection function, and able to send out an alarm.
- Auto detection of lead types: 3 leads, 5 leads, 6 leads and 12 leads.
- Drug calculation, oxygenation calculation, ventilation calculation, renal function calculation, hemodynamic calculation is available.
- Supports the commonly used clinical tool of early warning score (EWS).
- Waveform freezing.
- Automatic arrhythmia detection and analysis.
- ST segment analysis and real-time display of ST segment value.
- QT/QTc measurements.
- Visual and audible alarm with multiple priorities for physiological and technical alarms.
- Supports multi-language display and multiple input methods.
- Supports large capacity storage.
- Protection against defibrillator discharge, resistance against the interference from electro-surgical unit, and cardiac pacemaker pulse detection and inhibition.
- Be capable of networking with central monitoring system.
- Support 12leads ECG in full screen (optional).
- Supports a variety of operating modes, such as demonstration mode, night mode, standby mode, etc.
- USB data import / export function and application software upgrade are available.

Note


You can customize the module configuration by choosing required modules to meet your own needs. Therefore, your monitor may not have all the monitoring functions and accessories.

2.6 Product View

Note

All illustrations in this manual serve as examples only and may differ from what is actually seen.

2.6.1 Front View

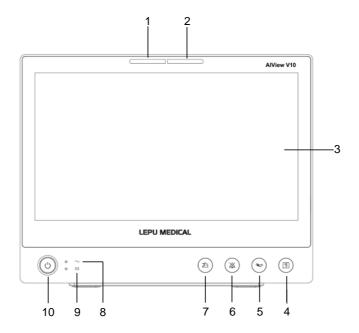

1 Alarm lamp

The alarm lamp is located on the left side of the top of the monitor. When an alarm occurs, this lamp lights and flashes corresponding with the alarm priority:

- High priority alarms: the lamp flashes red.
- · Medium priority alarms: the lamp flashes yellow.
- Low priority alarms: the lamp lights in yellow without flashing.
- 2 Technical alarm lamp

Technical alarm lamp is located on the right side of the top of the monitor. When a technical alarm occurs, this lamp lights and flashes corresponding with the alarm priority:

- · High priority alarms: the lamp flashes red.
- Medium priority alarms: the lamp flashes yellow.
- Low priority alarms: the lamp lights in yellow without flashing.
- 3 Display
- 4 Record Start/Stop hard key

Press to start a recording or stop the current recording.

5 NIBP Start/Stop hard key

Press to start an NIBP measurement or stops the current NIBP measurement.

6 Alarm Tone Pause hard key


Press to pause the current alarm sound.

7 Alarm Reset hard key

Press to acknowledge the on-going alarm.


- 8 Power indicator
- Green: AC power is connected.
- Off: AC power is not connected.
- 9 Battery indicator
- Yellow: AC power is connected and the battery is being charged.
- Green: AC power is connected and the battery is fully charged.
- Off: AC power is connected and no battery is installed.
- Off: the battery is installed and AC power is not connected.
- 10 Power switch / Power-on LED
- Press this switch to turn on the monitor, the backlight is always green.
- When the monitor is on, press and hold this switch to turn off the monitor, and the backlight is not lighted.

2.6.2 Rear View

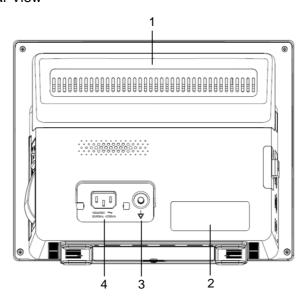

- 1 Handle
- 2 Device label
- 3 Equipotential grounding terminal
- 4 AC power connector

2.6.3 Left View

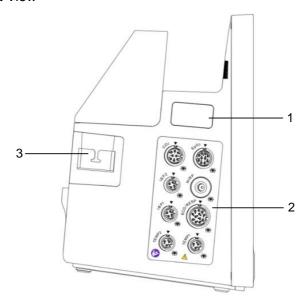


1 Reserved connector of Nellcor SpO₂ module

2 Connector and icon

Module connector	Description		
TEMP1, TEMP2	Temperature probe connector		
NIBP	NIBP cuff connector		
SpO ₂	SpO₂sensor connector		
ECG/RESP	ECG cable connector		
IBP1, IBP2	IBP cable connector		
CO ₂	CO ₂ module connector		

3 CO₂ module holder


2.6.4 Right View

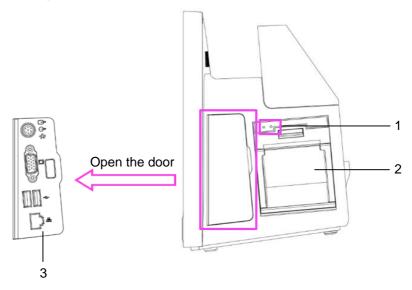

- 1 Recorder indicators
- 2 Recorder (optional)
- 3 Connectors

Connector Icon	Description	Connector Icon	Description		
\hookrightarrow	ECG Analog signal output connector		VGA connector		
\rightarrow	Nurse call connector	÷	USB connector		
小仆	Defibrillator synchronization analog output connector	晶	Network connector		

2.6.5 Bottom View

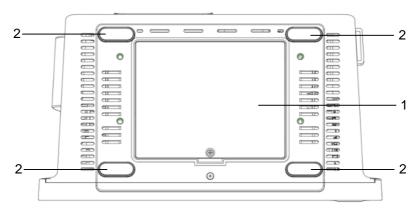

- 1 Battery compartment
- 2 Anti-slip foot pad

This page intentionally left blank.

Chapter 3 Getting Started

3.1 Unpacking and Checking

Before unpacking, examine the packaging carefully for signs of damage. If any damage is found, please contact the carrier immediately.

If the packaging is intact, perform unpacking inspection according to the following steps:

- 1. Open the package, take out the monitor and its accessories from the box carefully.
- 2. Check all materials according to the packing list.
- 3. Check the monitor for any mechanical damages.
- Check all the accessories for scratches or defects.

Please contact your local distributor or the manufacturer in case of any problems. We will offer the best solution for your satisfaction.



When disposing of the packaging materials, be sure to comply with your local waste control regulations or the hospital's waste disposal system.



Keep the packaging materials out of the reach of children.

Caution

Before use, verify whether the packages are intact, especially the packages of single use accessories. In case of any damage, do not apply it to patients.

Note

Save the packing case and packaging material as they can be used if the device must be reshipped.

3.2 Installation Precautions



Devices connected to the monitor must meet the requirements of the applicable IEC standards. The system configuration must meet the requirements of the IEC 60601-1-1 medical electrical systems standard. Any personnel who connect devices to the equipment's signal input/output port are responsible for providing evidence that the safety certification of the devices has been performed in accordance with IEC 60601-1-1. If you

have any question, please contact the manufacturer or your local distributor



⚠ Warning

If it is not evident from the equipment specifications whether a particular combination with other devices is hazardous, for example, due to summation of leakage currents, please consult the manufacturers or an expert in the field, to ensure the necessary safety of patients and all devices concerned will not be impaired by the proposed combination.



Caution

The monitor shall be installed by personnel authorized by manufacturer.



Note

The software copyright of the monitor is solely owned by the manufacturer. No organization or individual shall resort to modifying, copying, or exchanging it or to any other infringement on it in any form or by any means without due permission.

3.3 Environment Requirements

Select a place where the infrastructure and mains supply is well set up. Place the monitor in a safe and stable location where it can easily be viewed and operated.

The operating environment of the device must meet the requirements specified in this manual. Otherwise, unexpected consequences, e.g. damage to the device, could result.

The environment where the monitor is used shall be reasonably free from noise, vibration, dust, corrosive, flammable and explosive substances. If the monitor is installed in a cabinet, sufficient space in front and behind shall be left for convenient operation, maintenance and repair. Moreover, to maintain good ventilation, the monitor shall be at least 2 inches (5cm) away from around the cabinet.

When the monitor is moved from one place to another, condensation may occur as a result of temperature or humidity differences. In this case, never start the system before the condensation evaporates.



Caution

Do not locate the device in a place where the power plug is difficult to plug in and out.

3.4 Connecting to Power Source

3.4.1 Using AC Power Source

Before connecting the monitor to the AC mains, check that the voltage and frequency ratings of the power line are the same as those indicated besides the AC power input connector.

To connect the AC power source, follow the steps below:

- 1. Use the power cable provided with the monitor.
- Insert one end of it to the AC power connector of the monitor and the other end to the three-pin outlet of the power source with protected-earth.
- 3. Connect one end of the grounding wire to the equipotential grounding terminal on the rear panel of the monitor, and the other end to the equipotential system.
- 4. Make sure that the AC power indicator is on to ensure that the AC power supply is connected well.
- If necessary, connect one end of the provided ground wire to equipotential grounding terminal on the rear of the monitor, and connect the other end to one point of the equipotential grounding system.

3.4.2 Using the Battery

The monitor will be powered by the internal battery when the external power is not available. The battery icon will be displayed in the upper right corner of the screen. The monitor can switch between battery power and the external power without interrupting patient monitoring. If both the external power and the battery power are available, the monitor uses the external power in preference to the battery power.

When the battery power is low, the system will alarm for low battery. In this case, the battery can support the monitor to run for about 5 minutes. When the remaining battery power is not enough to support the normal operation of the monitor, the monitor will automatically shut down.



Caution

The provided battery of the monitor must be recharged after transportation or storage. So if the monitor is switched on without being connected to the AC power supply, it may not work properly due to insufficient battery power.

Note

The monitor can be used normally without any performance degradation when the battery is being charged.

Note

It is better to recharge the battery after it has been used up, and the charging time should be 13~15 hours long.

3.5 Turning on the Monitor

Press the power switch on the front panel of the monitor for about 3 seconds, the monitor automatically performs a self-test, then the alarm tone sounds and the alarm lamps illuminate. This indicates that the visible and audible alarm indicators function correctly. Then the monitor jumps from the startup screen to the main screen. This indicates that the monitor is started successfully.

Check all the applicable functions of the monitor to make sure that the monitor works normally.

⚠ Warning

Before each use, check the device for safe and normal operation. Do not use this device to monitor the patient if there are indications of damage or reminders of error. Please contact your local distributor or the manufacturer.

Note

The monitor runs on battery power without interruption when AC power is unavailable.

3.6 Checking the Recorder/Printer

If your monitor is equipped with a recorder, open the recorder's door to check if paper is properly installed. If there is no paper, refer to 19.5 Loading Paper for the method of installing the recording paper. If your monitor is not equipped with a recorder, you can print patient reports through an external network printer. For more information about network printer connection, refer to 20.2 Setting the Network Printer.

3.7 Operating and Navigating

Everything you need to operate the monitor is contained on its screen. Almost every element on the screen is interactive. Screen elements include measurement data, waveforms, quick keys,

information areas, alarms areas and menus. You can access the same element in different ways. For example, you can access a parameter setting menu by selecting the corresponding waveform area, or through the [Parameters] quick key on the main screen.

3.7.1 Using the Touchscreen

You can use the touchscreen to select a screen element by pressing directly on the monitor's screen.

3.7.2 Using the On-Screen Keyboard

You can use the on-screen keyboard to enter information:

- Enter the information by selecting one character after another.
- Select the Backspace key [to delete single characters or select [to delete the entire entry.
- Select the Up key [] to switch between uppercase and lowercase letters.
- Select the Enter key [Enter] to confirm the entry and close the on-screen keyboard.

If the monitor is connected with a physical keyboard, you can also use this keyboard instead of or in combination with the on-screen keyboard.

3.7.3 Using Keys

The monitor has three different types of keys:

Quick keys

A quick key is a configurable graphical key, allowing you to quickly access to some functions.

The quick key area is located at the bottom of the main screen. The [Main Menu] key is fixed at the left, and the [More] key is fixed at the right. Selecting the [More] quick key shows more quick keys. The quick keys displayed on the screen are configurable.

The following table shows available quick keys.

Label	Function	Label	Function
Main Menu	Enters the main menu.	ECG Full-Screen	Enters the ECG full screen.
More	Shows more quick keys.	ECG 12-Lead	Enters the ECG 12-Lead acquisition

Label Function		Label	Function	
			screen, only available when 12-lead function is configured.	
Review	Enter the [Review] screen.	Standby	Enters Standby mode.	
Freeze	Freezes waveforms.	Night Mode	Enters Night Mode / Exits Night Mode.	
Start NIBP	Starts an NIBP measurement or stops the current NIBP measurement.	Private Mode	Enters Private Mode / Exits Private Mode.	
Alarm Audio Paused	Pauses alarm tone.	Intubation Mode	Enters Intubation Mode / Exits Intubation Mode.	
Alarm Reset	larm Reset Acknowledges ongoing alarms and reset the alarm system.		Enters the Pause Monitoring mode / Restarts Monitoring.	
Stop All	Stops all NIBP measurements.	Venipuncture	Enters the NIBP setup screen and select [Venipuncture] to inflate the NIBP cuff to help venous puncture.	
Alarm Setup	Enters the [Alarms] setup screen.	Manual Event	Manually triggers and saves an event.	
Patient Info	Enters the [Patient] management screen.	Screenshot	Captures the current screen.	
Screens	Enters the [Screens] setup screen.		Enters the ambulatory ECG setup screen.	
Parameters	Enters the [Parameters] setup screen.	Volume Enters the [System] setup screen to adjust the volume.		
Calculations	Enters the [Calculations]	Real-time Print	Starts printing a real-time report.	

Label	Function	Label	Function	
	screen.			
Minitrends	Enters the [Minitrends] screen.	Record	Starts/Stops a recording.	
OxyCRG	Opens the [OxyCRG] screen.	EWS	Enters the [EWS] screen.	
Remote View	Opens the [Remote View] screen.	Config	Enters the [Config] screen.	

Note

The selection of quick keys available on your monitor depends on your monitor configuration and on the options purchased.

Hard keys

A hard key is a physical key on the monitor, such as the recording key on the front panel.

Pop-up keys

Pop-up keys are task-related graphical keys that appear automatically on the screen when required. For example, the confirmation pop-up key appears only when you need to confirm a change.

3.8 Screen Views

3.8.1 Screen Types

The monitor provides the following display views:

- Normal screen: meets most monitoring needs.
- Big Numerics screen: displays parameter numerics in big font size for long-distance observation.
- Minitrends screen: displays the recent graphic trends of parameters.
- OxyCRG screen: emphasizes on SpO₂ and Respiration monitoring.
- ECG Half-Screen: ECG half screen displays 7/8 ECG waveforms.
- ECG Full-Screen: ECG full screen displays 7/8 ECG waveforms.
- ECG 12-Lead: ECG full screen 12 lead analysis screen.
- Remote View: on the monitor, you can view the real time parameters and waveforms from patients on other remote monitoring devices networked via the central monitoring network system.



For 3-lead ECG monitoring, you cannot select [ECG Half-Screen], [ECG Full-Screen] and [ECG 12-Lead] screen.



Caution


The [ECG 12-Lead] screen is available only when the lead type is set to 12-lead.



In each screen, the display position and display switch of waveforms and parameters can be customized.

3.8.2 Screen Display

The following figure shows the normal screen:

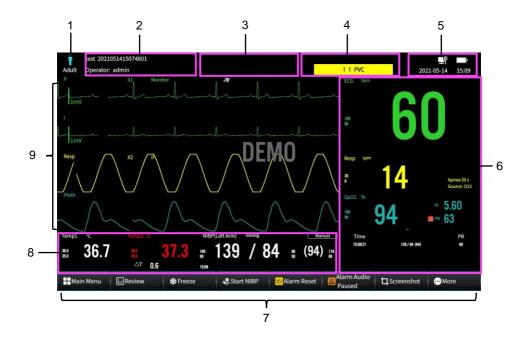

No.	Description
1	Patient type
	Patient information area (top line): displays patient information, including patient name, medical record number, etc. Clicking this area enters the [Patient Info] menu.
2	Operator information area (bottom line): displays operator name. Clicking this area enters the [Operator] menu.
	For more information, see Chapter 6 Managing Patients.
	Prompt information area (top line): displays prompt messages.
3	Technical alarm information area (bottom line): displays technical alarm messages.
4	Physiological alarm message area: displays high priority physiological alarm messages on the above; displays medium and low priority physiological alarm messages at the bottom.
5	System status area: displays network status, battery status and system time.
6	Parameter numerics area: displays parameter values, alarm limits, and alarm status. Clicking a parameter numeric block enters the corresponding parameter menu.
7	Quick key area: displays selected quick keys. The quick keys change with the configuration of the monitor.
8	Parameter waveform/numerics area: displays parameter waveforms, or parameter values, alarm limits, and alarm status.
9	Parameter waveform area: displays parameter waveforms.

3.9 Operating Modes

The monitor provides different operating modes.

3.9.1 Monitoring Mode

Monitoring mode is the most frequently used clinical mode for patient monitoring. When the monitor is turned on, it automatically enters Monitoring mode, which shows real time waveform and data.

3.9.2 Demo Mode

Demo mode is only used for demonstration purpose and detection of alarm function. The data and waveform in demo mode are generated by the system, and cannot be used to evaluate the physiological condition of patients.

To change the operating mode into the demo mode, follow the steps below.

- Click [Main Menu]→[Screens]→[Work Mode]. 1.
- 2 Select [Demo Mode], and then enter the password 123456.

To exit the demo mode, follow the steps below:

- 1. Click [Main Menu]→[Screens]→[Work Mode].
- 2. Select [Exit Demo Mode].



The demonstration function is mainly used to show the performance of the device and to train personnel. In clinical use, do not set the device to Demo mode, to avoid stimulated data being mistaken for a monitored patient's data, which may cause improper monitoring and delayed treatment.

3.9.3 Night Mode

The night mode is a special clinical monitoring mode. In the night mode, the brightness of the alarm lamp, the alarm volume, QRS volume and key volume of the monitor automatically decrease.

To avoid disturbing the patient, you can use the night mode.

To enter the night mode, follow the steps below:

- 1. Click [Main Menu]→[Screens]→[Work Mode].
- Select [Night Mode]. 2

After entering the night mode, the screen displays "Night Mode".

To exit the night mode, follow the steps below:

- Click [Main Menu]→[Screens]→[Work Mode]. 1.
- 2. Select [Exit Night Mode].



(Caution

If your monitor is connected to a central monitoring system (CMS), it automatically exits the Night Mode when it is disconnected from the CMS.



(T) Caution

Verify Night mode settings before entering Night mode. Pay attention to the potential risk if the setting value is low.

Note

The monitor resumes the previous settings after exiting Night mode.

3.9.4 Intubation Mode

Intubation mode is available for Resp and CO2 monitoring. The intubation mode is a special clinical monitoring mode.

The monitor has the following features after entering Intubation Mode:

- The physiological alarms related to Resp and CO₂ are blocked.
- The intubation mode symbol, intubation mode text and countdown are displayed with a red background in the physiological alarm information area.
- The alarm off symbol is displayed in the parameter area.

To enter the Intubation Mode, follow the steps below:

- 1. Click [Main Menu]→[Screens]→[Work Mode].
- Select [Intubation Mode].

The intubation time can be set to 1 min, 2 min, 3 min, 5 min, and the default is 2 min.

After the countdown, the monitor automatically exits the intubation mode. The physiological alarm is activated immediately after exiting the intubation mode.

To exit intubation mode manually, follow the steps below:

- 1. Click [Main Menu]→[Screens]→[Work Mode].
- 2. Select [Exit Intubation Mode].

3.9.5 Private Mode

Private mode is a special clinical monitoring mode. Private mode can be used when the patient information should be protected from visitors and other non-clinical personnel. In the private mode, the monitor does not display patient information and monitoring data. This provides controlled access to patient data and ensures confidentiality.

Private mode is only available when the monitor is connected with the CMS and the patient is admitted by the CMS. In the private mode, the monitor still monitors the patient, but the monitoring data is only displayed on the CMS.

To enter the Private Mode, follow the steps below:

- Click [Main Menu]→[Screens]→[Work Mode].
- 2. Select [Private Mode].

The monitor has the following features after entering Private Mode:

- No parameters and waveforms are displayed. The screen turns blank.
- Except for the low battery alarm, the monitor inactivates alarm tones and alarm lights for all other alarms.
- All system sounds, including heart beat tone, pulse tone and prompt tone, are muted.
- Monitoring data and alarms are presented only at the CMS.

The monitor automatically exits the private mode in any of the following situations:

- The monitor disconnects from the CMS.
- The low battery alarm occurs.



In Private mode, all audible alarms are suppressed and the alarm light is deactivated at the monitor. Alarms are presented only at the CMS. Please pay attention to the potential risks.



Caution

You cannot enter the private mode if a low battery alarm occurs.

3.9.6 Suspend Monitoring Mode

If you just want to stop monitoring temporarily, you can set the monitor to suspend monitoring.

To enter the Suspend Monitoring, follow the steps below:

- 1. Click [Main Menu]→[Screens]→[Work Mode]
- 2. Select [Suspend Monitoring].
- A confirmation dialog box "Are you sure you want to enter Suspend Monitoring mode?" pops up. Click [OK] to enter the suspend monitoring mode, and click [Cancel] to stay in the current screen.

The monitor has the following features after entering Suspend Monitoring mode:

- The screen displays "Suspend Monitoring".
- · All alarms are automatically reset, and no new alarms occur.
- Patient information and alarm presets remain unchanged.

Click the [Restart monitoring] button on the screen to exit the suspend monitoring mode.



In Suspend Monitoring mode, the monitor will pause patient monitoring and suppress all system sounds and alarms except for the battery low alarm. Please pay attention to the potential risks.

3.9.7 Standby Mode

You can temporarily stop patient monitoring without switching off the monitor by entering the standby mode.

To enter the Standby Mode, follow the steps below:

- 1. Click [Main Menu]→[Screens]→[Work Mode]
- 2. Select [Standby Mode].
- 3. A confirmation dialog box "Are you sure you want to enter Standby mode?" pops up. Click [OK] to enter the standby mode, and click [Cancel] to stay in the current screen.

After entering the standby mode, the screen displays the current date and time, and displays the word "Standby".

The monitor has the following features after entering Standby mode:

- The screen displays the word "Standby" and displays the current date and time.
- Stops all parameter measurements, data storage, recording, printing and network response.
- Disables all the alarms and prompt messages, except for the battery low alarm.
- After entering Standby mode for 30 seconds, the screen brightness will be automatically adjusted to the dimmest.

Click the [Exit] button on the screen to exit the standby mode.

⚠ Warning

In Standby mode, the monitor stops patient monitoring and suppress all system sounds and alarms except for the battery low alarm. Please pay attention to the potential risks.

3.10 Changing Monitor Settings

3.10.1 Selecting the Language

To set the user interface (UI) language, follow the steps below:

- 1. Press [Main Menu]→[System]→[System].
- 2. Select [Language] to open the language list.
- 3. Select the desired language from the list.

Note

To make the language change valid, please restart the monitor.

3.10.2 Setting the Date and Time

To set the system date and time, follow the steps below:

- Press [Main Menu]→[System]→[System].
- Set [Date Format]. Options: YYYY-MM-DD, DD-MM-YYYY, MM-DD-YYYY.
- 3. Set [Time Mode]. Options: 12 hours, 24 hours.
- 4. Set the current [Date] and [Time].

⚠ Warning

Changing the date and time affects the storage of trends and events and may result in loss of data.

Note

If the monitor is connected to a central monitoring system (CMS) or hospital Information system (HIS), the date and time are automatically taken from the CMS. In this case, you cannot change the date and time on the monitor.

3.10.3 Enabling Daylight Saving Time

The daylight saving time is disabled by default. You need to manually enable the daylight saving time. To do so, follow the steps below:

- Press[Main Menu]→ [Maintenance] → input password → press [Enter].
- 2. Select the [Time] tab.
- 3. Switch on [Summer Time].
- 4. Adjust daylight saving time settings as necessary.

3.10.4 Adjusting the Screen Brightness

To adjust the screen brightness, follow the steps below:

- 1. Press [Main Menu]→[System]→[System] to enter the system setup screen.
- Drag the slider to set the [Brightness].

Its setting range is "1~10", gradually brightened.

3.10.5 Adjusting the Volume

To adjust the keystroke sound and the touch-screen sound, the alarm volume and the beat volume, follow the steps below:

- Press [Main Menu]→[System]→[System] to enter the system setup screen.
- 2. Drag the slider to set [Key Volume], [Alarm Volume] and [Beat Volume] respectively.

The volume is gradually increasing.



Caution

When the volume is set to 0, the sound is turned off. It is not recommended to set the alarm volume and beat volume to 0 (Off). Pay attention to potential risks.

3.11 General Operations

3.11.1 Configuring the Displayed Quick Keys

You can set which quick keys need to be displayed on the screen. To do so, please refer to the following steps:

- 1. Access [Quick Keys] screen in either of the following ways:
 - Press the [Screens] quick key → select the [Quick Keys] tab.
 - Press [Main Menu] → [Screens], select the [Quick Keys] tab.
- 2. Select a block location to display a certain quick key from the top of this screen, and then select the quick key from the quick key list. For example, to display the [Screens] quick key at the first block, select the first block, and then select [Screens] from the list
- 3. Configure all the quick keys that need to be displayed on the screen in the same way.

3.11.2 Switching On or Off a Parameter

You can manually switch on or off a parameter when its module is configured. To do so, please refer to the following steps:

- Access [Parameters On/Off] screen in either of the following ways:
 - Press the [Screens] quick key → select the [Parameters On/Off] tab.
 - Press [Main Menu] → [Screens], select the [Parameters On/Off] tab.
- 2. Enable or disable desired parameters.

When a parameter is switched off, no measurements and alarms are provided.

3.11.3 Configuring the Normal Screen Layout

You can configure the parameter numerics, waveforms, and their sequence displayed on the normal screen. To do so, please refer to the following steps:

- Access [Layout] screen in either of the following ways:
 - Press the [Screens] quick key → select the [Layout] tab.
 - Press[Main Menu]→[Screens], select the [Layout] tab.
- 2. Select a parameter area and select an element to be displayed in this area from the pop-up list. The parameters and waveforms not selected will not be displayed on the screen.



ECG parameters and the first ECG waveform are always displayed on the first line of the parameter area and waveform area.



Turn off all other parameters except ECG parameter, then the screen can display an ECG signal within a vertical space of 30mm per ECG channel.

3.11.4 Setting Monitoring Parameters

Each parameter has its own setup menu to allow adjusting of the alarm and parameter settings.

Access [Parameters] screen in either of the following ways:

- Select the parameter numeric area of a parameter.
- Press the [Parameters] quick key.
- Press [Main Menu]→[Parameters].

Select the desired parameter. For details of each parameter setting, please refer to the respective parameter setup menu description in corresponding parameter measurement chapters.

3.11.5 Setting the Beat Mode

To set the beat mode, follow the steps below:

- Press [Main Menu]→[System]→[System] to enter the system setup screen.
- 2. Set the [Beat] mode. Options: Mode 1, Mode 2.

The frequency of heart beat in the two modes is different, so it is convenient for users to distinguish.

3.11.6 Selecting a Screen

The monitor enters the normal screen after it is powered on. The normal screen is most frequently used for patient monitoring.

To select other screens, please refer to the following steps:

- Access [Screen Selection] screen in either of the following ways:
 - Press the [Screens] quick key → select the [Screen Selection] tab.
 - Press[Main Menu]→[Screens], select the [Screen Selection] tab.
- 2. Select the desired screen.

3.11.7 Configuring the Big Numerics Screen

To configure the big numerics screen, please refer to the following steps:

- Access [Screen Selection] screen in either of the following ways:
 - Press the [Screens] quick key → select the [Screen Selection] tab.
 - Press[Main Menu]→[Screens], select the [Screen Selection] tab.
- 2. Select the [Big Numerics] option.
- 3. Select the [Big Numerics] tab.
- 4. Select a parameter numeric area or waveform area, and then select an element to be displayed in this area from the popup list.

3.11.8 Changing Parameter Colors

To set the color of measurement values and waveforms for each parameter, please refer to the following steps:

- Access [Parameters On/Off] screen in either of the following ways:
 - Press the [Parameters] quick key.
 - Press[Main Menu]→[Parameters].
- 2. Select the [Parameter Color] tab and set the colors of measurement values and waveforms for desired parameters.

3.11.9 Setting Password Protection

You can set whether changing alarm-related settings is password protected or not. To do so, follow the steps below:

- Press [Main Menu] → [Maintenance] → input password → press [Enter].
- 2. Select the [Alarm] tab.
- 3. Switch on or off [Alarm Setup Password] as needed.
 - If [Alarm Setup Password] is switched on, changing the alarm switch, alarm high and low limits, alarm priorities and alarm volume settings are password protected. The password is the user maintenance password (i.e., admin password) of the monitor.
 - If [Alarm Setup Password] is switched off, changing the alarm settings is not password protected.

3.12 Turning off the Monitor

To turn off the monitor, follow the steps below:

- 1. Confirm that patient monitoring has been completed.
- 2. Disconnect the cables and sensors from the patient.
- 3. Save or clear the patient data as required.
- 4. Press and hold the power switch for 3 seconds to turn off the monitor



Caution

Although not recommended, you can press and hold the power switch for 10 seconds to forcibly shut down the monitor when it cannot be shut down normally. However, this operation may cause loss or corruption of patient data, please proceed with caution.



Turning off the monitor does not disconnect the monitor from the AC mains. To completely disconnect the power supply, unplug the power cord.

Note

If the monitor is equipped with a rechargeable battery, charge the battery after using the monitor every time to ensure that there is sufficient electric power.

This page intentionally left blank.

Chapter 4 Networked Monitoring

You can connect the monitor to the central monitoring system (CMS), and AI-ECG server through wired or wireless network. If the monitor is networked, a network symbol is displayed on the screen.

4.1 Safety Information



Keep network authentication information, for example passwords, safe, to protect the network from being accessed by unauthorized users.

⚠ Warning

Do not connect non-medical devices to the monitor network.

⚠ Warning

Always set the wireless network according to local wireless regulations.

⚠ Warning

If wireless network signal is poor, there may be a risk of data loss in communicating with CMS.

⚠ Warning

RF interference may result in wireless network disconnection.

⚠ Warning

Disconnecting from the network may result in CMS-destined data loss and function failure. Check the patient in case of network disconnection and solve the network problem as soon as possible.

⚠ Warning

Ensure that the monitor IP address setting is correct. Changing the network settings may result in network disconnection. Contact your service personnel if there are any problems with the IP address.

4.2 Remote View

In the [Remote View] window, you can view real time waveforms, numeric information of all parameters and alarm information of the selected bed on the same network.

Caution

The IP addresses of the monitors configured with the remote view function should share the same network segment. The IP addresses of the monitors on the same LAN should be unique from each other; you cannot use the remote view function in the monitors in which an IP address conflict exits.

Caution

To have good remote monitoring, make sure the network connection is in good condition.

4.2.1 Opening the Remote View Window

Before opening the Remote View window, make sure the remote view function is configured on your monitor.

Enter the Remote View window in either of the following ways:

- Press the Remote View quick key.
- Press the [Screens] quick key → select [Remote View].
- Press [Main Menu] → [Screens], select [Remote View].

4.2.2 Setting the Remote View Window

Press the [Setup] button in the lower right corner of the Remote View window to open the Remote View Setup menu on which you can:

- Select the waveform to be viewed on the window in the waveform type list.
- Select the parameter to be viewed in the parameter list.
- Select bed No. of the bed to be viewed in the bed No. list.

4.3 Setting the Wired Network

To set the wired network, follow the steps below:

- 1. Enter the network setup screen in either of the following ways:
 - Press the network status icon in the upper right corner of the screen.
 - Press [Main Menu] → [System], select the [Network] tab.
- 2. Select the [Wired Network] tab.
- 3. Select how to get the IP address.

[Auto Acquire IP]: the monitor obtains the IP address automatically. [Use IP Address below]: you need to input the [IP address], [Subnet Mask] and [Gateway].

4.4 Setting the Wireless Network

To set the wireless network, follow the steps below:

- 1. Enter the network setup screen in either of the following ways:
 - Press the network status icon in the upper right corner of the screen.
 - Press [Main Menu] → [System], select the [Network] tab.
- 2. Select the [Wireless Network] tab.
- 3. Select how to get the IP address.

[Auto Acquire IP]: the monitor obtains the IP address automatically. [Use IP Address below]: you need to input the [IP address], [Subnet Mask] and [Gateway].

4. Press the [Connect] button to test the network connection.

4.5 Connecting the CMS

To set the central monitoring system (CMS), follow the steps below:

- 1. Enter the network setup screen in either of the following ways:
 - Press the network status icon in the upper right corner of the screen.
 - Press [Main Menu] → [System], select the [Network] tab.
- 2. Select the [Central Station] tab.
- 3. Switch on [Central Station].
- 4. Set the IP address and port number of the central station server.

Note

Make sure that CMS and the monitor are located in the same network segment. Every monitor should have its unique port number and IP address. Otherwise, its network connection will be failed anytime.

If your monitor is connected to the CMS:

- All patient information, measurement data and settings on the monitor can be transferred to the CMS.
- All patient information, measurement data and settings can be displayed simultaneously on the monitor and CMS. For some functions such as editing patient information, admitting a patient, discharging a patient, starting/stopping NIBP measurements, etc., bi-directional control can be achieved between your monitor and the CMS.

For more information on the CMS, refer to the Central Monitoring System Operator's Manual.

Note

Make sure the network connection between the monitor and the central monitoring system is in good condition.

4.6 Connecting the AI-ECG Server

To connect the AI-ECG server, follow the steps below:

- 1. Enter the network setup screen in either of the following ways:
 - Press the network status icon in the upper right corner of the screen.
 - Press [Main Menu]→[System], select the [Network] tab.
- 2. Select the [Al-ECG Server] tab.
- 3. Set the IP address and port number of the AI-ECG Server.
- Press the [Test] button to test the connection status of AI-ECG Server.
 - If the connection is successful, the [AI-ECG Server state] displays [Connected].
 - If the connection failed, it displays [Disconnected].

If your monitor is connected to the AI-ECG server of AI-ECG Platform:

- You can send the collected ECG information (including original waveforms, filter settings, etc.) to the AI-ECG server for 12-lead resting ECG analysis and diagnosis.
- Download and print the returned diagnosis reports at the monitor side.

If your monitor is connected to the AI-ECG server of AI-ECG Tracker:

- You can send the collected ECG information (including original waveforms, filter settings, etc.) to the AI-ECG server for single lead / 8-lead / 12-lead ambulatory ECG analysis and diagnosis.
- Download and print the returned diagnosis reports at the monitor side.

Chapter 5 Alarms

Alarms are triggered by physiological parameters that appear abnormal or by technical problems of the monitor. When an alarm occurs, the monitor indicates it through visual and audible alarm indications.

5.1 Safety Information



Before monitoring a new patient, always check that the monitor can work properly, the alarm system works properly, and the alarm settings are appropriate for the patient before starting the monitoring.

1 Warning

In order to ensure that the operator can accurately identify the alarms, it is recommended that the distance between the operator and the monitor should not exceed 4 meters. If the alarm event needs to be clearly distinguished, it is recommended that the distance between the operator and the monitor should not be more than 1 m (there should be no obstacle within the visual effective distance above).

⚠ Warning

Do not set the alarm limits beyond the measurement ranges, which may cause the alarm system to become ineffective.

⚠ Warning

For the same or similar equipment used in any separate area, there is a potential hazard if different alarm presets are used.

Caution

When the alarm system is powered off, or loses all power, the monitor will save the alarm settings and alarm logs if the power off time is not more than 30s. The stored alarm information does not change with the power off time.

Note

The alarm system function of the monitor can be checked and verified in the demo mode.

5.2 Alarm Categories

The monitor provides two different types of alarms: physiological alarms and technical alarms.

- Physiological alarms: also called patient status alarms, are triggered by parameter measurement exceeding the set alarm limits, or by an abnormal patient condition.
- Technical alarms: also called system status alarms, are triggered by a device malfunction or the monitoring result distortion due to improper operation or mechanical problems.

Apart from the physiological and technical alarms, the monitor can also display messages describing the system status or patient status in the prompt message area at the top of the screen.

For alarm events and prompt messages, see *Appendix B Alarm Messages*.

5.3 Alarm Priorities

By severity, the alarms are classified into the following priority levels:

- High priority alarms: indicates a life threatening situation or a severe device malfunction. High priority alarms require an immediate operator response.
- Medium priority alarms: indicates abnormal vital signs or a device malfunction. Medium priority alarms require a timely operator response.
- Low priority alarms: indicate a discomfort condition, a device malfunction, or an improper operation. Low priority alarms require the operator to be aware of this condition.
- Prompt messages: provide additional information of the patient or the monitor.

The monitor has preset alarm priorities for physiological alarm and technical alarm. For more information, see *B.1 Physiological Alarm Messages* and *B.2 Technical Alarm Messages*.

5.4 Alarm Mode

The monitor provides audible and visual alarm indications when an alarm occurs. For more information, see the following table.

Alarm Priority P	Medium Low Priority Priority Alarm Alarm	Prompt Message	Remarks
------------------	--	-------------------	---------

Alarm Indication	High Priority Alarm	Medium Priority Alarm	Low Priority Alarm	Prompt Message	Remarks
Alarm lamp	Red flashing Flashing frequency: 1.4Hz-2.8 Hz, visual duty cycle: 20%-60%	Yellow flashing Flashing frequency : 0.4Hz-0.8 Hz, visual duty cycle: 20%-60%	Yellow No flashing visual duty cycle: 100%	None	None
Tone Characterist ics	Do-Do-D oDo-Do- Do-Do -DoDo- Do	Do-Do-D o	Do	None	None
Alarm message	Black text inside a red box	Black text inside a yellow box	Black text inside a yellow box	White text	Alarm messages are displayed in the alarm informatio n area at the top of the screen. You can select the alarm messages to show the alarm list.
Alarm level symbol	111	!!	!	/	The symbols appear before the correspon ding alarm message.

Alarm Indication	High Priority Alarm	Medium Priority Alarm	Low Priority Alarm	Prompt Message	Remarks
Parameter value	Black text inside a red box	Black text inside a yellow box	Black text inside a yellow box	/	None

(T) Caution

When multiple alarms of different priorities occur simultaneously, the monitor selects the highest priority alarm to light the alarm lamp and issue the alarm tone. When multiple alarms of different priority levels occur simultaneously and should be displayed in the same area, all the alarm messages are displayed cyclically.

Caution

When multiple alarms of the same priority levels occur simultaneously and should be displayed in the same area, all the alarm messages are displayed cyclically.

5.5 Alarm Status Symbols

Apart from the alarm indications as described in 5.4 Alarm Mode, the monitor uses the following symbols to indicate the alarm status:

Alarm off: indicates that the alarm of a parameter is turned off or the system is in the alarm off status.

Alarm audio pause: indicates that audible alarm tones are paused.

Alarm audio off: indicates that audible alarm tones are turned off.

Alarm reset: indicates that alarms are acknowledged and the alarm system is reset. At this time, the audible alarm tones are turned off, but the visual alarm still keeps effective.

5.6 Changing Alarm Settings

5.6.1 Setting Parameter Alarm Properties

The system supports centralized setting of alarm properties for all parameters.

To do so, please refer to the following steps:

- 1. Access [Alarm Limits] screen in either of the following ways:
 - Press the [Alarms] quick key.
 - Press[Main Menu]→[Alarms].
- 2 Select a parameter tab and set alarm properties as desired.

You can also change the alarm properties of individual parameter from the corresponding parameter menu.

Click the [Defaults] button at the bottom of the screen to restore the default alarm settings.

5.6.2 Changing the Alarm Volume

To change the alarm volume, follow the steps below:

- Access [System] screen in either of the following wavs:
 - Click the volume icon in the upper right corner of the screen.
 - Press [Main Menu]→[System]→[System].
- 2. Set [Alarm Volume].

The alarm volume can be set from 0 to 10, the volume increases step by step. In general, the alarm volume ranges from 1-10. The alarm volume can only be set to 0 if the [Alarm Audio Pause Time] is set to [Permanent].



(I) Caution

Do not rely exclusively on the audible alarm system for monitoring. Adjustment of alarm volume to a low level may result in a hazard to the patient. Please pay close attention to the actual clinical condition of patients.



Caution

When adjusting the alarm volume, if it is impossible to ensure that the medical staff are always in the care of the monitor and the patient, it is recommended that the operator should not adjust the volume below the default setting value of the monitor, otherwise, the alarm may not be easily detected and irreversible injury may occur to the patient.

5.6.3 Setting the Alarm Audio Interval

To set the alarm audio interval, follow the steps below:

- Press[Main Menu]→[Maintenance]→ input password → press 1 [Enter].
- 2. Select the [Alarm] tab.

- 3. Set [High Alarm Audio Interval], [Medium Alarm Audio Interval] and [Low Alarm Audio Interval].
 - The setting range of [High Alarm Audio Interval] is 3~15s.
 Default setting is 10s.
 - The setting range of [Medium Alarm Audio Interval] is 3~30s. Default setting is 10s.
 - The setting range of [Low Alarm Audio Interval] is 16~30s.
 Default setting is 10s.

5.6.4 Setting the Alarm Audio Pause Time

To set the alarm audio pause time, follow the steps below:

- Press[Main Menu]→[Maintenance]→ input password → press [Enter].
- 2. Select the [Alarm] tab.
- Set the [Alarm Audio Pause Time].
 The alarm audio pause time can be set to [1min], [2min], [3min] or [Permanent]. Default setting is two minutes.

5.6.5 Setting the Switch of the Apnea Alarm Off

You can choose whether switching off the Apnea alarm is permissible or not.

To do so, please refer to the following steps:

- Press[Main Menu]→[Maintenance]→ input password → press [Enter].
- 2. Select the [Alarm] tab → select the [Other] tab.
- 3. Set the [Apnea Alarm Off].
 - [Disabled] (default setting): the Apnea alarm is always on. You cannot switch it off.
 - [Enabled]: you can switch off the Apnea alarm.



If you switch off the Apnea (zero respiration rate) alarm, the monitor will not issue the Apnea alarm when that situation occurs. This may result in a hazard to the patient. Keep the patient under close surveillance.

5.7 Pausing Alarm Sound

Press the [Alarm Audio Pause] quick key to pause the current alarm sound.

The monitor has the following features after the alarm sound is paused:

- The sound of all physiological alarms and technical alarms are switched off within the set alarm audio pause time.
- The remaining alarm audio pause time is displayed in the physiological alarm information area.
- The alarm audio pause symbol is displayed in the system status information area.

After reaching the alarm audio pause time, the monitor will automatically exit the alarm audio pause status. You can also cancel the alarm audio paused status by pressing the [Alarm Audio Pause] quick key.

5.8 Switching Off Alarm Sound

If [Alarm Audio Pause] is set to [Permanent] (see 5.6.4Setting the Alarm Audio Pause Time), press the [Alarm Audio Pause] quick key to switch off all alarm sound.

The monitor has the following features after the alarm sound is switched off:

- The sound of all physiological alarms and technical alarms are switched off.
- The alarm audio off symbol is displayed in the system status information area

To exit the alarm audio off status, press the [Alarm Audio Pause] quick key.

⚠ Warning

Pausing or switching off alarm sound may result in a hazard to the patient. Please pay attention to the potential risks.

5.9 Latching Alarms

Physiological alarms can be set to "latch" or "non latch" mode.

- Non latch: if you do not latch physiological alarms, their alarm indications disappear when the alarm condition ends.
- Latch: if you latch physiological alarms, all visual and audible alarm indications remains until the alarms are reset.

To latch physiological alarms, follow the steps below:

 Press[Main Menu]→[Maintenance]→ input password → press [Enter].

- 2. Select the [Alarm] tab.
- Switch on the [Physio. Alarm Latch]. 3.

To release the physiological alarm latch, switch off the [Physio. Alarm Latch].



(1) Caution

When the alarm system is reset, latched physiological alarms are cleared.

5.10 Viewing Alarms

You can view the current alarm in the alarm information area at the top of the screen. If the monitor has more than one physiological (technical) alarm, you can see the physiological (technical) alarm list by selecting the physiological (technical) alarm information area to enter the alarm list window. The alarm information list shows all currently active physiological or technical alarms, with the most recent one at the top of the list.

5.11 Confirming Alarms

To confirm alarms, follow the steps below:

- Select the technical or physiological alarm information area to enter the technical or physiological alarm information window.
- Select the check box(s) before one or more alarm messages. 2.
- 3. Press [Alarm Confirm].

The monitor has the following features after the alarm is confirmed:

- The alarm is silenced.
- A symbol appears before the alarm message.
- Technical alarms are changed to the prompt messages.

Press the [X] button on the right side of the confirmed alarm to cancel the confirmation of the alarm.

After canceling the alarm confirmation, the alarm sound is activated and the alarm confirmation symbol disappears.

5.12 Reviewing Alarms

In the technical or physiological alarm information window, press the [Review] button to enter the alarm event review screen. For more information, see Chapter 16 Review.

5.13 Resetting Alarms

Press the alarm reset hard key on the front panel of the monitor, or press the [Alarm Reset] quick key to confirm the ongoing alarms and reset the alarm system. When the alarm system is reset, the alarm

reset symbol displays in the system status information area.

Resetting Physiological Alarms

When the alarm system is reset, the sound of the ongoing physiological alarm (including the latch alarm) is silenced.

Resetting Technical Alarms

For technical alarms, when the alarm system is reset, the following occur:

- Technical alarms that can be completely cleared are cleared.
 For the cleared technical alarm, the monitor gives no alarm indications.
- Technical alarms that can clear sound and light are changed to prompt messages.



Caution

If a new alarm is triggered after the alarm system is reset, the alarm reset symbol will disappear and the alarm light and alarm tone will be reactivated.

Note

Alarm reset is not a toggle operation, pressing the alarm reset key again or several times only reset the current alarm event, rather than exit the alarm reset state.

5.14 Testing Alarms

The monitor automatically performs a self-test at startup. Check that an alarm tone is heard, the alarm indicator illuminates, one after the other, in red and purple. This indicates that the visible and audible alarm indicators functions correctly.

For further testing of individual measurement alarms, perform the measurement on yourself or use a simulator. Adjust alarm limits and check that appropriate alarm behavior is observed.

5.15 Processing Alarms

When the monitor gives an alarm, please refer to the following steps and take proper measures:

- 1. Check the patient's condition.
- 2. Confirm the parameter of the ongoing alarm or alarm category.
- 3. Identify the source of the alarm.
- 4. Take proper action to eliminate the alarm condition.
- 5. Make sure the alarm condition is corrected.

This page intentionally left blank.

Chapter 6 Managing Patients

6.1 Admitting a Patient

To admit and set a patient as the current monitoring patient, follow the steps below:

- 1. Access [Patient Info] screen in either of the following ways:
 - Press the patient information area in the upper left corner of the screen.
 - Press the [Patient Info] quick key.
 - Press[Main Menu]→[Patient], select the [Patient Info] tab.
- 2. Select or enter patient information.
 - [Patient ID]: the patient's medical record number.
 - [Last Name]: the patient's last name (family name).
 - [Middle Name]: the patient's middle name.
 - [First Name]: the patient's first name.
 - [Gender]: the patient's gender, Male, Female and Unspecified.
 - [Age]: the patient's age.
 - [Date of Birth]: the date of birth of the patient, in the format of year month day.
 - [Patient Type]: the patient's type, Adult (age > 12 years old),
 Pediatric (29 days < age ≤ 12 years old) and Neonate (age ≤ 28 days).
 - [Height]: the patient's height.
 - [Weight]: the patient's weight.
 - [Bed No.]: the patient's bed number.
 - [Paced]: Select "Yes" or "No" (For paced patients, select "Yes".).
- 3. Press [Yes], the monitor will apply this patient as the current monitoring patient.



Discharge the previous patient before starting to monitor a new patient. Failure to do so can lead to data being associated with the wrong patient.



The default Patient Type setting is Adult, and Paced setting is Unspecified. Set [Paced] and check if the Patient Type setting is correct for the patient.



For paced patients, set [Paced] to [Yes]. If it is incorrectly set to [No], the monitor could mistake a pace pulse for a QRS and fail to give an alarm when the ECG signal is too weak. For non-paced patients, set [Paced] to [No].

6.2 Quickly Admitting a Patient

If you do not have the time or information to fully admit a patient. Complete the rest of the patient information later.

To quickly admit a patient, follow the steps below:

- 1. Press[Main Menu]→[Patient], select the [Quick Admit] tab.
- 2. Press [Auto Generated] or use the on-screen keyboard or barcode reader to input the medical record number.
- If the current status is [Patient Not Admitted], press [OK], the
 monitor will use this patient as the current monitoring patient;
 otherwise, in the pop-up confirmation window, press [OK] to
 stop monitoring the previous patient and use the patient as the
 current monitoring patient.

Input patient information as soon as the patient is admitted.

Note

The monitor supports CMS admitting patients remotely.

6.3 Editing Patient Information

Edit patient information after a patient has been admitted, or when patient information is incomplete, or when it is necessary to change patient information.

To edit patient information, follow the steps below:

- 1. Access [Patient Info] screen in either of the following ways:
 - Press the patient information area in the upper left corner of the screen.
 - Press the [Patient Info] quick key.
 - Press[Main Menu]→[Patient], select the [Patient Info] tab.
- 2. Edit patient information as required.

Caution

The monitor will reload the configuration if you changed the patient type.

6.4 Starting Monitoring a Patient

To start monitoring a patient, follow the steps below:

- 1. Admit the patient.
- 2. Decide which parameter measurements you want to make.
- 3. Connect the required patient cables and sensors and make sure they are correctly connected.
- 4. Check that the patient settings, such as Patient Type, NIBP measuring mode, etc. are appropriate for the patient.
- 5. Perform desired measurements. For more information, see corresponding parameter measurement chapters.

6.5 Stopping a Parameter Measurement

To stop monitoring a parameter, follow the steps below:

- 1. Remove corresponding sensor from the patient.
- 2. Disconnect the sensor from the patient cable.
- 3. Disconnect the patient cable from the monitor.

6.6 Discharging a Patient

To manually discharge a patient, follow the steps below:

- 1. Access [Patient Info] screen in either of the following ways:
 - Press the patient information area in the upper left corner of the screen.
 - Press the [Patient Info] quick key.
 - Press[Main Menu]→[Patient], select the [Patient Info] tab.
- 2. Select [Discharge Patient] to discharge the current patient.

After a patient is discharged, all patient data, including patient information, trend data and physiological alarms, are cleared, the technical alarms are reset, and the monitor settings return to their defaults.



Caution

After a patient is discharged, the monitor enters the "Patient Not Admitted" state, and the data will be saved as historical patient data.



Caution

If the patient is not discharged before the monitor is turned off, the patient will still be the one before shutdown after the monitor is turned on again.

Note

The monitor supports remote manual discharge of patients through the CMS.

6.7 Managing Patient Data

6.7.1 Querying Patient Data

To query patient data, follow the steps below:

- 1. Access [History] screen in either of the following ways:
 - Press the patient information area in the upper left corner of the screen → select the [History] tab.
 - Press the [Patient Info] quick key → select the [History] tab.
 - Press [Main Menu]→[Patient], select the [History] tab.
- 2. Input query criteria.
- 3. Press [Query]. Then a list pops up, including all the patients that meet the query criteria.

6.7.2 Viewing Historical Patient Data

In the [History] screen, select the patient record to view, and press the [Review] button to enter the data review screen to view the patient's historical data. See *Chapter 16 Review* for details.

6.7.3 Importing / Exporting Patient Data

To import / export the data of the current patient and discharged patients, follow the steps below:

- 1. Connect the USB drive to the monitor's USB connector.
- 2. Press[Main Menu]→[Patient], select the [History] tab.
- 3. Select desired patients from the patient list.
- 4. Select [Import] or [Export].

6.7.4 Deleting Patient Data

To delete the data of discharged patients, follow the steps below:

- 1. Press[Main Menu]→[Patient], select the [History] tab.
- 2. Select desired patients from the patient list.
- Select [Delete].

Caution

If a patient is deleted, all data related to the patient (such as ECG waveform, alarm events, etc.) will be deleted and cannot be recovered.

Note

The data of the current patient under monitoring cannot be deleted.

6.8 Configuring Patient Information

You can set up patient information to be displayed on the [Patient Info] screen, such as registration number, patient ID, race, etc. To do so, please refer to the following steps:

- Press[Main Menu]→[Maintenance]→ input password → press [Enter].
- 2. Select [Patient] tab.
- 3. Select the patient information to be displayed on the [Patient Info] screen.
- 4. If necessary, select the custom patient information field and enter the name of the field.

Caution

If the monitor is connected to the central monitoring system (CMS), the patient information and user-defined fields are synchronized with the CMS.

6.9 Managing Operators

Access [Operator] screen in either of the following ways:

- Press the operator information area in the upper left corner of the main screen.
- Press[Main Menu]→[Patient], select the [Operator] tab.

After entering the [Operator] screen, you can switch on the [Operator Information], and the operator name will be displayed in the operator information area in the upper left corner of the main screen.

On the [Operator] screen, you can also perform the following operations:

- [Add]: add operator information.
- [Edit]: edit the operator information.
- [Delete]: delete the currently selected operator information.
- [Refresh]: refresh the current operator information list.

Caution

The operator named "admin" preseted by the system cannot be set as the current operator or deleted from the operator list.

Note

Editing and deleting operations only change the contents of the operator list, and do not change the operator information recorded in historical patients.

This page intentionally left blank.

Chapter 7 Monitoring ECG, Arrhythmia, ST, QT/QTc Analysis

7.1 Introduction

Electrocardiogram (ECG) is the main means to measure the electrical activity of the heart. The ECG signals can be detected through electrodes at the surface of the skin, and displayed on the monitor as waveforms and numerics.

ECG monitoring provides 3/5/6/12-lead ECG monitoring, ST segment analysis, arrhythmia analysis, QT/QTc measurements, and optional 12-lead resting ECG analysis via the AI algorithm.

7.2 Safety Information



Only use the patient cable and lead wires provided by the manufacturer. Using those from other suppliers may cause improper performance or poor protection during defibrillation.

⚠ Warning

Make sure that all electrodes are connected to the patient correctly before operation.

⚠ Warning

Check if the patient category setting is correct for the patient.

⚠ Warning

Ensure that the conductive parts of ECG electrodes and associated connectors, including the neutral electrode, do not come into contact with any other conductive parts including earth. Make sure that all electrodes are connected to the patient correctly.

1 Warning

For paced patients, set Pacemaker to Yes. Otherwise, it may cause the pacing pulse to be treated as a regular QRS complex, and when the ECG signal is too weak, the system cannot detect it and give alarms. For ventricular paced patients, episodes of ventricular tachycardia may not always be detected.

⚠ Warning

For non-paced patients, set Pacemaker to No.

⚠ Warning

Some pacemakers may cause false low heart rate or arrest alarms, because pacemaker artifacts, such as pacemaker overshoot, may cover the real QRS complex.

⚠ Warning

Pacemaker automatic recognition function is not suitable for pediatric and neonate patients, as well as patients receiving NMT stimulation.

⚠ Warning

For paced patients, the heart rate meter may record the pacing pulse in case of cardiac arrest or arrhythmia. Do not rely entirely on heart rate meter alarms when monitoring patients with pacemakers. Always keep these patients under close surveillance.

⚠ Warning

Do not use dissimilar metal electrodes, otherwise it will cause high polarization voltage. Reusable electrodes will withstand a large bias potential due to polarization, and the recovery time after defibrillation will be particularly long (more than 10 seconds). It is recommended to use disposable electrodes.

⚠ Warning

In surgical mode, the monitor can be used with high frequency surgical equipment. When used with electrosurgical equipment, the operator should pay attention to ensure the safety of the monitored patients and operate in strict accordance with this manual. After the elimination of high frequency signal and high frequency electromagnetic field, it can return to the previous operating mode within 10 seconds without losing any permanent stored data.

⚠ Warning

To minimize the hazard of burns during use of high-frequency electrosurgical units (ESU), the ECG electrodes should not be located between the surgical site and the ESU return electrode.

⚠ Warning

To minimize the hazard of burns during high-frequency surgical procedures, ensure that the monitor's cables and transducers never come into contact with the electrosurgical units (ESU).

Caution

Interference from an ungrounded equipment near the patient or electrosurgery usage can induce noise and artifact into the waveforms.

Caution

When the monitor is inoperable due to overload of ECG signal or saturation of any part of the amplifier, it will prompt "Lead off" to remind the operator.

Caution

Transient caused by cable circuitry blocks while monitoring may cause artifact on ECG signals yielding wrong heart rate reading and even triggering false alarm. If the electrodes and cable are located in proper places according to this manual's instructions for using electrodes, the chance of this transient occurrence will be decreased.

7.3 ECG Monitoring Preparation

7.3.1 Preparing the Patient Skin

The quality of the ECG waveform displayed on the monitor is the direct reflection of the ECG signal received at the electrode sites. The state of patient's skin directly affects the strength of ECG signal and the accuracy of monitoring information. As the skin is a poor conductor of electricity, therefore preparation of the patient's skin is very important to facilitate good electrode contact to the skin.

To properly prepare the patient skin, please refer to the following steps:

- 1. Select sites with intact skin, without impairment of any kind. Shave hair from sites, if necessary.
- 2. Wash sites thoroughly with soap and water. (Never use ether or pure alcohol, because this increases skin impedance).
- 3. Rub the skin briskly to increase capillary blood flow in the tissues and remove skin scurf and grease.

7.3.2 Connecting ECG Cable and Applying Electrodes

To connect the ECG cable and applying electrodes, follow the steps below:

- 1. Plug the patient cable into the ECG connector.
- Attach the snaps to the electrodes prior to placement. Apply some electrode gel on the electrodes if the electrodes are not electrolyte self-supplied.

3. Place the electrodes on the prepared sites. For more information, see 7.3.3 ECG Electrode Placement.



Caution

To ensure accurate ECG measurement, please select the appropriate electrode type and pay attention to the placement position of the electrodes.



① Caution

If any side-effect such as allergic or itchy reaction is found, remove the electrodes from the patients immediately.



(1) Caution

Use only the same type of electrodes recommended by the manufacturer on the same patient to avoid the change of resistance.

7.3.3 ECG Electrode Placement

The electrode identifiers, color codes and electrode placement position of the internationally accepted IEC (European standard) and AHA (American standard) are shown in the table below:


IEC Standard		AHA Standard		Electrode
Identifier	Color Code	Identifier Color Code		Placement Position
R	Red	RA	White	Directly below the clavicle and near the right shoulder. Right Arm: on the inside of each arm, between the wrist and the elbow.
L	Yellow	LA	Black	Directly below the clavicle and near the left shoulder. Left Arm: on the inside of each arm, between the wrist and the elbow.

IEC Standard		AHA Standard		Electrode	
Identifier	Color Code	Identifier	Color Code	Placement Position	
F	Green	LL	Red	On the left lower abdomen. Left Leg: on the inside of each calf, between the knee and the ankle.	
N or RF	Black	RL	Green	On the right lower abdomen. Right Leg: on the inside of each calf, between the knee and the ankle.	
С	White	V	Brown	On the chest in any of the C1-C6 (V1-V6) electrode positions.	
C1	White/Red	V1	Brown/Red	On the fourth intercostal space at the right sternal border.	

IEC Standard		AHA Standard		Electrode	
Identifier	Color Code	Identifier Color Code		Placement Position	
C2	White/Yellow	V2	Brown/Yellow	On the fourth intercostal space at the left sternal border.	
С3	White/Green	V3	Brown/Green	Midway between C2 (V2) and C4 (V4) electrode position.	
C4	White/Brown	V4	Brown/Blue	On the fifth intercostal space at the left midclavicular line.	
C5	White/Black	V5	Brown/Orange	On the left anterior axillary line, horizontal with the C4 (V4) electrode position.	

IEC Standard		AHA Standard		Electrode
Identifier	Color Code			Placement Position
C6	White/Violet	V6	Brown/Violet	On the left midaxillary line, horizontal with the C4 (V4) electrode position.

Electrode Placement



① Caution

For the 5-lead and 6-lead placement, place the chest electrode according to the physician's preference.



Caution

For actual use, please place the electrodes according to the physician's preference.

7.4 ECG Display

ECG waveform area

The figures below are for reference only. The display may be configured to look slightly different.



- 1 ECG lead label of the displayed waveform
- 2 ECG waveform gain
- 3 ECG filter mode
- 4 Notch filter status
- 5 Paced status: If [Paced] is set to [Yes], is displayed. If [Paced] is set to [No], is displayed.
- 6 1mV scale

ECG parameter area



- 1 HR alarm limits
- 2 Parameter label
- 3 HR unit
- 4 HR value



The display of ECG waveform area and parameter area will be different, depending on different lead types and settings.

7.5 Changing ECG Settings

7.5.1 Setting ECG Menu

Access [ECG] setup screen in either of the following ways:

- Select the ECG parameter area.
- Press the [Parameters] quick key.
- Press [Main Menu]→[Parameters].

Depending on the function configuration, the ECG menus are different, please refer to the actual display of the monitor you purchased.

In the ECG Setup screen, you can perform the following operations:

[Lead]: Select the lead type. Options: 3-lead, 5-lead, 6-lead, 12-lead and Auto. The monitor can automatically detect the lead type.

[ECG1], **[ECG2]**: Set ECG lead label of the displayed waveform. See the following table for details:

Lead Type	ECG1	ECG2
3-lead	Options: I, II, III.	
	The default is II.	
5-lead	Options: I, II, III, aVR, aVL, aVF, V.	Options: I, II, III, aVR, aVL, aVF, V.
	The default is II.	The default is V.
6-lead	Options: I, II, III, aVR, aVL, aVF, Va, Vb.	Options: I, II, III, aVR, aVL, aVF, Va, Vb.
	The default is II.	The default is I.
	[Va]: Va, V1, V2, V3, V4, V5, V6. The default is Va.	
	[Vb]: Vb, V1, V2, V3, V4, V5,	, V6. The default is Vb.
12-lead	Options: I, II, III, aVR, aVL, aVF, V1, V2, V3, V4, V5,	Options: I, II, III, aVR, aVL, aVF, V1, V2, V3, V4, V5, V6.
	V6. The default is II.	The default is V1.

[Speed]: ECG waveform speed. Options: 6.25mm/s, 12.5mm/s, 25mm/s and 50mm/s.

[Filter]: ECG waveform filter mode. Options: Monitor, Diagnostic, Surgery and ST.

- [Monitor]: use under normal monitoring conditions.
- [Diagnostic]: use when diagnostic quality ECG is required.
- [Surgery]: use when the signal is distorted by high frequency or low frequency interference. High frequency interference usually results in large amplitude spikes making the ECG signal look irregular. Low frequency interference usually leads to drifting or rough baseline. The surgery filter reduces artifacts and interference from electro-surgical units. Under normal measurement conditions, selecting this filter mode may suppress certain features or details of the QRS complexes.
- [ST]: recommended for ST monitoring.

[Gain]: ECG gain, to set the size of each ECG waveform.

The base gain is 10mm/mV.

Factor options: $x \frac{1}{4}$, $x \frac{1}{2}$, x 1, x 2 and Auto.

- [x 1/4]: make the height of 1mV ECG signal waveform become 2.5mm.
- [x 1/2]: make the height of 1mV ECG signal waveform become 5mm.
- [x 1]: make the height of 1mV ECG signal waveform become 10mm.
- [x 2]: make the height of 1mV ECG signal waveform become 20mm.
- [Auto]: let the monitor choose the optimal adjustment for all the ECG waves. When "Auto" is selected, the monitor will automatically select one of the above six options and update it timely.

[Notch Filter]: The notch filter removes the line frequency interference. The notch filter can only be switched on or off when the ECG filter mode is set to "Diagnostic". In other filter modes, the notch filter is always off.

Set notch filter frequency according to the power line frequency of your country. To set notch filter frequency, follow the steps below:

- Press [Main Menu]→[Maintenance]→ input password → press [Enter].
- 2. Select the [Module] tab.

3. Set [Notch Filter] to [50Hz] or [60Hz] according to the power line frequency.

[Grid]: Switch on or off [Grid] to show or hide grid background on the ECG waveform area.

Note

If the amplitude of ECG waveform is too large, the wave peak or the wave valley might not be displayed. In this case, you should change the waveform gain appropriately.

7.5.2 Setting ECG Alarm Properties

To set ECG alarm options, follow the steps below:

- 1. Access ECG alarm setup screen in either of the following ways:
 - Press the [Alarms] quick key → select the [ECG] tab.
 - Press [Main Menu]→[Alarms], select the [ECG] tab.
 - Select the ECG parameter area → press the [Alarms] button.
- 2. Set the alarm switch, high and low limit, alarm priority, print output and record output according to your needs.

[Alarm Source]: Options: Auto, HR, PR, HR+PR. The default is Auto.

7.5.3 Setting ECG Lead Off Alarm Priority

To set the priority for ECG lead off alarms, follow the steps below:

- Press[Main Menu]→[Maintenance]→ input password → press [Enter].
- 2. Select the [Alarm] tab.
- 3. Set [ECG Lead Off] from the drop-down menu. Options: High, Med, Low. The default is Prompt.

7.5.4 Setting the ECG Standard

Set the ECG standard according to the leadwires you are using. To set the ECG standard, follow the steps below:

- Press [Main Menu] → [Maintenance] → input password → press [Enter].
- 2. Select the [Module] tab.
- Set [ECG Standard] from the drop-down menu. Options: AHA, IEC.

7.6 About Arrhythmia Monitoring

Arrhythmia monitoring is intended for adult, pediatric and neonatal patients.

7.6.1 Safety Information



⚠ Warning

If you switch off all the arrhythmias alarms, the monitor cannot give any arrhythmias alarm when that situation occurs. This may result in a hazard to the patient. Keep the patient under close surveillance.



⚠ Warning

Heart rate reading may be affected by cardiac arrhythmias. Do not rely entirely on heart rate alarms when monitoring patients with arrhythmias. Always keep these patients under close surveillance.



Caution

The priority of lethal arrhythmia alarms is always high. It cannot be changed.

Note

Because arrhythmia detection needs a template ECG waveform as reference which is a piece of normal ECG waveform with regular rhythm and stable amplitude, it is necessary to re-activate the template learning when the patient is changed, or the arrhythmia detection is incorrect. For stronger arrhythmia detection, it is recommended to wait for a clean and stable ECG waveform before starting ARR detection during the monitoring.

Note

During arrhythmia detection, incorrect detection might occur if the non-ECG waveforms (e.g., square or triangle waveform) appear.

Note

Before starting the 1mV calibration signal, please turn off the arrhythmia detection.

Note

During Arrhythmia detection, the template learning is very important. The device requires a group of stable QRS complex waveforms to build up this template. If the system detects Arrhythmia incorrectly, please re-activate the template learning and obtain the correct template.

7.6.2 Changing Arrhythmia Alarm Settings

To set the arrhythmia alarm properties, follow the steps below:

- 1. Enter the [Alarms] screen in either of the following ways:
 - Press [Main Menu]→[Alarms].
 - Press the [Alarms] quick key.
- 2. Select the [ARR] tab → [Alarm Name] tab.
- 3. Set alarm properties as desired.

In the arrhythmias alarm setup screen, you can perform the following operations:

- [Defaults]: press to reset all settings to the defaults.
- [All On]: press to switch on all arrhythmia alarms.
- [Lethals Only]: press to switch on lethal arrhythmia alarms, and switch off other alarms.

7.6.3 Setting the Lethal Arrhythmia Alarms Switch

To allow you to disable the lethal arrhythmia alarms, follow the steps below:

- Press [Main Menu] → [Maintenance] → input password → press [Enter].
- 2. Select the [Alarm] tab → select the [ARR] item.
- 3. Set [V-Fib/V-TachOff] as follows.
 - [V-Fib/V-Tach Off] is set to [Disable] by default. In this case, you cannot switch off [V-Fib/V-Tach] alarm.
 - If you set [V-Fib/V-Tach Off] to [Enable], you can switch off the [V-Fib/V-Tach] alarm.

When the [V-Fib/V-Tach] alarm is switched off, the physiological alarm information area displays a message "V-Fib/V-Tach Alarm Off".

1 Warning

If you switch off the V-Fib/V-Tach alarm, the monitor will not issue the V-Fib/V-Tach alarm when that situation occurs. This may result in a hazard to the patient. Always keep the patient under close surveillance.

7.6.4 Changing Arrhythmia Alarm Threshold Settings

You can change threshold settings for certain arrhythmia alarms. When an arrhythmia exceeds its threshold, an alarm will be triggered.

To change the arrhythmia alarm threshold settings, follow the steps below:

- 1. Enter the [Alarms] screen in either of the following ways:
 - Press [Main Menu]→[Alarms].
 - Press the [Alarms] quick key.
- 2. Select the [ARR] tab → [Threshold] tab.
- 3. Set the threshold for the desired arrhythmia alarms.

The setting range of arrhythmia threshold is shown in the table below.

Arrhythmia	Threshold Range		
Asystole Delay	3-10s		
Pause Threshold	1.5, 2.0, 2.5, 3.0s		
Nonsus V-Tach	3-99 beats		
Run PVCs	3-99 beats		
V-Tach Rate	100-200 bpm, step: 5 bpm		
V-Brady Rate	15-60 bpm, step: 5 bpm		
Extreme Tachy	121-350 bpm		
Extreme Brady	0-49 bpm		
High HR	60-155 bpm, step: 5 bpm		
Low HR	40-120 bpm, step: 5 bpm		
SV Tachy	60-300 bpm, step: 5 bpm		
SV Brady	15-120 bpm, step: 5 bpm		
SV Sustained Beats	3-99 beats		
PVCs/min	1-100		
A-Fib (HR High)	100-300 bpm, step: 5 bpm		
Pauses/min	1-15		
AF/IrrRhy End Time	0, 1, 2, 3, 4, 5, 10, 15, 30 min		
Multif PVCs Window	3-31 beats		

7.6.5 Arrhythmia Analysis Classifications

Arrhythmia Event (Abbreviation)	Arrhythmia Event (In Full or Description)
Lethal Arrhythmia Events:	

Arrhythmia Event (Abbreviation)	Arrhythmia Event (In Full or Description)		
Asystole	Asystole		
V-Fib/V-Tach	Ventricular-Fibrillation/Ventricular-Tachycardia		
Vent Tachy	Ventricular Tachycardia		
Vent Brady	Ventricular Bradycardia		
Extreme Brady	Extreme Bradycardia		
Extreme Tachy	Extreme Tachycardia		
Non-lethal Arrhythmia Eve	nts:		
Nonsus V-Tach	Nonsustained Ventricular Tachycardia		
Vent Rhythm	Ventricular Rhythm		
Run PVCs	More than two consecutive Premature Ventricular Contractions		
Pair PVCs	A Pair of Premature Ventricular Contractions		
R on T	R Waves Interrupting T Waves		
Vent Bigeminy	Ventricular Bigeminy		
Vent Trigeminy	Ventricular Trigeminy		
PVCs/min	Premature Ventricular Contractions per Minute		
Multiform PVC	Multiform Premature Ventricular Contractions		
PVC	Premature Ventricular Contractions		
HR High	Heart Rate High		
HR Low	Heart Rate Low		
SV Tachy	Supraventricular Tachycardia		
SV Brady	Supraventricular Bradycardia		
A-Fib (HR High)	Atrial-Fibrillation (High Heart Rate)		
A-Fib	Atrial Fibrillation		
A-Fib End	Atrial Fibrillation End		
Irr Rhythm	Irregular Rhythm		
Irr Rhy End	Irregular Rhythm End		
Pause	Heartbeat Pause		
Missed Beats	Missed Beats		

Arrhythmia Event (Abbreviation)	Arrhythmia Event (In Full or Description)		
Pauses/min	Heartbeat Pauses per Minute		
Pacer Not Pacing	Pacer Not Pacing		
Pacer Not Capture	Pacer Not Capture		
PAC	Premature Atrial Contractions		
PACs Couplet	A Pair of Premature Atrial Contractions		
SV Bigeminy	Supraventricular Bigeminy		
SV Trigeminy	Supraventricular Trigeminy		
2nd Degree A-V Block	2nd Degree Atrioventricular Block		
1st Degree A-V Block	1st Degree Atrioventricular Block		

7.7 About ST Monitoring

ST segment of ECG waveform is the period from the end of ventricular depolarization to the beginning of ventricular repolarization, or from the end of QRS complex (J point) to the beginning of T wave. ST segment analysis is often used to monitor the oxygen supply and myocardial activity of patients.

ST segment analysis can only be performed when the [Filter] is set to [Diagnostic] or [ST].ST segment analysis is intended for adult, pediatric and neonatal patients.

7.7.1 Safety Information



Warning

This monitor provides information regarding changes in ST deviation levels. The clinical significance of the ST level change information should be determined by a physician.



🗥 Warning

ST segment deviation values may be affected by such factors as certain drugs or metabolic and conduction disturbances.



Warning

The ST algorithm has been tested for accuracy of the ST segment data. The significance of ST segment changes needs to be determined by a physician.

7.7.2 Enabling ST Analysis/Display ST Parameters

The ST monitoring function is disabled by default. Before you start ST monitoring, enable the ST analysis function. To do so, follow the steps below:

- 1. Enter the ST setup screen in either of the following ways:
 - Select the ST parameter area.
 - Press the [Parameters] quick key, select the [ST] tab.
 - Press [Main Menu] → [Parameters], select the [ST] tab.
- 2. Switch on [ST Analysis], the ST parameter area appears on the main screen.

The ST parameter display area is configured differently according to the ECG cable used:

- When you are using the 3-lead ECG leadwires, a separate ST parameter area does not appear on the display. The ST deviation value displays in the ECG parameter area.
- When you are using the 5-lead ECG leadwires, the ST parameter area displays 7 ST deviation values for lead I, II, III, aVR, aVL, aVF, V.
- When you are using the 6-lead ECG leadwires, the ST parameter area displays 8 ST deviation values for lead I, II, III, aVR, aVL, aVF, Va, Vb.
- When you are using the 12-lead ECG leadwires, the ST parameter area displays 12 ST deviation values for lead I, II, III, aVR, aVL, aVF, V1, V2, V3, V4, V5, V6.


This example shows the ST parameter area with 5-lead ECG. Your monitor screen may look slightly different from the illustration.



- Parameter label
- 2 ST measurement unit
- 3 ST alarm off symbol
- 4 Lead labels

- 5 ST numerics: a positive value indicates ST segment elevation, and a negative value indicates ST segment depression.
- 7.7.3 Displaying ST Segments in the Waveform Area
 To display ST segments in the waveform area, follow the steps
 below:
- 1. Enter the ST setup screen in either of the following ways:
 - Select the ST parameter area.
 - Press the [Parameters] quick key, select the [ST] tab.
 - Press [Main Menu] → [Parameters], select the [ST] tab.
- 2. Switch on [ST Segment], the ST segments appears in the waveform area.
- 3. Switch on [Display Markers] and [Display Baseline] when necessary.

The ST segment area displays the current ST segment and baseline ST segment, the current ST value and baseline ST value. The current ST segment is drawn in the same color as the ECG wave, usually green, superimposed over the stored reference segment, drawn in a different color. As shown in the following figure:



- 1 ST lead
- 2 Current ST value
- 3 Baseline ST value
- 4 Marker
- 5 1mV scale
- 7.7.4 Displaying ISO Point, J Point and ST Point Markers
 To display the ISO point, J point, and ST point marker on the ST segments in the waveform area, follow the steps below:

To display ST segments in the waveform area, follow the steps below:

- 1. Enter the ST setup screen in either of the following ways:
 - Select the ST parameter area.
 - Press the [Parameters] quick key, select the [ST] tab.
 - Press [Main Menu] → [Parameters], select the [ST] tab.
- 2. Switch on [Display Markers].

7.7.5 Displaying Baseline ST Segments

To display the baseline ST segments in the waveform area, follow the steps below:

- 1. Enter the ST setup screen in either of the following ways:
 - Select the ST parameter area.
 - Press the [Parameters] quick key, select the [ST] tab.
 - Press [Main Menu] → [Parameters], select the [ST] tab.
- 2. Switch on [Display Baseline], the baseline ST segment (white) appears.

7.7.6 Setting ST Alarm Properties

To set ST alarm options, follow the steps below:

- 1. Enter the ST alarm setup screen in either of the following ways:
 - Press the [Alarms] quick key, select the [ST] tab.
 - Press [Main Menu] → [Alarms], select the [ST] tab.
 - Select the ECG parameter area → press the [Alarms] button, select the [ST] tab.
- 2. Set the alarm switch, high and low limit, alarm priority, print output and record output according to your needs.

In the ST alarm setup screen, you can perform the following operations:

- [All On]: press to switch on all ST alarms.
- [All Off]: press to switch off all ST alarms.
- [Defaults]: press to reset all value to the defaults.

7.8 About QT/QTc Interval Monitoring

The QT interval is the time between the beginning of the Q-wave and the end of the T-wave. It represents the total duration of the depolarization (QRS duration) and repolarization (ST-T) phases of

the ventricles. QT interval monitoring can assist in the detection of long QT syndrome.

QT interval was negatively correlated with heart rate. The faster the heart rate, the shorter the QT interval, and vice versa. Therefore, several formulas are commonly used to correct the QT interval for heart rate. The heart rate corrected QT interval is abbreviated as QTc.

QT/QTc interval monitoring is intended for adult, pediatric and neonatal patients.


7.8.1 Enabling QT/QTc Monitoring

The QT monitoring function is disabled by default. Before you start QT monitoring, enable the QT analysis function.

To do so, follow the steps below:

- 1. Enter the QT setup screen in either of the following ways:
 - Select the QT parameter area.
 - Press the [Parameters] quick key, select the [QT] tab.
 - Press [Main Menu]→[Parameters], select the [QT] tab.
- 2. Switch on [QT Analysis], the QT parameter area appears on the main screen.

The following figure shows the QT parameter area. Your monitor screen may look slightly different.

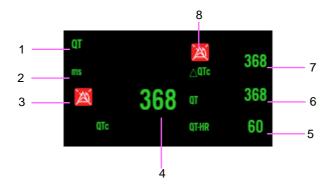

- 1 Parameter label
- 2 QT measurement unit
- 3 QTc alarm limit (if QTc alarm is off, the alarm off symbol is displayed)
- 4 QTc value

- 5 QT-HR value
- 6 QT value
- 7 ΔQTc value
- 8 Δ QTc alarm limit (if Δ QTc alarm is off, the alarm off symbol is displayed)

7.8.2 Selecting Leads for QT Calculation

You can select one lead or all leads for QT calculation. To do so, follow the steps below:

- 1. Enter the QT setup screen in either of the following ways:
 - Select the QT parameter area.
 - Press the [Parameters] quick key, select the [QT] tab.
 - Press [Main Menu] → [Parameters], select the [QT] tab.
- 2. Set [QT Analysis Lead]. [All] is selected by default, which means all leads are used for QT calculation.

7.8.3 Selecting the QTc Formula

The monitor uses the Hodges correction formula by default to correct the QT interval for heart rate. To select the other QTc formula, follow the steps below:

- 1. Enter the QT setup screen in either of the following ways:
 - Select the QT parameter area.
 - Press the [Parameters] quick key, select the [QT] tab.
 - Press [Main Menu] → [Parameters], select the [QT] tab.
- 2. Set [QTc Formula].

Hodeges: $QTc = QT+1.75 \times (HR-60)$

Bazett: QTc = QT × $(HR/60)^{1/2}$ Fredericia: QTc = QT × $(HR/60)^{1/3}$

Framingham: $QTc = QT+154 \times (1-60/HR)$

7.8.4 Setting QT Alarm Properties

To set QT alarm options, follow the steps below:

- 1. Enter the QT alarm setup screen in either of the following ways:
 - Press the [Alarms] quick key, select the [QT] tab.
 - Press [Main Menu]→[Alarms], select the [QT] tab.
 - Select the ECG parameter area → press the [Alarms] button, select the [QT] tab.
- 2. Set QTc and \triangle QTc alarm properties.

7.9 Factors Affecting ECG Signal

The following factors will affect the quality of acquired ECG signals:

- Interference from electro-surgical units.
- Unreasonable filter mode setting.
- · Poor grounding.
- Incorrect placement of electrodes.
- Use expired electrodes or use disposable electrodes repeatedly.
- The skin on which the electrodes are placed is unclean or poor contract caused by scurf and hair.

Chapter 8 Resting 12-Lead ECG Analysis

The monitor supports automatic acquisition of 12- lead resting ECG waveforms. After acquisition, the data is transmitted to the AI-ECG Platform server through the network for analysis. You can download, view and print the diagnosis report at the monitor side.

Note

The resting12-lead ECG analysis function is only available if the monitor you purchased is configured with 12-lead ECG.

8.1 Entering the 12-Lead Screen

To enter the 12-lead screen, follow the steps below:

- 1. Select the ECG parameter area to enter the ECG Setup screen.
- 2. From the popup list of the [Lead], select [12-lead].
- 3. From the bottom of the ECG Setup screen, select [ECG 12-Lead].

You can also enter the 12-lead screen by following the steps below:

- Press the [ECG 12-Lead] quick key.
- Press the [Screens] quick key → select [ECG 12-Lead].
- Press [Main Menu]→[Screens], select [ECG 12-Lead].

There are 12 ECG waveforms and 1 rhythm lead in the waveform area of the 12-lead screen. The rhythm lead is the ECG calculation lead before entering this screen.

8.2 Setting the 12-Lead ECG Acquisition

You can perform the following operations on the 12-lead screen:

- [Start / Stop]: press this button to start / stop ECG acquisition.
- [Freeze]: press this button to freeze the currently displayed waveforms on the screen and enter the freeze screen.
- [Real-time]: set the sampling mode, real-time sampling and pre-sampling can be selected. The default is real-time sampling.
- [10mm/mV]: set the gain of the waveforms.
 Options: 2.5mm/mV, 5mm/mV, 10mm/mV, 20mm/mV.
 The default is 10mm/mV.
- [25mm/s]: set the speed of the waveforms.
 Options: 25mm/s, 50mm/s. The default is 25mm/s.
- [6x2+1R]: set the 12-lead waveform layout.
 Options: 6x2+1R, 3x4+1R. The default is 6x2+1R.
- [10s]: set the acquisition time.
 Options: 10s, 20s, 30s, 60s. The default is 10s.
- [Exit]: press this button to exit the 12-lead screen and return to the main screen.
 - If you press this button to exit during the acquisition process, the system will pop up the exit confirmation prompt.

8.3 Connecting to the AI-ECG Server

Before initiating 12-lead ECG acquisition, please set up the network and connect the monitor to the server of AI-ECG Platform. For the specific setting method, please refer to 4.6 Connecting the AI-ECG Server.

8.4 Initiating 12-Lead ECG Acquisition

After connecting the AI-ECG server, before 12-lead ECG acquisition, please select and install electrodes according to the introduction of 7.3ECG Monitoring Preparation, check that all electrodes and cables have been properly connected, the patient information is set correctly, and always keep the patient quiet.

To initiate 12-lead ECG acquisition, press the [Start] button in the lower right corner of the [ECG 12-Lead] screen.

 Real-time sampling: acquire the ECG data of the set acquisition time after pressing the [Start] button. During the acquisition process, the remaining acquisition time is displayed. At the completion of acquisition, the system enters the preview screen. Pre-sampling: acquire the ECG data of 10 seconds before pressing the [Start] button. At the completion of acquisition, the system enters the preview screen.

In the preview screen, press [Save] to send the saved data to Al-ECG server for analysis. After the report is obtained, you can view it in the [Reports Mgmt] screen.

In addition to the above 12-leadECG analysis, the monitor also supports 12-lead analysis of stored historical waveforms. Follow this procedure:

- Press [Review] quick key or press [Main Menu] → [Review] to enter the review screen.
- 2. Select the [Full Disclosure] tab.
- 3. Select the desired waveform segment.
- 4. Press the [12-Lead ECG] button to enter the resting ECG acquisition screen.
- 5. Set the [Period].
- Press [Start].

The monitor will send the stored data corresponding to the selected time length, or the collected data of the selected time length, to the AI-ECG server (if connected) for analysis.

Note

[Start Time] is the time point of the selected waveform segment.

8.5 Reports Management

After ECG acquisition, press [Main Menu]→[Reports] to enter the reports management screen. You can perform the following operations in this screen:

- Press [Delete] to delete one or more selected patient record.
- Press [Preview] to enter the preview screen of ECG waveforms of the selected patient record.
- Press [Upload] to upload one or more selected patient record to the AI-ECG server.
- Press [Download] to download the diagnosis report of the selected patient record from the AI-ECG server.
- Press [View Report] to view the diagnosis report of the selected patient record.

• Press [to print the obtained diagnosis report of the selected patient record via the network printer.

Note

For the processing method of ECG data received by AI-ECG server, please refer to the Operator's Manual of ECG Analysis Software of AI-ECG Platform.

Note

Please configure the network printer before printing 12-lead ECG analysis reports.

This page intentionally left blank.

Chapter 9 Ambulatory ECG Analysis

The monitor supports automatic acquisition of single lead / 8-lead / 12-lead ambulatory ECG waveforms. After acquisition, the data is transmitted to the AI-ECG Tracker server through the network for analysis. You can download and print the diagnosis report at the monitor side.

9.1 Connecting to the AI-ECG Server


Before initiating ambulatory ECG acquisition, please set up the network and connect the monitor to the server of AI-ECG Tracker. For the specific setting method, please refer to *4.6 Connecting the AI-ECG Server*.

9.2 Electrode Placement

Refer to 7.3.1 Preparing the Patient Skin for the skin preparation for electrode placement.

Attach the snaps to the electrodes and then place the electrodes on the patient according to the lead type you have chosen. The following figures show the typical position of electrode placement. You can also refer to the position recommended by the analysis system and the physician.


→ 12-lead (10 Lead Wires) Electrode Placement



Color Label Color Label Color Colo
--

	AHA Color	AHA Label	IEC Color	IEC Label	Position
1	Brown/ Red	V1	White/ Red	C1	The fourth intercostal space at the right edge of sternum
2	Brown/ Yellow	V2	White/ Yellow	C2	The fourth intercostal space at the left edge of sternum
3	Brown/ Green	V3	White/ Green	C3	The position between V2 and V4
4	Brown/ Blue	V4	White/ Dark brown	C4	Midclavicular line at the fifth intercostal space
5	Brown/ Orange	V5	White/ Light blue	C5	Anterior axillary line at the same level as V4
6	Brown/ Purple	V6	White/ Purple	C6	Midaxillary line at the same level as V4 and V5
7	Black	LA	Yellow	L	Left shoulder
8	Red	LL	Green	F	The lower edge of rib cage, or the level of the navel at the position of middle clavicle line.
9	Green	RL	Black	N	The lower edge of rib cage, or the level of the navel at the position of middle clavicle line.
10	White	RA	Red	R	Right shoulder

^{→ 8-}lead (6 Lead Wires) Electrode Placement



	AHA Color	AHA Label	IEC Color	IEC Label	Position
1	Brown/ Red	V1	White/ Red	C1	The fourth intercostal space at the right edge of sternum
2	Brown/ Orange	V5	White/ Light Blue	C5	Anterior axillary line at the same level as V4
3	Black	LA	Yellow	L	The left shoulder
4	Red	LL	Green	F	The lower edge of rib cage, or the level of the navel at the position of middle clavicle line.
5	Green	RL	Black	N	The lower edge of rib cage, or the level of the navel at the position of middle clavicle line.
6	White	RA	Red	R	Right shoulder

① Caution

For an accurate ambulatory ECG analysis, it is suggested that Va should be placed in V1 and Vb in V5.

9.3 Initiating Ambulatory ECG Acquisition

Real-time ambulatory ECG acquisition

Press the [Holter] quick key to enter the [Holter] screen. You can perform the following operations in this screen:

- Select [Period] to set the duration of ambulatory ECG acquisition. Options: 24h, 48h, 72h.
- Press [Start] to start the ambulatory ECG acquisition.
- Press [Stop] to stop the ambulatory ECG acquisition after confirmation.
- Press [x] in the upper right corner of the screen to exit the Holter screen.

Note

[Start Time] is displayed automatically. The default is the current time. [Acquire Time] is the current acquisition time.

Historical ECG waveform acquisition

Press [Main Menu]→[Review]→[Full Disclosure], select a waveform segment in the waveform area, and then press the [Holter] button to enter the Holter screen. You can perform the following operations in this screen:

- Select [Period] to set the duration of ambulatory ECG acquisition. Options: 24h, 48h, 72h.
- Press [Start] to start the ambulatory ECG acquisition.
- Press [Stop] to stop the ambulatory ECG acquisition after confirmation.
- Press [x] in the upper right corner of the screen to exit the Holter screen.

Note

[Start Time] is displayed automatically. The default is the historical start time selected in the waveform area. [Acquire Time] is the current acquisition time.

At the completion of acquisition, the monitor automatically sends the data to the AI-ECG server (if connected) for analysis.

9.4 Reports Management

For the preview and print operations of the diagnostic reports, please refer to 8.5 Reports Management.

Note

For the processing method of ECG data received by AI-ECG server, please refer to the Operator's Manual of Ambulatory ECG Analysis Software of AI-ECG Tracker.

This page intentionally left blank.

Chapter 10 Monitoring Respiration (Resp)

10.1 Introduction

Respiration is monitored by measuring the impedance across the thorax via electrodes places on chest. When the patient is breathing or ventilated, the volume of air changes in the lungs, resulting in impedance changes between the electrodes. Impedance respiration rate (RR) is calculated from the signal representing these impedance changes, and a respiration waveform is displayed on the patient monitor screen.

Respiration monitoring is intended for adult, pediatric and neonatal patients.

10.2 Safety Information



When monitoring the patient's impedance respiration, do not use ESU-proof ECG cables. The monitor cannot measure impedance respiration with ESU-proof ECG cables.

⚠ Warning

The respiration measurement does not recognize the cause of apneas. It only indicates an alarm if no breath is detected when a preset time has elapsed since the last detected breath. Therefore, it cannot be used for diagnostic purpose.

⚠ Warning

If operating under conditions according to the EMC Standard IEC 60601-1-2 (Radiated Immunity 3V/m), field strengths above 3V/m may cause erroneous measurements at various frequencies. Therefore, it is recommended to avoid the use of electrically radiating equipment in close proximity to the impedance respiration measurement unit.

⚠ Warning

To avoid the hazard of burns during use of high-frequency electrosurgical units (ESU), the electrodes should not be located between the surgical site and the ESU return electrode. Place the ESU return electrode close to the operation area.



Impedance respiration monitoring is not suitable for patients who are very active, otherwise it may lead to false alarm.

10.3 Resp Monitoring Preparation


10.3.1 Preparing the Patient Skin

As the skin is a poor conductor of electricity, correct patient skin preparation for electrode placement is important for Resp measurement. You can refer to 7.3.1 Preparing the Patient Skin for how to prepare the skin.

10.3.2 Placing the Electrodes

Respiration measurement adopts the standard ECG electrode placement with standard ECG electrodes and cables. The respiration signal is always measured between two of the ECG electrodes. There are two standard ECG leads for selection: I lead (RA and LA) and II lead (RA and LL).

For electrode placement, see 7.3.2 Connecting ECG Cable and Applying Electrodes.

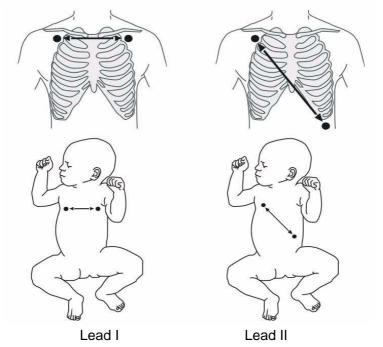

To optimize the respiration waveform, place the RA and LA electrodes horizontally when monitoring respiration with ECG Lead I; place the RA and LL electrodes diagonally when monitoring respiration with ECG Lead II.



Caution

Some patients (especially neonates) expand their chests laterally, causing a negative intrathoracic pressure. In these cases, it is better to place the two respiration electrodes in the right midaxillary and the left lateral chest areas at the patient's maximum point of the breathing movement to optimize the impedance respiration waveform.



Caution

Correct electrode placement can help to reduce interference from cardiac related impedance changes: avoid including the liver area and the ventricles of the heart between the respiratory electrodes. This is particularly important for neonates.



Caution

Some patients with restricted movements breathe mainly through the abdomen. In these cases, you may need to place the left leg electrode on the left abdomen at the point of maximum abdominal expansion to optimize the respiratory waveform.



Caution

Periodically inspect electrode application sites to ensure skin integrity. If there are signs of allergy, replace the electrodes or change the application site.



Note

Store the electrodes at room temperature. Open the electrode package immediately prior to use.




Note

Check that the electrode packages are intact and that the electrodes are not past the expiration date. Ensure the electrode gel is moist.


10.4 Resp Display

Resp waveform area



- 1 Resp lead label
- 2 Resp waveform gain
- 3 Resp lead label

Resp parameter area

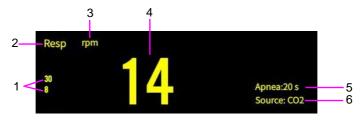

- 1 Alarm limits
- 2 Parameter label
- 3 Resp unit
- 4 Respiration rate (RR)
- 5 RR source
- 6 Apnea delay time

10.5 Changing Resp Settings

10.5.1 Setting Resp Menu

Access Resp setup screen in either of the following ways:

- Press Resp parameter area.
- Press the [Parameters] quick key → select the [Resp] tab.
- Press [Main Menu] → [Parameters], select the [Resp] tab.

Depending on the function configuration, the Resp menus are different, please refer to the actual display of the monitor you purchased.

In the Resp setup screen, you can perform the following operations:

• **[Speed]**: Respiration waveform sweeping speed. The larger the value, the faster the sweeping speed.

Options: 6.25mm/s, 12.5mm/s, 25mm/s, 50mm/s.

• **[Gain]**: Respiration amplification/gain times, used to adjust the amplitude of respiration waveform, the greater the gain, the higher the amplitude of waveform.

Options: x1/8, x1/4, x1/2, x1, x2, x4.

The basic gain is 10mm/mV.

X1 waveform scale with base gain

X1/8 one eighth scale size of the base gain

X1/4 one quarter scale size of the base gain

X1/2 half scale size of the base gain

X2 twice scale size of the base gain

X4 four times scale size of the base gain

• [Apnea Delay]: The timeout setting for apnea alarm (in second). Setting range: 10 to 40 seconds, the step is 5 second.

The Resp parameter area will display "Apnea: XX s (display the set Apnea delay time)"; when an apnea event is detected, an "Apnea" prompt will appear on the alarm information area, and an alarm tone will be issued.

 [Resp Lead]: set the respiration lead to get the best respiration waveform.

Options: I, II.

• [RR Source]: select the respiration signal source.

Options: Auto, CO₂ and ECG.

When you select [Auto], the monitor automatically selects the RR source according to the priority order: first CO₂, and then

ECG. The RR source name is displayed in the lower right corner of Resp parameter area.

When the manually selected RR source is not available, the monitor automatically switches the [RR Source] to [Auto].

10.5.2 Setting Resp Alarms

To set the Resp alarm options, follow the steps below:

- 1. Access Resp alarm setup screen in either of the following ways:
 - Press [Main Menu] → [Alarms] → select the [Resp] tab.
 - Press the [Alarms] quick key → select the [Resp] tab.
 - Press the Resp parameter area → press the [Alarms] button.
- 2. Set alarm properties as desired.
 - ① Caution

You can only switch off the apnea alarm when [Apnea Off] is set to [Enabled].

This page intentionally left blank.

Chapter 11 Monitoring Pulse Oxygen Saturation (SpO₂)

11.1 Introduction

Pulse oxygen saturation (SpO₂) monitoring is a non-invasive optical technique used to measure the amount of oxygenated hemoglobin (HbO₂) and pulse rate by measuring the absorption of selected wavelengths of light. The light generated in the emitter side of the sensor is partly absorbed when it passes through the monitored tissue. The amount of transmitted light is detected in the detector side of the sensor. When the pulsative part of the light signal is examined, the amount of light absorbed by the hemoglobin is measured and the pulse oxygen saturation can be calculated. The monitor is calibrated to display functional oxygen saturation. SpO₂ monitoring is intended for adult, pediatric and neonatal patients.

11.2 Safety Information



⚠ Warning

Check the SpO₂ sensor and cable before use. Do NOT use the damaged SpO₂ sensor.



⚠ Warning

DO NOT stare at the light of SpO₂ sensor (infrared light is invisible) when it is switched on, for the infrared light may do harm to the eyes.



⚠ Warning

Inspect SpO₂sensor application site every one to two hours to ensure skin quality and correct optical alignment, and change the measuring site periodically if necessary. If the skin quality changes, move the sensor to another site.



Warning

SpO₂ measuring site must be examined more carefully for some special patients. Do NOT place the SpO₂ sensor on the finger with edema or fragile tissue.



⚠ Warning

Avoid placing the SpO₂ sensor on the same extremity with an arterial catheter, blood pressure cuff, or intravascular infusion line, otherwise the blood flow could be interrupted by the cuff or the circulatory condition could make low blood perfusion so that would result in no pulse found or loss of pulse during SpO₂ monitoring and further cause false alarm.



Warning

If the sensor is too tight because the application site is too large or becomes too large due to edema, excessive pressure for prolonged periods may result in venous congestion distal from the application site, leading to interstitial edema, hypoxia, tissue ischemia, and inaccurate oxygen saturation measurements.



Warning

Continuous use of fingertip SpO₂ sensor may result in discomfort or pain, especially for those patients with microcirculatory problem. It is recommended that the sensor should NOT be applied to the same site for over two hours.



⚠ Warning

Excessive ambient light may affect the measuring result, it includes fluorescent lamp, dual ruby light, infrared heater, and direct sunlight etc.



🗥 Warning

Do not apply tape to secure the sensor in place or to tape it shut; venous pulsation may lead to inaccurate oxygen saturation measurements.



⚠ Warning

Vigorous movement of the patient, strong ambient light, or extreme electro-surgical interference may also affect the SpO₂ measuring accuracy.



Warning

Please do not use the SpO₂ sensor and the monitor when doing the MRI imaging, or burn may be caused by faradism.



Caution

For disposal SpO₂ sensor, if the sterile packaging is damaged, do not use it any more.



Caution

When the temperature of SpO₂ sensor is abnormal, do not use it any more.

(Caution

Please do not allow the cable to be twisted or bent.

Caution

Please do not use nail polisher or other cosmetic product on the nail.

Caution

The fingernail should be of normal length.

Caution

The SpO_2 sensor cannot be immersed into water, liquor or cleanser completely, because the sensor has no capability to resist the harmful ingress liquid.

(Caution

Do not disinfect any ${\sf SpO}_2$ sensor by irradiation, steaming, or ethylene oxide.

Note

The clinical study for SpO₂ measurement accuracy was done on human subjects according to Standard ISO 80601-2-61.

Note

A functional tester or SpO_2 simulator cannot be used to assess the accuracy of the oximeter or a SpO_2 sensor. However, it can be used to check how accurately a particular oximeter is reproducing the given calibration curve. Before testing the oximeter by a functional tester, please firstly ask the manufacturer which calibration curve is used, if necessary, request the manufacturer for its dedicated calibration curve and download it into the tester.


11.3 Measurement Interferences

- The SpO₂ measurement of the monitor may not work effectively for all kinds of patients, for whom with weak pulse due to shock, low ambient / body temperature, major bleeding, or use of vascular contracting drug, the measurement will be more sensitive to interference, if stable readings cannot be obtained at any time, stop to use the SpO₂ monitoring function.
- For those with a substantial amount of staining dilution drug (such as methylene blue, indigo green and acid indigo blue), or carbon monoxide hemoglobin (COHb), or methionine (Me+Hb)

- or thiosalicylic hemoglobin, and some with icterus problem, the SpO₂measurements may be inaccurate.
- The medicines such as dopamine, procaine, prilocaine, lidocaine and butacaine may also be a major factor blamed for serious error of SpO₂ measurements.
- As the SpO₂ value serves as a reference value for judgment of anemic anoxia and toxic anoxia, the measurement result of some patients with serious anemia may also present as good SpO₂ value.


11.4 SpO₂ Display

Plethysmogram




Pleth: abbreviation of plethysmogram. The Pleth waveform is processed by amplitude normalization.

SpO₂ parameter area

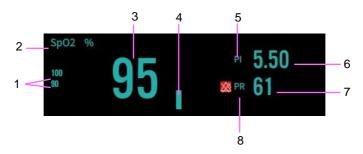

KRK SpO₂ module

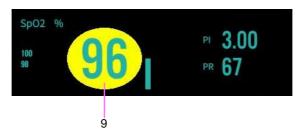

Nellcor SpO₂module

- 1 Alarm limits
- 2 SpO₂ label
- 3 SpO₂ value
- 4 Pulse intensity bar graph
- 5 Perfusion index (PI) label
- 6 Numerical value for the perfusion index
- 7 Pulse rate value
- 8 Label of pulse rate
- 9 SpO₂ value(for Nellcor SpO₂ module)

11.5 SpO₂ Monitoring Preparation


To prepare SpO₂ monitoring, follow the steps below:

- 1. Select an appropriate sensor according to the patient type and weight.
- Apply the sensor to the patient according to the instruction for use of the sensor.

We provide several probes for optional, please refer to the following description according to the probe/sensor you've purchased.

Type 1: SpO₂ Finger Clip Sensor


Insert the patient's index finger (middle finger or ring finger with proper nail length can be used as well) into the sensor, as shown in the figure below.



Type 2: SpO₂ Finger Rubber Sensor

Hold the sensor with its opening towards the patient's finger, the sensor should be oriented in such a way that the sensor side with a finger tip sign is positioned on the top.

Insert the patient's finger into the sensor until the fingernail tip rests against the stop at the end of the sensor. Adjust the finger to be placed evenly on the middle base of the sensor. Direct the cable along the top of the patient's hand. Apply adhesive tape to secure the cable if necessary.




Type 3: SpO₂ Ear Clip Sensor

Clip the sensor on the patient's earlobe, refer to the following figure:



Type 4: SpO₂ Sensor with L-type Wrapper Refer to the following connection method:

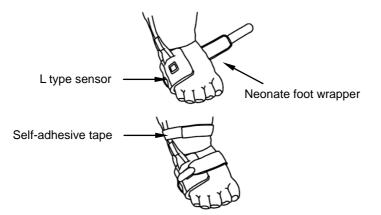

Type 5: Nellcor D-YS SpO₂ Sensor with Y-type Wrapper

For the connection method, please refer to the attached "Instructions For Use of NellcorTM SpO₂Sensor Multisite Reusable" according to the applicable patient.

- 3. Select an appropriate extension cable according to the connector type and plug the cable into the SpO₂ connector.
- 4. Connect the sensor to the extension cable.



Caution

Do not apply sensor too tightly as this results in venous pulsation which may severely obstruct circulation and lead to inaccurate measurements.



Caution

At elevated ambient temperatures, be careful with measurement sites that are not well perfused, because this can cause burns after prolonged application.



Caution

Avoid placing the sensor on extremities with an arterial catheter, an NIBP cuff or an intravascular venous infusion line.



Caution

For neonatal patients, make sure that all sensor connectors and adapter cable connectors are outside the incubator. The humid atmosphere inside can cause inaccurate measurements.

11.6 Changing SpO₂ Settings

11.6.1 Setting SpO₂ Menu

Enter the SpO₂ setup screen in either of the following ways:

- Select the SpO₂ parameter area.
- Press the [Parameters] quick key → select the [SpO₂] tab.
- Press[Main Menu]→[Parameters], select the [SpO₂] tab.

In the SpO₂ setup screen, you can perform the following operations:

- **[Speed]**: Pleth waveform sweeping speed. The larger the value, the faster the sweeping speed.
 - Options: 6.25mm/s, 12.5mm/s, 25mm/s, 50mm/s.
- **[Display PI]**: set whether to display the PI value in the SpO₂ parameter area.
- [PR Source]: set the PR source.

Options: Auto, SPO₂, IBP1, IBP2. The default is Auto. When you select Auto, the system will automatically select the first option in the drop-down menu as the PR source, and then select backward when the previous one does not exist. If specific PR source is selected, but the source is unavailable, the system will automatically execute Auto obtaining logic, that is, SpO₂> IBP1> IBP2.

- [NIBP Simul.]: When monitoring SpO₂ and NIBP on the same limb simultaneously, you can switch on NIBP Simul to lock the SpO₂ alarm status until the NIBP measurement ends. If you switch off NIBP Simul, low perfusion caused by NIBP measurement may lead to inaccurate SpO₂ readings and therefore cause false physiological alarms.
- **[Sat-Seconds]**: SatSeconds sensitivity setting, to set the max buffering time of activating SpO₂ alarm.

Options: Off, 10, 25, 50, 100. If you set SatSeconds to Off, it means that the SatSeconds alarm management function is disabled.

Formula: Sat-Seconds = SpO_2 points × seconds.

Set a SatSeconds limit, which allows SpO₂ to fall below or exceed the alarm limit for a certain period of time without triggering an alarm.



Caution

The Sat-Seconds setting is only available for Nellcor SpO₂ module.

11.6.2 Changing the SpO₂ Alarm Settings

To set SpO₂ alarm options, follow the steps below:

- 1. Enter the SpO₂ alarms setup screen in either of the following ways:
 - Select the SpO₂ parameter area → press the [Alarms] button.
 - Press the [Alarms] quick key → select the [SpO₂] tab.
 - Press[Main Menu]→[Alarms]→ select the [SpO₂] tab.
- 2. Set alarm properties as desired.
 - Caution

The SpO₂Desat (desaturation) alarm cannot be switched off by default.

11.6.3 Setting the Priority of the SpO₂ Sensor Off Alarm

To set the priority of the SpO_2 sensor off alarm, follow the steps below:

- Press[Main Menu]→[Maintenance]→ input password → press [Enter].
- 2. Select the [Alarm] tab.
- 3. Set [SpO₂ Sensor Off] from the drop-down menu. Options: High, Med, Low. The default is Low.

11.7 Changing PR Settings

11.7.1 Changing the PR Alarm Settings

To set PR alarm options, follow the steps below:

- 1. Enter the PR alarms setup screen in either of the following ways:
 - Press the [Alarms] quick key → select the [SpO₂] tab.
 - Press [Main Menu] →[Alarms]→ select the [PR] tab.
- 2. Set alarm properties as desired.

[Alarm Source]: options: Auto, HR, PR, HR + PR. The default is Auto.

11.7.2 Setting the PR Source

To set which parameter is used as a PR source, follow the steps below:

1. Enter the SpO₂setup screen. For the specific operation method, refer to *11.6.1 Setting SpO2 Menu*.

2.	Set [PR Source], select an appropriate PR source from the drop-down list.		

Chapter 12 Monitoring Temperature (Temp)

12.1 Introduction

The patient's body temperature can be measured by means of a thermistor probe (a semiconductor whose resistance changes with temperature). Very small amount of constant current is applied to the temperature probe to avoid self-heating. The voltage across the thermistor is measured, and further converted into a temperature reading according to the temperature-resistance characteristic for a specific type of thermistor.

Up to two temperature sites can be monitored simultaneously and the difference ($\triangle T$) between two measured sites is calculated. Temperature monitoring is intended for adult, pediatric and neonatal patients.

12.2 Safety Information



Caution

Verify that the probe detecting function works correctly before monitoring. Remove the temperature probe cable from the temperature probe connector, and check that the monitor can display the alarm message [Temp 1 sensor off] or [Temp 2 sensor off] and give alarm tones correctly.




Caution

When unplugging the probe, be sure to hold the head of the connector and pull it out.



There is a range of normal body temperature. At the same time, the temperature of different measurement sites is different. Therefore, the readings of different sites should not be compared directly.

12.3 Temp Display

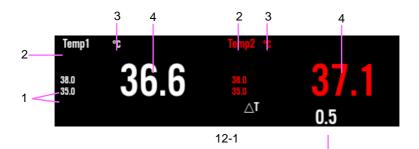

5

- 1 Temperature alarm limits
- 2 Temperature site
- 3 Temperature unit
- 4 Temperature value
- 5 Temperature difference (ΔT): Difference between two temperature sites.

12.4 Temp Monitoring Preparation

To prepare temperature monitoring, follow the steps below:

- 1. Select an appropriate probe for your patient according to patient type and measured site.
- 2. If an extension cable is needed, connect the temperature probe to the extension cable.
- Plug the probe or temperature cable to the temperature connector marked TEMP1 / TEMP2 on the left panel of the monitor. If using a disposable probe, connect the probe to the temperature cable.
- 4. Follow the probe manufacturer's instructions to connect the probe to the patient. Check that the settings are appropriate for the patient.

12.5 Changing Temp Settings

12.5.1 Setting Temp Menu

Enter Temp setup screen in either of the following ways:

- Press Temp parameter area.
- Press the [Parameters] quick key → select the [Temp] tab.
- Press[Main Menu]→[Parameters], select the [Temp] tab.

In Temp setup screen, you can perform the following operations:

- **[Temp1 Label]**: set the label of temperature channel 1 according to the measuring site.
 - Options: Temp1, Skin, Axil, Rectum.
- **[Temp2 Label]**: set the label of temperature channel 2 according to the measuring site.
 - Options: Temp2, Skin, Axil, Rectum.
- [Unit]: select the temperature unit.
 - Options: °C (centigrade), °F (Fahrenheit).

12.5.2 Setting Temp Alarms

To set the Temp alarm options, follow the steps below:

- 1. Access Temp alarm setup screen in either of the following ways:
 - Press the Temp parameter area → press the [Alarms] button.
 - Press the [Alarms] quick key → select the [Temp] tab.
 - Press[Main Menu]→[Alarms]→ select the [Temp] tab.
- 2. Set alarm properties as desired.

Chapter 13 Monitoring Non-Invasive Blood Pressure (NIBP)

13.1 Introduction

The monitor uses the oscillometric method to measure non-invasive blood pressure (NIBP). NIBP measurement is based on the principle that pulsatile blood flow through an artery creates oscillations of the arterial wall. A cuff is used to occlude the artery by inflating it above the patient's systolic pressure, the oscillometric devices measure the amplitude of pressure changes with pulsation in the cuff as the cuff pressure decreases. The pulsations increase in amplitude, and reach a maximum, then diminish along with the decrement of cuff pressure. The cuff pressure corresponding to the maximal pulse amplitude approximates to the mean artery pressure (MAP), the cuff pressure at the pulse amplitude backward reduced according to proper proportion is defined as systolic pressure (SYS), and the cuff pressure at the pulse amplitude forward reduced according to proper proportion is defined as diastolic pressure (DIA).

There are two kinds of NIBP measurement modules: KRK module and SunTech module. The monitor can automatically identify the module type.

NIBP monitoring is intended for adult, pediatric and neonatal patients.

13.2 Safety Information



⚠ Warning

Be sure to select the correct patient type setting for your patient before NIBP measurement. Do not apply the higher adult settings for pediatric or neonatal patients. Otherwise, it may present a safety hazard.



⚠ Warning

Before the measurement is carried out, select an appropriate measuring mode depending on the patient type (adult, pediatric or neonate).



⚠ Warning

When taking the blood pressure measurement on a neonatal patient, DO NOT operate in the Adult mode. The high inflation pressure may cause lesion or even body putrescence.



⚠ Warning

For SunTech NIBP module, when monitoring neonates, the monitor cannot identify the cuff type, so causing excessive cuff pressures on a neonate when taking the blood pressure measurement for a neonate in the "Adult" patient type setting. It is the responsibility of the user (physician or nurse) to always determine Adult or Neonate mode when initiating a BP measurement.



🔼 Warning

For KRK NIBP module, even though the monitor can identify the cuff type so it will stop inflation and indicate "Cuff error" when taking the blood pressure measurement for a neonate in the "Adult" patient type setting, the user (physician or nurse) should pay more attention to select the correct patient type.



⚠ Warning

NIBP monitoring is prohibited to those who have severe hemorrhagic tendency or with sickle cell disease, otherwise, partial bleeding will appear.



🖺 Warning

It is recommended to take the blood pressure measurement manually. Medical staff must be present when performing auto or sequential measurement.



Warning

DO NOT wrap the cuff on limbs with transfusion tube or intubations or skin lesion area, otherwise, injury may be caused to the limbs.



Warning

If the patient is moving or suffering tremble, hyperkinesia or arrhythmia, it may cause the inflation time of inflatable balloon endures longer, which may not only prolong the measurement time, but also result in the body wrapped by the cuff is troubled by purpura, hypoxemia and neuralgia because of the friction.



Warning

The air-hose which connects the cuff and monitor should be straightway without any tangle.



Caution

Prior to use of the cuff, empty the cuff until there is no residual air inside it to ensure accurate measurement.

Caution

DO NOT twist the air tube or put heavy things on it.

Caution

When unplugging the air tube, hold the head of the connector and pull it out.



Caution

The NIBP measurement will not be affected when the monitor is connected to the patient on whom the electro-surgical unit and defibrillator is being used.



Caution

The appearance of arrhythmia results in irregular heart beat which may affect the accuracy of NIBP measurement. It is recommended to take the measurement again at this situation.



Caution

The blood pressure measurements determined with this device are equivalent to those obtained by a trained observer using the cuff/stethoscope auscultatory method, within the limits prescribed by the American National Standard, manual, electronic, or automated sphygmomanometers.



The monitor can be used on the patients who are pregnant or pre-eclamptic, but close attention should be paid to such patients.



Caution

The performance of NIBP function can be affected by the extremes of temperature, humidity and altitude, please use it within the appropriate working environment.



The NIBP module of the device was clinically investigated according to the requirements of ISO 81060-2:2013.

13.3 Measurement Interferences

- The patient has serious angiospasm, vasoconstriction, or weak pulse.
- Do not take the measurement when the patient uses diuresis or vasodilator.

- Patients with severe bleeding tendency or sickle cells are forbidden to use the NIBP measurement, otherwise local bleeding may be caused.
- Do not apply cuff on the limb where skin damage has occurred or is expected.
- When extremely low or high heart rate or serious arrhythmia of the patient occurs. Especially auricular fibrillation will lead to unreliable or impossible measurement.
- When the patient is suffering from massive hemorrhage, hypovolemia, shock and other conditions with rapid blood pressure change or when the patient has too low body temperature, the reading will not be reliable, for reduced peripheral blood flow will lead to reduced arterial pulsation.
- For patients with severe coagulation disorders, it is necessary to determine whether to carry out automatic blood pressure measurement according to clinical evaluation, because there is a risk of hematoma at the friction between the limb and the cuff.

13.4 Measurement Modes

The following NIBP measurement modes are supported:

- Manual measurement on demand.
- Auto: repeated measurements at the set interval. Measuring at integral points are available.
- STAT: continual rapid series of measurements over a five-minute period, then return to the previous mode. The monitor will not stop making measurement until the measuring time is over 5 minutes or the operator stops it manually.
- Sequence: continual automatic measurement at set duration and interval of each stage.

In this mode, a complete measurement includes up to 7 phases (A, B, C, D, E, F, G). You can set the measurement duration of each cycle and the interval between two NIBP measurements.

 ABPM (ambulatory blood pressure monitoring): conduct NIBP measurements according to the set sequential mode.




"STAT" mode can only be used for adults.

Note

During the measurement in any mode, you can manually press the NIBP Start/Stop key " ot terminate the measurement.

13.5 NIBP Display

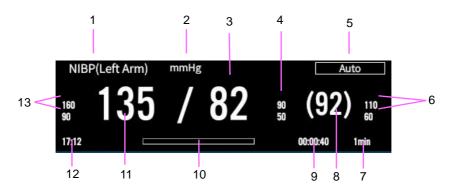

- 1 NIBP label and measurement site
- 2 NIBP unit: mmHg or kPa
- 3 Diastolic pressure
- 4 Diastolic pressure alarm limits. The alarm off icon is displayed when the alarm is set to off.
- 5 Measurement mode
- 6 Mean pressure alarm limits. The alarm off icon is displayed when the alarm is set to off.
- 7 For Auto NIBP, interval is displayed; for Sequence mode, the current phase and interval are displayed.
- 8 Mean pressure (displayed after measurement completed) or cuff pressure (displayed during the measurement)
- 9 Time to the next measurement (for Auto mode and Sequence mode)
- 10 Measurement progress bar
- 11 Systolic pressure
- 12 The last NIBP measurement time
- 13 Systolic pressure alarm limits. The alarm off icon is displayed when the alarm is set to off.

Note

NIBP measurement shows no waveform, only numerics are displayed in the parameter area.

Note

If NIBP measurement fails, "XX" is displayed; if NIBP measurement is not taken, "--" is displayed.

13.6 NIBP Monitoring Preparation


Before starting the NIBP measurement, make sure that the patient remains calm and is relaxed.

To place the NIBP cuff, follow the steps below:

Check to make sure that the patient type setting is correct.

- 1. Connect the cuff to the air tubing.
- 2. Connect the air tubing to the NIBP connector on the monitor. Avoid squeezing the pressure tubes. Air must pass unrestricted through the tubing.
- 3. Select an appropriate cuff according to the patient's age and limb circumference. The width of the cuff should be 40% (50% for neonates) of the limb circumference, or 2/3 of the length of the upper arm or the thigh. The inflatable part of the cuff should be long enough to encircle to overlap at least 50% to 80% of the limb.
- 4. Put on the cuff, unfold and wrap it around the patient's upper arm or thigh evenly to appropriate tightness.
- 5. Locate the cuff in such a way that the "ARTERY" mark "

 " is at a location where the clearest pulsation of brachial artery is observed. The cuff should fit snugly, but with enough room for two fingers to be placed between the cuff and the patient's arm (on adults), and loosely on neonates with little or no air present within the cuff. The cuff should be at the same level with the heart, and the lower end of the cuff should be 2cm above the elbow joint. As shown in the figure below:



(Caution

The wrong size of cuff may lead to inaccurate measurement results.



(Caution

Do not touch or apply external pressure against the cuff and air tubing during NIBP measurement. This may cause inaccurate blood pressure values.

13.7 Starting and Stopping NIBP Measurements

Use NIBP quick key or NIBP menu to start and stop NIBP measurement, as shown in the following table:

Task	By quick Key	From NIBP Menu
Start a manual measurement	Press the [Start NIBP] quick key	Select [Start NIBP] button
Start auto NIBP series	Select [Auto] for the measurement mode → set the measurement [Interval] → press the [Start NIBP] quick key	Select [Auto] for the measurement mode → set the measurement [Interval] → select the [Start NIBP] button
Start NIBP sequence measurement	Select [Sequence] for the measurement mode → set the sequential mode → press the [Start NIBP] quick key	Select [Sequence] for the measurement mode → set the measurement [Interval] → select the [Start NIBP] button
Start STAT measurement	/	Select the [NIBP STAT] button
Start ABPM measurement	Select [ABPM] for the measurement mode → set the sequential mode	Select [ABPM] for the measurement mode → set the sequential mode →

Task	By quick Key	From NIBP Menu
	→ press the [Start NIBP] quick key	select [Start NIBP] button
Stop the current NIBP measurements	Press the [Stop All] quick key	Select the [Stop All] button
End auto NIBP series or NIBP Sequence	Press the [Stop All] quick key	Select the [Stop All] button
End STAT measurement	Press the [Stop All] quick key	Select the [Stop All] button



⚠ Warning

Too frequent blood pressure measurements may cause purpura, ischemia and neuropathy in the limb with the cuff. Inspect the application site regularly to ensure skin quality and inspect the extremity of the cuffed limb for normal color, warmth and sensitivity. If any abnormality occurs, move the cuff to another place or stop the blood pressure measurement immediately.

Note

Start and stop NIBP measurement by pressing the NIBP Start/Stop key



13.8 Correcting the NIBP Measurements

The middle of the cuff should be at the level of right atrium. If the limb is not at the heart level, the measurement should be corrected as follows:

- Add 0.75mmHg (0.10kPa) to the displayed value for each centimetre higher.
- Deduct 0.75mmHg (0.10kPa) to the displayed value for each centimetre lower.

13.9 Changing NIBP Settings

13.9.1 Setting NIBP Menu

Enter NIBP setup screen in either of the following ways:

- Select the NIBP parameter area.
- Press the [Parameters] quick key → select the [NIBP] tab.

- Press[Main Menu]→[Parameters], select the [NIBP] tab.
 In the NIBP setup screen, you can perform the following operations:
- [Mode]: set the measurement mode.
 Options: Manual, Auto, Sequence, ABPM.
- [Limb]: select NIBP measurement site.
 Options: Left Arm, Right Arm, Left Leg, Right Leg.
- [Interval]: available only in "Auto" mode. Set the time interval between two NIBP measurements. When in "Auto" mode and the [Interval] is set, you must manually start NIBP measurement for the first time. The monitor starts the countdown and automatically starts the next NIBP measurement after reaching the set time interval.

Options: 1min, 2min, 2.5min, 3min, 5mins, 10min, 15min, 20min, 30min, 1h, 1.5h, 2h, 3h, 4h, 8h, Clock 30min, Clock 1h.

Clock: after the first measurement, the monitor automatically synchronizes NIBP automatic measurements with the real time clock. For example, if [Interval] is set to [Clock 30min], and NIBP auto measurement is started at 13:03, the next measurement will be taken at 13:30, and then at 14:00, 14:30, and so on.

Interval: after the first measurement, the monitor automatically repeats measurements at the set interval. For example, if [Interval] is set to [30min], and NIBP auto measurement is started at 13:03, the next measurement will be taken at 13:33, and then at 14:03, 14:33, and so on.

- [Initial Pressure]: set initial cuff inflation pressure. Its range is different depending on patient type. For the setting range of different patient types, see A. 11NIBP Specifications.
- [Sequential Mode]: Duration and Period can be selected.
 Select [Period] to set the starting time of the measurement.
 Select [Duration] to set the length of lasting time.
 This setting is available for [Sequence] and [ABPM] measurement modes.
- [Unit]: the pressure unit.
 Options: mmHg, kPa. 1kPa=7.5mmHg.

13.9.2 Setting NIBP Alarm Properties

To set NIBP alarm options, follow the steps below:

1. Enter the NIBP alarm setup screen in either of the following ways:

- Select the NIBP parameter area → press the [Alarms] button.
- Press the [Alarms] quick key → select the [NIBP] tab.
- Press[Main Menu]→[Alarms], select the [NIBP] tab.
- 2. Set alarm properties as desired.

13.9.3 Setting NIBP Measurement Timeout

NIBP measurements become outline fonts after a preset time. This feature prevents older values being misinterpreted as current measurements.

To adjust the timeout period for NIBP, follow the steps below:

- Press [Main Menu] → [Maintenance] → input password → press [Enter].
- 2. Select the [Module] tab.
- 3. Set the [Valid BP Period] for [NIBP].

Options: 5min, 10min, 15min, 30min, 1h. The default is 10min.

13.9.4 Displaying NIBP List

You can choose to display multi sets of the most recent NIBP measurement results in the parameter area at the bottom area of the screen. To do so, follow the steps below:

- 1. Enter [Layout] screen in either of the following ways:
 - Press the [Screens] quick key → select the [Layout] tab.
 - Press[Main Menu]→[Screens], select the [Layout] tab.
- 2. Press the position where the NIBP list needs to be displayed in the parameter area, and select [NIBP] → [NIBP List] from the drop-down list.

In the NIBP list, each NIBP record contains blood pressure data (systolic pressure, diastolic pressure, mean pressure) and pulse rate from NIBP.

13.10 NIBP Analysis

The monitor supports the analysis of collected blood pressure data, and displays the statistical results of NIBP analysis.

13.10.1 Entering the NIBP Analysis Screen

Enter the NIBP Analysis screen in either of the following ways:

 Select the NIBP List in the parameter area on the screen, select [NIBP Analysis].

- Press the [Review] quick key → select the [NIBP List] tab, select [NIBP Analysis].
- Press [Main Menu] → [Review], select the [NIBP List] tab, select [NIBP Analysis].

13.10.2 Setting the NIBP Analysis

Set the following information before starting the NIBP analysis.

- Time interval: set the time interval for analysis, including [Start Time] and [End Time].
- Analysis period: [Full Day], [Daytime] and [Night] are optional.

Full Day: 00:00:00-24:00:00 Daytime: 06:00:00-22:00:00 Night: 22:00:00-06:00:00

13.10.3 Viewing NIBP Analysis Results

Press the [Query] button, the system will automatically extract and analyze the ambulatory blood pressure data, and display the statistical results of ambulatory blood pressure analysis in the selected time period.

The statistical results of blood pressure data analysis are as follows:

Data Label	Description
Min	The minimum values of systolic pressure, diastolic pressure, mean arterial pressure and pulse measurement in the selected time interval.
Average	The average values of systolic pressure, diastolic pressure, mean arterial pressure and pulse measurement in the selected time interval.
Max	The maximum values of systolic pressure, diastolic pressure, mean arterial pressure and pulse measurement in the selected time interval.
SD	The standard deviations of systolic pressure, diastolic pressure, mean arterial pressure and pulse measurement in the selected time interval.
CV	The coefficient of variations of systolic pressure, diastolic pressure, mean arterial pressure and pulse measurement in the selected time interval.
SYS Load	The percentage of SBP measurements greater than the set SBP threshold.
DIA Load	The percentage of DBP measurements greater than the set

Data Label	Description
	DBP threshold.
AASI	Ambulatory Arterial Stiffness Index
Diurnal Rhythm	Blood pressure changes in a cycle of about 24 hours, the default is Dipper type blood pressure.
SYS Max	The time and date when the maximum systolic pressure value occurs in the selected time interval.
SYS Min	The time and date when the minimum systolic pressure value occurs in the selected time interval.
DIA Max	The time and date when the maximum diastolic pressure value occurs in the selected time interval.
DIA Min	The time and date when the minimum diastolic pressure value occurs in the selected time interval.
Number of Records	The total number of measurements in the selected time interval.
Valid Record Time	The total measurement time in the selected time interval.

13.11 Assisting Venous Puncture

Inflate the NIBP cuff to cause sub-diastolic pressure to block the venous blood vessel and therefore help venous puncture.

To assist venous puncture, follow the steps below:

- 1. Select the NIBP parameter area.
- 2. Set [Venipuncture].
- 3. Press the [Venipuncture] button at the bottom of the window to start inflating the cuff. At the same time, the NIBP parameter area will display the current cuff inflation pressure value and the remaining time of venipuncture.
- 4. Puncture vein and draw blood sample.
- Press the [Stop All] button at the bottom of the window, or press the [Stop All NIBP] quick key to deflate the cuff. If the cuff is not manually deflated, the cuff automatically deflates after a fixed period of time (170 seconds for adult and pediatric patient, 85 seconds for neonatal patient).

Caution

If your monitor is configured with SunTech NIBP module, then the cuff pressure range for adult is $120\sim180$ mmHg.

Note

During venous puncture, pressing the NIBP Start/Stop key "Cannot perform NIBP measurement."

13.12 Factors Affecting NIBP Measurement

Like common non-invasive blood pressure measurement, improper operation may cause inaccurate or blank result or misunderstanding of the measurement information when the oscillometric method is used to take the blood pressure measurement. These points need particular attention of the operators.

Requirements of the cuff:

- Appropriate cuff should be selected according to the age of the patient.
- Remember to empty the residual air in the cuff before the measurement is commenced.
- The cuff should be tightened to a degree where insertion of one finger is allowed.
- The lower end of the cuff should be 2cm above the elbow joint. Requirements for patient posture, setting and operation:
- The patient should be maintained at supine position so that the cuff and the heart are in a horizontal position and the most accurate measurement is taken. Other postures may lead to inaccurate measurement.
- Do not speak or move before or during the measurement. Care should be taken so that the cuff will not be hit or touched by other objects. The air tube which connects the cuff and monitor should be straight without any tangle.
- The measurement should be taken at appropriate intervals.
 Continuous measurement at too short intervals may lead to pressed arm, reduced blood flow and lower blood pressure, and resulting inaccurate measurement of blood pressure. It is

- recommended the measurement be taken at intervals of more than two minutes.
- Patients should be measured in a relaxed and calm state, otherwise the accuracy of blood pressure measurement data will be affected.
- When taking NIBP measurement on adult patients, the monitor may fail in giving the blood pressure measurement if the pediatric or neonate patient type is selected. When taking NIBP measurement on pediatric or neonatal patients, the operator must select correct patient type depending on different patients and do NOT operate with the adult patient type setting. The high inflation pressure for adult is not suitable for pediatric patients.
- With the oscillometric method, when blood pressure is measured, the inflation pressure of the cuff will be automatically adjusted according to the previous measurement. Generally, the initial inflation pressure is 160mmHg (for the adult mode) or 140mmHg (for pediatric) or 90 mmHg (for neonate) when it is powered on. When the blood pressure rises or the patient is changed, the sphygmomanometer may not be able to give the result after the first-time inflation. The monitor will automatically adjust the inflation pressure until the measurement is taken, after that, up to four times retry will be allowed.
- If the original parts are replaced with parts not provided by the manufacturer, it may cause measurement errors.

Chapter 14 Monitoring Invasive Blood Pressure (IBP)

14.1 Introduction

IBP monitoring can realize real-time monitoring of blood pressure changes during some heart surgeries and other major operations.

The monitor can monitor up to two-channel invasive blood pressures and displays the systolic, diastolic and mean blood pressures and a waveform for each pressure channel. IBP is measured by means of a catheter inserted directly into the circulatory system. A pressure transducer connected to the catheter converts the mechanical force exerted by the blood into an electrical signal, which is displayed graphically and numerically on the monitor screen.

IBP monitoring is intended for adult, pediatric, and neonatal patients.

14.2 Safety Information



All invasive measurements bring risks to patients. Use aseptic technology in the measurement and follow the accessory manufacturer's instructions.

⚠ Warning

Do Not use the damaged or expired pressure tube and transducer.

⚠ Warning

Use only the pressure transducer specified in this manual. Never reuse disposable pressure transducers.

⚠ Warning

The pressure tube which connects the catheter and the pressure transducer should be straightway without any tangle.

⚠ Warning

If air bubble appears in pressure tube, please fill the tube with saline solution again. Air bubble may cause inaccurate readings.

⚠ Warning

If measuring intracranial pressure (ICP) for the patient who is sitting, please keep the pressure transducer and the top of patient's ear at the same level. Incorrect leveling may give incorrect values.



⚠ Warning

Use the accessories specified by the manufacturer, when a defibrillator is



⚠ Warning

Improper use of a defibrillator may cause injury to the patient. The user should determine whether to perform defibrillation or not according to the patient's condition.



⚠ Warning

Before defibrillation, the user must ensure both defibrillator and monitor have passed the system test and can be safely used jointly.



⚠ Warning

Each time when connecting transducer kit or using a new transducer kit, zero calibration to the IBP transducer must be carried out.



⚠ Warning

Make sure that the applied parts never contact other conductive parts.



⚠ Warning

When using accessories, their operating temperature should be taken into consideration. For details, refer to instructions for use of accessories.



⚠ Warning

Mechanical shock to the invasive blood pressure transducer may cause severe shifts in zero balance and calibration, and cause inaccurate readings.



4 Warning

To reduce the hazard of burns during high-frequency surgical procedures, ensure that the monitor's cables and transducers never come into contact with the high-frequency surgical units.



⚠ Warning

Disposable IBP transducer cannot be reused.



When unplugging the cable from the monitor, be sure to hold the head of the connector and pull it out.




Before using the tube, cable and/or transducer, make sure that all accessories meet the performance requirements which is not changed by aging or environmental conditions.

14.3 IBP Display


IBP waveform area

The monitor can display 2 channels of IBP pressure waveform.

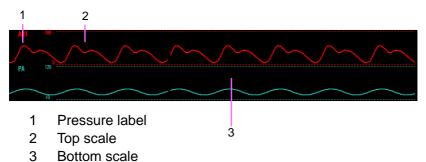

IBP parameter area

The monitor can display 2 pressure measurements.

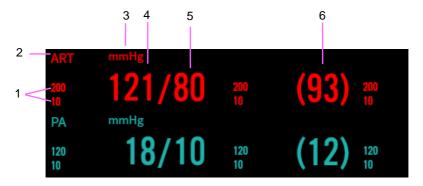

- 1 Alarm limits. The alarm off icon is displayed when the alarm is set to off.
- 2 Pressure label
- 3 IBP unit: mmHg or kPa
- 4 Systolic pressure
- 5 Diastolic pressure
- 6 Mean pressure

14.4 IBP Monitoring Preparation

To prepare IBP measurement, follow the steps below:

- 1. Plug one end of the IBP cable into the corresponding IBP connector on the left side of the monitor, and the other end to the IBP transducer.
- Flush the IBP transducer system to exhaust all air from the 2. catheter according to the manufacturer's instructions. Ensure that the system is free of air bubbles.
- Connect the IBP transducer to the patient, making sure that the 3. transducer is at the same horizontal level with the patient's heart.
- Select the proper pressure label for currently measured 4. pressure. For more information, see 14.5.1Setting IBP Menu.
- Zero the IBP transducer. After a successful zeroing, turn off the 5. three-way valve to the air and turn on the three-way valve to the patient.



Caution

Make sure that the cables of the transducer are not folded or twisted.



(T) Caution

Make sure that all air bubbles have been flushed from the IBP transducer system before making IBP measurements.



Caution

Make sure that all the transducers are zeroed correctly before making IBP measurements.

14.5 Changing IBP Settings

14.5.1 Setting IBP Menu

Enter IBP setup screen in either of the following ways:

- Select the IBP parameter area.
- Press the [Parameters] quick key → select the [IBP] tab.
- Press [Main Menu]→[Parameters], select the [IBP] tab.

The system enters the IBP1 setting window by default, you can switch to the IBP2 setting window.

In the IBP Setup screen, you can perform the following operations:

[IBP Label]: select the appropriate pressure label.

Label	Description	Label	Description
-------	-------------	-------	-------------

Label	Description	Label	Description
ART	Arterial blood pressure	PA	Pulmonary artery pressure
CVP	Central venous pressure	RAP	Right atrial pressure
LAP	Left atrial pressure	ICP	Intracranial pressure
P1	Auxiliary pressure 1	P2	Auxiliary pressure 2

P1 / P2 can be chosen if the actual measuring pressure is not in the list of ART, PA, CVP, RAP, LAP, and ICP.



Caution

The same label cannot be selected for different pressures.

[Calculation Mode]: Available only when the [IBP Label] is P1 or P2.

Options: Dynamic, Static.

In dynamic calculation, systolic blood pressure, diastolic blood pressure and mean pressure were measured

In static calculation, only mean pressure was measured.

- [Average Time]: the time period for averaging to calculate Mean Pressure. The setting range is 1~12s. The default value is 8s.
- [Pressure Unit]: options: mmHg, kPa. After setting the unit, the set unit will be displayed in the IBP parameter area. The units of IBP and NIBP are consistent.
- **[CVP Unit]**: options: mmHg, kPa, cmH2O, defaulting to mmHg.
- **[ICP Unit]**: options: mmHg, kPa, cmH2O, defaulting to mmHg.
- **[Speed]**: IBP waveform sweeping speed. The larger the value, the faster the sweeping speed.

Options: 6.25mm/s, 12.5mm/s, 25mm/s, 50mm/s.

• **[Filter]**: the pressure waveform filtering.

Options: 12.5Hz, 40Hz.

- **[Scale]**: Can be set to Auto and Manual. If Auto is selected, the size of the pressure's waveform will be adjusted automatically.
- **[Top Scale]**: Set the top scale of IBP waveform.
- [Bottom Scale]: Set the bottom scale of IBP waveform.
- [Zero IBP]: perform zero calibration for pressure transducer.

Press the [Zero IBP] button, a dialog box pops up on the screen, then press [Zero] to start calibration. After the zero calibration is completed, the message "Zero succeeded" will be displayed. If zero calibration fails, corresponding message will also be displayed.



Caution

Before performing zero calibration, please make sure that the transducer is well connected, otherwise the zero calibration cannot be carried out.

14.5.2 Setting IBP Alarm Properties

To set IBP alarm options, follow the steps below:

- Enter the IBP alarm setup screen in either of the following ways:
 - Press[Main Menu]→[Alarms], select the [IBP] tab.
 - Press the [Alarms] quick key → select the [IBP] tab.
 - Select the IBP parameter area → press the [Alarms] button.
- 2. Set alarm properties as desired.

14.5.3 Setting the Priority of the IBP No Transducer Alarm To set the priority of the IBP no transducer alarm, follow the steps below:

- Press [Main Menu] → [Maintenance] → input password → 1. press [Enter].
- Select the [Alarm] tab. 2.
- Set [IBP No Transducer] to [High], [Med]or [Low]. The default is 3. Low.

Chapter 15 Monitoring Carbon Dioxide (CO₂)

15.1 Introduction

 ${\rm CO_2}$ measuring principle is based on the fact that ${\rm CO_2}$ molecules absorb infrared light energy of specific wavelengths, with the amount of energy absorbed being directly related to the ${\rm CO_2}$ concentration. When an IR light beam is passed through a gas sample containing ${\rm CO_2}$, the electronic signal from a photo detector (which measures the remaining light energy), can be obtained. This signal is then compared to the energy of the IR source, and calibrated to accurately reflect ${\rm CO_2}$ concentration in the sample.

 CO_2 measurement is used to monitor the patient's respiratory status. The monitor provides the mainstream and sidestream methods for CO_2 monitoring.

- Mainstream measurement: directly insert a mainstream CO₂ sensor attached to an airway adapter into the patient's breathing system, allowing the inspired and expired gas to pass directly across the IR light path. The major advantages of mainstream sensors are fast response time and elimination of water traps. When using mainstream CO₂ sensors, check the window for the patient secretions pooled on periodically. Because that condition may affect the accuracy of the measurement or even make the sensor not work.
- Sidestream measurement: sidestream CO₂ sensors are located away from the airway, requiring a gas sample to be continuously aspirated from the breathing circuit and transported to the sensor by means of a pump. This type of system is needed for non-intubated patients. When using sidestream CO₂ sensors, there is a water trap or a part of the sampling tube with dehumidifying function. Please periodically check the flow sensor and tubing for excessive moisture or secretion buildup.

CO₂ monitoring is intended for adult, pediatric and neonatal patients.

15.2 Safety Information



Use the manufacturer approved accessories only.



Explosion Hazard: DO NOT use in the presence of flammable anesthetics or other flammable gasses. Use of the CO_2 Sensor in such environment may present an explosion hazard.



Electric Shock Hazard: Do not open the sensor cabinet at will, the CO₂ Sensor contains no user serviceable parts.

⚠ Warning

Electrical Shock Hazard: Always disconnect the CO_2 Sensor before cleaning. Do NOT use if it appears to have been damaged. Contact service personnel for help.

⚠ Warning

DO NOT sterilize or immerse the CO₂ sensor in liquids.

⚠ Warning

Do not use the CO₂ sensor when it is wet or has exterior condensation.

⚠ Warning

Do not apply excessive tension to any sensor cable or pneumatic tubing.

⚠ Warning

If the CO_2 sensor fails to respond as described in this manual, do not use it until approved for use by qualified personnel.

⚠ Warning

Reuse, disassembly, cleaning, disinfecting the single patient use CO₂ cannula kits and on-airway adapters may compromise functionality and system performance, leading to a user or patient hazard. Performance is not guaranteed if an item labeled as single patient use is reused.

⚠ Warning

Inspect the sidestream on-airway adapters and sidestream sampling kits for damage prior to use. DO NOT use the sidestream on-airway adapters and sidestream sampling kits if they appear to be damaged or broken.

⚠ Warning

If the CO_2 waveform (Capnogram) appears abnormal, inspect the CO_2 airway adapters and replace if needed.



⚠ Warning

Place the exhaust vent of the CO₂ sensor in drafty ambient and do not let anything block the exhaust vent.



⚠ Warning

Periodically check the CO₂/Flow sensor and tubing for excessive moisture or secretion buildup. Do not use them if there is excessive moisture or exterior condensation.



4 Warning

Prevent electrostatic discharge (ESD) and electromagnetic interference (EMI) to and from other equipment.



4 Warning

DO NOT position the sensor cables or tubing in any manner that may cause entanglement or strangulation.



Caution

When changing sampling tube, it is suggested to choose the default sampling tube with dehumidifying function. The sampling tube without dehumidifying function may be easily blocked by excessive moisture. (Service life: ordinary sampling tube: 6~12 hours; the sampling tube with dehumidifying function: about 120 hours.)



Caution

If the measurement shows an abnormity caused by sampling tube block, please replace it.



Caution

The total length of the sampling tube and extending airway tube shouldn't be longer than 3 meters, too long may cause measurement abnormity. If using T connector sampling cannula kits, please insert the sampling tube with the tubes upward to avoid the effects of excessive moisture.



Caution

Cyclic pressure up to 10kPa (100cmH₂O) can affect the accuracy of measurement.



Caution

The monitor does not have automatic barometric pressure compensation function. Due to the different altitudes in different areas, set the barometric pressure value manually according to the local barometric pressure during CO₂ monitoring. For more information, see *Appendix D Typical Pressures* and CO2 Readings at Altitudes.



(I) Caution

When CO₂ monitoring is not required, disconnect the sampling line from the monitor.



(1) Caution

Do not block the airway. Do not squeeze or bend the sampling line.

Note

CO₂ sensor is a precision measurement component, please use it correctly and store it properly.

Note

Disposal of the CO₂ Sensor and its accessories should comply with national and/or local requirements.

Note

In the presence of electromagnetic devices (i.e., electrocautery), patient monitoring may be interrupted due to electromagnetic interference. Electromagnetic fields up to 20V/m will not adversely affect system performance.

Note

Nitrous oxide, elevated levels of oxygen, helium and halogenated hydrocarbons can influence the CO₂ measurement.

Note

Excessive moisture in the CO₂ may affect the accuracy of the flow measurement.


15.3 CO₂ Display

CO₂ waveform area



- Parameter label
- 2 CO₂ waveform gain

CO₂ parameter area

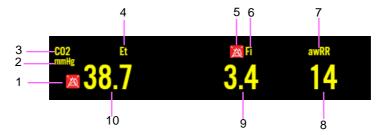

- 1 End tidal CO₂ alarm limits. The alarm off icon is displayed when the alarm is set to off.
- 2 CO₂ Unit
- 3 Label of CO₂
- 4 Label of end tidal CO₂ (EtCO₂)
- 5 FiCO₂ alarm limits. The alarm off icon is displayed when the alarm is set to off.
- 6 Label of fraction of inspired CO₂ (FiCO₂)
- 7 Airway respiration rate (awRR)
- 8 awRR value
- 9 FiCO₂ value
- 10 EtCO₂ value

15.4 Zeroing the CO₂ Sensor

In the CO_2 setup screen, press the [Zero] button to open a dialogue window for CO_2 zero calibration. At this time, place the sampling kit of the CO_2 sensor in a drafty place. Then press the [Zero] button in the dialogue window to perform the zero-resetting. The current zero

status will be displayed in the dialogue window. There are three effective zero status: Zeroing, Zero succeeded, Zero failed.

⚠ Warning

When perform a zero calibration during the measurement, disconnect the sensor from the patient's airway first.

⚠ Warning

Please do not rely on the readings during zeroing.

Note

The message of zero status prompts during zero calibration, but there is no audible and visual alarm.

15.5 Connecting CO₂ Sensor

15.5.1 Connecting the Sidestream CO₂ Sensor

To connect the sidestream CO₂ sensor, follow the steps below:


- 1. Insert one end of the CO₂ sensor cable into the connector marked "CO₂" on the connector panel of the monitor.
- 2. Insert the sampling tubing with adapter into the CO₂ sensor as shown in the figure below:




- After finishing sensor connection, make sure that the air inlet of the sampling tube is exposed to room air and away from all sources of CO₂, including the ventilator, the patient's and operator's breathing.
- 4. Wait 2 minutes for the sensor to warm up.

15.5.2 Sidestream Tubing Types


Default tubing configuration
 Adapter and sampling tube (single patient use)




Extended airway tube for connecting to sampling tube (Single patient use)



Optional sampling cannula kits
 T connector sampling cannula kits



Nasal sidestream cannula kits




Oral sidestream cannula kits




15.5.3 Connecting the Mainstream CO₂ Sensor

To connect the mainstream CO₂ sensor, follow the steps below:

- Insert on end of the CO₂ sensor cable into the connector marked with "CO₂" on the connector panel of the monitor.
- Select an appropriate airway connector and connect it with the adapter, then insert the CO₂ adapter into the CO₂ sensor as shown in the figures below:

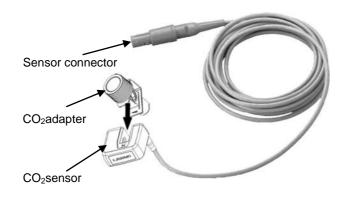

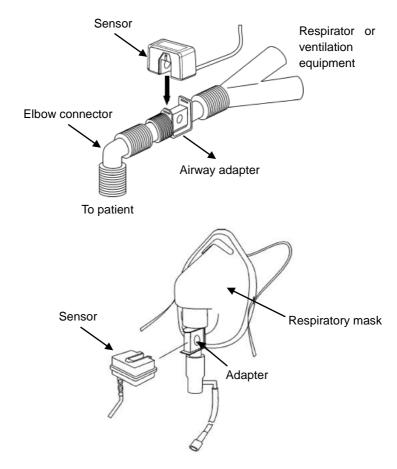

- After finishing sensor connection, make sure that the air inlet of the sampling tube is exposed to room air and away from all sources of CO₂, including the ventilator, the patient's and operator's breathing.
- 4. Wait 2 minutes for the sensor to warm up.

15.6 Changing CO₂ Parameter Settings

15.6.1 Setting CO₂ Menu

Enter CO₂ setup screen in either of the following ways:

- Select the CO₂ parameter area.
- Press the [Parameters] quick key → select the [CO₂] tab.
- Press [Main Menu] → [Parameters], select the [CO₂] tab.

In the CO₂ Setup screen, you can perform the following operations:

- [Speed]: CO₂ waveform sweeping speed.
 - The larger the value, the faster the sweeping speed.
 - Options: 6.25mm/s, 12.5mm/s, 25mm/s, 50mm/s.
- [Gain]: gain times, used to adjust the amplitude of CO₂ waveform.

The greater the gain, the higher the amplitude of waveform.

Options: x1/4, x1/2, x1, x2, x4.

The basic gain is 10mm/mV.

X1/4: one quarter scale size of the base gain

X1/2: half scale size of the base gain

X1: waveform scale with base gain

X2: twice scale size of the base gain

X4: four times scale size of the base gain

- [Unit]: set the CO₂ measurement unit.
 - Options: %, kPa and mmHg. If the unit is changed, then the parameter value will change and refresh timely. The unit will be displayed on parameter area.
- **[Temp(°C)]**: set the temperature value of the current measured air flow. Setting range: 0.0~50.0.The default is 35.0.
- **[CO2 Flow]**: set the flow rate of the CO₂ sampling. Its value is 50ml/min.
- **[Period]**: set the calculating cycle of the CO₂ value.

Options: 1b (calculate once every respiration cycle), 10s (calculate once every 10 seconds) and 20s (calculate once every 20 seconds).

 [Balance Gas]: set the balance gas in patient's respiration air flow

There are three kinds of selectable balance gas: "Air", "N2O" and "He", namely: air, nitrous oxide and helium. If no specific balance gas is given, the balance gas can be set as "Air".

- [Gas Compensation]: adjust the concentration of the compensating gas in patient's respiration air flow. Generally, the compensating gas is Oxygen, so it can be called oxygen compensation concentration. Setting range: 1~100; Unit: %; Default value: 16.
- **[AG]**: set whether adding the anesthetic gas to patient's respiration air flow and the concentration of anaesthetic gas. Setting range: 0.0~20.0; Unit: %; Default value: 0. The default status is not adding anaesthetic gas, that's to say, the concentration is 0.0%.
- [Atmospheric Pressure]: set ambient atmospheric pressure.
 Setting range: 400~850; Unit: mmHg.
 It can be determined by barometer or the ambient altitude.
 Altitude can be used to determine the typical barometric pressure if a barometer is not available, refer to Appendix D Typical Pressures and CO2 Readings at Altitudes for details.

15.6.2 Setting CO₂ Alarm Properties

To set CO₂ alarm options, follow the steps below:

- 1. Enter CO₂ alarm setup screen in either of the following ways:
 - Select the CO₂ parameter area → press the [Alarms] button.
 - Press the [Alarms] quick key → select the [CO₂] tab.
 - Press [Main Menu] →[Alarms], select the [CO₂] tab.
- 2. Set alarm properties as desired.

15.7 Measurement Limitations

The following factors may influence the measurement accuracy:

- Leaks or internal venting of sampled gas.
- Mechanical shock.
- Cyclic pressure up to 10kPa (100cmH₂O).

• Other sources of interference, if any.

This page intentionally left blank.

Chapter 16 Review

16.1 Review Overview

You can review the trend data, events, 12-lead ECG analysis results and waveforms, full disclosure waveforms, and so on, through the Review screen. You can also view the trend data through the Minitrends screen, or the OxyCRG screen, so that you can understand how the patient's condition is developing.

To enter the Review screen:

Select the [Review] quick key, or select [Main Menu]→[Review]. The Review screen contains tabs to display trend data in tabular, graphic, or other forms.

16.2 Tabular Trends Review

The tabular trends review screen displays trend data in a tabular form.

In the tabular trends review screen, you can perform the following operations:

- Browse trend data in either of the following ways:
- Drag the slider on the time line left or right, to locate the trend data at a specific time. At the same time, the data displayed in the current screen will be refreshed accordingly.
- Press the [<<] or [>>] button on the right side of the time line, to jump to the previous or next tabular trend to observe more data.
- Slide your finger up and down on the screen to observe the data of other parameters.
- To change the tabular trend group, select the parameter label to be displayed in the pop-up menu of [Group Setup].
- To change the resolution of the tabular trend data, set the [Resolution]. The resolution of tabular trends defines the interval of displaying trend data displayed on the screen.

A short interval is especially suited for neonatal monitoring, where the clinical situation may change very quickly in a short time. In adult monitoring, where the patient's status typically changes more gradually, a longer interval may be more informative.

Resolution can be set to: 5s, 30s, 1min, 5min, 10min, 15min, 30min, 1h, 2h, 3h.

To print a tabular trends report, select [] or [] icon.

16.3 Graphic Trends Review

The graphic trends review screen displays trend data in a visual format.

In the graphic trends review screen, you can perform the following operations:

- Browse graphic trends in either of the following ways:
- Drag the slider on the time line left or right, or move the cursor (blue vertical line) on the trend graph, to locate the trend data at a specific time. At the same time, the data displayed in the current screen will be refreshed accordingly.
- Press the [<] or [>] button on the right side of the time line, to move the cursor to the left or right.
- Press the [<<] or [>>] button on the right side of the time line, to jump to the previous or next page of graphic trends.
- Slide your finger up and down on the screen to observe the graphic trends of other parameters.
- To change the graphic trend group, select the parameter label to be displayed in the pop-up menu of [Group Setup].
- Select [Zoom] to set the length of trend data displayed on the current screen.
 - Options: 5min, 10min, 15min, 30min, 1h, 2h, 4h, 8h, 12h, 24h, 48h.
- To print a graphic trends report, select [] or [] icon.

16.4 NIBP List Review

The monitor can display the latest 2000 groups of NIBP measurement data in the NIBP List review screen. All measurement data can't be displayed on the current screen due to the screen limitation. The current screen can display up to 7 groups of measurement data. You can switch the screen manually to see more measurement data. If the monitor has stored 2000 groups of data, if new data is generated, the earliest data will be discarded.

Enter the NIBP List review screen in either of the following ways:

- Select the NIBP List in the parameter area on the screen.
- Press the [Review] quick key → select the [NIBP List] tab.
- Press [Main Menu] → [Review], select the [NIBP List] tab.

In the NIBP List review screen, you can perform the following operations:

- Press the [<<] or [>>] button in the lower right corner of the screen to turn the page to view the NIBP measurement data.
- Press the page area to select the required page number to view the NIBP measurement data.
- Press [NIBP Analysis] to enter the NIBP analysis screen. For more information, see 13.10 NIBP Analysis.

16.5 Events Review

The monitor stores events in real time. You can view arrhythmia events, manual events, physiological alarm events, technical alarm events and alarm logs in the Events review screen.

The Events screen displays the event list. Events are displayed in descending chronological order, with the most recent displayed at the top.

To configure the filter, select [Filter Setup] and set the desired filter criterion.

- You can filter events by the alarm priority for arrhythmia events.
- You can filter events by the alarm priority or parameter group for physiological and technical alarm events.

16.6 Full Disclosure Review

You can review up to 140 hours of waveform data on the full disclosure review screen.

You can view the compressed waveforms, full waveforms and numeric values.

In the Full Disclosure screen, you can also perform the following operations:

- Browse full disclosure waveforms in either of the following ways:
- Drag the slider on the time line left or right, to locate the waveform at a specific time.
- Press the [<<] or [>>] button on the right side of the time line, to jump to the previous or next full disclosure waveforms.
- Slide your finger up and down on the screen to observe the waveforms at other time points.
- Select [Lead] to set the desired waveforms to be stored and displayed. Up to three channels of waveforms can be displayed.

- Options: ECG(I), ECG(II), ECG(III), ECG(aVR), ECG(aVL), ECG(aVF), ECG(V1), ECG(V2), ECG(V3), ECG(V4), ECG(V5), ECG(V6).
- Select [Duration] to set the length of displayed waveforms. Options: 1min, 2min, 5min and 10min.
- Select ECG waveform speed from the speed pop-up list.
 Options: 6.25mm/s, 12.5mm/s, 25mm/s, 50mm/s.
- Select the gain of ECG waveforms in the gain pop-up list.
 Options: x 1/4, x 1/2, x 1, x 2.
- Select [Detail] to view the full waveforms and parameter values. You can perform the following operations on this screen:
- Select ECG waveform speed from the [Speed] pop-up list. Options: 6.25mm/s, 12.5mm/s, 25mm/s, 50mm/s.
- Select the gain of ECG waveforms in the [Gain] pop-up list. Options: x 1/4, x 1/2, x 1, x 2.
- Select [Overview] to switch to the compressed waveform screen.
- [12-Lead ECG]: when 12-lead ECG analysis function is configured, after selecting the start time of the waveform, press this button to conduct 12-lead ECG analysis for the waveform of the selected time length. For more information, see8.4Initiating 12-Lead ECG Acquisition.
- [Holter]: after selecting the start time of the waveform, press this button to conduct ambulatory ECG analysis for the waveform of the selected time length. For more information, see 9.3 Initiating Ambulatory ECG Acquisition.
- Select [HRV] to enter the HRV analysis preview screen.
 In this screen, you can view the statistical results of HRV analysis, including HR trend chart, R-R interval histogram, R-R interval difference histogram, R-R interval scatter plot, R-R interval difference scatter plot, and HRV parameter calculation value list.
- To print a compressed waveform report, select [] or [] icon.

16.7 ST Review

When ST analysis is enabled, you can view the ST segments and values saved by the monitor in the ST review screen.

In the ST review screen, you can perform the following operations:

- In the pop-up menu of [Trend Group], select ST lead and HR.
- Select [Zoom] to set the length of data displayed on the current screen. Options: 8min, 30min, 1h, 2h, 4h, 8h, 12h, 24h, 48h.
- Select [Detail] to view the ST segment details of the current time.
 - In the ST segment details screen, you can perform the following operations:
- View the anterior (V1-V4), inferior (II, III, aVF, aVR) and lateral (I, aVL, V5, V6) ST segments.
- Select [Save Ref.] to save the currently displayed ST segment as the ST reference. The save is temporary and lost after the monitor is switched off or discharging the patient.
- Select [Display Ref.] or [Hide Ref.] to display or hide ST reference. When [Display Ref.] is selected, the current ST segment and ST reference are displayed in the waveform area, and the ST reference time is displayed on the bottom of the waveform area.
- Select [Display Marker] or [Hide Marker] to display or hide markers.
- > Select [Trends] to return to the trend chart screen.
- To print ST data, select [3] or [6] icon.

16.8 OxyCRG Review

The OxyCRG screen displays the trend curves of HR, SpO₂, Resp, RR and EtCO₂. HR and SpO₂ are displayed by default, other parameters are configurable.

16.8.1 Entering the OxyCRG Screen

Enter the [OxyCRG] screen in either of the following ways:

- Press the [OxyCRG] quick key.
- Press the [Screens] quick key → select [OxyCRG].
- Press [Main Menu] → [Screens], select [OxyCRG].

In the OxyCRG screen, you can perform the following operations:

- Select the length of data displayed on the current screen from the Zoom popup list.
- Options: 1min, 2min, 4min, 8min. The default is 2min.
- Select the parameter label in the parameter pop-up list.

- Options: Resp, RR, EtCO₂. The default is Resp.
- Press the [Review] button to enter the OxyCRG review screen.

16.8.2 Exiting the OxyCRG Screen

Exit the [OxyCRG] screen in either of the following ways:

- Press the [x] button in the upper right corner of the [OxyCRG] screen. Press the [Screens] quick key, select the screen to be entered.
- Press [Main Menu] → [Screens], select the screen to be entered.

16.8.3 Entering the OxyCRG Review Screen

You can review up to 24 hours of trend curves on the OxyCRG review screen.

Enter the [OxyCRG] review screen in either of the following ways:

- Press the [OxyCRG] quick key → [Review].
- Press the [Review] quick key → select [OxyCRG].
- Press [Main Menu] → [Review], select the [OxyCRG] tab.

In the OxyCRG Review screen, you can perform the following operations:

- On the left side of the screen displays the OxyCRG events list, you can view the parameter trends, compressed waveform, and parameter values of the selected event.
- Select [Zoom] to set the length of data displayed on the current screen. Options: 5min, 10min, 30min, 1h, 2h, 4h, 8h, 12h, 24h. The default is 8h.
- To print an OxyCRG review report, select [] or [] icon.

16.9 Minitrends Screen

The Minitrends screen shows the recent graphic trends of parameters.

16.9.1 Entering the Minitrends Screen

Enter the [Minitrends] screen in either of the following ways:

- Press the [Minitrends] quick key.
- Press the [Screens] quick key → select [Minitrends].
- Press [Main Menu]→[Screens], select [Minitrends].

On the Minitrends screen, the parameter label is displayed above each trend curve, the scale is on the left side, and the time line is at the bottom of the screen.

16.9.2 Exiting the Minitrends Screen

Exit the [Minitrends] screen in either of the following ways:

- Press the [Screens] quick key, select the screen to be entered.
- Press [Main Menu]→[Screens], select the screen to be entered.

16.10 Screenshot Review

The monitor provides the function of screen capture. Press the [Screenshot] quick key (configurable) to capture and save the current screen display to the monitor.

In the Screenshot review screen, you can perform the following operations:

- On the left side the screen displays the screenshot records list, you can view the details of the captured pictures.
- Select the [Rename] button to modify the name of the selected screenshot.
- To print the selected screenshot, select [1] icon.

Chapter 17 Calculations

17.1 Introduction

The monitor provides calculation function. The calculated values, which are not directly measured, are computed based on the values you provide.

You can perform the following calculations:

- Drug calculations
- Hemodynamic calculations
- Oxygenation calculations
- Ventilation calculations
- Renal calculations



Check that the entered values are correct and the calculated values are appropriate. We assume no responsibility for any consequences caused by wrong entries and improper operations.



The calculation function is independent of other monitoring functions and can therefore be used for patients being monitored by other monitors. Any operation in a calculation window does not affect the patient monitored by the current monitor.

17.2 Drug Calculations

The monitor provides the dosage calculation for 30 kinds of medicine, including: Aminophylline, Dobutamine, Dopamine, Adrenaline, Heparin, Lidocaine, Nitroglycerin, Sodium Nitroprusside, Isoproterenol, Oxytocin, Diltiazem, Esmolol, Fentanyl, Amrinone, Insulin, Labetalol, Lorazepam, Midazolam, Milrinone, Nicardipine, Norepinephrine, Phenylephrine, Procainamide, Propofol, Vasopressin, Drug A, Drug B, Drug C, Drug D, Drug E. While Drug A through Drug E are user defined.

17.2.1 Calculation Procedure

To perform drug calculation, follow the steps below:

- 1. Enter the drug calculation screen in either of the following ways:
 - Press the [Calculations] quick key, select the [Drug] tab.
 - Press [Main Menu] → [Calculations], select the [Drug] tab.

- 2. Set [Drug Name] and [Patient Type]. If the dose of drug is weight dependent, you must switch on [Weight Based] and input the patient's weight.
- 3. Enter the known values, for example Drug Amount and Solution Volume.
- 4. Press the [Calculate] button to do the calculation. The calculated values are displayed on the screen automatically.

17.2.2 Checking the Titration Table

When the concentration calculation of a drug is OK in the first tab, the titration table in the second tab ("Titration Table") can be browsed. Use the titration table to see what dose of a drug your patient will receive at different infusion rates.

• [Calculation Based]: to make item as the independent variable, other items will be dependent variables.

Options: Dose, Infusion Rate

[Infusion Rate]: by selecting it, the titration table is listed in the sequence of increased infusion rate.

[Dose]: by selecting it, the titration table is listed in the sequence of increased drug dose.

- [Step]: set the interval between two adjacent titration table items.
- [Dose Type]: set the type of dose unit in the titration table.
 Options: Dose/min, Dose/h, Dose/kg/min, Dose/kg/h.
 The changing of unit will cause the re-calculation of [Infusion Rate] according to formulas mentioned in the next section.

17.2.3 Drug Calculation Formula

Description Unit		Formula	
Drug Amount	g series: mcg, mg, g Unit series: Unit, kU, MU	Drug Amount = Dose × Infusion Duration	
	mEq series: mEq		
Drug Amount (weight based)	g series: mcg, mg, g Unit series: Unit, kU, MU mEq series: mEq	Drug Amount (weight based) = Dose × Infusion Duration × Weight	
Solution	ml	Solution Volume = Infusion	

Description	Unit	Formula
Volume		Rate x Infusion Duration
Dose	Dose/h, Dose/min	Dose = Infusion Rate x Concentration
Dose (weight based)	Dose/kg/h, Dose/kg/min	Dose (weight based) = Infusion Rate × Concentration / Weight
Concentration	mcg/ml, mg/ml, g/ml, Unit/ml, KU/ml, MU/ml, mEq/ml	Concentration = Drug Amount / Solution Volume
Infusion Duration	h	Infusion Duration = Drug Amount / Dose
Infusion Duration (weight based)	h	Infusion Duration (weight based) = Drug Amount / (Dose x Weight)
Infusion Rate	ml/h	Infusion Rate = Dose / Concentration
Infusion Rate (weight based)	ml/h	Infusion Rate = Dose × Weight / Concentration

Remarks:

- Dose/h: refers to the dosage per hour
- Dose/min: refers to the dosage per minute
- (Dose/min) = (Dose/h) / 60
- Dose/kg/h: refers to the dosage per kilogram of body weight per hour
- (Dose/kg/h) = (Dose/h) / patient weight
- Dose/kg/min: refers to the dosage per kilogram of body weight per minute
- (Dose/kg/min) = (Dose/min) / patient weight

17.2.4 Titration Table Calculation Formula

Description	Unit	Formula
Infusion Rate	ml/h	Infusion Rate = Dose / Concentration
Infusion Rate (weight based)	ml/h	Infusion Rate = Dose × Weight / Concentration
Dose	Dose/h, Dose/min	Dose = Infusion Rate x Concentration
Dose (weight based)	Dose/kg/h, Dose/kg/min	Dose (weight based) = Infusion Rate × Concentration / Weight

17.3 Hemodynamic Calculations

17.3.1 Calculation Procedure

To perform hemodynamic calculation, follow the steps below:

- Enter the hemodynamic calculation screen in either of the following ways:
 - Press the [Calculations] quick key, select the [Hemodynamics] tab.
 - Press [Main Menu] → [Calculations], select the [Hemodynamics] tab.
- Enter the known values.
- 3. Press the [Calculate] button, the system will calculate the value of each output parameter according to the calculation formula.

An abnormal calculated value is indicated by a yellow background. An invalid calculated value is indicated by "---". A calculated value greater than the normal upper limit is indicated by an up arrow " \uparrow ". A calculated value lower than the normal lower limit is indicated by a down arrow " \downarrow ".

In the [Hemodynamics] screen, you can also perform the following operations:

- Select [Range] to view the normal range of each parameter.
- Select [Unit] to view the unit of each parameter.

17.3.2 Input Parameters for Hemodynamic Calculations

Input	Full Name /	Unit	Adjustable
Parameter	Description		Range
Height	Patient height	cm	20.0-300.0

Input Parameter	Full Name / Description	Unit	Adjustable Range
Weight	Patient weight	kg	0.1-499.0
HR	Heart rate	bpm	0-300
MAP	Mean arterial pressure	mmHg	0-300
CVP	Central venous pressure	mmHg	0-40
C.O.	Cardiac output	L/min	0.1-20.0
PAW	Pulmonary artery wedge pressure	mmHg	0-40
MPAP	Mean pulmonary artery pressure	mmHg	1-120
LVD	Axial diameter of left ventricle	mm	0-120

17.3.3 Output Parameters and Formulas for Hemodynamic Calculations

Output Parameter	Full Name /Description	Unit	Formula	Reference Range
C.I.	Cardiac Index	liters/min/ m ²	C.O. / BSA	2.5-4.0
SV	Stroke Volume	ml	C.O. / HR	60-100
SVI	Stroke Volume Index	ml/m²	SV / BSA	33-47
SVR	Systemic Vascular Resistance	Dynes-sec /cm ⁻⁵	79.96*(MAP - CVP) / C.O.	800-1200
SVRI	Systemic Vascular Resistance Index	dynes-sec /cm ⁻⁵ /m ²	SVR*BSA	970-2390
PVR	Pulmonary Vascular Resistance	dynes·sec /cm ⁻⁵	79.96*(paM AP-PAW) / C.O.	150-250
PVRI	Pulmonary Vascular Resistance Index	dynes-sec /cm ⁻⁵ /m ²	PVR*BSA	255-285
LCW	Left Cardiac Work	kg-m	0.0136*MA P*C.O.	5.4-10.0
LCWI	Left Cardiac Work Index	kg-m/m ²	LCW/BSA	3.0-5.5
LVSW	Left Ventricle Stroke Work	g·m	0.0136*MA P*SV	8-10
LVSWI	Left Ventricle Stroke Work Index	g·m/m²	LVSW/BSA	50-62
RCW	Right Cardiac Work	kg-m	0.0136 × paMAP × C.O.	
RCWI	Right Cardiac Work Index	kg-m/m ²	RCW/BSA	0.54-0.66

Output Parameter	Full Name /Description	Unit	Formula	Reference Range
RVSW	Right Ventricle Stroke Work	g⋅m	0.0136*paM AP*SV	51-61
RVSWI	Right Ventricle Stroke Work Index	g·m/m²	RVSW/BSA	5-10
EF	Ejection Fraction	m ²	(SV/t)*100	40-60

Remarks:

- BSA (Body Surface Area) = Weight 0.425 * Height 0.725 * 0.007184
- t = (7.0 / (2.4 + lv_d/10)) * lv_d * lv_d * lv_d / 1000 (lv_d: left ventricle diameter)
- paMAP corresponds to MPAP

17.4 Oxygenation Calculations

17.4.1 Calculation Procedure

To perform oxygenation calculation, follow the steps below:

- 1. Enter the oxygenation calculation screen in either of the following ways:
 - Press the [Calculations] quick key, select the [Oxygenation] tab.
 - Press [Main Menu] → [Calculations], select the [Oxygenation] tab.
- 2. Enter the known values.
- 3. Press the [Calculate] button, the system will calculate the value of each output parameter according to the calculation formula.

An abnormal calculated value is indicated by a yellow background. An invalid calculated value is indicated by "---".

A calculated value greater than the normal upper limit is indicated by an up arrow " \\dagger*".

A calculated value lower than the normal lower limit is indicated by a down arrow " \dagger*".

In the [Oxygenation] screen, you can also perform the following operations:

- Select [Range] to view the normal range of each parameter.
- Select [Unit] to view the unit of each parameter.

17.4.2 Input Parameters for Oxygenation Calculations

Input Parameter	Full Name / Description	Unit	Adjustable Range
Height	Height	cm	20.0-300.0
Weight	Weight	kg	1.0-250.0
C.O.	Cardiac output	L/min	0.1-20.0
Hb	Hemoglobin	g/L	50-200
RQ	Respiratory quotient		0.1-1.5
FiO2	Percentage fraction of inspired oxygen	%	18-100
CaO2	Arterial oxygen content	ml/L	10-400
ATMP	Atmospheric pressure	mmHg	300-1200
PaO2	Partial pressure of oxygen in the arteries	mmHg	10-800
CvO2	Venous oxygen content	ml/L	10-400
Partial pressure of carbon dioxide in the arteries		mmHg	0-200
VO2	Oxygen consumption	ml/min	50-1000

17.4.3 Output Parameters and Formulas for Oxygenation Calculations

Output Parameter	Full Name /Description	Unit	Formula	Reference Range
BSA	Body surface area	m ²	Wt ^{0.425} *Ht ^{0.725} *0.0 07184	
VO ₂ calc	Oxygen consumption	ml/mi n	(SaO2-SvO ₂)*13. 4*Hb * C.O.	
C(a-v)O ₂	Arteriovenous oxygen content difference	ml/L	CaO ₂ - CvO ₂	42-59
O₂ER	Oxygen extraction ratio	%	VO ₂ /(CaO ₂ *C.O.) *100	24-28
DO ₂	Oxygen delivery	ml/mi n	CaO ₂ * C.O.	950-1150
PAO ₂	Partial pressure of oxygen in the alveoli	mmH g	(FiO ₂ *100)*(ATM P-47)–(PaCO ₂ /R Q)	
AaDO ₂	Alveolar-arteri al oxygen difference	mmH g	(FiO ₂ *100)*(ATM P-47)–(PaCO ₂ /R Q)-PaO ₂	10-15
CcO ₂	Pulmonary capillary oxygen content	ml/L	(Hb*1.34)+((FiO ₂ *100)*(ATMP-47) -(PaCO ₂ / RQ))*0.0031)	
Qs /Qt	Pulmonary venous admixture	%	{[(Hb*1.34)+(((Fi O ₂ *100)*(ATMP- 47)-(PaCO ₂ /RQ)) *0.0031)]-CaO ₂)/{ [(Hb*1.34)+(((FiO ₂ *100)*(ATMP-47)-(PaCO ₂ /RQ))*0 .0031)]-CvO ₂ }*1 00	3.0-5.0
C.O.calc	Calculated cardiac output	L/min	VO ₂ / (CaO ₂ -CvO ₂)	0.1-20.0

Output Parameter	Full Name /Description	Unit	Formula	Reference Range
PaO ₂ /FiO ₂	Oxygenation index	mmH g	PaO ₂ /(FiO ₂ *100)	
AaO ₂ /PaO ₂	Ratio of alveolar-arteri al oxygen partial pressure difference to oxygen partial pressure		[(FiO2*100)*(AT MP-47)–(PaCO ₂ / RQ) - PaO ₂] / PaO ₂	
DO ₂ I	Oxygen delivery index	ml/mi n/m²	(CaO ₂ * C.O.)/BSA	
VO ₂ I	Oxygen consumption index	ml/mi n/m²	(CaO ₂ – CvO ₂)*C.O./BSA	

17.5 Ventilation Calculations

17.5.1 Calculation Procedure

To perform ventilation calculation, follow the steps below:

- Enter the ventilation calculation screen in either of the following ways:
 - Press the [Calculations] quick key, select the [Ventilation] tab.
 - Press [Main Menu] → [Calculations], select the [Ventilation] tab.
- Enter the known values.
- 3. Press the [Calculate] button, the system will calculate the value of each output parameter according to the calculation formula.

An abnormal calculated value is indicated by a yellow background. An invalid calculated value is indicated by "---".

A calculated value greater than the normal upper limit is indicated by an up arrow " \uparrow ".

A calculated value lower than the normal lower limit is indicated by a down arrow " \dagger*".

In the [Ventilation] screen, you can also perform the following operations:

- Select [Range] to view the normal range of each parameter.
- Select [Unit] to view the unit of each parameter.

17.5.2 Input Parameters for Ventilation Calculations

Input Parameter	Full Name / Unit		Adjustable Range
FiO ₂	Percentage fraction of inspired oxygen	%	18-100
PeCO ₂	End-tidal CO ₂ pressure	mmHg	0-114
PaO ₂	Partial pressure of oxygen in the arteries	mmHg	10-800
RQ	Respiratory quotient		0.1-1.5
ATMP	Atmospheric pressure	mmHg	300-1200
RR	Respiratory rate	rpm	4-120
PaCO ₂	Partial pressure of carbon dioxide in the arteries	mmHg	1-200
TV	Tidal volume	ml	15-2000

17.5.3 Output Parameters and Formulas for Ventilation Calculations

Output Parameter	Full Name /Description	Unit	Formula	Reference Range
PAO ₂	Partial pressure of oxygen in the alveoli	mmHg	FiO ₂ *(ATMP-47) -(PaCO ₂ / RQ)	
AaDO ₂	Alveolar-arteri al oxygen difference	mmHg	FiO ₂ *(ATMP-47) -(PaCO ₂ /RQ) - PaO ₂	
PaO ₂ /FiO ₂	Oxygenation index	mmHg	PaO ₂ /FiO ₂	
Pa/AO ₂	Arterial to alveolar oxygen ratio	%	PaO ₂ /(FiO ₂ *(AT MP-47)–(PaCO ₂ /RQ))	
AaDO ₂ /PaO ₂	Respiratory index		(FiO ₂ *(ATMP-47)–(PaCO ₂ /RQ)- PaO ₂)/PaO ₂	
MV	Minute volume	L/min	TV * RR / 1000	
Vd	Volume of physiological dead space	ml	((PaCO ₂ -PeCO ₂)/PaCO ₂)*TV	145-155
Vd/Vt	Physiologic dead space in percent of tidal volume	%	((PaCO ₂ -PeCO ₂)/PaCO ₂)*100%	25-40
VA	Alveolar volume	L/min	(TV-((PaCO ₂ -Pe CO ₂)/PaCO ₂)*T V) * RR	

17.6 Renal Function Calculations

17.6.1 Calculation Procedure

To perform renal function calculation, follow the steps below:

- 1. Enter the renal function calculation screen in either of the following ways:
 - Press the [Calculations] quick key, select the [Renal] tab.

- Press [Main Menu] → [Calculations], select the [Renal] tab.
- 2. Enter the known values.
- 3. Press the [Calculate] button, the system will calculate the value of each output parameter according to the calculation formula.

An abnormal calculated value is indicated by a yellow background. An invalid calculated value is indicated by "---".

A calculated value greater than the normal upper limit is indicated by an up arrow " \uparrow ".

A calculated value lower than the normal lower limit is indicated by a down arrow " \downarrow ".

In the [Renal] screen, you can also perform the following operations:

- Select [Range] to view the normal range of each parameter.
- Select [Unit] to view the unit of each parameter.

17.6.2 Input Parameters for Renal Function Calculations

Input Parameter	Full Name / Description	Unit	Adjustable Range
Height	Height	cm	20-300
Weight	Weight	kg	1-250
URK	Urine potassium	mmol/L	1-9999
URNa	Urine sodium	mmol/L	0-9999
Urine	24 hours urine	ml/24h	0-5000
Posm	Plasma osmolality	mOsm/kgH2O	100-500
Uosm	Urine osmolality	mOsm/kgH2O	200-2000
SerNa	Serum sodium	mmol/L	50-300
SCr	Serum creatinine	umol/L	45-90
UCr	Urine creatinine	umol/L	100-5000
BUN	Blood urea nitrogen	mmol/L	0-10

17.6.3 Output Parameters and Formulas for Renal Function Calculations

Output Parameter	Full Name / Description	Unit	Formula	Reference Range
URNaEx	Urine sodium excretion	mmol/2 4h	URNa*Urine/10 00ml	51-102
URKEx	Urine potassium excretion	mmol/2 4h	URK*Urine/100 0ml	
Na/K	Excretion ratio of urine sodium and potassium	%	URNa/URK*100 %	
CNa	Sodium clearance	ml/24h	(URNa*Urine)/S erNa	
Clcr	Creatinine clearance rate	ml/min	(Urine * UCr) / (SCr * 1440)	
FENa	Fractional excretion of sodium	%	(URNa*Scr)/(Se rNa*UCr) * 100%	
Cosm	Osmolar clearance	ml/min	(Uosm*Urine/24 /60)/Posm	
CH2O	Free water clearance	ml/h	V*(1-Uosm/Pos m)	-120~-25
U/Posm	Urine to plasma osmolality ratio		Uosm / Posm	3.0-4.5
BUN/Scr	Blood urea nitrogen-seru m creatinine ratio		BUN / Scr	
U/SCr	Urine-serum creatinine ratio		Ucr / Scr	

17.7 Early Warning Score (EWS)

The early warning score (EWS) can help you recognize the early sign of deterioration in patients based on vital signs and clinical

observations. Depending on the score calculated, appropriate recommendations are displayed.

The monitor supports the following scoring systems:

- NEWS (National Early Warning Score)
- MEWS (Modified Early Warning Score)
- CART (Cardiac Arrest Risk Triage)

There are two scoring type: total score and single parameter score.

- Total score: add all the subscores of each parameter selected to calculate the total early warning score. When the total score is out of range, actions are recommended.
- Single parameter score: a subscore is given for each parameter based on the entered value. When any subscore is outside of the thresholds, actions are recommended.



The EWS system is not applicable to pregnant women and people under 12 years old.



NEWS is not applicable to spinal cord injury (SCI) patients.

⚠ Warning

The EWS scores and recommended actions are for reference only and cannot be directly used for diagnostic interpretation.

⚠ Warning

EWS cannot be used as an index of prognosis. It is not a clinical judgement tool. Clinicians must use their clinical judgement in conjunction with the EWS tool at all times.

17.7.1 Scoring Parameters

Scoring parameters of each scoring systems are different, as shown in the table below:

Scoring System	Scoring Parameters
NEWS	Consciousness, Supply O ₂ (oxygen supply status), RR, PR, SpO ₂ , Temp, SBP (systolic pressure)
MEWS	Consciousness, RR, Temp, SBP (systolic pressure), HR
CART	RR, HR, DBP (diastolic pressure), Age

17.7.2 Displaying the EWS Parameter Area

To display the EWS parameter area, follow the steps below:

- Access [Layout] screen in either of the following ways:
 - Press the [Screens] quick key → select the [Layout] tab.
 - Press [Main Menu] → [Screens], select the [Layout] tab.
- Select the parameter area where you want to display the EWS 2. score, and then select [Timer] from the popup list.

17.7.3 Entering the EWS Screen

Enter the EWS screen in either of the following ways:

- Press the [EWS] parameter area.
- Press the [EWS] quick key.
- Press the [Calculations] quick key, select the [EWS] tab.
- Press [Main Menu] → [Calculations], select the [EWS] tab.

17.7.4 Performing EWS Scoring

To perform scoring, follow the steps below:

- Select [Clear] to clear the previous score and update values of 1. currently monitored parameters.
- Select [Score] system, calculating [Mode] and [Refresh] period 2. as needed.
- Select [Conscious] and switch on or off [Supply O2], measure or 3. manually enter the values of other required parameters.
- Press [Calculate] to obtain the total score. 4.



Caution

Before calculating the score, press [Clear] to clear the previous score.



(I) Caution

You can get the score only when all required parameters have been measured or entered.

17.7.5 Auto Scoring

When [Mode] is set to [Auto], the monitor automatically calculates the total score when the following conditions occur:

- At the completion of the preset refresh period (time interval);
- · At the completion of each NIBP measurement;
- When an alarm occurs to the parameter for scoring.

17.7.6 EWS Settings

NEW	NEWS Settings					
No.	Parameter	Setting Range	Unit	Default Setting		
1	Consciousness	Alert, Confusion, Voice, Pain		Alert		
2	Supply O2	On, Off		Off		
3	RR	0-150	rpm	Current RR value / empty		
4	SpO ₂	0-100%	%	Current SpO ₂ value / empty		
5	Temp	0-50	°C	Current Temp value / empty		
6	SBP	0-300	mmHg	Current SBP value / empty		
7	PR	0-350	bpm	Current PR value / empty		

NEW	NEWS Settings					
No.	Parameter Setting Range		Unit	Default Setting		
1	Consciousness	Alert, Reacting to Voice, Reacting to Pain, Unresponsive	/	Alert		
2	RR	0-150	rpm	Current RR value / empty		
3	Temp	0-50	°C	Current Temp value / empty		
4	SBP	0-300	mmHg	Current SBP value / empty		
5	HR	0-350	bpm	Current HR value / empty		

CAR	CART Settings					
No.	Parameter	Setting Range	Unit	Default Setting		
1	RR	0-150	rpm	Current RR value / empty		
2	DBP	0-300	mmHg	Current SBP value / empty		
3	HR	0-350	bpm	Current HR value / empty		
4	Age	0-150	Year	Current patient age		

This page intentionally left blank.

Chapter 18 Other Functions

18.1 Freezing Waveforms

During patient monitoring, you can freeze the currently displayed waveforms on the screen so that you can have a close examination of the patient's status.

18.1.1 Entering Freeze Screen

In the Non-Freeze status, press the [Freeze] quick key to exit the current operating screen. Freeze status is entered and the pop-up Freeze menu appears on the bottom of the screen.

In Freeze status, all waveforms are frozen and will no longer be refreshed. Nevertheless, the Parameter area refreshes and the data is stored normally.

18.1.2 Exiting Freeze Screen

In the Freeze status, press the [X] button at the upper right corner of the freeze menu to close the freeze menu and exit the freeze screen. After exiting Freeze status, the system will clear screen waveforms and resume displaying real-time waveforms from left to right in the waveform area.

18.1.3 Reviewing Frozen Waveforms

You can review a waveform of up to 120 seconds before it is frozen by moving the waveform. Press the [<] or [>] button in the Freeze screen to view the frozen waveforms. At the lower right corner of the bottom-most waveform displays the freeze time. The initial frozen time is 0.0s. With the waveforms scrolling, the freeze time changes at an interval of 1 second. For example, -2.0s means two seconds before the frozen time. This change will be applied for all waveforms on the screen.

18.2 Using the On-Screen Timer

The monitor has a Timer function to notify you when a preset time period is expired.

18.2.1 Displaying the Timer

To display a timer, follow the steps below:

- 1. Access [Layout] screen in either of the following ways:
 - Press the [Screens] quick key → select the [Layout] tab.

- Press [Main Menu] → [Screens], select the [Layout] tab.
- 2. Select the parameter area where you want to display the timer, and then select [Timer] from the popup list.

18.2.2 Using the Timer

You can perform the following operations on the timer:

- [Start/Pause]: starts/pauses the timer.
- · [Reset]: clears and resets the timer.
 - ⚠ Warning

Do not use the timer for critically ill patients.

Note

You cannot set the timer while it is working.

18.3 Nurse Call

When there is an alarm, the monitor outputs nurse call signal to the hospital's nurse call system to notify the nurse.

The monitor provides nurse call port which is connected to nurse call system through the nurse call cable to perform the nurse call function.

To enable the nurse call function, follow the steps below:

- Press [Main Menu] → [Maintenance] → input password → press [Enter].
- Select the [Sig. Out] (Signal Output) tab → switch on [Nurse Call].

Alarms are indicated on the nurse call device only when the following conditions are met:

- The nurse call system is enabled.
- A user-defined alarm occurs.
- Alarms are not paused or reset.

⚠ Warning

Do not rely exclusively on the nurse call system for alarm notification. Remember that the most reliable alarm notification combines audible and visual alarm indications with the patient's clinical condition.

18.4 Managing Configurations

When performing continuous monitoring on a patient, the clinical professional often needs to adjust the monitor's settings according to the patient's condition. The collection of all these settings is called a configuration. The system configuration items can be classified as: parameter configuration items, alarm configuration items, conventional configuration items, and user maintenance items. In order to configure the monitor more effectively and quickly, the monitor provides different sets of configurations to accommodate the varying patient types. You can change some settings from a certain set of configuration and then save the changed configuration as a user configuration.

18.4.1 Restoring Default Configuration

During monitoring, you may change some settings in some cases, but these changes may not be appropriate or correct, especially when updating patients. Therefore, you should restore the factory default configuration according to your need, so as to ensure that the various configurations of the monitor are suitable for the monitored patients.

The monitor will load the pre-set default configuration in the following cases:

- A patient is admitted.
- A patient is discharged.
- Patient data is cleared.
- Patient type is changed.

The default configurations include: Factory Defaults (Adult), Factory Defaults (Pediatric), Factory Defaults (Neonate).

The restored configuration is subject to the patient type (adult, pediatric or neonate). This configuration can be either factory configuration or a saved user configuration.

18.4.2 Saving Current Settings

Current settings can be saved as a user configuration. Up to 18 user configurations can be saved. To save current settings, follow the steps below:

- 1. Press [Main Menu] → [System], select the [Configurations] tab.
- 2. Select [Save as].
- 3. In the popup dialog box, enter the configuration name.

4. Select [Enter] to import the configuration as a user configuration.

18.4.3 Deleting a Configuration

To delete a configuration, follow the steps below:

- 1. Press [Main Menu] → [System], select the [Configurations] tab.
- 2. Select the configuration you want to delete.
- 3. Select [Delete].
- 4. Select [Yes] in the popup dialog box.

18.4.4 Loading a Configuration

You can load a desired configuration to ensure that all the settings are appropriate for your patient. To load a configuration, follow the steps below:

- 1. Press [Main Menu] → [System], select the [Configurations] tab.
- 2. Select a desired configuration.
- 3. Select [Load].
- 4. Select [Yes] in the popup dialog box.



The monitor may configure some settings by default when you load a configuration of different software version with the current configuration.

18.4.5 Exporting a Configuration

To export the current monitor's configuration, follow the steps below:

- 1. Connect the USB drive to the monitor's USB port.
- 2. Press [Main Menu] → [System], select the [Configurations] tab.
- 3. Select the configuration you want to export.
- 4. Select [Export].
- 5. Enter the name of the configuration to export.
- 6. Select [Enter].
- 7. Select [Yes] in the popup dialog box when a status message reports completion of the transfer.

18.4.6 Importing a Configuration

To import the configuration from the USB drive to the monitor, follow the steps below:


1. Connect the USB drive with the saved configuration file to the monitor's USB port.

- 2. Press [Main Menu] → [System], select the [Configurations] tab.
- 3. Select [Import].
- 4. Select the configuration you want to import, and select [Open].
- 5. Enter the name of the configuration to import.
- 6. Select [Enter] to import the configuration as a user configuration.

Chapter 19 Recording

19.1 Recorder

A thermal recorder can be used for the monitor and output patient information, measurement data, up to three waveforms, etc. Built-in thermal recorder may be used due to the different configuration.



- 1 Power indicator:
 - On (green light): the recorder works correctly.
 - Off: the monitor is switched off.
- 2 Error indicator:
 - On (red light): the recorder is out of paper, or the thermal paper is not loaded properly.
 - Off: the paper is loaded correctly.
- 3 Recorder door open button
- 4 Paper compartment

19.2 Setting up the Recorder

Press [Main Menu] → [Reports], select the [Recorder Setup] tab to enter the recorder setting screen. You can configure the recorder as follows:

• [Wave 1], [Wave 2], [Wave 3]: select the desired waveform.

Note

The recorder can output up to three waveforms at a time.

Note

Only ECG waveform can be selected for [Wave 1]. [Wave 1], [Wave 2] and [Wave 3] cannot be set to the same options (for example, [Wave 2] and [Wave 3] cannot be set to Resp at the same time).

Note

The recorder can record up to 2 ECG waveforms at a time.

- [Duration]: set the duration of real-time recording.
 Options: Continuous, 8s, 16s, 32s, the default is 8s.
 When it is set to [Continuous], [Timed Record Interval] is deactivated, and the recorder will not stop recording the real-time waveform until the recording is manually stopped by pressing the record key.
- [Timed Record Interval]: set the time interval for automatic recording.

Options: Off, 10min, 20min, 30min, 40min, 50min, 1h, 2h, 3h, 4h. The default setting is switched off.

[Speed]: set the speed for recording waveforms.
 Options: 25mm/s, 50mm/s, the default setting is 25mm/s.

19.3 Starting Recordings

19.3.1 Manually Starting Recordings

To manually start a recording, you can either:

- Press the hard key on the front panel of the monitor.
- Press the button on the top right corner of the current screen.

19.3.2 Automatic Recordings

In the following conditions, you can set the recorder to automatically start recording:

Recording at a preset interval
 The recorder starts automatic recording according to the set interval for [Timed Record Interval]. For more information, see 19.2Setting up the Recorder.

Recording when a parameter alarm is triggered

To enable automatic recording via recorder when a parameter alarm is triggered, follow the steps below:

- 1. Select the tab related to parameter alarm in either of the following ways:
 - Press the [Alarm Setup] quick key.
 - Select the parameter numeric area of a parameter → press the [Alarm Setup] button.
 - Press the [Parameters] quick key → select the required parameter → press the [Alarm Setup] button.
- 2. Switch on the alarm switch [On/Off] and the recording switch [Rec Output] for the parameter.

19.4 Stopping Recordings

Press the hardkey on the front panel of the monitor to stop the current recording.

Recordings stop automatically in the following conditions:

- The recording is completed.
- The recorder runs out of paper.
- Malfunction stops the recorder from running properly.

19.5 Loading Paper

To load the thermal recording paper, follow the steps below:

- 1. Press and hold down the open button to open the recorder door.
- Insert a new roll of paper into the paper compartment properly, with printing side facing upwards. Pull about 2cm of the paper out.
- 3. Close the recorder door.

19.6 Removing Paper Jam

If the recorder works incorrectly or produces unusual sounds, check if there is a paper jam. Remove the paper jam in the following way:

- 1. Open the recorder door.
- 2. Take out the paper and tear off the draped part.
- 3. Reload the paper and close the recorder door.

19.7 Precautions

Observe the following precautions when using the recorder:

- Only standard thermo-sensitive recording paper can be used.
 Otherwise, it may cause damage to the recorder's thermo-sensitive print head, the recorder may not function, or the recording quality may be poor.
- When the recorder is working, the recording paper goes out steadily. Do not pull the paper outward with force. Otherwise the recorder may be damaged.
- Do not leave the recorder door open unless you reload paper or remove troubles.
- Do not use anything that may destroy the thermal element.
- Do not add unnecessary force to the thermo-sensitive print head.

This page intentionally left blank.

Chapter 20 Printing

20.1 Supported Printer

The monitor can output patient reports via a connected network printer. The currently supported printer type is HP Laser Jet M203-M206 laser printer.



Caution

For more information about the printer, refer to the document accompanying the printer. With product upgrades, the monitor may support additional printers without prior notice. If you have any doubts about the compatibility of the printer used with this monitor, contact the manufacturer.

20.2 Setting the Network Printer

To set the network printer, follow the steps below:

- Press [Main Menu] → [Maintenance] → input password → press [Enter].
- 2. Select the [Print] tab.
- 3. Set the [Printer IP Address].
- 4. Press the [Test] button to verify whether the printer is connected normally.



Caution

The IP address of the network printer must be in the same LAN as the monitor.

20.3 Starting a Printing Task

20.3.1 Manual Printing

Print a report manually in one of the following ways:

- Press the button on the top right corner of the current screen.
- Press the [Real-time Print] quick key at the bottom of the main screen

20.3.2 Automatic Printing

To enable automatic printing reports via a network printer when a parameter alarm is triggered, follow the steps below:

- 1. Select the tab related to parameter alarm in either of the following ways:
 - Press the [Alarm Setup] quick key.
 - Select the parameter numeric area of a parameter → press the [Alarm Setup] button.
 - Press the [Parameters] quick key → select the required parameter → press the [Alarm Setup] button.
- 2. Switch on the alarm switch [On/Off] and the printing switch [Print Output] for the parameter.

Note

Before sending a print request, make sure that there is enough paper in the printer.

20.4 Stopping a Printing Task

To stop a printing task, follow the steps below:

- 1. Press [Main Menu] → [Reports], select the [Print Queen] tab.
- 2. Select desired printing tasks and then select [Delete].

20.5 Configuring Reports

20.5.1 Configuring ECG Reports

To configure ECG reports, follow the steps below:

- 1. Press [Main Menu] → [Reports], select the [Report Setup] tab.
- 2. Select [ECG] tab.
- 3. Set the desired options.

The menu settings are described below:

- [Print ECG Grid]: set whether to print grids on ECG waveforms of a printout.
 - The default setting is switched off.
 - Switching on means that the 5x5(mm²) grid background will be printed on the ECG waveforms.
- [12-Lead Format]: select the format of 12-lead ECG waveforms on a printout.
- 6x2+1: displays 12-lead ECG waveforms on one page in two columns, with 6 lines in each column, and one rhythm lead waveform at the bottom.
- 3x4+1: displays 12-lead ECG waveforms on one page in 4 columns, with 3 lines in each column, and one rhythm lead waveform at the bottom.
- [Rhythm Lead 1]: select the lead that will be used as Rhythm Lead 1.
 - Options: I, II, III, aVR, aVL, aVF, V1, V2, V3, V4, V5, V6
- [12-ECG Sequence]: set whether all leads show simultaneous or sequential intervals of time, when displaying or printing 2 or more columns.
 - Options: Sequential, Simultanious.
- [Sequential]: 12-lead ECG data are recorded sequentially and displayed in 3 lines and 4 columns with 2.5 seconds of ECG data for each column.
- [Simultanious]: record simultaneous 12-lead ECG data.

20.5.2 Configuring Real-time Reports

To configure real-time reports, follow the steps below:

- 1. Press [Main Menu] → [Reports], select the [Report Setup] tab.
- 2. Select the [Real-time] tab.
- 3. Set the desired options.

The menu settings are described below:

- [Speed]: set the waveform speed.
 Options: 12.5mm/s, 25mm/s, 50mm/s, Auto.
- [Print Current Waves]: prints the real-time report for the currently displayed waveforms.
- [Print Specified Wave]: prints the real-time report for the desired waveforms configured.
- [Duration]: set the duration of printing real-time waveform. Options: 10s, 20s, 30s, 40s, 50s, 60s, Continuous.

The default setting is 10s. When it is set to [Continuous], [Timed Record Interval] is deactivated, and the recorder will not stop recording the real-time waveform until the recording is manually stopped.

20.5.3 Configuring Tabular Trends Reports

To configure tabular trends reports, follow the steps below:

- 1. Press [Main Menu] → [Reports], select the [Report Setup] tab.
- 2. Select the [Tabular Trend] tab.
- 3. Set the desired options.

The menu settings are described below:

- [Start Date]: select the date before which a tabular trends report will be printed.
- [Start Time]: select the time before which a tabular trends report will be printed.
- [Period]: select the period during which a tabular trends report will be printed.

Options: 30min, 1h, 2h, 4h, 8h, 12h, 24h, 48h, 72h, 96h.

The default setting is 48h.

• [Resolution]: select the resolution of the tabular trends printed on a report.

Options: 5s, 30s, 1min, 5min, 10min, 15min, 30min, 1h, 2h, 3h, NIBP, Auto. The default setting is Auto.

[Auto]: using the [Resolution] setting of the Tabular Trends review screen.

[NIBP]: the tabular trends will be printed at the interval of acquiring the NIBP values.

[Print Format]: select the printing principle.

Options: Time Priority, Parameter Priority.

The default setting is Parameter Priority.

- [Time Priority]: print one page span of report with time listed by row and parameter listed by column when [Resolution] is set to [Auto].
- [Parameter Priority]: print one page span of report with parameters listed by row and time listed by column when [Resolution] is set to [Auto].

20.5.4 Configuring Graphic Trends Reports

To configure graphic trends reports, follow the steps below:

- 1. Press [Main Menu] → [Reports], select the [Report Setup] tab.
- 2. Select the [Graphic Trend] tab.
- 3. Set the desired options.

The menu settings are described below:

- [Start Date]: select the date before which a graphic trends report will be printed.
- [Start Time]: select the time before which a graphic trends report will be printed.
- [Period]: select the period during which a graphic trends report will be printed.
- [Trend Group]: select the contents of the printed graphic trends report.

20.5.5 Configuring Event Reports

To configure event reports, follow the steps below:

- 1. Press [Main Menu] → [Reports], select the [Report Setup] tab.
- 2. Select the [Event] tab.
- 3. Set the print content of the event report. Options: List, Detail, Select All.

20.6 Viewing Printing Status

To view the status of printing tasks, follow the steps below:

Press [Main Menu] → [Reports], select the [Print Queen] tab.

Each printing task includes the following information:

- Report type
- Print time
- Operator
- Operator ID
- Printing status, for example, printing, failed, retrying, and waiting.

In the [Print Queue] screen, you can view the list of current printing tasks, delete the currently selected print tasks, or delete all printing tasks.

This page intentionally left blank.

Chapter 21 Battery

21.1 Introduction

The monitor is equipped with a lithium-ion rechargeable battery to support its normal operation when the external power is not available.

21.2 Safety Information



⚠ Warning

Keep the battery out of the reach of children.



⚠ Warning

Use only the battery specified by the manufacturer. Use of unspecified battery may cause a risk of fire or explosion.



🗥 Warning

While replacing the battery, do not use unspecified battery to avoid damage to the device.



⚠ Warning

Keep the battery in their original package until you are ready to use them.



⚠ Warning

Keep the battery away from liquid.



⚠ Warning

Do not crush, drop or puncture the battery. Mechanical abuse can lead to internal damage and internal short circuits. If a battery has been dropped or banged against a hard surface, whether damage is externally visible or not, remove the battery from use and dispose of it properly.



🗥 Warning

If the battery shows signs of damage or signs of leakage, replace it immediately. Use caution in removing the battery. Avoid contacting the leakage.



⚠ Warning

The battery can only be charged by this monitor.

1 Warning

Do not disassemble the battery, place it in high ambient temperature (above 60° C) environment, burn the battery or short-circuit it. Otherwise, it may cause a risk of fire, explosion, battery leaks or high temperature and even personal injury.

⚠ Warning

The lithium-ion rechargeable battery has a service life. Replace it when its service life expires. Failure to replace the battery on time may cause serious damage to your equipment from battery overheating.

Caution

Remove the battery before transporting the monitor or the monitor will be laid aside for a long time.

① Caution

Do not supply power for other electronic devices via the battery.

21.3 Installing the Battery

The battery must be installed and replaced by service personnel trained and authorized by the manufacturer. The monitor is not equipped with battery when it leaves the factory. Contact the service personnel to install the battery before using it for the first time.

To install the battery, follow the steps below:

- Turn off the monitor, disconnect the power cord and other cables.
- 2. Place the monitor face down on the table.
- 3. Use a Phillips screwdriver to loosen the fixing screws on the battery cover and open the battery cover.
- 4. Insert the battery into the battery compartment and keep the battery cable outward.
- 5. Insert the battery cable plug into the corresponding socket.
- 6. Straighten out the battery cable, fix the battery, close the battery cover, and tighten the fixing screws.

21.4 Battery Indication

The battery status indicator, on-screen battery icons and related alarm messages indicate the battery status.

21.4.1 Battery Status Indicators

The description of battery status indicators are as follows:

Indicator Color	Battery Status
Green	AC power is connected and the battery is fully charged.
Yellow	AC power is connected and the battery is being charged.
	AC power is connected and no battery is installed.
Off	The battery is installed and AC power is not connected.

21.4.2 Battery Icons

The battery icon in the upper right corner of the monitor screen indicates the battery status:

Battery Icon	Description
	The battery is working correctly. The white portion represents the remaining capacity of the battery.

	The battery power is low and needs to be charged. When this icon appears, the battery can power the monitor for up to 30 minutes.
	The battery is almost depleted and needs to be charged immediately. Otherwise, the monitor will automatically shut down after 5 minutes.
*	The battery is being charged.
	No battery is installed

21.4.3 Battery-related Alarms

When the battery is low, the "Low battery" alarm will be triggered. When the battery is almost depleted, the "Battery depleted" alarm will be triggered. In this case, immediately connect the AC power supply to the monitor and charge the battery. Otherwise, the monitor will automatically shut down soon.

For more information on battery-related alarms, see *Appendix B Alarm Messages*.

21.5 Charging the Battery

After the monitor is connected to AC power supply, it can automatically charge the battery even though the monitor is turned off.

21.6 Maintaining the Battery

21.6.1 Battery Optimization

The performance of the battery deteriorates over time. It is recommended to optimize the battery every three months. If the battery is not optimized for a long time, the battery capacity display may be inaccurate, causing the incorrect judgment of remaining battery runtime.

To optimize the battery, follow the steps below:

- 1. Disconnect the monitor from the patient and stop all monitoring and measuring procedures.
- 2. Allow the battery to be charged uninterruptedly until it is fully charged.

- 3. Allow the monitor to run on the battery until the battery is completely depleted and the monitor automatically shuts down.
- 4. Fully charge the battery again for use or charge it to 40%-60% for storage.



Do not use the monitor to monitor patient during the battery optimization.

Caution

Do not interrupt charging or discharging during battery optimization.

21.6.2 Checking Battery Performance

The performance of the battery deteriorates over time. You should check the battery performance every three months. If you suspect that the battery breaks down, the battery performances should also be inspected.

See steps 1 to 3 of 21.6.1 Battery Optimization to check the battery performance. The operating time of the battery reflects its performance directly. If the operating time of a battery is noticeably shorter than that stated in the specifications, the battery may have reached its service life or be malfunctioning. If the battery performance meets the requirement, fully charge the battery again for use or charge it to 40%-60% for storage.



Battery operating time depends on device configuration and operation. For example, too high display brightness or frequent NIBP measurements will shorten the battery operating time.

21.7 Storing the Battery

Keep the battery terminals away from metallic objects when storing the battery. If the battery needs to be stored for a long time, place it in a cool environment.

The stored battery should also be optimized regularly. For the optimization method, see *21.6.1 Battery Optimization*.



Remove the battery from the monitor if the monitor is not used for a long time (for example, several weeks). Otherwise the battery may over discharge, which may damage the battery.



It will greatly shorten the service life of the battery if it is stored in a high temperature environment for a long time.

21.8 Replacing and Recycling the Battery

Replace the battery if it is damaged, aging or cannot store power, and recycle it correctly. Properly dispose of the battery according to your local regulations.

Chapter 22 Cleaning and Disinfection

22.1 Safety Information



⚠ Warning

Do not immerse the device and accessories in liquid.



⚠ Warning

Do not pour liquid on the device or accessories. Do not allow the liquid permeate into the device.



4 Warning

Do not use abrasive materials or any strong corrosive solvents for cleaning to avoid scratches or damages to the device.



⚠ Warning

The parts contacted by the infected or suspected patient should be disinfected.



⚠ Warning

The manufacturer is not responsible for the effectiveness of the disinfectant or disinfection method used as a means of infection control. Please consult your hospital's infection control director or epidemiologist for advice.

22.2 Recommended Cleaning Agents

Supported cleaning agents include:

- Sodium hypochlorite (10%, bleaching powder for washing)
- Ethanol (70%~75%)

Supported cleaning tools include:

Cotton ball, soft gauze, soft brush and soft cloth.

22.3 Cleaning

Clean the exterior surface of the monitor monthly or more frequently if needed. Consult your hospital's regulations before cleaning the monitor.

To clean the monitor, follow the steps below:

1. Turn off the monitor and disconnect it from the AC power supply cable and accessories

- 2. Clean the surface of the monitor with a clean soft gauze moistened with one of the recommended cleaning agents.
- 3. Wipe off all the cleaning agent residue with a clean dry cloth. Dry your monitor in a ventilated, cool place.



Keep the cleaning agent away from the connectors of the monitor and accessories while cleaning the device housing.

$\hat{m{\Lambda}}$ Caution

Use non-aggressive cleaning agent to clean the surface of the monitor and the display screen.

⚠ Caution

Most cleaning agents must be diluted before usage.

22.4 Disinfection

Disinfect the monitor in accordance with the disinfection procedures of your hospital. Clean the monitor before disinfection.

⚠ Warning

Ethanol is flammable. Please keep away from fire while using the ethanol disinfectant.

⚠ Warning

People allergic to ethanol are forbidden to use the ethanol disinfectant.

Caution

Rubber and plastic products will harden after prolonged contact with alcohol disinfectants, hence the residual disinfectant should be removed in time after disinfection.

Caution

Do not use radiation or steam for disinfection.

(I) Caution

Please avoid contact with the metal parts when user disinfects the device with peroxide or chlorine-containing disinfectants.

22.5 Sterilization

It is not allowed to sterilize the monitor and related accessories unless stated in their operation instructions.

22.6 Cleaning the Print Head

If the thermal printer has been used for a long time, deposits of paper debris may collect on the print head, which may affect the print quality and shorten the lifetime of the roller. Follow this procedure to clean the thermo-sensitive print head:

- Take measures against the static electricity such as Disposable Wrist Strap for the work.
- 2. Open the printer door and take out the paper.
- 3. Gently wipe around the print head using cotton swabs dampened with Ethanol.
- 4. After the Ethanol has completely been dried, reload the paper and close the printer door.



Caution

The thermal head may be hot after completing the recording task. Do not clean the thermal head of the recorder immediately.

22.7 Cleaning, Disinfection and Sterilization of Accessories For the cleaning, disinfection and sterilization methods of reusable accessories, refer to the instructions for use that accompany the accessories.

Chapter 23 Care and Maintenance

In order to ensure the normal operation of the monitor and maintain its service life, please pay attention to the maintenance of the monitor. Refer to the detailed provisions in the sales contract for the warranty period of main unit and accessories of the monitor.

23.1 Safety Information



No modification of this device is allowed.



This device contains no user serviceable parts.

⚠ Warning

The safety checks or maintenance involving any disassembly of the device should be performed by professional service personnel. Otherwise, undue device failure and possible health hazards could result.

⚠ Warning

A comprehensive inspection for the monitor (including functions and safety inspections) should be carried out by qualified personnel every year or after each maintenance.

① Caution

If the user does not regularly check or maintain the monitor, it may affect its performance and safety.

Caution

If the user cannot implement a satisfactory maintenance plan, it may disable the monitor functions and endanger human health.

Caution

The SpO_2 calibration of the monitor has been carried out before delivery, and user does not need to calibrate it again during the operation.

Caution

If you find any signs of damage of the monitor or accessories, do not use them.

① Ca

The device and accessories shall not be serviced or maintained while in use on a patient.

Caution

If you discover a problem with any of the device, contact your service personnel or our company.



Caution

Use and store the device within the specified temperature, humidity, and altitude ranges.



Caution

When disposing of the packaging material, be sure to observe the applicable waste control regulations and keep it out of the reach of children.



Caution

At the end of its service life, the device, as well as its accessories, must be disposed of in compliance with the local regulations regarding the disposal of such products. If you have any questions concerning disposal of the device, please contact our company.

23.2 Daily Inspection

Before using the monitor, the checks below should be carried out:

- Check the monitor for any mechanical damage;
- Inspect the exposed parts and the inserted parts of all the cables and the accessories;
- Examine all the functions of the monitor that are likely to be used for patient monitoring, and ensure that it is in good working condition;
- Make sure that the monitor is grounded properly.
- Pay close attention to the fluctuation of the local power supply voltage. A power voltage regulator is recommended when necessary.

In case any indication of damage about the function of the monitor is detected and proven, it is not allowed to apply it to the patient for any monitoring. Please contact the local dealer or our company, and we are to offer the best solution as soon as possible for your satisfaction.

23.3 Routine Maintenance

The monitor is designed with a service life of 10 years.

It is strongly recommended to use the product within its life cycle, or it may cause inaccurate measurement. During the long-term use, it is recommended that the user check and calibrate the monitor once a year to ensure the measurement accuracy. Due to the high risk of product aging in the last year of the service life, please pay close attention to the inspection results. Dispose of the monitor and its accessories when their service life is reached.

The inspection items mainly include:

- · Check whether the safety signs are damaged.
- Check the main unit and accessories for mechanical and functional damages.
- Carry out the protective grounding impedance, leakage current and insulation resistance test according to the requirements of IEC60601-1.
- Verify the functions of the device according to the operator's manual.

The test and results recording should be carried out by trained and qualified personnel with the safety test knowledge. Please maintain the monitor if any problem is detected in the above tests.

23.4 Battery Maintenance

Perform battery maintenance regularly to maintain its useful life.

- Check the battery regularly. If it is damaged, contact the manufacturer to purchase a battery of the same model and specification for replacement.
- It is recommended to use the battery once a month to ensure its power capability and long service life, and recharge it after run out of its power capacity.
- Please keep the battery power between 50% to 80% when the monitor is laid aside for a long time. The battery should be charged every 3 months to avoid irreversible capacity loss caused by low battery due to self-discharge during the long time storage.

23.5 ECG Calibration

The ECG signal may be inaccurate due to hardware or software problems. As a result, the ECG wave amplitude becomes greater or smaller.

You can print out the square wave and wave scale, and then measure the difference between them if necessary. If the difference exceeds 5%, contact your service personnel.

To calibrate the ECG module, follow the steps below:

- Press[Main Menu]→[Maintenance]→ input password → press [Enter].
- 2. Select the [Module] tab→[ECG] tab.
- 3. Switch on [Calibration].

4. Switch off [Calibration] to end the calibration of ECG module.



During ECG calibration, the patient cannot be monitored.

23.6 NIBP Maintenance

23.6.1 NIBP Leakage Test

The NIBP leakage test checks the integrity of the system and of the valve. In order to avoid significant error of blood pressure measurement or even no measurement result caused by air leakage in the pneumatic system including the cuff during measuring, it is recommended to check if there is leakage in the pneumatic system. The NIBP leakage test should be performed at least once a year or when you doubt the NIBP measurements. The NIBP leakage test should be performed by the qualified service personnel only. To perform the NIBP leakage test, follow the steps below:

- 1. Press[Main Menu]→[Maintenance]→ input password → press
- 2. Select the [Module] tab → [NIBP] tab.
- 3. Select [Leakage Test].
 - Caution


[Enter].

Please remove the cuff from patient while performing the leakage test.

23.6.2 NIBP Pressure Accuracy Verification

NIBP pressure accuracy verification is a function to inspect the accuracy of pressure measurement by the NIBP module inside the device. Technician or device manager should perform pressure accuracy verification every six months or a year in order to check if the pressure measurement still conforms to the requirement of product performance. If the deviation is beyond the declared specification, it is permitted to return it to factory for repair or calibration.

Before verification, please connect the monitor to a precision pressure meter as the reference equipment like a mercury pressure meter.

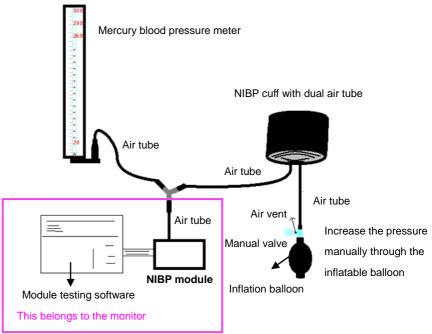

+ Mode 1: Automatic inflation for the pressure accuracy verification
At this mode, the monitor can activate the inflation, so the pressure
will increase automatically until it exceeds the limit value specified in
the table below. This pressure limit value depends on the patient
type selection as shown in the table below:

Patient Type	Mode 1 (Maximum pressure value)	Mode 2 (Over-pressure protection pressure value)
Adult	240mmHg	300mmHg
Pediatric	200mmHg	240mmHg
Neonate	120mmHg	150mmHg

During the inflation, the monitor will close the deflating valve, and the pressure value will be shown during the process. If there is no manual deflation operation, the pressure will persist until deflation by manual operation, so it is necessary to use a manual valve for doing adequate deflation in several steps to verify the pressure accuracy in the full scale of measurement range.

★ Mode 2: Manual inflation for the pressure accuracy verification

At this mode, the pressure should be increased manually by a pumping balloon, and the verification can be done by applying different pressure value manually. If the increased pressure exceeds the given limit as shown in the table above, the monitor will deflate automatically because of over-pressure protection.

To perform the NIBP pressure accuracy verification, follow the steps below:

- Press[Main Menu]→[Maintenance]→ input password → press [Enter].
- 2. Select the [Module] tab → [NIBP] tab.
- Select [Auto Pressure Test] to perform automatic inflation for the pressure accuracy verification. Or select [Manual Pressure Test] to perform manual inflation for the pressure accuracy verification.



Pressure accuracy verification must be operated by technician or device manager. Physicians and nurses are not allowed to do the verification, it is very dangerous especially when the pressure cuff is still on patients.



Caution

After the verification, do press the button again to return to normal working mode, then continue other operation, or the NIBP measurement key will be invalid.

23.7 CO₂Calibration

For sidestream CO₂ module, a calibration is needed every year or when the measured values have a great deviation.

For maintream CO_2 module, no calibration is needed. If calibration is required, contact your service personnel.

23.8 IBP Calibration

This section is for professional technician only.

To avoid inaccurate pressure readings, the monitor requires a valid zero. Zero the transducer in accordance with your hospital policy. The IBP transducer should be zeroed in the following conditions:

- When you use a new transducer or tubing.
- Each time you reconnect the IBP transducer or adapter cable.

- If you think the monitor's pressure readings are not correct.
- When you select another measuring label, the monitor displays the prompt message *Unzeroed*.

There is two methods for calibration: zero calibration and pressure value calibration.

Calibration procedure:

- Press[Main Menu]→[Maintenance]→ input password → press [Enter].
- 2. Select the [Module] tab → [IBP] tab.
- 3. Select [IBP Channel], and input 0mmHg for the pressure.
- 4. Press the [Calibration] button. After the calibration is completed, the message "Zero succeeded" will be displayed.
- 5. Then input 100mmHg for the pressure.
- 6. Press the [Calibration] button. After the calibration is completed, the message "Calibration succeeded" will be displayed. If the calibration fails, corresponding message will also be displayed.



IBP transducer calibration is prohibited when monitoring a patient.



Before performing calibration, please make sure that the transducer is well connected, otherwise the calibration cannot be carried out.

23.9 Storage, Packaging and Transportation

If the monitor will not be used for a long time, wipe it clean and keep it in the packaging, which shall be kept in a dry and well ventilated room free from dust and corrosive gases.

The monitor is packed in high quality corrugated cartons with foam inside to protect the monitor against damage during transportation. The outer packaging box is marked with gross weight and dimension.

The monitor should be transported by land (vehicle or railway) or air in accordance with the contractual terms. Do not hit or drop it with force during transportation.

23.10 Viewing Version Information

When performing maintenance for the monitor, you may need to check the system information.

To view the system software version, hardware version, module version, firmware version, and other version information, follow the steps below:

- Press[Main Menu]→[Maintenance]→ input password → press [Enter].
- 2. Select the [Version] tab.

You can also press the [Main Menu] → [System], and select [Version] tab to view the software version, monitor name, monitor ID and monitor network information (MAC and IP address).

This page intentionally left blank.

Chapter 24 Troubleshooting

This chapter lists the problems that are likely to occur. If the problem persists after corrective actions have been taken, contact the manufacturer or your local distributor.

24.1 Prompt Messages

The monitor prompts messages to indicate the current system status. Follow the instructions in the table below to eliminate the problems. NIBP

Status / Error	Description	Corrective Actions
Self-test failed	NIBP module self-test failed during power on, sensor or other hardware errors.	Module abnormal or faulty, it is recommended to power on again. If this symptom cannot be eliminated, it is recommended to replace the NIBP module or return to the factory for repair.
System error	Abnormal condition of CPU, such as register overflow, divided by zero.	Module abnormal or faulty, it is recommended to power on again. If this symptom cannot be eliminated, it is recommended to replace the NIBP module or return to the factory for repair.
Measurement timeout	Adult exceeds 180s and neonates exceeds 90s.	Normal module operating report, not error or fault. The module itself has an error return that defines the measurement timeout. Start timing at the beginning of measurement, more than 85s in neonate mode and 175s in non neonate mode.
Weak signal	Very weak signal because of the cuff, or the patient has very weak pulse.	Normal module operating report, not error or fault.
Cuff error	Cuff is not wrapped correctly, or is not connected.	Normal module operating report, not error or fault.

Status / Error	Description	Corrective Actions
Air leak	Air moving part, tube or the cuff leak air.	Check the cuff for air leakage. Check the tightness of the module airway. Recondition the module pneumatic components.
Pressure error	Unstable cuff pressure or tangled cuff tubing.	Check the airway, especially the hose, for kinks. Recondition the module.
Over range	Very weak signal because of the cuff, or the patient has very weak pulse.	Normal module operating report, not error or fault.
Over motion	The repeated measurement due to moving, excessive noise during the stepping inflation and measuring pressure and pulse, e.g. during patient shaking motion.	Normal module operating report, not error or fault.
Overpressure detected	The blood pressure amplifier is saturated by excessive motion disturbance.	Check whether the airway or air tubing is blocked. Recondition the module.
Exceed measurement range	When any measured value of systolic blood pressure, diastolic blood pressure or mean artery pressure exceeds the nominal measurement range, this technical alarm will be triggered.	Normal application software report, not an error or fault.
Timeout	Indicates that the operation has timed out.	Remeasure

Temp

Status / Error	Description	Corrective Actions
Temperature self-test failed	Power on hardware self-test of temp module failed.	Module abnormal or faulty, it is recommended to power on again. If this symptom cannot be eliminated, it is recommended to replace the Temp module or return to the factory for repair.

ECG

Status / Error	Corrective Actions
Lead(s) off	Normal module operating report, not error or fault.
Unable to detect HR	Normal application software report, not an error or fault.

SpO_2

Status / Error	Corrective Actions
Probe off	Normal module operating report, not error or fault.
SpO ₂ module faulty	It is recommended to replace the SpO ₂ module or return to the factory for repair.
Unable to detect SpO ₂	Normal application software report, not an error or fault.

IBP

Status / Error	Description	Corrective Actions
Transducer error	The transducer signal appears.	The transducer is faulty or the signal line inside the device appears, it is recommended to replace the transducer or return to the factory for repair.
Probe off	IBP cable connector not connected.	Normal prompt message, not an error or fault.
Not zeroed	Each time connecting transducer or selecting another measuring label, perform zero calibration for the module.	Normal prompt message, not an error or fault.
Zeroing OK	Zero calibration result, after successful zero calibration, you can enter the normal measurement process.	Normal prompt message, not an error or fault.
Zeroing failed	Zero calibration failed. The possible reasons are as follows: Transducer not connected The measured pressure is pulsating Zero pressure out of the measuring range Zero calibration time not set	Normal prompt message, not an error or fault.

CO₂

Status / Description	Corrective Actions
----------------------	--------------------

Status / Error	Description	Corrective Actions
Sensor over temp	When the temperature of the sensor is higher than 40°C, the module will send out the information automatically.	Module hardware error or module failure, please return to the factory for repair or replace the sensor.
Sensor faulty	Hardware error, EEPROM checksum error or module failure.	Module hardware error or module failure, please return to the factory for repair or replace the sensor.
No parameter	Barometric pressure and/or gas compensations have not been set since power on. For CO ₂ to be calculated with the stated accuracy, these values should be set whenever the sensor is plugged in.	Wait for the module to complete the setting of barometric pressure and gas compensation. If the information still exists after more than 20 seconds, consider the following reasons: the module barometric pressure and gas compensation settings are wrong, and the application software fails to issue the setting command.
Module in sleep mode	The sensor is currently in standby state.	Normal module operating report, not error or fault. If this prompt appears during the normal monitoring, it is recommended to start the monitoring operation again for the sensor.
Zero in progress	The module is in the process of zeroing.	Normal report during zero operation, not error or fault.
Sensor warm up	After power on, the module has a preheating process, mainly to detect the temperature of the sensor.	Normal module operating report, not error or fault.
Zero required	When the module's auto zero error occurs.	It is suggested to reset the sensor to zero at this time. If the zero operation fails for more than three times or the request is still reported, it indicates that the

Status / Error	Description	Corrective Actions
		sensor is faulty. Please return to the factory for repair or replace the sensor.
CO₂ out of range	The value being calculated is greater than the upper CO ₂ limit (150mmHg). The maximum value output is the upper CO ₂ limit.	It is recommended to perform sensor zeroing at this time. If the zeroing operation fails for more than three times or the error is still reported, the sensor is faulty. Please return to the factory for repair or replace the sensor.
Check airway adapter	Usually caused when the airway adapter is removed from the sensor or when there is an optical blockage on the windows of the airway adapter. May also be caused by failure to perform sensor zero when adapter type is changed.	Correctly connect the adapter to eliminate the error. Check if the round transparent window of the adapter is blocked or damaged. It is recommended to replace the adapter.
Check sampling line	When the sampling line is blocked or kinked, the pneumatic pressure is outside the expected range.	Check for blockage in the sampling line. Check whether the sampling line is tangled. The error can be eliminated when the airway is unblocked.
Sensor off	When the software system fails to receive any CO ₂ data for more than 2 seconds, it is considered that the sensor is off at this time.	Monitoring application software setting status, not reported by the module itself, not an error or fault.
Sensor not ready	When setting the zero operation, the sensor status is not ready. Possible reasons	Normal report during zero operation, not error or fault.

Status / Error	Description	Corrective Actions
	include: Breaths detected	
	The preheating is not completed, and the sensor temperature is not stable	
	The sensor is still in sleep mode	
	Sensor barometric pressure and gas compensation settings are not completed	
Zero in progress	The status information returned by the module during the zero operation.	Normal report during zero operation, not error or fault.
Zero failed and breaths detected	Breathing is detected within 20 seconds of the zero operation.	It is recommended to ensure that there is no breathing gas for at least 20 seconds before the zeroing operation, and perform the zero operation under the condition of clear air to avoid operation failure or zero deviation.

Battery

Status / Error	Corrective Actions
Low battery	Charge the battery in time

24.2 Common Faults

Check the solutions below before requesting service, if you encounter the problems when using the monitor or accessories. If the problem persists, contact your service personnel.

24.2.1 Display Troubleshooting

When there is no display on the screen, follow the steps below:

1. Shut down the device and unplug the power cable.

- 2. Use a universal meter to check if the outlet has proper voltage.
- 3. Check the power cable is in good condition, and that it has been properly connected to the monitor and outlet.
- 4. Remove the fuse from the back cover of this device, and make sure it is in good condition.
- 5. If all of the above is in good condition, there may be an issue with display screen.

24.2.2 Power Supply Troubleshooting

Symptoms	Possible Causes	Corrective Actions
Battery cannot be recharged	Battery is defective	Replace the battery
and/or fully charged	Main board is defective	Replace the main board

24.2.3 Alarm Troubleshooting

Alarm lamp & alarm sound

Symptoms	Possible Causes	Corrective Actions	
The alarm LED does not light	Mainboard is defective	Replace the main board	
No alarm	Audible alarm is disabled	Check if " is displayed. If yes, the audible alarm is disabled.	
sound is issued	Speaker is defective	Replace the speaker	
	Mainboard is defective	Replace the main board	

System alarm

- When the parameter value is higher or lower than the alarm limits, the alarm will issue. Please check whether the alarm limit value is proper or the condition of the patient.
- In case of ECG alarm, check the patient's current condition and check whether the connection of electrode and lead wire is normal.
- Lead(s) off. Please check the connection of the leads.

Probe off. Please check the connection of the probes.

24.2.4 ECG Troubleshooting

If there are excessive ECG signal interferences or the baseline is too thick, always check the following:

- Check if the plate electrodes are properly located, and if valid plate electrodes are used.
- Check whether the lead wires are properly inserted. If no ECG waveform displayed, check if the ECG lead wires are broken.
- Make sure the mains outlet has standard grounding wire.
- Check if the grounding wire of the apparatus is properly grounded.

24.2.5 SpO₂ and NIBP Troubleshooting

If there is no blood pressure and pulse oxygen measurement results, always check the following:

- Check if the blood pressure cuff is properly wrapped around the arm according to the operating instructions, if the cuff leaks, and if the inlet is closely connected with the NIBP jack on the side panel.
- Check if the indicator of the pulse oxygen sensor flashes (do not look directly at the lamp in the pulse oximetry sensor) and if the pulse oxygen sensor is properly connected to the SpO₂connector on the side panel.

24.2.6 IBP Troubleshooting

Symptoms	Possible Causes	Corrective Actions
	Device malfunction	The pressure hardware may be faulty. Contact the manufacturer or your local distributor.
Unable to	Out of range	Confirm that you have selected the value for calibration value that you applying to the transducer, and repeat the calibration.
calibrate	No transducer is detected	Check that the transducer is connected and try again.
	Unstable signal is measured	Confirm that there are no disturbance to transducer, and repeat the calibration.

Symptoms	Possible Causes	Corrective Actions	
	Perform zero first	No valid zero. Zero the transducer first.	
	Device malfunction	The pressure hardware may be faulty. Contact the manufacturer or your local distributor.	
	Excessive offset	Confirm that the transducer is vented to air and try again. If this fails, the hardware may	
Unable to zero	Unstable signal is measured	be faulty, please change a new adapter cable and try again. If it fails, change a new transducer and try again. If it still fails, please contact the manufacturer or your local distributor.	
	No transducer is detected	Check that the transducer is connected and try again. If this fails, exchange the adapter cable and try again. If this fails, exchange the transducer.	
	Plusatile pressure	Confirm that the transducer is vented to air, not to the patient, and try again.	

24.2.7 CO₂Troubleshooting

No CO₂ readings

Symptoms	Error Type	Description	Corrective Actions
Sensor temperature is too high	Hardware error	The temperature of the sensor is greater than 40°C.	Repair or replace CO ₂ sensor
Sensor faulty	Hardware error	Hardware error, EEPROM check error, or module failure	Repair or replace CO ₂ sensor

Troubleshooting the sidestream CO_2 sampling When the sampling system of the sidestream CO_2 module works incorrectly, always check the following:

- Check if the sampling line is kinked.
- If not, remove it from the water trap.

 If the monitor gives a message indicating the airway still works incorrectly, it indicates that the water trap must have been blocked, and you should replace with a new one. Otherwise, you can determine that the sampling line must have been blocked. Replace with a new sampling line.

Chapter 25 Accessories

The accessories listed in this chapter comply with the requirements of IEC 60601-1-2 when in use with the patient monitor. The accessory material that contacts the patients has undertaken the bio-compatibility test and is verified to be in compliance with ISO 10993-1. For details about the accessories, refer to the instructions for use provided with the accessory.



⚠ Warning

Use accessories specified in this chapter. Using other accessories may cause damage to the patient monitor or not meet the claimed specifications in this manual.



🖺 Warning

Check the accessories and their packages for any sign of damage. Do not use them if any damage is detected.



4 Warning

Reuse of disposable accessories may cause a risk of contamination and affect the measurement accuracy.



⚠ Warning

Although the accessory material that contacts patients has been evaluated biologically and the biological safety meets the requirements of ISO 10993-1, very few people may have allergic reaction, and those with allergic reaction should stop using it!



(I) Caution

The accessories may not meet the performance specifications if stored or used outside the specified temperature and humidity ranges. If accessory performance is degraded due to aging or environmental conditions, contact your service personnel.



Caution

Use the accessories before the expiration date if an expiration date is indicated.



Caution

Do not use expired accessories.

Caution

Discard disposable accessories according to your local regulations or hospital regulations.

Note

Part No. is subject to change without prior notice, please refer to the label of parts or the supplied package list.

Note

This manual describes all the accessories that are validated for use. Not all accessories are available in every market. Please check availability with your local supplier.

Note

For the replacement cycle and replacement method of the accessories, refer to the instructions for use provided with the accessory.

25.1 ECG Accessories

No.	Accessories	Model/Part No.	Description	Applicable Patient
1.	ECG cable and electrode	KE-IGB031/ 15010028	3-lead, snap, defibrillation-proof, reusable	
2.	ECG cable and electrode	KE-IGB051/ 15010020	5-lead, snap, defibrillation-proof	Adult/ Pediatric/
3.	ECG cable and electrode	KE-IGB061/ 15010029	6-lead, snap, defibrillation-proof	Neonate
4.	ECG cable and electrode	KE-IGB101/ 15010030	12-lead, snap, defibrillation-proof	

25.2 Temp Accessories

No.	Accessories	Model/ Part No.	Description	Applicable Patient
		MACOOA A /450		Adult/
1.	Temp probe	W0001A/150 80004	10K skin surface	Pediatric/
				Neonate

25.3 SpO₂ Accessories

	20.0 CP CZ / (COCCOCNICO)					
No.	Accessories	Model/ Part No.	Description	Applicable Patient		
1.	Nellcor SpO ₂ sensor	DS100A	Finger-clip, reusable	Adult/Pediatric		
2.	NellcorSpO ₂ sensor	D-YS	Y-type, reusable	Neonate		
3.	NellcorSpO ₂ sensor extension cable	DOC-10	Reusable	Adult/Pediatric/N eonate		
4.	SpO ₂ sensor	KS-AE01	Ear-clip, reusable	Adult/Pediatric/N eonate		
5.	SpO ₂ sensor	KS-AC01	Finger-clip, reusable	Adult		
6.	SpO ₂ sensor	KS-AR01	Large soft finger-cot, reusable	Adult		
7.	SpO ₂ sensor	KS-AR02	Soft finger-cot, reusable	Pediatric		
8.	SpO ₂ sensor	KS-ALW 02	L-type, with wraps, reusable	Pediatric/ Neonate		
9.	SpO ₂ sensor	KS-ALW 02S	L-type, with wraps, disposable, non-sterile	Neonate		
10.	SpO ₂ sensor extension cable	KS-AExt 01	Reusable	Adult/Pediatric/N eonate		

25.4 NIBP Accessories

No.	Accessories	Model/ Part No.	Description	Applicable Patient
1.	Cuff	98-0084- 95	12cm-19cm, reusable	Adult/Pediatric
2.	Cuff	98-0084- 96	17cm-25cm, reusable	Adult/Pediatric
3.	Cuff	98-0084-	23cm-33cm,	Adult/Pediatric

No.	Accessories	Model/ Part No.	Description	Applicable Patient
		97	reusable	
4.	Cuff	98-0084- 98	31cm-40cm, reusable	Adult/Pediatric
5.	Cuff	KN-232	10cm-19cm, reusable	Adult/Pediatric
6.	Cuff	KN-233	18cm-26cm, reusable	Adult/Pediatric
7.	Cuff	KN-241	25cm-35cm, reusable	Adult/Pediatric
8.	Cuff	KN-243	33cm-47cm, reusable	Adult/Pediatric

25.5 CO₂ Accessories

No.	Accessories	Model/ Part No.	Description	Applicable Patient
1-1	CO ₂ module (sidestream)	LoFlo	Sidestream	
1-2	Sampling cannula	#3475-00	Disposable, non-sterile	Adult/Pediatric/N eonate
2-1	CO ₂ module (mainstream)	CAPONS TAT 5	Mainstream	
2-2	Sampling adapter	#606300	Disposable, non-sterile	Adult
3-1	CO ₂ module (sidestream)	KM7003	Sidestream	
3-2	CO ₂ sampling line	1510012 1	240cm-φ2.5*1.6 , two male heads	Adult/Pediatric/N
3-3	Filter	2500-000 0218	T4F/T3	eonate
4-1	CO ₂ module (mainstream)	KM7012	Mainstream	
4-2	Airway adapter	2301-000 0034	V9 / mainstream	Adult

25.6 IBP Accessories

No.	Accessories	Model/ Part No.	Description	Applicable Patient
1.	IBP transducer	15030121	Disposable	Adult/Pediatric/N
2.	IBP cable	15039057	4 pin, plastic, reusable	eonate

25.7 Other Accessories

No.	Accessories	Specification / Model
1.	Rechargeable lithium battery	HYLB-2260/10.95V/2750mAh
2.	Rechargeable lithium battery	HYLB-2261/10.95V/5500mAh

This page intentionally left blank.

Appendix A Technical Specifications

A.1 Safety Specifications

Standards	Safety standards	IEC 60601-1 IEC 60601-2-27
	Anti electric-shock type	Class I and internally powered device
	Anti electric-shock degree	Type CF with defibrillation protection
	Electromagnetic compatibility	Group I, Class A
	Operation mode	Continuous
Classifications	Degree of protection against harmful ingress of water	IPX2
	Disinfection/sterilization method	Refer to Chapter 22 Cleaning and Disinfection for details.
	Installation method	Non-permanent installation device
	Degree of safety of application in the presence of flammable anesthetic mixture with air or with oxygen or nitrous oxide	The device is not suitable for use in the presence of a flammable anesthetic mixture with air or with oxygen or nitrous oxide

A.2 Environmental Specifications

Environment	Temperature	Relative Humidity (non-condensing)	Atmospheric Pressure
Operating	5°C ~ 40°C	15% ~ 95%	57.0kPa ~ 107.4kPa
Storage and Transportation	-20°C ~ +60°C	10% ~ 95%	50.0kPa ~ 107.4kPa

A.3 Power Supply Specifications

External Power Supply				
Input Voltage	100 -240 V~			
Input Current	t 2.0 – 0.9A			
Frequency	50/60Hz			
Battery				
Configuration	Standard	Optional		
Туре	Lithium ion rechargeable battery	Lithium ion rechargeable battery		
Rated Voltage	10.95 V	10.95 V		
Battery Capacity	2750 mAh	5500 mAh		
Run Time	After the battery is fully charged, NIBP will perform a measurement every 15 minutes in the standard configuration of the monitor, and the continuous working time is not less than 4 hours.	After the battery is fully charged, NIBP will perform a measurement every 15 minutes under the standard configuration of the monitor, and the continuous working time is not less than 8 hours.		
Charging Time	When charged by external AC power supply, after the device is turned off, the charging time is as follows: Time of charging to 90% is less than 4 hours. Time of charging to 100% is less than 5 hours. When charged by external AC power supply, after the device is turned on, the charging time is as follows: Time of charging to 90% is less than 10 hours. Time of charging to 100% is less than 13 hours.	When charged by external AC power supply, after the device is turned off, the charging time is as follows: Time of charging to 90% is less than 8 hours. Time of charging to 100% is less than 10 hours. When charged by external AC power supply, after the device is turned on, the charging time is as follows: Time of charging to 90% is less than 20 hours. Time of charging to 100% is less than 26 hours.		

Shutdown	At least 5 minutes (since the first low battery alarm)
Delay	

A.4 Physical Specifications

Model	AlView V10、AlView PH10	AlView V12、AlView PH12
Main Unit Size	≤290mm×170mm×230mm	≤330mm×170mm×25 mm
(L×W×H)		
Net Weight of the Main Unit	≤ 3 kg	≤4 kg
Display Screen	11.6 inches, color TFT LCD screen	13.3 inches, color TFT LCD screen
	Resolution:	Resolution:
	1366×768 pixels	1920×1080 pixels
Indicators	Power button backlight: 1 (Green) AC power indicator: 1 (Green) Battery status indicator: 1 (Yellow and green) Alarm indicator: 1 alarm indicator (Red and yellow) 1 technical alarm indicator (Red and yellow)	
Speaker	Give tones include but not limited to: alarm tones (45db to 85db), button tones, QRS tones and power-on self-check sound. Support PITCH TONE and multi-level tone modulation. The alarm tones comply with IEC 60601-1-8.	
Connector	AC power input connector: 1 Network connector: 1 USB connector: 2 VGA connector: 1 Equipotential grounding terminal: 1 Multi-function connector: 1 (used as ECG analog output connector, synchronous defibrillation analog output connector or nurse call connector) Parameter connector: 1 ECG/RESP connector 1 NIBP connector	

	2 TEMP connectors
	2 IBP connectors
	1 CO ₂ connector
Thermal	Thermal dot matrix recorder
recorder	Horizontal resolution: 8 dot/mm
	Vertical resolution: 8 dot/mm
	Recording paper width: 50 mm ± 1 mm
	Paper speed: 25 mm/s, 50 mm/s, error ≤±5%

A.5 Signal Outputs Specifications

Auxiliary output	
Standard	Meets the requirements of IEC 60601-1 for short-circuit protection and leakage current
ECG analog output	
Bandwidth	0.5 Hz ~ 40 Hz
(-3dB; reference frequency: 10Hz)	
QRS delay	< 25ms(non-paced)
Output sensitivity	0.4 V/mV5%
Baseline level	2.20 ± 0.2 V
Output impedance	≤ 100 Ω
Duration of short-circuit	Short circuit to ground for 1 minute, no fault after disconnection.
Defibrillation synchronization signal output	
Output impedance	≤ 100 Ω
Maximum time delay	30 ms
Amplitude	High level: 3.5 V to 5 V, providing a maximum of 10 mA output current; Low level: < 0.5 V, receiving a maximum of 5 mA input current.
Pulse width	100 ms ± 10%

Rising and falling time	≤ 1 ms
Duration of short-circuit	Short circuit to ground for 1 minute, no fault after disconnection.
Nurse call signal output	
Amplitude	10~15V
Maximum load current	350mA
Duration of short-circuit	Lasting short-circuits is allowable, and it can return to normal automatically.
Alarm Output	
Alarm delay	The screen shows that the parameter value reaches the alarm condition, and the alarm is not delayed. From the monitor to the remote device, delays 0.5s.
Alarm signal sound pressure level range	45 db(A) to 85 db(A) within a range of one meter

A.6 Data Storage

Patients	100
Trend data	240 hours
Full-disclosure waveforms	140 hours
NIBP measurements	2000 sets
Physiological alarm events	1000events
Technical alarm events	1000events
Reports	20 sets

A.7 Wi-Fi Specifications

Protocol	IEEE 802.11 a/b/g/n (2.4GHz & 5GHz)
Operating	2412 MHz – 2484 MHz
frequency	4.9 GHz – 5.975 GHz
Modulation mode	OFDM with BPSK, QPSK, 16-QAM, and 64-QAM, 802.11b with CCK and DSSS
Wireless security	WPA/WPA2-Personal

features	WPA/WPA2 Enterprise for Client
	EAP-TLS
	EAP-FAST
	EAP-TTLS
	PEAP-MSCHAP-v2
Data security	AES128/256, SHA256/384/512, RSA, ECC, ECDH, RNG, CRC

A.8 ECG Specifications

ECG		
Compliant standards	IEC 60601-2-27: 2011 and IEC 60601-2-25: 2011	
Lead type	3-lead: I, II, III	
	5-lead: I, II, III, aVR, aVL, aVF, V	
	6-lead: I, II, III, aVR, aVL, aVF, Va, Vb	
	12-lead: I, II, III, aVR, aVL, aVF, V1 to V6	
Sampling rate	500Hz	
Bandwidth	0.05 Hz ~ 150 Hz	
Amplitude quantisation	4.9 μV/LSB	
Waveform	6.25mm/s, 12.5mm/s, 25mm/s, 50mm/s	
sweeping speed	error: ≤ ±5%	
Frequency	Diagnostic mode: 0.05 Hz ~ 150 Hz	
response	Monitor mode: 0.5 Hz ~ 40 Hz	
	Surgery mode: 1 Hz~ 20 Hz	
	ST mode: 0.05 Hz ~ 40 Hz	
	Use A and E methods based on IEC 60601-2-25 to determine frequency response.	
Display sensitivity	2.5mm/mV(x1/4), 5mm/mV(x1/2), 10mm/mV(x1), 20mm/mV(x2), Auto	
Common mode rejection ratio	Surgery mode, monitor mode, ST mode > 105dB	
	Diagnostic mode > 90dB	
Input impedance	> 10 MΩ	
Input signal range	-10.0mV ~ +10.0mV (peak-to-peak value)	

Electrode polarization voltage range	±800 mV
Input offset current	≤0.1µA
Baseline recovery time	<5 s after defibrillation
Patient leakage current	10μΑ
System noise	≤30 µV (p-v RTI)
Calibration voltage	1mV, error range ±5%
ESU protection	ESU cutting power: 300 W
	ESU coagulating power: 100 W
	Recovery time: <10 s
	Heart rate change under ESU interference: <±10%
Defibrillation protection	Recovery time of electrode polarization: <10 s
Pace Pulse	
Pulse rejection	It only can suppress non-overshoot pacing pulses with
	an amplitude of ±2mV ~ ±700mV and a pulse width of
	0.1 ms ~ 2 ms. And it can also suppress the pacing
	pulses in IEC 60601-2-27-2011, including the presence of atrial and ventricular pacing pulses. The minimum input slew rate is 5.5V/s RTI
HR	
Measurement range	15bpm ~ 350bpm
Resolution	1 bpm
Measurement accuracy	±1% or ±1 bpm, whichever is greater
Alarm limit setting range	High limit: 16bpm ~ 350bpm
	Low limit: 15bpm ~ 349bpm
Tall T-wave	For T wave with QRS wave of 100ms, QT interval of

rejection capability	350ms, duration of 180ms and amplitude lower than 1.2mV, the heart rate calculation is not affected.	
Minute heart rate averaging	The lastest 8 RR intervals are all in a certain range of average heart beats.	
algorithm	Display refresh rate: 1 beat/s	
Response time to heart rate	Meets the requirements of IEC 60601-2-27: Clause 201.7.9.2.9.101 b) 5).	
changes	From 80 bpm to 120 bpm: less than 8 s	
	From 80 bpm to 40 bpm: less than 8 s	
Accuracy of heart rate meter and its response to irregular rhythm	In compliance with the requirements in Clause 201.7.9.2.9.101 b) 4) of IEC 60601-2-27, the heart rate after 20 seconds of stabilization is displayed as follows:	
	Ventricular bigeminy (waveform A1): 80 bpm	
	Slow alternating ventricular bigeminy (waveform A2): 60 bpm	
	Rapid alternating ventricular bigeminy (waveform A3): 120 bpm	
	Bidirectional systoles (waveform A4): 90 bpm	
Time to alarm for tachycardia	< 11s (applicable to all clauses of IEC 60601-2-27)	
ST Segment Analy	sis	
Measurement range	-2.0 mV~+2.0 mV	
Measurement accuracy	-0.8 mV~0.8 mV: ±0.02 mV or ±10%, whichever is greater.	
	Beyond this range: not defined.	
Resolution	0.01 mV	
ST alarm high limit	(low limit + 0.2 mV) ~ 2.0 mV	
ST alarm low limit	-2.0 mV ~ (high limit - 0.2 mV)	
QT/QTc Analysis		
Measurement range	QT: 200 ms ~ 800ms	
	QTc: 200 ms ~ 800ms	
	QT-HR: 15 to 150 bpm for adult, 15 to 180 bpm for	

	pediatric and neonate
Measurement	QT: 30 ms
accuracy	QTc, QT-HR: not defined
Resolution	QT: 4 ms
	QTc: 1 ms
	QT-HR: 1 bpm
QTc alarm high limit	200 ms ~ 800ms, step: 1 ms
ΔQTc alarm high limit	30 ms ~ 200ms, step: 1 ms

A.9 Resp Specifications

Respiration rate measurement	Adult: 0 rpm ~ 120 rpm		
range	Pediatric and neonate: 0 rpm ~ 150 rpm		
Respiration rate measurement	7 ~ 120 rpm: ±2 rpm or ±2%, whichever is greater		
accuracy	0 ~ 6 rpm: not defined		
Alarm limit setting	Adult	Pediatric and neonate	
range	High limit: 1rpm ~ 120rpm	High limit: 1rpm ~ 150rpm	
	Low limit: 0 rpm ~ 119 rpm	Low limit: 0 rpm ~ 149	
Alarm accuracy	±1 rpm	,	
Apnea alarm delay setting range	5 s ~ 120 s		

A.10 Temp Specifications

Compliant standards	ISO 80601-2-56: 2017
Measurement range	0°C ~50°C (32°F ~122°F)
Measurement accuracy	within the range of $0^\circ\!\mathrm{C} \sim 50^\circ\!\mathrm{C}$, the maximum allowable

	error is ±0.1℃ (without probe)
	within the range of 25°C ~ 45.0°C, the maximum allowable error is ± 0.2 °C within other measurement ranges, the maximum allowable error is ± 0.4 °C
Minimum time for accurate measurement	Body surface: <100 s
System response time	<150 s
Alarm limit setting range	High limit: 0.1 $^{\circ}$ C ~ 50.0 $^{\circ}$ C Low limit: 0.0 $^{\circ}$ C ~ 49.9 $^{\circ}$ C
Alarm accuracy	±0.1℃

A.11 NIBP Specifications

Compliant standards	IEC 80601-2-30: 2018
Measurement method	Manual, Auto, Sequence, ABPM
Automatic measurement mode repetition intervals	1min, 2min, 2.5min, 3min, 5mins, 10min, 15min, 20min, 30min, 1h, 1.5h, 2h, 3h, 4h, 8h, Clock 30min, Clock 1h
Continuous measurement mode time	5 min
Maximum single measurement time	Adult and pediatric: no more than 180s Neonate: no more than 90s
Venipuncture measurement time	Adult and pediatric: no more than 180s Neonate: no more than 90s
Venipuncture pressure setting range	Adult: 80mmHg (10.7kPa) ~ 180mmHg (24kPa) Pediatric: 80mmHg (10.7kPa) ~ 130 mmHg (17.3kPa)

	Neonate: 70mmHg (9.3kPa) ~ 110mmHg (14.7kPa)			
Static pressure measurement range	0 mmHg ~ 300 mmHg (0.0 kPa ~ 40.0 kPa)			
Static pressure measurement accuracy	±3 mmHg (±0.4 kPa)			
Initial inflating	KRK blood pressure module			
pressure setting range	Adult: 80 mmHg -	~ 280 mmHg	(10.6 kPa ~ 3	37.2 kPa)
J	Pediatric: 80 mmHg ~ 210 mmHg (10.6 kPa ~ 27.9 kPa)			
	Neonate: 60 mml	Neonate: 60 mmHg ~ 140 mmHg (7.8 kPa ~ 18.2 kPa)		
	Suntech blood pressure module			
	Adult: 120 mmHg ~ 280 mmHg (15.9 kPa ~ 37.2 kPa)			
	Pediatric: 80 mmHg ~ 250 mmHg (10.6 kPa ~ 33.25 kPa)			
	Neonate: 60 mmHg ~ 140 mmHg (7.8 kPa ~ 18.2 kPa)			
Default value of initial inflating pressure	Adult: 160 mmHg (21.3 kPa) Pediatric: 140 mmHg (18.6 kPa) Newborn: 90 mmHg (12.0 kPa)			
Overvoltage protection	KRK blood pressure module: Adult: ≤297 mmHg (39.5kPa) ±3 mmHg (±0.4kPa) Pediatric: ≤247 mmHg (32.9kPa) ±3 mmHg (±0.4kPa) Neonate: ≤147 mmHg (19.6kPa) ±3 mmHg (±0.4kPa)			
	Suntech blood pressure module: Adults/Pediatric: ≤297 mmHg (39.5 kPa) ±3mmHg (±0.4 kPa)			Č
Monitoring range	Neonate: ≤147 mmHg (19.6 kPa) ±3mmHg (±0.4 kPa) KRK blood pressure module			(±0.7 KF a)
g range	Blood pressure (unit)	Adult	Pediatric	Neonate

	SYS	mmHg	25~290	25~240	25~140
		kPa			
		кга	3.3 ~ 38.6	3.3~31.9	3.3 ~ 18.6
	MAP	mmHg	15~260	15~215	15 ~ 125
		kPa	2.0 ~ 34.6	2.0 ~ 28.6	2.0 ~ 16.6
	DIA	mmHg	10~250	10~200	10~115
		kPa	1.3~33.3	1.3~26.6	1.3 ~ 15.3
	Sunted	h blood pr	essure modu	le	
	Blood (unit)	pressure	Adult	Pediatric	Neonate
	SYS	mmHg	40 ~ 260	40~230	40 ~ 130
		kPa	5.3 ~ 34.6	5.3 ~ 30.6	5.3 ~ 17.3
	MAP	mmHg	26 ~ 220	26~183	26~110
		kPa	3.5 ~ 29.3	3.5 ~ 24.4	3.5 ~ 14.6
	DIA	mmHg	20~200	20~160	20~100
		kPa	2.6 ~ 26.6	2.6~21.3	2.6 ~ 13.3
Monitoring accuracy	Average deviation ≤±5mmHg (±0.67 kPa) Standard deviation ≤8mmHg (1.067 kPa)				
Alarm limit setting range		pressure	Adult	Pediatric	Neonate
	High limit		(26 ~ 290)/	(26 ~ 240)/	(26 ~ 140)/
		limit	(3.5 ~ 38.6)	(3.5 ~ 30.0)	(3.5 ~ 18.6)
	SYS	Low	(25 ~ 289)/	(25 ~ 239)/	(25 ~ 139)/
	limit	iimit	(3.3 ~ 38.5)	(3.3 ~ 31.8)	(3.3 ~ 18.5)

	MAP -	High limit	(16 ~ 260)/ (2.1 ~ 34.6)	(16 ~ 215)/ (2.1 ~ 28.6)	(16 ~ 125)/ (2.1 ~ 16.6)
		Low limit	(15 ~ 259)/ (2.0 ~ 34.5)	(15 ~ 214)/ (2.6 ~ 28.5)	(15 ~ 124)/ (2.6 ~ 16.5)
	DIA	High limit	(11 ~ 250)/ (1.5 ~ 33.3)	(11 ~ 200)/ (1.5 ~ 26.6)	(11 ~ 115)/ (1.5 ~ 15.3)
		Low limit	(10 ~ 249)/ (1.3 ~ 33.1)	(10 ~ 199)/ (1.3 ~ 26.5)	(10 ~ 114)/ (1.3 ~ 15.2)

A.12 SpO₂ Specifications

Compliant standards	ISO 80601-2-61: 2011
Measurement range	KRK SpO ₂ module: 0% ~ 100%
	Nellcor SpO ₂ module: 1% ~ 100%
Measurement accuracy	KRK SpO ₂ module: 70%~100%: ±2% 50%~69%: ±3% 0%~49%: not defined
	Nellcor SpO ₂ module: 70%~100%: ±2% (adult/pediatric) 70%~100%: ±3% (neonate) 70%~100%: ±3% (weak perfusion) 70%~100%: ±3% (adult/neonate, with motion interference)

	40/ 000/ 4 1 5 1	
	1%~69%: not defined	
Sensor	KRK SpO ₂ module:	
	Wavelength: Red light: 660nm, Infrared light: 905nm	
	Maximum optical output power: ≤2mW	
	Nellcor SpO ₂ module:	
	Wavelength: Red light: 660nm, Infrared light: 900nm	
	Maximum optical output power: ≤15mW	
Data update cycle	≤8s	
Perfusion index	KRK SpO ₂ module:	
(PI) measurement range	0.1% ~ 20%, the measurement accuracy is not defined	
	Nellcor SpO ₂ module:	
	0.03% ~ 20%, the measurement accuracy is not defined	
Alarm limit setting range	High limit: 1% ~ 100%	
3.	Low limit: 0% ~ 99%	
Alarm accuracy	70%~100%: ±1%	

A.13 PR Specifications

Alarm limit setting range	High limit: 1 bpm ~ 300 bpm			
	Low limit: 0 bpm ~ 299 bpm			
Alarm accuracy	±1% or ±1bpm, whichever is greater			
PR from NIBP mod	dule			
	KRK blood pressure module Suntech blood pressure module			
Measurement range	30bpm ~ 300bpm	30bpm ~ 220bpm		
Measurement accuracy	±3bpm or ±3%, ±3bpm or ±2%, whichever is greater			
PR from SpO ₂ module				
	KRK SpO2 module	KRK SpO2 module Nellcor SpO2 module		

Measurement range	30bpm ~ 250bpm	20bpm ~ 250bpm		
Measurement accuracy	±2bpm or ±2%, whichever is greater	±3bpm		
PR from IBP module				
Measurement range	20bpm ~ 250bpm			
Measurement accuracy	±3bpm			

A.14 CO₂ Specifications

Compliant standards	ISO 80601-2-55: 2018
Measurement mode	Sidestream and mainstream
Measurement range	0 mmHg ~ 150 mmHg (0 kPa ~ 20.0 kPa)
	0 mmHg ~ 40 mmHg (0 kPa ~ 5.3 kPa), the error is ±2 mmHg (±0.26 kPa)
Measurement accuracy	41 mmHg ~ 70 mmHg (5.5 kPa ~ 9.3 kPa), the error is ±5%
	71 mmHg ~ 100 mmHg (9.4 kPa ~ 13.3 kPa), the error is ±8%
	101 mmHg ~ 150 mmHg (13.4 kPa ~ 20.0 kPa), the error is ±10%
Alarm limit	High limit: 0.1mmHg ~ 150mmHg (0 kPa ~ 20kPa)
setting range	Low limit: 0 mmHg ~ 149.9mmHg (0 kPa ~ 19.9kPa)
Alarm accuracy	±1mmHg (±0.13kPa)
Sampling rate (sidestream)	50 ml/min fixed flow rate
Response time	Sidestream:
and rise time	response time < 9 s (KM7003 CO ₂ module)

	response time < 7 s (LoFlo CO ₂ module)
	Mainstream: rise time <60 ms
Drift of	Short-term: The module works for more than 4 hours, and the maximum drift does not exceed 0.8mmHg.
measurement accuracy	Long-term: The module works for more than 120 hours and still meets the specified performance standards.
	The time of reaching the specified working performance after the CO ₂ module is switched on:
Warm-up time	Mainstream: Parameters can be displayed within 15 s, and the ambient temperature is 25°C, and it takes 2 minutes to reach the specified working performance standard.
	Sidestream: Parameters can be displayed within 20 s, and the ambient temperature is 25°C, and it takes 2 minutes to reach the specified working performance standard.
Maximum time interval of intervention	When the sampling gas temperature is 37 degrees, the indoor temperature is 23 degrees, and the sampling relative humidity is 100%, the maximum time interval for the operator to intervene in the water and gas treatment system is 120 hours.
Apnea	
Measurement	Sidestream: 2 rpm~150 rpm
range	Mainstream: 0 rpm~150 rpm
Measurement accuracy	±2 rpm
Apnea alarm delay	0~60 s

A.15 IBP Specifications

Compliant standards	IEC 60601-2-34: 2011	
	Static monitoring	Dynamic monitoring
Measurement range	-50mmHg ~ 300mmHg (-6.7kPa ~ 40.0kPa)	ART: 0mmHg ~ 300mmHg (0kPa ~ 40.0kPa)
		PA: -6mmHg ~ 120mmHg

		(-0.80kPa ~ 16.0kPa)	
		CVP/LAP/RAP/ICP:	
		-10mmHg ~ 40mmHg	
		(-1.3kPa ~ 5.3kPa)	
		AUXP1/AUXP2:	
		-50mmHg ~ 300mmHg	
		(-6.7kPa ~ 40.0kPa)	
Measurement	±3mmHg(±0.4kPa)	±4mmHg (±0.5kPa) or	
accuracy		±4%, whichever is greater	
Resolution	1mmHg (0.1kPa)	1mmHg (0.1kPa)	
Alarm limit setting	ART (SYS, DIA, MAP):		
range (adult)	High limit: 1mmHg ~ 300mmHg (0.1kPa ~ 40.0kPa)		
	Low limit: 0mmHg ~ 299	9mmHg (0kPa ~ 36.7kPa)	
	PA (SYS, DIA, MAP):		
	High limit: 1mmHg ~ 12	0mmHg (0.1kPa ~ 16.0kPa)	
	Low limit: 0mmHg ~ 119	9mmHg (0kPa ~ 15.8kPa)	
	CVP, RAP, LAP, ICP (SYS	S, DIA, MAP):	
	High limit: -9mmHg ~ 40	0mmHg (-1.2kPa ~ 5.3kPa)	
	Low limit: -10mmHg ~ 3	39mmHg (-1.3kPa ~ 5.2kPa)	
Alarm accuracy	±1mmHg (±0.1kPa)		
Pressure sensor	Sensitivity: 5V/Volt/mmHg)	
	Impedance range: 300-30	Ω000	
IBP Transducer volume output	< 0.02mm³/100mmHg		

Appendix B Alarm Messages

This chapter lists only the most important physiological and technical alarm messages. Some messages appearing on your monitor may not be included.

B.1 Physiological Alarm Messages

Alarm Category	Alarm Messages	Default Priority
Conoral	XX High	Med
General	XX Low	Med
	Asystole	High
	V-Fib/V-Tach	High
	Vent Tachy	High
	Vent Brady	High
	Extreme Tachy	High
	Extreme Brady	High
	Nonsus V-Tach	Med
	Vent Rhythm	Med
Arrhythmia	Run PVCs	Med
	Pair PVCs	Med
	R on T	Med
	Vent Bigeminy	Med
	Vent Trigeminy	Med
	PVCs/min	Med
	Multiform PVC	Med
	PVC	Med
	HR High	Med

Alarm Category	Alarm Messages	Default Priority
	HR Low	Med
	SV Tachy	Med
	SV Brady	Med
	A-Fib (HR High)	Med
	A-Fib	Med
	A-Fib End	Med
	Irr Rhythm	Med
	Irr Rhy End	Med
	Pause	Med
	Pauses/min	Med
	Missed Beats	Med
	Pacer Not Pacing	Med
	Pacer Not Capture	Med
	PAC	Med
	PACs Couplet	Med
	SV Bigeminy	Med
	SV Trigeminy	Med
	2nd Degree A-V Block	Med
	1st Degree A-V Block	Med
500	Extreme Tachy	High
ECG	Extreme Brady	High
Resp	Apnea	High
0.0	SpO₂ Desat	High
SpO ₂	SpO ₂ Event	Low

Alarm Category	Alarm Messages	Default Priority
PR	Pulse not found	High
CO ₂	Apnea	High

Note: "XX" represents a measurement or parameter label, such as HR, ST, RR, \mbox{SpO}_2 or PR, etc.

B.2 Technical Alarm Messages

Default Priority	Alarm Source	Alarm Messages
	System	Battery low, unknown error
High	CO ₂	CO ₂ sensor failure, CO ₂ sensor temperature too high
	ECG / SpO ₂	Lead(s) off, Probe off
Medium	CO ₂	CO ₂ sensor off, Zero required, CO ₂ out of range, check airway adapter, check sampling line, zero failed (in zero operation window)
Low	NIBP	Self test failed, system error, measurement timeout, signal weak, cuff error, air leakage, pressure error, out of range, arm motion, overpressure detected, signal saturation, test air leakage
	Temp	Self test failed

B.3 Nellcor SpO₂ Alarm Messages

Default Priority	Alarm Event	Remarks
High	SpO ₂ INOP	Such alarm will not display on alarm

Default Priority	Alarm Event	Remarks
	SpO ₂ firmware error	information area, but it will be recorded as alarm event.
	Communication error	
	SpO ₂ sensor faulty	
	SpO ₂ hardware error	
	SpO ₂ module faulty	
	SpO ₂ sensor error	It means that the SpO ₂ sensor identification fails.
Madiona	SpO ₂ sensor disconnected	The sensor cable or extension cable is not connected to the monitor.
Medium	SpO₂sensor off	It means that the sensor cable is connected, but the sensor is out of the measuring site.

Appendix C Default Settings

This chapter lists only the most important default settings of your monitor as it is delivered from the factory.

Note

If your monitor has been ordered preconfigured to your requirements, the settings at delivery will be different from those listed here.

C.1 Alarm Default Settings

Item Parameter		Adult	Pediatric	Neonate
	Switch	On	On	On
	High	120 bpm	160 bpm	200 bpm
	Low	50 bpm	75 bpm	100 bpm
	Priority	Med	Med	Med
HR/PR	Alarm Outputs	Off	Off	Off
	Alarm Source	Auto	Auto	Auto
ST-I, ST-II, ST-III,	Switch	Off	Off	Off
ST-aVR, ST-aVL, ST-aVF, ST-V1,	High	0.2mV	0.2mV	0.2mV
ST-V2, ST-V3, ST-V4, ST-V5,	Low	-0.2mV	-0.2mV	-0.2mV

Item		Adult	Pediatric	Neonate
Parameter		710011	· oaiaiio	110011410
ST-V6, ST-V, ST-Va, ST-Vb	Priority	Med	Med	Med
	Alarm Outputs	Off	Off	Off
	Switch	Off	Off	Off
	High	500	480	460
QTc	Priority	Med	Med	Med
	Alarm Outputs	Off	Off	Off
	Switch	Off	Off	Off
	High	60	60	60
ΔQTc	Priority	Med	Med	Med
	Alarm Outputs	Off	Off	Off
	High	30 rpm	30 rpm	100 rpm
	Low	8 rpm	8 rpm	30 rpm
RR	Switch	On	On	On
KK	Priority	Med	Med	Med
	Alarm Outputs	Off	Off	Off
Annon	Switch	On	On	On
Apnea	Priority	High	High	High

Item		Adult	Pediatric	Neonate
Parameter	Parameter			
	Apnea Delay	5-120s	10-60s	10-60s
	Alarm Outputs	Off	Off	Off
	High	38.0 ℃	38.0 ℃	38.0 ℃
	Low	35.0 ℃	35.0 ℃	35.0 ℃
Temp1,	Switch	On	On	On
Temp2	Priority	Med	Med	Med
	Alarm Outputs	Off	Off	Off
	ΔΤ	2.0 ℃	2.0 ℃	2.0 ℃
	Switch	On	On	On
ΔΤ	Priority	Med	Med	Med
	Alarm Outputs	Off	Off	Off
	Switch	On	On	On
	High	100 %	100 %	95 %
C~O	Low	90 %	90 %	90 %
SpO ₂	Priority	Med	Med	Med
	Alarm Outputs	Off	Off	Off
	Switch	On	On	On
SpO ₂ Desat	Low	80 %	80 %	80 %
	Priority	High	High	High

Item		Adult	Pediatric	Neonate
Parameter		riduit	- Calatilo	rtoonato
	Alarm Outputs	Off	Off	Off
	Switch	Off	Off	Off
	High	2 %	2%	2%
SpO ₂ Event	Priority	Low	Low	Low
	Alarm Outputs	Off	Off	Off
	Switch	On	On	On
	High	120 bpm	160 bpm	200 bpm
	Low	50 bpm	75 bpm	100 bpm
PR	Priority	Med	Med	Med
	Alarm Outputs	Off	Off	Off
	Alarm Source	Auto	Auto	Auto
	Switch	On	On	On
	High	160 mmHg	120 mmHg	90 mmHg
NIBP-S	Low	90 mmHg	70 mmHg	40 mmHg
NIBP-5	Priority	Med	Med	Med
	Alarm Outputs	Off	Off	Off
	Switch	On	On	On
NIBP-D	High	90 mmHg	70 mmHg	60 mmHg
	Low	50 mmHg	40 mmHg	20 mmHg

Item Parameter		Adult	Pediatric	Neonate
	Priority	Med	Med	Med
	Alarm Outputs	Off	Off	Off
	Switch	On	On	On
	High	110 mmHg	90 mmHg	70 mmHg
AUDD M	Low	60 mmHg	50 mmHg	25mmHg
NIBP-M	Priority	Med	Med	Med
	Alarm Outputs	Off	Off	Off
	Switch	On	On	On
	High	50mmHg	50mmHg	45mmHg
EtCO ₂	Low	25mmHg	25mmHg	30mmHg
_	Priority	Med	Med	Med
	Alarm Outputs	Off	Off	Off
	Switch	On	On	On
	High	4mmHg	4mmHg	4mmHg
FiCO ₂	Low	0	0	0
_	Priority	Med	Med	Med
	Alarm Outputs	Off	Off	Off
ART-S/	Switch	On	On	On
ART-D/	High	200 mmHg	160 mmHg	140 mmHg
ART-M	Low	10 mmHg	10 mmHg	10mmHg

Item Parameter		Adult	Pediatric	Neonate
	Priority	Med	Med	Med
	Alarm Outputs	Off	Off	Off
	Switch	On	On	On
DA 0/	High	120 mmHg	100 mmHg	90 mmHg
PA-S/ PA-D/	Low	10 mmHg	10 mmHg	10mmHg
PA-M	Priority	Med	Med	Med
	Alarm Outputs	Off	Off	Off

C.2 System Default Settings

Screen	Item	Default Setting
	Lead	Auto
	ECG1	II
	ECG2	1
ECC Setup	Speed	25mm/s
ECG Setup	Gain	x 1
	Filter	Monitor
	Notch Filter	On
	Grid	Off
	ST Analysis	Off
ST Setup	ST Segment	Off
	Display Markers	Off
QT Setup	QT Analysis	Off

Screen	Item	Default Setting	
	QT Analysis Lead	All	
	QTc Formula	Hodges	
	Speed	6.25mm/s	
Danie Oatum	Gain	×2	
Resp Setup	Resp Lead	II	
	RR Source	Auto	
	Speed	25mm/s	
	Display PI	Off	
SpO ₂ Setup	PR Source	Auto	
	NIBP Simul.	Off	
	Sat-Seconds	Off	
	Temp1 Label	Temp1	
Temp Setup	Temp2 Label	Temp2	
Unit		$^{\circ}$	
	Mode	Manual	
	Limb	Left Arm	
	Interval	15min	
	Unit	mmHg	
NIBP Setup	Initial Pressure	Adult: 160 mmHg Pediatric: 140 mmHg Neonate: 90 mmHg	
	Sequential Mode	Period	
	Venipuncture	Auto	
	Sequence (Period)	Phase Duration Interval	

Screen	Item	Default	Setting	
		Α	1h	10min
		В	12h	15min
		С	8h	30min
		D	4h	15min
		Е	Off	
		F	Off	
		G	Off	
		Phase	Duration	Interval
		A	Current time - Current time + 1 hour	10min
	Sequence (Duration)	В	Current time +1 hour - 22:00 on that day	15min
		С	22:00 on that day - 6:00 the next day	30min
		D	6:00 on the second day - 24 hours on the second day	15min
		E	Off	
		F	Off	
		G	Off	
CO ₂ Setup	Speed	12.5mm	n/s	

Screen	Item	Default Setting
	Gain	X1/2
	Unit	mmHg
	Temp(°C)	35
	CO2 Flow	50ml/min
	Period	10s
	Balance Gas	Air
	Gas Compensation	16
	AG	0
	Atmospheric Pressure	760mmHg
	IBP Label	IBP1: ART IBP2: PA
	Calculation Mode	Dynamic
	Average Time	8s
	Pressure Unit	mmHg
	CVP Unit	cmH2O
IBP Setup	ICP Unit	mmHg
	Speed	25mm/s
	Filter	12.5Hz
	Scale	Auto
	Top Scale	IBP1: 300 IBP2: 120
	Bottom Scale	0
Normal Screen	Waveform 1	ECG II
Setup	Waveform 2	ECG I

Screen	Item	Default Setting
	Waveform 3	Resp
	Waveform 4	SpO ₂
	Parameter 1	ECG
	Parameter 2	Resp
	Parameter 3	SpO ₂
	Parameter 4	NIBP
	Parameter 5	Temp1
	Key Volume	3
	Beat Volume	2
	Alarm Volume	6
System Setup	Screen Brightness	6
	Beat	Mode 2
	Date Format	YYYY-MM-DD
	Time Mode	12 hours
	Туре	Adult
	Gender	Unspecified
Patient Info	Height	cm
	Weight	kg
	Paced	No
	Physio. Alarm Latch	Off
Maintenance - Alarm	Alarm Audio Paused Time	2min
	High Alarm Audio Interval(s)	10

Screen	Item	Default Setting
	Med Alarm Audio Interval(s)	15
	Low Alarm Audio Interval(s)	25
	ARR - V-Fib/V-Tach Off	Enable
	ECG lead off	Low
	IBP No Transducer	Low
	SPO ₂ Sensor Off	Low
	Apnea Off	Disable

Appendix D Typical Pressures and CO₂ Readings at Altitudes

	Atmospheric	EtCO ₂ Reading		
Altitude	Pressure (mmHg)	(%)	(mmHg)	
0m	760	5	38.0	
70m	754	5	37.7	
100m	751	5	37.5	
200m	743	5	37.1	
1500m	641	5	32.0	
3000m	537	5	26.8	
5000m	420	5	21.0	

This page intentionally left blank.

Appendix E EMC Compliance

Table 1
Guidance and manufacturer's declaration-electromagnetic emission for all EQUIPMENT and SYSTEMS

The Patient Monitor is intended for use in the electromagnetic environment specified below. The customer or the user of the equipment or system should assure that it is used in such an environment.

one and a decare that it is deed in each an environment.			
Emissions test	Compliance	Electromagnetic environment-guidance	
RF emissions CISPR 11	Group 1	Patient Monitor uses RF energy only for its internal function. Therefore, its RF emissions are very low and are not likely to cause any interference in nearby electronic equipment.	
RF emissions CISPR 11	Class A	Patient Monitor is suitable for use in all establishments other than domestic and those directly connected to the	
Harmonic emissions IEC 61000-3-2	Class A	public low-voltage power supply network that supplies buildings used for domestic purposes.	
Voltage fluctuations/flicker emissions IEC 61000-3-3	Complies		

Table 2
Guidance and manufacturer's declaration-electromagnetic immunity for all EQUIPMENT and SYSTEMS

The Patient Monitor is intended for use in the electromagnetic environment specified below. The customer or the user of the equipment or system should assure that it is used in such an environment.

Immunity test	IEC60601 test level	Compliance level	Electromagnetic environment -guidance
Electrostatic discharge (ESD) IEC61000-4-2	±8kV contact ±2kV, ±4kV, ±8kV, ±15kV air	±8kV contact ±2kV, ±4kV, ±8kV, ±15kV air	Floors should be wood, concrete or ceramic tile. if floors are covered with synthetic material, the relative humidity should be at least 30%.
Electrical fast transient/burst IEC61000-4-4	±2kV for power supply lines ±1 kV for input/output lines	±2kV for power supply lines ±1 kV for input/output lines	Mains power quality should be that of a typical commercial or hospital environment.
Surge IEC 61000-4-5	±1kV differential mode ±2kV common mode	±1kV differential mode ±2kV common mode	Mains power quality should be that of a typical commercial or hospital environment.
Voltage dips, short interruptions and voltage variations on power supply input lines IEC61000-4-11	$0 \% U_T; 0.5$ cycle g) At 0° , 45° , 90° , 135° , 180° , 225° , 270° and 315° $0 \% U_T; 1$ cycle and $70 \% U_T;$ $25/30$ cycles Single phase: at 0° $0 \% U_T;$	$0 \% U_T; 0.5$ cycle g) At $0^{\circ}, 45^{\circ}, 90^{\circ}, 135^{\circ}, 180^{\circ}, 225^{\circ}, 270^{\circ}$ and 315° $0 \% U_T; 1$ cycle and $70 \% U_T; 25/30$ cycles Single phase: at 0°	Mains power quality should be that of a typical commercial or hospital environment. If the user of the equipment or system requires continued operation during power mains interruptions, it is recommended that the equipment or system be powered from an

	250/300 cycle	0 % U _T ; 250/300 cycle	uninterruptible power supply or a battery.
Power frequency (50Hz/60Hz) magnetic field IEC61000-4-8	30A/m	30A/m	Power frequency magnetic fields should be at levels characteristic of a typical location in a typical commercial or hospital environment.

NOTE: U_T is the a.c. mains voltage prior to application of the test level.

Table 3
Guidance and manufacturer's declaration – electromagnetic immunity for EQUIPMENT and SYSTEM that are not LIFE-SUPPORTING

Patient Monitor is intended for use in the electromagnetic environment specified below. The customer or the user of Patient Monitor should assure that it is used in such an electromagnetic environment.

Immunity test	IEC 60601 test level	Compliance level	Electromagnetic environment - guidance
Conducted RF IEC	3 Vrms 150 kHz to 80 MHz	3 V 150 kHz to 80 MHz	Portable and mobile RF communications equipment should be used no closer to any part of Patient Monitor, including cables, than the
61000-4-6	6 V in ISM and amateur radio bands between 0,15 MHz and 80 MHz	6 V in ISM and amateur radio bands between 0,15 MHz and 80 MHz	recommended separation distance calculated from the equation applicable to the frequency of the transmitter.
		3 V/m	Recommended separation distance
Radiated	3 V/m 80 MHz to 2.7 GHz	80 MHz to 2.7 GHz	$d = \left[\frac{3.5}{V_{\perp}}\right] \sqrt{P}$
RF IEC 61000-4-3	385 MHz-5785 MHz Test specifications for ENCLOSURE PORT IMMUNITY to RF wireless communication equipment (Refer to table 9 of IEC 60601-1-2: 2014)	385 MHz-5785 MHz Test specifications for ENCLOSURE PORT IMMUNITY to RF wireless communication equipment (Refer to table 9 of IEC 60601-1-2: 2014)	$d = \left[\frac{12}{V_2}\right]\sqrt{P}$ $d = \left[\frac{3.5}{E_1}\right]\sqrt{P}$ $80\text{MHz to }800\text{MHz}$ $d = \left[\frac{7}{E_1}\right]\sqrt{P}$ 800MHz $to 2.7\text{GHz}$ Where P is the maximum output power rating of the transmitter in watts (W) according to the transmitter

manufacturer and d is the recommended separation distance in metres (m).b Field strengths from fixed RF transmitters. as determined by an electromagnetic site survey, a should be less than the compliance level in each frequency range.b Interference may occur in the vicinity of equipment marked with the following symbol. $\left(\left(\bigodot \right) \right)$

NOTE 1: At 80 MHz and 800 MHz, the higher frequency range applies.

NOTE 2: These guidelines may not apply in all situations. Electromagnetic propagation is affected by absorption and reflection from structures, objects and people.

a: The ISM (industrial, scientific and medical) bands between 150 kHz and 80 MHz are 6,765 MHz to 6,795 MHz; 13,553 MHz to 13,567 MHz; 26,957 MHz to 27,283 MHz; and 40,66 MHz to 40,70 MHz. The amateur radio bands between 0,15 MHz and 80 MHz are 1,8 MHz to 2,0 MHz, 3,5 MHz to 4,0 MHz, 5,3 MHz to 5,4 MHz, 7 MHz to 7,3 MHz, 10,1 MHz to 10,15 MHz, 14 MHz to 14,2 MHz, 18,07 MHz to 18,17 MHz, 21,0 MHz to 21,4 MHz, 24,89 MHz to 24,99 MHz, 28,0 MHz to 29,7 MHz and 50,0 MHz to 54,0 MHz.

b: Field strengths from fixed transmitters, such as base stations for radio (cellular / cordless) telephones and land mobile radios, amateur radio, AM and FM radio broadcast and TV broadcast cannot be predicted theoretically with accuracy. To assess the electromagnetic environment due to fixed RF transmitters, and electromagnetic site survey should be considered. If the measured field strength in the location in which Patient Monitor is used exceeds the applicable RF compliance level above, the Patient Monitor should be observed to verify normal operation. If abnormal performance is observed, additional measures may be necessary, such as re-orienting or relocating the Patient Monitor.

c: Over the frequency range 150 kHz to 80 MHz, field strengths should be

less than 3V/m.

Table 4
Recommended separation distances between portable and mobile RF communications equipment and the equipment or system for EQUIPMENT and SYSTEM that are not LIFE-SUPPORTING

The Patient Monitor is intended for use in an electromagnetic environment in which radiated RF disturbances are controlled. The customer or the user of the equipment or system can help prevent electromagnetic interference by maintaining a minimum distance between portable and mobile RF communications equipment (transmitters) and the equipment or system as recommended below, according to the maximum output power of the communications equipment.

	Separation distance according to frequency of transmitter (m)			
Rated maximum output power of transmitter (W)	150kHz to 80MHz outside ISM and amateur radio bands $d = \left[\frac{3.5}{V_{\perp}}\right]\sqrt{P}$	150kHz to 80MHz in ISM and amateur radio bands $d = \left[\frac{12}{V_2}\right]\sqrt{P}$	80 MHz to 800 MHz $d = \left[\frac{3.5}{E_{\perp}}\right]\sqrt{P}$	800 MHz to 2.7 GHz $d = \left[\frac{7}{E_1}\right] \sqrt{P}$
0.01	0.12	0.20	0.035	0.07
0.1	0.38	0.63	0.11	0.22
1	1.2	2.00	0.35	0.70
10	3.8	6.32	1.10	2.21
100	12	20.00	35	70

For transmitters rated at a maximum output power not listed above, the recommended separation distance d in metres (m) can be determined using the equation applicable to the frequency of the transmitter, where p is the maximum output power rating of the transmitter in watts (W) according to the transmitter manufacturer.

NOTE 1: At 80 MHz and 800 MHz, the separation distance for the higher frequency range applies.

NOTE 2: These guidelines may not apply in all situations. Electromagnetic propagation is affected by absorption and reflection from structures, objects and people.

§15.19 Labeling requirements.

This device complies with part 15 of the FCC Rules. Operation is subject to the following two conditions: (1) This device may not cause harmful interference, and (2) this device must accept any interference received, including interference that may cause undesired operation.

§ 15.21 Information to user.

Any Changes or modifications not expressly approved by the party responsible for compliance could void the user's authority to operate the equipment.

§ 15.105 Information to the user.

Note: This equipment has been tested and found to comply with the limits for a Class B digital device, pursuant to part 15 of the FCC Rules. These limits are designed to provide reasonable protection against harmful interference in a residential installation. This equipment generates uses and can radiate radio frequency energy and, if not installed and used in accordance with the instructions, may cause harmful interference to radio communications. However, there is no guarantee that interference will not occur in a particular installation. If this equipment does cause harmful interference to radio or television reception, which can be determined by turning the equipment off and on, the user is encouraged to try to correct the interference by one or more of the following measures:

- -Reorient or relocate the receiving antenna.
- -Increase the separation between the equipment and receiver.
- -Connect the equipment into an outlet on a circuit different from that to which the receiver is connected.
- -Consult the dealer or an experienced radio/TV technician for help.

P/N: 3502-2530019 Revision: V1.2

This equipment complies with FCC radiation exposure limits set f orth for anuncontrolled environment. This equipment should be in stalled and operated withminimum distance 20cm between the ra diator & your body.

Operations in the 5.15-5.35GHz band are restricted to indoor usage only.

Shenzhen Creative Industry Co., Ltd.

Manufacturer address: Floor 5, BLD 9, BaiWangXin High-Tech Industrial Park, Songbai Road, Xili Street, Nanshan District, 518110

Shenzhen, PEOPLE'S REPUBLIC OF CHINA

Tel: +86-755-26431658 Fax: +86-755-26430930

Website: www.creative-sz.com Email: info@creative-sz.com