

Column Stand

for ISOVOLT and ERESKO X-ray Equipment



The column-stand has been designed to accommodate commonly used stationary and portable X-ray system setups and facilitate various types of X-ray inspections on a safe and flexible mobile platform.

It contains a robust chassis equipped with different wheel-sets (depending on the ground surface), a column stand with a height adjustable and rotatable holding fixture, a carrier plate for X-ray generators and accessories and a number of tube-yokes with quick locks and brakes allowing rotation and swivel. Additionally, the horizontal offset can be further extended by means of an optional telescopic holding fixture.

Lifting range goes from approx. 500 mm (19.7") to approx. 2700 mm (106.3") and can be ergonomically adjusted by a self-arresting crank drive.

The carrier plate of the column stand provides space for a complete bi-polar ISOVOLT Titan E generator set including a standard cooler and the required counterbalance. Cable clamps and ties are attached to support and simplify High-Voltage cable routing.



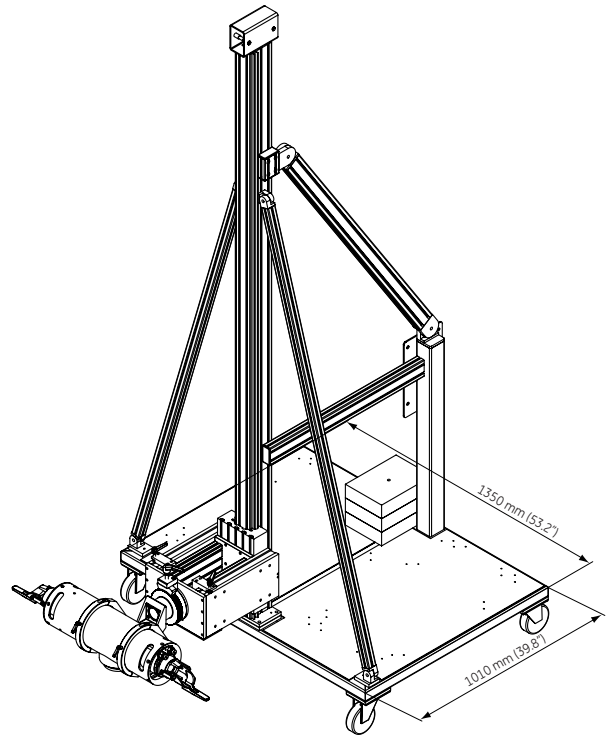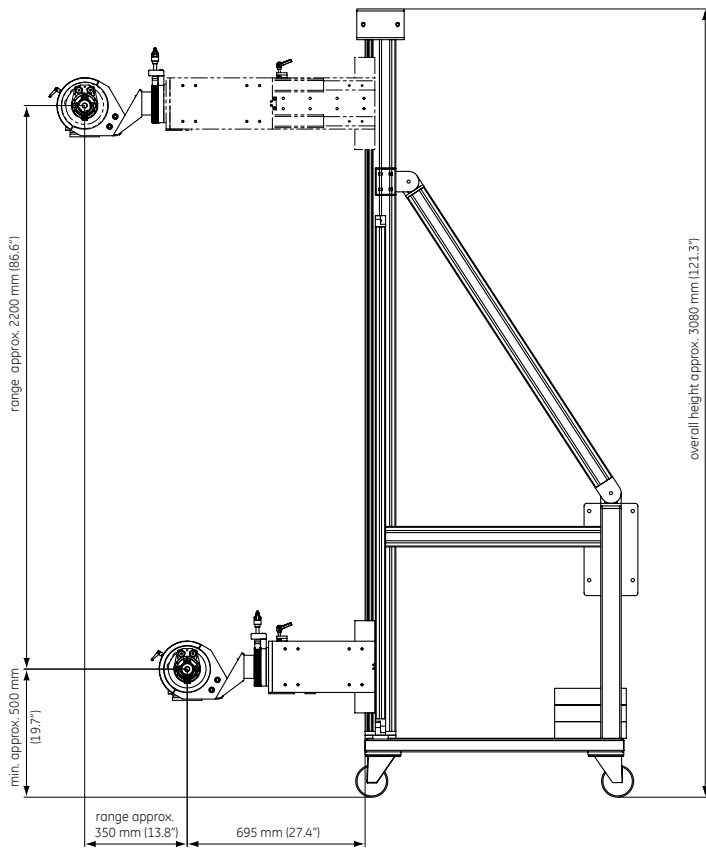

Column Stand with Tube Yoke for ISOVOLT 420/450 kV Tubehousing 2553652

Column Stand with Tube Yoke for ISOVOLT 420 kV Tubehousing 2553622


Column Stand with Tube Yoke for ISOVOLT 225 kV Tubehousing 2553632

Column Stand with Tube Yoke for ISOVOLT 160 kV Tubehousing 2553642

Telescopic Holding Fixture 6313370

Column Stand with Support Fork for ERESKO 42 MF3/4 2553701

Column Stand with Support Fork for ERESKO 65 MF3/4 2553702

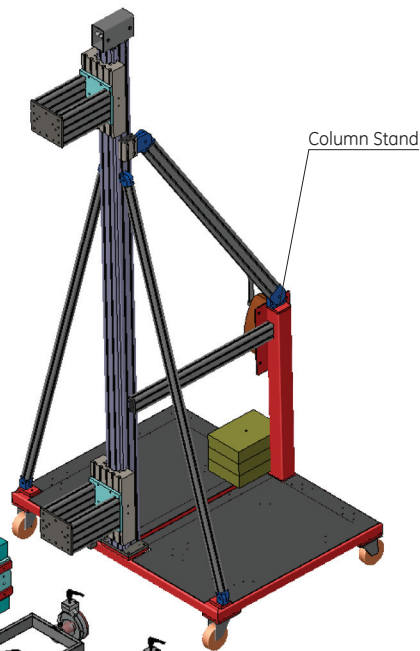

www.ge-mcs.com

GEIT-30058EN (11/10)

© 2010 General Electric Company. All Rights Reserved. Specifications are subject to change without notice. GE is a registered trademark of General Electric Company. Other company or product names mentioned in this document may be trademarks or registered trademarks of their respective companies, which are not affiliated with GE.

Contact: GE Sensing & Inspection Technologies GmbH, Bogenstrasse 41, 22926 Ahrensburg, Germany, T +49 (0)4102 807 0