

GozioHealth: Fusion Beacon

Model: FUSION1

Version: 0.9 - DRAFT

GETTING STARTED GUIDE



FCC Compliance Statement

This device complies with Part 15 of the FCC Rules. Operation is subject to the following two conditions: (1) this device may not cause harmful interference, and (2) this device must accept any interference received, including interference that may cause undesired operation.

CAUTION

Change or modification not expressly approved by the party responsible for compliance could void the user's authority to operate this equipment. This equipment has been tested and found to comply with the limits for a Class B digital device, pursuant to Part 15 of the FCC Rules. These limits are designed to provide reasonable protection against harmful interference in a residential installation. This equipment generates, uses and can radiate radio frequency energy and, if not installed and used in accordance with the instructions, may cause harmful interference to radio communications. However, there is no guarantee that interference will not occur in a particular installation. If this equipment does cause harmful interference to radio or television reception, which can be determined by turning the equipment off and on, the user is encouraged to try to correct the interference by one or more of the following measures:

- Reorient or relocate the receiving antenna.
- Increase the separation between the equipment and receiver.
- Connect the equipment into an outlet on a circuit different from that to which the receiver is connected.
- Consult the dealer or an experienced radio/TV technician for help.


CAUTION

Any changes or modifications not expressly approved by the grantee of this device could void the user's authority to operate the equipment.

RF Exposure Warning

This equipment must be installed and operated in accordance with provided instructions and the antenna(s) used for this transmitter must be installed to provide a separation distance of at least 2.5 cm from all persons and must not be co-located or operating in conjunction with any other antenna or transmitter. End-users and installers must be provided with antenna installation instructions and transmitter operating conditions for satisfying RF exposure compliance.

Fusion Beacon Components

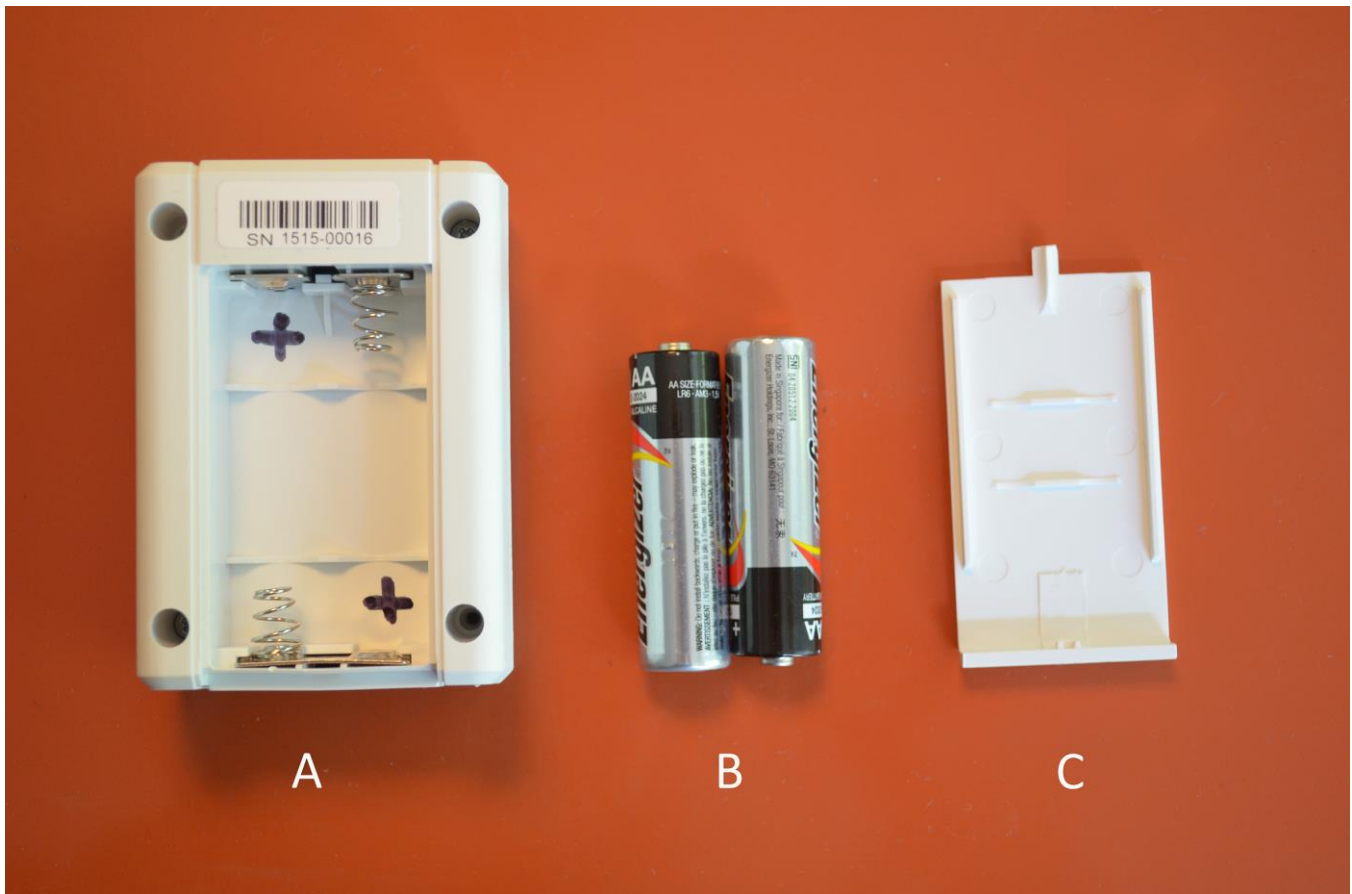


A. Fusion Beacon enclosure with battery cover removed

B. Two 1.5V Alkaline Batteries – Size AA

C. Battery Cover

Getting Started

1. Insert AA Batteries into the battery compartment of the Fusion Beacon as shown. Be careful to observe correct battery polarity.

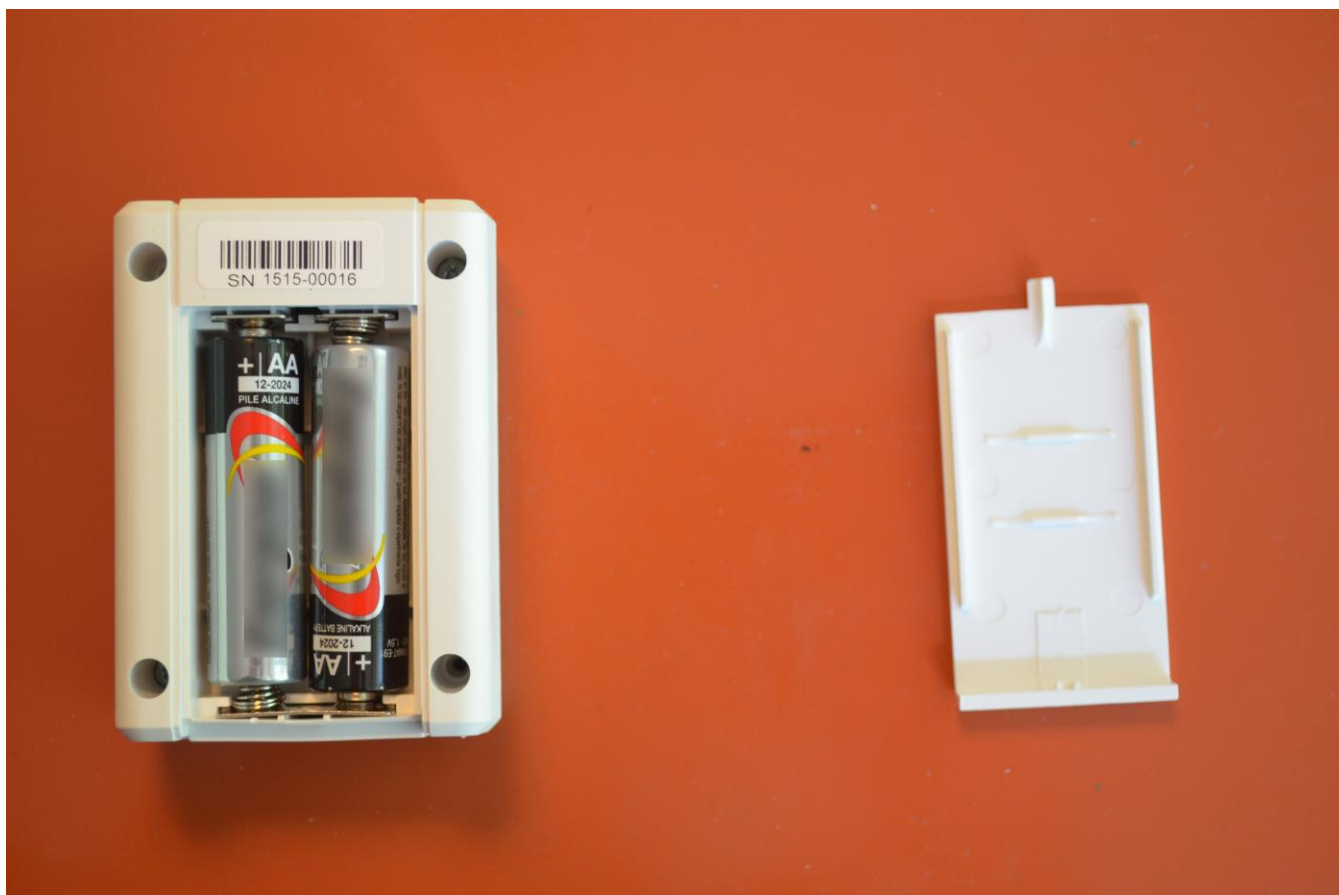

2. Attach Batter Cover by first placing cover over the battery compartment as show, then sliding cover closed until a 'click' is detected and the bottom of the batter cover is flush with the bottom of the fusion beacon.



3. Once the Fusion Beacon's batteries are properly inserted the beacon will automatically start advertising its presence and will continue to do so until the batteries are either removed or depleted.

No further user action is required.

Gozio and Gozio Health is a trademark of Gozio Inc. All other trademarks referenced, depicted, or otherwise used in connection with the Services (the "Third-Party Trademarks") belong to their respective owners or licensees and Gozio Inc. is not affiliated with, sponsored by, or otherwise associated with such entities unless such a relationship is explicitly identified in the Services. The Third-Party Trademarks may not be used to disparage any applicable third-party, any of their products or services, or in any manner in which, in our reasonable judgment, may damage any goodwill in the Third-Party Trademarks.