



Medtronic

Activa® SC

37602

Multi-program neurostimulator

Implant manual

! USA Rx only

CE0123
2010

Explanation of symbols on product or package labeling

Refer to the appropriate product for symbols that apply.



Open here



Do not reuse



Do not resterilize



Sterilized using ethylene oxide



Consult instructions for use



Date of manufacture



Manufacturer



Use by



Temperature limitation



Serial number

CE0123

Conformité Européenne (European Conformity). This symbol means that the device fully complies with AIMD Directive 90/385/EEC (NB 0123).



Authorized representative in the European Community



For USA audiences only



Do not use if package is damaged

PIN No.

Pin number

Medtronic®, Activa®, and SoftStart/Stop® are trademarks of Medtronic, Inc., registered in the U.S. and other countries.

Table of contents

Description 9

Package contents 9

Patient identification card 9

Device specifications 9

Declaration of conformity 12

Instructions for use 13

Verifying neurostimulator operation 13

Connecting the extension to the neurostimulator 13

Implanting the neurostimulator 15

Checking system integrity 16

Completing the implant procedure 16

Refer to the indications sheet for indications and related information.

Refer to the appropriate information for prescribers booklet and any additional associated product information for contraindications, warnings, precautions, component disposal, and other important device therapy information.

Refer to the MRI Guidelines for Medtronic Deep Brain Stimulation Systems instructions for use manual for the MRI conditions and MRI-specific contraindication, warnings, and precautions for conducting an MRI scan.


Refer to the System Eligibility Battery Longevity reference manual for neurostimulator selection and battery longevity calculations.

! USA Refer to the clinical summary booklet for information on the clinical study results of the neurostimulation system, individualization of treatment, adverse events summary, and use in specific populations.

Description


The Medtronic Activa SC Model 37602 Neurostimulator is part of a neurostimulation system for deep brain stimulation.

Package contents

- Neurostimulator
- Torque wrench
- Product literature
-  Warranty card
- Registration form
- Patient identification card

Patient identification card

A patient identification card is packaged with this device. Advise the patient to carry the identification card at all times.

 The patient identification card packaged with the device is temporary; a permanent card will be mailed to the patient when Medtronic receives the registration form.

The implant registration form registers the device warranties and creates a record of the device in Medtronic's implant data system.

Device specifications

The neurostimulator is a multi-program device that delivers stimulation through one lead. The stimulation settings are stored in programs. A program is a specific combination of pulse width, rate, and amplitude settings acting on a specific electrode combination. Up to two programs can be combined into a group. When using more than one program, the pulses are delivered sequentially—first a pulse from one program, then a pulse from the next program.

Pulse width, amplitude, and electrode polarity for each program within the group can have different values. Rate, rate limits, SoftStart/Stop and Cycling for each program within the group have the same values.

Table 1. Operating values for the Activa SC Model 37602 neurostimulator

Programmable parameter	Operating range and resolution^a
Number of defined groups	1 to 4
Number of programs per group	1 to 2
Electrode configuration ^b	1 to 4 electrodes per lead as anode (+), cathode (-), or Off; case defined as anode or Off
Amplitude (voltage mode)	0 to 10.5 V with 0.05-V or 0.1-V resolution
Amplitude (current mode)	0 to 25.5 mA with 0.1-mA resolution
Amplitude – upper patient limit	Tracking limit (by hemisphere): +0 to +2 (0.2 resolution); +2 to +4.5 (0.5 resolution)
Amplitude – lower patient limit	Tracking limit (by hemisphere): -0 to -2 (0.2 resolution); -2 to -4.0 (0.5 resolution); full range ^c
Pulse width	60 to 450 μ s (10- μ s resolution)
Pulse width – upper patient limit	Tracking limit: +0 to +100 μ s (10- μ s resolution)
Pulse width – lower patient limit	Tracking limit: -0 to -100 μ s (10- μ s resolution)
Rate (voltage mode)	2 to 250 Hz (resolution: 1 Hz from 2 Hz to 10 Hz, 5 Hz from 10 Hz to 250 Hz) ^d
Rate (current mode)	30 to 250 Hz (5-Hz resolution) ^d
Rate – upper patient limit	Tracking limit: +0 to +50 Hz (10-Hz resolution)
Rate – lower patient limit	Tracking limit: -0 to -50 Hz (10-Hz resolution)
SoftStart/Stop	Off, On: 1-, 2-, 4-, or 8-second ramp duration
Cycling	Off, On: 0.1 s to 24 hr (resolution: 0.1 s from 0.1 s to 1 s, 1 s from 1 s to 59 s, 1 min from 1 min to 59 min, 1 hr from 1 hr to 24 hr)

^a Interlocks will prevent the use of some parameter combinations.

^b In current mode, a maximum of 2 electrodes (including the case) can be configured: one as anode (+) and one as cathode (-).

^c Full range = -10.5 V (voltage mode); -25.5 mA (current mode).

^d Rate limited to 125 Hz when two programs are active on a single lead.

Table 2. Physical characteristics of the Activa SC Model 37602 neurostimulator^a

Description	Value
Connector type	Quadrapolar, two bore ^b
Height	55 mm (2.2 in)
Length	60 mm (2.4 in)
Thickness	11 mm (0.4 in)
Weight	45 g (1.6 oz)
Volume	28 cm ³
Power source	4.5 Amp hours, 3.2 V HCSVO ^c cell
Temperature limitation	-18 °C to +52 °C (0 °F to +126 °F)
Serial number model designator ^d	NLA
Radiopaque identification (ID) code	NLA
Transmitter	
Carrier frequency	175 kHz
Output level (at 300 m)	-48.7 dBuV/m

^a All measurements are approximate.

^b Compatible with two-pronged extension.

^c Hybrid combined silver vanadium oxide.

^d The serial number is the model designator followed by a number. The clinician programmer displays the entire serial number beginning with the model designator.

Table 3. Material of components in the Activa SC Model 37602 package

Components	Material	Material contacts human tissue
Neurostimulator		
Case	Titanium	Yes
Connector block	Polyurethane, silicone rubber, silicone medical adhesive	Yes
Grommets, seals	Silicone rubber	Yes
Setscrews	Titanium alloy	Yes
Adhesive	Silicone medical adhesive	Yes
Torque wrench		
Handle	Polyetherimide	Yes
Shaft	Stainless steel	Yes

Declaration of conformity

Medtronic declares that this product is in conformity with the essential requirements of Directive 90/385/EEC on Active Implantable Medical Devices.

For additional information, contact the appropriate Medtronic representative listed on the inside back cover of this manual.

Instructions for use

Implanting physicians should be experienced in stereotactic and functional neurosurgery and deep brain stimulation procedures, as well as thoroughly familiar with all product labeling.



Cautions:

- When using sharp instruments near the neurostimulator, be extremely careful to avoid nicking or damaging the case or the connector block. Damaging the neurostimulator may require surgical replacement.
- Do not use saline or other ionic fluids at connections, which could result in a short circuit.

Verifying neurostimulator operation

Before opening the sterile neurostimulator package, verify that the neurostimulator is operable by using the clinician programmer to interrogate the neurostimulator and read the neurostimulator battery service life. (Refer to the software manual for instructions on how to read the battery service life.)



Caution: Do not implant a neurostimulator if it was dropped onto a hard surface from a height of 30 cm (12 in) or more, because the neurostimulator may be damaged and fail to operate properly.

Note: The neurostimulator pocket may be flushed with an antibiotic solution; do not submerge the neurostimulator in fluid.

Connecting the extension to the neurostimulator



Caution: Before connecting components, wipe off any body fluids and dry all connections. Fluids in the connection may result in stimulation at the connection site, intermittent stimulation, or loss of stimulation.

1. Wipe the extension connector pins with sterile gauze. If necessary, use sterile (United States Pharmacopeia [USP]) water or a nonionic antibiotic solution.
2. Make sure the connector block receptacles are dry and clean.
3. Insert the appropriate extension connector pins into the appropriate neurostimulator socket until they are seated fully within the connector block (Figure 1). If resistance is felt while inserting the connector pins, use the torque wrench (packaged with the neurostimulator) to retract the setscrews.

Note: To retract the setscrews, insert the torque wrench into the self-sealing grommet and rotate the setscrews counterclockwise; however, do not remove the setscrews from the connector block.

**Cautions:**

- Do not insert the extension connector into the connector block if the setscrews are not sufficiently retracted. If the setscrews are not retracted, the extension connector pins may damage the setscrews and the extension connector pins will not be seated fully into the connector block.
- Limit counter-clockwise rotations of the neurostimulator setscrews when retracting them. Too many counter-clockwise rotations may disengage the setscrew from the connector block.

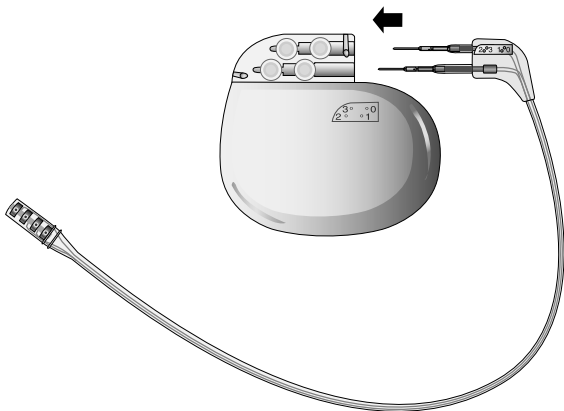


Figure 1. Insert the extension connector pins fully into the neurostimulator.

4. Fully insert the torque wrench into each self-sealing grommet of the connector block and tighten each setscrew (Figure 2).

Note: The torque wrench must be oriented to the same angle as the setscrew (Figure 2).



Cautions:

- Be sure the torque wrench is fully inserted into the self-sealing grommet. If the torque wrench is not fully inserted, the setscrew may be damaged, resulting in intermittent or loss of stimulation.
- Before tightening the setscrews, ensure that the extension connector pins are inserted into the connector block to prevent damaging the connector block.
- Verify that each leaf of the self-sealing grommet is closed after the torque wrench is withdrawn. If fluid leaks through a grommet seal that is not fully closed, the patient may experience shocking, burning, or irritation at the neurostimulator implant location, or intermittent stimulation or loss of stimulation may occur.




Figure 2. Tightening the setscrews in the self-sealing grommet.

Implanting the neurostimulator

1. Place the neurostimulator into the subcutaneous pocket with the Medtronic logo facing outward, away from muscle tissue, and ensure that the extension is not bent sharply.



Cautions:

- Ensure that the neurostimulator is placed no deeper than 4 cm (1.5 in) below the skin and is parallel to the skin. If the neurostimulator is too deep or is not parallel to the skin, telemetry may be unsuccessful.
- Do not coil excess extension in front of the neurostimulator. Wrap excess extension around the perimeter (Figure 3) of the neurostimulator to minimize subcutaneous pocket depth, help minimize potential damage during neurostimulator replacement surgery, help minimize potential kinking of the extension, and minimize interference with telemetry. Excess extension should not exceed two wraps around the perimeter of the neurostimulator.

Extension lengths requiring more than two wraps can interfere with telemetry.

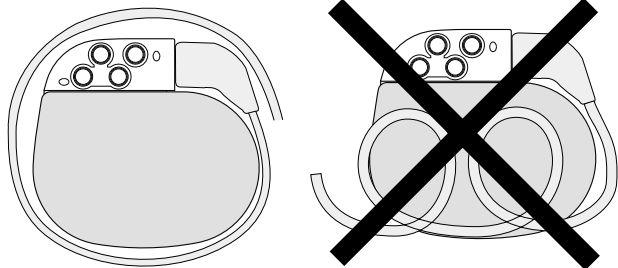


Figure 3. Wrap excess extension around the perimeter of the neurostimulator.

2. Use the suture holes in the connector block to secure the neurostimulator to the muscle fascia with nonabsorbable silk.

Checking system integrity

Caution: To use the nonsterile clinician programmer in a sterile field, place a sterile barrier between the patient and the programming head to prevent infection. Do not sterilize any part of the clinician programmer. Sterilization may damage the programmer.

Note: The neurostimulator should be in the pocket during system interrogation for integrity to ensure proper readings.

1. To ensure proper connection of the extension to the neurostimulator, use the clinician programmer to program the lead configuration and basic stimulation parameters, check the battery status, and check the electrode impedances to rule out a short or open circuit.
2. If the system integrity test results are not acceptable, refer to "Connecting the extension to the neurostimulator" on page 13.

Completing the implant procedure

1. Close and dress all incisions.
2. Ensure that a patient control device is given to the patient.
3. Complete the device tracking and patient registration paperwork and return the documents to Medtronic.

Contacts:**Asia:**

Medtronic International Ltd.
Tel. 02919-1300
Fax 02891-6830

Medtronic Asia Ltd.

Tel. (02)-548-1148
Fax (02)-518-4786

Australia:

Medtronic Australasia Pty. Ltd.
97 Waterloo Road
North Ryde, NSW 2113
Australia
Tel. +61-2-9857-9000
Fax +61-2-9878-5100
Toll-free 1-800-668-670

Austria:

Medtronic Österreich GmbH
Tel. 01-240440
Fax 01-24044-100

Belgium:

Medtronic Belgium S.A.
Tel. 02-456-0900
Fax 02-460-2667

Canada:

Medtronic of Canada Ltd.
Tel. (1-905)-460-3800
Fax (1905)-826-6620

Czech Republic:

Medtronic Czechia s.r.o.
Tel. 2-965-795-80
Fax 2-965-795-89

Denmark:

Medtronic Danmark A/S
Tel. 45-32-48-18-00
Fax 45-32-48-18-01

Finland:

Medtronic Finland Oy/LTD
Tel. (09)-755-2500
Fax (09)-755-25018

France:

Medtronic France S.A.S.
Tel. 01-5538-1700
Fax 01-5538-1800

Germany:

Medtronic GmbH
Tel. (02159)-81490
Fax (02159)-8149100

Greece:

Medtronic Hellas S.A.
Tel. 210-67-79-099
Fax 210-67-79-399

Hungary:

Medtronic Hungária Kft.
Tel. 1-889-06-00
Fax 1-889-06-99

Ireland:

Medtronic Ireland Ltd.
Tel. (01)-890-6522
Fax (01)-890-7220

Italy:

Medtronic Italia SpA
Tel. 02-241371
Fax 02-241381
Tel. 06-328141
Fax 06-3215812

Japan:

Medtronic Japan
Tel. 03-6776-0017
Fax 03-6774-4645

Latin America:

Medtronic, Inc.
Tel. (1305)-500-9328
Fax (1786)-709-4244

Norway:

Medtronic Norge AS
Tel. 67-10-32-00
Fax 67-10-32-10

Poland:

Medtronic Poland Sp. z.o.o.
Tel. (022)-465-69-00
Fax (022)-465-69-17

Portugal:

Medtronic Portugal, Lda.
Tel. 21-724-5100
Fax 21-724-5199

Russia:

Medtronic Russia
Tel. (8495) 580-7377
Fax (8495) 580-7378

Slovakia:

Medtronic Slovakia, o.z.
Tel. 0268 206 911
Fax 0268 206 999

Spain:

Medtronic Ibérica, S.A.
Tel. 91-625-0400
Fax 91-650-7410

Sweden:

Medtronic AB
Tel. 08-568-585-00
Fax 08-568-585-01

Switzerland:

Medtronic (Schweiz) AG

Tel. 031-868-0100

Fax 031-868-0199

The Netherlands:

Medtronic B.V.

Tel. (045)-566-8000

Fax (045)-566-8668

Turkey:

Medtronic Turkey

Tel. +90 216 636 1000

Fax +90 216 636 1008

U.K.:

Medtronic U.K. Ltd.

Tel. 01923-212213

Fax 01923-241004

USA:

Medtronic, Inc.

Tel. (1-763)-505-5000

Fax (1-763)-505-1000

Toll-free: (1-800)-328-0810



Medtronic

Manufacturer

Medtronic, Inc.
710 Medtronic Parkway,
Minneapolis, MN 55432-5604,
USA
www.medtronic.com
Tel. +1-763-505-5000
Fax +1-763-505-1000

Authorized Representative in the European Community



Medtronic B.V.
Earl Bakkenstraat 10,
6422 PJ Heerlen,
The Netherlands
Tel. +31-45-566-8000
Fax +31-45-566-8668

Europe/Africa/Middle East Headquarters

Medtronic International Trading Sàrl
Route du Molliau 31,
Case Postale 84
CH - 1131 Tolothenaz,
Switzerland
www.medtronic.eu
Tel. +41-21-802-7000
Fax +41-21-802-7900

Asia-Pacific

Medtronic International Ltd.
Suite 1106-11, 11/F, Tower 1, The Gateway,
25 Canton Road, Tsimshatsui,
Kowloon,
Hong Kong
Tel. +852-2919-1300
Fax +852-2891-6830

Contacts for specific countries are listed inside this cover.



* M 9 3 9 2 3 8 A 0 3 8 *

© Medtronic, Inc. 2016
All Rights Reserved

M939238A038 Rev A