Medtronic		Neurological Medtronic Confidential Title Model 37751 INSR patient manual	
Medtronic Confidential This Document is the Property of Medtronic, Inc. and must be accounted for. Information hereon is confidential. DO NOT reproduce it, reveal it to unauthorized persons or send it outside Medtronic without proper authorization.		Writer Theresa King-Hunter	Date 24 August 2004
Part No.	Part No. Rev	Comments	
A08366001	Α	Global market release	

DO NOT PRINT THIS FORM WHEN PRINTING THE LITERATURE PIECE.

DO NOT COUNT THIS FORM IN THE LITERATURE PIECE PAGE COUNT.

REVISION HISTORY: SEE PDM WEBSITE FOR INFORMATION.

1. Materials:

Covers

• Grade #1, 80 lb. white gloss coated cover stock, minimum brightness level: 89

Tex

60 lb. white smooth opaque text stock

Labels

- N/A
- 2. Colors: To confirm all colors, graphics and text, refer to electronic file

Front Cover

4-color cover and solid gloss varnish

Back Cover

Black text and graphics; solid gloss varnish

Body

 2-color text and graphics (PMS 301, black, percentages of PMS 301 or percentages of black)

Labels

- N/A
- 3. Size: $4.6'' \pm 0.2$ (w) x $6.0'' \pm 0.2$ (h)
- 4. Type of Binding: Clear plastic coil, MWE lay-flat, or perfect bound
- 5. Other:
 - · Cover and text whiteness must match visually.
- 6. Literature Piece Page Count (Including covers, excluding this form): 86
- 7. Note to print supplier: Supplier may add up to three blank pages at the end of the document before the back cover sheet as needed. If more are required, contact the purchasing agent.
- 8. Vendor-supplied information *may appear* at an appropriate location on the literature piece (eg, part number, bar code, etc.).
- 9. Graphics Content and Layout to be as shown and per Medtronic electronic file that is supplied (stored) by Medtronic Neuro.



RECHARGER Charging System user manual

37751



IUSA Rx Only



Medtronic $^{\otimes}$, Restore $^{\text{M}}$, and SoftStart $^{\text{M}}$ are trademarks of Medtronic, Inc.

IUSA FCC Information

The following is communications regulation information on the Model 37751 Patient Programmer.

FCC ID: LF537751

This device complies with part 15 Rules. Operation is subject to the following two conditions: (1) this device may not cause harmful interference and (2) this device must accept any interference received, including interference that may cause undesired operation.

IMPORTANT: Changes or modifications to this product not authorized by Medtronic, Inc., could void the FCC Certification and negate your authority to operate this product.

NeuroPatntR00

Contents

Label symbols

Introduction 1

Purpose of the device 10

Warnings 10

Precautions 11

How to use this manual

Parts of your charging system

How your charging system works

Recharger keys and screens

Recharger keys 19

Recharger screens 21

Using your charging system 25

Battery and charging information 26

Recharger and Neurostimulator

Recharger 27

Neurostimulator

Neurostimulator battery status

Charging your neurostimulator battery

Turning the neu	rostimulator ON and OFF
while charging	39
Accessories 4	.1

Accessories 41

Using the recharger pouch 41
Using the charging system carrying case 41

Identification label 41

3 Troubleshooting 43

Recharger screens 44
Warning screens 44
Information screens 49
Possible problems and solutions 56

User assistance 63

4 Maintenance 65

Recharger maintenance tasks 66
Checking the recharger battery 67
Charging your recharger battery 69
Cleaning and care 72
Safety and technical checks 73
Battery and device disposal 75

Declaration of conformity 75

Contents

4

English 37751 03/2005

Specifications 76

Glossary 78

Index 80

Printing instructions:

Label symbols

Explanation of symbols on products and packaging. Refer to the appropriate product to see symbols that apply.



CE 0123

Conformité Européenne (European Conformity). This symbol means that the device fully complies with AIMD Directive 90/385/EEC (NB 0123) and R&TTE Directive 1999/5/EC.



The use of this device might be subject to individual country licensing regimes in Europe.



Caution: consult accompanying documents



Serial number



Storage temperature



Relative humidity

-abel symbols

6

English

37751

03/2005



Atmospheric pressure



IEC 60601-1/EN60601-1, Type BF equipment



Non-ionizing electromagnetic radiation



Class II equipment



System meets the applicable Canadian [C22.2-601.1-M90 (R2001)] and US (UL 60601-1:2003) electrical safety standard requirements.



For USA audiences only

Printing instructions:

8

English 37751 03/2005

A08366001 Rev X



Purpose of the device

The Medtronic Model 37751
Charging System is designed to charge the Medtronic
Model 37711 Restore
Neurostimulator. The Restore
Neurostimulation System is intended to provide electrical stimulation to relieve severe, intractable pain. Restore
Neurostimulation System indications, contraindications, risks and benefits, warnings, precautions, and individualization of treatment information is located in the Model 37742 Patient Programmer: Pain Therapy User Manual.

Warnings

 DO NOT use the recharger on an unhealed wound. The recharger, antenna, and belt are not sterile, and contact with the wound can cause an infection.

English 37751 03/2005

A08366001

Do not use the AC power supply near water or during a lightning storm. Electric shock, serious injury, or death may result.

Precautions

- Charge the neurostimulator when you see a low battery (\Box) screen on the patient programmer or recharger; this prevents the battery from overdischarging (see glossary). If the neurostimulator battery is allowed to overdischarge, charging is not possible; however, the clinician may be able to restore the battery function. Allowing the neurostimulator battery to overdischarge will permanently affect the neurostimulator in one of the following ways:
 - Battery function is restored; however, charging sessions may be more frequent because battery capacity has been reduced.
 - Battery function is not restored, and the neurostimulator must be surgically

Printing instructions:

12

replaced. Battery function is not restored because:

- The neurostimulator battery is permanently damaged.
- The neurostimulator battery has been overdischarged and restored twice before. The third time the battery is overdischarged, the neurostimulator will reach end of service. Surgery is required to replace the neurostimulator.
- Do not expose the recharger or antenna to extremely hot [eg, hot cars, saunas, or direct sunlight; +40°C (104°F)] or cold [eg, walk-in freezers; -20°C (-4°F)] environments. The recharger and antenna are sensitive to temperature extremes and can become damaged.
- Use only the Medtronic neurological charging system components to charge your recharger. Use of non-Medtronic

Introduction 1

- charging equipment to charge the recharger can damage your charging system components.
- When operating a charging system, use special care near flammable or explosive atmospheres. An interaction between the flammable or explosive atmospheres and the battery in the device could occur. The consequences of using a batterypowered device near flammable or explosive atmospheres are unknown.

How to use this manual

This manual is designed to help you understand your charging system. Ask your clinician to explain anything that is unclear.

- Chapter 1, "Introduction," describes the recharger keys and screens and how the system works.
- Chapter 2, "Using your charging system," describes the recharger and how to perform specific tasks.

ntroduction 1

- Chapter 3, "Troubleshooting," describes recharger warning and information screens, how to solve possible charging system problems, and who to contact if your recharger is lost or broken.
- Chapter 4, "Maintenance," describes how to care for your recharger and contains system specifications and battery information.
- A glossary is provided at the end of this manual.

Parts of your charging system

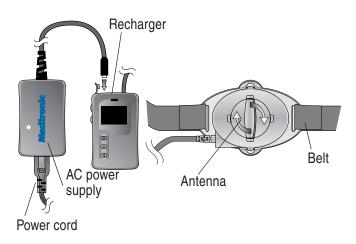


Figure 1.1 Parts of your charging system.

Recharger: The recharger is a hand-held device for charging the battery in your neurostimulator. It can also turn your neurostimulator ON or OFF. The display on the recharger provides information on your charging system.

AC power supply and power cord: This device is used to charge the recharger using AC power. If you need to charge your

37751 03/2005 English

neurostimulator but your recharger battery is low, connect your recharger to the AC power supply to conduct a charging session. The power cord plugs into an electrical outlet and connects the AC power supply to the recharger. The power supply is a universal component.

Note: Use only the power supply provided by Medtronic with your charging system.

Antenna: The antenna connects to the recharger to establish communication with your neurostimulator. You can adjust a dial on the antenna to improve the charging efficiency between the recharger and the neurostimulator.

Belt: The belt allows you to keep the antenna directly over your neurostimulator during a charging session.

Pouch: The recharger fits into a pouch that can be attached to the belt so you can maintain your normal activities during a charging session.

English 37751 03/2005

System carrying case: The carrying case is used to store the recharger, the charging system components, and your patient programmer.

How your charging system works

The charging system is used to charge your implanted neurostimulator battery. The battery in your recharger is similar to the rechargeable batteries commonly found in electronic devices. The battery typically lasts for approximately 5 years, depending upon your therapy needs and how often you use your recharger.

Rechargeable batteries lose some of their power every day, even when not used. Charging sessions restore power to the recharger battery.

 Charge the neurostimulator when you see a low battery (\Box) screen on the patient programmer or recharger; this prevents

Printing instructions:

the battery from overdischarging (see glossary). If the neurostimulator battery is allowed to overdischarge, charging is not possible; however, the clinician may be able to restore the battery function. Allowing the neurostimulator battery to overdischarge will permanently affect the neurostimulator in one of the following ways:

- Battery function is restored; however, charging sessions may be more frequent because battery capacity has been reduced.
- Battery function is not restored, and the neurostimulator must be surgically replaced. Battery function is not restored because:
 - The neurostimulator battery is permanently damaged.
 - The neurostimulator battery has been overdischarged and restored twice before. The third time the battery is overdischarged, the

18

English 37751 03/2005

neurostimulator will reach end of service. Surgery is required to replace the neurostimulator.

Recharger keys and screens

Recharger keys

Five keys on the recharger allow you to control the recharger and turn your neurostimulator ON and OFF.



Figure 1.2 Recharger keys.

- NEUROSTIMULATOR ON (2): Turns your neurostimulator ON.
- NEUROSTIMULATOR OFF : Turns your neurostimulator OFF.
- START CHARGE/TEST : Begins charging the neurostimulator.
- **STOP CHARGE** Ends or interrupts charging the neurostimulator.
- AUDIO CONTROL : Turns your recharger ON.

Note: When your recharger is ON, pressing the AUDIO CONTROL key turns audible status tones ON and OFF. The AUDIO CONTROL key is also used to display the recharger battery status.

Recharger screens

Figure 1.3 shows the recharger screens.

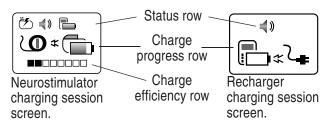


Figure 1.3 Recharger screens.

The screens are separated into either two or three rows of icons.

Status row – Displays icon information for the recharger or neurostimulator.

During a neurostimulator charging session, on the status row you will see:

- Neurostimulator is ON (♠) or OFF (♠)
- Audio (sound) is ON (\triangleleft) or OFF ($\not\triangleleft$)
- Battery charge status of the recharger (needs recharging to full, respectively)

22

 The recharger is plugged into the AC power supply (--). If the recharger is not plugged into a power supply, this area of the screen will be blank.

During a recharger charging session, the status row displays:

Audio (sound) is ON (◄») or OFF (◄)

Charge progress row – Indicates the progress of the charging session.

During a neurostimulator charging session, you will see:

 Current charge status of the neurostimulator battery. A flashing battery icon (

indicates the neurostimulator is charging. When charging is complete, the NEUROSTIMULATOR CHARGING COMPLETE screen will display. During a recharger charging session, you will see:


- Current charge status of the recharger battery. A flashing battery icon () indicates the recharger is charging. When charging is complete, the RECHARGER CHARGING COMPLETE screen will display.
- The connection icon (), indicating that the power supply is connected to an operational electrical outlet.

Charge efficiency row – Displays a series of boxes indicating the efficiency of the charging signal between the neurostimulator and recharger. More solid black boxes (a maximum of eight) indicate a more efficient charging signal and a shorter charging session (**EXECUTE**). The least efficient charge is indicated by empty boxes (■■□□□□□□). If you see six empty boxes, adjust the antenna to continue charging.

Introduction 1

24

English 37751 03/2005

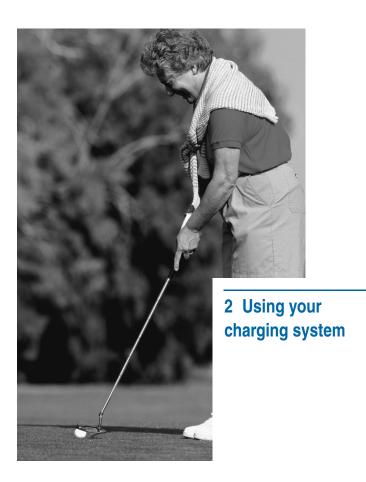

This chapter includes information on:

- the recharger battery and the charging procedure.
- neurostimulator battery status icons.
- charging your neurostimulator.
- how to turn your neurostimulator ON or OFF during a charging session.
- the charging system accessories.

Battery and charging information Recharger and Neurostimulator

Charge the recharger or neurostimulator even if you are not using them for an extended period of time.



NeuroPatntR03

26

English 37751 03/2005

- You can charge the neurostimulator and recharger at the same time. Follow the instructions for both procedures ("Charging your neurostimulator battery" on page 32 and "Charging your recharger battery" on page 69) at the same time.
- Ensure you charge the batteries in your recharger and neurostimulator before they are low.

Recharger

- As your recharger ages, you will need to charge the battery more often.
- The recharger battery might have run low since it was manufactured and shipped. You might need to charge it before you use it the first time.

Using your charging system

Neurostimulator

- Your ability to locate your neurostimulator and the depth of the neurostimulator determine the efficiency of the charging session. With practice, you will find the best location on your skin for placing your recharger and antenna.
- If your neurostimulator is on while you are charging the battery, your charging session might last longer.
- Depending on your therapy needs, charging your neurostimulator could take from one hour to more than 12 hours per week.
- You can partially charge your neurostimulator if you do not have enough time for a complete charging session.
- You can charge your neurostimulator at any time; you do not have to wait for a low battery message.

English 37751 03/2005

Neurostimulator battery status

Use your patient programmer to check your neurostimulator battery charge level every day. Refer to the manual supplied with the patient programmer.

If either message in Table 2.1 is displayed, you must recharge the neurostimulator battery.

Table 2.1 When to charge the neurostimulator.


When you see this The neurostimulator battery charge level is low, and soon your therapy will not be available. Charge the neurostimulator battery. Press the gray AUDIO key on the recharger

to clear the message.

Table 2.1 When to charge the neurostimulator. (continued)

When you see this

It means



The neurostimulator battery charge level is low. Stimulation has stopped.

Charge the neurostimulator battery now. Press the green Start charge/test key to clear the screen.

Caution: Charge the neurostimulator when you see a low battery () screen on the patient programmer or recharger; this prevents the battery from overdischarging (see glossary). If the neurostimulator battery is allowed to overdischarge, charging is not possible; however, the clinician may be able to restore the battery function.

Allowing the neurostimulator battery to overdischarge will permanently affect the neurostimulator in one of the following ways:

- Battery function is restored; however, charging sessions may be more frequent because battery capacity has been reduced.
- Battery function is not restored, and the neurostimulator must be surgically replaced.
 Battery function is not restored because:

English 37751 03/2005

Table 2.1 When to charge the neurostimulator. (continued)

When you see this It means

The neurostimulator battery is permanently damaged.

The neurostimulator battery has been overdischarged and restored twice before. The third time the battery is overdischarged, the neurostimulator will reach end of service. Surgery is required to replace the neurostimulator.

Charging your neurostimulator battery

Check with your clinician prior to using your recharger for the first time. When your neurostimulator needs to be charged, follow the steps below.

Notes:

- You might need to charge the recharger battery before you charge your neurostimulator battery. Refer to "Recharger maintenance tasks" on page 66.
- Based on the configuration of your implanted neurostimulator, you might need to use more than one template (Figure 2.1) to ensure the antenna remains positioned correctly over your neurostimulator.
- Press your bare skin where your neurostimulator is located to determine the best place for the belt and antenna.

English 37751 03/2005

Notes:

- Do not place the antenna or belt over bulky clothing or bandages.
- The antenna may be placed directly on your skin. However, if the antenna irritates your skin, you might want to wear a thin undergarment to protect your skin.
- Put on your belt, with the template centered over your neurostimulator (Figure 2.1) and secure the belt.
 Reposition your template, if necessary.




Figure 2.1 Place the belt over your neurostimulator.

3. Place the antenna in the template, and press it into the belt until it snaps into the openings on the template (Figure 2.2).

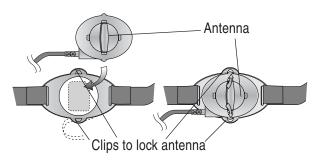


Figure 2.2 Attach the antenna to the belt.

4. Press the green START CHARGE/TEST
key. The recharger wait screen will appear on the recharger display
(Figure 2.3). The RECHARGER WAIT
screen indicates that the neurostimulator
and recharger are trying to communicate.




Figure 2.3 RECHARGER WAIT screen.

When charging begins, the recharger displays a new screen indicating the

English 37751 03/2005

neurostimulator battery charge level and efficiency of the charging session (Figure 2.4).




Figure 2.4 Neurostimulator battery charge level and charging efficiency.

The battery charge level updates throughout the charging session. Charging sessions can take a few minutes to more than 12 hours. depending on the charging efficiency, how often you charge, and your therapy needs.

Notes:

- If you need to interrupt your charging session, press the **STOP CHARGE** (XXX) key.
- You might hear periodic clicking noises during recharging, and you might see the screen refresh.

Using your charging system

5. If the recharger screen shows a less efficient session, use the dial on the antenna to try to make the session more efficient. Turn the dial on the antenna one quarter turn in either direction (Figure 2.5). Press the green START CHARGE/TEST key. The recharger will display an updated efficiency status.

Note: The efficiency status screen will not be updated unless the START CHARGE/TEST key is pressed.

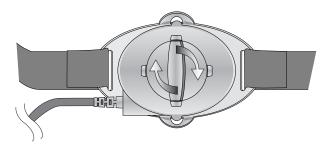


Figure 2.5 Adjusting the antenna dial.

Note: Repeat step 5 until the recharger screen indicates a more efficient charging session. Charging efficiency is affected by factors such as implant depth, and

English 37751 03/2005

- efficiency will vary between patients. You and your clinician can work together to identify the best efficiency for you.
- 6. Periodically check the progress of the charging session by reviewing the icons on your recharger screen. If you see 6 empty boxes (■■□□□□□□) adjust the antenna to continue charging.
- 7. When your neurostimulator has a charge sufficient for use, you will see the following screen:




Figure 2.6 NEUROSTIMULATOR CHARGE SUFFICIENT FOR USE screen.

8. You can press the STOP CHARGE key to quit your charging session, if desired. You will hear three tones if the audio is ON. If you wait for the system to fully charge your neurostimulator, the

37751 03/2005 English

NEUROSTIMULATOR CHARGING COMPLETE screen will be displayed on the recharger display, and you will hear one tone, if the audio is ON (Figure 2.7).




Figure 2.7 NEUROSTIMULATOR CHARGING COMPLETE screen.

Carefully expand the clips to unlock the antenna and remove it from the belt (Figure 2.8).




Figure 2.8 Removing the antenna.

10. Remove the belt and store the belt, antenna, and recharger in the charging system carrying case.

English 37751 03/2005

Using your charging system 2

Turning the neurostimulator ON and OFF while charging

You can turn your neurostimulator ON or OFF during a charging session.

To turn the neurostimulator ON while charging:

- 1. Press the Neurostimulator on (5) key.
- **2.** If audio is enabled, listen for the confirmation tone.
- **3.** Verify that the NEUROSTIMULATOR ON icon (♠) is displayed on the recharger screen.

To turn the neurostimulator OFF while charging:

- Press the NEUROSTIMULATOR OFF (5) key.
- **2.** If audio is enabled, listen for the confirmation tone.
- Verify that the NEUROSTIMULATOR OFF icon () is displayed on the recharger screen.

Note: If you want to adjust stimulation using your patient programmer before your neurostimulator is completely charged, press the STOP CHARGE (XXX) key on the recharger. You might need to remove the antenna so your patient programmer can communicate with your neurostimulator. Adjust stimulation with your patient programmer. Resume the charging session by pressing the START CHARGE/TEST (A) key.

English 37751 03/2005

Accessories

Using the recharger pouch

The recharger comes with a small pouch that you can wear on a belt during a charging session. Using this allows you to remain active during a charging session.


Using the charging system carrying case

The recharger comes with a carrying case to store the recharger and accessories. Using the case keeps the components clean and free from damage.

Identification label

Place an identification label on the back of your recharger in case the recharger is lost. Jsing your charging system

42

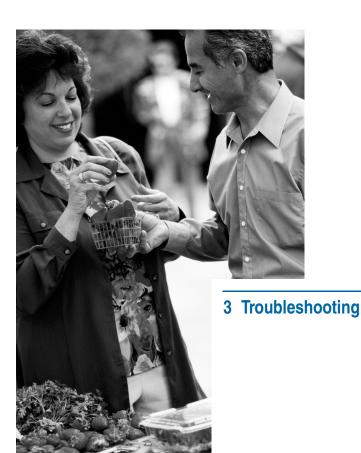

This section will help you solve problems with your charging system. It also provides information on when to call your clinician or Medtronic.

Note: If you cannot solve a problem, or if a problem is not described here, contact your clinician.



Recharger screens

The recharger displays warning (\bigwedge) and information (\bigcirc) screens to provide you with information about your system, alert you to a problem with your system, or to guide you during recharger use.

Warning screens

Warning screens (\(\bullet \)) indicate a problem with the recharger, the antenna, or the neurostimulator. If the audio is ON, three tones alert you to the screen. Table 3.1

44


describes warning screens and provides instructions (see blue text) on how to resolve the problem and clear the screen.

Table 3.1 Recharger warning screens


Warning screen

Cause and action

Reposition antenna



You tried to turn your neurostimulator ON or OFF during a charging session, but the recharger did not communicate successfully with the neurostimulator.



Reposition your antenna over your neurostimulator. Try again to turn your neurostimulator ON or OFF.



The communication between your recharger and your neurostimulator was interrupted or could not be established.

Reposition your antenna over your neurostimulator, and press the green START CHARGE/TEST key.


Table 3.1 Recharger warning screens (continued)

Warning screen

Cause and action

Charge your neurostimulator battery

The neurostimulator battery charge level is low. Stimulation has stopped.



Press the green START CHARGE/TEST key to clear the screen.

Charge the neurostimulator battery now.

Caution: Charge the neurostimulator when you see a low battery () screen on the patient programmer or recharger; this prevents the battery from overdischarging (see glossary). If the neurostimulator battery is allowed to overdischarge, charging is not possible; however, the clinician may be able to restore the battery function.

Allowing the neurostimulator battery to overdischarge will permanently affect the neurostimulator in one of the following ways:

- Battery function is restored; however, charging sessions may be more frequent because battery capacity has been reduced.
- Battery function is not restored, and the neurostimulator must be surgically replaced.
 Battery function is not restored because:

46


Table 3.1 Recharger warning screens (continued)


Warning screen Cause and action

The neurostimulator battery is permanently damaged.

The neurostimulator battery has been overdischarged and restored twice before. The third time the battery is overdischarged, the neurostimulator will reach end of service. Surgery is required to replace the neurostimulator.


Charge your recharger battery





Charge your recharger with the AC power supply.

Call doctor



Your neurostimulator has reached end of service. Stimulation has stopped.

37751

Call your doctor immediately.

03/2005 English

Warning screen

Cause and action

Call clinician



Your system is not working correctly. Stimulation might have stopped.

Call your clinician and provide the specific error code shown on the recharger display.

Information screens

Information screens ((i)) provide information and instructions on how to proceed. If the audio is ON, three tones alert you to the message. Press the AUDIO key on the recharger to clear the screen. Table 3.2 describes information screens.

Table 3.2 Recharger information screens


Information **Description and action** screen Check antenna The antenna connection to the recharger is loose or your (i)antenna is not connected. Check that the antenna and recharger are making full contact. Connect or tighten the connection and retry. The antenna or recharger might require service. Call Medtronic. Refer to the addresses and phone numbers on the inside back cover of this manual.


Table 3.2 Recharger information screens (continued)

Information screen

Description and action

Move to a cooler environment; ensure your system is not too hot





Allow the antenna to cool and retry. Store the charging system components in a cool, dry place.

Your skin temperature is too warm for a successful charging session.



Move to a cool location, remove any excess clothing, allow your skin temperature to cool, and retry.

The antenna may require service.

Contact Medtronic. Refer to the addresses and phone numbers on the inside back cover of this manual.

Table 3.2 Recharger information screens (continued)

Information screen


Description and action

Note: This screen might appear during a recharging session, even if the antenna surface does not feel warm to you. Recharging will stop when this screen is displayed because the antenna is too warm for the system to work properly. Recharging will begin again once the surface temperature of the recharger antenna is within the operating range of the system.

Recharger system information



AB34; v5.1 QR26.78 The Audio Control and




Press the STOP CHARGE key to clear this message.

Table 3.2 Recharger information screens (continued)

	(continued)
Information screen	Description and action
Charge your neurostimulator battery	The neurostimulator battery charge level is low and stimulation will stop soon.
(i)	Charge your neurostimulator battery using the recharger.
Charge your recharger	The recharger battery charge level is low.
	Charge your recharger battery using the AC power supply.
Finish	The neurostimulator battery is

Finish neurostimulator charging session



The neurostimulator battery is only partially charged.

You did not completely charge the neurostimulator battery. Finish charging your neurostimulator battery using the recharger, if desired.

Table 3.2 Recharger information screens (continued)

	(continued)
Information screen	Description and action
Finish recharger charging session	The recharger battery is only partially charged.
	You did not completely charge the recharger battery. Finish charging your recharger battery using the AC power supply, if desired.
Neurostimulator charging complete	The neurostimulator battery contains sufficient charge for use.
	Press the AUDIO key to clear the message.
Recharger charging	The recharger battery is fully charged.
complete	Press the AUDIO key to clear the message.

Table 3.2 Recharger information screens (continued)

Information screen
Call clinicia

Description and action



There is a problem with a component of your system.

Call your clinician and provide the specific error code shown on the recharger display.

Call clinician



Your neurostimulator needs to be replaced, because stimulation will stop soon.

Call your clinician and provide the message shown on the recharger display.

Possible problems and solutions

The following table will help you solve problems or identify when to call your clinician. Problems are described in the left column (**bold black text**). The right column lists possible causes of the problem (plain text) and how to correct the problem (**bold blue text**).

Note: If a problem is not resolved after several attempts or if a problem is not described in the following table, contact your clinician.

Troubleshooting
3.3
Table

T _i	Table 3.3 Troubleshooting
Problems	Causes and actions
Your recharger screen does not turn on when you try to charge your neurostimulator	The recharger battery is low. Attach the AC power supply to the recharger. The recharger is broken. Contact your doctor.
You cannot turn ON your neurostimulator with the recharger	Electronic devices might be interfering with the recharger communication signal. Move away from all electronic devices (eg, TVs, computer monitors, or microwaves), and retry.

Table 3.3 Troubleshooting (continued)

	(555) 8:
Problems	Causes and actions
Your AC power supply will not turn ON (the light on	The power cord might not be plugged into the AC power supply or electrical outlet.
the supply does not turn green when you plug it in)	Connect the power cord to the electrical outlet.
	The connection to the power cord might be loose.
	Reseat the electrical cord on the AC power supply.
	The power cord connected to the AC power supply might be incompatible with the electrical outlet.
	Obtain an adapter for the type of electrical outlet you are using.

58

Table 3.3 Troubleshooting (continued)

Remove the recharger or antenna from the If the AC power supply is plugged into an electrical outlet, interrupt the flow of electricity to the outlet. Unplug the power Causes and actions supply. water. Si Your recharger or antenna falls into water **Problems**

If the recharger or antenna is dirty, wipe it with a towel dampened with clean water.
 Shake the recharger or antenna.
 If you see or hear water inside, wipe it dry with a clean towel. Repeat steps 4 and 5.

When the recharger or antenna is dry, try to

use it.

9

(continued)
Troubleshooting
Table 3.3

IdDie	lable 3.3 Houbleshooming (confinited)
Problems	Causes and actions
Your AC power supply falls into water	1. Turn off the power, preferably at the breaker fuse box, if the AC power cord is plugged into an electrical outlet. Unplug the power supply.
	2. Remove the AC power supply from water.
	3. If it is dirty, wipe it with a towel dampened with clean water.

hear water inside, repeat steps 4 and 5 until electrical outlet. A green light on the top of Shake the AC power supply. If you see or the power supply will come on if it is Plug the power cord into a GROUNDED he power supply is thoroughly dry. working properly. S. 9

Leave the AC power supply on a dry towel

ior a few hours.

4

Troubleshooting 3

Table 3.3 Troubleshooting (continued)

lable 3	lable 3.3 Iroubleshooting (continued)
Problems	Causes and actions
Your recharger, antenna, or AC power supply falls off a cabinet or table	The recharger, antenna, and AC power supply are designed to withstand falls of short distances. Try the recharger, antenna, or AC power supply; they should work.
Your recharger is beeping	You cannot resolve the problem or you see a screen other than those described in this section. Contact your clinician to resolve the problem.
Your recharger screen is blank	The recharger wait screen did not appear when you pressed the START CHARGE/TEST key. Connect your recharger to the AC power supply and follow the directions for charging your recharger on page 69. Note: If the Recharger charging screen does not appear after you connect the recharger to the AC power supply, contact your clinician.

62

User assistance

Your recharger has been designed and tested to provide trouble-free service. If repair or service is needed, contact your clinician or a Medtronic sales office. Refer to the list of Medtronic contacts at the end of this manual.

The serial number is located on the back of the recharger. This number identifies each recharger. If you contact Medtronic about your recharger, refer to the serial number.

If your recharger stops working – First try the steps in Table 3.3. Otherwise, contact Medtronic

If you lose your recharger – Contact your clinician to order a new recharger.

To register the recharger for service covered by the warranty, complete and mail the warranty registration.

63

PatntCh03.fm 8/23/04 8:00 am Size 4.625" x 6.0" (117 mm x 152 mm) UC200xxxxxx EN

Medtronic Confidential NeuroPatntR03

Troubleshooting 3

64

English 37751 03/2005

Rev X



Maintenance 4

This section describes how to care for and dispose of your recharger and accessories.

Recharger maintenance tasks

Maintaining the battery in your recharger ensures that you can charge your neurostimulator battery when needed. For information on charging and the batteries within the recharger, see "Battery and charging information" on page 26.



Maintenance 4

Checking the recharger battery

Press the gray AUDIO key on the recharger to turn ON your recharger and check the recharger battery charge level. The RECHARGER BATTERY CHARGE LEVEL screen displays the current battery charge level (Figure 4.1).




Figure 4.1 RECHARGER BATTERY CHARGE LEVEL screen and icons.

Charge your recharger with the AC power supply when you see either of the screens in Table 4.1.

Table 4.1 When to charge the recharger


When you see this

It means



The recharger battery charge level is low and will lose power soon. Charge the recharger battery.

Press the AUDIO key to clear the message, and charge the recharger battery.



The recharger battery lost or is about to lose power.

Charge the recharger battery immediately.

Maintenance 4

Charging your recharger battery

Follow the steps below to charge the recharger battery using the AC power supply.

1. Plug the AC power supply into your AC outlet (Figure 4.2). A green light indicates it has power.

▲ Warning: Do not use the AC power supply near water or during a lightning storm. Electric shock, serious injury, or death may result.



Figure 4.2 Plug in the AC power supply.

2. Connect the recharger to the AC power supply (Figure 4.3). The recharger will automatically start to charge when connected to the AC power supply, and

the RECHARGER CHARGING SESSION screen will be displayed. (Figure 4.4). The charging session could take several hours, depending on the charge level of the batteries.

Note: To interrupt a recharger charging session, disconnect the recharger from the AC power supply.



Figure 4.3 Connect the recharger to the AC power supply.

Figure 4.4 illustrates a RECHARGER CHARGING SESSION screen.

70




Figure 4.4 RECHARGER CHARGING SESSION screen.

3. When the charging session is complete, the recharger will show a RECHARGER CHARGING COMPLETE screen (Figure 4.5.)




Figure 4.5 RECHARGER CHARGING COMPLETE screen.

- **4.** Unplug the AC power supply from the electrical outlet.
- 5. Disconnect the AC power supply from the recharger.
- **6.** Return the recharger, power cord, and AC power supply to the system carrying case.

Cleaning and care

Follow these guidelines to ensure that the recharger system and accessories function properly:

- Keep the recharger, antenna, and AC power supply out of the reach of children.
- Use the recharger, antenna, and AC power supply only as instructed by your clinician and this manual.
- Handle the recharger, antenna, and AC power supply with care. Do not drop, strike or step on the components.
- Do not dismantle or tamper with the recharger, antenna, or AC power supply.
- Clean the outside of the recharger, antenna, and AC power supply with a damp cloth when necessary. Mild household cleaners will not damage the components.
- The recharger, antenna, and AC power supply are not waterproof. Do not allow moisture to get inside the components.

72

The belt, with the antenna removed, can be washed with a mild laundry detergent in a washing machine and dried in a dryer on a low heat setting.

Safety and technical checks

Periodic safety and technical checks or periodic maintenance of the recharger are not required.

The recharger contains no user-serviceable parts. If the recharger requires repair or is nonfunctional, send it to the appropriate address listed below.

USA

Medtronic, Inc. Neurological Division MSN600 PO Box 1250 Minneapolis, MN 55440-9087

Medtronic EOC
Medical Equipment Service Europe
Earl Bakkenstraat 10
6422 PJ Heerlen
The Netherlands
Tel. 31-455664880
Fax 31-455668028

Battery and device disposal

Dispose of worn out devices according to local regulations. Do not incinerate. If you no longer need your recharger and would like to donate it, contact your clinician.

Declaration of conformity

Medtronic declares that this product is in conformity with the essential requirements of Directive 1999/5/EC on Radio and Telecommunications Terminal Equipment and Directive 90/385/EEC on Active Implantable Medical Devices.

For additional information, contact Medtronic. Refer to the list of Medtronic contacts at the end of this manual.

Printing instructions:

Specifications

The following table lists the specifications for your recharger.

Table 4.2 Recharger specifications

Table 112 Hedharger epecineations		
Parameter	Specification	
Power source	2 non-removable lithium-ion batteries (rechargeable)	
Operating temperature	+10 to +35°C (+50 to +95°F)	
Storage temperature	-20 to +40°C (-4 to +104°F)	
Operating/storage relative humidity	30% to 95%	
Operating atmospheric pressure	700 hPa to 1060 hPa (20.7 in. Hg to 31.3 in. Hg)	
Storage atmospheric pressure	700 hPa to 1060 hPa (20.7 in. Hg to 31.3 in. Hg)	
Recharger size	Approximately 13 x 8 x 3.18 cm (5 x 3 x 1.25 inches)	
Recharger weight, including battery	Approximately 227 g (8 oz.)	

76

Table 4.2 Recharger specifications (continued)

Parameter	Specification
Battery life	5 years (life of device) ^a
Power supply voltage	100-240V voltage (auto-ranging)
Rated frequency	50/60 Hz
Input current	0.35 A
Outputs	0.85 A, 8.4 V dc (V charge) 0.5 A, 10 V dc (V base)
Mode of operation	Continuous

^a The longevity of your recharger battery is dependent upon how often you use your recharger.

Printing instructions:

Glossary

Caution – A statement describing actions that could result in damage to or improper functioning of a device.

Clinician – A health care professional such as a doctor or nurse.

Contraindication – A condition or circumstance when a person should not have a neurostimulation system.

Indication – The purpose of the neurostimulation system and the medical condition for which it may be implanted.

Neurostimulator – The power source of a neurostimulation system. It contains the battery and electronics that control the stimulation you feel.

Overdischarge – The neurostimulator battery continues to lose charge even after you see a low battery () screen. Eventually, the battery loses enough charge to permanently affect the neurostimulator. If this occurs, the battery is overdischarged.

Glossary

English 37751 03/2005

Patient programmer – A hand-held device that allows you to turn your neurostimulator ON and OFF. It is also used to adjust some of the stimulation settings.

Precaution - See "Caution".

Recharger – The component of the Restore Neurostimulation System that is used to charge your neurostimulator battery.

Stimulation – The delivery of electrical pulses to the area where pain signals are blocked. Stimulation blocks some pain signals from reaching the brain.

Template – The cut-out area in the plastic part of the charging system belt.

Warning – A statement describing an action or situation that could harm the patient.

Warning screen – A screen displayed on the recharger that alerts you to a problem with the charging system.

Index

```
AC power supply
   description 15
   troubleshooting 58, 59, 61, 62
Accessories 41
Antenna
   description 16
   troubleshooting 59, 60, 62
Antenna dial
   about 16
   adjusting 36-37
Audio control key 19, 20
Audio tones 38, 44
Battery (neurostimulator)
   See Neurostimulator battery
Battery (recharger)
   See Recharger battery
Belt 16
Care 72
Carrying case 17, 41
Charge efficiency row 23
Charge progress row 22
Charging efficiency 23, 36-37
Charging neurostimulator and recharger at same
time 27
Charging session
   neurostimulator battery 34-38
   recharger battery 70-71
```

Index

80

```
Charging system
   cleaning and care 72
   how it works 17
    parts 15-17
Charging the neurostimulator battery
   procedure 32-38
   turning neurostimulator ON and OFF while
       charging 39-40
Charging the recharger battery 69-71
Checking recharger battery 67–68
Cleaning 72
Dial (antenna)
    about 16
   adjusting 36-37
Disposing of devices 75
Identification label 41
Information screens 49-55
Interrupting
   neurostimulator battery charging session 35
   recharger battery charging session 70
Keys, recharger 19
Maintenance 66-71
Neurostimulation system 10
Neurostimulator
   charging information 26-27, 28
   turning ON and OFF while charging 39-40
    See also Neurostimulator battery
```

```
Neurostimulator battery
   battery level messages 29-30, 46
   charging 32-38
   checking status 29
   interrupting charging session 35
   See also Neurostimulator
Neurostimulator OFF key 19, 20
Neurostimulator ON key 19, 20
Patient programmer 29
Pouch 16, 41
Power cord 15
Power supply
   See AC power supply
Precautions 11-13
Recharger
   charging information 26-27
   description 15
   troubleshooting 57, 59, 60, 62
   See also Recharger battery
Recharger battery
   about 17
   charging 69-71
   checking charge level 67-68
   interrupting charging session 70
   maintaining 66-71
   See also Recharger
Recharger keys 19
```

Index

82

Recharger screens about 21-23 information screens 49-55 Neurostimulator charging session screen 21 Recharger charging session screen 21 warning screens 44-48 Recharger system See Charging system Repair address 73 Screens See Recharger screens Serial number 63 Specifications 76 Start charge/Test key 19, 20 Status row 21 Stop charge key 19, 20, 35 Template 33 Test (Start charge/Test) key 19, 20 Tones, audio 38, 44 Troubleshooting 44-62 Turning neurostimulator ON and OFF while charging 39-40 Warning screens 44-48 Warnings 10-11 Warranty registration 63

Index

84

Medtronic Confidential NeuroPatntR00

Contacts:

Asia: Medtronic International Ltd. Suite 1602 16/F, Manulife Plaza, The Lee Gardens, 33 Hysan Avenue, Causeway Bay, Hong Kong Tel. 852-2891-4068 Fax 852-2591-0313

Medtronic Asia Ltd. 3 Floor Peter Building, 570-6 Shinsa-Dong Kangnam-ku, Seoul 135-120, South Korea

Tel. 82-2-548-1148 Fax 82-2-518-4786 **Australia**: Medtronic Australasia Pty. Ltd.
Unit 4/446 Victoria Road, Gladesville NSW 2111

Tel. 02-9879-5999 Fax 02-9879-5100 **Austria**: Medtronic Österreich G.m.b.H.

Millennium Tower, Handelskai 94-96, 1200 Vienna

Belgium: Medtronic Belgium S.A. Boechoutlaan 55, 1853 Strombeek-Bever Tel. 02-456-0900 Fax 02-460-2667

Canada: Medtronic of Canada Ltd. 6733 Kitimat Road, Mississauga, Ontario L5N 1W3

Tel. 01-24044 Fax 01-24044-100

Ontario L5N 1W3
Tel. 905-826-6020 Fax 905-826-6620 **Denmark:** Medtronic-ViCare A/S

Birkerød Kongevej 150B, DK-3460 Birkerød Tel. 45-823366 Fax 45-823365

Finland: Medtronic Finland OY/LTD Sahaajankatu 24, P.O. Box 230

FIN-00810 Helsinki Tel. 9-755-2500 Fax 9-755-25018

France: Medtronic France S.A.S. 122, avenue du Général Leclerc, 92514 Boulogne-Billancourt Cedex Tel. 01-5538-1700 Fax 01-5538-1800

Germany: Medtronic GmbH Emanuel-Leutze-Straße 20, 40547 Düsseldorf, P.O. Box 110738

Tel. 0211-52930 Fax 0211-5293100

Greece: Medtronic Hellas S.A. Agias Varvaras 5, 15231 Halandri, Athens Tel. +30 2 10-677 90 99 Fax 30 2 10-677 93 99

Italy: Medtronic Italia SpA P.zza Indro Montanelli 30,20099 Sesto San Giovanni (MI). Tel. 02-241371. Fax 02-241381.

Via Lucrezio Caro, 63, 00193 Roma Tel. 06-328141 Fax 06-3215812 Japan: Medtronic Japan Solid Square West Tower 6F, 580 Horikawa-cho, Saiwai-ku, Kawasaki, Kanagawa 210-0913. Tel. 044-540-6112 Fax 044-540-6200

Latin America Headquarters: Medtronic, Inc. 710 Medtronic Parkway, Minneapolis, MN 55432-5604 USA Tel. 763-514-4000 Fax 763-514-4879

The Netherlands: Medtronic B.V. Earl Bakkenstraat 10, P.O.Box 2542, 6401 DA Heerlen Tel. 045-5668000 Fax 045-5668668

Norway: Medtronic Vingmed AS Fjordveien 1, Postboks 366, 1323 Høvik Tel. 67 58 06 80 Fax 67 10 12 12

Portugal: Medtronic Portugal, Lda. Rua Tomás da Fonseca, Torre E 8, andar A,B, 1600 - 209 Lisboa Tel.21-724-5100 Fax 21-724-5199

Spain: Medtronic Ibérica, S.A.
Centro Empresarial Miniparc III, Edificio K,
Calle Caléndula, 93, El Soto de la Moraleja,
28109 Alcobendas - Madrid
Tel. 91-625-0400 Fax 91-650-7410

Sweden: Medtronic AB Dackevägen 33, Box 265 S-177 25 Järfälla Tel. 08-5222-0000 Fax 08-5222-0050 Internet: www.medtronic.se

Switzerland: Medtronic (Schweiz) AG Route du Molliau 31 Case Postale 84 CH-1131 Tolochenaz Tel. 021-803-8000 Fax 021-803-8099

U.K. and Ireland: Medtronic U.K. Ltd. Suite 1, Sherbourne House, Croxley Business Center, Watford, Herts WD1 8YE, United Kingdom Tel. 1923-212213 Fax 1923-241004



Manufacturer

Medtronic, Inc. 710 Medtronic Parkway Minneapolis, MN 55432-5604 USA Internet: www.medtronic.com

Tel. 1-763-505-5000 Fax 1-763-505-1000

Medtronic E.C. Authorized Representative/Distributed by

Medtronic B.V. Earl Bakkenstraat 10 6422 PJ Heerlen The Netherlands Tel. 31-45-566-8000 Fax 31-45-566-8668

Europe/Africa/Middle East

Headquarters

Medtronic Europe Sàrl Route du Molliau 31 Case Postale CH-1131 Tolochenaz Switzerland Internet: www.medtronic.co.uk Tel. 41-21-802-7000 Fax 41-21-802-7900

Asia-Pacific

Medtronic International Ltd. Suite 1602 16/F, Manulife Plaza The Lee Gardens, 33 Hysan Avenue Causeway Bay Hong Kong Tel. 852-2891-4068 Fax 852-2591-0313

Contacts for specific countries are listed inside this cover.



* A O 8 3 6 6 0 0 1 *

© Medtronic, Inc. 2005 All Rights Reserved A08366001