




ACL Reconstruction System Overview

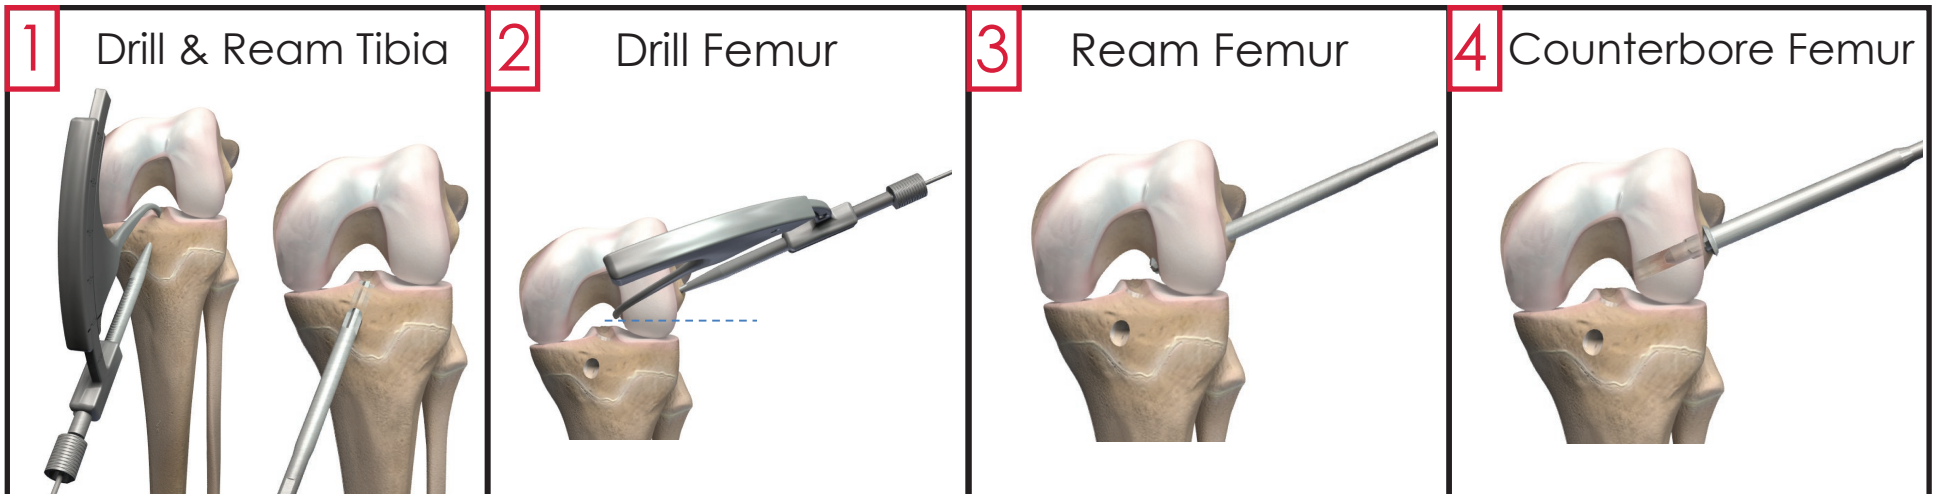

Fluoroscopy recommended for all drilling

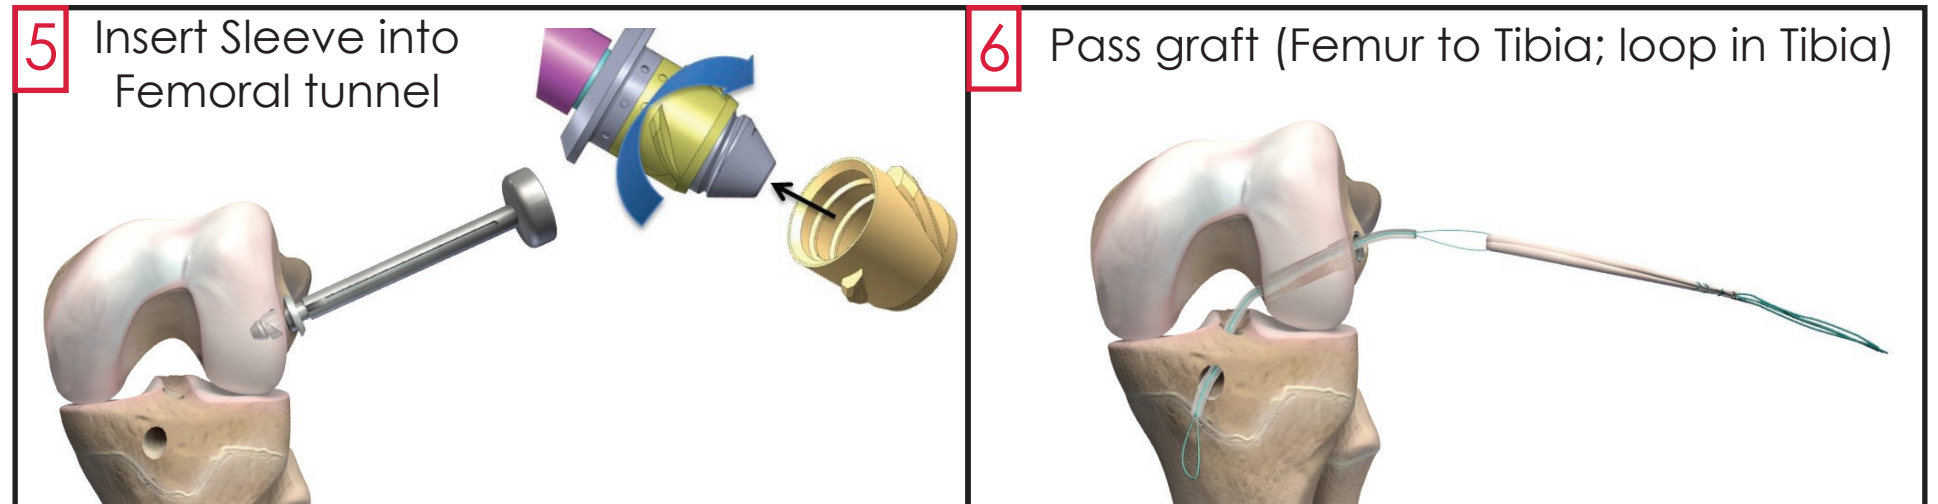


ACL Reconstruction System Overview

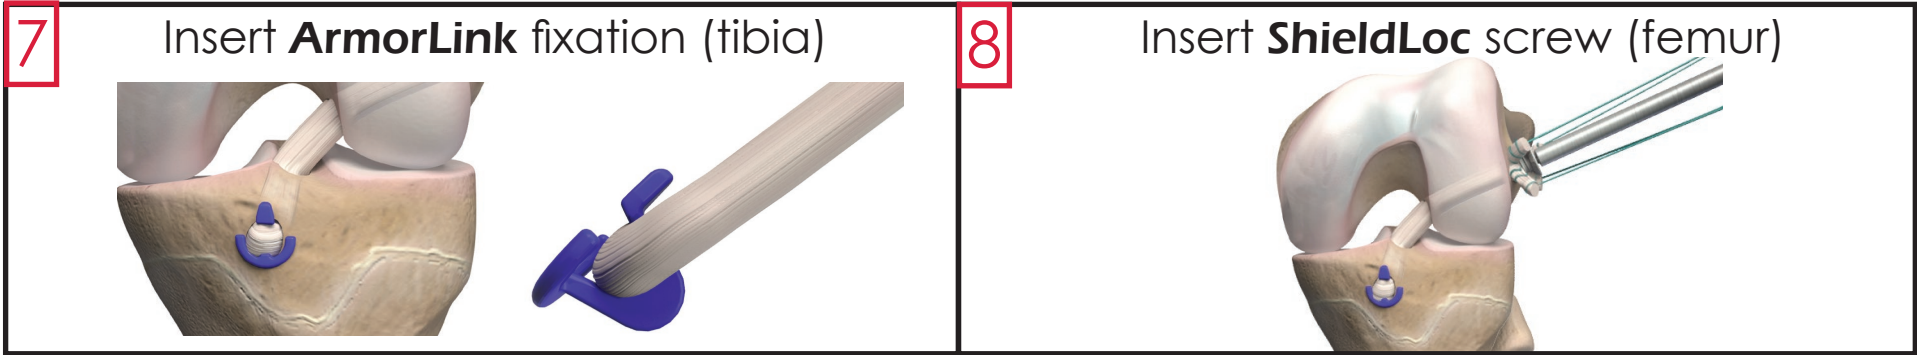

ArmorLink™
(Sterile Packed)

Product Description	Color	Part Number	Size (mm)
6mm ArmorLink	Blue	10-1008-1060	6
6.5mm ArmorLink	Bronze	10-1008-1065	6.5
7mm ArmorLink	Green	10-1008-1070	7
7.5mm ArmorLink	Dark Blue	10-1008-1075	7.5
8mm ArmorLink	Magenta	10-1008-1080	8
8.5mm ArmorLink	Teal	10-1008-1085	8.5
9mm ArmorLink	Aqua	10-1008-1090	9
10mm ArmorLink	Purple	10-1008-1100	10

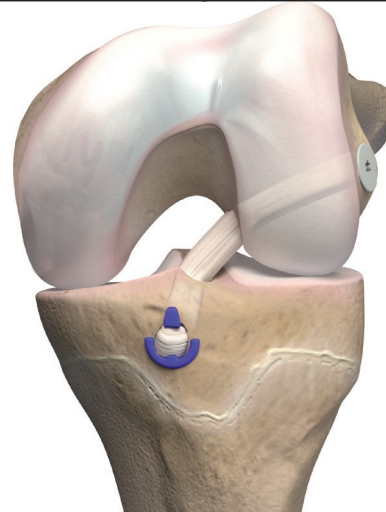


ACL Disposable Items

Product Description	Part Number	Packaging
ACL Disposable Kit	11-1008-5000	Sterile Packed
<i>Contents: 0.5mm Guide Wire - qty 1, 2.5mm Drill Tip Guide Pin - qty 2, Tunnel Plug - qty 2, Graft Passer - qty 1</i>		
0.5mm x 250mm Guide Wire	01-1008-0050	Non-Sterile Loose Inventory
2.5mm Drill Tip Guide Pin	01-1008-0051	Non-Sterile Loose Inventory



ShieldLoc™
(Sterile Packed)



Product Description	Driver	Part Number	Size (mm)
6mm ShieldLoc	T15	10-1008-4060	6
6.5mm ShieldLoc	T15	10-1008-4065	6.5
7mm ShieldLoc	T20	10-1008-4070	7
7.5mm ShieldLoc	T25	10-1008-4075	7.5
8mm ShieldLoc	T25	10-1008-4080	8
8.5mm ShieldLoc	T25	10-1008-4085	8.5
9mm ShieldLoc	T25	10-1008-4090	9
10mm ShieldLoc	T25	10-1008-4100	10

Indications: The OrthoPediatics ACL Reconstruction System is intended for fixation of tendons and ligaments during orthopedic reconstruction procedures such as Anterior Cruciate Ligament (ACL) Reconstruction.



IFU, cleaning instructions and surgical techniques may be obtained by calling OrthoPediatics® Customer Service at 574-268-6379. Read and understand indications, warnings and adverse effects explained in IFU's prior to use.

OrthoPediatics, Children Are Not Just Small Adults, PediPlates, PediLoc, PediFlex, PLEO, PediNail, Response, Scwire, ShieldLoc, ArmorLink and the Pedi logo are trademarks of OrthoPediatics Corp. OrthoPediatics, Children Are Not Just Small Adults, PediPlates, PediLoc, Scwire and the Pedi logo are registered trademarks in the United States. The Pedi logo is a registered trademark in Australia and New Zealand, and a registered Community Trade Mark.

2850 Frontier Drive • Warsaw, IN 46582 • ph: 574.268.6379 or 877.268.6339 • fax: 574.268.6302 • www.OrthoPediatics.com

OrthoPediatics Corp. ©2014 SA-1008-01-02 Rev A