

sleep  number®

ADJUSTABLE BASE
ASSEMBLY GUIDE



Congratulations

You're about to take the personalized comfort of your SLEEP NUMBER® bed to the ultimate level. By adding an adjustable base, you're creating an even more personalized sleep environment and enhancing the customized comfort of the bed that can significantly improve your sleep quality.

At SLEEP NUMBER®, we're dedicated to improving your sleep with new and innovative products—everything from beds to bedding solutions designed to help you sleep just right. We know that you, too, will fall in love with Sleep Number® comfort, quality, and customer service—and a truly individualized sleep experience.



What's Inside

Congratulations! Your new SLEEP NUMBER® adjustable base is set up and ready to enjoy. Inside, you'll find instructions for the easy-to-use remote. Whether reading, relaxing or sleeping soundly, we know you'll fall in love with comfort you can adjust in every way. Look to *Sleep Number* for innovations with your individual needs in mind.

Adjustable Base: What's Included	pg XX
Your Adjustable Base at a Glance	pg XX
Your Remote at a Glance	pg XX
Preparing Your Adjustable Base Control™ System and Remote	pg XX
Installing Your Mattress	pg XX
Optional Accessories	pg XX
Assembling Your Headboard Brackets	pg XX
Replacing Snap Latches	pg XX
Product Care	pg XX
Warranty	pg XX
Advisory	pg XX
Frequently Asked Questions	pg XX
Welcome to Sleep Number InnerCircle®	pg XX



Before You Begin

Assembling Your Adjustable Base

Carefully check the contents of your base boxes.

Make sure you have the correct number of components for the size of bed you purchased. If you are missing any items listed to the right, please call 1.800.472.7185 or email Customer Service at customerservice@selectcomfort.com

Adjustable Base: What's Included

	Twin	Full/ Queen	King	Split/ Flex Top King
Remote	1	1	1	2
Adjustable Base Control™ System	1	1	1	1
4-inch Leg	4	4	8	8
Caster	4	4	8	8
Mattress Retainer Kit	1	1	2	2
Bed Strap Kit <small>King bases only</small>	0	0	1	1
Power Cord	1	1	1	1
Under-bed Lights <small>FlexFit Plus™ only</small>	1	2	2	2

Adjustable Base Components

Remote



May vary by model

Adjustable Base Control™ System



FPO

May vary by model

4-inch Legs



Casters



Mattress Retainer Kit



Bed Strap Kit



FlexFit Plus™ only

Power Cord



Under-bed Lights




FPO

King bases only

Your Base at a Glance

- A** Left Adjustable Base
- B** Right Adjustable Base
- C** Junction Cables
- D** Adjustable Base Control™ System Back
- E** Adjustable Base Control™ System Front

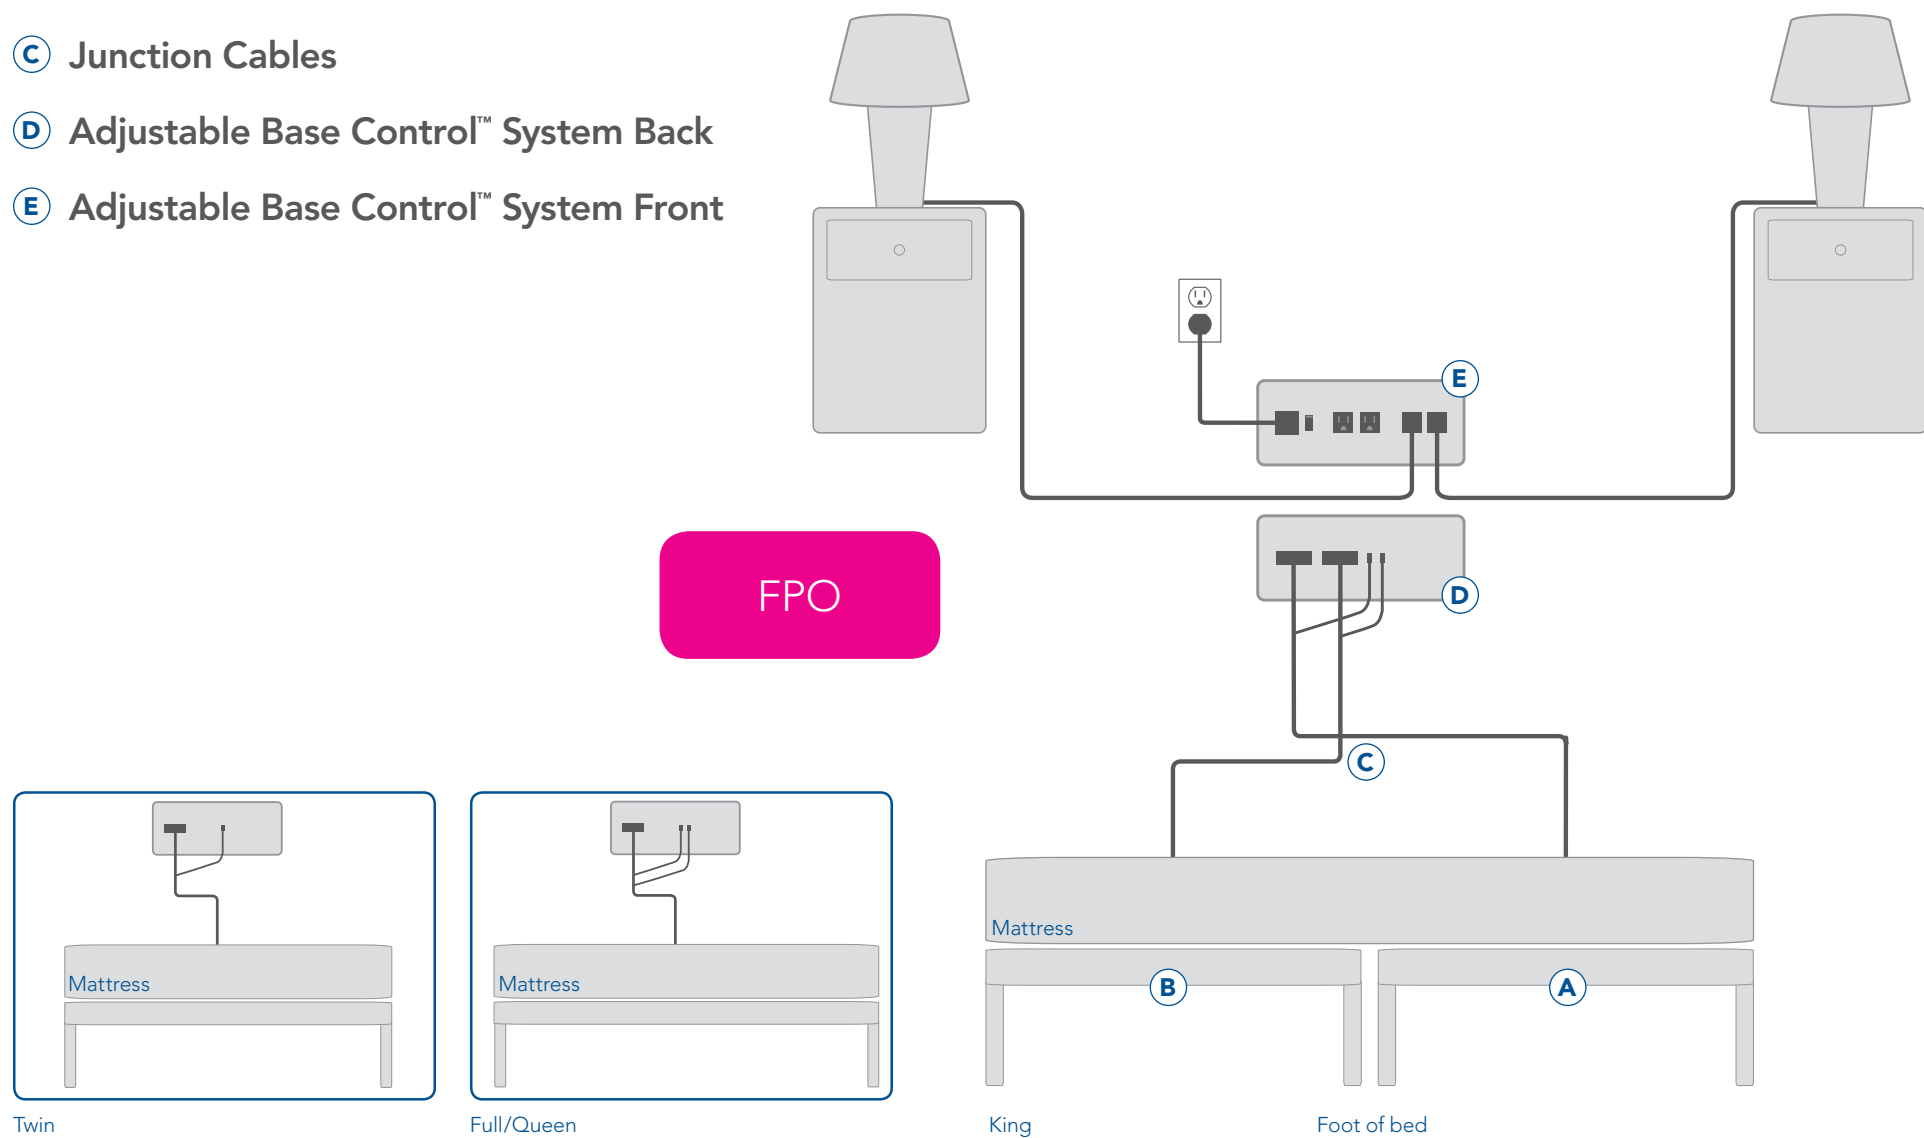

Twin

Full/Queen

King



Foot of bed

Your Adjustable Base Control™ System at a Glance

- A** Power Cord Connector
Connect the AC power cord.
- B** Reset Button
Resets the Adjustable Base Control™ box.
- C** Outlets (FlexFit PLUS™ only)
Constant power for the Firmness Control™ system, alarm clock, etc.
- D** Left Night Stand (FlexFit PLUS™ only)
Independent control of left night stand from remote.
- E** Right Night Stand (FlexFit PLUS™ only)
Independent control of left night stand from remote.
- F** Left Sleep Number®
Adjustable Base Connection (King Only)
- G** Right Sleep Number®
Adjustable Base Connection (King Only)
- H** Flat Base Button
Press to return base to flat position.
- I** Nightlight (FlexFit PLUS™ only)
Connection for under-bed lighting.



Your Remote at a Glance

Press the  Home button on your FlexFit™ or FlexFit PLUS™ remote to bring up the menu. For FlexTop™ bases, press the Menu/Select button  to bring up the menu. From here you can change your SLEEP NUMBER® setting, rename your side of the bed, find customer support information and more.



- Sleep Number®**
 - Return to your favorite *Sleep Number* setting at any time.
 - Adjust *Sleep Number* setting.
 - **Find Sleep Number®** guides you to your ideal level of firmness, comfort and support.
- Bed Position**
 - Set or change your bed position, or adjust the head and foot position using the Up/Down buttons.
- System**
 - **Rename Side** to name either side of the bed.
 - **Customer Support** gives you contact information if you have any questions.
 - Change setting and view notifications
 - **Back** returns you to the main menu.
- Exit**
 - Displays the most recent *Sleep Number* setting.

FlexFit PLUS™ Remote

- Head/Foot**
 - Press to select head or foot and use the Up/Down buttons to adjust bed position
- Favorite**
 - Choose popular bed positions including Read, Watch TV, and Zero Gravity
- Lights**
 - Turn on or off lights that are plugged in to your FlexFit PLUS™ adjustable base
 - Options include under-bed nightlight, right nightstand, and left nightstand
 - Brighten or dim under-bed lighting in the **System** menu
- Up/Down Buttons**
 - Adjust your SLEEP NUMBER® setting or your bed position. Scroll up or down in any menu
- Enter Button**
 - Press to select an option



- My Sleep Number® Setting button**
 - Press this button to return to your *Sleep Number* setting
- Side Button**
 - Press to choose your side of the bed
- Home**
 - Select **Sleep Number®**, **Bed Position**, **Sleep IQ** (when purchased), and **System**
- Massage**
 - Choose type of massage or experience a customized full body massage
- Timer**
 - Set to change bed position and turn off massage and/or lights

FlexFit™ Remote

- Head/Foot**
 - Press to select head or foot and use the Up/Down buttons to adjust bed position
- Favorite**
 - Choose popular bed positions including Read, Watch TV, and Zero Gravity
- Up/Down Buttons**
 - Adjust your SLEEP NUMBER® setting or your bed position. Scroll up or down in any menu
- Enter Button**
 - Press to select an option



FlexTop™ Remote

- My Sleep Number® Setting button**
 - Press this button to return to your *Sleep Number®* setting
- Side Button**
 - Press to choose your side of the bed
- Up/Down Buttons**
 - Adjust your SLEEP NUMBER® setting or your bed position. Scroll up or down in any menu
- Menu/Select**
 - Lets you select your favorite *Sleep Number* setting, bed position and more



Important Safety Instructions

When using an electrical furnishing, basic precautions should always be followed, including the following:

DANGER – To reduce the risk of electric shock:

1. Always unplug this furnishing from the electrical outlet before cleaning.

WARNING – To reduce the risk of burns, fire, electric shock, or injury to persons:

1. Unplug from outlet before putting on or taking off parts.
2. Close supervision is necessary when this furnishing is used by, or near children, invalids, or disabled persons.
3. Use this furnishing only for its intended use as described in these instructions. Do not use attachments not recommended by the manufacturer.
4. Never operate this furnishing if it has a damaged cord or plug, if it is not working properly, if it has been dropped or damaged, or dropped into water. Return the furnishing to a service center for examination and repair.
5. Keep the cord away from heated surfaces.
6. Never operate the furnishing with the air openings blocked. Keep the air openings free of lint, hair, and the like.
7. Never drop or insert any object into any opening.
8. Do not use outdoors.
9. Do not operate where aerosol (spray) products are being used or where oxygen is being administered.
10. To disconnect, turn all controls to the off position, then remove plug from outlet.
11. Contains Always On Receptacles. To Reduce Risk of Electric Shock – Disconnect power strip from power source before servicing any equipment connected to the power strip.
12. Never place items on top of the control box.
13. For grounded products the following statement:

WARNING: Risk of Electric Shock – Connect this furnishing to a properly grounded outlet only.

SAVE THESE INSTRUCTIONS.


GROUNDING INSTRUCTIONS

(a) For all grounded, cord-connected products:

This product must be grounded. If it should malfunction or breakdown, grounding provides a path of least resistance for electric current to reduce the risk of electric shock. This product is equipped with a cord having an equipment-grounding conductor and a grounding plug. The plug must be plugged into an appropriate outlet that is properly installed and grounded in accordance with all local codes and ordinances.

DANGER – Improper connection of the equipment-grounding conductor can result in a risk of electric shock. Check with a qualified electrician or serviceman if you are in doubt as to whether the product is properly grounded. Do not modify the plug provided with the product – if it will not fit the outlet, have a proper outlet installed by a qualified electrician.

(b) For a grounded, cord-connected product rated less than 15 amperes and intended for use on a nominal 120-volt supply circuit, the instructions in either 1) or 2)

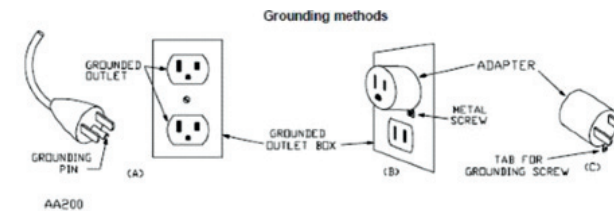

1) This product is for use on a nominal 120-volt circuit, and has a grounding plug that looks like the plug illustrated in sketch A (see Figure 63.1). A temporary adapter that looks like the adapter illustrated in sketches B and C able to be used to connect this plug to a 2-pole receptacle as shown in sketch B if a properly grounded outlet is not available. The temporary adapter should be used only until a properly grounded outlet (sketch A) can be installed by a qualified electrician. The green colored rigid ear, lug, or the like extending from the adapter must be connected to a permanent ground such as a properly grounded outlet box cover. Whenever the adapter is used, it must be held in place by a metal screw.

2) This product is for use on a nominal 120-volt circuit and has a grounding plug that looks like the plug illustrated in sketch A (see Figure 63.1). Make sure that the product is connected to an outlet having the same configuration as the plug. No adapter should be used with this product.

(c) For all other grounded, cord connected products: This product is for use on a circuit having a nominal rating more than 120 volts (or this product is rated more than 15 amperes and is for use on a circuit having a nominal rating of 120 volts) and is factory-equipped with a specific electric cord and plug to permit connection to a proper electric circuit. Make sure that the product is connected to an outlet having the same configuration as the plug. No adapter should be used with this product. If the product must be reconnected for use on a different type of electric circuit, the reconnection should be made by qualified service personnel.

(d) For permanently connect products:

This product must be connected to a grounded metal, permanent wiring system, or an equipment-grounding conductor must be run with the circuit conductors and connected to the equipment-grounding terminal or lead on the product.

Preparing Your Adjustable Base Control™ System & Remote

1 Adjustable Base Control™ System Placement

- Place the Adjustable Base Control™ system on the floor under the head of the bed.
- Plug the power cord into the Adjustable Base Control™ system. Do NOT connect to power at this time.
- **FlexFit PLUS™ only:** Plug night stand lights (not included) into corresponding “Left Night Stand” and “Right Night Stand” outlets on the Adjustable Base Control system. See diagram on page XX for outlet locations.



2 Connect Your Adjustable Base(s)


- Plug the junction cable(s) under the adjustable base(s) into the Adjustable Base Control™ system.

NOTE: King size beds have a left and right junction cable.

2a Connect Your Under-Bed Lighting (FlexFit PLUS™ only)

- For Twin size beds, you will install one light; for Full, Queen, and King size beds you'll install two lights. See the diagrams at right for under-bed light placement.
- Peel the adhesive backing off one LED light and install the light on the vertical surface inside the rail under the adjustable base, facing toward the center of the bed (see diagram for location). For Full, Queen, and King beds, install the second light on the second base with the light facing toward the center of the bed (see diagram for location). Ensure that each light faces toward the center of the bed.
- Plug the LED connector(s) into junction cable(s) attached to the underside of the adjustable base.
- Plug the junction cable connector(s) at the head of the bed into the Adjustable Base Control™ system.

NOTE: Lights should face inward toward the center of the bed to create a glow when illuminated. Brightness can be adjusted with the remote. Lights installed facing outward will create a floodlight effect.

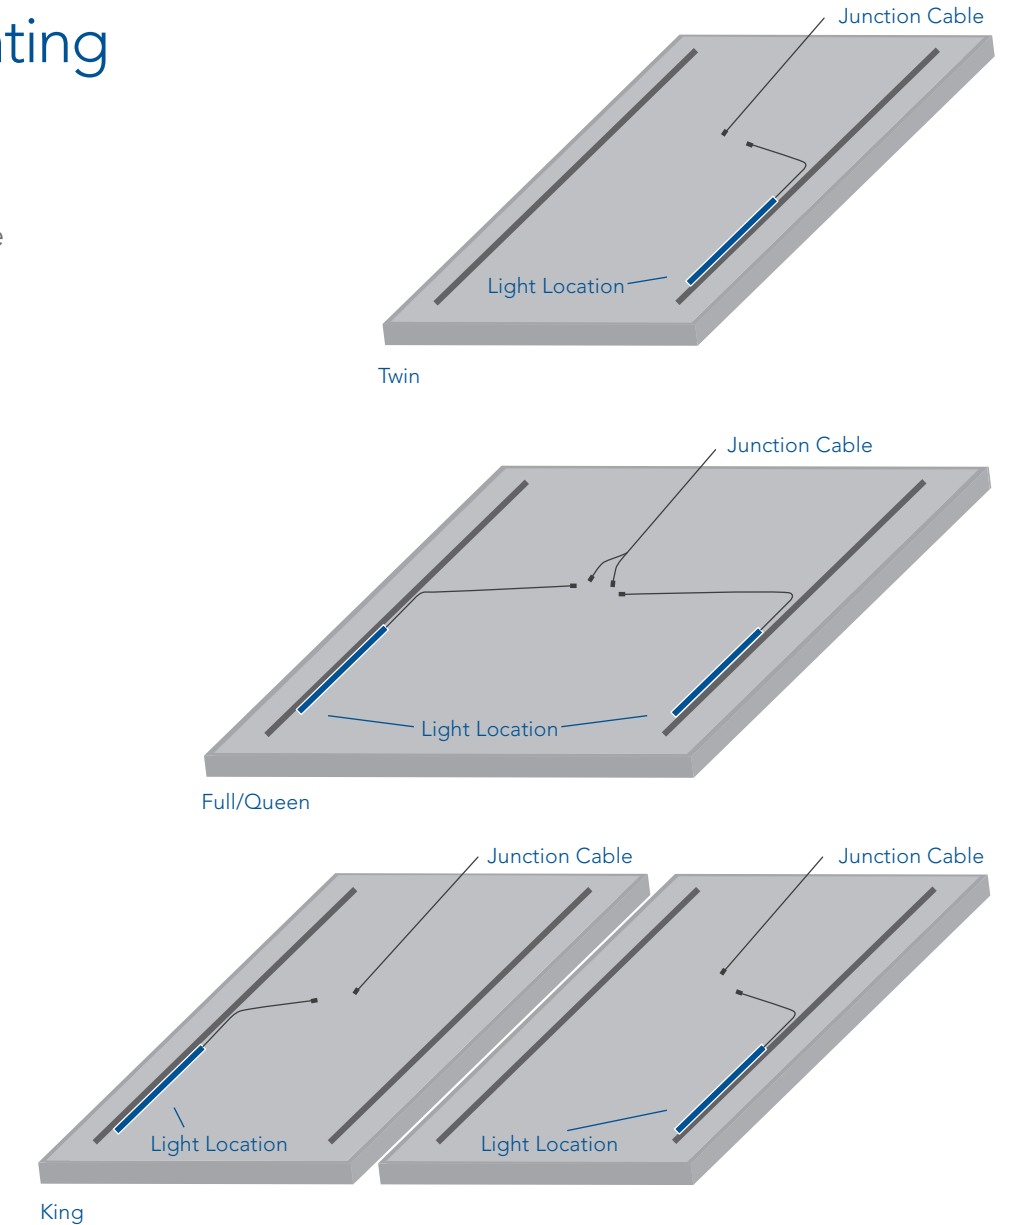

Bottom of base shown.

3 Pair Your Remote With Your Firmness Control™ System & Adjustable Base Control™ System

- Insert (2) AA batteries (included) into the remote and press any button on the remote to illuminate the screen.
- A setup screen will appear on the remote. Follow the on-screen instructions to complete setup, and add additional remotes.

NOTE: For beds without a Sleep Number® Firmness Control™ system, select **Skip** on the Setup screen and proceed to step 4.

4 Pairing Replacement Remotes

- Using your first remote, select **System**, then **Settings**, then **Add Remote**.
- Follow the on-screen instructions to complete setup

1 Prepare Your Adjustable Base

Tools Required: utility knife, Phillips® head screwdriver

WARNING: Exercise extreme caution when using utility knife. The danger of serious finger cuts is possible if utility knife is not used correctly.

IMPORTANT: Wash hands before beginning installation. Residue on hands will easily transfer to cloth-covered bed components.

- Verify adjustable base setup is complete.
- Identify four locator pins on the top of the adjustable base. Locator pins mark the threaded hole locations used for SLEEP NUMBER® mattress attachment.
- Remove all four locator pins and install (4) hex head bolts.




Pull out each locator pin from the threaded lugs.

Installing Your Mattress


2 Align Mattress

- Unzip the *Sleep Number* mattress cover and set cover top aside.
- Position the bottom of the *Sleep Number* mattress cover on top of the adjustable base ensuring the head of the mattress cover (side with openings for air hoses) is matched with the head of the adjustable base. Make sure the air chambers and foam border walls are not installed, leaving only the fabric mattress cover forming a box (diagram A below).
- Invert the mattress cover by pulling the sides of the mattress cover down over the adjustable base (diagram B below).
- At each hex head bolt location, use the utility knife to make a small cut (no larger than ¼" long) through the mattress cover fabric.
- Pull sides of mattress cover back up to their original position. Remove the mattress cover.

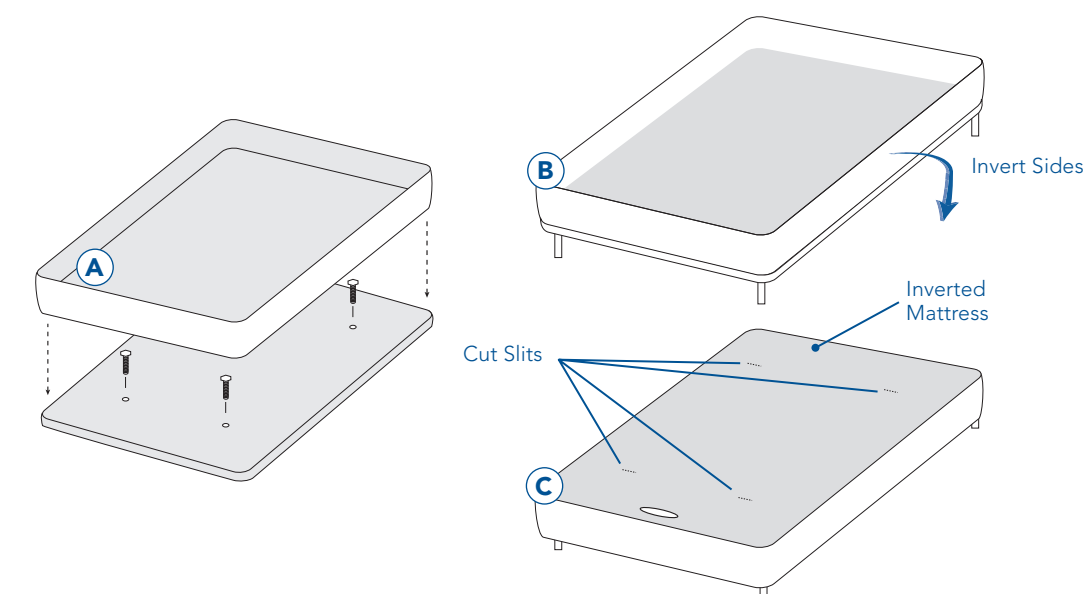


3 Install Mattress Retainer Kit

- Remove hex head bolts
- Place the bottom attachment pieces between the adjustable base and mattress cover bottom at each hex head bolt location
- Place the mattress cover bottom back on the base. Align the mattress cover with the adjustable base ensuring that the head of the mattress is matched with the head of the base.
- Place the top attachment pieces over the four cuts and insert hex head bolts.
- Tighten all four hex head bolts to finger tight. Do not over tighten.
- Complete mattress setup per the SLEEP NUMBER® mattress installation instructions.

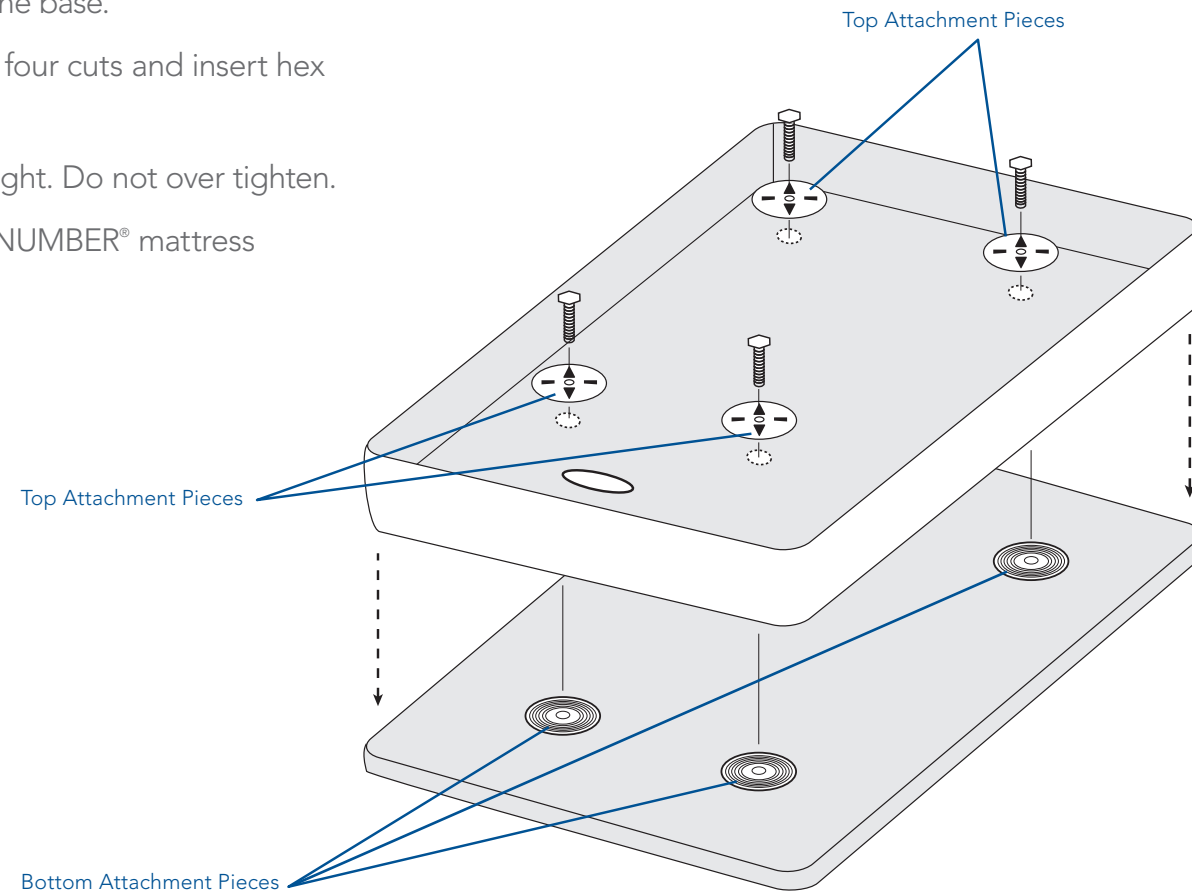

Optional Accessories Size Chart

Bed Type	A Frame Width	B Base Width	C Base Length	FlexTop™ Weight	FlexFit™ Weight	FlexFit Plus™ Weight
Twin Extra-Long	28"	37"	79.5"	110 lbs.	116 lbs.	138 lbs.
Full	38"	52.5"	73.5"	142 lbs.	147 lbs.	162 lbs.
Queen	38"	58.5"	79.5"	145 lbs.	150 lbs.	173 lbs.
Cal.King (per side)	28"	35.5"	83.5"	113 lbs.	118 lbs.	138 lbs.
King (per side)	28"	37"	79.5"	110 lbs.	116 lbs.	138 lbs.

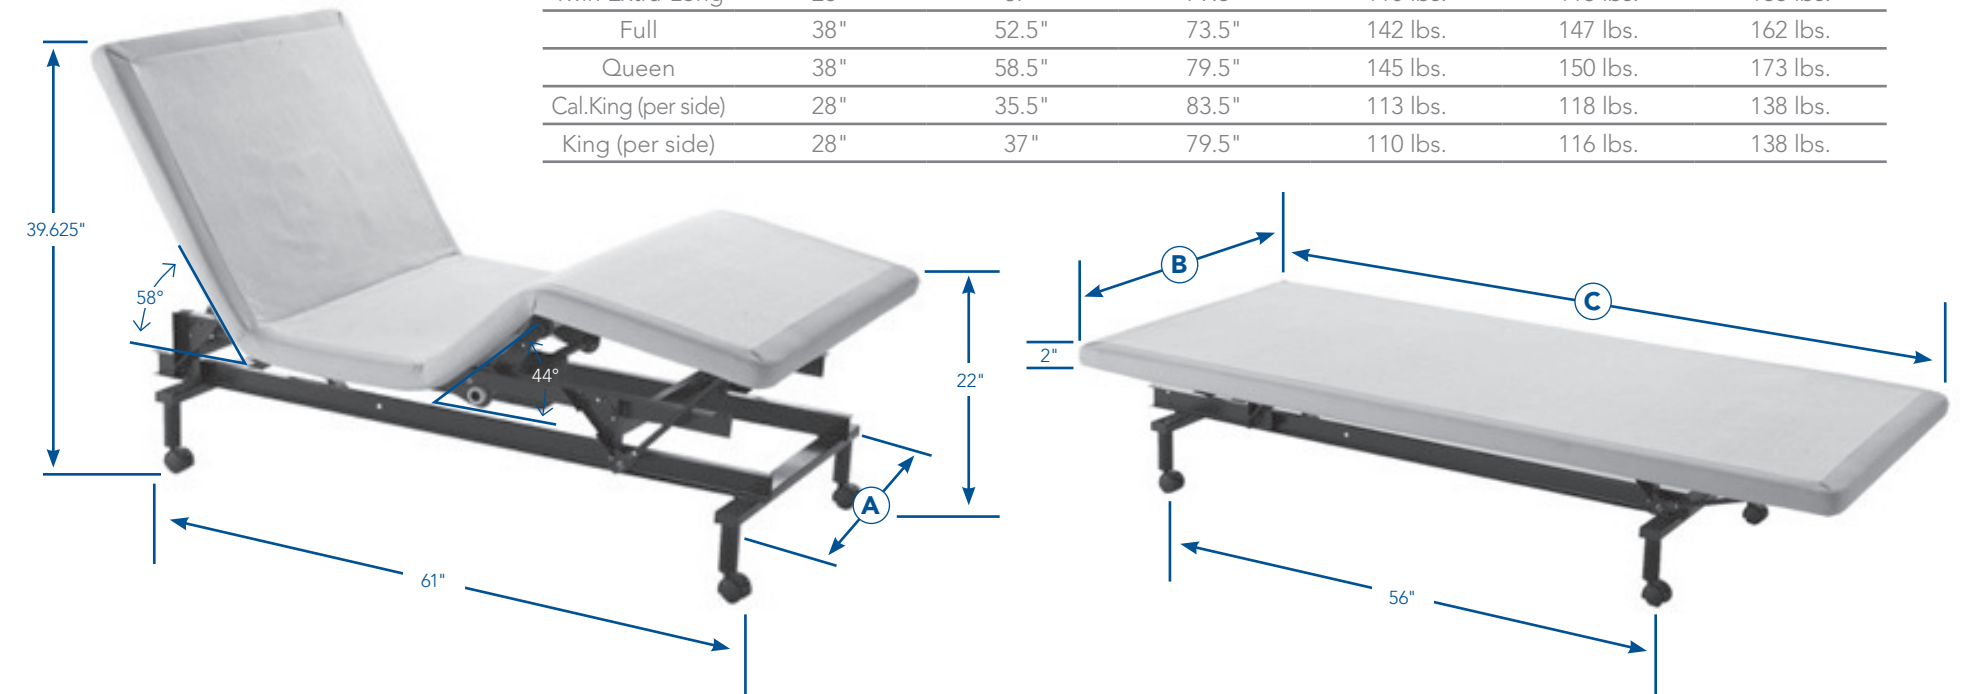

	Glide Only	Threaded Caster	Standard 4" Leg (without caster)	Standard 4" Leg (with caster)	Standard 7" Leg (without caster)	Standard 7" Leg (with caster)	Standard 9" Leg (without caster)	Standard 9" Leg (with caster)	Standard 11" Leg (without caster)
D Height to Frame	1.5 - 1.9	2.5	4.1	6.6	7.125	9.6	9.1	11.6	11.1
E Height to Base	8.9 - 9.5	10.1	11.8	14.3	14.75	17.3	16.8	19.3	18.8
F Height to Mattress	10.9 - 11.5	12.1	13.8	16.3	16.75	19.3	18.8	21.3	20.8
Under-Bed Clearance	0	0.5	2.5	5	6	8	8	10	10

Optional Accessories

The FlexTop™, FlexFit™ and FlexFit PLUS™ adjustable bases fit standard bedroom furniture. If your furniture does not accommodate the adjustable base please contact Customer Service at 1-800-472-7185 for potential solutions. Call 1-800-580-7216 for accessory pricing and to order the accessories listed in the chart to the right.

Swing Away Hinges (Split King Only)

For easy under-bed cleaning and bed-making access. Split King beds easily split apart with the swing away hinges that attach between the headboard and each side of the split king bed. Two hinges included.

Legs

For increased bed height and under-bed storage. Select from three leg height options to replace the standard 4" legs. Four legs per set. See diagram on page X for bed height dimensions.

Caster Cups

Required for use of adjustable bases on hardwood floors. Install under caster wheels to prevent the bed from moving on hardwood flooring. Four cups per set.

Adjustable Retainer Bar Kit

For use with non-SLEEP NUMBER® beds. Sleep Number beds use our patented mattress-retaining kit to attach the mattress to the adjustable base. The retainer bar is required when other mattresses are used with the adjustable base to prevent the mattress from sliding when you raise the head of the bed.

Glides

Our lowest bed-height option. Glides replace the standard 4" legs. Four glides per set. See diagram on page X for bed height dimensions. Note: headboard brackets cannot be used with glides.

Threaded Casters

Our second-lowest bed-height option. Threaded casters replace the standard 4" legs. Four threaded casters per set. See diagram on page X for bed height dimensions. NOTE: headboard brackets cannot be used with threaded casters.

Optional Accessories

	Code	Qty.
Glides (headboard bracket cannot be used with glides)	107397	4
Caster Cups	116449	4
Threaded Caster	TBD	4
7" Legs with Casters	107399	4
9" Legs with Casters	116447	4
11" Legs	116448	4
Swing Away Hinge Kit	107396	1
Adjustable Retainer Bar Kit	117450	1
FlexTop™ and FlexFit™ Headboard Bracket Assembly	Full	118102
	Queen	118103
	Twin/E. King/Split King	118101
	Cal. King/Split Cal. King	118104
FlexFit™ PLUS Headboard Bracket Assembly	Full	118106
	Queen	118107
	Twin/E. King/Split King	118105
	Cal. King/Split Cal. King	118108

Optional Accessories

Glides



Caster Cups



Legs



Threaded Casters




Swing Away Hinge Kit



Adjustable Retainer Bar Kit



Headboard Bracket Assembly

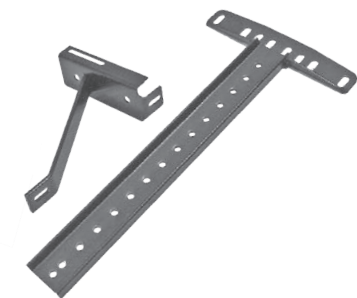

Assembling Your Headboard Brackets (optional)

1 Install Headboard Brackets



- Headboard brackets are only needed for non-freestanding headboards.
- Use remote to raise the head section of the bed to access the adjustable base frame.
- Locate the headboard bracket assembly. On one side of the adjustable base frame, locate two holes for channel headboard bracket mounting.



FPO

2 Position Channel Connector


- For Full size beds, use inner mounting holes. For Queen, King or California King beds, use outer mounting holes.
- Position channel connector so the flat side is flush against adjustable base frame. Attach channel connector to adjustable base frame using two 1½-inch hex head bolts/nuts.

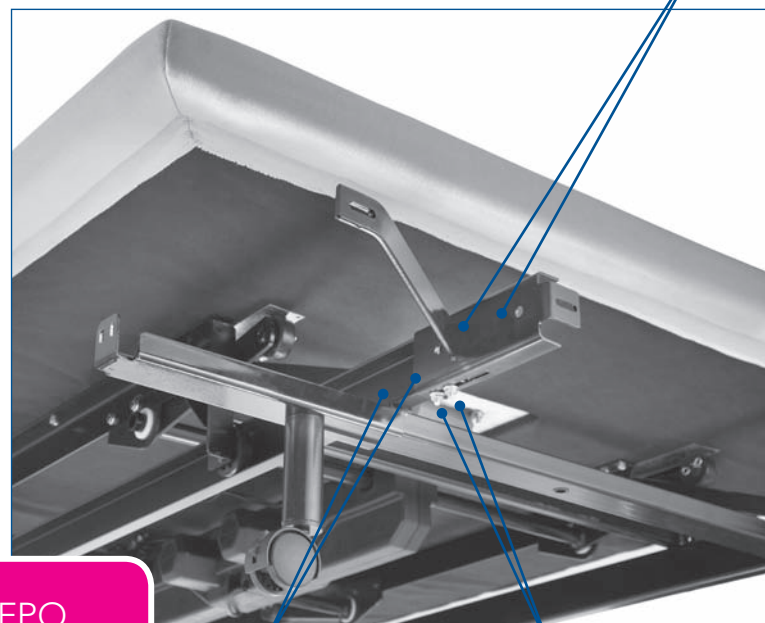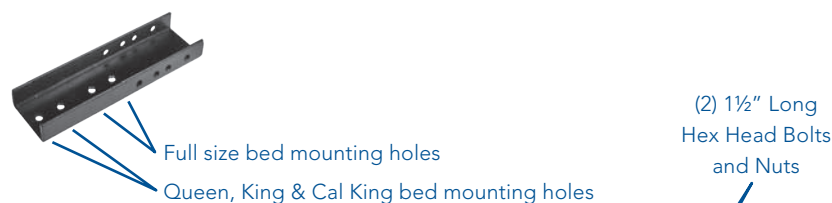

FPO

3 Attach Headboard Bracket Channel


- Using two 3-inch carriage bolts/nuts, attach one headboard bracket channel to the first channel connector.
- Hand tighten bolts/nuts (loosely) to allow adjustment of the headboard bracket channels.

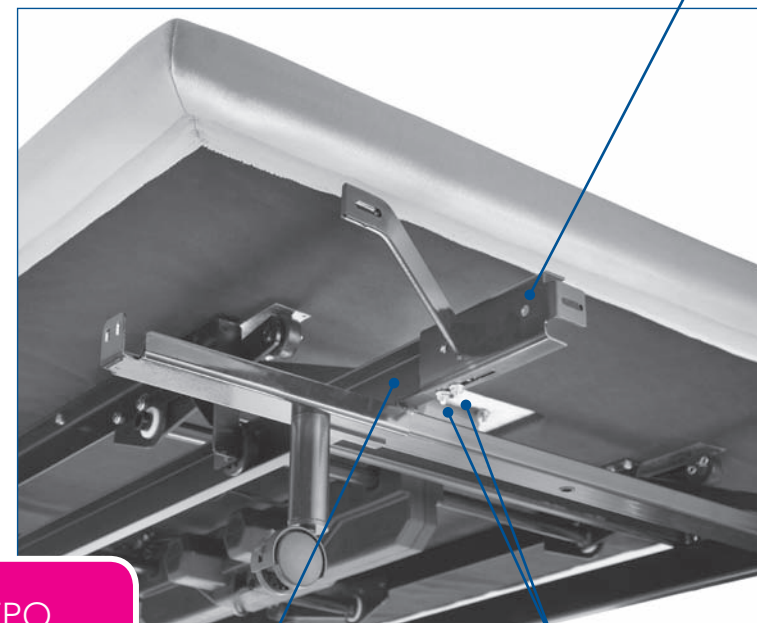

FPO

4 Attach Headboard Bracket Flange


- Attach one headboard bracket flange to one of the bracket channels with two 1-inch hex head bolts/nuts.
- Repeat on the other side to attach the second headboard bracket flange.
- Slide headboard bracket assemblies (in or out) to achieve a distance of 1½ inches (38.1 mm) to 2 inches (50.8 mm) between the edge of the adjustable base and the headboard bracket flange assemblies.

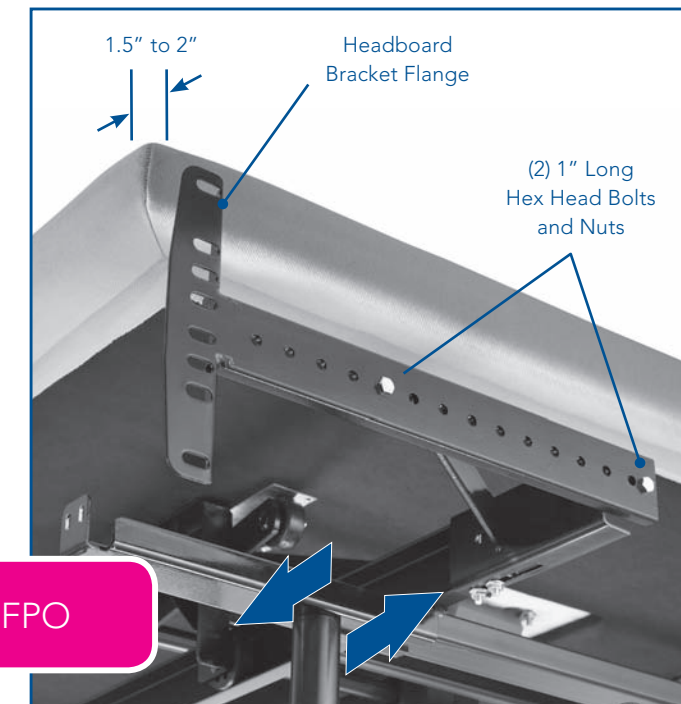

FPO

5 Adjust and Secure Brackets

- Firmly tighten the 3-inch carriage bolts on both headboard bracket channels.
- Measure the distance (center-to-center) between the mounting holes in the headboard.
- Measure the center-to-center distance between the mounting slots of the headboard bracket flanges.
- If bracket flange adjustment is required to accept the headboard, remove the 1-inch hex head bolts and move flanges side-to-side to adjust. Reinstall bolts. Tighten all headboard mounting bolts.

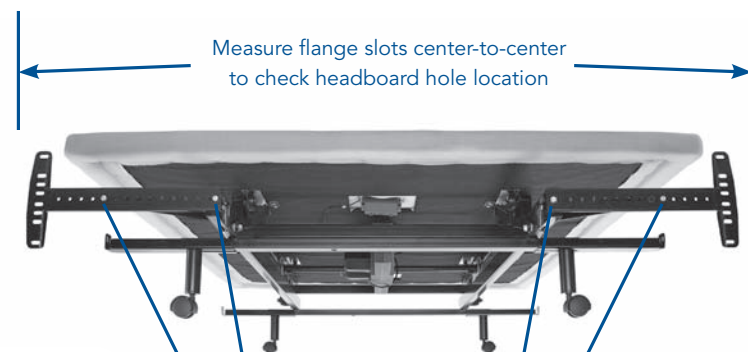

FPO

Remove 1-inch hex head bolts and relocate flanges to achieve center-to-center distance required for headboard mounting holes


6 Install Headboard

- Securely install your headboard.

IMPORTANT SAFETY NOTICE:

The bottom of the headboard cross member must be positioned so that there is no more than 3 inches (76.2mm) between the headboard and the top of the mattress.

WARNING: Do not exceed 3 inches (76.2mm) in order to avoid a person or pet being caught in the space (referenced below) while the bed is in motion. Failure to follow this instruction could result in serious personal injury or death.

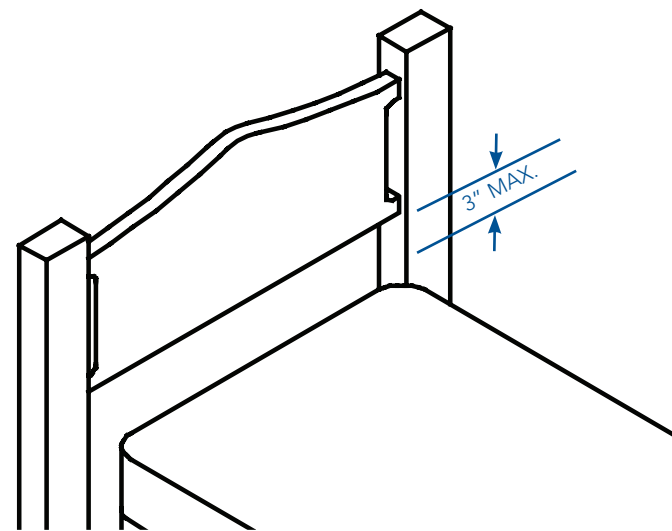

Headboard cross member location must not exceed 3 inches (76.2mm) from the top of the mattress.

Replacing Snap Latches on Beds with Base Silhouette

1 Raise Foot of the Bed

- Using your remote, fully raise the foot of your bed to allow ample working space.

WARNING: Danger of Entrapment. To prevent serious or fatal injuries from entrapment, do not allow a person (adult or child) or pet to play under the bed or base or with any remote controls.

2 Remove Silhouette Footboard


- Remove the Silhouette footboard by pulling out from the top of the footboard down toward the floor.
- Completely detach the footboard from the sideboards.



(FlexFit™ & FlexFit Plus™ Only)


3 Remove Snap Latch(es)

- Using a 7/16 inch wrench, unscrew the two bolts to remove the snap latch on the sideboard of the Silhouette. Repeat for other side as needed.

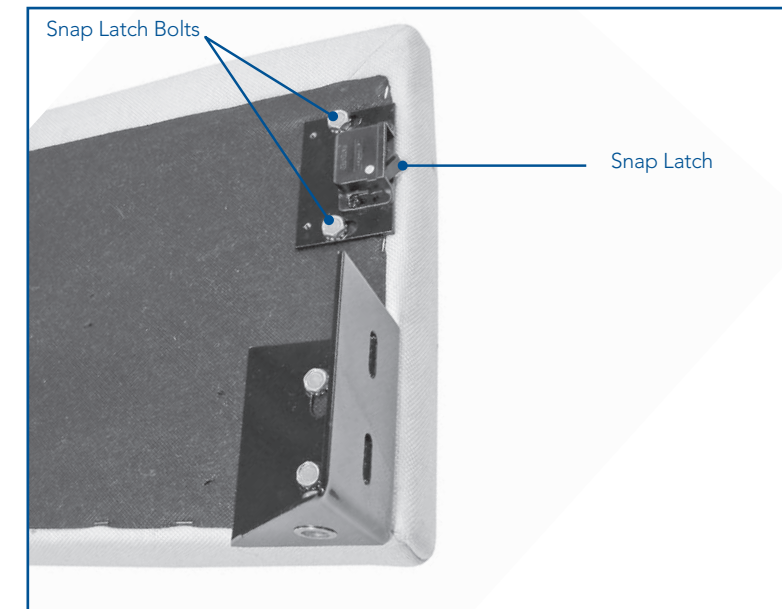


4 King Bases Only

- After removing the snap latches from the sideboards, remove the center snap latch, if necessary

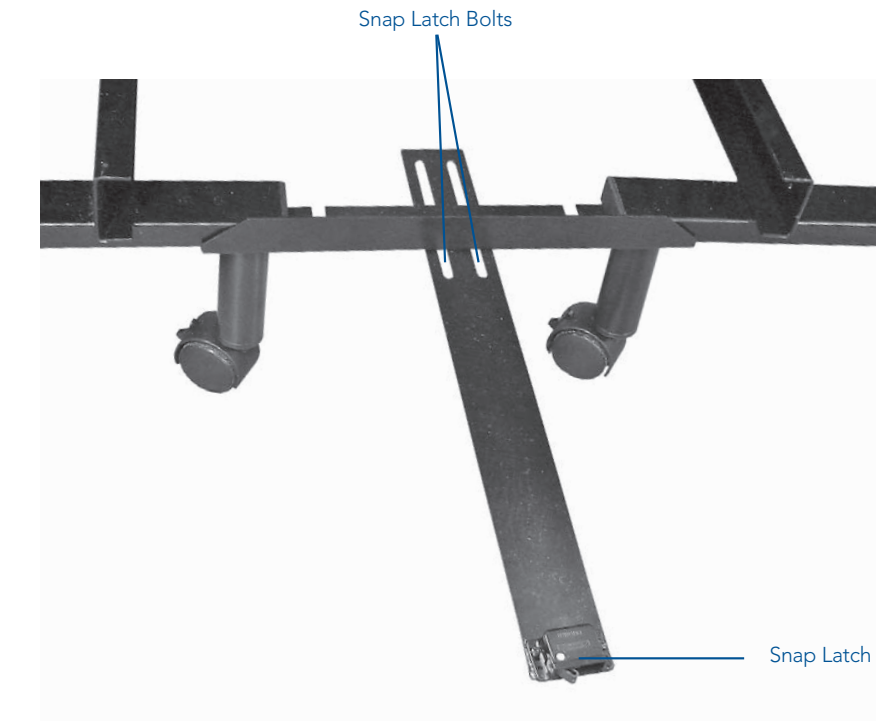

5 Attach New Snap Latch(es)

- After removing the snap latch(es) from the sideboards, place the new snap latch(es) in the same areas and loosely replace the bolts, allowing movement for alignment.
- For King size beds, replace the center snap latch, if necessary. Loosely replace the bolts, allowing movement for alignment.

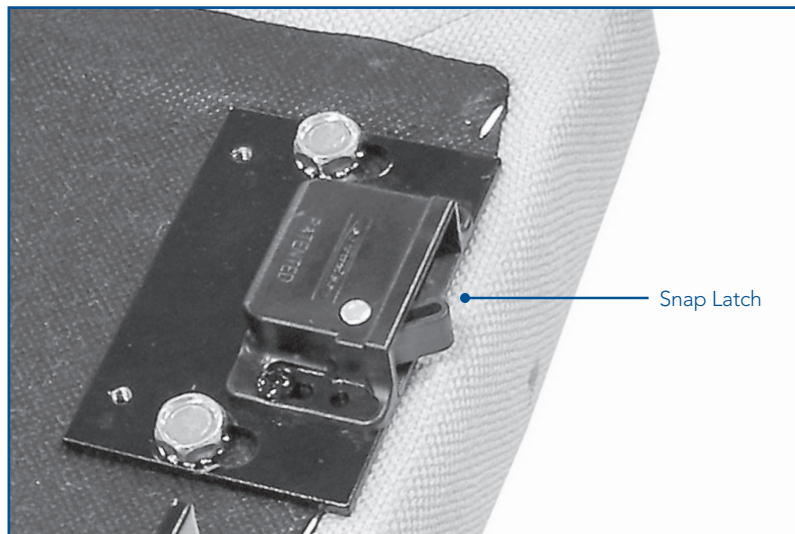


6 Reconnect Footboard and Align to Silhouette

- Reconnect the Silhouette footboard and align the footboard to the Silhouette sideboards, eliminating any gaps.



7 Tighten Bolts

- Once aligned, with Silhouette footboard attached, use the wrench to tighten all bolts on snap latches.

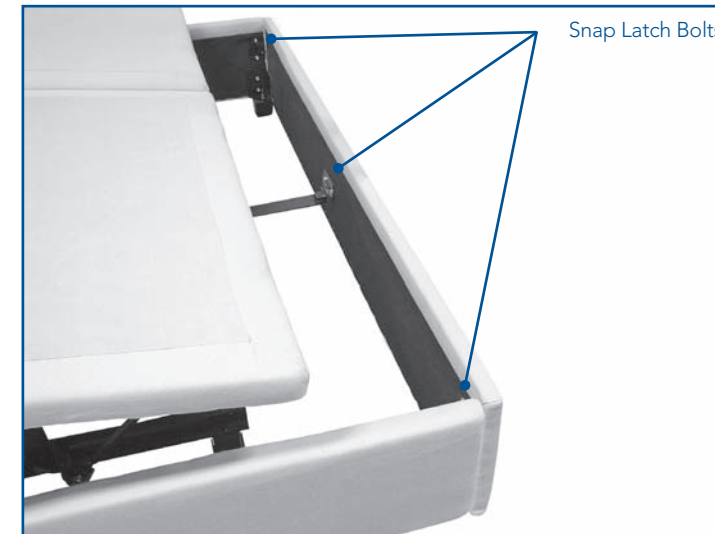

Product Care

Cleaning Your Remote

- Wipe the body with a clean cloth dampened with a mild soap and water solution.
- Wipe the display screen with a clean, dry, lint-free cloth.

CAUTION: Do not immerse in water or place in dishwasher.



Moving Your Sleep Number® Bed

- Always disassemble the base. Bag all hardware so that it is not lost.
- The mattress can be fully inflated, capped off and packaged in a mattress box for moving.
- If you don't have a mattress box, double-bag the cover and foam to prevent stains. Deflate and box the air chamber(s) to prevent possible damage.
- Pack the Firmness Control™ system in a box with packing material. Transport with minimal exposure to shock and vibration.
- Tuck the remote, air chamber caps and instructions in the box with the Firmness Control™ system to prevent them from being lost.

Moving Your Adjustable Base

- Copy to come

FlexFit™ Warranty

2-5-25 Warranty

Leggett & Platt, Incorporated (“L&P”) warrants this adjustable base to the consumer who is the original purchaser (the “purchaser”), subject to the terms and conditions set forth herein. This warranty begins on the “warranty commencement date” which is the date of purchase for new unused bases and the date of manufacture for bases that have been used as floor or display models. Thus, on a floor model base, the warranty is a portion of the limited 25 year warranty.

Full 2 Year Warranty

This adjustable base is warranted against defects in workmanship or materials for a period of 2 years from the warranty commencement date. Upon notice during the first 2 years after the warranty commencement date, L&P will repair or replace (at no cost to the purchaser) any defective adjustable base part, and L&P will pay all authorized labor and shipping costs associated with the repair or replacement of any parts found to be defective.

5 Year Limited Warranty

During the third through the fifth year from the warranty commencement date, upon receipt of notice, L&P will replace any adjustable base part found to be defective. This limited 5 year warranty shall not apply unless the defective part is returned to L&P within 10 days of purchaser’s receipt of the replacement part. Purchaser shall pay all service and shipping costs related to the replacement of the defective part.

25 Year Limited Warranty

Upon notice during the sixth year through the twenty-fifth year from the warranty commencement date, L&P will replace, upon terms and conditions set forth in this paragraph, any mechanical base part found to be defective. Electronics, electrical components, drive motors and massage motors are excluded. This limited 25 year warranty shall not apply unless the defective part is returned to L&P within 10 days of purchaser’s receipt of the replacement part. In years 6–25, purchaser shall pay all service and shipping costs related to the replacement of the defective part.

Additional Terms and Conditions

This warranty does not apply; (a) to any damage caused by the purchaser; (b) if there has been any repair or replacement of adjustable base parts by an unauthorized person; (c) if the adjustable base has been mishandled (whether in transit or by other means), subjected to physical or electrical abuse or misuse, or otherwise operated in any manner inconsistent with the operation and maintenance procedures outlined in this document and this warranty; (d) to damage to mattresses, fabric, cables, electrical cords or items supplied by dealers. Contact the dealer for warranty information on these items; (e) if there

has been any modification of the adjustable base without prior written consent by L&P; (f) to costs for unnecessary service calls, including costs for in-home service calls solely for the purpose of educating the consumer about the adjustable base or finding an unsatisfactory power connection; (g) if the recommended weight restriction is not followed (refer to Advisory section on page 25), the warranty will be void.

Repairs to or replacement of an adjustable base or its components under the terms of this limited warranty will apply to the original warranty period and will not serve to extend such period.

The decision to repair or to replace defective parts under this warranty shall be made, or cause to be made, by L&P at its option and in its sole discretion.

Repair or replacement shall be the sole remedy of the purchaser. There shall be no liability on the part of L&P for any special, indirect, incidental, or consequential damages or for any other damage, claim, or loss not expressly covered by the terms of this warranty.

This limited warranty does not include reimbursement for inconvenience, removal, installation, setup time, loss of use, shipping, or any other costs or expenses. Leggett & Platt or its service technicians shall not be responsible for moving furniture or any other items not attached to the adjustable base in order to perform service on the adjustable base.

It is the sole responsibility of the purchaser to provide adequate space and accessibility to the adjustable base. In the event that the technician is unable to perform service due to lack of accessibility, the service call will be billed to the purchaser and the service will have to be rescheduled.

L&P makes no other warranty whatever, express or implied, and all implied warranties of merchantability and fitness for a particular purpose are disclaimed by L&P and excluded from this agreement. Some states do not allow the exclusion or limitation of incidental or consequential damages, so the above limitation or exclusion may not apply to every purchaser.

This warranty gives the purchaser specific legal rights, and the purchaser may also have other rights, which may vary from state to state. This warranty is valid in all 50 states, Puerto Rico, and Canada. For warranty or other questions please contact Select Comfort Customer Service first.

CONTACT INFORMATION: Select Comfort, Customer Service Department, 9800 59th Ave N, Minneapolis, MN 55442, 1-800-472-7185

Silhouette Warranty

Subject to the terms and conditions and for the period set forth herein, Leggett & Platt, Incorporated (“L&P”) warrants to the original consumer purchaser (the “Purchaser”) that this silhouette kit is free of defects in material or workmanship caused by the manufacturer. This warranty begins on the date of the original retail purchase (“Warranty Commencement Date”).

2 Year Limited Warranty

Upon proper notice received during the two years after the original retail purchase, L&P will repair or replace (at no cost to the Purchaser) any silhouette kit found by L&P to have a defect covered by this warranty, and L&P will pay the original purchaser all labor and shipping costs authorized by L&P for repair or replacement of such part.

Additional Terms and Conditions

This warranty does not apply: (a) to any damage caused by the Purchaser or any person other than the manufacturer of the silhouette kit; (b) if there has been any repair or replacement of silhouette kit by an unauthorized person; (c) if the silhouette kit has been mishandled (whether in transit or by other means), subjected to physical or other abuse or misuse, or otherwise operated, used, or maintained in any manner inconsistent with the operation and maintenance procedures outlined in this warranty or in any manufacturer instructions; (d) to tears, flattening of nap, pilling, fading or shrinking; (e) when heavy soiling or abuse is evident; and (f) to wear and tear, defined as the deterioration/damage that naturally and inevitably occurs as a result of normal use, wear or aging.

TO THE EXTENT ALLOWED BY APPLICABLE LAW: (i) NEITHER THIS WARRANTY NOR THE WARRANTIES, IF ANY, IMPLIED BY LAW, SHALL EXTEND TO ANY PERSON OTHER THAN THE ORIGINAL PURCHASER; (ii) REPAIR OR REPLACEMENT AS PROVIDED IN THIS WARRANTY SHALL BE THE SOLE REMEDY OF THE PURCHASER; AND (iii) L&P DISCLAIMS, EXCLUDES, AND IN NO EVENT SHALL HAVE ANY LIABILITY FOR ANY SPECIAL, INDIRECT, INCIDENTAL, OR CONSEQUENTIAL DAMAGES OR ANY OTHER DAMAGE, CLAIM, OR LOSS NOT EXPRESSLY COVERED BY THE TERMS OF THIS WARRANTY. Some states do not allow the exclusion or limitation of incidental or consequential damages, so the above limitation or exclusion may not apply to every purchaser.

This limited warranty does not include reimbursement for inconvenience, removal, installation, setup time, loss of use, shipping, or any other costs or expenses. L&P or its service technicians shall not be responsible for moving furniture or any other items in order to perform service under this warranty.

L&P makes no other warranty whatever, express or implied, and all implied warranties, including any warranties of merchantability or fitness for a particular purpose, are disclaimed by L&P and excluded from this agreement to the extent permitted by applicable law. Implied warranties, if any, which under applicable law cannot be disclaimed or excluded, are hereby limited to the same warranty periods as the express

warranty herein, and are subject to the same terms, conditions, and limited remedies stated in this warranty.

This warranty gives the Purchaser specific legal rights, and the Purchaser may also have other rights, which may vary from state to state. This warranty is valid in the United States, Puerto Rico, and Canada. Notices and claims under this warranty must be in writing and submitted to:

Select Comfort
Customer Service Department
9800 59th Avenue North
Minneapolis, MN 55442
1-800-580-7216

Advisory

Important Information

Read the following information carefully before using this product. This adjustable base has been quality-engineered with design features to optimize your comfort and safety when operated properly.

Product Ratings

The bed lift motors are not designed for continuous use. Reliable operation and full life expectancy will be realized as long as the lift motors do not operate any more than 5 minutes over a 30 minute period, or approximately 15% duty cycle. Note: Massage equipped beds are not designed for continuous, extended massage operation.

Massage systems are rated for a maximum of 2 hours of use within any 6 hour period. Any attempt to circumvent or exceed product ratings will shorten the life expectancy of the product and may void the warranty. The recommended weight restrictions for FlexFit™ adjustable bases are as follows: DC equipped - 600 lb (272 kg) all sizes. The bed will structurally support the recommended weights distributed evenly across the head and foot sections. This product is not designed to support or lift this amount in the head or foot sections alone. NOTE: Exceeding the recommended weight restrictions could damage the adjustable bed and void the warranty. For best performance, consumers should enter and exit the adjustable bed with the bed in the flat (horizontal) position.

CAUTION: DO NOT SIT ON THE HEAD OR FOOT SECTIONS WHILE IN THE RAISED POSITION.

Operating Information

- After bed assembly is complete, operate remote to ensure proper bed functions.
- Keep moving parts free of obstruction (including sheets, clothing, tubing, wiring, and products using electric power cords) during bed operation.
- Distribute body weight evenly over bed surface. Do not place entire weight on raised head or foot sections of the bed, including during repositioning and entering or exiting bed.

FCC Compliance

This device complies with part 15 of the FCC Rules. Operation is subject to the following two conditions: (1) This device may not cause harmful interference, and (2) this device must accept any interference received, including interference that may cause undesired operation.

Any attempt to make changes or modifications to the remote (e.g. an intentional radiator) could void the user's authority to operate the remote according to FCC certification (section 15.231).

Small Children/Pets Warning

CAUTION: Immediately dispose of packaging material as it can smother small children and pets. To avoid injury, children or pets should not be allowed to play under or on the bed. Children should not operate this bed without adult supervision.

Hospital Use Disclaimer

CAUTION: This base is designed for in-home use only. It is not approved for hospital use and does not comply with hospital standards. Do not use this base with tent type oxygen therapy equipment or near explosive gases.

Pacemaker Warning

CAUTION: If the massage feature is in use, this product produces a vibrating sensation. It is possible that individuals with heart assist pacemakers may experience a sensation similar to exercise. Consult physician for complete information.

Raising/Lowering Mechanisms

The raise/lower feature will emit a minimal humming sound during operation. This is normal. During operation, the lift arm wheels make contact with the platform support of the bed. This applies slight tension on the moving components and resonance is reduced to a minimum level. If excessive noise or vibration is experienced, reverse the movement action (up or down) of the base with the remote. This should realign the base's activating mechanisms to the proper operational position.

Service Requirements

NOTE: Service technicians are not responsible for moving furniture, removing headboards and footboards or any items required to perform maintenance on the adjustable bed. In the event the technician is unable to perform service due to lack of accessibility, the service call will be billed to the purchaser and the service will have to be rescheduled.

Lubrication

This product is designed to be maintenance free. The lift motors are permanently lubricated and sealed—no additional lubrication is required. Do not apply lubricant to lift motor lead screws or any nylon nuts or the bed may inadvertently creep downward from the elevated position.

Locking Caster Safety Feature

This product is equipped with locking casters to prohibit the bed from movement. For best results, place rubber caster cups under locking casters when the bed is located on smooth or hard surface flooring. (It is possible for locking caster equipped beds to slide without the use of rubber caster cups.) To activate locking casters, push down on the lock tab. To



disengage the locking mechanism, push up on the lock tab (see illustration below).

Massage Operation

The massage feature will emit a minimal tone during operation. This is normal. When the massage level is increased, motor resonance will intensify accordingly.

Location Environment

The level of sound experienced during FlexFit™ operation is directly related to the location environment. For example, when a bed is located on a hardwood floor with the massage feature in operation, a vibrating tone will be audible. To minimize this resonance, place a piece of carpet—or optional rubber caster cups—under each leg or caster of the bed. See the Optional Accessories section on page XX of this manual for rubber caster cup order information. It is possible to experience vibration or noise from the headboard brackets, headboards or footboards if mounting bolts are not firmly tightened.

Frequently Asked Questions

Base FAQ's

- Q. What if I can't get my support beams flush with the side rails?
- A. Make sure the letter on the support beam matches the letter on the side rail. For example, the end of the support beam labeled "A" should connect to the side rail labeled "A." Additional force may be required.
- Q. How can I get my pins in all the side rails?
- A. Slide pins into side rails in the middle. Make sure that the top of the side rail is flush with the top of the support beam.
- Q. What can I do if I can't get the deck panel over the notches?
- A. First, make sure all the pins are in place. Then, push the panel inward into place.
- Q. Where is the hardware for the footboard brackets?
- A. The same hardware for attaching the legs to the base is used for attaching the brackets (sold separately).



FPO
Change from Troubleshooting,
John providing content?

Mattress FAQ's

- Q. Where are the air chamber caps? And where should I store them?
- A. The caps are in the Firmness Control™ system box. Please store these in the mattress cover at the head of the bed in case you should ever need to temporarily cap your air chamber(s).
- Q. What if my memory foam comfort layer is small or irregular?
- A. Gently shake the layer as you place it. It will recover its full size overnight.
- Q. What if I feel like I'm rolling toward the center of the mattress?
- A. Although rare, these sensations could be experienced if one side of the mattress is softer than the other side quite soft. Call Customer Service for a remedy to this situation if bothersome.
- Q. What if I notice a rubber smell from the air chamber(s)?
- A. The odor you may smell is non-toxic and will fade over time. To minimize the smell, unzip the mattress cover and allow the air chamber to air out for a few hours. Laying a couple of dryer sheets on top of the air chamber will also help mask any odor by adding a fresh scent.
- Q. Why are there body impressions on the mattress cover?
- A. For a fuller look, use your Sleep Number® 100 function. Body impressions in a normal innerspring mattress would indicate that the spring support is compressing or breaking down. The SLEEP NUMBER® bed features air, which we believe is superior in every way for comfort and support. Since air cannot break down, you receive the same support throughout the life of the bed, starting from the very first day.

FPO
Change from Troubleshooting,
John providing content?

Firmness Control™ System FAQ's

Q. Why does my Sleep Number® setting change?

- A. Your SLEEP NUMBER® setting is based on the combination of body weight, volume of air in the air chamber and sleep position. Several factors may contribute to fluctuations in your *Sleep Number* setting:
- Temperature can cause changes in your *Sleep Number* setting. For example, a heated mattress pad will cause the *Sleep Number* setting to increase.
 - Barometric pressure related to your *Sleep Number* setting to
 - Weight can affect your *Sleep Control*™ system acts similarly higher *Sleep Number* setting
 - Different sleep positions can The more concentrated the *Sleep Number* setting will be side). When weight is distributed in one air chamber, it is more likely that the *Sleep Number* setting will be lower (e.g., when you lie on your back or stomach).

Q. What do I do if the Firmness Control™ system doesn't run?


- A. Make sure the power cord is securely plugged into the Firmness Control™ system and a surge protector. Verify that the power cord is plugged into an outlet that has power and is not connected to a wall switch.

Q. I feel the mattress is losing air. What should I do?

- A. Air loss can be caused by an unsecured hose connection, a defective air chamber, or a defective Firmness Control™ system. First, make sure the hoses and hose extensions are securely connected to the air chambers. If you do not find any damaged or loose connections, identify which of the following situations matches your situation and follow the instructions for remedying your issue.

NOTE: To avoid variations in your *Sleep Number* setting or level of comfort, make sure that you are lying in your preferred sleep position when adjusting and checking your *Sleep Number* setting.

If you have a dual air chamber bed and suspect only one (1) side of your SLEEP NUMBER® bed is getting softer:

- Inspect the o-ring and connectors for cracking or damage.
- Switch the hoses on the air chambers so the left hose (marked with ) is attached to the right air chamber and the right

hose is securely connected to the left air chamber. Make sure the *Sleep Number* setting(s) of the bed.



- If you feel the level of the bed's firmness on one side of the bed over time, you may have had a problem with the hoses when the hoses were switched. If you notice the correct positions and continue to use the bed as usual.
- If an air chamber feels softer after switching hoses, contact Customer Service with the results (the issue stayed on the same side of the bed or it moved to the other side after switching hoses).

If you have a dual air chamber bed and both (2) air chambers are getting softer or you have a single air chamber bed and feel the air chamber getting softer:



Remote Control FAQ's

Q. How do I capitalize a letter in the middle of my name?

- A. Select the letter and press the Up/Down buttons   simultaneously.


Q. How many characters can I use for my name?

- A. Up to 11.

Q. My remote says there's an inflation/connectivity error. What should I do?

- A. An error message lets you know an issue has been detected, along with prompts for how to fix it. If the error is still not resolved, you will be instructed to visit sleepnumber.com/chat or to call us at 1.800.511.0054.

Q. How do I restore the remote's original settings?

- A. To erase all stored information, press the home button , select **System**, select **Setting**, select **Reset Preferences**, select **Factory Reset** and follow the instructions on the remote.





Q. Why won't my remote turn on?

- A. You may need to replace or check the orientation of the batteries. Your remote comes with two AA batteries that should last about six months with normal use. If new batteries don't resolve the issue, please visit sleepnumber.com/chat or call us at 1.800.472.7185.



Q. Why don't I see Sleep IQ™ in my menu screen?

- A. You need to have purchased the Sleep IQ™ system to have access to the Sleep IQ™ data on the remote.


Q. How do I save my Sleep Number® setting?

- A. Press the side button  to choose your side of the bed. Press the Up/Down buttons   to choose your Sleep Number setting, then press the My *Sleep Number*® setting button  on top of your remote for the two seconds to save.




Q. How do I save my customized bed positions?

- A. Adjust the bed position to your preference and hold the Favorite button  for 2 seconds to save over the bed positions. If you wish to reset the bed positions back to the original position setting, press the Home button , select **System**, select **Settings**, select **Reset Preferences**, select **Bed Positions** and follow the instructions on the remote.



Q. How do I reset my timer?

- A. Press the Timer button  and choose from the menu to adjust the timers that are set. Scroll to select a new time option or select **Timer Off**.


Q. How do I dim my under-bed nightlight?

- A. Press the Home button , then select **System**, select **Settings**, select **Reset Preferences**, select **Nightlight**, then press the Up or Down   button to adjust to your brightness preference.

Q. How do I turn my nightstand lights on or off with the remote?

- A. Press the Light button , then select the lights you want on or off and press Enter . A lightbulb icon will appear when the light selected is on and will disappear when the light is turned off.

Q. How do I change the name on my remote?

- A. Press Home , then select **System**, select **Settings**, select **Reset Preferences**, select **Rename Side** and follow the directions on the remote to enter a new name.

Welcome to Sleep Number InnerCircle[®]

Congratulations on the purchase of your SLEEP NUMBER[®] bed. As a *Sleep Number* bed owner you are now an Insider, a member of our InnerCircle.SM Soon you'll be enjoying all the benefits of a better night's sleep on your new *Sleep Number* bed.

Register Today for Insiders-Only Benefits

Go to sleepnumber.com/innercircle

Simply register your bed to start receiving exclusive discounts. Plus, you'll get access to pass-along coupons to share with friends and family, and everyone you know who could use a better night's sleep.

Receive special savings.

You'll always get 10% off every purchase. And, throughout the year, we'll send you additional Insider-exclusive offers on beds and bedding.

Earn rewards.

Improve the lives of friends and family by sharing what you love about your *Sleep Number* bed. Enjoy an exclusive Insiders reward of \$100 for referrals ONE through NINE who purchase a bed. When your 10th referral purchases, you will receive another \$699 for a total of \$1,599 in rewards.

Be the first to know.

As an Insider, you'll be the first to know about our latest innovations, from new *Sleep Number* beds to bedding solutions that will improve your sleep.



Help is just a click or phone call away.

If you ever have questions or need help finding your ideal comfort, please visit us at sleepnumber.com/chat to chat with a live representative 7 a.m. – 11 p.m. (Central Standard Time) daily or call [1.800.472.7185](tel:18004727185)

Representatives are available by phone
(Central Standard Time):

Monday-Friday	8 a.m. – 8 p.m.
Saturday	8:30 a.m. – 5 p.m.
Sunday	Closed



9800 59th Avenue North, Minneapolis, MN 55442



©2013 Select Comfort 7/13