

Instruction Guide



SpectraPen mini Software

Please read the Guide before operating this product



Manual Version: 2022/01

© PSI (Photon Systems Instruments), spol. s r.o.

www.psi.cz

This document and its parts can be copied or provided to a third party only with the express permission of PSI.

The contents of this manual have been verified to correspond to the specifications of the device. However, deviations cannot be ruled out. Therefore, a complete correspondence between the manual and the real device cannot be guaranteed. The information in this manual is regularly checked, and corrections may be made in subsequent versions.

The visualizations shown in this manual are only illustrative.

This manual is an integral part of the purchase and delivery of equipment and its accessories and both Parties must abide by it.

TABLE OF CONTENT

1	Software installation	4
2	Data transfer	4
3	Software menu	6
4	Data visualization.....	7
5	Troubleshooting and Customer Support	12
6	Appendix	12
6.1	Programming custom index in SpectraPen	12
6.1.1	Function description	13

1 SOFTWARE INSTALLATION

1. Download the SpectraPen software from PSI website <https://handheld.psi.cz/products/spectrapen-mini/#download> to your computer and launches the SpectraPen program.
2. To activate all software features register the SpectraPen software as follows (Fig. 1).
 - Select: Help > **Register**
 - Enter serial registration number, which is available in download section on PSI website
 - Select: OK

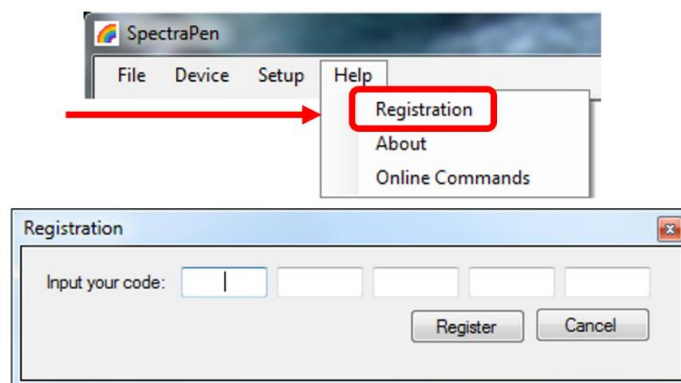


Fig. 1 Software registration.



It is not possible to download data from the SpectraPen device without software registration.

2 DATA TRANSFER

For data transfer from mobile application to your computer select **Share** and choose your preferred option (Fig. 2).

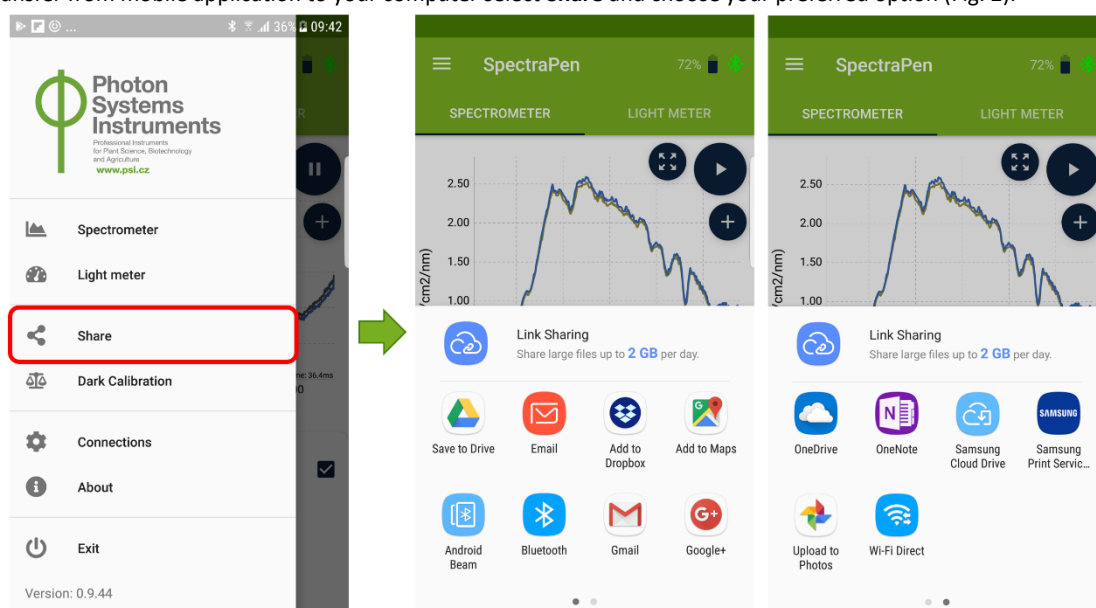


Fig. 2 Data export and sharing via available communication channels.



It is not possible to download data from the SpectraPen device without software registration.

Open your data in .spec format using the SpectraPen software (Fig. 3).


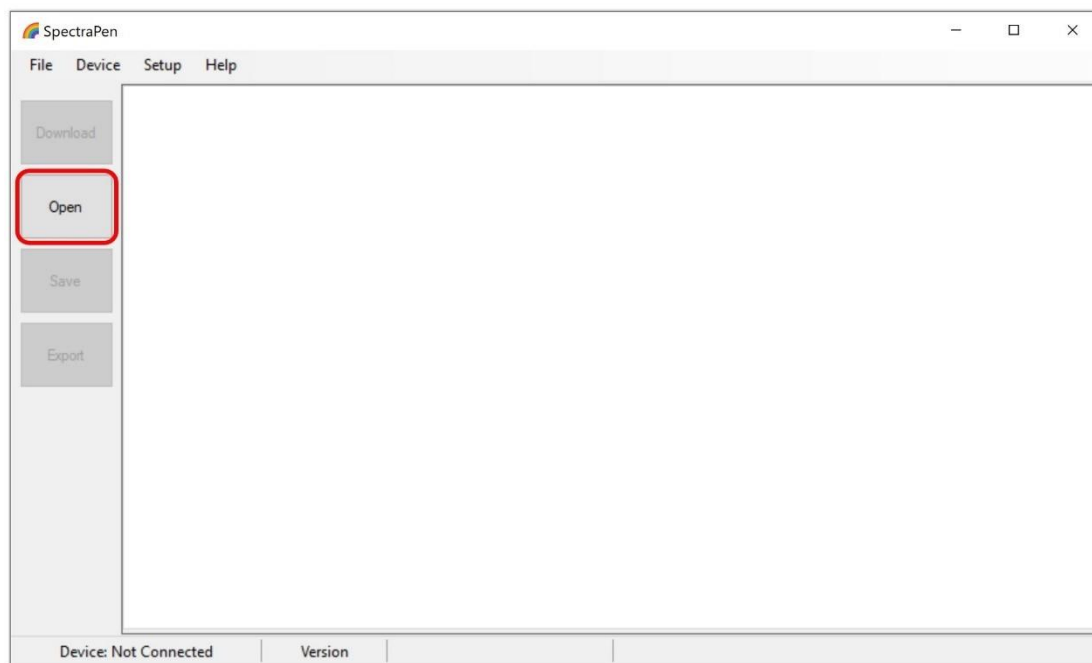


Fig. 3 Opening data in SpectraPen software.

3 SOFTWARE MENU


MENU: File

Load	Loads previously saved data files.
Save	Saves data to hard disc.
Export	Exports data in .txt format.
Export to JSON	Exports data in JavaScript Object Notation.
Close	Closes the current experiment.
Close All	Closes all open experiments.
Exit	Exits the program.

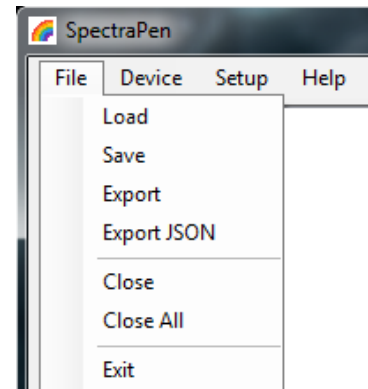


MENU: Device – NOT ACTIVE FOR SP mini

Connect	Detects and connects the device.
Update Firmware	Used for firmware updates.
Attach GPS File	Used to download data from the GPS module of the old versions of the SpectraPen or PolyPen.
Memory Erase	Erases data from the memory of connected device.
Online Control	Online control of the device.

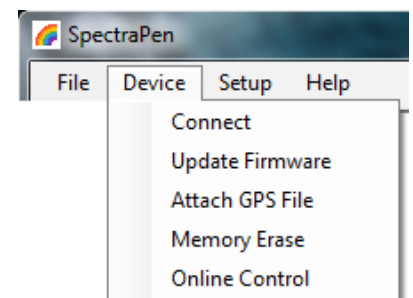


MENU: Setup

Update Software	Used for software updates.
Settings	On/off – Auto memory erase after download. Selection of separator for the csv file after its export and following opening in Excel (TAB, SEMICOLON, COMMA, SPACE).

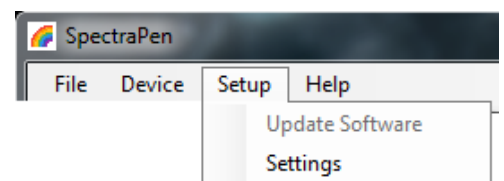

MENU: Help

Registration	Used for the SpectraPen software registration.
About	Offers basic information about the program.

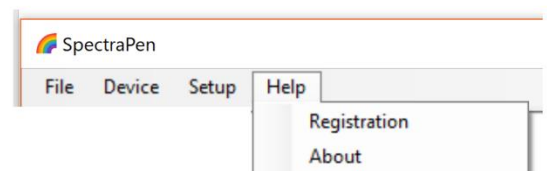

4 DATA VISUALIZATION

1. Visualization modes: **Scope** mode window is always displayed as the default. To view irradiance data go to **Irradiance** tab (Fig. 4).

	Scope mode represents non-calibrated spectrum.
---	--

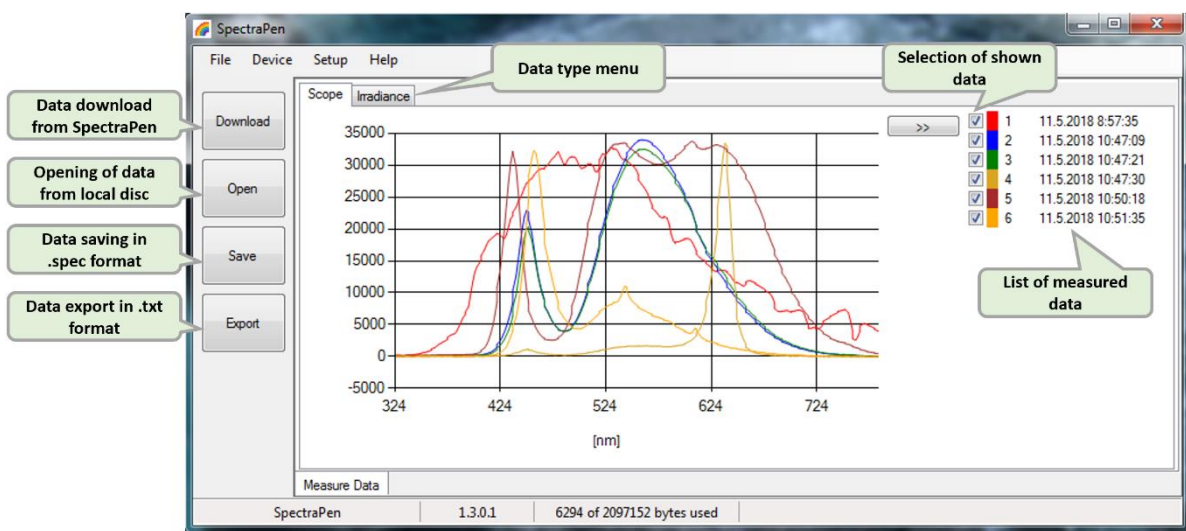


Fig. 4 Scope spectra.

2. All data that are downloaded are displayed in the Scope window after download from the SpectraPen. The user can select the set of measurements to be displayed by marking and unmarking the data from the **selection** list (Fig. 4).
3. Right click on list of measured data enables **edit data name**, **delete** selected measurement or **show and hide** all measured data in the graph– Select all measure and Clear all measure (Fig. 5).

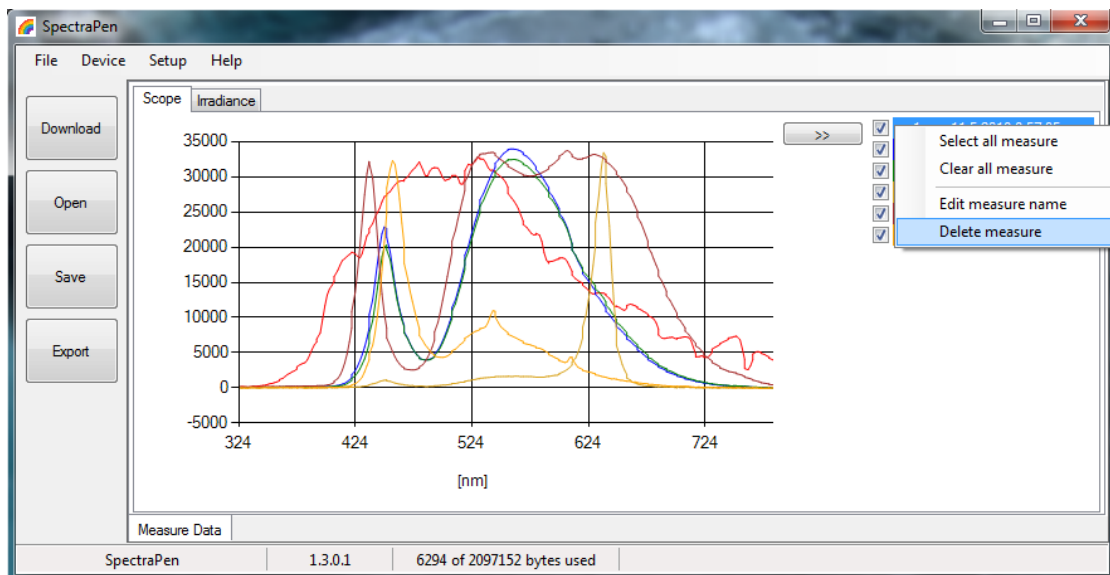


Fig. 5 Options for list of data.

- In the graph **marker** feature is available, which enables display of the numeric values for wavelength and light irradiance for the selected wavelength of the scan (Fig. 6). Use the mouse to select the given point. In top right corner of the graph (red rectangle) is displayed exact value for the selected point on the x-axis and y-axis.

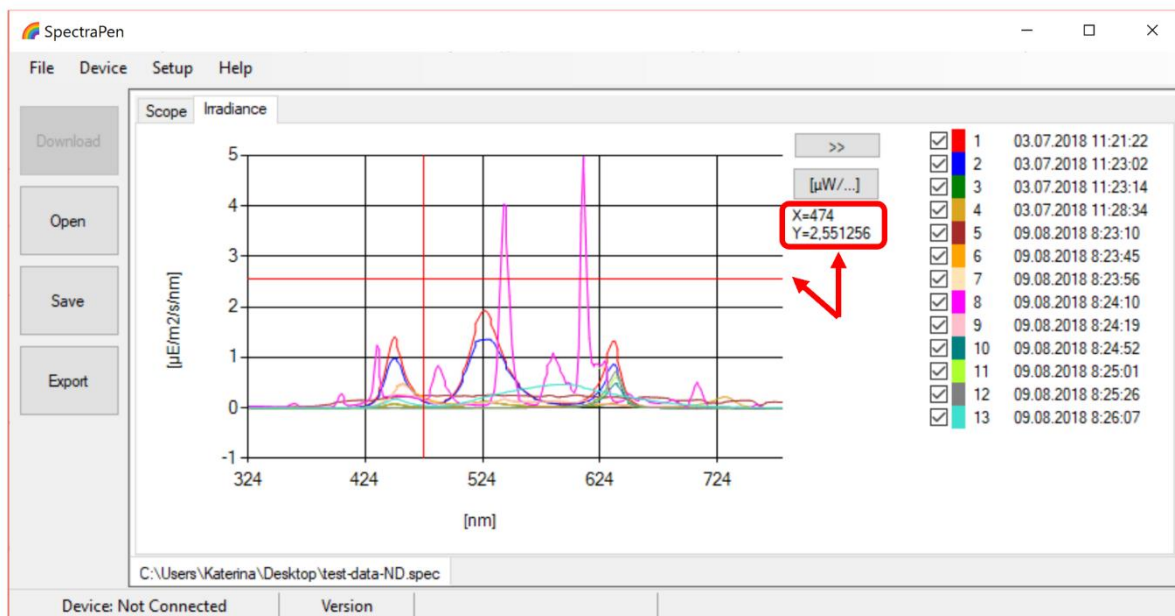


Fig. 6 Marker feature.

- To **zoom in on the data displayed in the graph** select an area of the displayed graph (Fig. 7). To reverse these steps and return to original display use minus icon in the corners of the zoom area marked with red rectangles in Fig. 7.

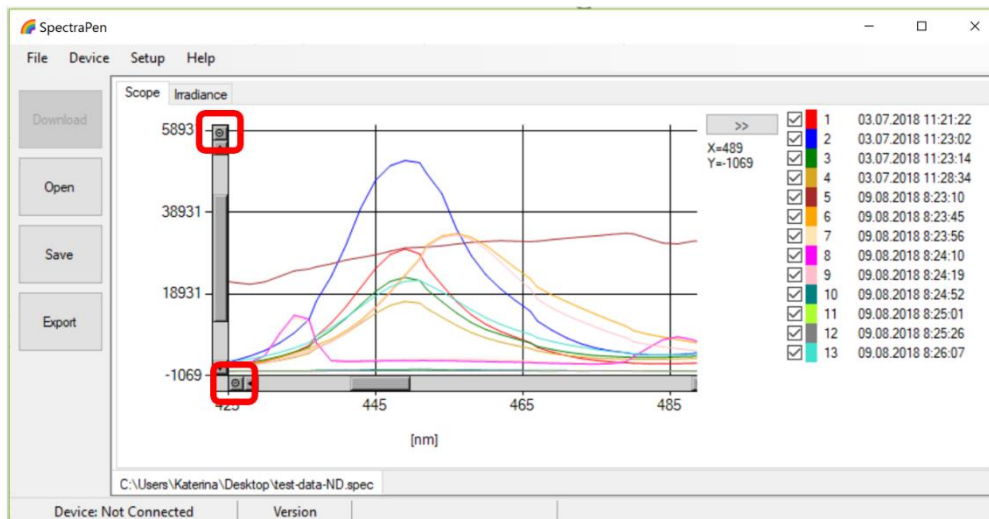


Fig. 7 Zoom function.

6. Select **Irradiance** tab to view the irradiance data stored either as $\mu\text{mol}/\text{m}^2/\text{s}/\text{nm}$ or per $\mu\text{Watts}/\text{cm}^2/\text{nm}$. To change the units in which the spectra is displayed click on the unit icon as shown in (Fig. 8).
7. To view the light meter data for the spectral scans acquired click on the unit icon as depicted by red arrow in Fig. 8. Irradiance and illuminance **light meter numerical values** for each scan are displayed as LUX, PAR or IRRADIANCE values (Fig. 9).

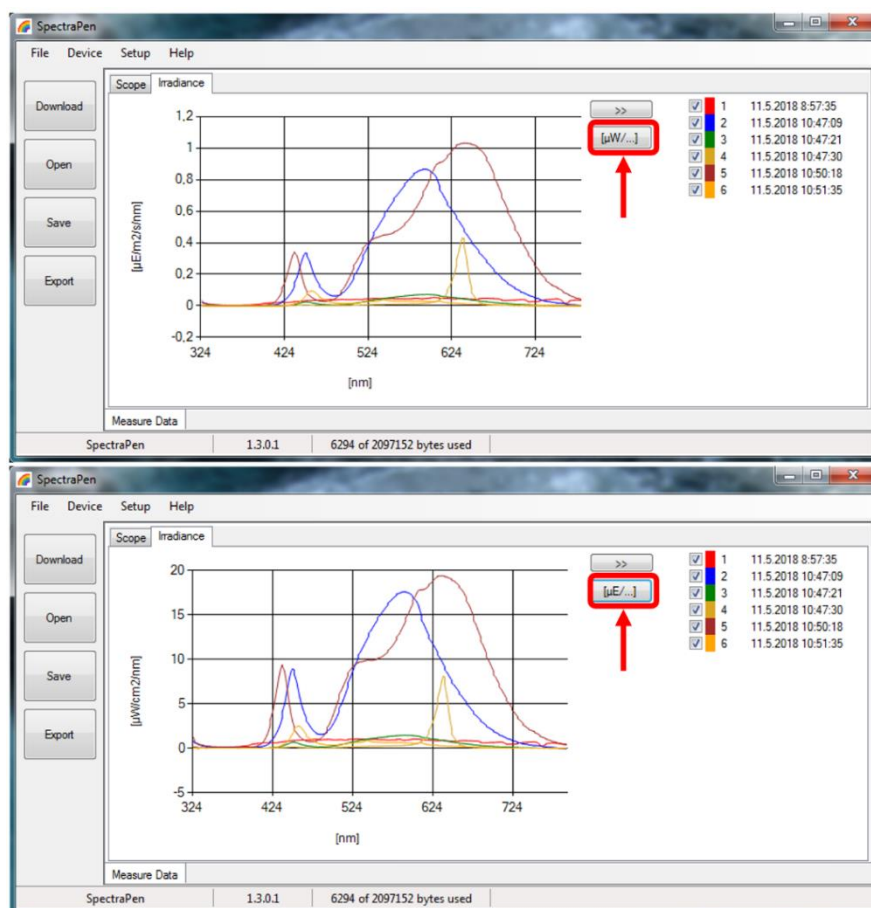


Fig. 8 Irradiance shown in different units.

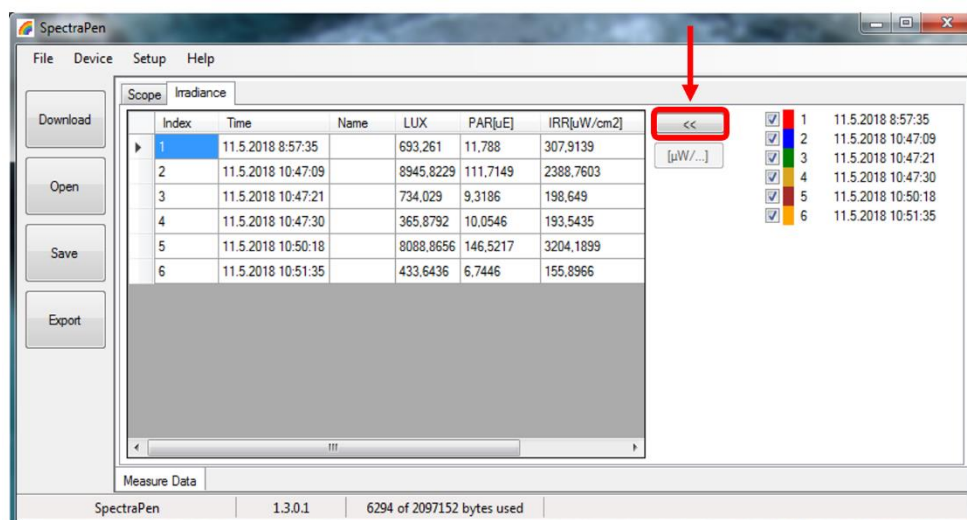


Fig. 9 Numerical values of measured light intensities.

8. To Save the experiment select **File>Save**. All data stored in the device memory will be saved irrespective of the data selection in the SpectraPen software. The file will be stored as .spec. Spec files stores all Scope and Light meter data.
9. Select **File>Export** to export the data in .txt format. Export function allows the user to specify the type of data. The options are:
Spectrum (Fig. 10) – all raw scope data for entire range of measured wavelengths are exported including data for the dark scan.
Spectrum scope – scope data normalized to dark spectrum scan are exported for all acquired scans or set of selected measurements.

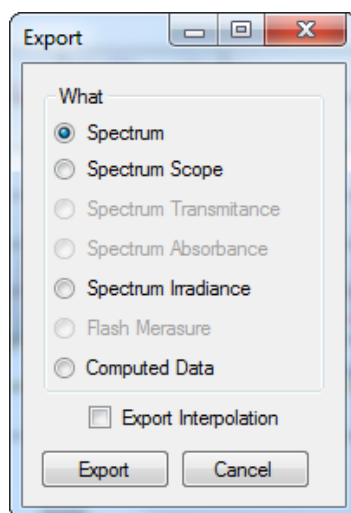


Fig. 10 Export options.

Spectrum Irradiance – irradiance data for all measurements are exported. The user can choose to export the numeric values either in $\mu\text{E}/\text{m}^2/\text{s}/\text{nm}$, $\mu\text{W}/\text{cm}^2/\text{nm}$ or both (Fig. 11).

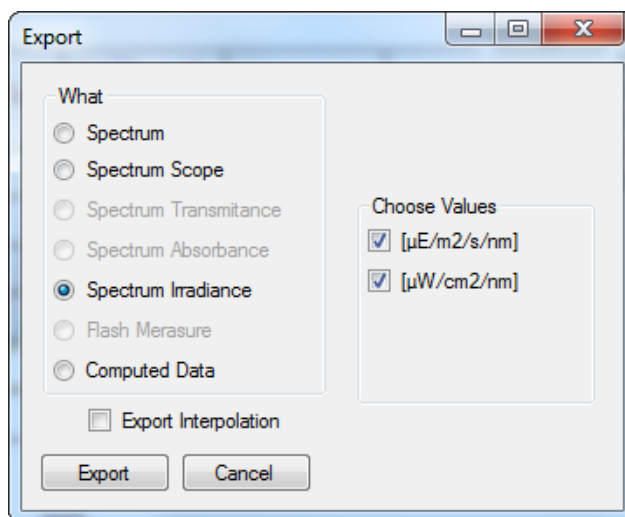


Fig. 11 Export of Irradiance spectrum.

Computed Data – computed numeric values for Scope and Irradiance are exported for all measurements. The user can choose if only Scope numeric values or Irradiance numeric values are exported. For irradiance values, numeric data for Photon flux density and PAR in $\mu\text{mol}/\text{m}^2/\text{s}$ units, irradiance in $\mu\text{W}/\text{cm}^2$ units and illuminance in LUX units are exported (Fig. 12).

Export interpolation – if this option is marked the spectrum is exported with step of 1 nm.

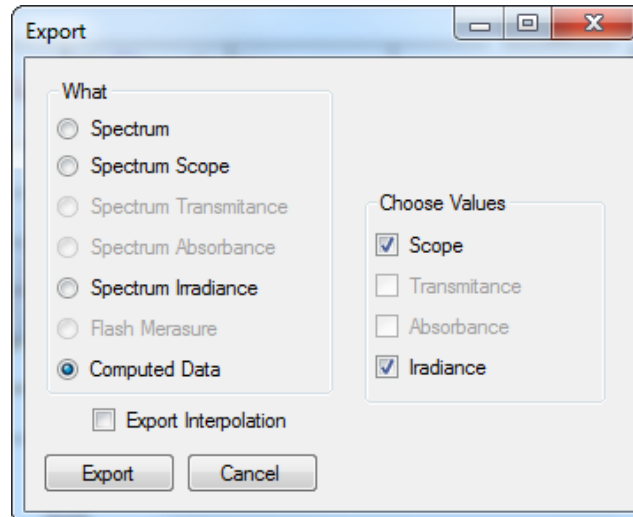


Fig. 12 Export of computed values.

5 TROUBLESHOOTING AND CUSTOMER SUPPORT

In case of problems with the SpectraPen SW visit **FAQ** on our websites (<http://psi.cz/support/faq>) or contact customer support by email to support@psi.cz, or contact your local distributor.

6 APPENDIX

6.1 PROGRAMMING CUSTOM INDEX IN SPECTRAPEN

The SpectraPen software enables programming custom indexes, which can be used for wide range of calculation based on the measured spectrum.

1. Go to the main **SpectraPen folder** in your PC (Usually in Program Files).
2. Open the file **Config > Formulas.txt**.
3. Write your index into this .txt file and save it (Fig. 13).

Index example:

Scope:PSIindex:PSI test index:Scope[600nm]/ Scope[500nm]

Scope – the index is placed in the bookmark Scope in data in the software

PSIindex – name of the index in the SpectraPen software and in exported data

PSI test index – full name of the index (not showed)

Scope[600nm]/ Scope[500nm] – equation for calculation; calculated from 500 and 600 nm of Scope spectra



```
Soubor Úpravy Formát Zobrazení Nápověda
Transmittance:NDVI:Normalized Difference Vegetation Index:(Transmittance[780nm]-Transmittance[630nm])/(Transmittance[780nm]+Transmittance[630nm])
Transmittance:SR:Simple Ratio Index:Transmittance[780nm]/Transmittance[630nm]
Transmittance:MCARI1:Modified Chlorophyll Absorption Ratio Index 1:1.2*(2.5*(Transmittance[780nm]-Transmittance[670nm]))-1.3*(Transmittance[780nm]-Transmittance[550nm]))
Transmittance:OSAVI:Optimized Soil-Adjusted Vegetation Index:(1+0.16)*(Transmittance[780nm]-Transmittance[670nm])/(Transmittance[780nm]+Transmittance[670nm]+0.16)
Transmittance:G:Greenness Index:Transmittance[554nm]/Transmittance[677nm]
Transmittance:MCARI2:Modified Chlorophyll Absorption Ratio Index:((Transmittance[780nm]-Transmittance[670nm])-0.2*(Transmittance[780nm]-Transmittance[550nm]))*(Transmittance[780nm]/Transmittance[670nm])
Transmittance:TCARI:Transformed CAR Index:3*((Transmittance[780nm]-Transmittance[670nm]))-0.2*(Transmittance[780nm]+Transmittance[550nm]))*(Transmittance[780nm]/Transmittance[670nm])
Transmittance:TVI:Triangular Vegetation Index:0.5*(120*(Transmittance[750nm]-Transmittance[550nm]))-200*(Transmittance[670nm]-Transmittance[550nm]))
Transmittance:ZMI:Zarco-Tejada & Miller Index:Transmittance[750nm]/Transmittance[710nm]
Transmittance:SPRI:Simple Ratio Pigment Index:Transmittance[430nm]/Transmittance[680nm]
Transmittance:NPQI:Normalized Phaeophytinization Index:(Transmittance[415nm]-Transmittance[435nm])/(Transmittance[415nm]+Transmittance[435nm])
Transmittance:PRI:Photochemical Reflectance Index:(Transmittance[531nm]-Transmittance[570nm])/(Transmittance[531nm]+Transmittance[570nm])
Transmittance:NPQI:Normalized Pigment Chlorophyll Index:(Transmittance[680nm]-Transmittance[430nm])/(Transmittance[680nm]+Transmittance[430nm])
Transmittance:Ctr1:Carter Indices 1:Transmittance[695nm]/Transmittance[420nm]
Transmittance:Ctr2:Carter Indices 2:Transmittance[695nm]/Transmittance[760nm]
Transmittance:Lic1:Lichtenthaler Indices 1:(Transmittance[780nm]-Transmittance[680nm])/(Transmittance[780nm]+Transmittance[680nm])
Transmittance:Lic2:Lichtenthaler Indices 2:Transmittance[440nm]/Transmittance[690nm]
Transmittance:SIP1:Structure Intensive Pigment Index:(Transmittance[780nm]-Transmittance[450nm])/(Transmittance[780nm]+Transmittance[650nm])
Transmittance:GMI:Gitelson and Merzlyak Indices 1:Transmittance[750nm]/Transmittance[550nm]
Transmittance:GMI2:Gitelson and Merzlyak Indices 2:Transmittance[750nm]/Transmittance[700nm]
Transmittance:ARI1:Anthocyanin Reflectance Index 1:1/Transmittance[550nm]-1/Transmittance[700nm]
Transmittance:ARI2:Anthocyanin Reflectance Index 2:Transmittance[790nm]*(1/Transmittance[550nm]-1/Transmittance[700nm])
Transmittance:CRI1:Carotenoid Reflectance Index 1:1/Transmittance[510nm]-1/Transmittance[550nm]
Transmittance:CRI2:Carotenoid Reflectance Index 2:1/Transmittance[510nm]-1/Transmittance[700nm]
Transmittance:RDVI:Renormalized Difference Vegetation Index:(Transmittance[780nm]-Transmittance[670nm])/((Transmittance[780nm]+Transmittance[670nm])^0.5)
Irradiance:LUX:LUX:683*integral(IrradianceE,360nm,780nm)
Irradiance:PAR[uE]:PAR[uE]:integral(IrradianceE,400nm,700nm)
Irradiance:IRR[uW/cm2]:Irradiance[uW/cm2]:integral(IrradianceW,340nm,780nm)
Transmittance:TBR_N10(uW/cm2):Transmittance[uW/cm2]:integral(IrradianceW,640nm,1050nm)
Scope:PSIindex:PSI test index:Scope[600nm]/ Scope[500nm]
```

Fig. 13 New index in the Formulas file.

4. Restart the SpectraPen Software.
5. The new index appears in the selected bookmark in the data (Fig. 14).
6. For export of this index choose the option “Computed values” and selected spectrum in the export table.

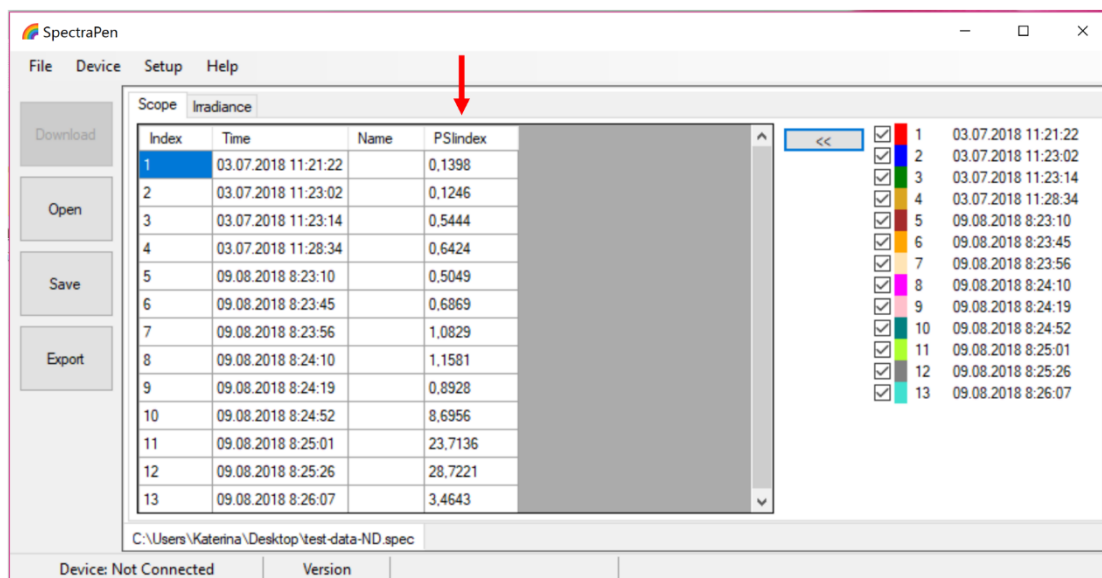


Fig. 14 New index.

6.1.1 FUNCTION DESCRIPTION

Different mathematical functions can be used in SpectraPen software syntax to create new custom formulas.

min, max -

`min(value1, value2)`

value1 - number, variable, function

value2 – number, variable, function

- only one value can be function!

`min(array)`

array – array of numbers

example1: `max(Scope)`

example2: `min(Irradiance)`

example3: `min(Scope[760nm], max(Scope[450], Scope[680]))`

example4: `max(Irradiance[550nm], (5+4)*4)`

ln – the natural (base e) logarithm of specified number

`ln(value)`

value – number, variable, function

example1: `ln(5)`

example2: `ln(Irradiance[760nm])`

example3: $\ln(\max(\text{Irradiance}[550\text{nm}], \text{Irradiance}[480\text{nm}])))$

example4: $\ln((5+4)*4)$

log – the logarithm of specified number in a specified base.

$\log_B(\text{value})$

B – base - number

value – number, variable, function

example1: $\log_2(5)$

example2: $\log_5(\text{Scope}[760\text{nm}])$

example3: $\log_{10}(\max(\text{Scope}[550\text{nm}], \text{Scope}[480\text{nm}])))$

example4: $\log_{10}((5+4)*4)$

sqrt – the square root of a specified number

$\text{sqrt}(\text{value})$

value – number, variable, function

example1: $\text{sqrt}(5)$

example2: $\text{sqrt}(\text{Scope}[760\text{nm}])$

example3: $\text{sqrt}(\max(\text{Scope}[550\text{nm}], \text{Scope}[480\text{nm}])))$

example4: $\text{sqrt}(((5+4)*4) + 6)$

^ - specified number raised to the specified power

$\text{value}^{\text{power}}$

value – number, variable, function

power – number, variable, function

example1: $\text{Irradiance}[760\text{nm}]^{\text{Irradiance}[550\text{nm}]}$

example2: $\min(\text{Irradiance}[760\text{nm}], \text{Irradiance}[550\text{nm}])^{\max(\text{Irradiance}[435\text{nm}], \text{Irradiance}[430\text{nm}])}$

example3: $\text{Transmittance}[760\text{nm}]^{0.5}$

integral - express the area under the curve of a graph of the function in the interval

$\text{integral}(\text{function_values}, \text{from}, \text{to})$

function_values – input values for integral compute

from,to – limit values

example1: `integral(IrradianceL, 360nm, 700nm)`

example2: `integral(IrradianceE, 360nm, 700nm) * IrradianceE[450]`