



# TRANSFER SETTINGS

## MiniMed™ 670G Replacement Pump

**STEP 1:** Before you send your original pump back, copy your current settings onto the Insulin Pump Settings Form. If for any reason you cannot copy the settings, please contact your healthcare professional or reference your CareLink™ Personal reports.

**STEP 2:** Insert a AA battery into your new pump. You can use either a lithium, alkaline or rechargeable battery.

**STEP 3:** Follow the instructions found in this guide to enter the settings that you have recorded on the Insulin Pump Settings Form into your new pump. For additional information on your pump, please consult the User Guide.

We recommend that you record all settings on this form to refer to as you enter them into new pump.

**DELIVERY SETTINGS**

**BOLUS WIZARD SETUP**

Menu > Options > Delivery Settings > Bolus Estimate Setup

Bolus Wizard:  On  Off

**Carb Ratio:**

12:00 A \_\_\_\_\_ - \_\_\_\_\_ g/U  
 \_\_\_\_\_ - \_\_\_\_\_ g/U  
 \_\_\_\_\_ - \_\_\_\_\_ g/U

**Insulin Sensitivity Factor:**

12:00 A \_\_\_\_\_ - \_\_\_\_\_ mg/dL per U  
 \_\_\_\_\_ - \_\_\_\_\_ mg/dL per U  
 \_\_\_\_\_ - \_\_\_\_\_ mg/dL per U

**BG Target:**

12:00 A \_\_\_\_\_ - \_\_\_\_\_ mg/dL  
 \_\_\_\_\_ - \_\_\_\_\_ mg/dL  
 \_\_\_\_\_ - \_\_\_\_\_ mg/dL

Active Insulin Time: \_\_\_\_\_ hr

**BASAL PATTERN SETUP**

Menu > Basal > Delivery Settings > Basal Pattern Setup

Basal 1: \_\_\_\_\_ Basal Pattern Name: \_\_\_\_\_  
 12:00 A \_\_\_\_\_ U/hr 12:00 A \_\_\_\_\_ U/hr  
 \_\_\_\_\_ U/hr \_\_\_\_\_ U/hr  
 \_\_\_\_\_ U/hr \_\_\_\_\_ U/hr

**PRESET TEMP SETUP**

Menu > Options > Delivery Settings > Preset Temp Setup

Preset Temp Name: \_\_\_\_\_  
 Type \_\_\_\_\_ Percent \_\_\_\_\_ % Duration \_\_\_\_\_ hr

**DUAL/SQUARE WAVE:**

Menu > Options > Delivery Settings > Dual/Square Wave

Dual:  On  Off Square:  On  Off

**PRESET BOLUS SETUP**

Menu > Options > Delivery Settings > Preset Bolus Setup

Preset Bolus Name: \_\_\_\_\_  
 Bolus: \_\_\_\_\_ U Type: \_\_\_\_\_  
 % \_\_\_\_\_ Now \_\_\_\_\_ Square Duration \_\_\_\_\_ hr

**DELIVERY SETTINGS (CONT.)**

**BOLUS INCREMENT:**

Menu > Options > Delivery Settings > Bolus Increment

0.025U  0.05U  0.1U

**MAX BASAL/BOLUS:**

Menu > Options > Delivery Settings > Max Basal/Bolus

Max Basal: \_\_\_\_\_ U/hr Max Bolus: \_\_\_\_\_ U

**EASY BOLUS:**

Menu > Options > Delivery Settings > Easy Bolus

On  Off Step Size \_\_\_\_\_ U

**AUTO SUSPEND:**

Menu > Options > Delivery Settings > Auto Suspend

On \_\_\_\_\_ hr  Off

**BOLUS SPEED:**

Menu > Options > Delivery Settings > Bolus Speed

Standard  Quick

**UTILITIES**

**TURN SENSOR ON:**

Menu > Options > Utilities > Sensor Settings

Sensor:  On  Off

**DISPLAY OPTIONS:**

Menu > Options > Utilities

Brightness \_\_\_\_\_  Auto Backlight \_\_\_\_\_ sec / min

**DEVICE OPTIONS:**

S/N: \_\_\_\_\_  
 S/N: \_\_\_\_\_  
 S/N: \_\_\_\_\_

**AUTO MODE:**

Menu > Options > SmartGuard

Auto Mode:  On  Off

Auto Mode BG alert:  On  Off

**SENSOR SETTINGS: HIGH SETUP** Menu > Options > SmartGuard > High Setup

High Limit	Alert before high	Time before high	Alert on high	Rise Alert	Rise Limit*
12:00 A - _____ mg/dL	<input type="checkbox"/> On	_____ min	<input type="checkbox"/> On	<input type="checkbox"/> On	Custom _____ mg/dL/min or ↑   ↑↑   ↑↑↑
_____ - _____ mg/dL	<input type="checkbox"/> On	_____ min	<input type="checkbox"/> On	<input type="checkbox"/> On	Custom _____ mg/dL/min or ↑   ↑↑   ↑↑↑
_____ - _____ mg/dL	<input type="checkbox"/> On	_____ min	<input type="checkbox"/> On	<input type="checkbox"/> On	Custom _____ mg/dL/min or ↑   ↑↑   ↑↑↑

**SNOOZE** Menu > Options > SmartGuard > Snooze High Snooze: \_\_\_\_\_ hr

**SENSOR SETTINGS: LOW SETTINGS** Menu > Options > SmartGuard > Low Setup

Low Limit	Alert before low	Alert on low	Suspend before low	Suspend on low	Resume basal alert**
12:00 A - _____ mg/dL	<input type="checkbox"/> On	<input type="checkbox"/> On	<input type="checkbox"/> On	<input type="checkbox"/> On	<input type="checkbox"/> On
_____ - _____ mg/dL	<input type="checkbox"/> On	<input type="checkbox"/> On	<input type="checkbox"/> On	<input type="checkbox"/> On	<input type="checkbox"/> On
_____ - _____ mg/dL	<input type="checkbox"/> On	<input type="checkbox"/> On	<input type="checkbox"/> On	<input type="checkbox"/> On	<input type="checkbox"/> On

**SNOOZE** Menu > Options > SmartGuard > Snooze Low Snooze: \_\_\_\_\_ hr


\*Option only available when Rise Alert is on

\*\*Option only available when Suspend on low or Suspend before low is on

## STARTUP WIZARD

Once you've inserted the battery, the pump powers up and the **Startup Wizard** begins, it will guide you through setting language, time format, and current time and date.


1. Select **English**.
2. When the **Select Time Format** screen appears, select a **12 Hour** or a **24 Hour** time format.
3. When **Enter Time** screen appears, the hour will be flashing. Press **^** or **v** to the correct hour and press **O**.
4. The minutes will be flashing. Press **^** or **v** to the correct minutes and press **O**.
5. The **AM / PM** will be flashing. Press **^** or **v** if needed and press **O**. Select **Next**.
6. When the **Enter Date** screen appears, select **Year**. Press **^** or **v** to correct year and press **O**. Repeat this step for setting **Month** and **Day**. Select **Next**.
7. The rewinding screen will briefly appear, followed by a confirmation message. Select **Ok**.

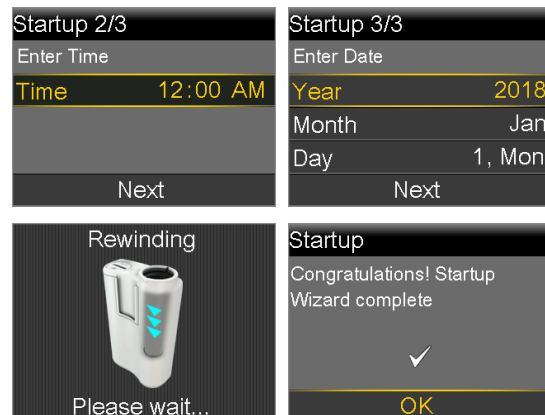

## SETTING MAX BASAL

*Menu > Options > Delivery Settings*


1. Select **Max Basal/Bolus** and press **O**.
2. Select **Max Basal** to enter the **U/hr** amount. Use **^** and **v** to set the **Max Basal** amount. Press **O**.
3. Select **Save**.

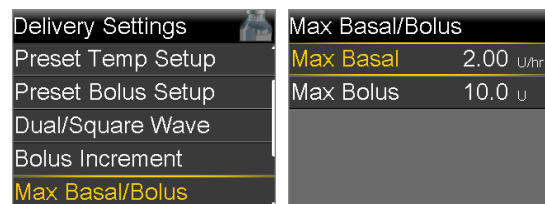

## SETTING MAX BOLUS

*Menu > Options > Delivery Settings*


1. Select **Max Basal/Bolus** and press **O**.
2. Select **Max Bolus** to enter the **U/hr** amount. Use **^** and **v** to set the **Max Bolus** amount. Press **O**.
3. Select **Save**.

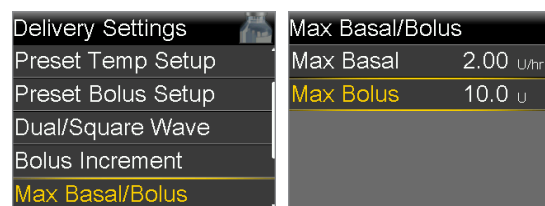

## SETTING BASAL PATTERN

*Menu > Basal > Delivery Settings > Basal Pattern Setup*

1. Select **Basal 1**.
2. Select **Options**, then select **Edit**.
3. Press **O** to enter **End** time. Press **O** to leave the **End** time at **12:00A**. If you are setting multiple rates use **^** or **v** to change the **End** time and press **O**.
4. Press **^** to enter **U/hr** and press **O**.
5. Continue adding **End** times and basal rates as needed, otherwise select **Done**.
6. Review the basal rates, if you need to correct, press **↩** to go back to edit mode. If Basal rates are correct select **Save**.


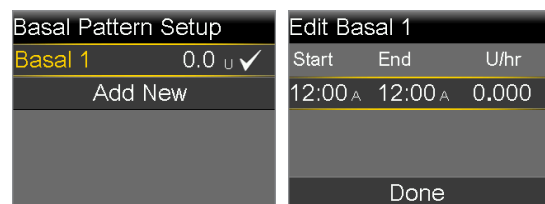


## TURN BOLUS WIZARD ON AND SETUP

### Menu > Options > Delivery Settings > Bolus Estimate Setup

1. Select **Bolus Wizard** to turn **On**.
2. Press **▼** to see the rest of the message then select **Next**.
3. Review the description of **Carb Ratio** and select **Next**.
4. Press **○** to enter **End** time. Press **○** again to leave the **End** time at **12:00A**. If you are setting multiple Carb Ratios use **▲** or **▼** to change the **End** time, then press **○**.
5. Press **▲** or **▼** to enter g/U then press **○**.  
Continue adding **End** times and **Carb Ratios** as needed.
6. Select **Next** when done.
7. Review the description of **Sensitivity Factor** and select **Next**.
8. Press **○** to enter **End** time. Press **○** again to leave the **End** time at **12:00A**. If you are setting multiple **Sensitivity Factors**, use **▲** or **▼** to change the **End** time, then press **○**.
9. Press **▲** or **▼** to enter **mg/dL per U**, then press **○**.  
Continue adding **End** times and **Sensitivity Factors** as needed.
10. Select **Next** when done.
11. Review the description of **BG Target** and select **Next**.
12. Press **○** to enter **End** time. Press **○** again to leave the **End** time at **12:00A**. If you are setting multiple **BG Targets**, use **▲** or **▼** to change the **End** time, then press **○**.
13. Press **▲** or **▼** to enter **Lo** and then press **○**.
14. Press **▲** or **▼** to enter **Hi** and then press **○**.  
Continue adding **End** times and **BG Targets** as needed.
15. Select **Next** when done.
16. Review the description of **Active Insulin Time** and select **Next**.
17. Press **○** to enter **Duration** time.
18. Press **▲** or **▼** to enter **hr** then press **○**.
19. Select **Save**.

The **Bolus Wizard** setup is now complete.

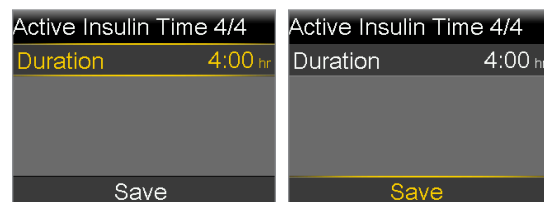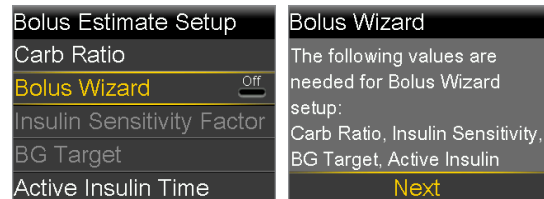


**Note:** The settings shown are for illustration purposes only — your settings may be different.

## TURN SENSOR ON

*Menu > Options > Utilities > Sensor Settings*

1. Select **Sensor** to turn feature **On**.

You can now access the **SmartGuard** menu and enter the settings.

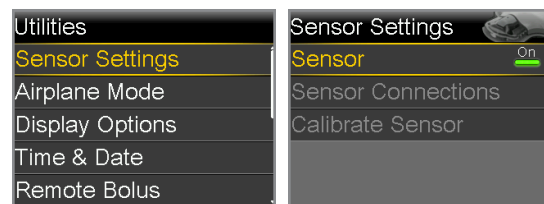

## SETTING UP HIGH SETTINGS

*Menu > Options > SmartGuard*

1. Select **High Setup**.
2. Press **○** on the time segment. Press **○** again to leave the **End** time at **12:00A**. If setting multiple time segments, press **▲** to enter **End** time of first segment, and press **○**.
3. Press **▲** or **▼** to set **Hi** limit and press **○**. Press **○** to continue.
4. Select each feature you wish to turn on. If a feature is on, select it again to turn it back off.
5. Once settings are selected, select **Next** and then select **Done**.
6. Verify that settings are correct and select **Save**.
7. If snooze time needs to be changed, press **▼** to **Snooze** and press **○**.

Select **High Snooze**. Press **▲** or **▼** to enter the correct time and press **○**. Select **Save**.

Your **High Setup** is now complete.




## SETTING UP LOW SETTINGS

*Menu > Options > SmartGuard*

1. Select **Low Setup**.
2. Press **○** on the time segment. Press **○** again to leave the **End** time at **12:00A**. If setting multiple time segments, press **▲** to enter **End** time of first segment, and press **○**.
3. Press **▲** or **▼** to set **Lo** limit and press **○**. Press **○** to continue.
4. Select each feature you wish to turn on. If a feature is on, select it again to turn it back off.
5. Once settings are selected, select **Next** and then select **Done**.
6. Verify that settings are correct and select **Save**.
7. If snooze time needs to be changed, press **▼** to **Snooze** and press **○**.

Select **Low Snooze**. Press **▲** or **▼** to the correct time and press **○**. Select **Save**.

Your **Low Setup** is now complete.

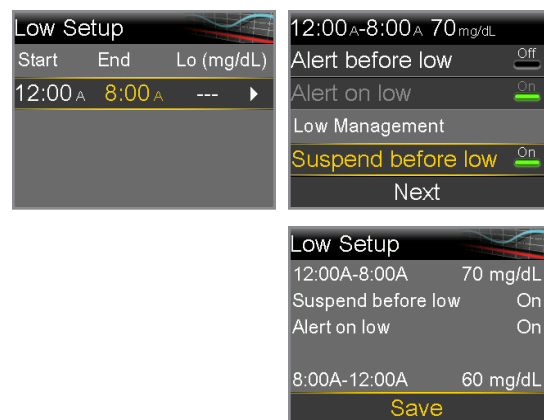


*Turn to page 5 to continue setting sensor settings*

## TURN AUTO MODE ON

*Menu > Options > SmartGuard*

1. Select **Auto Mode**.
2. Select **Auto Mode** again to turn feature **On**.
3. Check the screen to make sure that Auto Mode is set to **On**.  
Select **Save**.

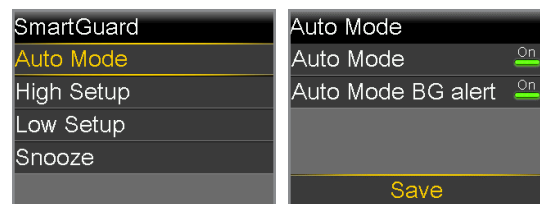

## CONNECT THE TRANSMITTER

*Menu > Options > Utilities > Device Options > Connect Device > Auto Connect*

1. Press **▼** to read the rest of the message and then press **▶** and select **Continue**.
2. *Make sure the transmitter is fully charged and remove it from the charger.*
3. Select **Search** on the pump.
4. Confirm that the **SN** (serial number) on the pump screen matches the **SN** on the transmitter.
5. If they match, select **Confirm**.

*The **Manage Devices** screen will appear with the **SN**. Your transmitter and pump are now connected.*



Please take some time to review ALL your entries and ensure they are correct.

## In Need of Technical Assistance?

Our **24-Hour HelpLine** is here to help.

**Call 1.800.646.4633**

For medical advice, call your Healthcare Team.

**Note:** *If you turn Auto Mode on before the 48 hour warm up is complete, you may receive an alert at midnight to Enter a BG for Auto Mode. You may want to wait until day 3 of your pump wear to avoid this alert at midnight.*