

Calibration certificates RISE equipment used for test report 2P03617

	Serial number on equipment	RISE number	File name/ Page number
R&S FSW 43	100 560	902 073	902 073 FSW43.pdf
R&S ESU 26	100 409	901 553	901 553 ESU26.pdf
R&S ZNB 40	101 544	BX50051	BX50051 ZNB40.pdf
Bilog antenna Schaffner 6143A	23 169	504 079	2 – 9
EMCO Horn Antenna 3115	9509-4562	502 175	10 – 14
EMCO Horn Antenna 3115	00143 161	902 212	15 – 19
EMCO Horn Antenna 3116	9904-2426	503 279	20 – 24
Mixer FS-Z60	100 996	BX90566	25 – 31
Mixer FS-Z90	101 871	BX90567	32 – 38
Mixer FS-Z110	101 467	BX81425	39 – 48
Mixer FS-Z170	100 974	BX81426	49 – 55
Mixer FS-Z220	100 967	BX81427	56 – 62
Flann STD Gain Horn Antenna 20240-20	Manufacturer provided gain 407	BX92412	63
Flann STD Gain Horn Antenna 22240-20	Manufacturer provided gain 258 660	BX92413	64
Flann STD Gain Horn Antenna 24240-20	Manufacturer provided gain 141	BX92414	65
Flann STD Gain Horn Antenna 26240-20	Manufacturer provided gain 124 440	BX92416	66
Flann STD Gain Horn Antenna 27240-20	Manufacturer provided gain 281	BX92417	67
Flann STD Gain Horn Antenna 29240-20	Manufacturer provided gain 46	BX92419	68
Flann STD Gain Horn Antenna 30240-20	Manufacturer provided gain 29	BX92420	69



NATIONAL PHYSICAL LABORATORY

Teddington Middlesex UK TW11 0LW Telephone +44 20 8977 3222



Certificate of Calibration

BICONICAL-LOG HYBRID ANTENNA

Model: Teseq CBL 6143A

Serial number: 23169

This certificate is issued in accordance with the laboratory accreditation requirements of the United Kingdom Accreditation Service. It provides traceability of measurement to the SI system of units and/or to units of measurement realised at the National Physical Laboratory or other recognised national metrology institutes. This certificate may not be reproduced other than in full, except with the prior written approval of the issuing laboratory.

FOR:

RISE
Brinellgatan 4
SE-504 62 BORÅS
Sweden

Order no. IX84237

DESCRIPTION:

Teseq CBL 6143A biconical-log hybrid antenna with an operating frequency range of 30 MHz to 3000 MHz. The low frequency elements were of a modified triangular type (L-shaped).

IDENTIFICATION:

The antenna is marked with the manufacturer's serial number 23169. The antenna was calibrated with the customer supplied 6 dB attenuator attached, with the customer number BX61531.

MEASUREMENTS COMPLETED ON: 4 July 2018

The reported uncertainty is based on a coverage factor k=2, providing a level of confidence of approximately 95%

Reference : 2018050459-1

Page 1 of 8

Date of Issue : 4 July 2018

(Authorised Signatory)

Checked by : *D A Knight*

Signed : *D A Knight*

Name : D A Knight

on behalf of NPLML



This certificate is consistent with the capabilities that are included in Appendix C of the MRA drawn up by the CIPM. Under the MRA, all participating institutes recognise the validity of each other's calibration and measurement certificates for the quantities, ranges and measurement uncertainties specified in Appendix C (for details see <http://www.bipm.org>).

NATIONAL PHYSICAL LABORATORY

Continuation Sheet

MEASUREMENT PROCEDURE

Antenna Factor

The measurement method is traceable to field standards which have been validated on the national standard open field site (OFS) at NPL. The OFS comprises a 60 m by 30 m metal ground plane, flat to within ± 6 mm. The receiver linearity has been calibrated, traceable to national standards, and its frequency accuracy has been shown to be better than 10 ppm. On request a complete set of antenna factors, and the complex components of the reflection coefficient can be supplied in ASCII format by email.

The antenna was positioned in the configuration required for each measurement, and where necessary the RF cables were supported in order to minimise parasitic reflections. A summary of the applicable parameters for each measurement is given below. Each summary refers to a later table which contains a subset of results, and the accompanying graphs present the full data set.

The antenna was calibrated according to ANSI C63.5 (see Annex) as one of three antennas, which were calibrated by the height scanning method described in the procedure. The customer's antenna is defined as the Antenna Under Test (AUT). The other antenna in any pair is defined as ANT2. HP and VP are horizontal and vertical polarisation respectively.

Summary of applicable parameters in Table 1

Measurement range	From 30 MHz to 1000 MHz
Measurement parameter	ANSI C63.5:2017 10.0 m separation, AUT Scanned (1.0 m - 4.0 m), ANT2 at HP 2.0 m Near Free Space Antenna Factors
Measurement uncertainty *	± 1.0 dB

- * The reported expanded uncertainty is based on a standard uncertainty multiplied by a coverage factor $k = 2$, providing a coverage probability of approximately 95 %. The uncertainty evaluation has been carried out in accordance with UKAS requirements. The uncertainty applies only to the measured values and gives no indication of the long term stability of the antenna. See annex concerning exemptions to the stated uncertainty.

Balance Test (applies to frequencies below 300 MHz - see Annex)

This test indicated no significant balun imbalance.

The balun balance was measured according to ANSI C63.5:2017, with an estimated expanded uncertainty of ± 0.25 dB.

NATIONAL PHYSICAL LABORATORY

Continuation Sheet

Return Loss and VSWR

The antenna was positioned in a near free-space environment and the complex reflection coefficient, S_{11} , was measured. The result is presented as return loss and VSWR. The estimated uncertainty in the measured reflection coefficient is ± 0.05 units.

NOTES

The antenna was assembled following the markings on the elements and the balun.

The 10 m separation was measured from the marked reference = 0.523 m from the antenna tip.

During calibration NPL uses good quality matching attenuators on the transmit and receive cables, which ensure a return loss better than 10dB. In order to meet the CISPR 16-1-4 requirement for emission measurements a calibrated attenuator should be used on the receive cable to ensure a minimum match of 10dB. When requested NPL will calibrate the antenna with a supplied attenuator attached and the attenuation will be included in the antenna factor and the measured return loss. Alternatively, if no attenuator is supplied, the calibrated value of the attenuator may be included in the loss of the receive cable. ANSI C63.4:2014 requires a match of 2.5:1 VSWR, which equates to a return loss of 7.4dB; it is possible to meet this requirement with a 4dB attenuator. It is recommended to use a 6dB attenuator for hybrid or biconical antennas which have a poor match at 30MHz.

ENVIRONMENT

The measuring equipment was in a temperature controlled room at $22^{\circ}\text{C} \pm 2^{\circ}\text{C}$. In our experience there is no significant variation in the performance of passive antennas in the temperature range -5°C to $+35^{\circ}\text{C}$.

ANNEX TO NPL CERTIFICATE

The annex describes some sources of possible measurement uncertainty when biconical-log hybrid antennas are used for emission testing. The antenna factor uncertainty and any additional measurement uncertainty can be combined by following the guidance given by UKAS[1].

- [1] The expression of uncertainty in EMC testing, LAB 34, UKAS, August 2002.
- [2] The annex for the biconical-log hybrid antenna can be found on the NPL website, www.npl.co.uk, search on "Antennas and Field Probes support documentation" with the address <http://www.npl.co.uk/emc-certificates>

NATIONAL PHYSICAL LABORATORY

Continuation Sheet

Table 1
ANSI C63.5:2017 10.0 m separation,
AUT Scanned (1.0 m - 4.0 m), ANT2 at HP 2.0 m
Teseq CBL 6143A, s/n 23169

Frequency (MHz)	Antenna Factor (dB/m)	Frequency (MHz)	Antenna factor (dB/m)
30	28.4	520	23.1
40	23.4	540	24.1
60	16.1	560	24.5
80	13.3	580	24.4
100	16.0	600	24.4
120	18.7	620	24.6
140	18.4	640	24.9
160	16.6	660	24.6
180	16.2	680	24.7
200	17.5	700	24.7
220	18.5	720	25.0
240	17.8	740	25.3
260	18.5	760	25.5
280	18.7	780	25.9
300	19.2	800	25.7
320	19.6	820	25.8
340	19.7	840	26.1
360	20.3	860	26.2
380	20.8	880	26.6
400	22.0	900	26.3
420	21.6	920	26.4
440	21.9	940	26.6
460	22.5	960	26.9
480	22.9	980	26.9
500	22.9	1000	27.4

Reference : 2018050459-1

Page 4 of 8


Date of Issue : 4 July 2018

Checked by : TF

NATIONAL PHYSICAL LABORATORY

Continuation Sheet

Figure 1
ANSI C63.5:2017 10.0 m separation,
AUT Scanned (1.0 m - 4.0 m), ANT2 at HP 2.0 m
Teseq CBL 6143A, s/n 23169.

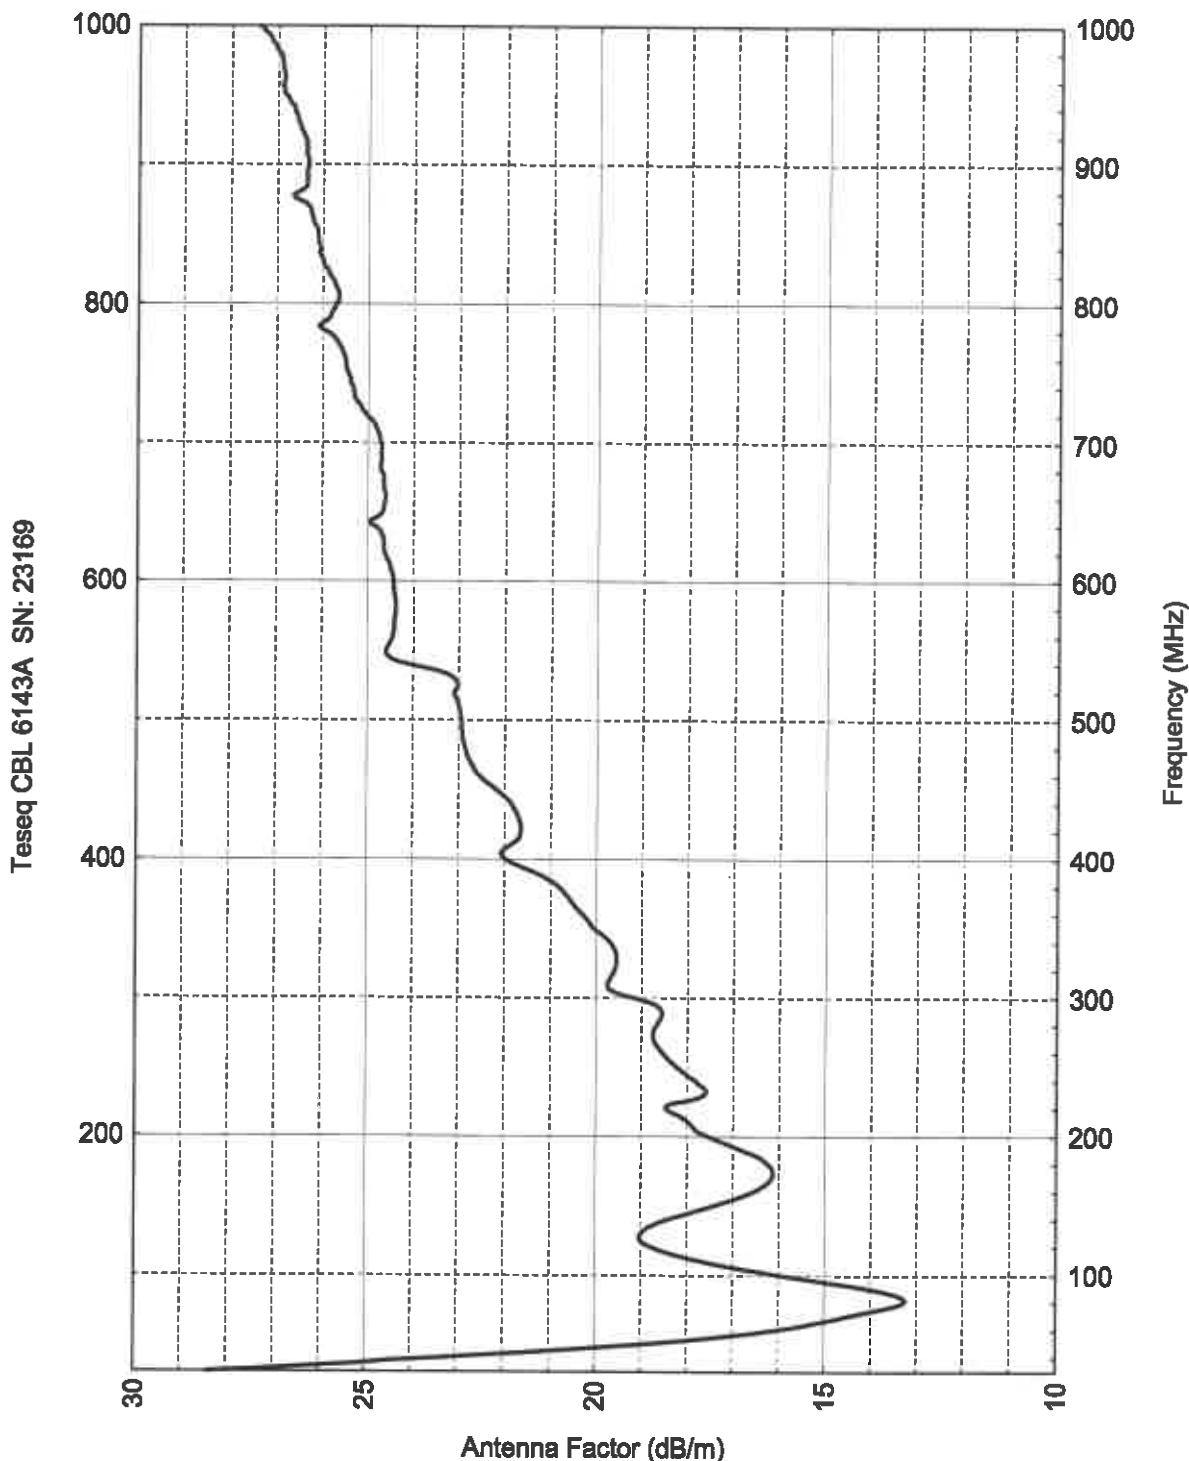

Reference : 2018050459-1

Date of Issue : 4 July 2018


Checked by : TF

Page 5 of 8

NATIONAL PHYSICAL LABORATORY

Continuation Sheet

Figure 2
VSWR
Teseq CBL 6143A, s/n 23169.

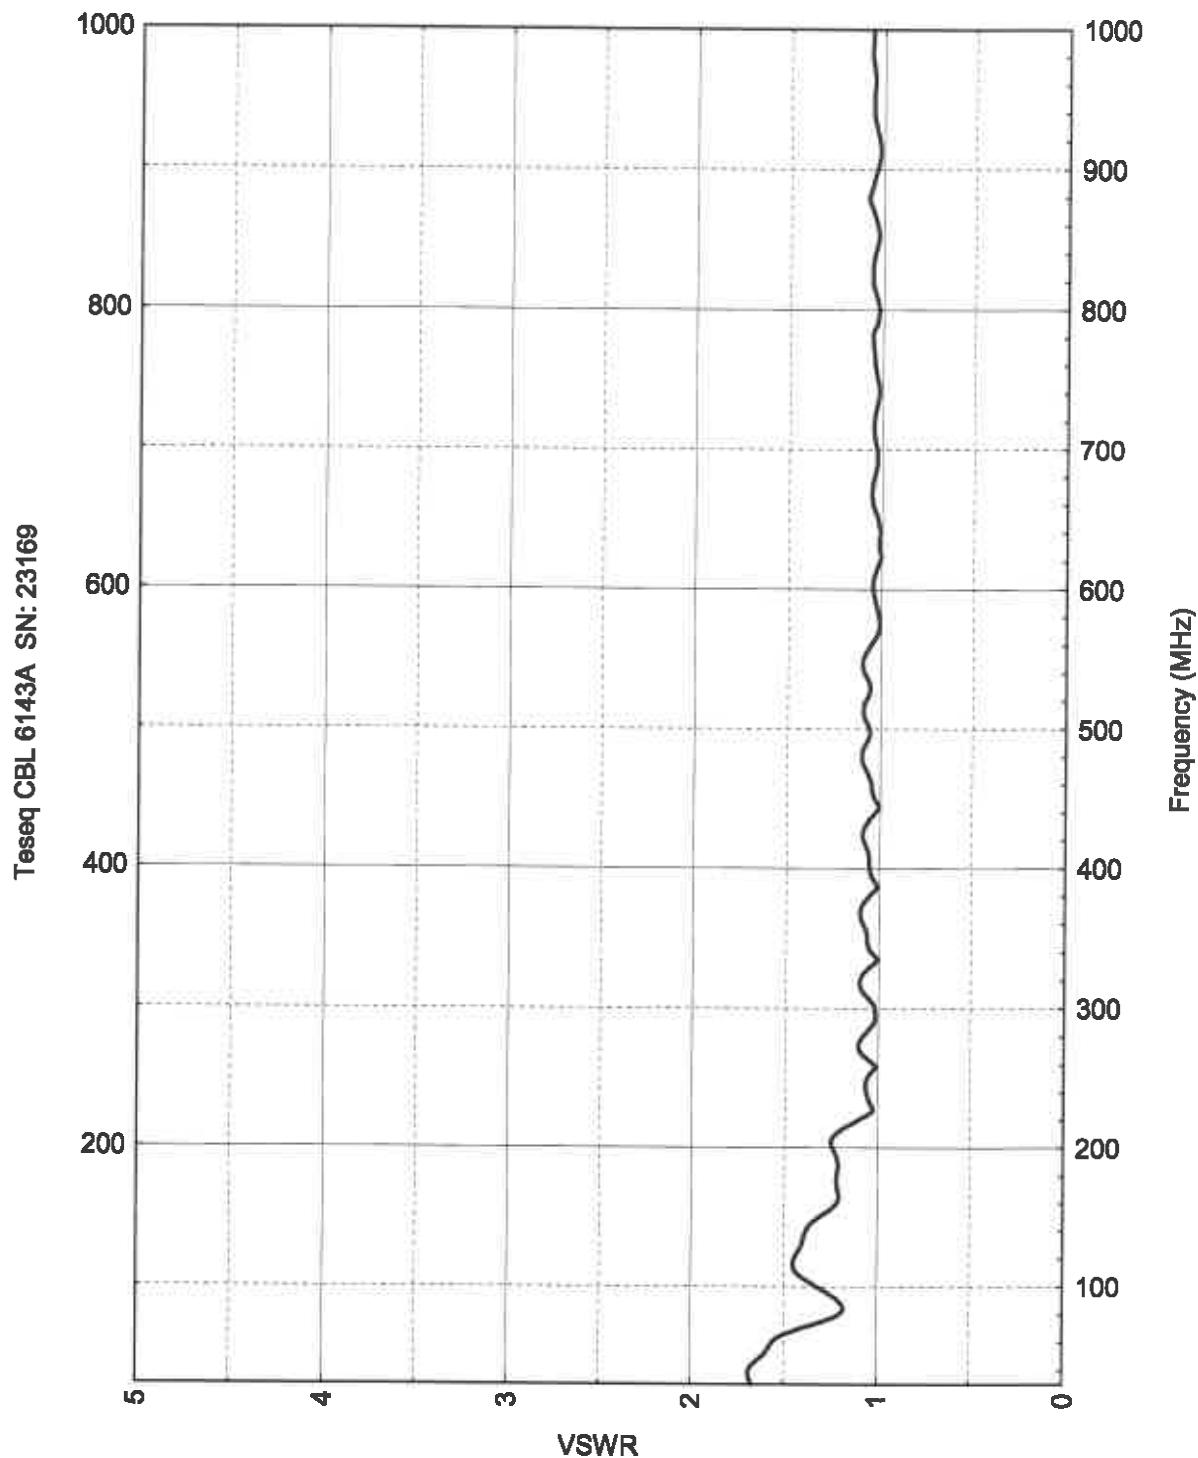

Reference : 2018050459-1

Date of Issue : 4 July 2018


Checked by : *TF*

Page 6 of 8

NATIONAL PHYSICAL LABORATORY

Continuation Sheet

Figure 3
Return Loss for antenna model: Teseq CBL 6143A, s/n 23169.

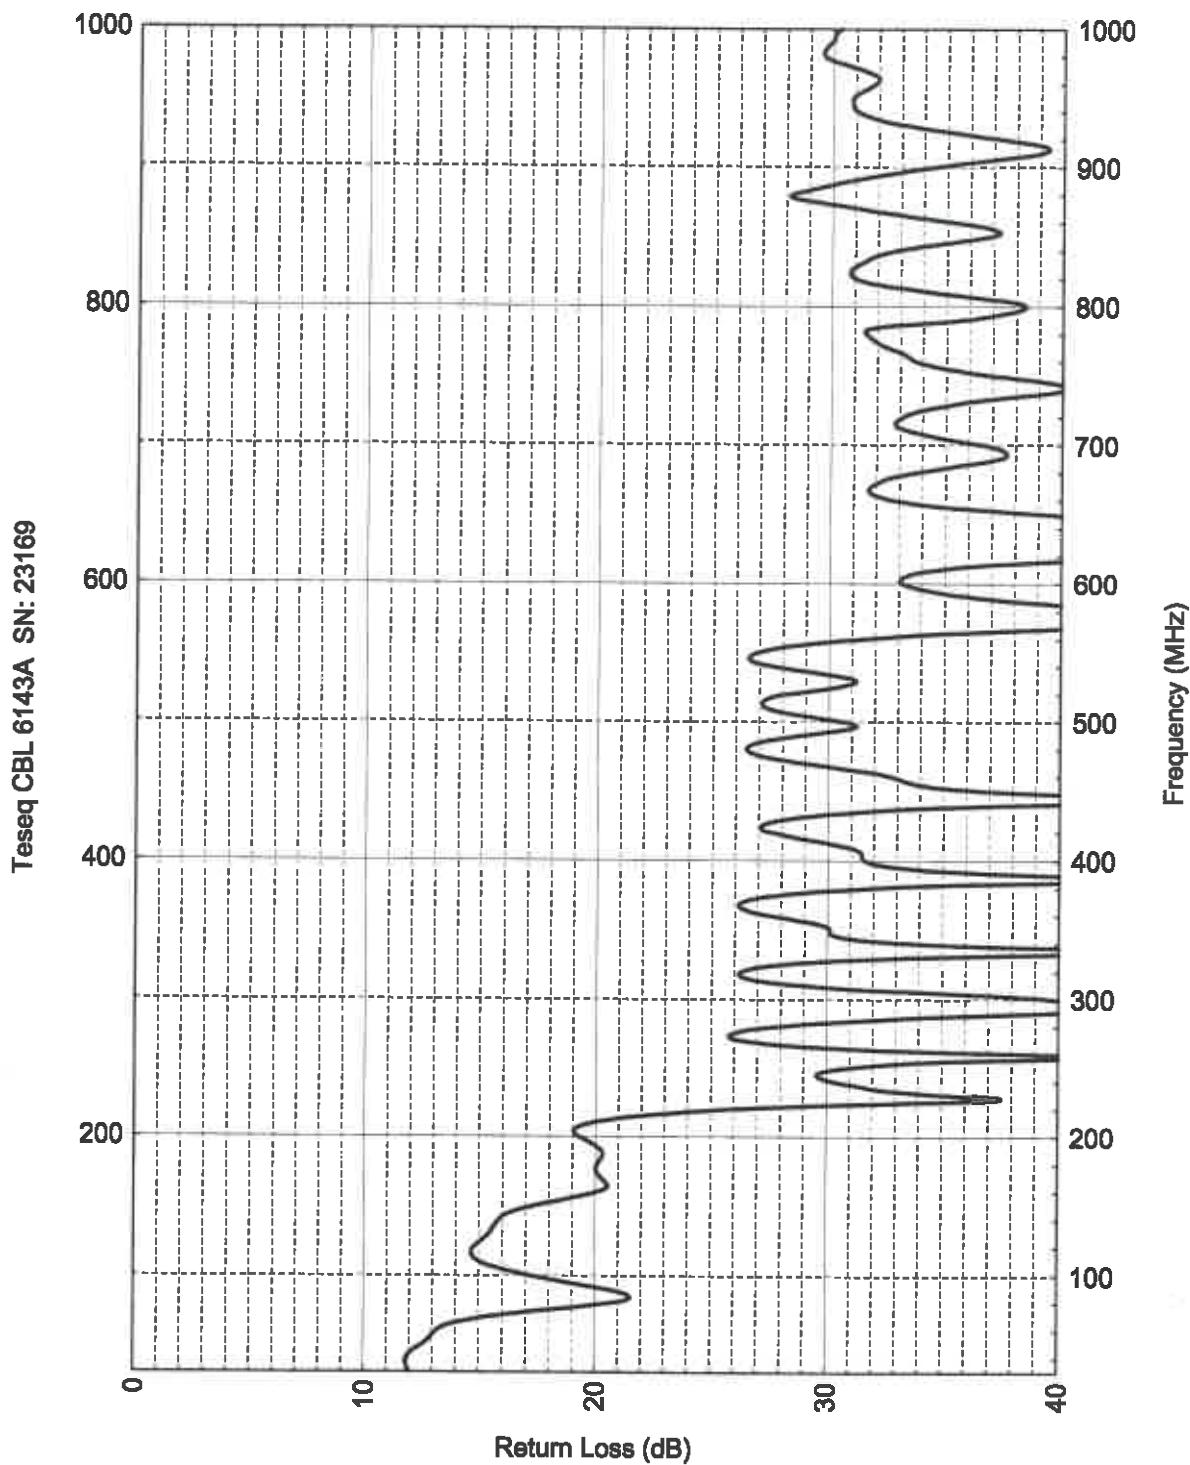

Reference : 2018050459-1

Date of Issue : 4 July 2018


Checked by : TF

Page 7 of 8

NATIONAL PHYSICAL LABORATORY

Continuation Sheet

Figure 4
Balance test for antenna model: Teseq CBL 6143A, s/n 23169.

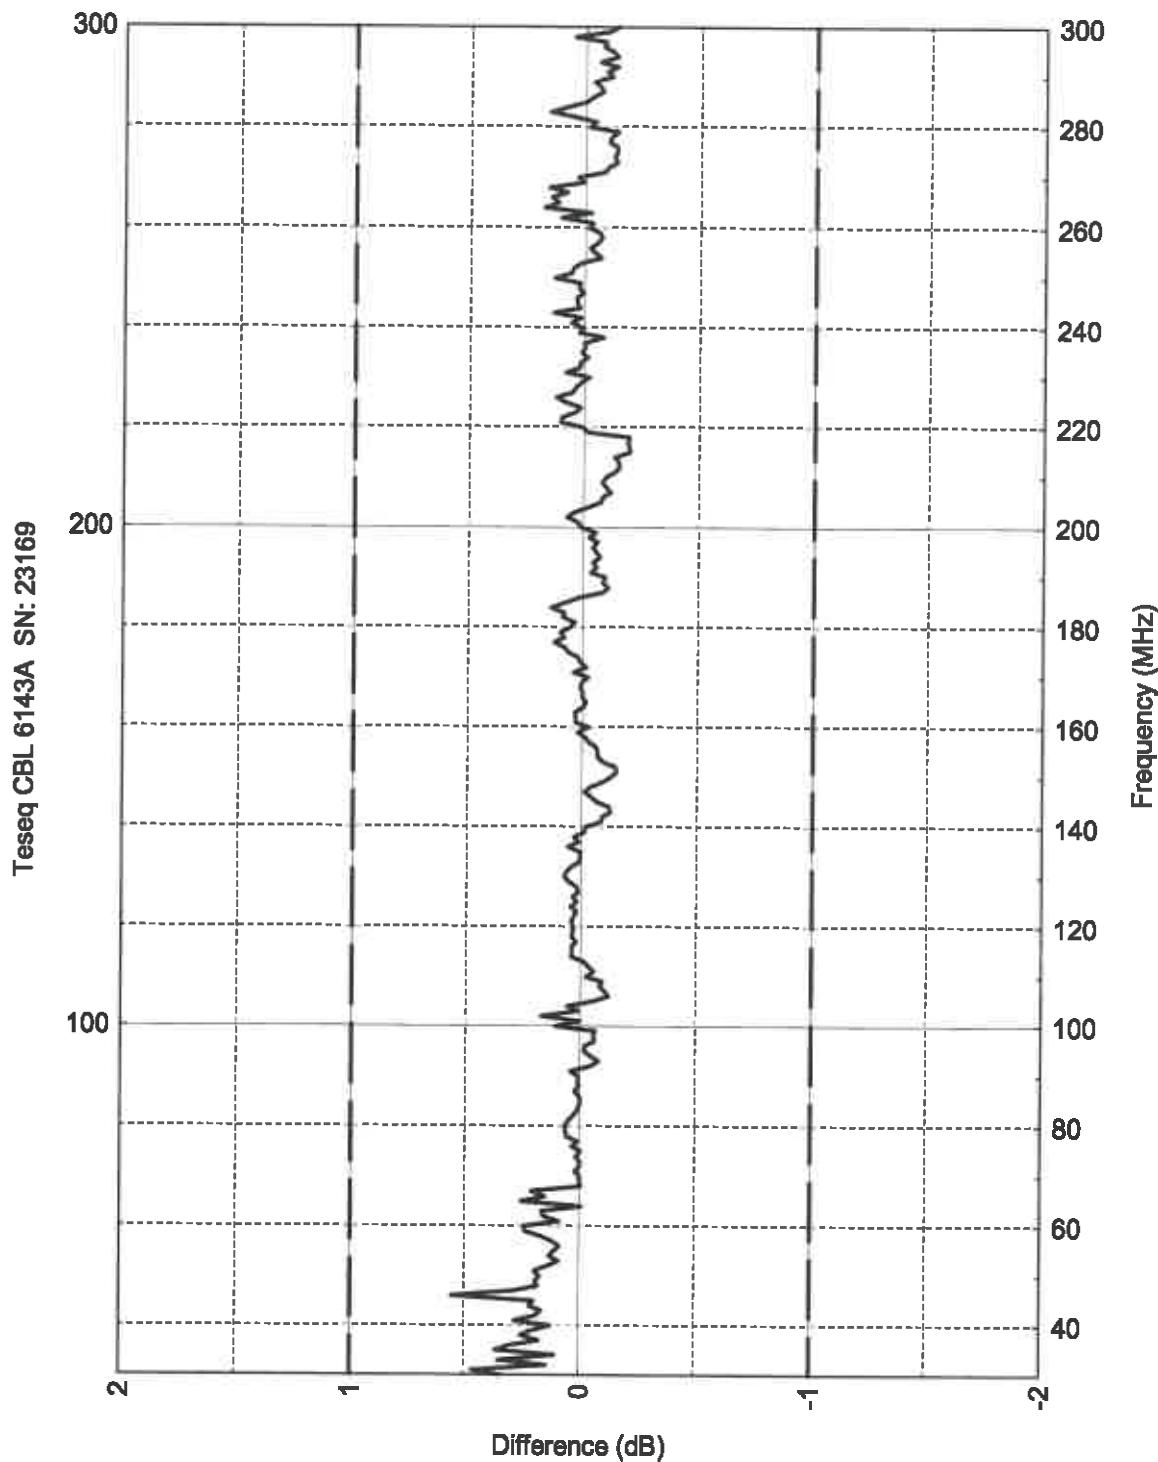

Reference : 2018050459-1

Date of Issue : 4 July 2018

Checked by : TF

Page 8 of 8



NATIONAL PHYSICAL LABORATORY

Teddington Middlesex UK TW11 0LW Telephone +44 20 8977 3222

Certificate of Calibration



EMCO 3115
Double Ridged Guide Horn Antenna s/n 9509-4562

This certificate is issued in accordance with the laboratory accreditation requirements of the United Kingdom Accreditation Service. It provides traceability of measurement to the SI system of units and/or to units of measurement realised at the National Physical Laboratory or other recognised national metrology institutes. This certificate may not be reproduced other than in full, except with the prior written approval of the issuing laboratory.

FOR:

RISE
Brinellgatan 4
SE-504 62 BORÅS
Sweden

DESCRIPTION:

EMCO 3115 Double Ridged Guide Horn Antenna

IDENTIFICATION:

s/n 9509-4562

CALIBRATION FREQUENCIES: 0.7 GHz to 18.0 GHz in 0.1 GHz steps

DATE(S) OF CALIBRATION: 28 June to 5 July 2018

Reference: 2018050459-2

Page 1 of 5

Date of Issue: 6 July 2018

Signed: D G Gentle

(Authorised Signatory)

Checked by:

Name: D G Gentle

on behalf of NPLML



This certificate is consistent with the capabilities that are included in Appendix C of the MRA drawn up by the CIPM. Under the MRA, all participating institutes recognise the validity of each other's calibration and measurement certificates for the quantities, ranges and measurement uncertainties specified in Appendix C (for details see <http://www.bipm.org>).

NATIONAL PHYSICAL LABORATORY

Continuation Sheet

MEASUREMENTS

In the following, the IEEE definition of gain is used: the gain of an antenna in a given direction is defined as "the ratio of the radiation intensity, in a given direction, to the radiation intensity that would be obtained if the power accepted by the antenna were isotropically radiated". The apparent gain is obtained by multiplying the gain by the factor $(1 - |\Gamma|^2)$, where Γ is the reflection coefficient of the antenna.

The apparent gain of the antenna was measured by the three antenna technique. The antenna separation was 3 m, measured from the aperture of the antenna. A vector network analyser was used to measure the complex reflection coefficients of the antennas and components used in the measurement circuit. Mismatch corrections were calculated from these measurements and applied to the measured gains to give the apparent gains. The antenna factors were calculated from the apparent gains using the following formula:

$$AF = 30.23 + 20\log_{10}(F_{\text{GHz}}) - G_{\text{dBi}} \quad [\text{dB } (1/\text{m})]$$

where F_{GHz} is the frequency in GHz and G_{dBi} is the apparent gain in dBi.

All measurements were made in a temperature controlled electromagnetic anechoic chamber in a screened laboratory at a temperature of $23 \pm 2^\circ \text{C}$.

CALIBRATION DATA

This certificate contains a subset of the full calibration data. A complete set of results will be provided via email in Excel format.

MEASUREMENT UNCERTAINTIES

The estimated uncertainty in the apparent gain is $\pm 1.0 \text{ dB}$ for frequencies below 1.0 GHz and $\pm 0.8 \text{ dB}$ for frequencies 1.0 GHz and above. The uncertainties in the real or imaginary parts of the reflection coefficients are given in the table below. The reported expanded uncertainty is based on a standard uncertainty multiplied by a coverage factor $k = 2$, providing a coverage probability of approximately 95 %. The uncertainty evaluation has been carried out in accordance with UKAS requirements. These uncertainties apply only to the measured values and give no indication of the long term stability of the antenna.

Uncertainties in the components of the reflection coefficients.

Frequency range [GHz]	Uncertainty in real or imaginary parts
0.7 to 0.9	$\pm 0.050 \text{ units}$
1.0 to 1.5	$\pm 0.015 \text{ units}$
1.6 to 18.0	$\pm 0.011 \text{ units}$

NATIONAL PHYSICAL LABORATORY

Continuation Sheet

RESULTS

Apparent Gain and Antenna Factor at 3 m from the antenna aperture.		
Frequency [GHz]	Gain 3 m [dBi]	Antenna Factor [dB (1/m)]
0.70	-1.1	28.2
0.80	2.4	25.9
0.90	5.1	24.2
1.00	5.7	24.6
1.50	8.3	25.5
2.00	8.8	27.4
2.50	9.8	28.4
3.00	9.8	29.9
3.50	10.0	31.1
4.00	9.9	32.4
4.50	11.0	32.3
5.00	10.7	33.5
5.50	10.9	34.1
6.00	11.5	34.3
6.50	12.1	34.4
7.00	11.8	35.4
7.50	11.4	36.3
8.00	11.6	36.7
8.50	11.4	37.4
9.00	11.3	38.0
9.50	11.4	38.4
10.00	10.8	39.4
10.50	10.9	39.7
11.00	12.2	38.8
11.50	12.5	39.0
12.00	12.5	39.4
12.50	13.3	38.8
13.00	13.4	39.1
13.50	12.3	40.5
14.00	11.6	41.6
14.50	10.7	42.7
15.00	12.7	41.0
15.50	16.1	37.9
16.00	16.7	37.6
16.50	16.2	38.4
17.00	14.1	40.7
17.50	10.6	44.5
18.00	8.0	47.3

Reference: 2018050459-2

Checked by: 


Page 3 of 5

NATIONAL PHYSICAL LABORATORY

Continuation Sheet

Reflection Coefficients and VSWR			
Freq [GHz]	Real Part	Imaginary Part	VSWR
0.70	0.801	0.241	11.26
0.80	0.641	-0.143	4.82
0.90	0.373	-0.201	2.47
1.00	0.370	-0.177	2.39
1.50	-0.162	-0.219	1.75
2.00	-0.337	-0.006	2.02
2.50	-0.238	0.066	1.65
3.00	-0.134	0.087	1.38
3.50	0.091	0.085	1.29
4.00	0.139	-0.112	1.44
4.50	-0.092	-0.094	1.30
5.00	-0.183	0.171	1.67
5.50	-0.003	0.306	1.88
6.00	0.160	0.172	1.62
6.50	0.166	-0.070	1.44
7.00	-0.023	-0.171	1.42
7.50	-0.114	-0.021	1.26
8.00	0.019	0.088	1.20
8.50	0.134	0.019	1.31
9.00	0.132	-0.118	1.43
9.50	-0.010	-0.239	1.63
10.00	-0.238	-0.176	1.84
10.50	-0.149	0.060	1.38
11.00	-0.095	-0.053	1.24
11.50	-0.121	0.016	1.28
12.00	-0.009	0.050	1.11
12.50	0.043	-0.053	1.15
13.00	-0.051	-0.129	1.32
13.50	-0.152	-0.044	1.38
14.00	-0.093	0.091	1.30
14.50	0.100	0.083	1.30
15.00	0.193	-0.125	1.60
15.50	0.042	-0.303	1.88
16.00	-0.183	-0.268	1.96
16.50	-0.292	-0.037	1.84
17.00	-0.122	0.215	1.66
17.50	0.216	0.129	1.67
18.00	0.218	-0.235	1.95

Reference: 2018050459-2


Checked by: 

Page 4 of 5

NATIONAL PHYSICAL LABORATORY

Continuation Sheet

EMCO 3115 Double Ridged Guide Horn Antenna s/n 9509-4562

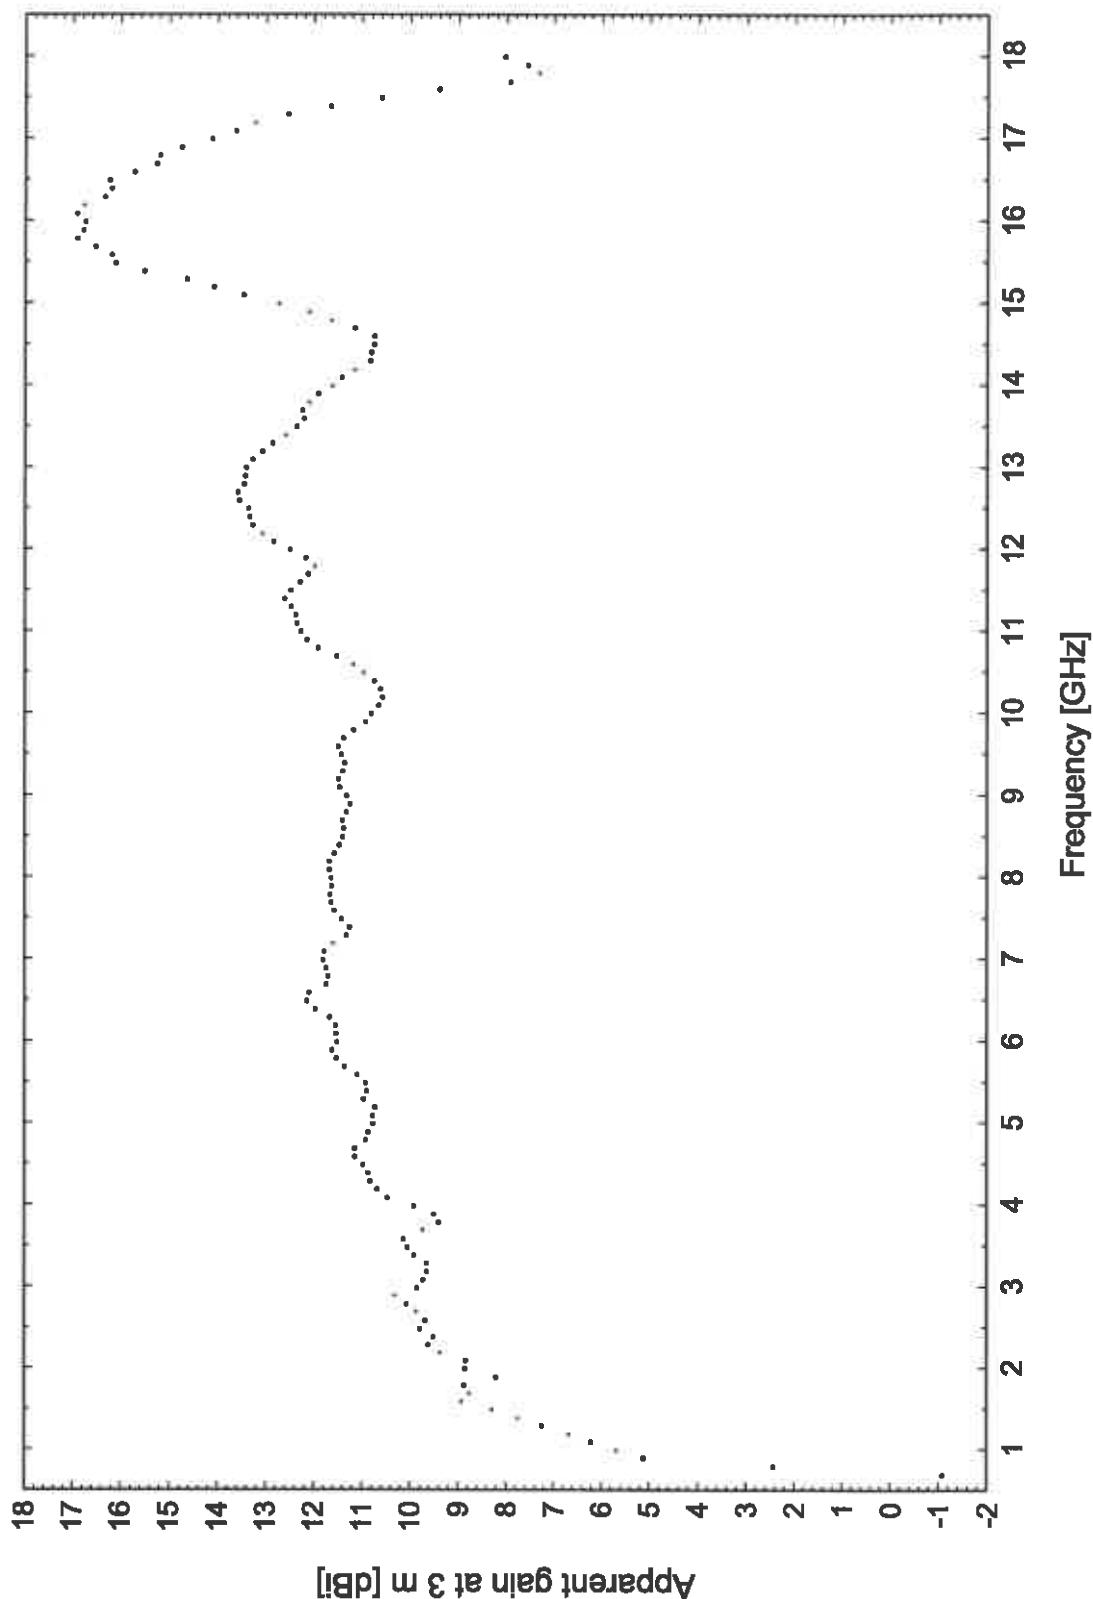

Reference: 2018050459-2

Checked by: *Ehnull*

Page 5 of 5



NATIONAL PHYSICAL LABORATORY

Teddington Middlesex UK TW11 0LW Telephone +44 20 8977 3222



Certificate of Calibration

ETS-Lindgren 3115

Double Ridged Guide Horn Antenna S/N: 00143161

This certificate is issued in accordance with the laboratory accreditation requirements of the United Kingdom Accreditation Service. It provides traceability of measurement to the SI system of units and/or to units of measurement realised at the National Physical Laboratory or other recognised national metrology institutes. This certificate may not be reproduced other than in full, except with the prior written approval of the issuing laboratory.

FOR:

RISE
Box 857
Se 501 15
Boras
Sweden

DESCRIPTION: ETS-Lindgren 3115 Double Ridged Guide Horn Antenna

IDENTIFICATION: S/N:00143161

CALIBRATION FREQUENCIES: 1.0 GHz to 18.0 GHz in 0.1 GHz steps

DATE(S) OF CALIBRATION: 11 December 2018

Reference: 2018100184-1

Page 1 of 5

Date of Issue: 11 December 2018

Signed: D G Gentle

(Authorised Signatory)

Checked by:

Name: D G Gentle

on behalf of NPLML



This certificate is consistent with the capabilities that are included in Appendix C of the MRA drawn up by the CIPM. Under the MRA, all participating institutes recognise the validity of each other's calibration and measurement certificates for the quantities, ranges and measurement uncertainties specified in Appendix C (for details see <http://www.bipm.org>).

NATIONAL PHYSICAL LABORATORY

Continuation Sheet

MEASUREMENTS

The measurements were made in accordance with the ANSI 63.5:2017 standard. The results of this calibration comply with the basic requirement set out in section 5.1.3.1 a) i) ii) of the standard: "AFs measured at distances with $0.62 \sqrt{D^3 / \lambda} \leq R < 2D^2 / \lambda$ shall be deemed acceptable at the calibrated distance" for radiated emission measurements.

In the following, the IEEE definition of gain is used: the gain of an antenna in a given direction is defined as "the ratio of the radiation intensity, in a given direction, to the radiation intensity that would be obtained if the power accepted by the antenna were isotropically radiated". The apparent gain is obtained by multiplying the gain by the factor $(1 - |\Gamma|^2)$, where Γ is the reflection coefficient of the antenna.

The apparent gain of the antenna was measured by the three antenna technique. The antenna separation was 3 m, measured from the aperture of the antenna. A vector network analyser was used to measure the complex reflection coefficients of the antennas and components used in the measurement circuit. Mismatch corrections were calculated from these measurements and applied to the measured gains to give the apparent gains. The antenna factors were calculated from the apparent gains using the following formula:

$$AF = 30.23 + 20\log_{10}(F_{\text{GHz}}) - G_{\text{dBi}} \quad [\text{dB (1/m)}]$$

where F_{GHz} is the frequency in GHz and G_{dBi} is the apparent gain in dBi.

All measurements were made in a temperature controlled electromagnetic anechoic chamber in a screened laboratory at a temperature of $23 \pm 2^\circ \text{C}$.

CALIBRATION DATA

This certificate contains a subset of the full calibration data. A complete set of results will be provided via email in Excel format.

MEASUREMENT UNCERTAINTIES

The estimated uncertainty in the apparent gain is $\pm 0.8 \text{ dB}$ and the uncertainties in the real or imaginary parts of the reflection coefficients are given in the table below. The reported expanded uncertainty is based on a standard uncertainty multiplied by a coverage factor $k = 2$, providing a coverage probability of approximately 95%. The uncertainty evaluation has been carried out in accordance with UKAS requirements. These uncertainties apply only to the measured values and give no indication of the long term stability of the antenna.

Uncertainties in the components of the reflection coefficients.

Frequency range [GHz]	Uncertainty in real or imaginary parts
1.0 to 1.5	$\pm 0.015 \text{ units}$
1.6 to 18.0	$\pm 0.011 \text{ units}$



NATIONAL PHYSICAL LABORATORY

Continuation Sheet

RESULTS

Apparent Gain and Antenna Factor at 3 m from the antenna aperture.		
Frequency [GHz]	Gain 3 m [dBi]	Antenna Factor [dB (1/m)]
1.00	6.6	23.6
1.50	8.3	25.5
2.00	7.8	28.4
2.50	10.4	27.8
3.00	10.7	29.1
3.50	10.7	30.4
4.00	10.5	31.7
4.50	11.3	32.0
5.00	11.3	32.9
5.50	11.3	33.8
6.00	10.5	35.3
6.50	10.9	35.6
7.00	10.5	36.6
7.50	10.4	37.3
8.00	11.3	37.0
8.50	11.3	37.5
9.00	11.7	37.6
9.50	11.8	38.0
10.00	12.0	38.2
10.50	12.1	38.5
11.00	12.6	38.5
11.50	12.7	38.7
12.00	13.0	38.8
12.50	13.4	38.8
13.00	12.7	39.8
13.50	12.3	40.6
14.00	11.9	41.2
14.50	12.4	41.0
15.00	13.9	39.9
15.50	14.6	39.5
16.00	14.9	39.5
16.50	13.6	41.0
17.00	12.6	42.2
17.50	12.1	43.0
18.00	12.6	42.7

NATIONAL PHYSICAL LABORATORY

Continuation Sheet

Reflection Coefficients and VSWR			
Freq [GHz]	Real Part	Imaginary Part	VSWR
1.00	0.119	-0.161	1.50
1.50	-0.331	-0.011	1.99
2.00	-0.400	0.172	2.54
2.50	-0.158	0.225	1.76
3.00	0.000	0.175	1.43
3.50	0.172	0.208	1.74
4.00	0.283	0.107	1.87
4.50	0.102	0.010	1.23
5.00	-0.060	0.150	1.38
5.50	0.058	0.278	1.80
6.00	0.255	0.164	1.87
6.50	0.348	-0.053	2.08
7.00	0.234	-0.254	2.05
7.50	-0.008	-0.222	1.57
8.00	-0.065	-0.003	1.14
8.50	0.069	0.055	1.19
9.00	0.133	-0.067	1.35
9.50	0.080	-0.205	1.57
10.00	-0.052	-0.245	1.67
10.50	-0.135	-0.162	1.53
11.00	-0.129	-0.069	1.34
11.50	-0.109	-0.030	1.25
12.00	-0.094	0.002	1.21
12.50	-0.050	0.000	1.10
13.00	-0.030	-0.059	1.14
13.50	-0.091	-0.109	1.33
14.00	-0.188	-0.061	1.49
14.50	-0.219	0.090	1.62
15.00	-0.104	0.254	1.76
15.50	0.114	0.268	1.82
16.00	0.262	0.133	1.83
16.50	0.280	-0.043	1.79
17.00	0.179	-0.162	1.63
17.50	0.037	-0.116	1.28
18.00	0.092	0.074	1.27

Reference: 2018100184-1

Page 4 of 5


Checked by:



NATIONAL PHYSICAL LABORATORY

Continuation Sheet

ETS-Lindgren 3115 Double Ridged Guide Horn Antenna s/n 00143161

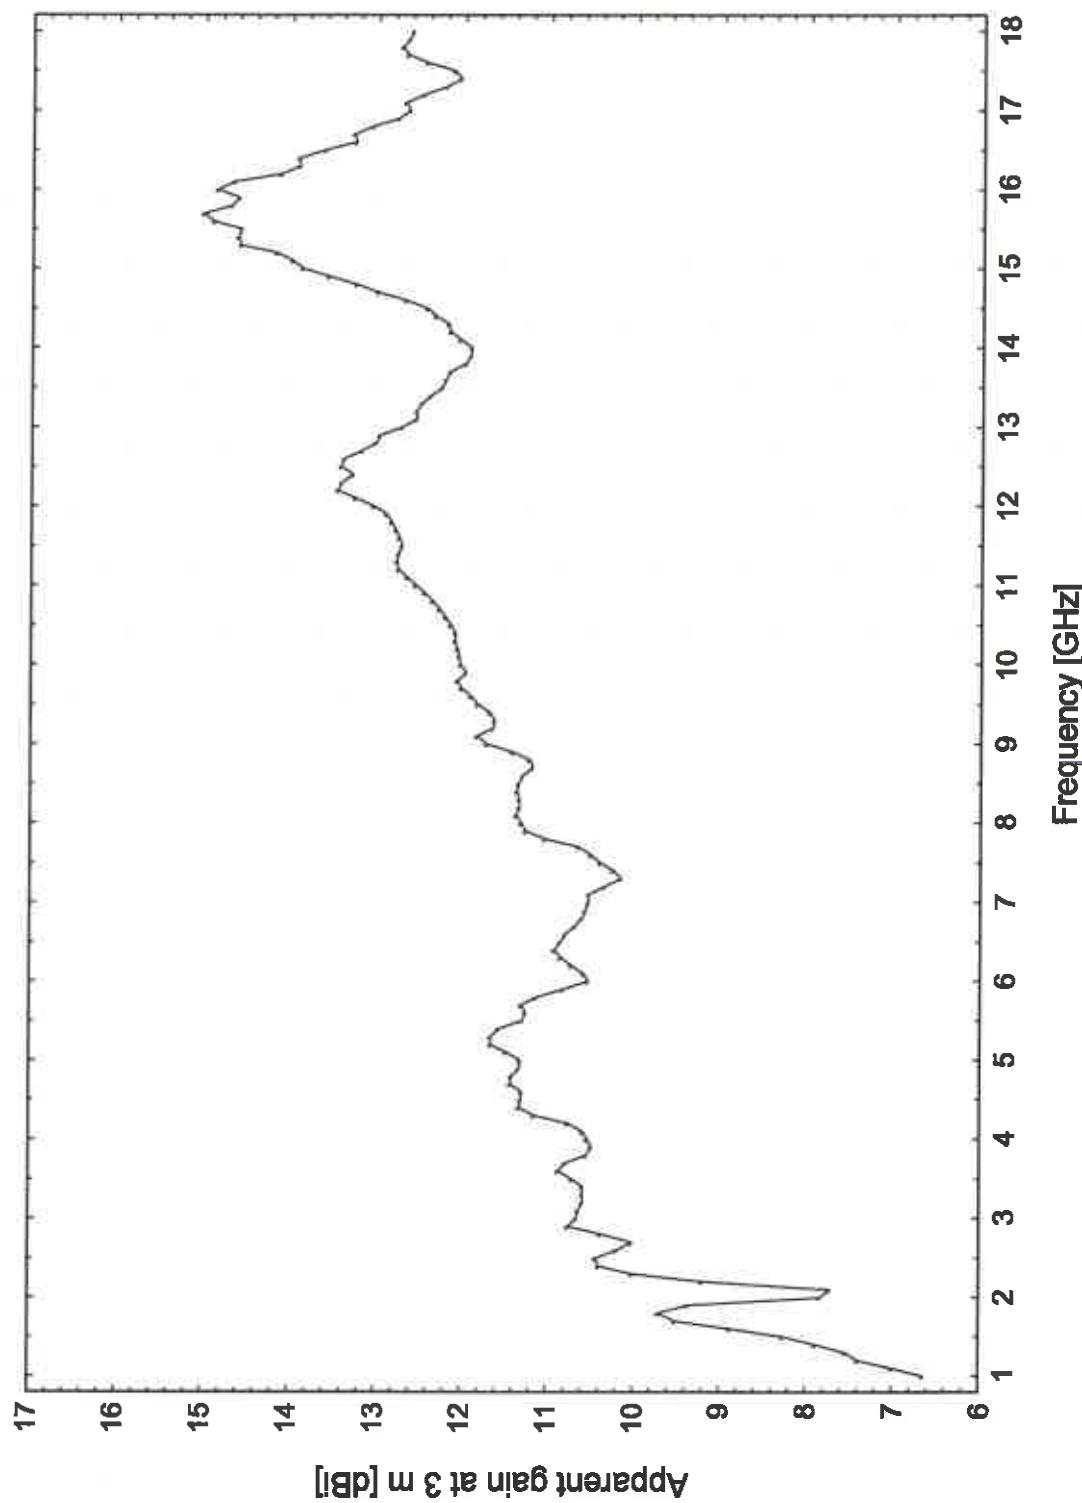


Reference: 2018100184-1

Page 5 of 5

Checked by:

A. Bearshore



NATIONAL PHYSICAL LABORATORY

Teddington Middlesex UK TW11 0LW Telephone +44 20 8977 3222



Certificate of Calibration

EMCO 3116
Double Ridged Guide Horn Antenna S/N: 9904-2426

This certificate is issued in accordance with the laboratory accreditation requirements of the United Kingdom Accreditation Service. It provides traceability of measurement to the SI system of units and/or to units of measurement realised at the National Physical Laboratory or other recognised national metrology institutes. This certificate may not be reproduced other than in full, except with the prior written approval of the issuing laboratory.

FOR:

RISE
Brinellgatan 4
SE-504 62 BORÅS
Sweden

DESCRIPTION: EMCO 3116 Double Ridged Guide Horn Antenna
IDENTIFICATION: S/N 9904-2426
CALIBRATION FREQUENCIES: 18.00 GHz to 40.00 GHz in 0.25 GHz steps
DATE(S) OF CALIBRATION: 19 July 2018

Reference: 2018050459-3

Page 1 of 5

Date of Issue: 20 July 2018

Signed: DG Gentle

(Authorised Signatory)

Checked by:

Name: D G Gentle

on behalf of NPLML



This certificate is consistent with the capabilities that are included in Appendix C of the MRA drawn up by the CIPM. Under the MRA, all participating institutes recognise the validity of each other's calibration and measurement certificates for the quantities, ranges and measurement uncertainties specified in Appendix C (for details see <http://www.bipm.org>).

NATIONAL PHYSICAL LABORATORY

Continuation Sheet

MEASUREMENTS

In the following, the IEEE definition of gain is used: the gain of an antenna in a given direction is defined as “the ratio of the radiation intensity, in a given direction, to the radiation intensity that would be obtained if the power accepted by the antenna were isotropically radiated”. The apparent gain is obtained by multiplying the gain by the factor $(1 - |\Gamma|^2)$, where Γ is the reflection coefficient of the antenna.

The apparent gain of the antenna was measured by the three antenna technique. The antenna separation was 3 m measured from the aperture of the antenna. A vector network analyser was used to measure the complex reflection coefficients of the antennas and components used in the measurement circuit. Mismatch corrections were calculated from these measurements and applied to the measured gains to give the apparent gains. The antenna factors were calculated from the apparent gains using the following formula:

$$AF = 30.23 + 20\log_{10}(F_{\text{GHz}}) - G_{\text{dBi}} \quad [\text{dB (1/m)}]$$

where F_{GHz} is the frequency in GHz and G_{dBi} is the apparent gain in dBi.

All measurements were made in a temperature controlled electromagnetic anechoic chamber in a screened laboratory at a temperature of $23 \pm 2^\circ \text{C}$.

CALIBRATION DATA

This certificate contains a subset of the full calibration data. A complete set of results will be provided via email in Excel format.

MEASUREMENT UNCERTAINTIES

The estimated uncertainty in the apparent gain is $\pm 0.8 \text{ dB}$ and the uncertainty in the real or imaginary parts of the reflection coefficients are given in the table below. The reported expanded uncertainty is based on a standard uncertainty multiplied by a coverage factor $k = 2$, providing a coverage probability of approximately 95 %. The uncertainty evaluation has been carried out in accordance with UKAS requirements. These uncertainties apply only to the measured values and give no indication of the long term stability of the antenna.

Uncertainties in the components of the reflection coefficients.

Frequency range [GHz]	Uncertainty in real or imaginary parts
18.00 to 26.50	$\pm 0.028 \text{ units}$
26.75 to 40.00	$\pm 0.043 \text{ units}$

NATIONAL PHYSICAL LABORATORY

Continuation Sheet

RESULTS

Apparent Gain and Antenna Factor at 3 m from the antenna aperture.		
Frequency [GHz]	Gain 3 m [dBi]	Antenna Factor [dB (1/m)]
18.00	11.9	43.4
18.50	11.6	44.0
19.00	11.2	44.6
19.50	10.7	45.4
20.00	10.7	45.5
20.50	10.9	45.6
21.00	10.5	46.2
21.50	10.6	46.3
22.00	11.0	46.0
22.50	11.2	46.1
23.00	11.8	45.6
23.50	11.9	45.8
24.00	12.5	45.4
24.50	12.8	45.2
25.00	12.5	45.7
25.50	12.3	46.1
26.00	12.3	46.2
26.50	12.3	46.4
27.00	12.6	46.2
27.50	12.6	46.4
28.00	12.5	46.7
28.50	12.8	46.5
29.00	12.8	46.6
29.50	13.2	46.4
30.00	13.5	46.3
30.50	13.4	46.6
31.00	13.1	47.0
31.50	13.0	47.2
32.00	12.5	47.9
32.50	11.9	48.6
33.00	11.3	49.3
33.50	10.5	50.2
34.00	10.2	50.6
34.50	10.0	51.0
35.00	9.2	51.9
35.50	10.0	51.2
36.00	11.5	49.8
36.50	13.3	48.2
37.00	14.9	46.7
37.50	15.7	46.0
38.00	16.0	45.8
38.50	16.3	45.6
39.00	16.5	45.6
39.50	15.9	46.2
40.00	15.1	47.2

Reference: 2018050459-3

Page 3 of 5

Checked by: 

NATIONAL PHYSICAL LABORATORY

Continuation Sheet

Reflection Coefficients and VSWR			
Freq [GHz]	Real Part	Imaginary Part	VSWR
18.00	0.123	0.000	1.28
18.50	0.095	-0.151	1.43
19.00	-0.059	-0.200	1.53
19.50	-0.163	-0.145	1.56
20.00	-0.238	-0.067	1.66
20.50	-0.253	0.070	1.71
21.00	-0.167	0.159	1.60
21.50	-0.102	0.182	1.53
22.00	-0.017	0.207	1.52
22.50	0.063	0.152	1.39
23.00	0.085	0.116	1.34
23.50	0.142	0.066	1.37
24.00	0.133	-0.034	1.32
24.50	0.072	-0.083	1.25
25.00	0.015	-0.101	1.23
25.50	-0.055	-0.078	1.21
26.00	-0.068	-0.007	1.15
26.50	-0.037	0.023	1.09
27.00	-0.008	0.044	1.09
27.50	0.045	0.031	1.12
28.00	0.062	-0.012	1.13
28.50	0.068	-0.047	1.18
29.00	0.055	-0.105	1.27
29.50	-0.005	-0.138	1.32
30.00	-0.062	-0.138	1.36
30.50	-0.122	-0.124	1.42
31.00	-0.179	-0.066	1.47
31.50	-0.194	0.008	1.48
32.00	-0.177	0.081	1.48
32.50	-0.114	0.145	1.45
33.00	-0.025	0.142	1.34
33.50	0.032	0.090	1.21
34.00	0.039	0.017	1.09
34.50	-0.013	-0.027	1.06
35.00	-0.062	-0.015	1.14
35.50	-0.084	0.009	1.18
36.00	-0.103	0.041	1.25
36.50	-0.100	0.085	1.30
37.00	-0.075	0.120	1.33
37.50	-0.031	0.150	1.36
38.00	0.031	0.145	1.35
38.50	0.064	0.103	1.28
39.00	0.073	0.073	1.23
39.50	0.072	0.042	1.18
40.00	0.060	0.020	1.13


Reference: 2018050459-3

Checked by: 

Page 4 of 5

NATIONAL PHYSICAL LABORATORY
Continuation Sheet

EMCO 3116 Double Ridged Guide Horn Antenna s/n 9904-2426

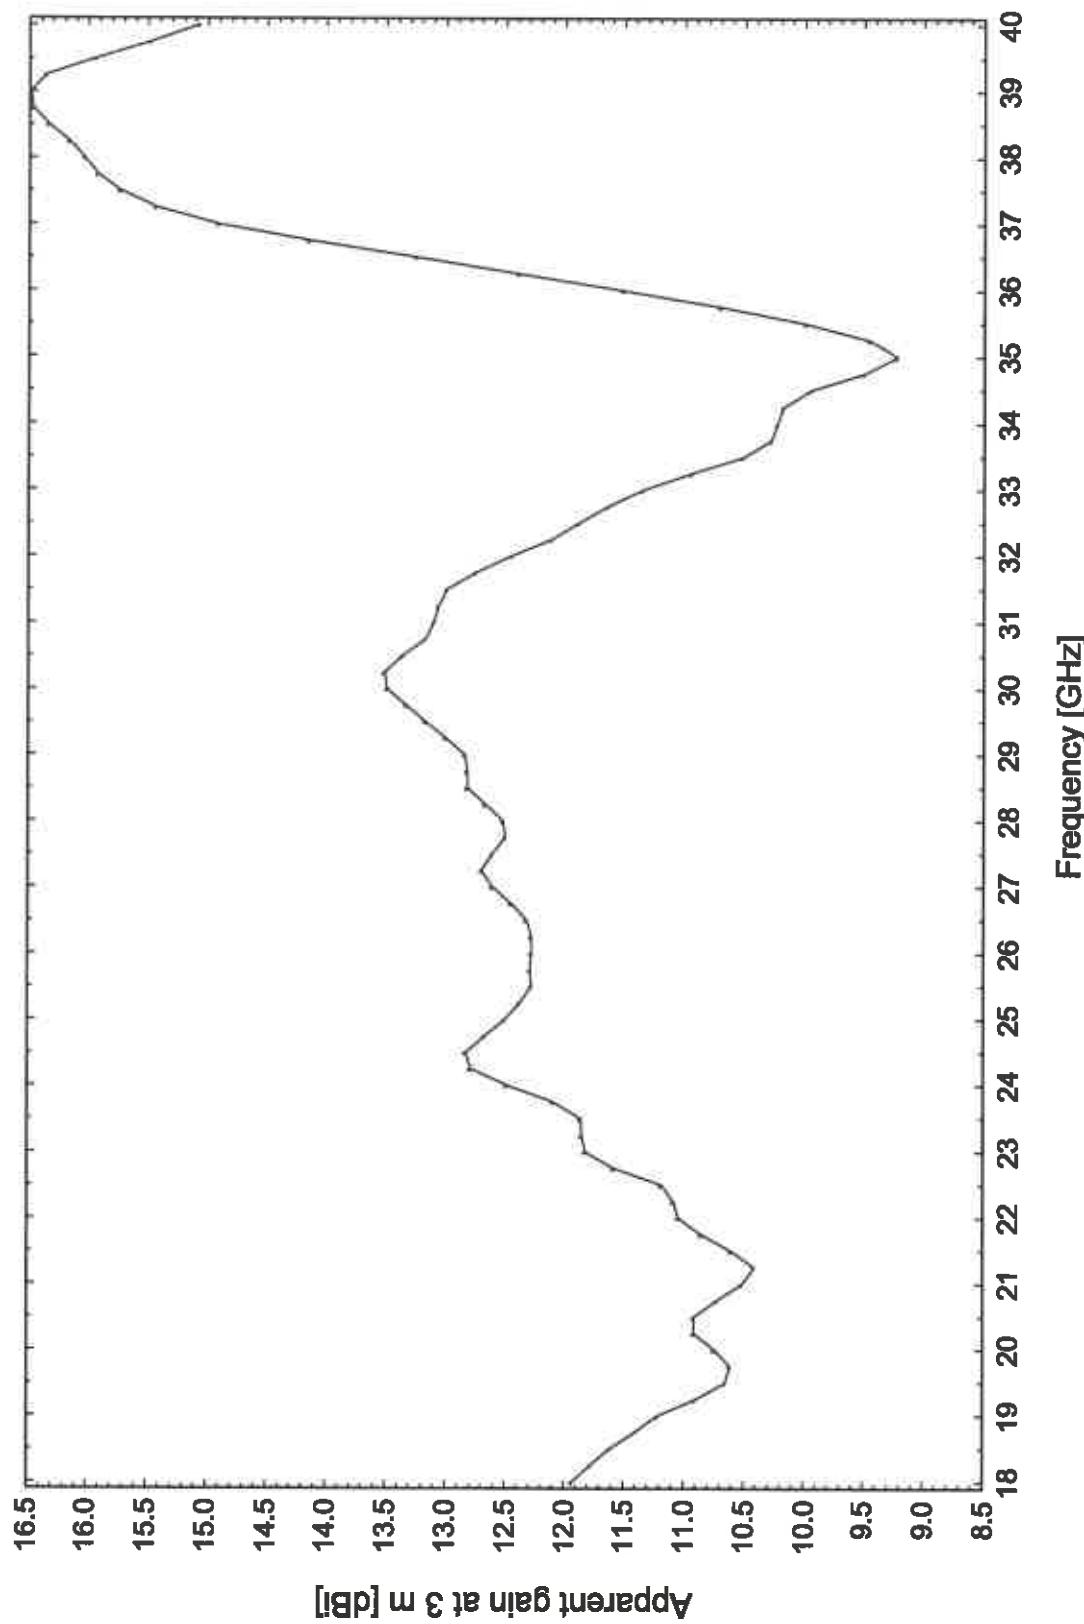

Reference: 2018050459-3

Checked by: *[Signature]*

Page 5 of 5



Radiometer Physics
A Rohde & Schwarz Company

Calibration Certificate

Kalibrierschein

Certificate Number 24-0060-100996-01

Zertifikatsnummer

Unit Data

Item Gegenstand	Harmonic Mixer, 40 GHz to 60 GHz		
Manufacturer Hersteller	RPG		
Type Typ	RPG FS-Z60		
Material Number Materialnummer	1048.0171.02	Serial Number Seriennummer	100996
Asset Number Inventarnummer			

This calibration certificate documents, that the named item is tested and measured against defined specifications. Measurement results are located usually in the corresponding interval with a probability of approx. 95% (coverage factor $k = 2$). Calibration is performed with test equipment and standards directly or indirectly traceable by means of approved calibration techniques to the PTB/DKD or other national/international standards, which realize the physical units of measurement according to the International System of Units (SI). In all cases where no standards are available, measurements are referenced to standards of the R&S laboratories. Principles and methods of calibration correspond with EN ISO/IEC 17025. This calibration certificate may not be reproduced other than in full. Calibration certificates without signatures are not valid. The user is obliged to have the object recalibrated at appropriate intervals.

Order Data

Customer
Auftraggeber

Order Number
Bestellnummer

Date of Receipt
Eingangsdatum

Dieser Kalibrierschein dokumentiert, dass der genannte Gegenstand nach festgelegten Vorgaben geprüft und gemessen wurde. Die Messwerte lagen im Regelfall mit einer Wahrscheinlichkeit von annähernd 95% im zugeordneten Wertebereich (Erweiterte Messunsicherheit mit $k = 2$). Die Kalibrierung erfolgte mit Messmitteln und Normalen, die direkt oder indirekt durch Ableitung mittels anerkannter Kalibriertechniken rückgeführt sind auf Normale der PTB/DKD oder anderer nationaler/internationaler Standards zur Darstellung der physikalischen Einheiten in Übereinstimmung mit dem Internationalen Einheitensystem (SI). Wenn keine Normale existieren, erfolgt die Rückführung auf Bezugsnormale der R&S-Labore. Grundsätze und Verfahren der Kalibrierung beziehen sich auf EN ISO/IEC 17025. Dieser Kalibrierschein darf nur vollständig und unverändert weiterverbreitet werden. Kalibrierscheine ohne Unterschriften sind ungültig. Für die Einhaltung einer angemessenen Frist zur Wiederholung der Kalibrierung ist der Benutzer verantwortlich.

Performance

Place and Date of Calibration
Ort und Datum der Kalibrierung

Meckenheim, 2018-12-04

Scope of Calibration
Umfang der Kalibrierung

Standard Calibration

Statement of Compliance
(Incoming)
Konformitätsaussage
(Anlieferung)

New device

Statement of Compliance
(Outgoing)
Konformitätsaussage
(Auslieferung)

All measured values are within the data sheet specifications.

Extend of Calibration Documents
Umfang des Kalibrierdokuments

2 pages Calibration Certificate
5 pages Outgoing Results

Radiometer Physics GmbH; Meckenheim

Date of Issue
Ausstellungsdatum

Head of Laboratory
Laborleitung

Person Responsible
Bearbeiter

2018-12-05

Schulze

Grossmindorf

Page (Seite) 1/2
Vers2010-05-05/
RPG2014-02-28

Calibration Method
Kalibrieranweisung**RPG-PAQA-TN-2014-002**Relative Humidity 20 % - 80 %
Relative LuftfeuchteAmbient Temperature
Umgebungstemperatur(23 ⁺⁷₋₃) °C
Working standards used (having a significant effect on the accuracy)
 Verwendete Gebrauchsnormale (mit signifikantem Einfluss auf die Genauigkeit)

Item Gegenstand	Type Typ	Serial Number Seriennummer	Calibration Certificate Number Kalibrierscheinnummer	Cal. Due Kalibr. bis
Vector Network Analyzer	R&S® ZVA67	101097	20-300432406	2020-07-21
Powersensor	R&S® NRP-Z55	140093	20-300426315	2019-05-17
Powersensor	R&S® NRP-Z57	101423	20-541799	2019-04-27
Calibration Kit	WR19	U10001	24-0060-U10001-01	2019-02-01

UGB1 A compliance statement may be possible where a confidence level of less than 95 % is acceptable.
 Die Bestätigung der Konformität ist möglich, sofern ein Grad des Vertrauens von weniger als 95 % akzeptabel ist.

UGB2 A non-compliance statement may be possible where a confidence level of less than 95 % is acceptable.
 Die Bestätigung der Nicht-Konformität ist möglich, sofern ein Grad des Vertrauens von weniger als 95 % akzeptabel ist.

Ref.: ILAC-G8:03/2009 'Guidelines on the Reporting of Compliance with Specification'.

Notes
 Anmerkungen


If the new product is stored under the climate conditions as specified in the data sheet upon delivery, the product's accuracy is not significantly affected within 12 month after its calibration in our factory. In this case, the recommended calibration interval starts on the date when the product is actually put into operation.

Outgoing Results

The following abbreviations may be used in this document

- {a} No measurement uncertainty stated because the errors always add together.
So it is sure that a measurement result evaluated as "PASS" is pass.
 - {b} The measurement uncertainty depends on the measurement result. The stated measurement uncertainty is valid for the close area around the specification. Measurement results outside the close area have a higher measurement uncertainty but are within the specification.
 - {c} Functional test, therefore no measurement uncertainty is stated.
 - {d} Typical value, refer to performance test.
 - {e} The measurement uncertainty is taken into account when setting the measuring system.
- DL or DT Data Limit for symmetrical tolerance limits
 DLL Datasheet Lower Limit
 DUL Datasheet Upper Limit
 MU Measurement Uncertainty
 MLL or MLV Measurement Uncertainty Lower Value
 MUL or MUV Measurement Uncertainty Upper Value
 Nom. Nominal Value
 Dev. Deviation
 MErr. Measurement Error
 Act. Actual Value
 UGB Uncertainty Guard Band: Measuring uncertainty violates the data (spec.) limit.
 UGB1 Measurement results marked as UGB1 show conformity with a probability of >50 % and <95 %.
 UGB2 Measurement results marked as UGB2 show non-conformity with a probability of >50 % and <95 %.
 DU Datasheet Uncertainty

Explanation of charts

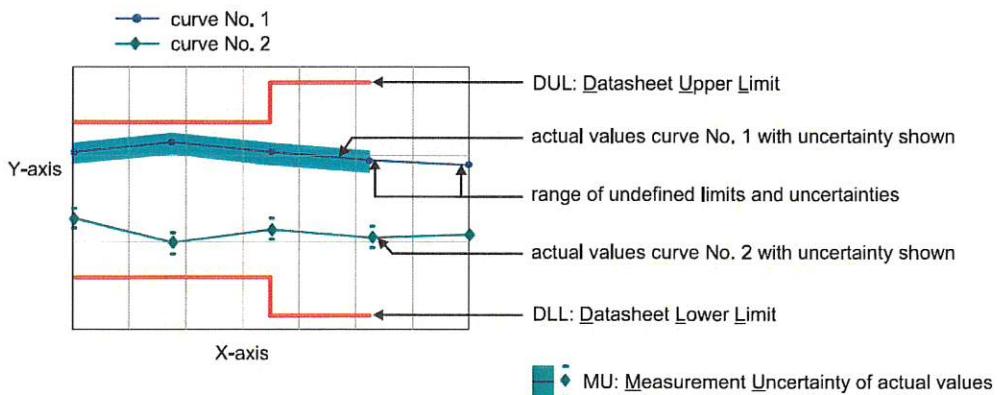


Software used for measurement

Item Type	Version	Remark
Measurement Studio Professional Edition	2013	
MixerCertification	7_09	

1.1 RF Input – VSWR


Measurement uncertainty: 0.05 (VSWR)

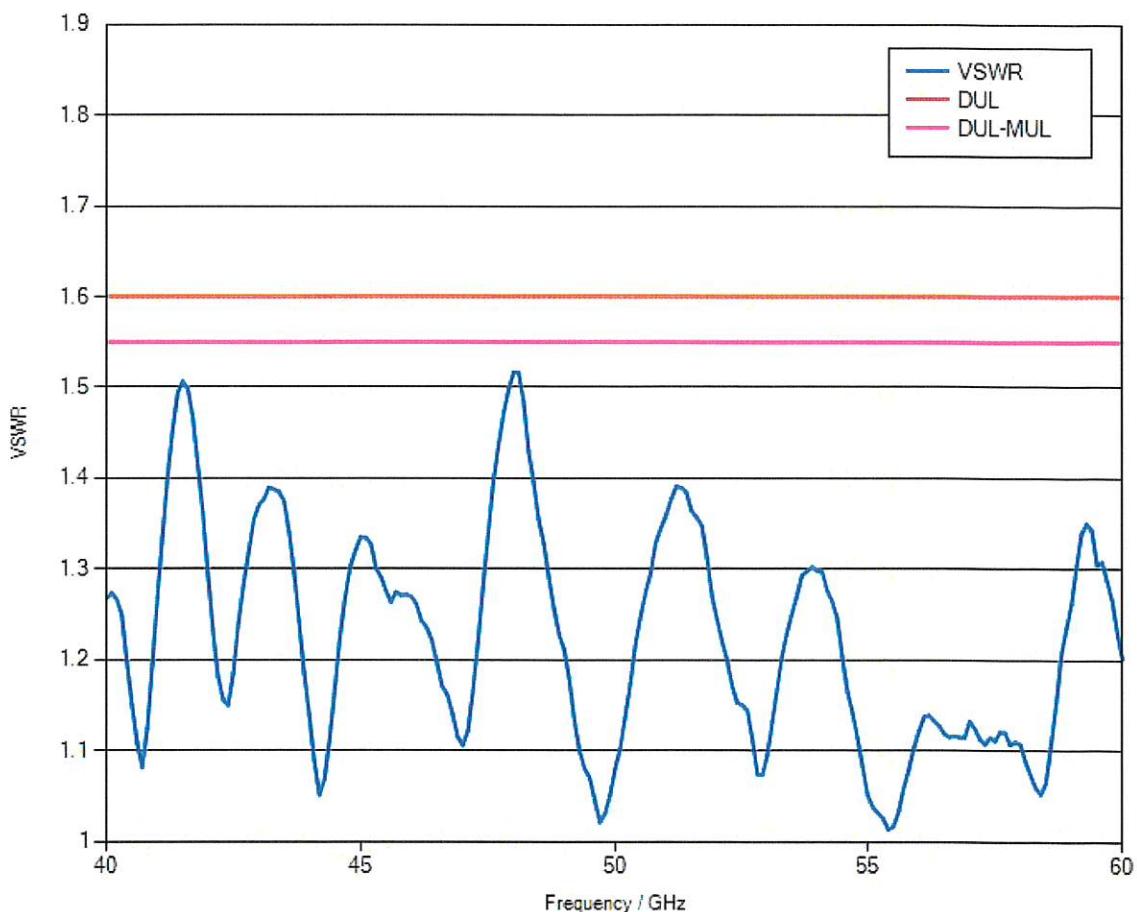

1.2 Conversion loss

LO level +13 dBm nominal
Bias 0 A

Measurement uncertainty: 1.5 dB

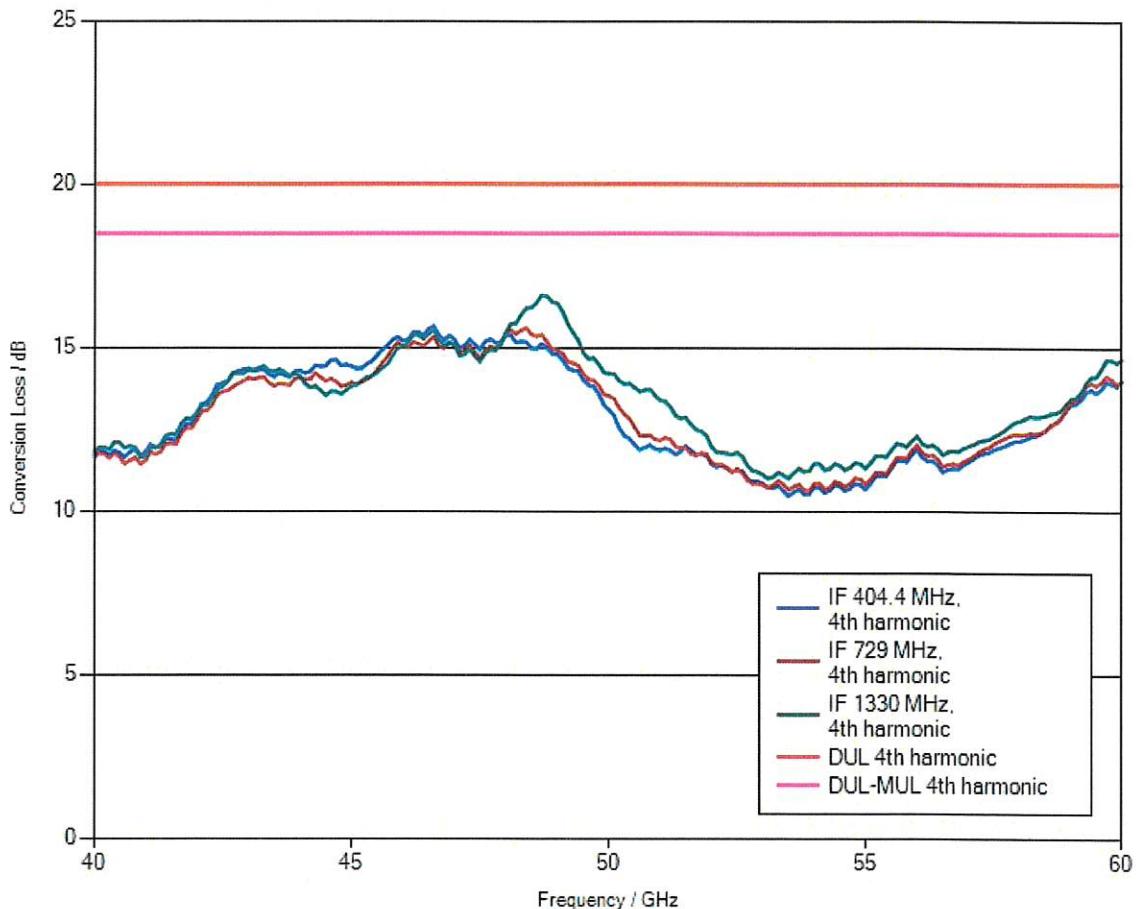

Note: Numeric calibration data can be found attached to the PDF file of the calibration certificate.
Click the “paper clip” symbol to display the file.

The file has been renamed for safety reasons.

When downloading the file onto your PC, please delete the “.file” extension and unzip the data.

1.3 Frequency response within 1 GHz

	DUL	Actual (worst case)	Evaluation
IF = 404.4 MHz, 4th harmonic	4 dB	1.97 dB	PASS
IF = 729 MHz, 4th harmonic	4 dB	1.7 dB	PASS
IF = 1330 MHz, 4th harmonic	4 dB	2.12 dB	PASS



Calibration Certificate

Kalibrierschein

Certificate Number 24-0090-101871-01

Zertifikatsnummer

Unit Data

Item Gegenstand	Harmonic Mixer, 60 GHz to 90 GHz		
Manufacturer Hersteller	ROHDE & SCHWARZ		
Type Typ	R&S® FS-Z90		
Material Number Materialnummer	1048.0371.02	Serial Number Seriennummer	101871
Asset Number Inventarnummer			

This calibration certificate documents, that the named item is tested and measured against defined specifications. Measurement results are located usually in the corresponding interval with a probability of approx. 95% (coverage factor k = 2). Calibration is performed with test equipment and standards directly or indirectly traceable by means of approved calibration techniques to the PTB/DKD or other national/international standards, which realize the physical units of measurement according to the International System of Units (SI). In all cases where no standards are available, measurements are referenced to standards of the R&S laboratories. Principles and methods of calibration correspond with EN ISO/IEC 17025. This calibration certificate may not be reproduced other than in full. Calibration certificates without signatures are not valid. The user is obliged to have the object recalibrated at appropriate intervals.

Order Data

Customer Auftraggeber

Order Number
Bestellnummer

Date of Receipt
Eingangsdatum

Dieser Kalibrierschein dokumentiert, dass der genannte Gegenstand nach festgelegten Vorgaben geprüft und gemessen wurde. Die Messwerte lagen im Regelfall mit einer Wahrscheinlichkeit von annähernd 95% im zugeordneten Wertebereich (Erweiterte Messunsicherheit mit k = 2). Die Kalibrierung erfolgte mit Messmitteln und Normalen, die direkt oder indirekt durch Ableitung mittels anerkannter Kalibriertechniken rückgeführt sind auf Normale der PTB/DKD oder anderer nationaler/internationaler Standards zur Darstellung der physikalischen Einheiten in Übereinstimmung mit dem Internationalen Einheitensystem (SI). Wenn keine Normale existieren, erfolgt die Rückführung auf Bezugsnormale der R&S-Labore. Grundsätze und Verfahren der Kalibrierung beziehen sich auf EN ISO/IEC 17025. Dieser Kalibrierschein darf nur vollständig und unverändert weiterverbreitet werden. Kalibrierscheine ohne Unterschriften sind ungültig. Für die Einhaltung einer angemessenen Frist zur Wiederholung der Kalibrierung ist der Benutzer verantwortlich.

Performance

Place and Date of Calibration
Ort und Datum der Kalibrierung

Meckenheim, 2019-01-10

Scope of Calibration
Umfang der Kalibrierung

Standard Calibration

Statement of Compliance
(Incoming)
Konformitätsaussage
(Anlieferung)

New device

Statement of Compliance
(Outgoing)
Konformitätsaussage
(Auslieferung)

All measured values are within the data sheet specifications.

Extend of Calibration Documents
Umfang des Kalibrierdokuments

2 pages Calibration Certificate
5 pages Outgoing Results

Radiometer Physics GmbH; Meckenheim

Date of Issue
Ausstellungsdatum

Head of Laboratory
Laborleiter

Person Responsible
Bearbeiter

2019-01-11

Schulze

Heinze

Page (Seite) 1/2
Vers2010-05-05/
RPG2014-02-28

Calibration Method
Kalibrieranweisung**RPG-PAQA-TN-2014-002**Relative Humidity 20 % - 80 %
Relative LuftfeuchteAmbient Temperature
Umgebungstemperatur(23 ⁺⁷₋₃) °C

Working standards used (having a significant effect on the accuracy)
 Verwendete Gebrauchsnormale (mit signifikantem Einfluss auf die Genauigkeit)

Item Gegenstand	Type Typ	Serial Number Seriennummer	Calibration Certificate Number Kalibrierscheinnummer	Cal. Due Kalibr. bis
Vector Network Analyzer	R&S® ZVA67	101097	20-300432406	2020-07-21
Powersensor	R&S® NRP-Z55	140093	20-300426315	2019-05-17
Powersensor	R&S® NRP-Z58	101063	0001-300474490	2019-08-06
Calibration kit	WR12	E10001	RPG-PAQA-TN-2014-005	2019-02-01

UGB1 A compliance statement may be possible where a confidence level of less than 95 % is acceptable.
 Die Bestätigung der Konformität ist möglich, sofern ein Grad des Vertrauens von weniger als 95 % akzeptabel ist.

UGB2 A non-compliance statement may be possible where a confidence level of less than 95 % is acceptable.
 Die Bestätigung der Nicht-Konformität ist möglich, sofern ein Grad des Vertrauens von weniger als 95 % akzeptabel ist.

Ref.: ILAC-G8:03/2008 'Guidelines on the Reporting of Compliance with Specification'.

Notes
Anmerkungen


If the new product is stored under the climate conditions as specified in the data sheet upon delivery, the product's accuracy is not significantly affected within 12 month after its calibration in our factory. In this case, the recommended calibration interval starts on the date when the product is actually put into operation.

Outgoing Results

The following abbreviations may be used in this document

- {a} No measurement uncertainty stated because the errors always add together.
So it is sure that a measurement result evaluated as "PASS" is pass.
 - {b} The measurement uncertainty depends on the measurement result. The stated measurement uncertainty is valid for the close area around the specification. Measurement results outside the close area have a higher measurement uncertainty but are within the specification.
 - {c} Functional test, therefore no measurement uncertainty is stated.
 - {d} Typical value, refer to performance test.
 - {e} The measurement uncertainty is taken into account when setting the measuring system.
- DL or DT Data Limit for symmetrical tolerance limits
 DLL Datasheet Lower Limit
 DUL Datasheet Upper Limit
 MU Measurement Uncertainty
 MLL or MLV Measurement Uncertainty Lower Value
 MUL or MUV Measurement Uncertainty Upper Value
 Nom. Nominal Value
 Dev. Deviation
 MErr. Measurement Error
 Act. Actual Value
 UGB Uncertainty Guard Band: Measuring uncertainty violates the data (spec.) limit.
 UGB1 Measurement results marked as UGB1 show conformity with a probability of >50 % and <95 %.
 UGB2 Measurement results marked as UGB2 show non-conformity with a probability of >50 % and <95 %.
 DU Datasheet Uncertainty

Explanation of charts

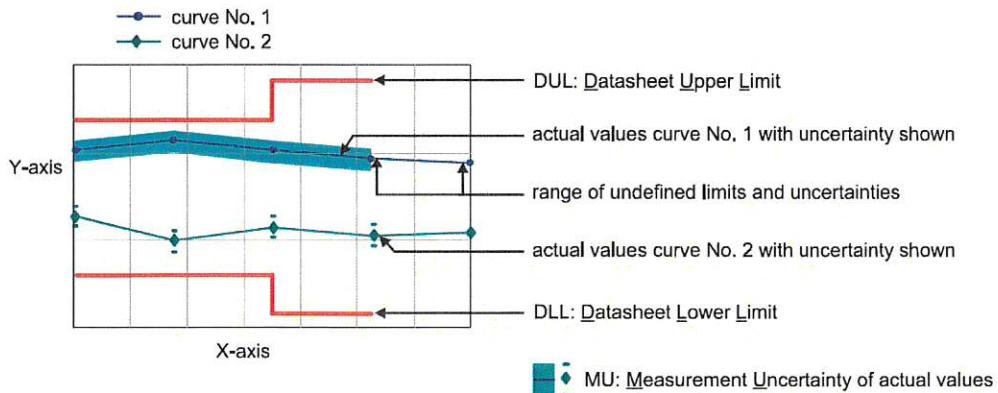


Software used for measurement

Item Type	Version	Remark
Measurement Studio Professional Edition	2013	
MixerCertification	7_09	

1.1 RF Input – VSWR


Measurement uncertainty: 0.05 (VSWR)

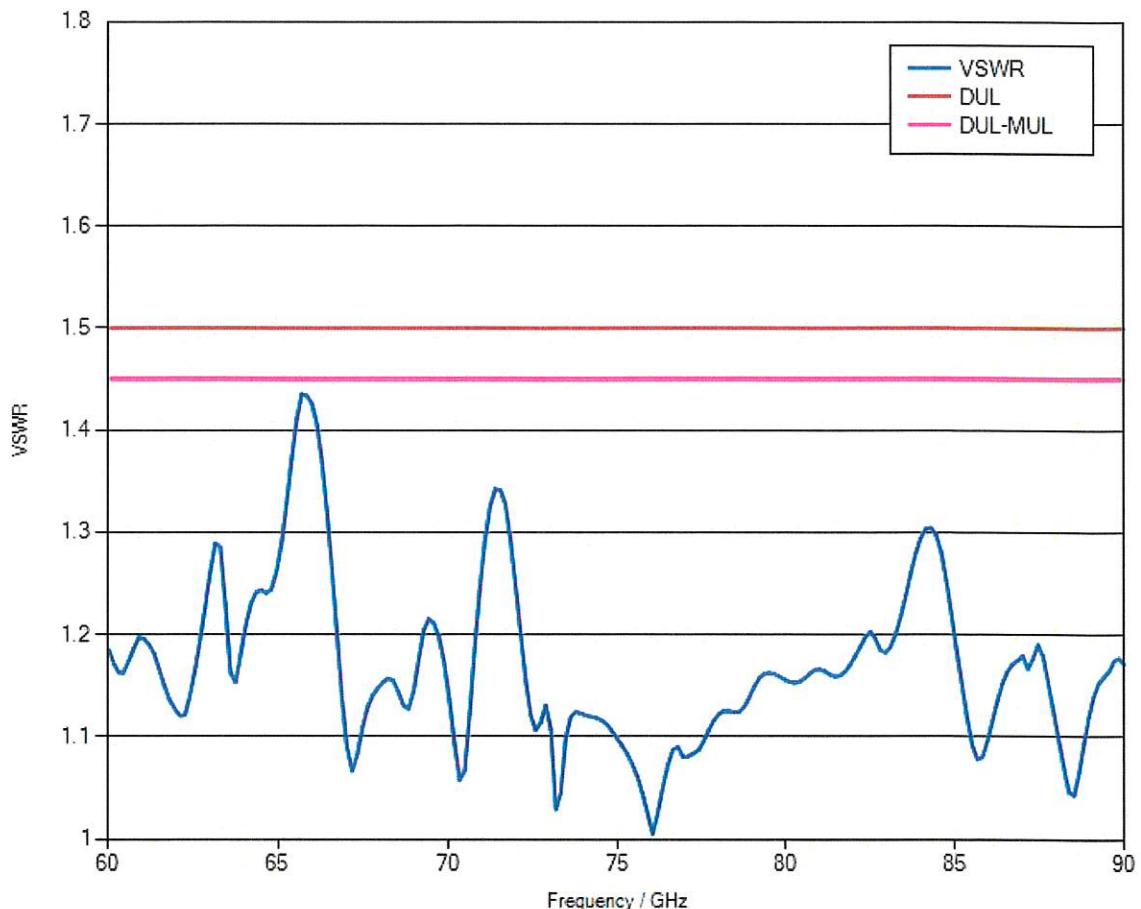

1.2 Conversion loss

LO level +14 dBm nominal
Bias 0 A

Measurement uncertainty: 1.5 dB

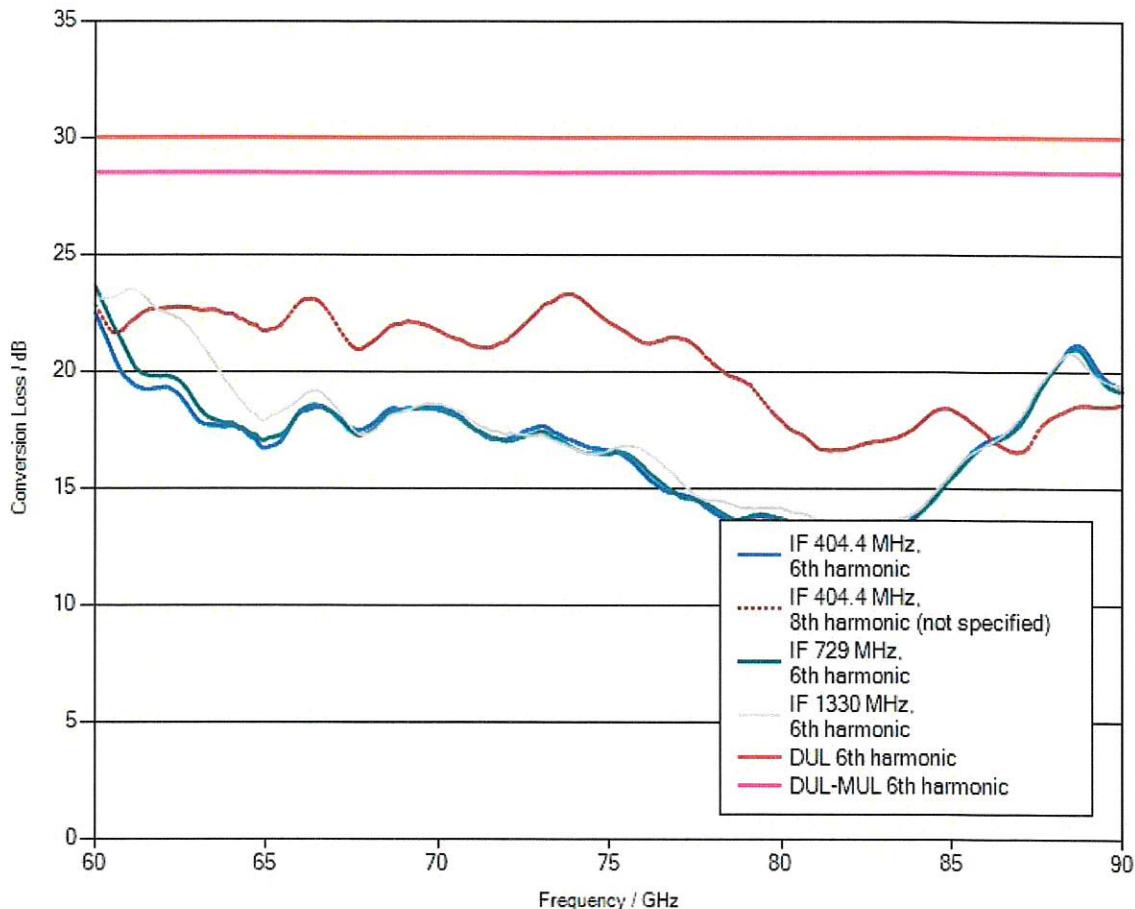

Note: Numeric calibration data can be found attached to the PDF file of the calibration certificate.
Click the “paper clip” symbol to display the file.

The file has been renamed for safety reasons.
When downloading the file onto your PC, please delete the “.file” extension and unzip the data.

1.3 Frequency response within 1 GHz

	DUL	Actual (worst case)	Evaluation
IF = 404.4 MHz, 6th harmonic	6 dB	2.76 dB	PASS
IF = 404.4 MHz, 8th harmonic	not specified	1.83 dB	not specified
IF = 729 MHz, 6th harmonic	6 dB	2.71 dB	PASS
IF = 1330 MHz, 6th harmonic	6 dB	2.02 dB	PASS



Calibration Certificate

Kalibrierschein

Certificate Number 24-0110-101467-02

Zertifikatsnummer

Unit Data

Item Gegenstand	Harmonic Mixer, 75 GHz to 110 GHz		
Manufacturer Hersteller	ROHDE & SCHWARZ		
Type Typ	R&S® FS-Z110		
Material Number Materialnummer	1048.0471.02	Serial Number Seriennummer	101467
Asset Number Inventarnummer			

This calibration certificate documents, that the named item is tested and measured against defined specifications. Measurement results are located usually in the corresponding interval with a probability of approx. 95% (coverage factor $k = 2$). Calibration is performed with test equipment and standards directly or indirectly traceable by means of approved calibration techniques to the PTB/DKD or other national/international standards, which realize the physical units of measurement according to the International System of Units (SI). In all cases where no standards are available, measurements are referenced to standards of the R&S laboratories. Principles and methods of calibration correspond with EN ISO/IEC 17025. This calibration certificate may not be reproduced other than in full. Calibration certificates without signatures are not valid. The user is obliged to have the object recalibrated at appropriate intervals.

Order Data

Customer Auftraggeber	RISE Research Institutes of Sweden AB Brinellgatan 4 504 62 Boras Sweden
--------------------------	---

Order Number Bestellnummer	8800000961
Date of Receipt Eingangsdatum	2018-07-16

Performance

Place and Date of Calibration Ort und Datum der Kalibrierung	Meckenheim, 2018-07-23
Scope of Calibration Umfang der Kalibrierung	Standard Calibration
Statement of Compliance (Incoming) Konformitätsaussage (Anlieferung)	All measured values are <u>within the data sheet specifications.</u>

Statement of Compliance (Outgoing) Konformitätsaussage (Auslieferung)	All measured values are <u>within the data sheet specifications.</u>
Extend of Calibration Documents Umfang des Kalibrierdokuments	2 pages Calibration Certificate 5 pages Outgoing Results 3 pages Incoming Results

2 pages Calibration Certificate 5 pages Outgoing Results 3 pages Incoming Results

Dieser Kalibrierschein dokumentiert, dass der genannte Gegenstand nach festgelegten Vorgaben geprüft und gemessen wurde. Die Messwerte liegen im Regelfall mit einer Wahrscheinlichkeit von annähernd 95% im zugeordneten Wertebereich (Erweiterte Messunsicherheit mit $k = 2$). Die Kalibrierung erfolgte mit Messmitteln und Normalen, die direkt oder indirekt durch Ableitung mittels anerkannter Kalibriertechniken rückgeführt sind auf Normale der PTB/DKD oder anderer national/internationaler Standards zur Darstellung der physikalischen Einheiten in Übereinstimmung mit dem Internationalen Einheitensystem (SI). Wenn keine Normale existieren, erfolgt die Rückführung auf Bezugsnormale der R&S-Labore. Grundsätze und Verfahren der Kalibrierung beziehen sich auf EN ISO/IEC 17025. Dieser Kalibrierschein darf nur vollständig und unverändert weiterverbreitet werden. Kalibrierscheine ohne Unterschriften sind ungültig. Für die Einhaltung einer angemessenen Frist zur Wiederholung der Kalibrierung ist der Benutzer verantwortlich.

Radiometer Physics GmbH; Meckenheim

Date of Issue
Ausstellungsdatum

2018-07-23

Head of Laboratory
Laborleitung

Schulze

Person Responsible
Bearbeiter

Gottbehuet

Page (Seite) 1/2
Vers2010-05-05/
RPG2014-02-28

Calibration Method
Kalibrieranweisung**RPG-PAQA-TN-2014-002**Relative Humidity 20 % - 80 %
RelativeLuftfeuchteAmbient Temperature
Umgebungstemperatur(23 ⁺⁷₋₃) °C

Working standards used (having a significant effect on the accuracy) Verwendete Gebrauchsnormale (mit signifikantem Einfluss auf die Genauigkeit)				
Item Gegenstand	Type Typ	Serial Number Seriennummer	Calibration Certificate Number Kalibrierscheinnummer	Cal. Due Kalibr. bis
Vector Network Analyzer	R&S® ZVA67	101097	20-300432406	2020-07-21
Powersensor	R&S® NRP-Z55	140093	20-300426315	2019-05-17
Powersensor	R&S® NRP-Z58	100886	0033_D-K-15195-01-01_2018-05	2019-05-02
Calibration kit	WR10	W10001	RPG-PAQA-TN-2014-005	2019-02-01

UGB1 A compliance statement may be possible where a confidence level of less than 95 % is acceptable.
Die Bestätigung der Konformität ist möglich, sofern ein Grad des Vertrauens von weniger als 95 % akzeptabel ist.

UGB2 A non-compliance statement may be possible where a confidence level of less than 95 % is acceptable.
Die Bestätigung der Nicht-Konformität ist möglich, sofern ein Grad des Vertrauens von weniger als 95 % akzeptabel ist.

Ref.: ILAC-G8:03/2009 'Guidelines on the Reporting of Compliance with Specification'.

Notes Anmerkungen


If the new product is stored under the climate conditions as specified in the data sheet upon delivery, the product's accuracy is not significantly affected within 12 month after its calibration in our factory. In this case, the recommended calibration interval starts on the date when the product is actually put into operation.

Outgoing Results

The following abbreviations may be used in this document

{a}	No measurement uncertainty stated because the errors always add together. So it is sure that a measurement result evaluated as "PASS" is pass.
{b}	The measurement uncertainty depends on the measurement result. The stated measurement uncertainty is valid for the close area around the specification. Measurement results outside the close area have a higher measurement uncertainty but are within the specification.
{c}	Functional test, therefore no measurement uncertainty is stated.
{d}	Typical value, refer to performance test.
{e}	The measurement uncertainty is taken into account when setting the measuring system.
DL or DT	Data Limit for symmetrical tolerance limits
DLL	Datasheet Lower Limit
DUL	Datasheet Upper Limit
MU	Measurement Uncertainty
MLL or MLV	Measurement Uncertainty Lower Value
MUL or MUU	Measurement Uncertainty Upper Value
Nom.	Nominal Value
Dev.	Deviation
MErr.	Measurement Error
Act.	Actual Value
UGB	Uncertainty Guard Band: Measuring uncertainty violates the data (spec.) limit.
UGB1	Measurement results marked as UGB1 show conformity with a probability of >50 % and <95 %.
UGB2	Measurement results marked as UGB2 show non-conformity with a probability of >50 % and <95 %.
DU	Datasheet Uncertainty

Explanation of charts

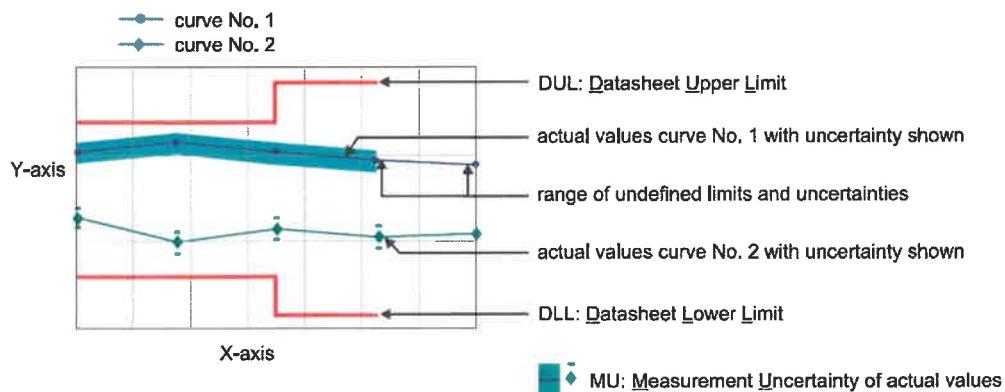

Software used for measurement**Item Type**

Measurement Studio Professional Edition
MixerCertification


Version

2013
7_08

Remark

1.1 RF Input – VSWR


Measurement uncertainty: 0.05 (VSWR)

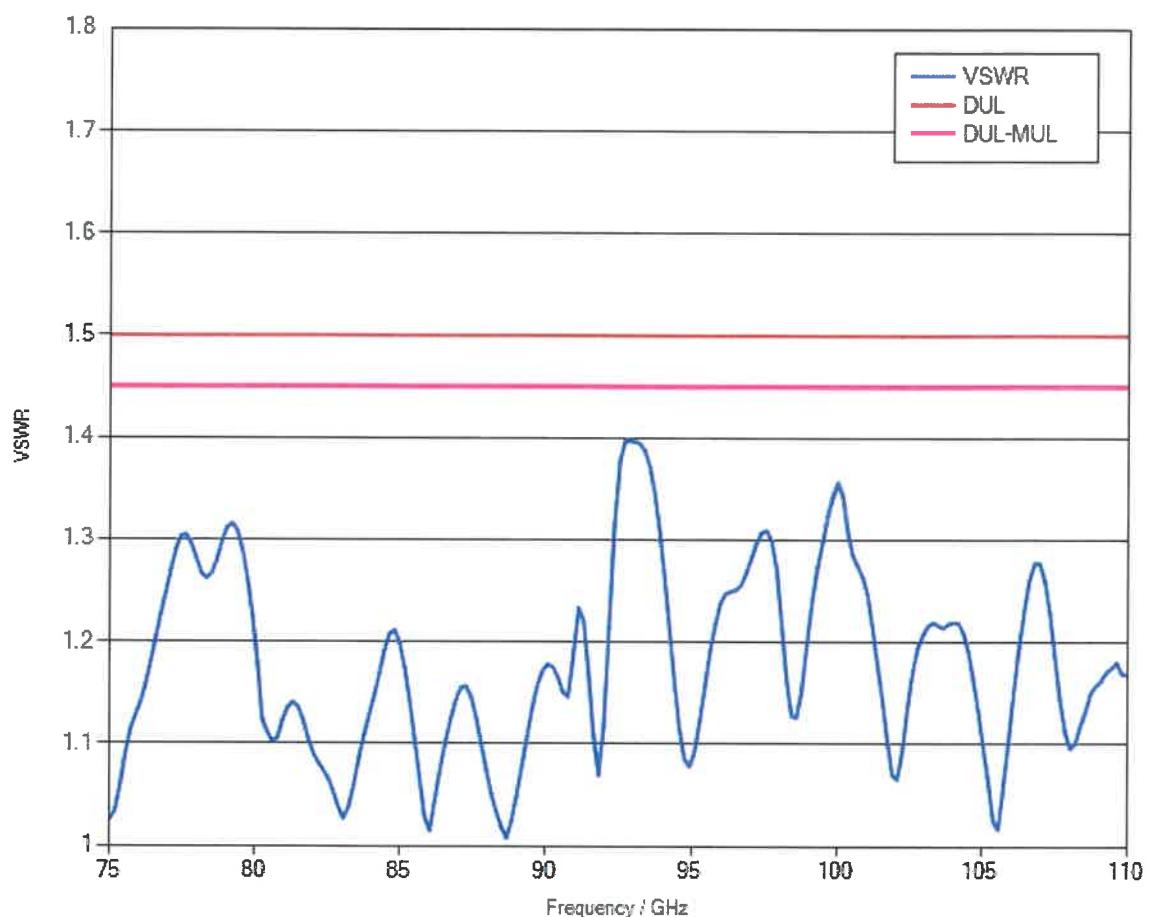

1.2 Conversion loss

LO level +15.5 dBm nominal
Bias 0 A

Measurement uncertainty: 1.6 dB

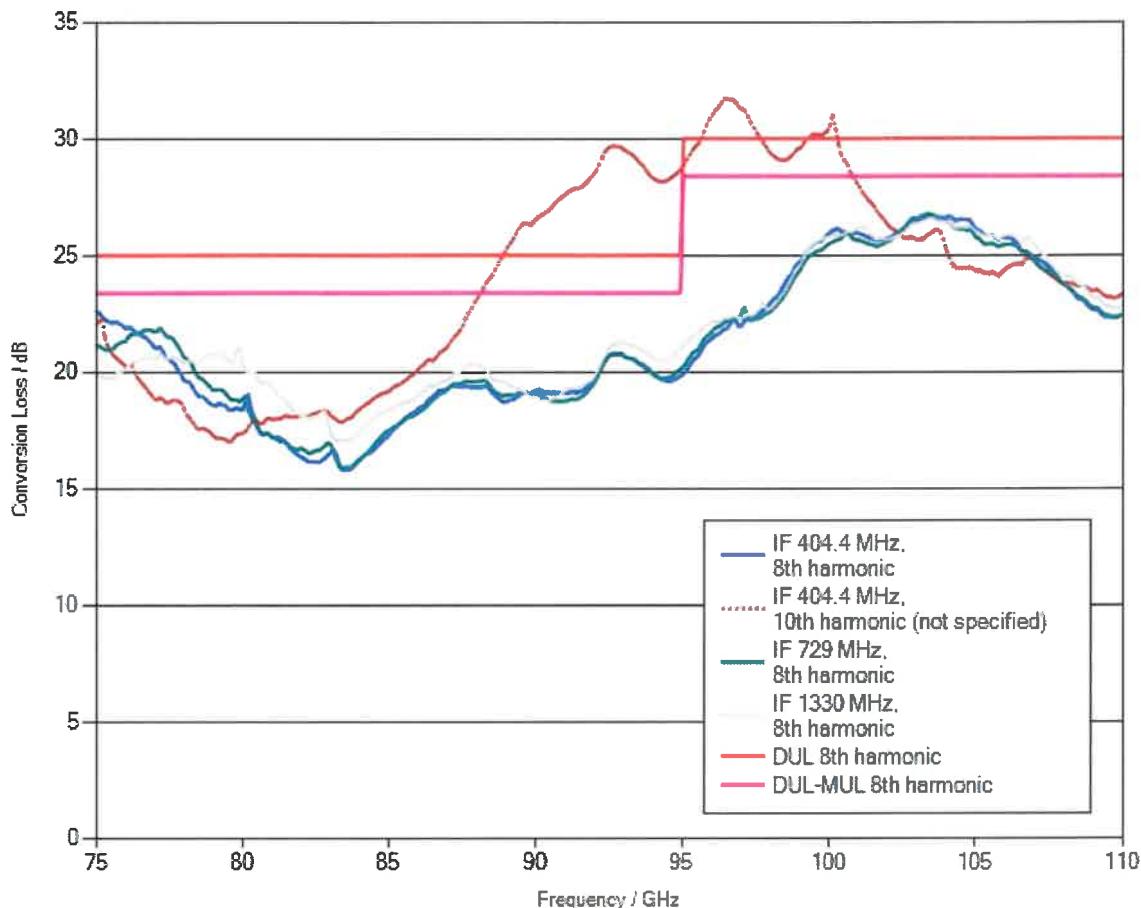

Note: Numeric calibration data can be found attached to the PDF file of the calibration certificate.
Click the “paper clip” symbol to display the file.

The file has been renamed for safety reasons.

When downloading the file onto your PC, please delete the “.file” extension and unzip the data.

1.3 Frequency response within 1 GHz


	DUL	Actual (worst case)	Evaluation
IF = 404.4 MHz, 8th harmonic	6 dB	1.93 dB	PASS
IF = 404.4 MHz, 10th harmonic	not specified	3.31 dB	not specified
IF = 729 MHz, 8th harmonic	6 dB	1.97 dB	PASS
IF = 1330 MHz, 8th harmonic	6 dB	2.11 dB	PASS

1 Incoming Results

The following abbreviations may be used in this document

{a}	No measurement uncertainty stated because the errors always add together. So it is sure that a measurement result evaluated as "PASS" is pass.
{b}	The measurement uncertainty depends on the measurement result. The stated measurement uncertainty is valid for the close area around the specification. Measurement results outside the close area have a higher measurement uncertainty but are within the specification.
{c}	Functional test, therefore no measurement uncertainty is stated.
{d}	Typical value, refer to performance test.
{e}	The measurement uncertainty is taken into account when setting the measuring system.
DL or DT	Data Limit for symmetrical tolerance limits
DLL	Datasheet Lower Limit
DUL	Datasheet Upper Limit
MU	Measurement Uncertainty
MLL or MLV	Measurement Uncertainty Lower Value
MUL or MUV	Measurement Uncertainty Upper Value
Nom.	Nominal Value
Dev.	Deviation
MErr.	Measurement Error
Act.	Actual Value
UGB	Uncertainty Guard Band: Measuring uncertainty violates the data (spec.) limit.
UGB1	Measurement results marked as UGB1 show conformity with a probability of >50 % and <95 %.
UGB2	Measurement results marked as UGB2 show non-conformity with a probability of >50 % and <95 %.
DU	Datasheet Uncertainty

Explanation of charts

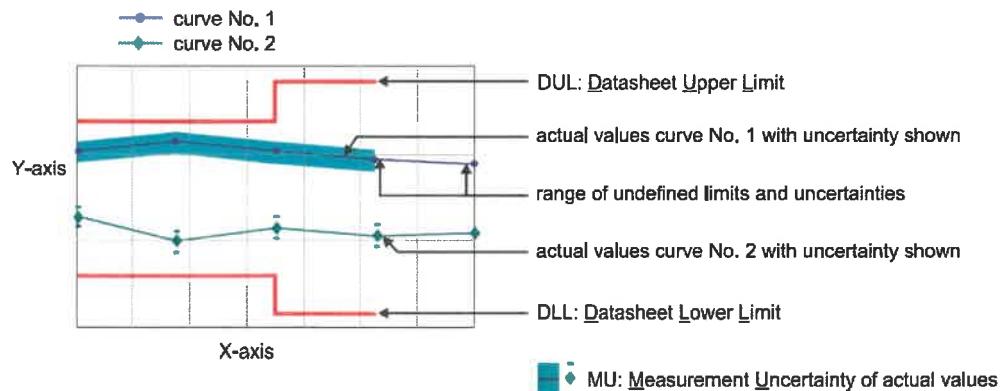

Material Number 1048.0471.02

Serial Number 101467

Certificate Number 24-0110-101467-02

(Incoming)


Software used for measurement

Item Type	Version
Measurement Studio Professional Edition	2013
MixerCertification	7_08

Remark

Incoming Report

1.1 Deviation between actual and previous conversion loss

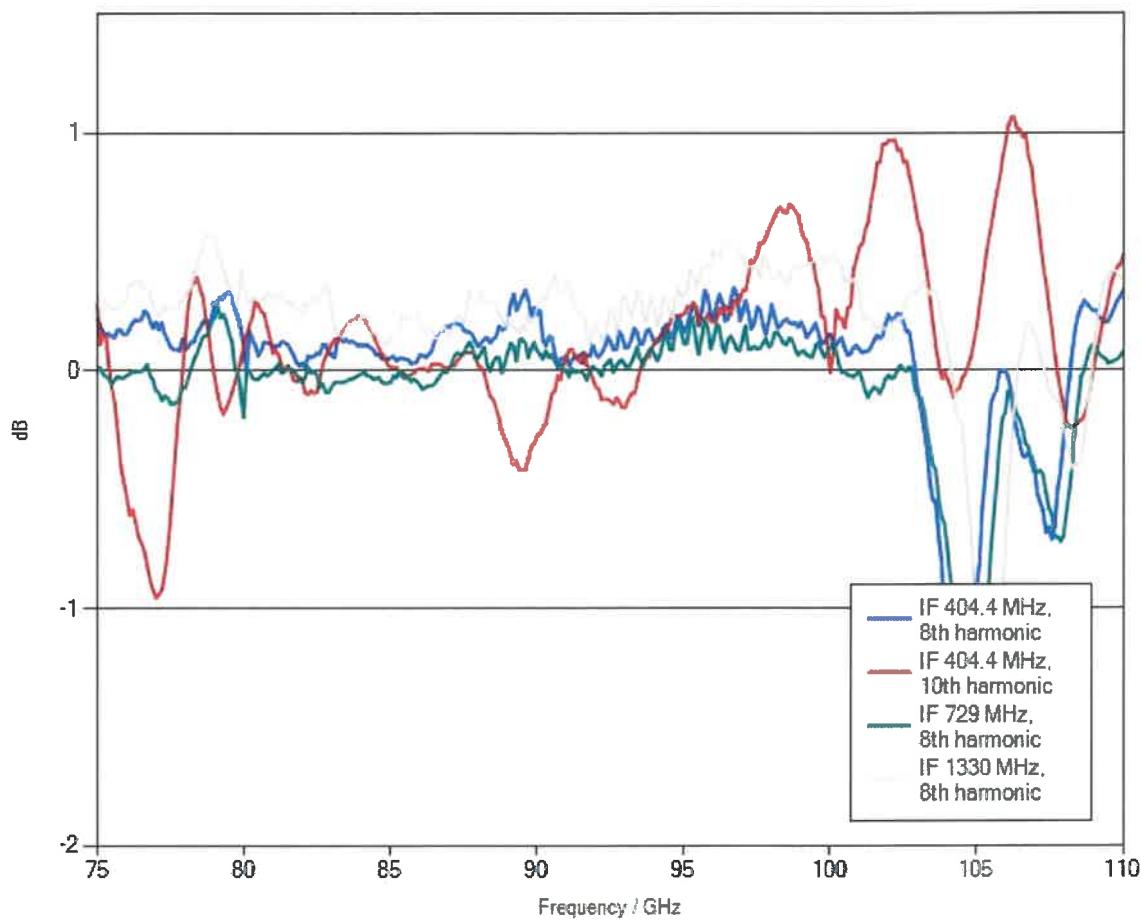



Calibration Certificate

Kalibrierschein

Certificate Number 24-0170-100974-01

Zertifikatsnummer

Unit Data

Item Gegenstand	Harmonic Mixer, 110 GHz to 170 GHz		
Manufacturer Hersteller	RPG		
Type Typ	RPG FS-Z170		
Material Number Materialnummer	3622.0714.02	Serial Number Seriennummer	100974
Asset Number Inventarnummer			

This calibration certificate documents, that the named item is tested and measured against defined specifications. Measurement results are located usually in the corresponding interval with a probability of approx. 95% (coverage factor $k = 2$). Calibration is performed with test equipment and standards directly or indirectly traceable by means of approved calibration techniques to the PTB/DKD or other national/international standards, which realize the physical units of measurement according to the International System of Units (SI). In all cases where no standards are available, measurements are referenced to standards of the R&S laboratories. Principles and methods of calibration correspond with EN ISO/IEC 17025. This calibration certificate may not be reproduced other than in full. Calibration certificates without signatures are not valid. The user is obliged to have the object recalibrated at appropriate intervals.

Order Data

Customer Auftraggeber

Order Number Bestellnummer

Date of Receipt Eingangsdatum

Performance

Place and Date of Calibration Ort und Datum der Kalibrierung	Meckenheim, 2018-02-05
---	------------------------

Scope of Calibration Umfang der Kalibrierung	Standard Calibration
---	----------------------

Statement of Compliance (Incoming) Konformitätsaussage (Anlieferung)	New device
---	------------

Statement of Compliance (Outgoing) Konformitätsaussage (Auslieferung)	All measured values are <u>within the data sheet specifications.</u>
--	--

Extend of Calibration Documents Umfang des Kalibrierdokuments	2 pages Calibration Certificate 5 pages Outgoing Results
--	---

Dieser Kalibrierschein dokumentiert, dass der genannte Gegenstand nach festgelegten Vorgaben geprüft und gemessen wurde. Die Messwerte lagen im Regelfall mit einer Wahrscheinlichkeit von annähernd 95% im zugeordneten Wertebereich (Erweiterte Messunsicherheit mit $k = 2$). Die Kalibrierung erfolgte mit Messmitteln und Normalen, die direkt oder indirekt durch Ableitung mittels anerkannter Kalibriermethoden rückgeführt sind auf Normale der PTB/DKD oder anderer national/internationaler Standards zur Darstellung der physikalischen Einheiten in Übereinstimmung mit dem Internationalen Einheitensystem (SI). Wenn keine Normale existieren, erfolgt die Rückführung auf Bezugsnormale der R&S-Labore. Grundsätze und Verfahren der Kalibrierung beziehen sich auf EN ISO/IEC 17025. Dieser Kalibrierschein darf nur vollständig und unverändert weiterverbreitet werden. Kalibrierscheine ohne Unterschriften sind ungültig. Für die Einhaltung einer angemessenen Frist zur Wiederholung der Kalibrierung ist der Benutzer verantwortlich.

Radiometer Physics GmbH; Meckenheim

Date of Issue Ausstellungsdatum

Head of Laboratory Laborleitungen

Person Responsible Bearbeiter

2018-02-05

Schulze

Dick

Calibration Method
Kalibrieranweisung

RPG-PAQA-TN-2014-002

Relative Humidity 20 % - 80 %
Relative Luftfeuchte

Ambient Temperature
Umgebungstemperatur

(23 ⁺⁷) °C

Working standards used (having a significant effect on the accuracy)
Verwendete Gebrauchsnormale (mit signifikantem Einfluss auf die Genauigkeit)

Item Gegenstand	Type Typ	Serial Number Seriennummer	Calibration Certificate Number Kalibrierscheinnummer	Cal. Due Kalibr. bis
Vector Network Analyzer Powersensor	R&S® ZVA67 R&S® NRP-Z55	101097 140093	20-300432406 20-300426315	2020-07-21 2018-05-17

UGB1 A compliance statement may be possible where a confidence level of less than 95 % is acceptable.
Die Bestätigung der Konformität ist möglich, sofern ein Grad des Vertrauens von weniger als 95 % akzeptabel ist.

UGB2 A non-compliance statement may be possible where a confidence level of less than 95 % is acceptable.
Die Bestätigung der Nicht-Konformität ist möglich, sofern ein Grad des Vertrauens von weniger als 95 % akzeptabel ist.

Ref.: ILAC-G8:03/2009 'Guidelines on the Reporting of Compliance with Specification'.

Notes
Anmerkungen


If the new product is stored under the climate conditions as specified in the data sheet upon delivery, the product's accuracy is not significantly affected within 12 month after its calibration in our factory. In this case, the recommended calibration interval starts on the date when the product is actually put into operation.

Outgoing Results

The following abbreviations may be used in this document

- {a} No measurement uncertainty stated because the errors always add together.
So it is sure that a measurement result evaluated as "PASS" is pass.
 - {b} The measurement uncertainty depends on the measurement result. The stated measurement uncertainty is valid for the close area around the specification. Measurement results outside the close area have a higher measurement uncertainty but are within the specification.
 - {c} Functional test, therefore no measurement uncertainty is stated.
 - {d} Typical value, refer to performance test.
 - {e} The measurement uncertainty is taken into account when setting the measuring system.
- DL or DT Data Limit for symmetrical tolerance limits
 DLL Datasheet Lower Limit
 DUL Datasheet Upper Limit
 MU Measurement Uncertainty
 MLL or MLV Measurement Uncertainty Lower Value
 MUL or MUV Measurement Uncertainty Upper Value
 Nom. Nominal Value
 Dev. Deviation
 MErr. Measurement Error
 Act. Actual Value
 UGB Uncertainty Guard Band: Measuring uncertainty violates the data (spec.) limit.
 UGB1 Measurement results marked as UGB1 show conformity with a probability of >50 % and <95 %.
 UGB2 Measurement results marked as UGB2 show non-conformity with a probability of >50 % and <95 %.
 DU Datasheet Uncertainty

Explanation of charts

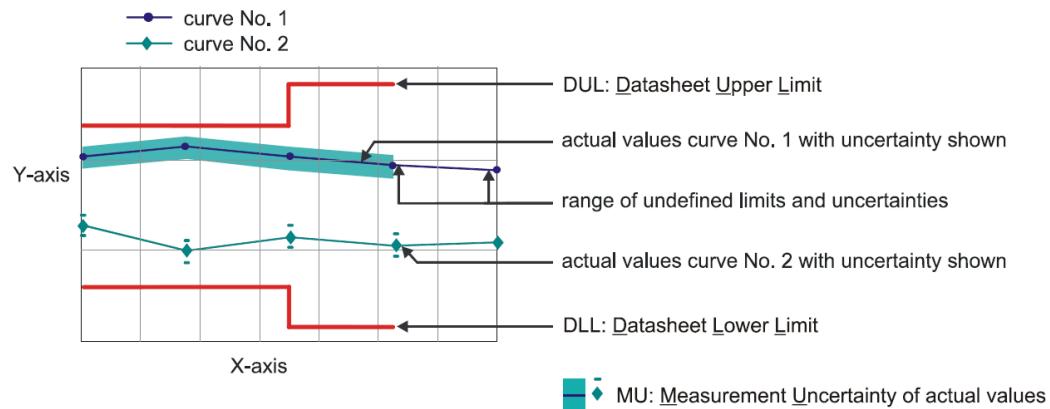

Software used for measurement**Item Type**

Measurement Studio Professional Edition
MixerCertification


Version

2013
7_08

Remark

1.1 RF Input – VSWR


Measurement uncertainty: 0.05 (VSWR)

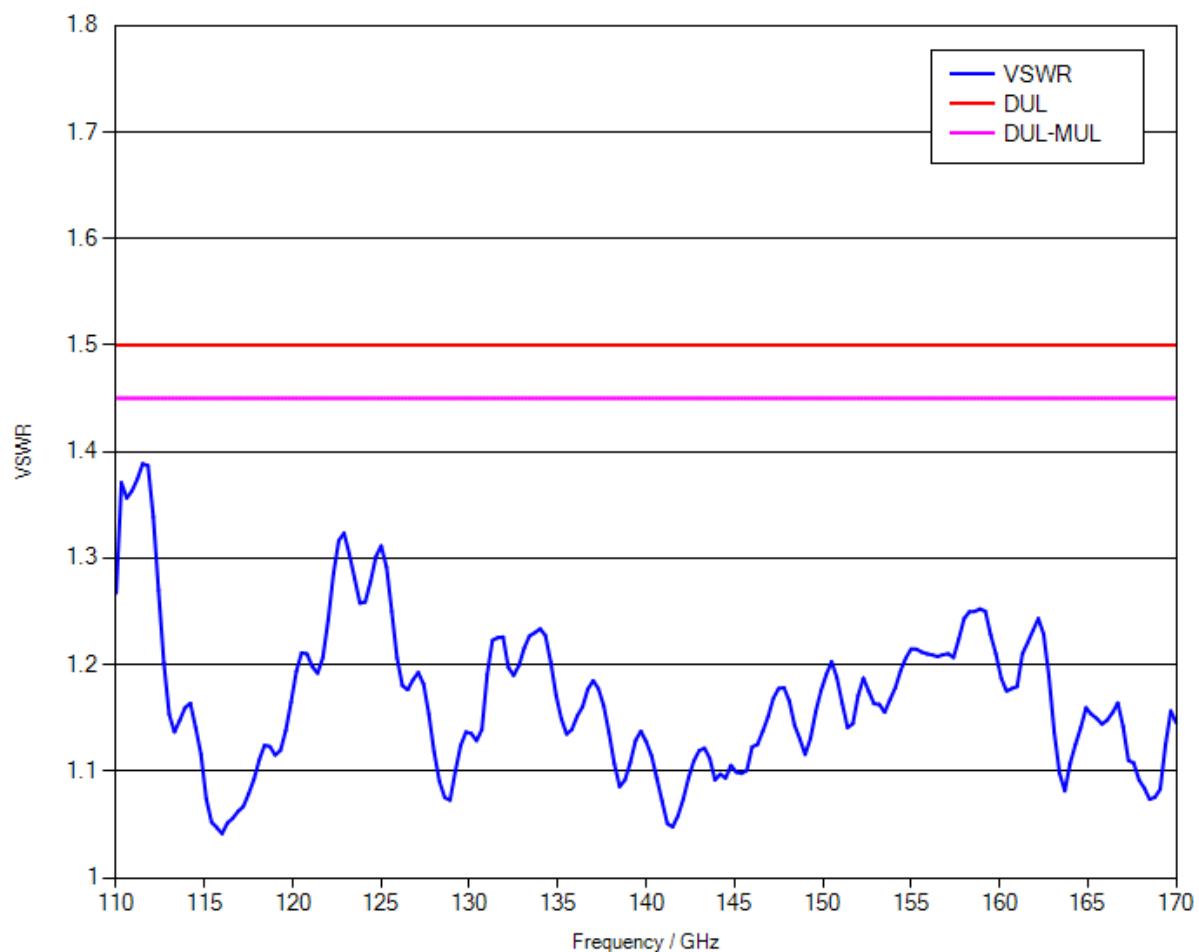

1.2 Conversion loss

LO level +15.5 dBm nominal
Bias 0 A

Measurement uncertainty: 1.5 dB

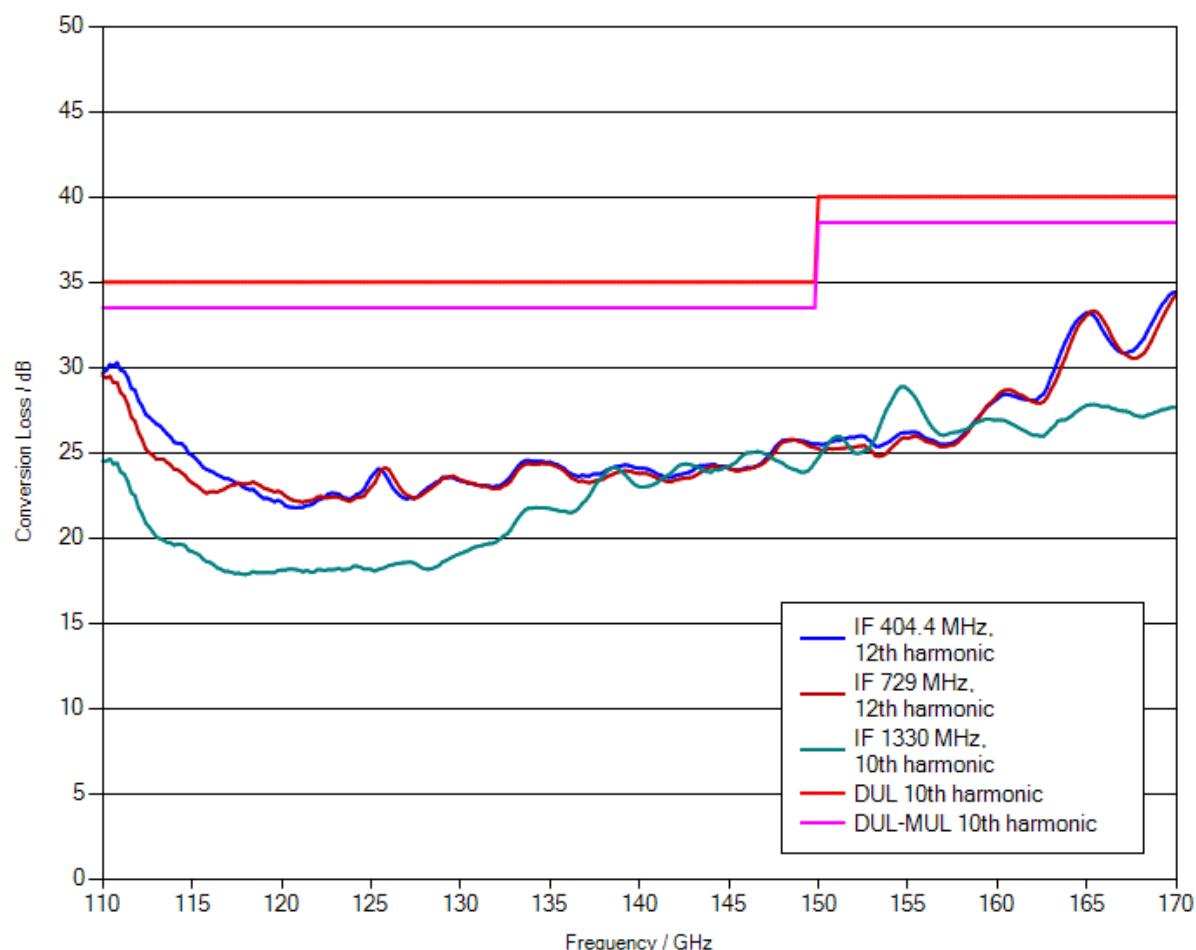

Note: Numeric calibration data can be found attached to the PDF file of the calibration certificate.
Click the “paper clip” symbol to display the file.

The file has been renamed for safety reasons.

When downloading the file onto your PC, please delete the “.file” extension and unzip the data.

1.3 Frequency response within 1 GHz

	DUL	Actual (worst case)	Evaluation
IF = 404.4 MHz, 12th harmonic	6 dB	2.14 dB	PASS
IF = 729 MHz, 12th harmonic	6 dB	2.15 dB	PASS
IF = 1330 MHz, 10th harmonic	6 dB	1.99 dB	PASS



Calibration Certificate

Kalibrierschein

Certificate Number 24-0220-100967-01

Zertifikatsnummer

Unit Data

Item Gegenstand	Harmonic Mixer, 140 GHz to 220 GHz		
Manufacturer Hersteller	RPG		
Type Typ	RPG FS-Z220		
Material Number Materialnummer	3593.3250.02	Serial Number Seriennummer	100967
Asset Number Inventarnummer			

This calibration certificate documents, that the named item is tested and measured against defined specifications. Measurement results are located usually in the corresponding interval with a probability of approx. 95% (coverage factor $k = 2$). Calibration is performed with test equipment and standards directly or indirectly traceable by means of approved calibration techniques to the PTB/DKD or other national/international standards, which realize the physical units of measurement according to the International System of Units (SI). In all cases where no standards are available, measurements are referenced to standards of the R&S laboratories. Principles and methods of calibration correspond with EN ISO/IEC 17025. This calibration certificate may not be reproduced other than in full. Calibration certificates without signatures are not valid. The user is obliged to have the object recalibrated at appropriate intervals.

Order Data

Customer Auftraggeber

Order Number Bestellnummer

Date of Receipt Eingangsdatum

Performance

Place and Date of Calibration Ort und Datum der Kalibrierung

Meckenheim, 2018-03-01

Scope of Calibration Umfang der Kalibrierung

Standard Calibration

Statement of Compliance (Incoming) Konformitätsaussage (Anlieferung)

New device

Statement of Compliance (Outgoing) Konformitätsaussage (Auslieferung)
--

All measured values are within the data sheet specifications.

Extend of Calibration Documents Umfang des Kalibrierdokuments
--

2 pages Calibration Certificate
5 pages Outgoing Results

Dieser Kalibrierschein dokumentiert, dass der genannte Gegenstand nach festgelegten Vorgaben geprüft und gemessen wurde. Die Messwerte lagen im Regelfall mit einer Wahrscheinlichkeit von annähernd 95% im zugeordneten Wertebereich (Erweiterte Messunsicherheit mit $k = 2$). Die Kalibrierung erfolgte mit Messmitteln und Normalen, die direkt oder indirekt durch Ableitung mittels anerkannter Kalibriermethoden rückgeführt sind auf Normale der PTB/DKD oder anderer national/internationaler Standards zur Darstellung der physikalischen Einheiten in Übereinstimmung mit dem Internationalen Einheitensystem (SI). Wenn keine Normale existieren, erfolgt die Rückführung auf Bezugsnormale der R&S-Labore. Grundsätze und Verfahren der Kalibrierung beziehen sich auf EN ISO/IEC 17025. Dieser Kalibrierschein darf nur vollständig und unverändert weiterverbreitet werden. Kalibrierscheine ohne Unterschriften sind ungültig. Für die Einhaltung einer angemessenen Frist zur Wiederholung der Kalibrierung ist der Benutzer verantwortlich.

Radiometer Physics GmbH; Meckenheim

Date of Issue Ausstellungsdatum

Head of Laboratory Laborleiter

Person Responsible Bearbeiter

2018-03-02

Schulze

Grossmindorf

Page (Seite) 1/2
Vers2010-05-05/
RPG2014-02-28

Calibration Method
Kalibrieranweisung

RPG-PAQA-TN-2014-002

Relative Humidity 20 % - 80 %
Relative Luftfeuchte

Ambient Temperature
Umgebungstemperatur

(23 ⁺⁷) °C

Working standards used (having a significant effect on the accuracy)
Verwendete Gebrauchsnormale (mit signifikantem Einfluss auf die Genauigkeit)

Item Gegenstand	Type Typ	Serial Number Seriennummer	Calibration Certificate Number Kalibrierscheinnummer	Cal. Due Kalibr. bis
Vector Network Analyzer Powersensor	R&S® ZVA67 R&S® NRP-Z55	101097 140093	20-300432406 20-300426315	2020-07-21 2018-05-17

UGB1 A compliance statement may be possible where a confidence level of less than 95 % is acceptable.
Die Bestätigung der Konformität ist möglich, sofern ein Grad des Vertrauens von weniger als 95 % akzeptabel ist.

UGB2 A non-compliance statement may be possible where a confidence level of less than 95 % is acceptable.
Die Bestätigung der Nicht-Konformität ist möglich, sofern ein Grad des Vertrauens von weniger als 95 % akzeptabel ist.

Ref.: ILAC-G8:03/2009 'Guidelines on the Reporting of Compliance with Specification'.

Notes
Anmerkungen


If the new product is stored under the climate conditions as specified in the data sheet upon delivery, the product's accuracy is not significantly affected within 12 month after its calibration in our factory. In this case, the recommended calibration interval starts on the date when the product is actually put into operation.

Outgoing Results

The following abbreviations may be used in this document

- {a} No measurement uncertainty stated because the errors always add together.
So it is sure that a measurement result evaluated as "PASS" is pass.
 - {b} The measurement uncertainty depends on the measurement result. The stated measurement uncertainty is valid for the close area around the specification. Measurement results outside the close area have a higher measurement uncertainty but are within the specification.
 - {c} Functional test, therefore no measurement uncertainty is stated.
 - {d} Typical value, refer to performance test.
 - {e} The measurement uncertainty is taken into account when setting the measuring system.
- DL or DT Data Limit for symmetrical tolerance limits
 DLL Datasheet Lower Limit
 DUL Datasheet Upper Limit
 MU Measurement Uncertainty
 MLL or MLV Measurement Uncertainty Lower Value
 MUL or MUV Measurement Uncertainty Upper Value
 Nom. Nominal Value
 Dev. Deviation
 MErr. Measurement Error
 Act. Actual Value
 UGB Uncertainty Guard Band: Measuring uncertainty violates the data (spec.) limit.
 UGB1 Measurement results marked as UGB1 show conformity with a probability of >50 % and <95 %.
 UGB2 Measurement results marked as UGB2 show non-conformity with a probability of >50 % and <95 %.
 DU Datasheet Uncertainty

Explanation of charts

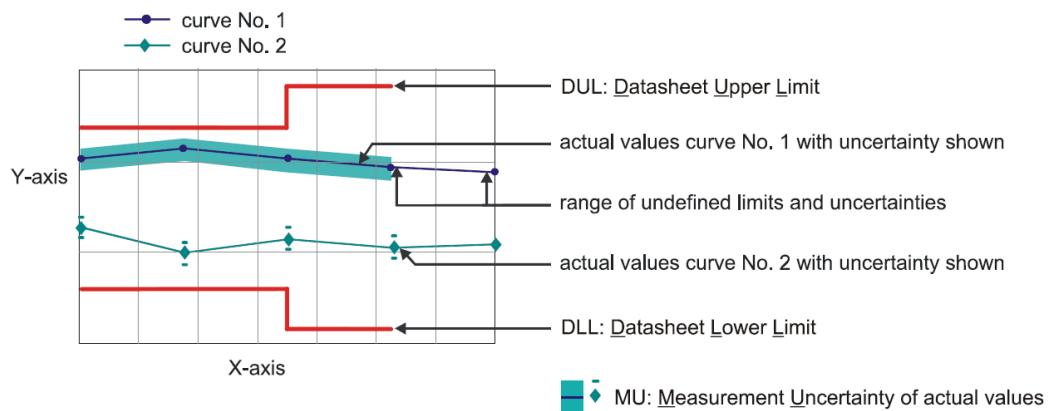

Software used for measurement**Item Type**

Measurement Studio Professional Edition
MixerCertification


Version

2013
7_08

Remark

1.1 RF Input – VSWR


Measurement uncertainty: 0.05 (VSWR)

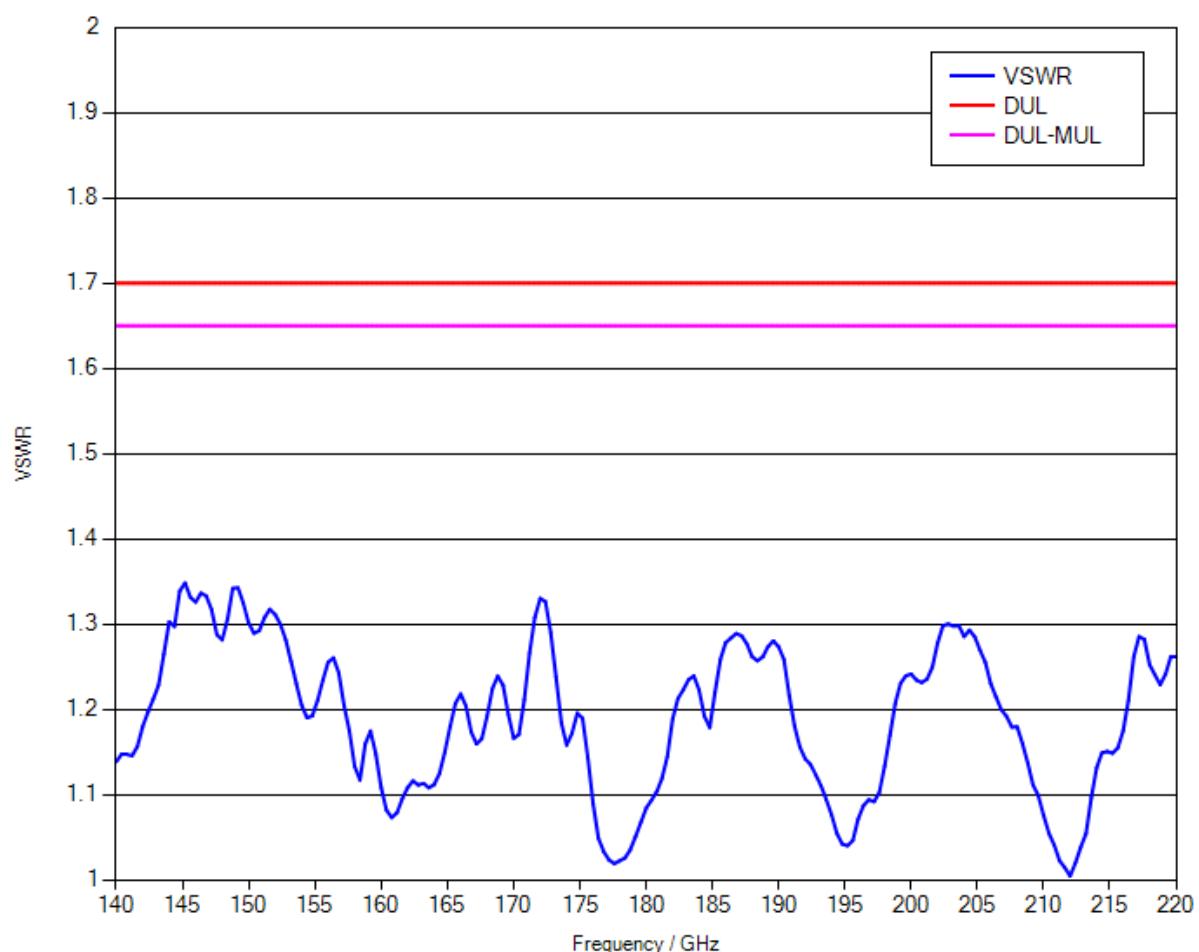

1.2 Conversion loss

LO level +13 dBm nominal
Bias 0 A

Measurement uncertainty: 4 dB

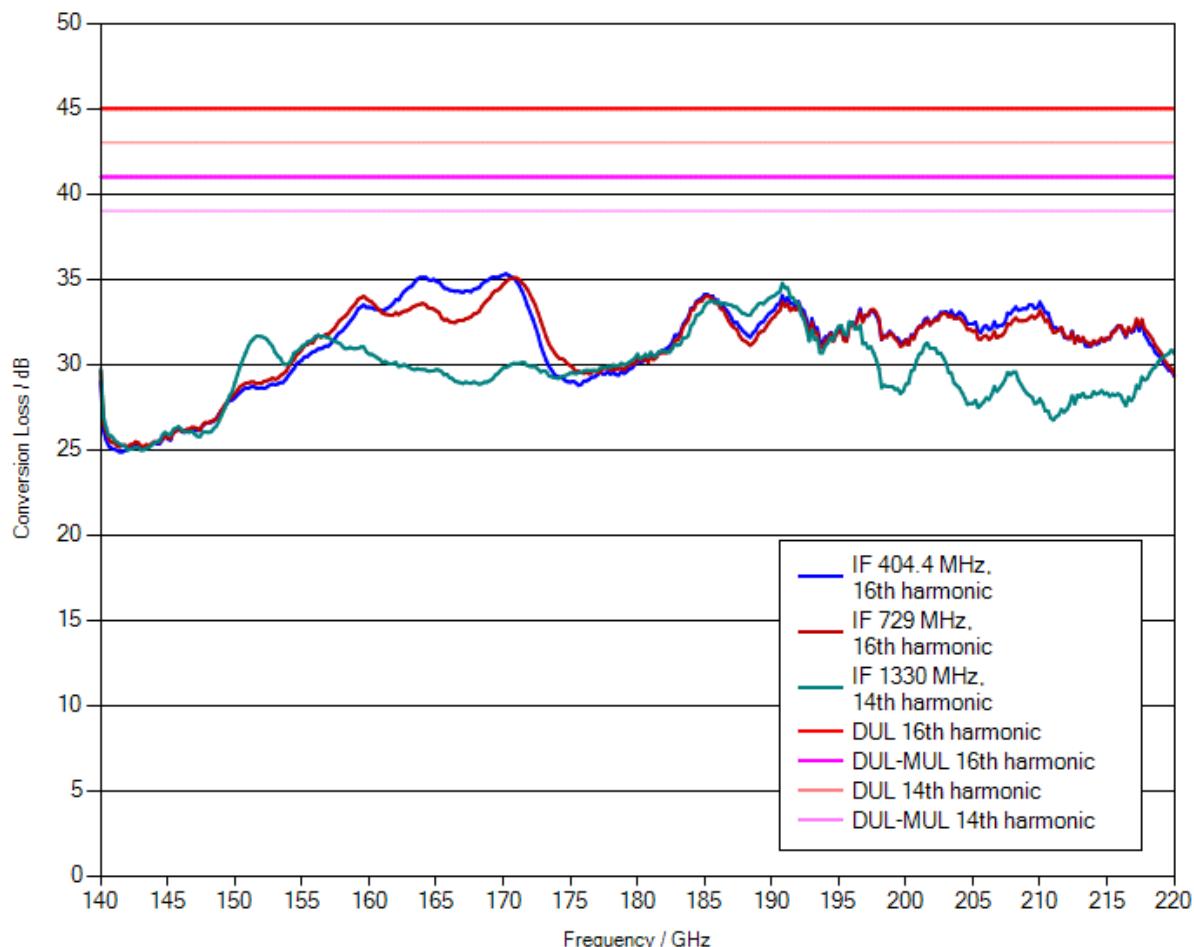

Note: Numeric calibration data can be found attached to the PDF file of the calibration certificate.
Click the “paper clip” symbol to display the file.

The file has been renamed for safety reasons.

When downloading the file onto your PC, please delete the “.file” extension and unzip the data.

1.3 Frequency response within 1 GHz

	DUL	Actual (worst case)	Evaluation
IF = 404.4 MHz, 16th harmonic	6 dB	4 dB	PASS
IF = 729 MHz, 16th harmonic	6 dB	4.22 dB	PASS
IF = 1330 MHz, 14th harmonic	6 dB	4.13 dB	PASS



Standard Gain Horn


Model 20240-20

Waveguide Size:
Nominal Gain:
Operating Frequencies:

WG20 (WR42, R220)
20 dBi
17.6 - 26.7 GHz


Overall Length (A):
Aperture Width (B):
Aperture Height (C):
Waveguide Width (D):
Waveguide Height (E):
Flare Length (F):

120.3 mm (4.736 inch)
52.00 mm (2.047 inch)
37.40 mm (1.472 inch)
10.668 mm (0.420 inch)
4.318 mm (0.170 inch)
115.20 mm (4.535 inch)

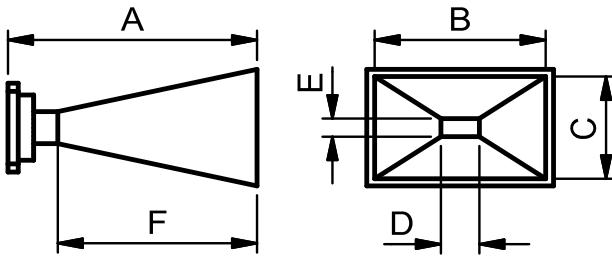

Typical Performance Data

Frequency (GHz)	Gain (dBi)	Beamwidth		Frequency (GHz)	Gain (dBi)	Beamwidth		Frequency (GHz)	Gain (dBi)	Beamwidth	
		E-Plane	H-Plane			E-Plane	H-Plane			E-Plane	H-Plane
17.6	18.11	23.1°	22.3°	20.7	19.42	19.7°	19.0°	23.85	20.54	17.1°	16.5°
17.7	18.15	23.0°	22.2°	20.85	19.48	19.5°	18.8°	24	20.59	17.0°	16.4°
17.85	18.22	22.8°	22.0°	21	19.54	19.4°	18.7°	24.15	20.64	16.9°	16.3°
18	18.29	22.6°	21.8°	21.15	19.59	19.2°	18.6°	24.3	20.69	16.8°	16.2°
18.15	18.36	22.4°	21.6°	21.3	19.65	19.1°	18.4°	24.45	20.74	16.6°	16.1°
18.3	18.42	22.2°	21.4°	21.45	19.71	19.0°	18.3°	24.6	20.79	16.5°	16.0°
18.45	18.49	22.1°	21.3°	21.6	19.76	18.8°	18.2°	24.75	20.83	16.4°	15.9°
18.6	18.56	21.9°	21.1°	21.75	19.82	18.7°	18.0°	24.9	20.88	16.3°	15.8°
18.75	18.62	21.7°	20.9°	21.9	19.87	18.6°	17.9°	25.05	20.93	16.3°	15.7°
18.9	18.69	21.5°	20.8°	22.05	19.93	18.5°	17.8°	25.2	20.97	16.2°	15.6°
19.05	18.75	21.4°	20.6°	22.2	19.98	18.3°	17.7°	25.35	21.02	16.1°	15.5°
19.2	18.82	21.2°	20.4°	22.35	20.03	18.2°	17.6°	25.5	21.06	16.0°	15.4°
19.35	18.88	21.0°	20.3°	22.5	20.09	18.1°	17.4°	25.65	21.11	15.9°	15.3°
19.5	18.94	20.9°	20.1°	22.65	20.14	18.0°	17.3°	25.8	21.15	15.8°	15.2°
19.65	19.00	20.7°	20.0°	22.8	20.19	17.9°	17.2°	25.95	21.20	15.7°	15.1°
19.8	19.06	20.6°	19.8°	22.95	20.24	17.7°	17.1°	26.1	21.24	15.6°	15.0°
19.95	19.13	20.4°	19.7°	23.1	20.29	17.6°	17.0°	26.25	21.28	15.5°	15.0°
20.1	19.19	20.3°	19.5°	23.25	20.35	17.5°	16.9°	26.4	21.33	15.4°	14.9°
20.25	19.25	20.1°	19.4°	23.4	20.40	17.4°	16.8°	26.55	21.37	15.3°	14.8°
20.4	19.31	20.0°	19.2°	23.55	20.45	17.3°	16.7°	26.7	21.41	15.2°	14.7°
20.55	19.36	19.8°	19.1°	23.7	20.50	17.2°	16.6°				

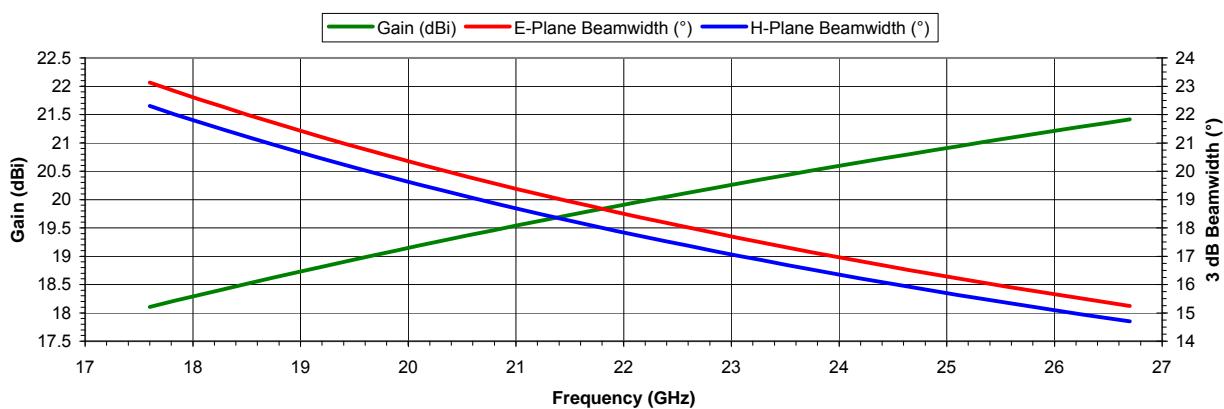

Notes:

Gain calculations based on NRL Report 4433 - accuracy to approx ± 0.3dBi
 Half-power (3dB) beamwidth estimates calculated using $50.8 \lambda / C$ (E-Plane) and $68.1 \lambda / B$ (H-Plane). This is a 'large aperture' approximation that breaks down at gain values smaller than around 12 dBi. For 10dBi Standard Gain Horns, beamwidths are approximately 63° at the lowest frequency and 48° at the highest frequency.

FLANN MICROWAVE LTD

Dunmere Road
Bodmin, Cornwall
PL31 2QL
United Kingdom
Tel: +44 (0)1208 777777
Fax: +44 (0)1208 76426

sales@flann.com


FLANN MICROWAVE INC

One Boston Place
Suite 2600
Boston
Massachusetts, MA 02108-4407
Tel: 617 621 7034
Fax: 617 577 8234

STANDARD GAIN HORN


Model 22240-20

Waveguide Size:	WG22 (WR28, R320)
Nominal Gain:	20 dBi
Operating Frequencies:	26.4 - 40.1 GHz
Overall Length (A):	86.0 mm (3.386 inch)
Aperture Width (B):	34.20 mm (1.346 inch)
Aperture Height (C):	24.80 mm (0.976 inch)
Waveguide Width (D):	7.112 mm (0.280 inch)
Waveguide Height (E):	3.556 mm (0.140 inch)
Flare Length (F):	75.00 mm (2.953 inch)

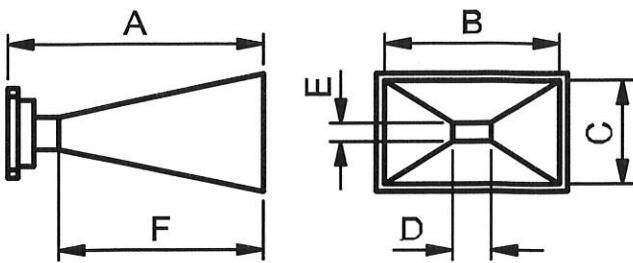

Typical Performance Data

Frequency (GHz)	Gain (dBi)	Beamwidth		Frequency (GHz)	Gain (dBi)	Beamwidth		Frequency (GHz)	Gain (dBi)	Beamwidth	
		E-Plane	H-Plane			E-Plane	H-Plane			E-Plane	H-Plane
26.4	18.03	23.3°	22.6°	31.5	19.47	19.5°	18.9°	36.75	20.69	16.7°	16.2°
26.5	18.06	23.2°	22.5°	31.75	19.53	19.3°	18.8°	37	20.74	16.6°	16.1°
26.75	18.14	22.9°	22.3°	32	19.60	19.2°	18.6°	37.25	20.80	16.5°	16.0°
27	18.22	22.7°	22.1°	32.25	19.66	19.0°	18.5°	37.5	20.85	16.4°	15.9°
27.25	18.29	22.5°	21.9°	32.5	19.72	18.9°	18.4°	37.75	20.90	16.3°	15.8°
27.5	18.37	22.3°	21.7°	32.75	19.78	18.7°	18.2°	38	20.95	16.2°	15.7°
27.75	18.44	22.1°	21.5°	33	19.84	18.6°	18.1°	38.25	21.00	16.0°	15.6°
28	18.52	21.9°	21.3°	33.25	19.90	18.5°	17.9°	38.5	21.05	15.9°	15.5°
28.25	18.59	21.7°	21.1°	33.5	19.96	18.3°	17.8°	38.75	21.10	15.8°	15.4°
28.5	18.66	21.5°	20.9°	33.75	20.02	18.2°	17.7°	39	21.15	15.7°	15.3°
28.75	18.73	21.4°	20.8°	34	20.08	18.1°	17.6°	39.25	21.20	15.6°	15.2°
29	18.80	21.2°	20.6°	34.25	20.14	17.9°	17.4°	39.5	21.25	15.5°	15.1°
29.25	18.87	21.0°	20.4°	34.5	20.19	17.8°	17.3°	39.75	21.30	15.4°	15.0°
29.5	18.94	20.8°	20.2°	34.75	20.25	17.7°	17.2°	40	21.34	15.3°	14.9°
29.75	19.01	20.6°	20.1°	35	20.31	17.5°	17.1°	40.1	21.36	15.3°	14.9°
30	19.08	20.5°	19.9°	35.25	20.36	17.4°	16.9°				
30.25	19.14	20.3°	19.7°	35.5	20.42	17.3°	16.8°				
30.5	19.21	20.1°	19.6°	35.75	20.48	17.2°	16.7°				
30.75	19.28	20.0°	19.4°	36	20.53	17.1°	16.6°				
31	19.34	19.8°	19.3°	36.25	20.58	16.9°	16.5°				
31.25	19.41	19.6°	19.1°	36.5	20.64	16.8°	16.3°				

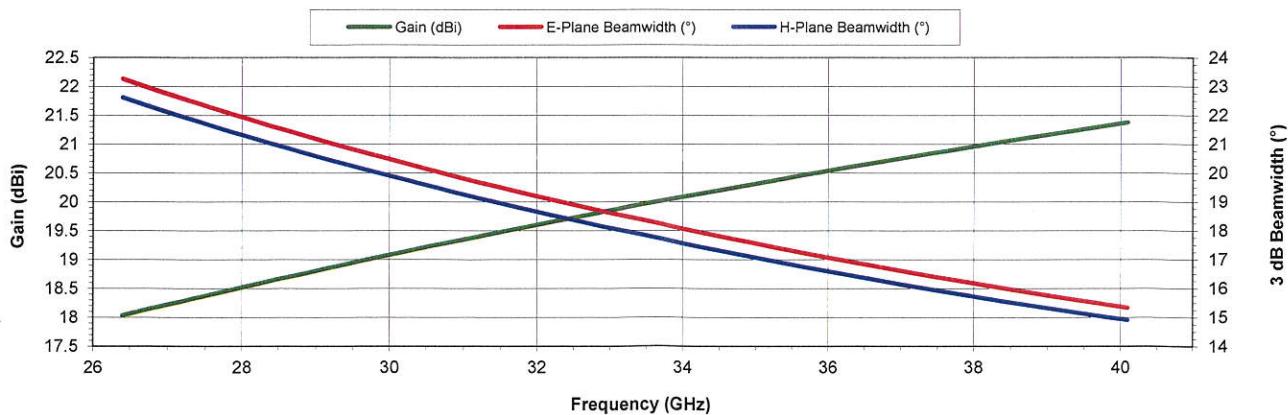

Notes:

Gain calculations based on NRL Report 4433 - accuracy to approx ± 0.3dBi. Antenna Gain is only valid within the 'far-field' of the antenna. For more details, please see Ch 16, 'Antenna Theory, Analysis & Design' Balanis, Wiley or Ch 18 'Antenna', Kraus, McGraw-Hill.

Half-power (3dB) beamwidth estimates calculated using $50.8 \lambda / C$ (E-Plane) and $68.1 \lambda / B$ (H-Plane). This is a 'large aperture' approximation that breaks down at gain values smaller than around 12 dBi. For 10dBi Standard Gain Horns, beamwidths are approximately 63° at the lowest frequency and 48° at the highest frequency.



FLANN MICROWAVE

Dunmere Road
Bodmin, Cornwall
PL31 2QL
United Kingdom

Tel: +44 (0) 1208 777777
Fax: +44 (0) 1208 76426
mail@flann.com
www.flann.com



STANDARD GAIN HORN

Model No: 24240-20

Nominal Gain: 20dB

Typical Performance Data

3dB Beamwidth (deg.)

Frequency (GHz)	Gain dBi (acc. ± .25dB)	E-PLANE	H-PLANE
39.3	18.0	24	23
40.0	18.2	23	22
41.0	18.4	23	22
42.0	18.6	22	21
43.0	18.8	22	21
44.0	19.0	21	20
45.0	19.2	21	20
46.0	19.3	20	20
47.0	19.5	20	19
48.0	19.7	19	19
49.0	19.9	19	18
50.0	20.0	19	18
51.0	20.2	18	18
52.0	20.3	18	17
53.0	20.5	18	17
54.0	20.6	17	17
55.0	20.8	17	16
56.0	20.9	17	16
57.0	21.1	16	16
58.0	21.2	16	16
59.0	21.4	16	15
59.7	21.4	16	15



FLANN MICROWAVE

Dunmere Road

Cornwall

Tel: +44 (0) 1208 77777

Email: mail@flann.com

PL31 2QL

Bodmin
England

Fax: +44 (0) 1208 76426
www.flann.com



BS EN ISO 9002 Certificate No. 2536

STANDARD GAIN HORN

Model No: 26240-20dB

Nominal Gain: 20dB

Typical Performance Data

3dB Beamwidth (deg.)

Frequency (GHz)	Gain dBi (acc. ± .25dB)	E-PLANE	H-PLANE
60.5	18.1	23	23
62.0	18.3	23	22
64.0	18.6	22	22
66.0	18.9	21	21
68.0	19.1	21	20
70.0	19.4	20	20
72.0	19.6	19	19
74.0	19.8	19	19
76.0	20.0	18	18
78.0	20.2	18	18
80.0	20.4	17	17
82.0	20.5	17	17
84.0	20.8	17	17
86.0	21.0	16	16
88.0	21.2	16	16
90.0	21.4	16	16
92.0	21.6	15	15



FLANN MICROWAVE

Dunmere Road

Cornwall

Tel: +44 (0) 1208 77777

Email: mail@flann.com

PL31 2QL

Bodmin

England

Fax: +44 (0) 1208 76426


www.flann.com



Standard Gain Horn


Model 27240-20

Waveguide Size:	WG27 (WR10, R900)
Nominal Gain:	20 dBi
Operating Frequencies:	73.8 - 112 GHz
Overall Length (A):	32.5 mm (1.280 inch)
Aperture Width (B):	12.40 mm (0.488 inch)
Aperture Height (C):	9.00 mm (0.354 inch)
Waveguide Width (D):	2.540 mm (0.100 inch)
Waveguide Height (E):	1.270 mm (0.050 inch)
Flare Length (F):	26.00 mm (1.024 inch)

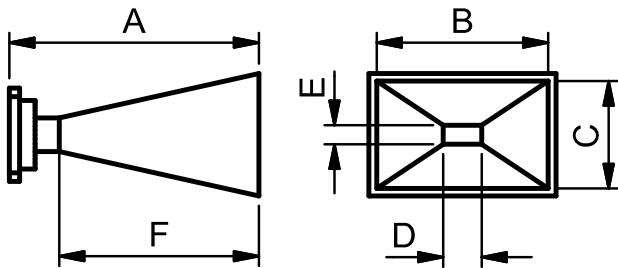

Typical Performance Data

Frequency (GHz)	Gain (dBi)	Beamwidth E-Plane	Beamwidth H-Plane	Frequency (GHz)	Gain (dBi)	Beamwidth E-Plane	Beamwidth H-Plane	Frequency (GHz)	Gain (dBi)	Beamwidth E-Plane	Beamwidth H-Plane
73.8	18.12	22.9°	22.3°	89.25	19.66	19.0°	18.4°	105	20.92	16.1°	15.7°
74.25	18.17	22.8°	22.2°	90	19.72	18.8°	18.3°	105.75	20.98	16.0°	15.6°
75	18.26	22.6°	21.9°	90.75	19.79	18.6°	18.1°	106.5	21.03	15.9°	15.5°
75.75	18.34	22.3°	21.7°	91.5	19.85	18.5°	18.0°	107.25	21.08	15.8°	15.3°
76.5	18.42	22.1°	21.5°	92.25	19.92	18.3°	17.8°	108	21.14	15.7°	15.2°
77.25	18.50	21.9°	21.3°	93	19.98	18.2°	17.7°	108.75	21.19	15.6°	15.1°
78	18.57	21.7°	21.1°	93.75	20.04	18.0°	17.6°	109.5	21.24	15.4°	15.0°
78.75	18.65	21.5°	20.9°	94.5	20.11	17.9°	17.4°	110.25	21.29	15.3°	14.9°
79.5	18.73	21.3°	20.7°	95.25	20.17	17.8°	17.3°	111	21.34	15.2°	14.8°
80.25	18.80	21.1°	20.5°	96	20.23	17.6°	17.1°	111.75	21.39	15.1°	14.7°
81	18.88	20.9°	20.3°	96.75	20.29	17.5°	17.0°	112	21.41	15.1°	14.7°
81.75	18.95	20.7°	20.1°	97.5	20.35	17.3°	16.9°				
82.5	19.03	20.5°	20.0°	98.25	20.41	17.2°	16.8°				
83.25	19.10	20.3°	19.8°	99	20.47	17.1°	16.6°				
84	19.17	20.1°	19.6°	99.75	20.53	17.0°	16.5°				
84.75	19.24	20.0°	19.4°	100.5	20.58	16.8°	16.4°				
85.5	19.31	19.8°	19.3°	101.25	20.64	16.7°	16.3°				
86.25	19.38	19.6°	19.1°	102	20.70	16.6°	16.1°				
87	19.45	19.4°	18.9°	102.75	20.76	16.5°	16.0°				
87.75	19.52	19.3°	18.8°	103.5	20.81	16.3°	15.9°				
88.5	19.59	19.1°	18.6°	104.25	20.87	16.2°	15.8°				

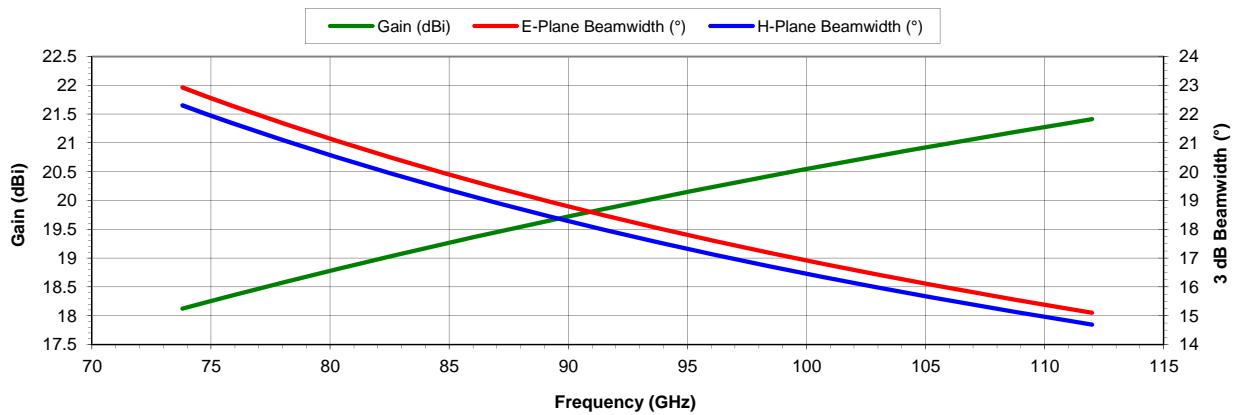

Notes:

Gain calculations based on NRL Report 4433 - accuracy to approx ± 0.3dBi
 Half-power (3dB) beamwidth estimates calculated using $50.8 \lambda / C$ (E-Plane) and $68.1 \lambda / B$ (H-Plane). This is a 'large aperture' approximation that breaks down at gain values smaller than around 12 dBi. For 10dBi Standard Gain Horns, beamwidths are approximately 63° at the lowest frequency and 48° at the highest frequency.



FLANN MICROWAVE

Dunmere Road
 Bodmin, Cornwall
 PL31 2QL
 United Kingdom


Tel: +44 (0) 1208 777777
 Fax: +44 (0) 1208 76426
mail@flann.com
www.flann.com



STANDARD GAIN HORN


Model 29240-20

Waveguide Size:	WG29 (WR6, R1400)
Nominal Gain:	20 dBi
Operating Frequencies:	114 - 173 GHz
Overall Length (A):	24.4 mm (0.961 inch)
Aperture Width (B):	8.50 mm (0.335 inch)
Aperture Height (C):	6.40 mm (0.252 inch)
Waveguide Width (D):	1.651 mm (0.065 inch)
Waveguide Height (E):	0.826 mm (0.033 inch)
Flare Length (F):	18.00 mm (0.709 inch)

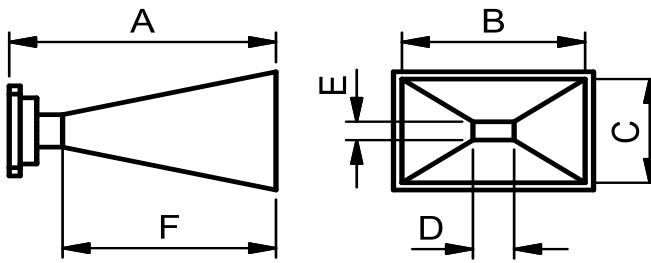

Typical Performance Data

Frequency (GHz)	Gain (dBi)	Beamwidth		Frequency (GHz)	Gain (dBi)	Beamwidth		Frequency (GHz)	Gain (dBi)	Beamwidth	
		E-Plane	H-Plane			E-Plane	H-Plane			E-Plane	H-Plane
114	18.73	20.9°	21.1°	135	20.08	17.6°	17.8°	156	21.19	15.2°	15.4°
115	18.80	20.7°	20.9°	136	20.13	17.5°	17.7°	157	21.24	15.2°	15.3°
116	18.87	20.5°	20.7°	137	20.19	17.4°	17.5°	158	21.28	15.1°	15.2°
117	18.94	20.3°	20.5°	138	20.25	17.2°	17.4°	159	21.33	15.0°	15.1°
118	19.01	20.2°	20.3°	139	20.30	17.1°	17.3°	160	21.38	14.9°	15.0°
119	19.08	20.0°	20.2°	140	20.36	17.0°	17.2°	161	21.42	14.8°	14.9°
120	19.14	19.8°	20.0°	141	20.42	16.9°	17.0°	162	21.47	14.7°	14.8°
121	19.21	19.7°	19.8°	142	20.47	16.8°	16.9°	163	21.52	14.6°	14.7°
122	19.28	19.5°	19.7°	143	20.52	16.6°	16.8°	164	21.56	14.5°	14.6°
123	19.34	19.3°	19.5°	144	20.58	16.5°	16.7°	165	21.61	14.4°	14.6°
124	19.41	19.2°	19.4°	145	20.63	16.4°	16.6°	166	21.65	14.3°	14.5°
125	19.47	19.0°	19.2°	146	20.68	16.3°	16.4°	167	21.70	14.2°	14.4°
126	19.53	18.9°	19.1°	147	20.74	16.2°	16.3°	168	21.74	14.2°	14.3°
127	19.60	18.7°	18.9°	148	20.79	16.1°	16.2°	169	21.78	14.1°	14.2°
128	19.66	18.6°	18.8°	149	20.84	16.0°	16.1°	170	21.83	14.0°	14.1°
129	19.72	18.4°	18.6°	150	20.89	15.9°	16.0°	171	21.87	13.9°	14.0°
130	19.78	18.3°	18.5°	151	20.94	15.8°	15.9°	172	21.91	13.8°	14.0°
131	19.84	18.2°	18.3°	152	20.99	15.7°	15.8°	173	21.95	13.8°	13.9°
132	19.90	18.0°	18.2°	153	21.04	15.5°	15.7°				
133	19.96	17.9°	18.1°	154	21.09	15.4°	15.6°				
134	20.02	17.8°	17.9°	155	21.14	15.3°	15.5°				

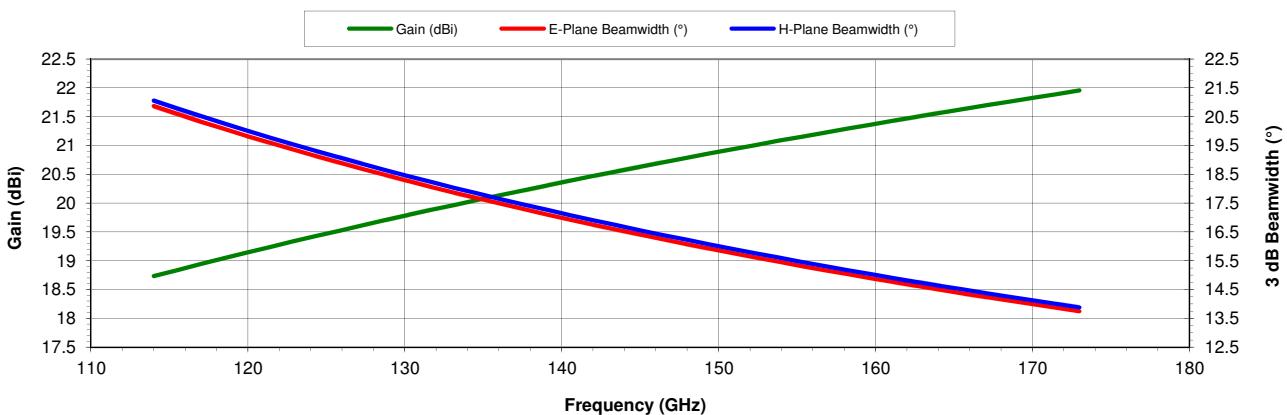

Notes:

Gain calculations based on NRL Report 4433 - accuracy to approx ± 0.3dBi. Antenna Gain is only valid within the 'far-field' of the antenna. For more details, please see Ch 16, 'Antenna Theory, Analysis & Design' Balanis, Wiley or Ch 18 'Antenna', Kraus, McGraw-Hill.

Half-power (3dB) beamwidth estimates calculated using $50.8 \lambda / C$ (E-Plane) and $68.1 \lambda / B$ (H-Plane). This is a 'large aperture' approximation that breaks down at gain values smaller than around 12 dBi. For 10dBi Standard Gain Horns, beamwidths are approximately 63° at the lowest frequency and 48° at the highest frequency.



FLANN MICROWAVE
Dunmere Road
Bodmin, Cornwall
PL31 2QL
United Kingdom

Tel: +44 (0) 1208 777777
Fax: +44 (0) 1208 76426
mail@flann.com
www.flann.com





Standard Gain Horn


Model 30240-20

Waveguide Size:
Nominal Gain:
Operating Frequencies:

WG30 (WR5, R1800)
20 dBi
145 - 220 GHz


Overall Length (A):
Aperture Width (B):
Aperture Height (C):
Waveguide Width (D):
Waveguide Height (E):
Flare Length (F):

17.5 mm (0.689 inch)
6.80 mm (0.268 inch)
5.00 mm (0.197 inch)
1.295 mm (0.051 inch)
0.648 mm (0.026 inch)
14.50 mm (0.571 inch)

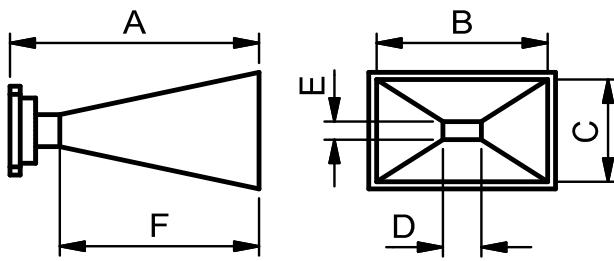

Typical Performance Data

Frequency (GHz)	Gain (dBi)	Beamwidth		Frequency (GHz)	Gain (dBi)	Beamwidth		Frequency (GHz)	Gain (dBi)	Beamwidth	
		E-Plane	H-Plane			E-Plane	H-Plane			E-Plane	H-Plane
145	18.78	21.0°	20.7°	175.5	20.30	17.3°	17.1°	207	21.56	14.7°	14.5°
145.5	18.81	20.9°	20.6°	177	20.37	17.2°	17.0°	208.5	21.61	14.6°	14.4°
147	18.89	20.7°	20.4°	178.5	20.43	17.1°	16.8°	210	21.67	14.5°	14.3°
148.5	18.98	20.5°	20.2°	180	20.50	16.9°	16.7°	211.5	21.72	14.4°	14.2°
150	19.06	20.3°	20.0°	181.5	20.56	16.8°	16.5°	213	21.77	14.3°	14.1°
151.5	19.14	20.1°	19.8°	183	20.62	16.6°	16.4°	214.5	21.82	14.2°	14.0°
153	19.21	19.9°	19.6°	184.5	20.69	16.5°	16.3°	216	21.87	14.1°	13.9°
154.5	19.29	19.7°	19.4°	186	20.75	16.4°	16.1°	217.5	21.92	14.0°	13.8°
156	19.37	19.5°	19.2°	187.5	20.81	16.2°	16.0°	219	21.97	13.9°	13.7°
157.5	19.45	19.3°	19.1°	189	20.87	16.1°	15.9°	220	22.01	13.8°	13.6°
159	19.52	19.2°	18.9°	190.5	20.93	16.0°	15.8°				
160.5	19.60	19.0°	18.7°	192	20.99	15.9°	15.6°				
162	19.67	18.8°	18.5°	193.5	21.05	15.7°	15.5°				
163.5	19.74	18.6°	18.4°	195	21.11	15.6°	15.4°				
165	19.82	18.5°	18.2°	196.5	21.17	15.5°	15.3°				
166.5	19.89	18.3°	18.0°	198	21.23	15.4°	15.2°				
168	19.96	18.1°	17.9°	199.5	21.28	15.3°	15.0°				
169.5	20.03	18.0°	17.7°	201	21.34	15.1°	14.9°				
171	20.10	17.8°	17.6°	202.5	21.39	15.0°	14.8°				
172.5	20.16	17.7°	17.4°	204	21.45	14.9°	14.7°				
174	20.23	17.5°	17.2°	205.5	21.50	14.8°	14.6°				

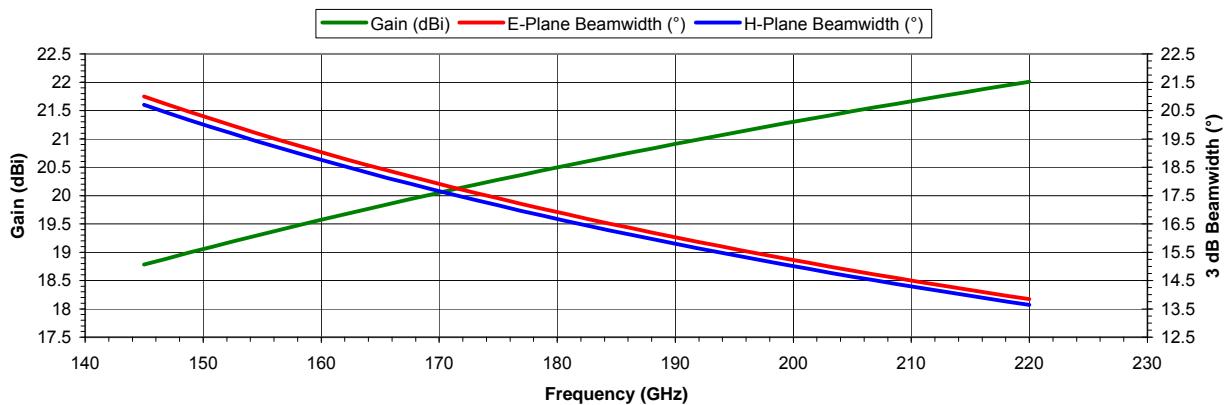

Notes:

Gain calculations based on NRL Report 4433 - accuracy to approx ± 0.3dBi

Half-power (3dB) beamwidth estimates calculated using $50.8 \lambda / C$ (E-Plane) and $68.1 \lambda / B$ (H-Plane). This is a 'large aperture' approximation that breaks down at gain values smaller than around 12 dBi. For 10dBi Standard Gain Horns, beamwidths are approximately 63° at the lowest frequency and 48° at the highest frequency.

FLANN MICROWAVE LTD

Dunmere Road
Bodmin, Cornwall
PL31 2QL
United Kingdom
Tel: +44 (0)1208 777777
Fax: +44 (0)1208 76426

sales@flann.com

FLANN MICROWAVE INC

One Boston Place
Suite 2600
Boston
Massachusetts, MA 02108-4407
Tel: 617 621 7034
Fax: 617 577 8234