



1
Assessment and Progress

A
8/1/2016 - 8/7/2016 (7 Days)

B
7/21/2016 - 7/27/2016 (7 Days)

Percentile comparison Average A

25-75%

0-90%

This report is designed to help you view your glucose management while on your MiniMed® system. You can use this report with your healthcare professional (HCP) to improve the duration of time spent in Auto Mode and determine what events caused some of your Auto Mode exits.

Start first at these date ranges. Make sure the dates you would like to review are listed here. **Date Range A** is the current date range from the time you uploaded your pump. You can select 7 or 14 days to start. **Date Range B** is the date range from past dates, for example, you can select a range of dates to before the time you started Auto Mode, if you are wearing the MiniMed 670G system, in order to see the changes in your glucose management. You can also use a date range to include your last doctor visit to see how your glucose has progressed since your last visit.


2

	Date Range A	Date Range B
Auto Mode (%)	14% (1d 00hrs)	86% (6d 00hrs)
Auto Mode (%)	97% (6d 19hrs)	150 ± 56 mg/dL
Auto Mode (%)	6.9%	174 ± 65 mg/dL
Auto Mode (%)	7.8 / 5.0	24 units
Auto Mode (%)	12U (49%)	12U (51%)
Auto Mode (%)	Every 3.0 days	Every 3.0 days
Auto Mode (%)	4.8	170 ± 24g
Auto Mode (%)	3:00 hrs	3:00 hrs

Large time/date change	0	0				
Unidentified	0	0	170 ± 15g	3:00 hrs	3:00 hrs	


* Most recent pump settings are displayed




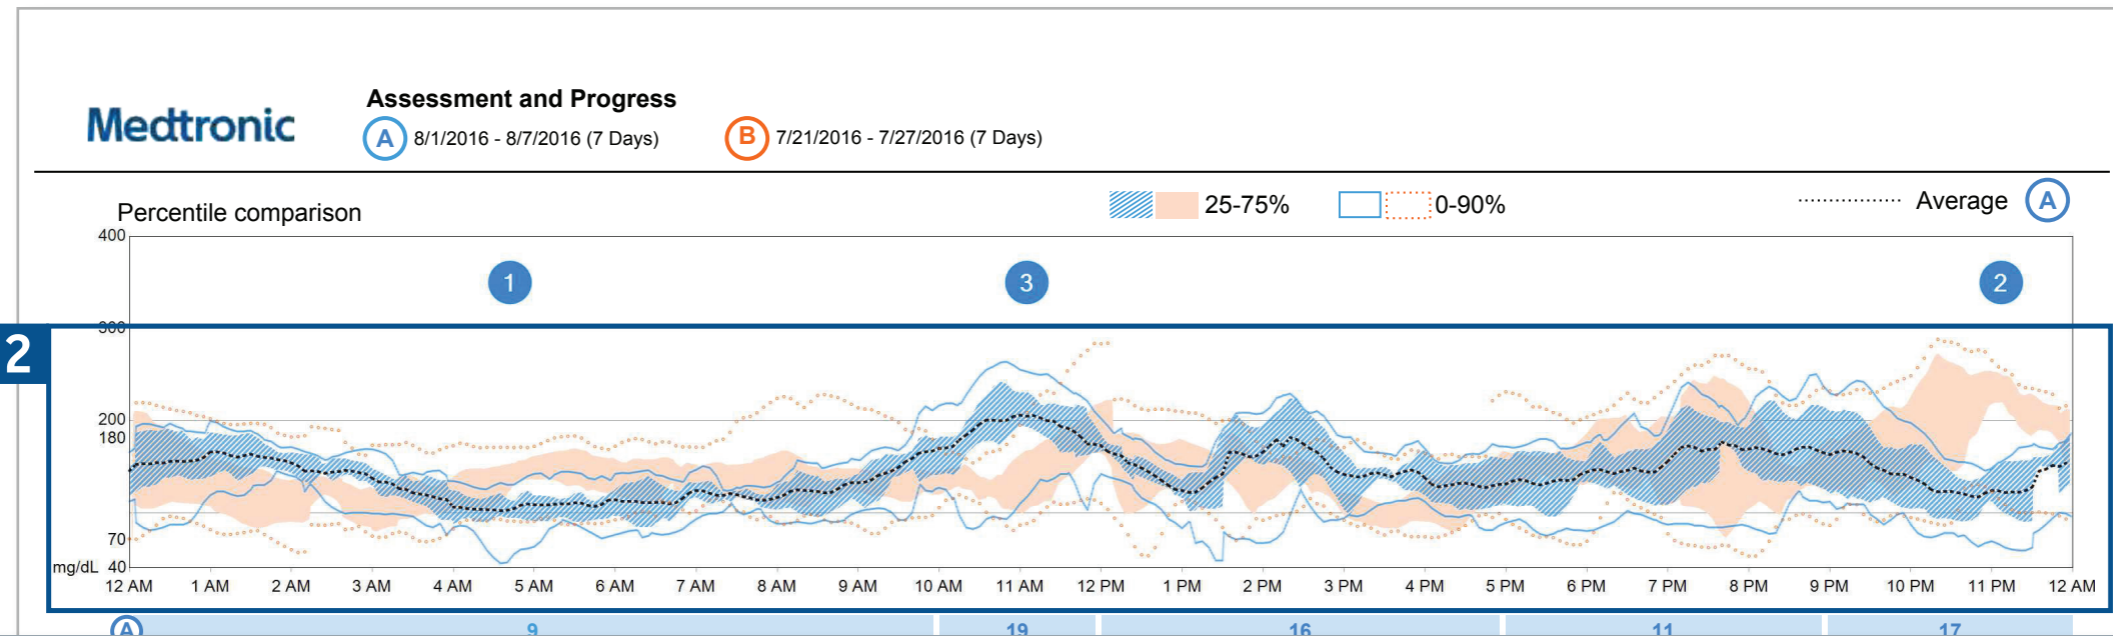


In this graph you can see that there are two color shaded areas of data. These areas are referred to as plots of information from your continuous glucose monitoring (CGM) device. The blue plot is your pump and sensor information from the dates in [Date Range A](#). Because this is the most recent information downloaded from your pump, an average sensor glucose (SG) line is calculated and shown as a dotted black line in the middle. The dark shading in blue represents 25-75% of all your sensor readings, meaning this is where most of your glucose readings have been. Remember, your CGM records up to 288 SG values on a daily basis, from those 288 values, 25-75% of them are represented in the darker shade. The remaining or excess data are in the 0-90% range shown within the solid blue line.


Your data from [Date Range B](#), is colored in orange behind the blue plot. This section of the report should be reviewed with your HCP to see progress from your last visit or your last device settings change. Do you see less shading in the blue plot below 70mg/dL compared to the orange plot? This is a good discussion to start with your HCP to see if you are having difficulty and frequency with low glucose.

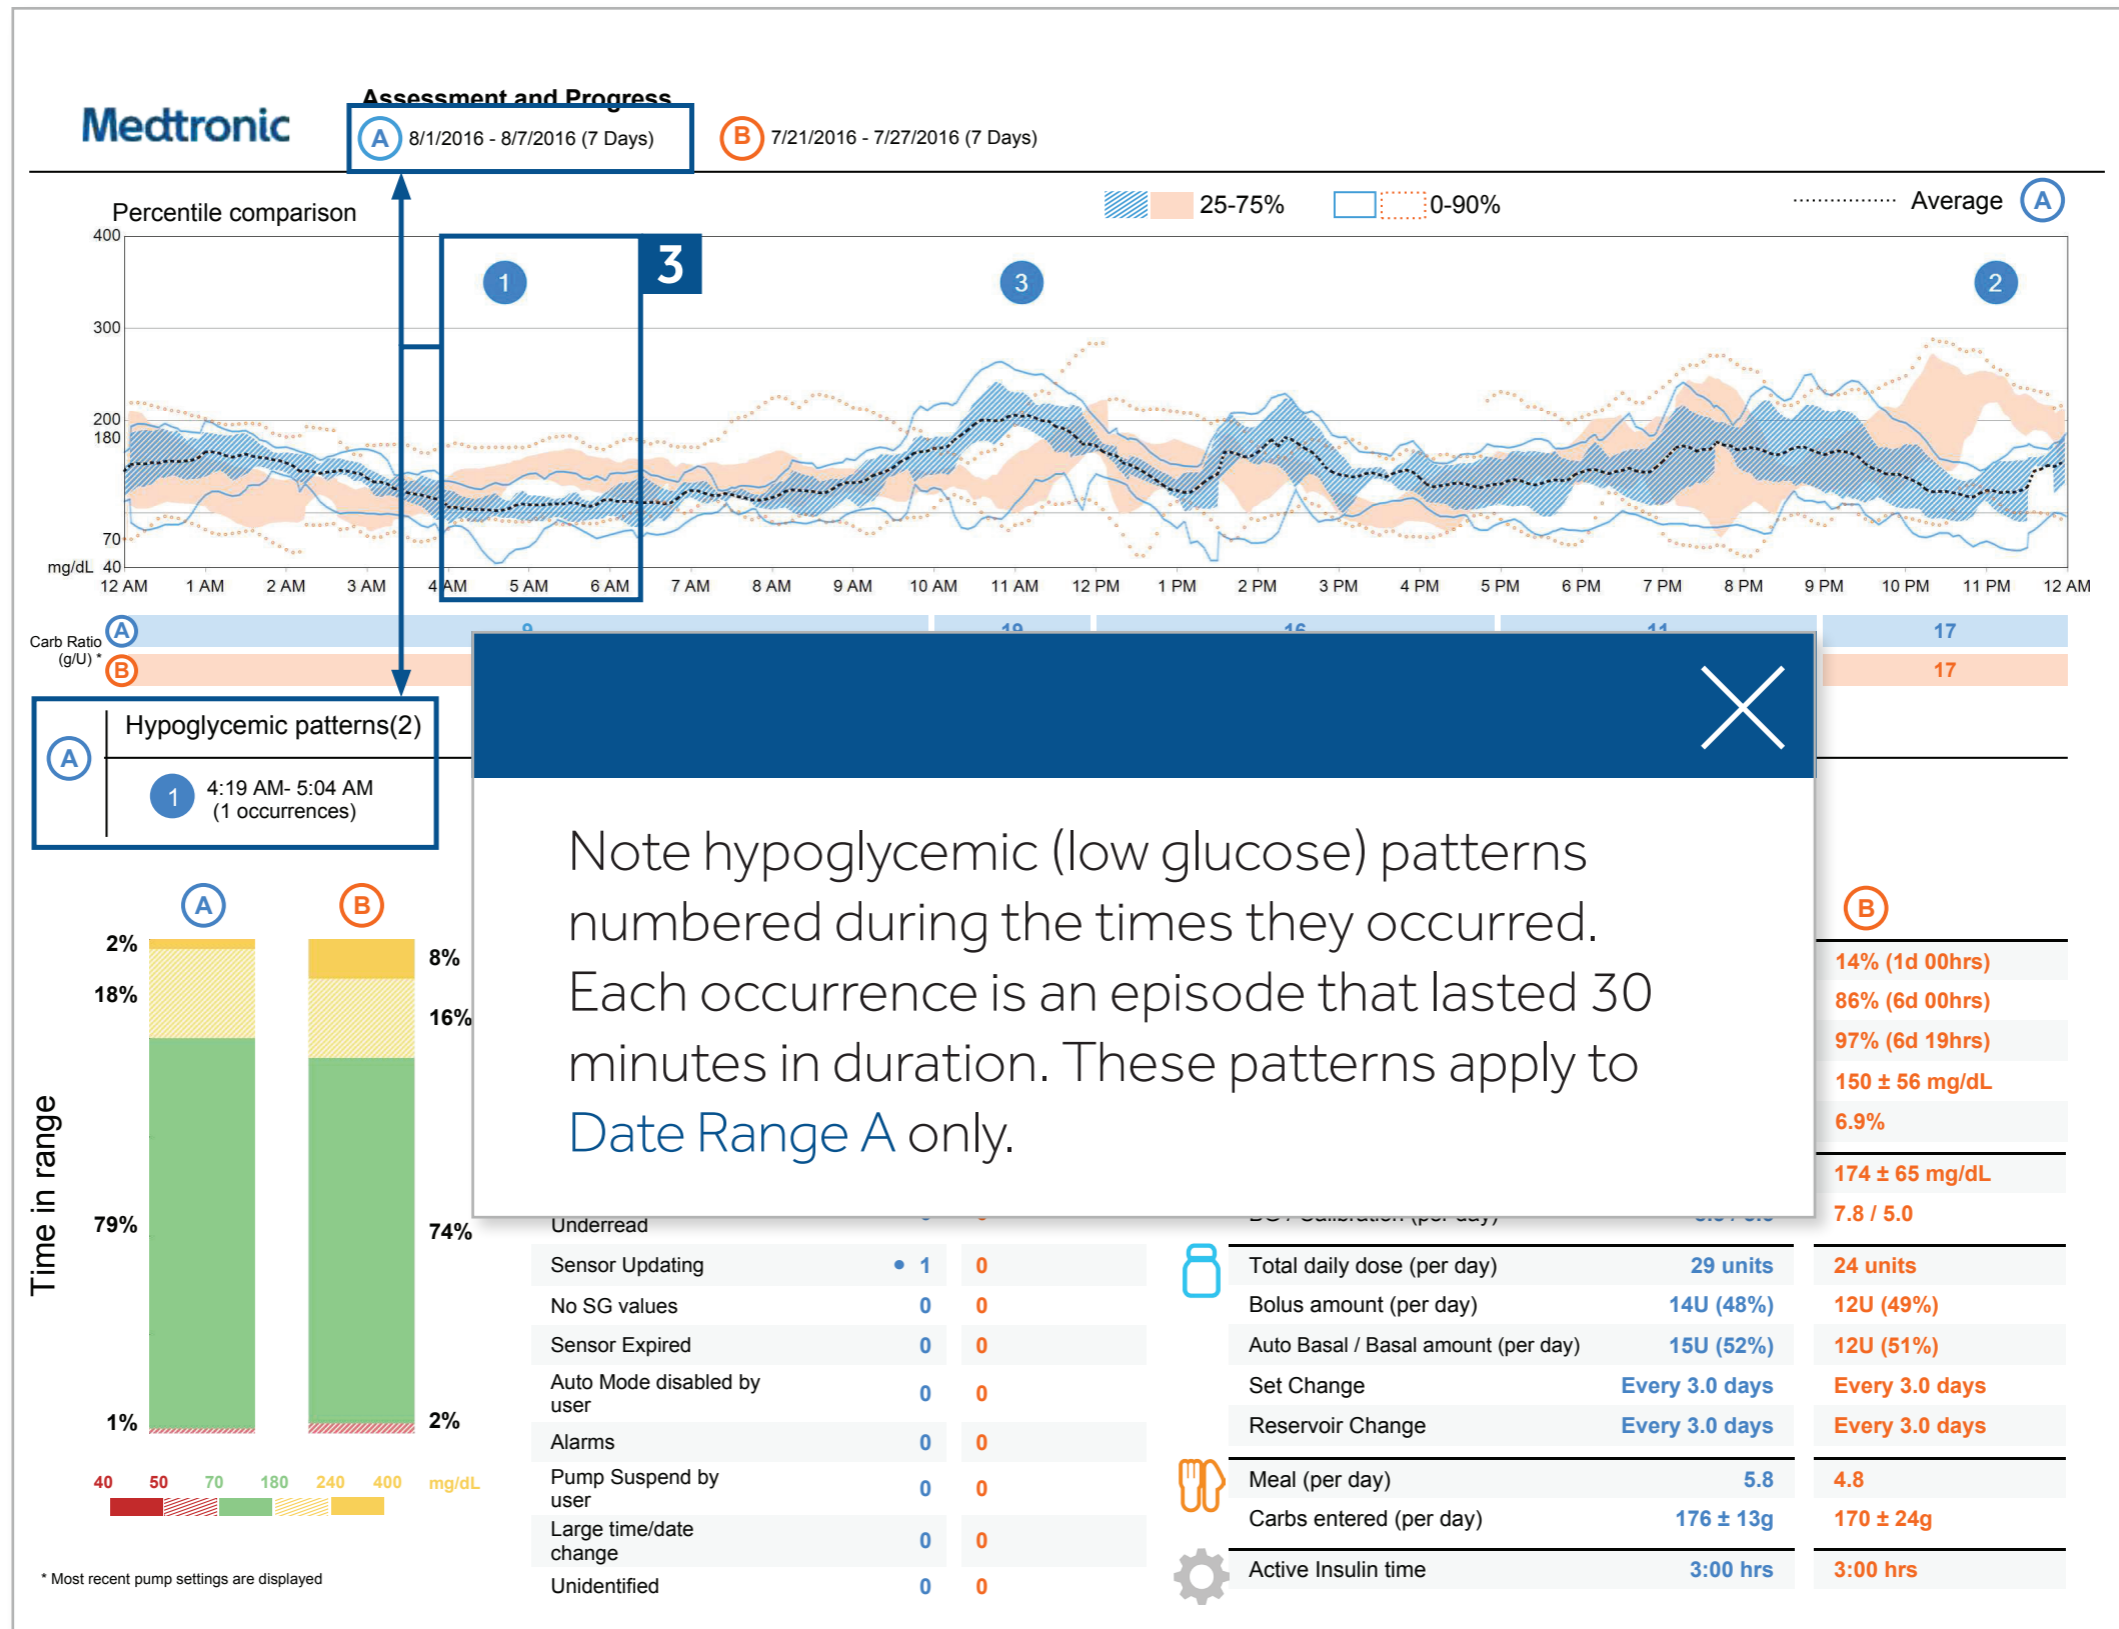


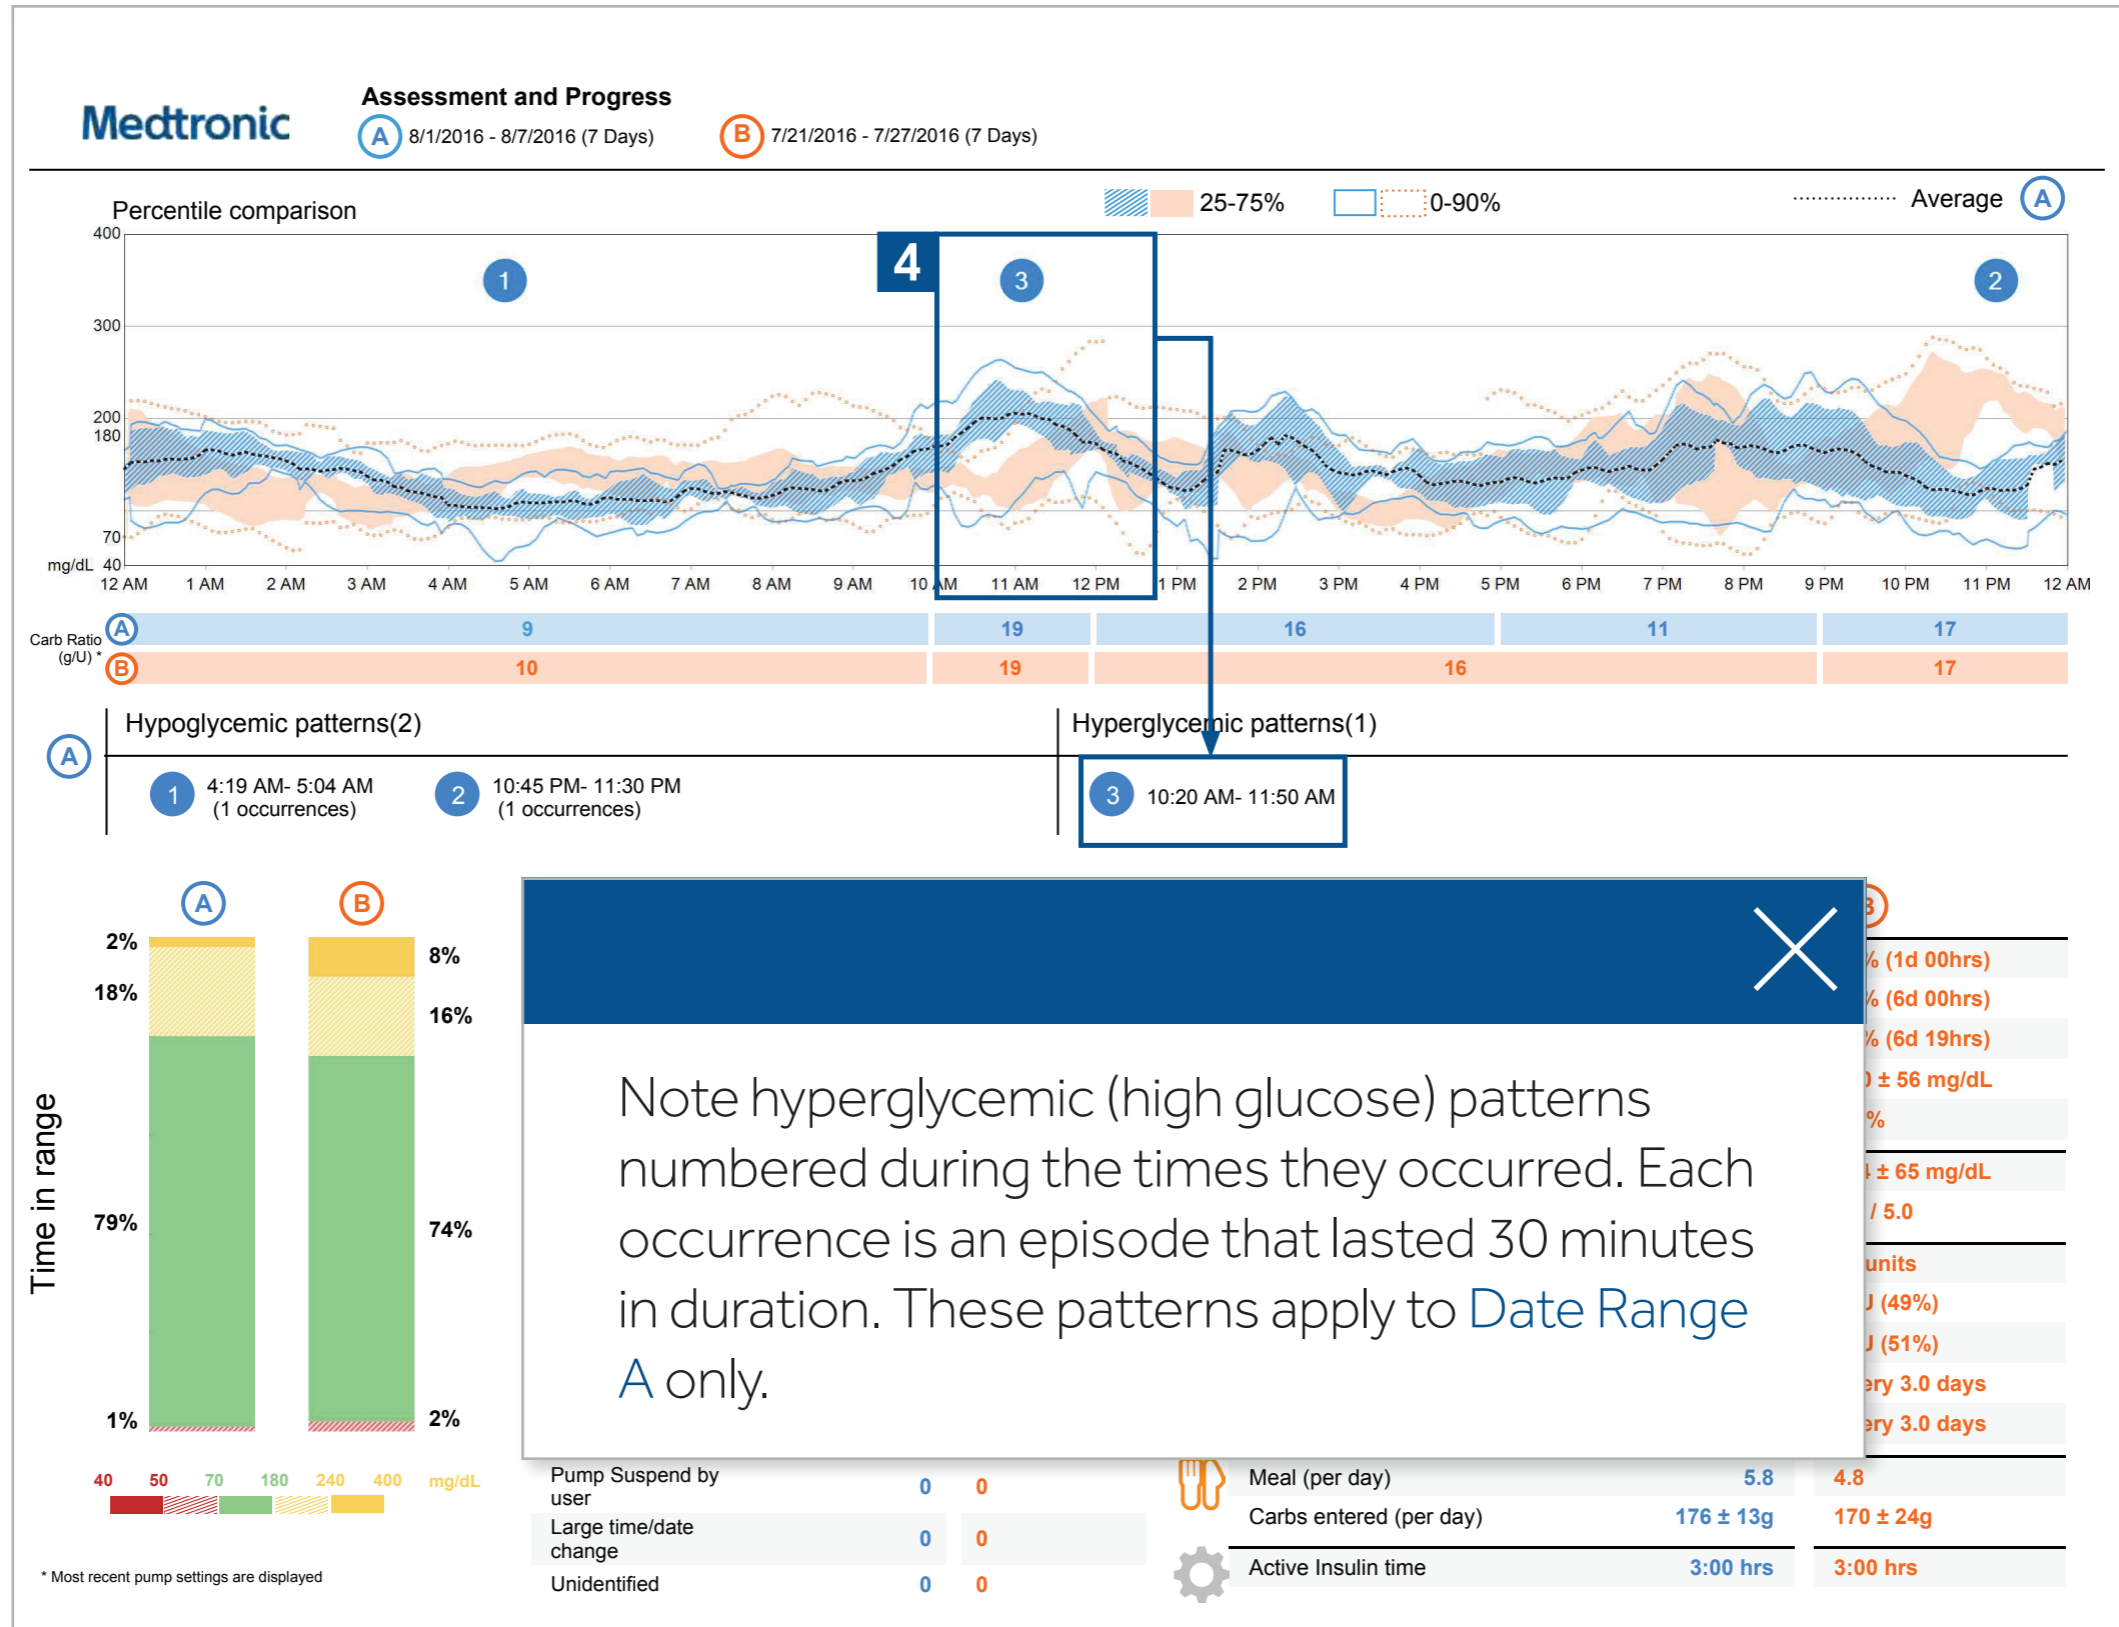


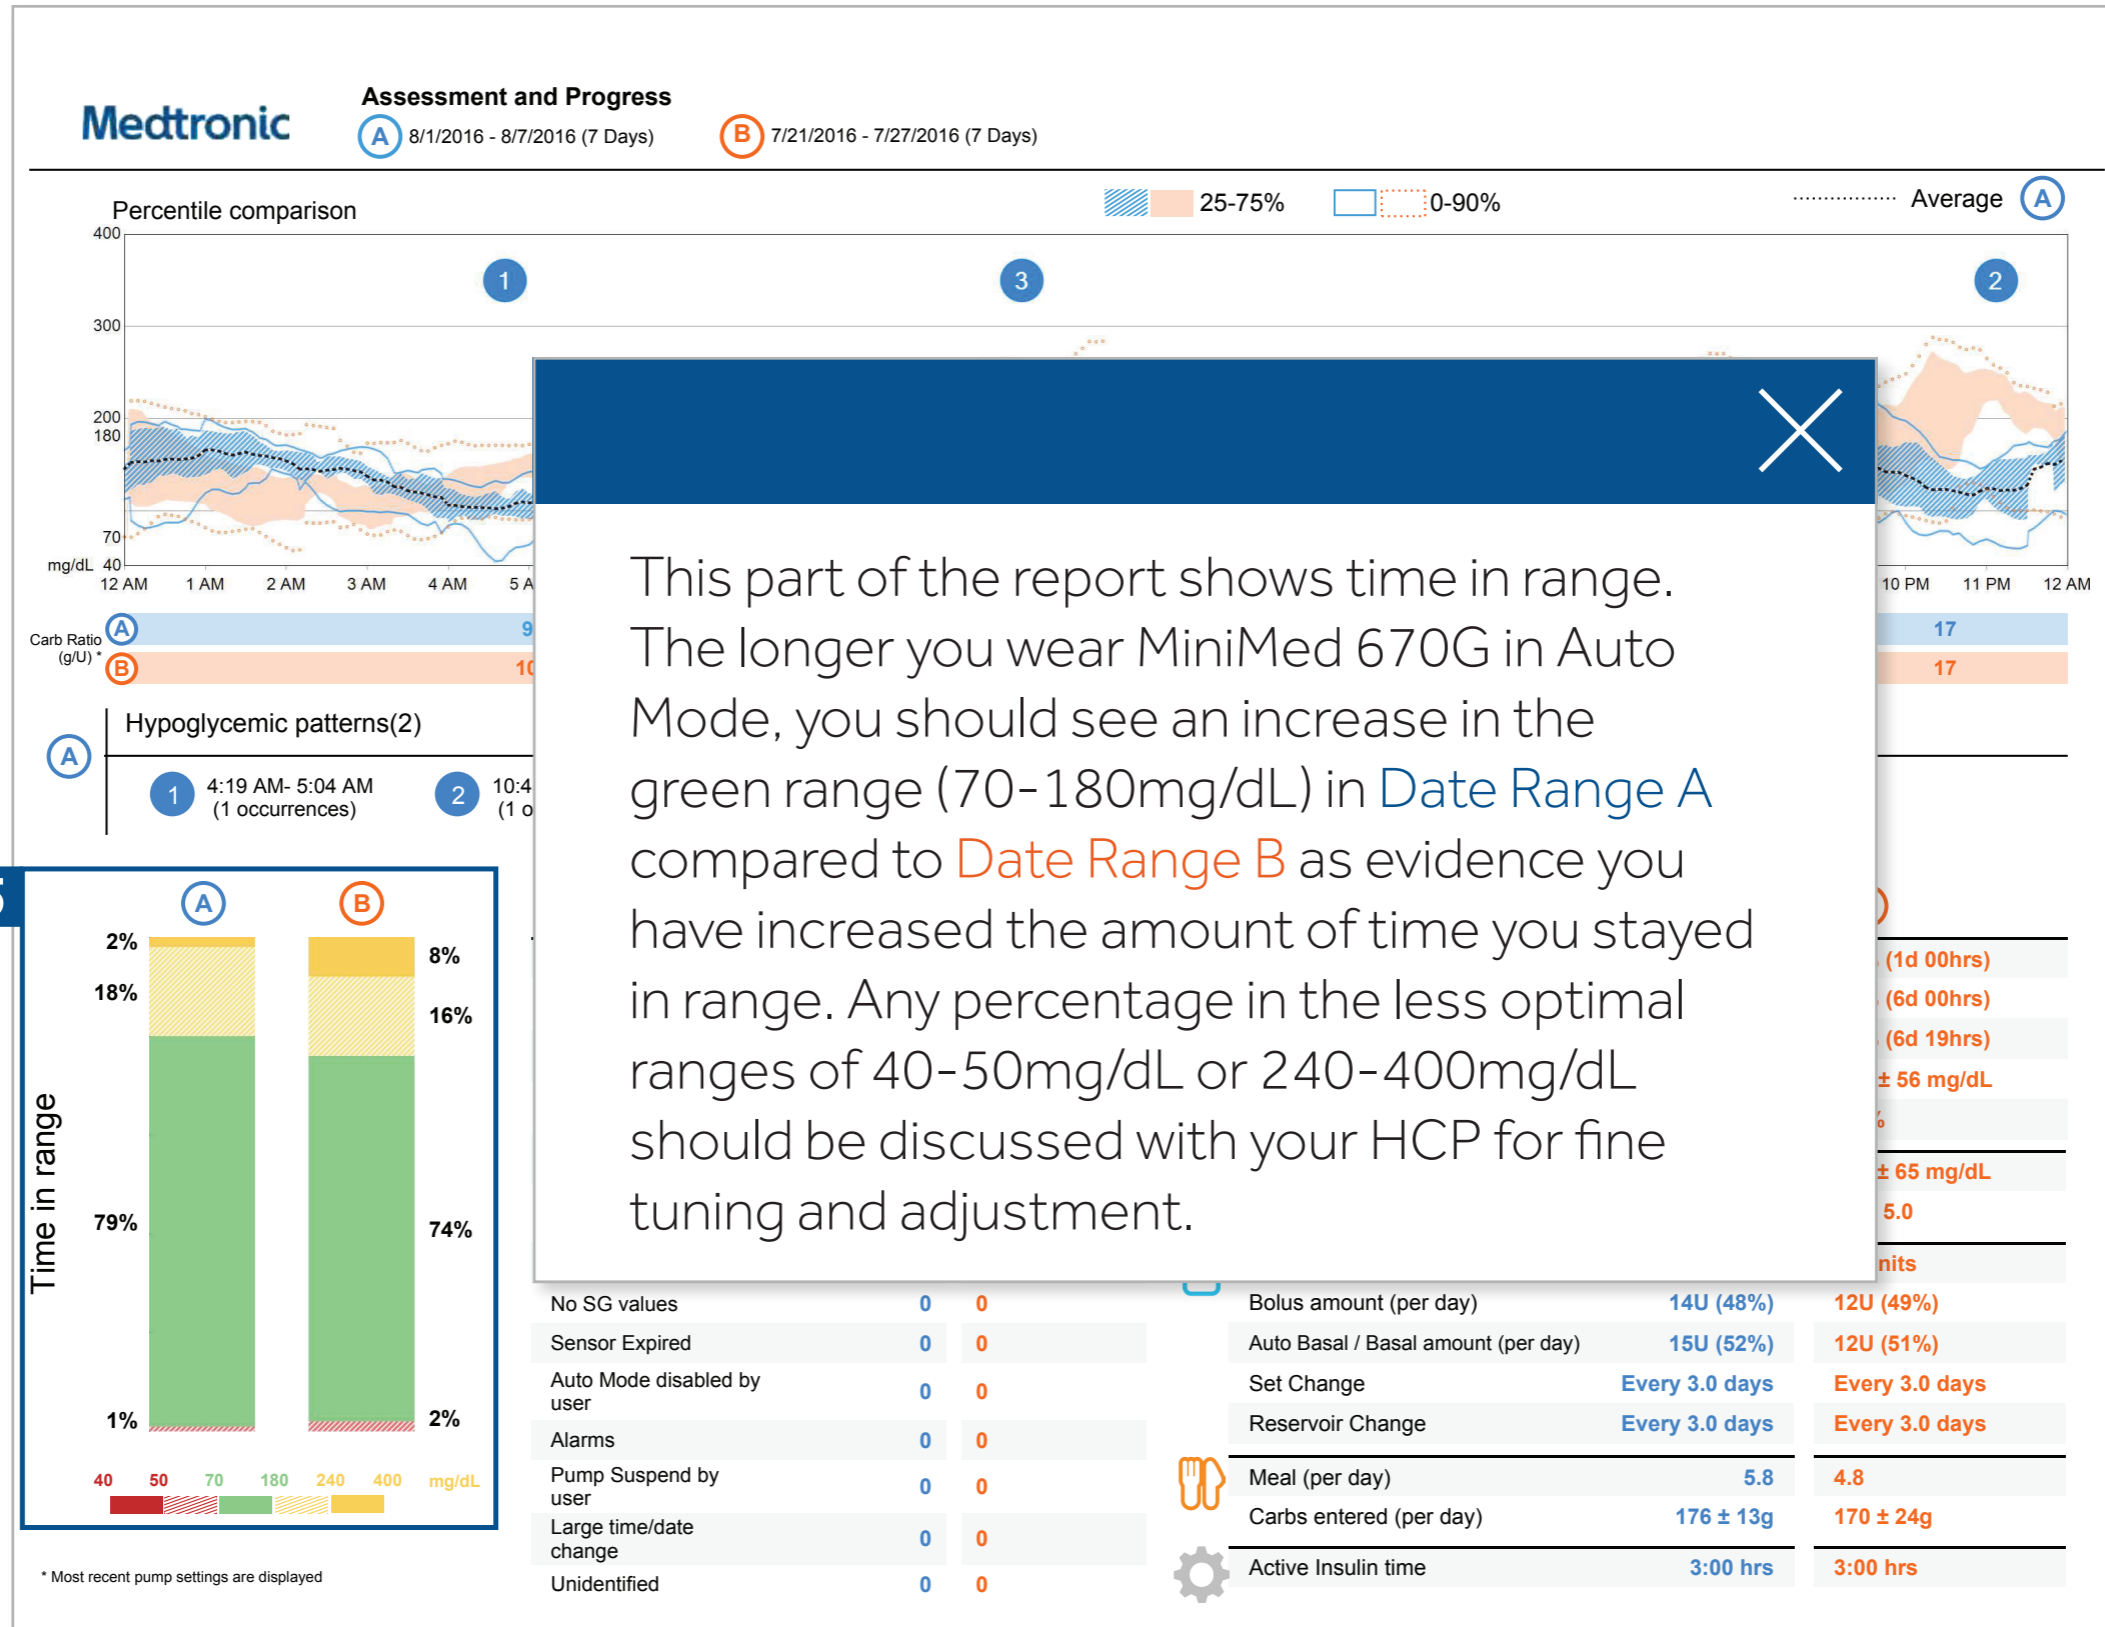

This part of the report shows time in range. The longer you wear MiniMed 670G in Auto Mode, you should see an increase in the green range (70-180mg/dL) in **Date Range A** compared to **Date Range B** as evidence you have increased the amount of time you stayed in range. Any percentage in the less optimal ranges of 40-50mg/dL or 240-400mg/dL should be discussed with your HCP for fine tuning and adjustment.

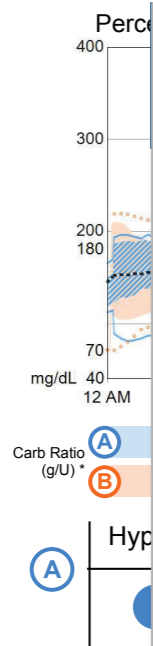


This table can be used to help you understand the frequency and causes of your Auto Mode exits, if you have the MiniMed 670G system. Review this section with your HCP to uncover behaviors that will assist you in returning to Auto Mode.

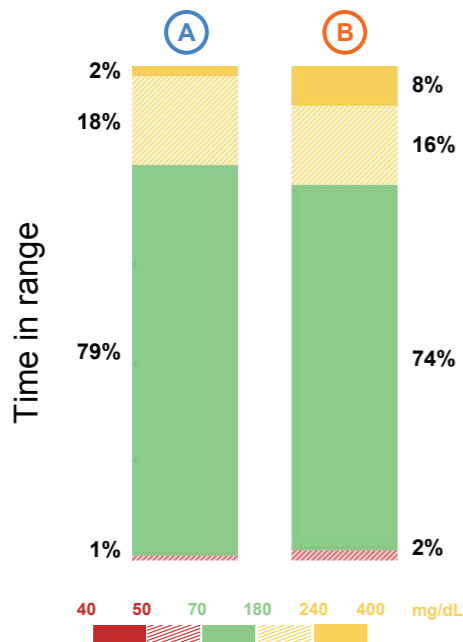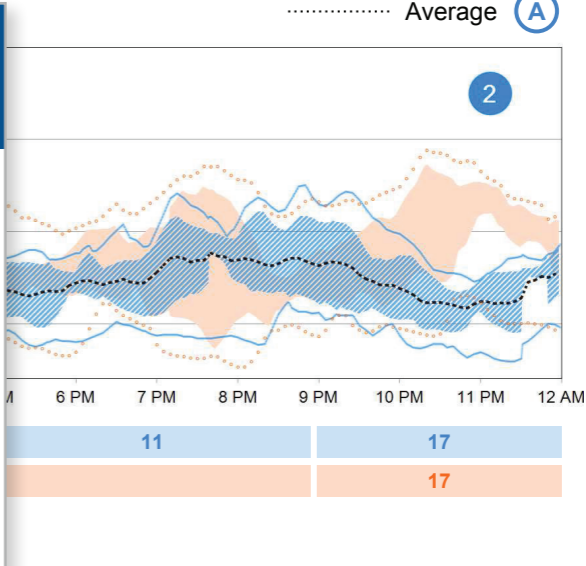

* Most recent pump settings are displayed

Auto Mode Exits	A	B
No Calibration	0	0
High SG Auto Mode Exit	0	0
Auto Mode max delivery	0	0
Auto Mode min delivery	1	0
BG required for Auto Mode	1	0
Sensor Algorithm Underread	0	0
Sensor Updating	1	0
No SG values	0	0
Sensor Expired	0	0
Auto Mode disabled by user	0	0
Alarms	0	0
Pump Suspend by user	0	0
Large time/date change	0	0
Unidentified	0	0

Statistics	A	B
Auto Mode (per week)	98% (6d 20hrs)	14% (1d 00hrs)
Manual Mode (per week)	2% (3hrs)	86% (6d 00hrs)
Sensor Wear (per week)	96% (6d 18hrs)	97% (6d 19hrs)
Average SG ± SD	143 ± 43 mg/dL	150 ± 56 mg/dL
Estimated A1C	6.6%	6.9%
Average BG	144 ± 34 mg/dL	174 ± 65 mg/dL
BG / Calibration (per day)	8.5 / 5.6	7.8 / 5.0
Total daily dose (per day)	29 units	24 units
Bolus amount (per day)	14U (48%)	12U (49%)
Auto Basal / Basal amount (per day)	15U (52%)	12U (51%)
Set Change	Every 3.0 days	Every 3.0 days
Reservoir Change	Every 3.0 days	Every 3.0 days
Meal (per day)	5.8	4.8
Carbs entered (per day)	176 ± 13g	170 ± 24g
Active Insulin time	3:00 hrs	3:00 hrs

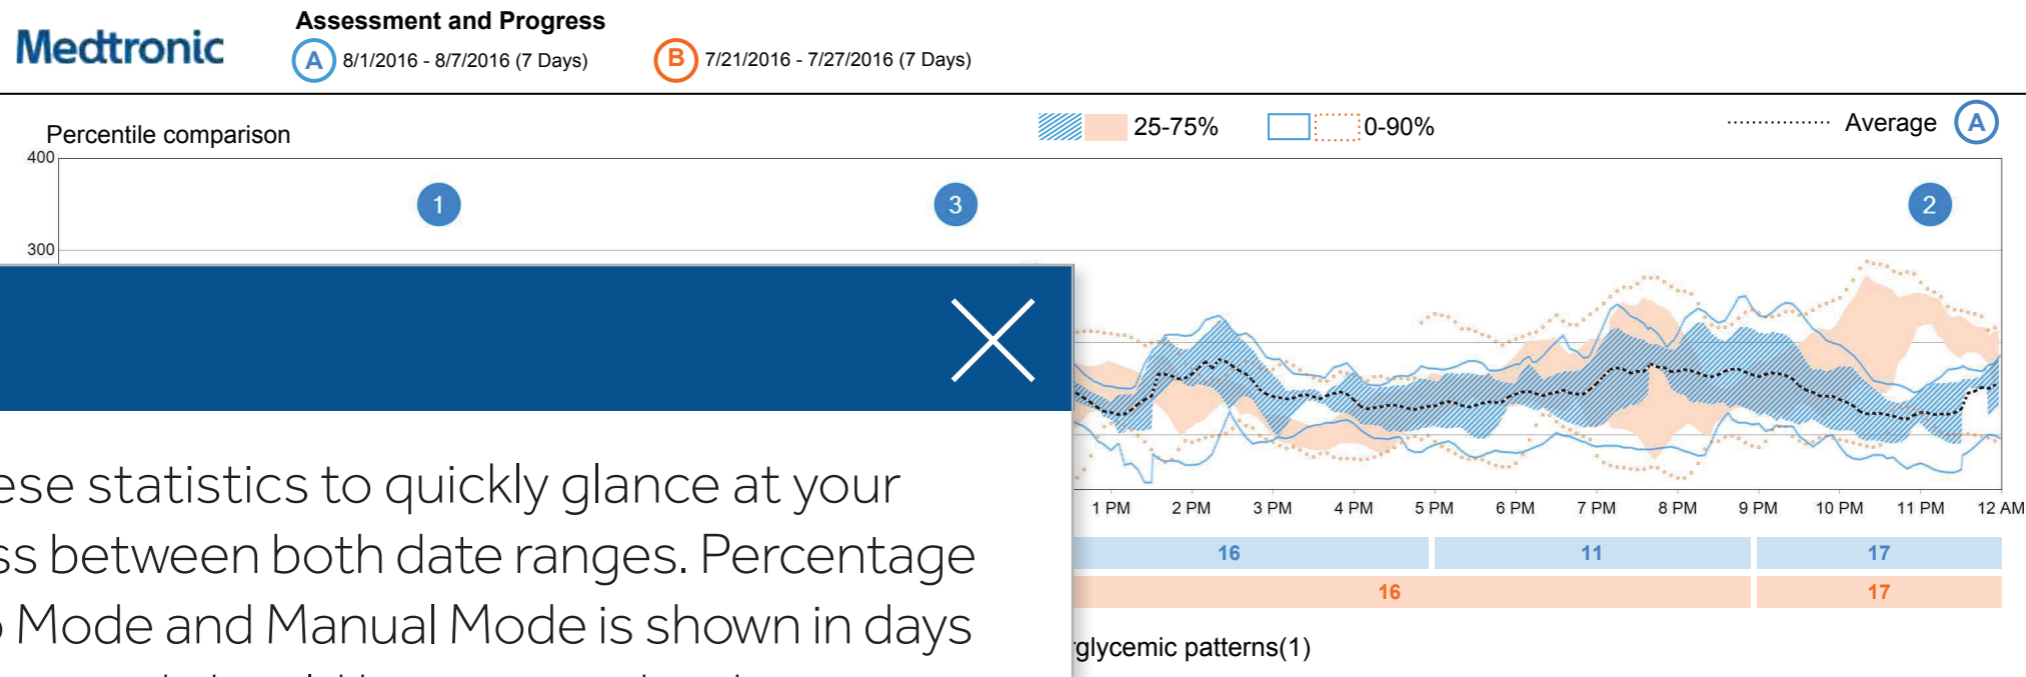


Use these statistics to quickly glance at your progress between both date ranges. Percentage of Auto Mode and Manual Mode is shown in days and hours and should be reviewed with your HCP to optimize your glucose management while using the MiniMed 670G system.

Take a look at your sensor wear and your average SG. This is an average of all your sensor glucose readings. Does your average SG appear to be in the range of your glucose control goals?

Estimated A1C is a calculation based on all available SG values and should not be used as a replacement for a lab A1C prescribed by your HCP.

Statistics	(A)	(B)
Auto Mode (per week)	98% (6d 20hrs)	14% (1d 00hrs)
Manual Mode (per week)	2% (3hrs)	86% (6d 00hrs)
Sensor Wear (per week)	96% (6d 18hrs)	97% (6d 19hrs)
Average SG \pm SD	143 \pm 43 mg/dL	150 \pm 56 mg/dL
Estimated A1C	6.6%	6.9%
Average BG	144 \pm 34 mg/dL	174 \pm 65 mg/dL
BG / Calibration (per day)	8.5 / 5.6	7.8 / 5.0
Total daily dose (per day)	29 units	24 units
Bolus amount (per day)	14U (48%)	12U (49%)
Auto Basal / Basal amount (per day)	15U (52%)	12U (51%)
Set Change	Every 3.0 days	Every 3.0 days
Reservoir Change	Every 3.0 days	Every 3.0 days
Meal (per day)	5.8	4.8
Carbs entered (per day)	176 \pm 13g	170 \pm 24g
Active Insulin time	3:00 hrs	3:00 hrs

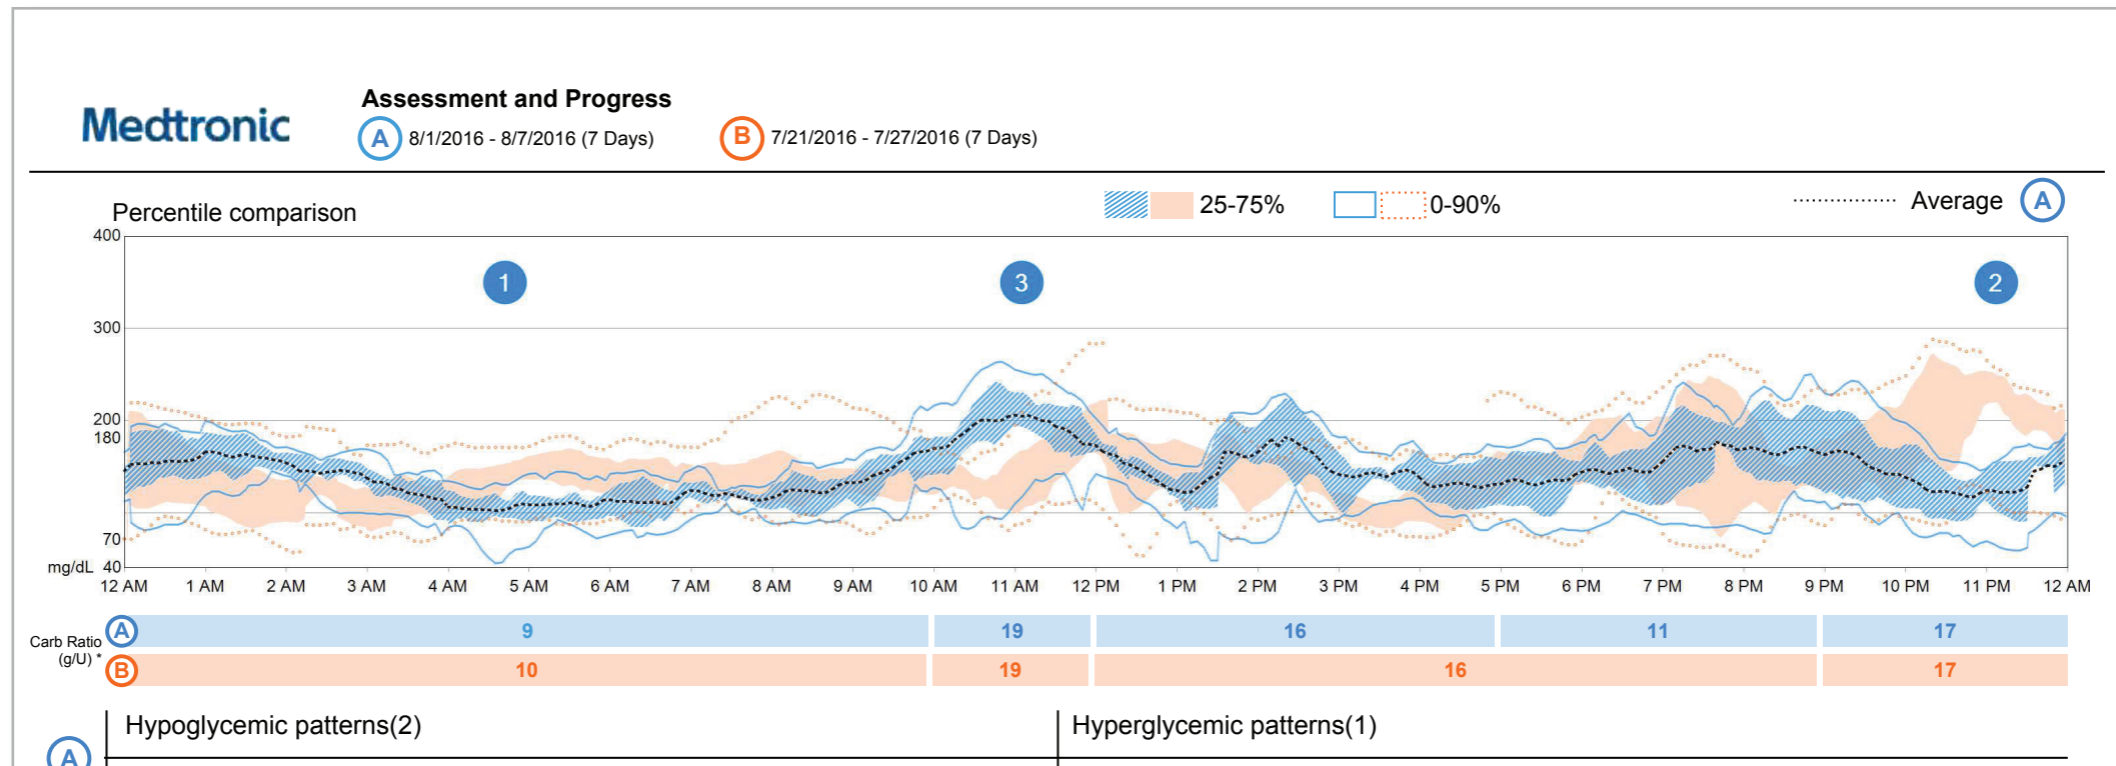


Did your average blood glucose (BG) in **Date Range A** improve from **Date Range B**? Are you maintaining 3 to 4 BG readings/day according to the American Diabetes Association (ADA) guidelines? Do you calibrate 3-4 times/day for optimal sensor performance? There will be times when you calibrate more than this because the system has requested you to do so.

10:20 AM- 11:50 AM

Statistics

	(A)	(B)
Auto Mode (per week)	98% (6d 20hrs)	14% (1d 00hrs)
Manual Mode (per week)	2% (3hrs)	86% (6d 00hrs)
Sensor Wear (per week)	96% (6d 18hrs)	97% (6d 19hrs)
Average SG ± SD	143 ± 43 mg/dL	150 ± 56 mg/dL
Estimated A1C	6.6%	6.9%
Average BG	144 ± 34 mg/dL	174 ± 65 mg/dL
BG / Calibration (per day)	8.5 / 5.6	7.8 / 5.0
Total daily dose (per day)	29 units	24 units
Bolus amount (per day)	14U (48%)	12U (49%)
Auto Basal / Basal amount (per day)	15U (52%)	12U (51%)
Set Change	Every 3.0 days	Every 3.0 days
Reservoir Change	Every 3.0 days	Every 3.0 days
Meal (per day)	5.8	4.8
Carbs entered (per day)	176 ± 13g	170 ± 24g
Active Insulin time	3:00 hrs	3:00 hrs

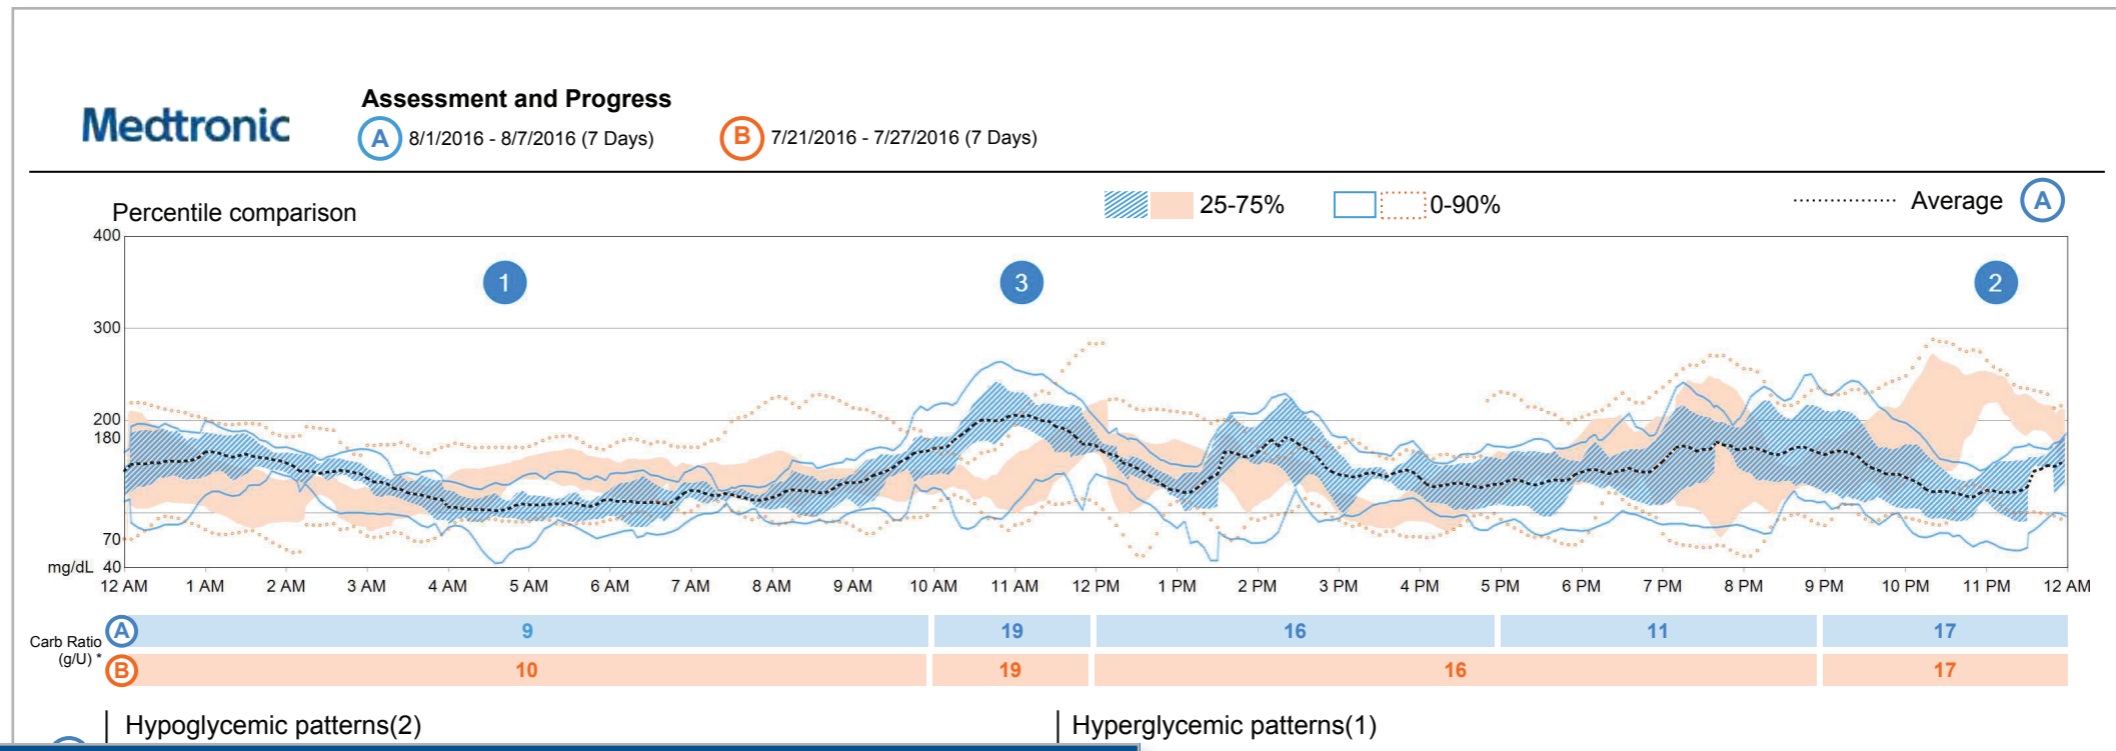


This table shows you the distribution of your insulin usage. Take a look at your insulin total daily dose. How much insulin do you use on average per day? You can use this number to see how much insulin is needed on a monthly basis.

Are you changing your infusion on the recommended routine given by your HCP? Are you changing your reservoir every 2-3 days?

10:20 AM- 11:50 AM

Statistics

	(A)	(B)
Auto Mode (per week)	98% (6d 20hrs)	14% (1d 00hrs)
Manual Mode (per week)	2% (3hrs)	86% (6d 00hrs)
Sensor Wear (per week)	96% (6d 18hrs)	97% (6d 19hrs)
Average SG ± SD	143 ± 43 mg/dL	150 ± 56 mg/dL
Estimated A1C	6.6%	6.9%
Average BG	144 ± 34 mg/dL	174 ± 65 mg/dL
BG / Calibration (per day)	8.5 / 5.6	7.8 / 5.0
Total daily dose (per day)	29 units	24 units
Bolus amount (per day)	14U (48%)	12U (49%)
Auto Basal / Basal amount (per day)	15U (52%)	12U (51%)
Set Change	Every 3.0 days	Every 3.0 days
Reservoir Change	Every 3.0 days	Every 3.0 days
Meal (per day)	5.8	4.8
Carbs entered (per day)	176 ± 13g	170 ± 24g
Active Insulin time	3:00 hrs	3:00 hrs

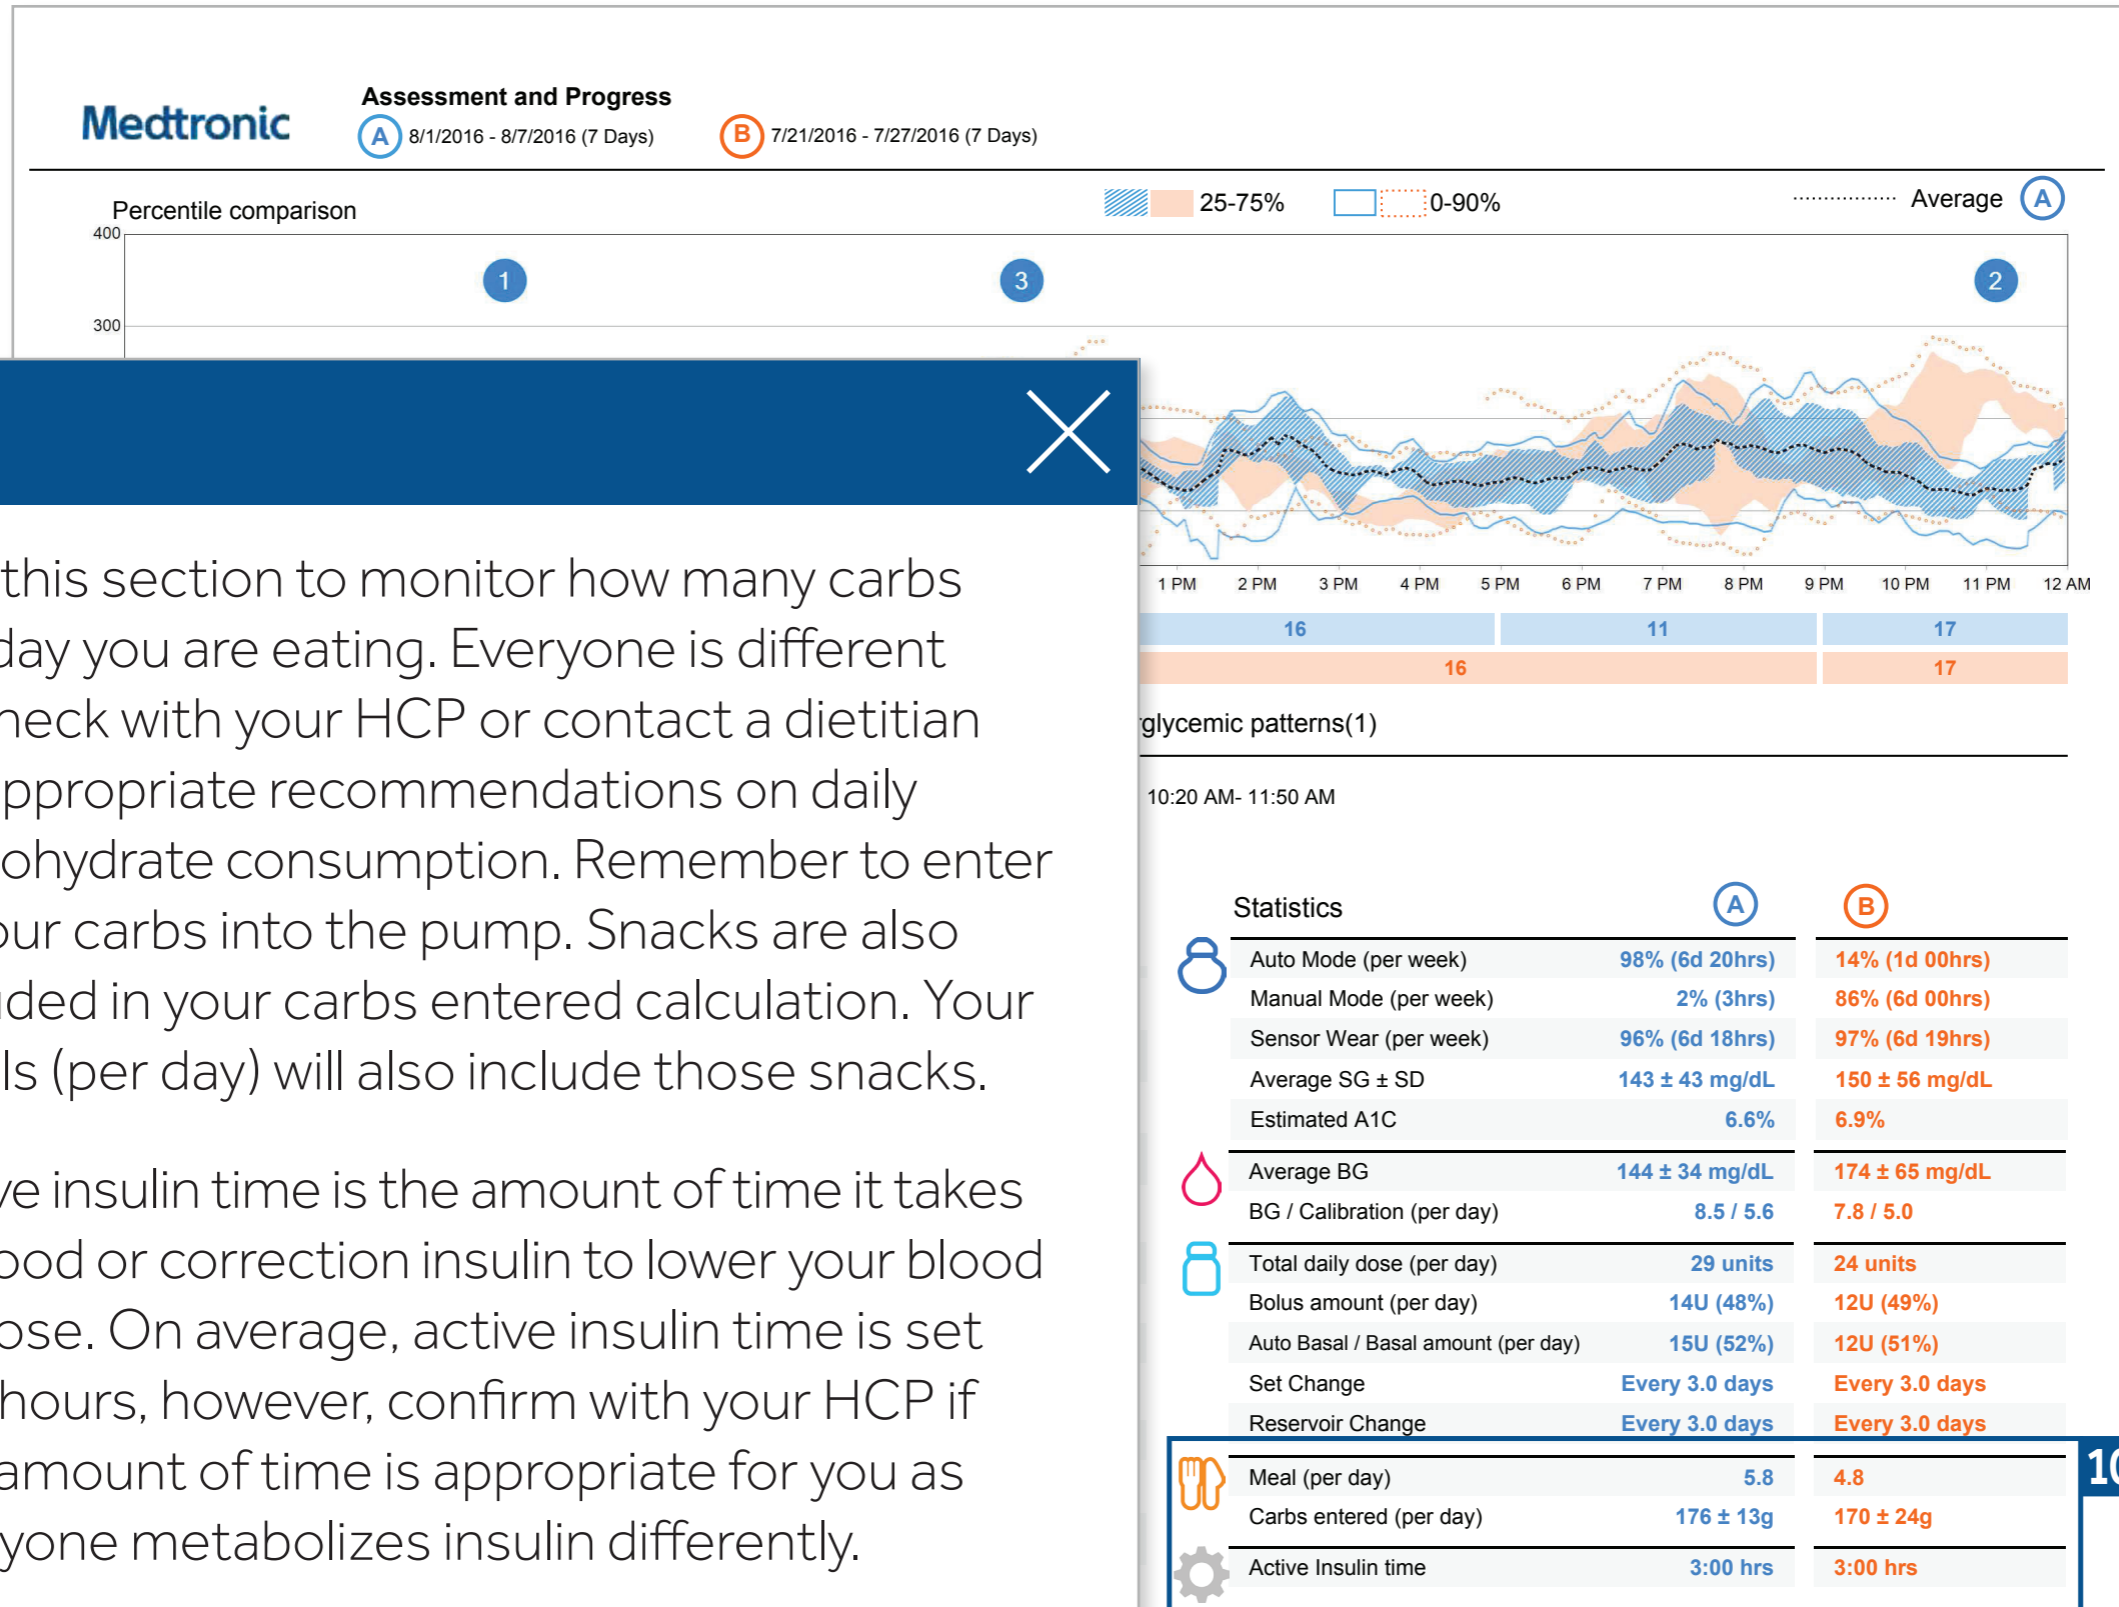

Use this section to monitor how many carbs per day you are eating. Everyone is different so check with your HCP or contact a dietitian for appropriate recommendations on daily carbohydrate consumption. Remember to enter all your carbs into the pump. Snacks are also included in your carbs entered calculation. Your meals (per day) will also include those snacks.

Active insulin time is the amount of time it takes for food or correction insulin to lower your blood glucose. On average, active insulin time is set to 3 hours, however, confirm with your HCP if this amount of time is appropriate for you as everyone metabolizes insulin differently.

Medtronic

18000 Devonshire Street
Northridge, CA 91325
USA
800.646.4633

Toll-free: 800.328.2518
(24-hour technical support for
physicians and medical professionals)

CareLink and MiniMed are registered trademarks of Medtronic MiniMed, Inc.
950M16445-011 20170315 © 2017 Medtronic MiniMed, Inc. All Rights Reserved.

www.medtronicdiabetes.com