

POSITIVE AND NEGATIVE DUCT ACCREDITATION (PANDA) SYSTEM AIRFLOW™ INSTRUMENTS MODEL PAN300 SERIES

OPERATION AND SERVICE MANUAL

P/N 6005447, REV B
MARCH 2021



START SEEING THE BENEFITS OF REGISTERING TODAY!

Thank you for your TSI instrument purchase. Occasionally, TSI releases information on software updates, product enhancements and new products. By registering your instrument, TSI will be able to send this important information to you.

<http://register.tsi.com>

As part of the registration process, you will be asked for your comments on TSI products and services. TSI's customer feedback program gives customers like you a way to tell us how we are doing.



UNDERSTANDING, ACCELERATED

TSI Incorporated - Visit our website **www.tsi.com** for more information.

USA
UK
France
Germany

Tel: +1 800 874 2811
Tel: +44 149 4 459200
Tel: +33 1 41 19 21 99
Tel: +49 241 523030

India
China
Singapore

Tel: +91 80 67877200
Tel: +86 10 8219 7688
Tel: +65 6595 6388

Copyright©

TSI Incorporated / 2011-2021 / All rights reserved.

Address

TSI Incorporated / 500 Cardigan Road / Shoreview, MN 55126 / USA

Fax No.

(651) 490-3824

LIMITATION OF WARRANTY AND LIABILITY (effective February 2015)

(For country-specific terms and conditions outside of the USA, please visit www.tsi.com.)

Seller warrants the goods, excluding software, sold hereunder, under normal use and service as described in the operator's manual, to be free from defects in workmanship and material for **24 months**, or if less, the length of time specified in the operator's manual, from the date of shipment to the customer. This warranty period is inclusive of any statutory warranty. This limited warranty is subject to the following exclusions and exceptions:

- a. Hot-wire or hot-film sensors used with research anemometers, and certain other components when indicated in specifications, are warranted for 90 days from the date of shipment;
- b. Pumps are warranted for hours of operation as set forth in product or operator's manuals;
- c. Parts repaired or replaced as a result of repair services are warranted to be free from defects in workmanship and material, under normal use, for 90 days from the date of shipment;
- d. Seller does not provide any warranty on finished goods manufactured by others or on any fuses, batteries or other consumable materials. Only the original manufacturer's warranty applies;
- e. This warranty does not cover calibration requirements, and seller warrants only that the instrument or product is properly calibrated at the time of its manufacture. Instruments returned for calibration are not covered by this warranty;
- f. This warranty is **VOID** if the instrument is opened by anyone other than a factory authorized service center with the one exception where requirements set forth in the manual allow an operator to replace consumables or perform recommended cleaning;
- g. This warranty is **VOID** if the product has been misused, neglected, subjected to accidental or intentional damage, or is not properly installed, maintained, or cleaned according to the requirements of the manual. Unless specifically authorized in a separate writing by Seller, Seller makes no warranty with respect to, and shall have no liability in connection with, goods which are incorporated into other products or equipment, or which are modified by any person other than Seller.

The foregoing is **IN LIEU OF** all other warranties and is subject to the **LIMITATIONS** stated herein. **NO OTHER EXPRESS OR IMPLIED WARRANTY OF FITNESS FOR PARTICULAR PURPOSE OR MERCHANTABILITY IS MADE. WITH RESPECT TO SELLER'S BREACH OF THE IMPLIED WARRANTY AGAINST INFRINGEMENT, SAID WARRANTY IS LIMITED TO CLAIMS OF DIRECT INFRINGEMENT AND EXCLUDES CLAIMS OF CONTRIBUTORY OR INDUCED INFRINGEMENTS. BUYER'S EXCLUSIVE REMEDY SHALL BE THE RETURN OF THE PURCHASE PRICE DISCOUNTED FOR REASONABLE WEAR AND TEAR OR AT SELLER'S OPTION REPLACEMENT OF THE GOODS WITH NON-INFRINGEMENTS.**

TO THE EXTENT PERMITTED BY LAW, THE EXCLUSIVE REMEDY OF THE USER OR BUYER, AND THE LIMIT OF SELLER'S LIABILITY FOR ANY AND ALL LOSSES, INJURIES, OR DAMAGES CONCERNING THE GOODS (INCLUDING CLAIMS BASED ON CONTRACT, NEGLIGENCE, TORT, STRICT LIABILITY OR OTHERWISE) SHALL BE THE RETURN OF GOODS TO SELLER AND THE REFUND OF THE PURCHASE PRICE, OR, AT THE OPTION OF SELLER, THE REPAIR OR REPLACEMENT OF THE GOODS. IN THE CASE OF SOFTWARE,

SELLER WILL REPAIR OR REPLACE DEFECTIVE SOFTWARE OR IF UNABLE TO DO SO, WILL REFUND THE PURCHASE PRICE OF THE SOFTWARE. IN NO EVENT SHALL SELLER BE LIABLE FOR LOST PROFITS, BUSINESS INTERRUPTION, OR ANY SPECIAL, INDIRECT, CONSEQUENTIAL OR INCIDENTAL DAMAGES. SELLER SHALL NOT BE RESPONSIBLE FOR INSTALLATION, DISMANTLING OR REINSTALLATION COSTS OR CHARGES. No Action, regardless of form, may be brought against Seller more than 12 months after a cause of action has accrued. The goods returned under warranty to Seller's factory shall be at Buyer's risk of loss, and will be returned, if at all, at Seller's risk of loss.

Buyer and all users are deemed to have accepted this LIMITATION OF WARRANTY AND LIABILITY, which contains the complete and exclusive limited warranty of Seller. This LIMITATION OF WARRANTY AND LIABILITY may not be amended, modified or its terms waived, except by writing signed by an Officer of Seller.

Service Policy

Knowing that inoperative or defective instruments are as detrimental to TSI as they are to our customers, our service policy is designed to give prompt attention to any problems. If any malfunction is discovered, please contact your nearest sales office or representative, or call TSI's Customer Service department at (800) 680-1220 (USA) or (001 651) 490-2860 (International) or visit www.tsi.com.

Trademarks

TSI and TSI logo are registered trademarks of TSI Incorporated in the United States and may be protected under other country's trademark registrations.

CONTENTS

CHAPTER 1 UNPACKING AND PARTS IDENTIFICATION.....	1
CHAPTER 2 PREPARING PAN300 SYSTEM FOR AIR DUCT LEAK TESTING	5
CHAPTER 3 PERFORMING A DUCT LEAKAGE TEST	11
Measuring Duct Static Pressure	11
Measuring Duct Leakage Flow	12
Turning on the PAN300 Duct Leakage Tester.....	12
Using Leakage Test Application in the Model TA465-P	13
Troubleshooting Guide	16
APPENDIX A SPECIFICATIONS.....	17
APPENDIX B LEAKAGE TESTING STANDARDS HIGHLIGHTS ...	21
Standards Supported.....	21
EU Standards	22
US Standards	25
APPENDIX C TYPICAL SETUP.....	29
APPENDIX D PROCEDURE FOR USING SMOKE PELLETS IN LEAKAGE TESTERS	31


(This page intentionally left blank)


Chapter 1

Unpacking and Parts Identification

Carefully unpack the PANDA system and instrument cases from the shipping container. Check the individual parts against the list of components below. If anything is missing or damaged, notify TSI® Incorporated (TSI®) immediately.

The PANDA system consists of the following:

Qty	Description	Part Number	Reference Picture
1	Low flow nozzle	6002598	
1	Primary duct adapter spigot plus rubber bung (to fit to test duct)	6002638	
1	Cam lock primary spigot (to connect flexi-duct to PANDA)	6002607	
2	Ø4-in. (100-mm) adjustable over lock straps	6002683	
1	13-ft (4-m) long Ø4-in. (100-mm) plastic flexible duct	6002667	
2	20-in. (500-mm) silicone tubes (red)	AFL9020004	

Qty	Description	Part Number	Reference Picture
2	20-in. (500-mm) silicone tubes (blue)	AFL9020005	
1	16-ft (5-m) silicone tube (blue)	AFL9020005	
1	Smoke cap holder assembly	AFL71549801	
1	Smoke pellets	AFL9004167	
1	K-type thermocouple probe	AFL82859201	
3	Instrument adapter	AFL82859401	
1	Operation and User's manual	6005447	

The following two instruments should be used in conjunction with the PANDA unit:

TA465-P Multi-function Instrument		Refer to TA465 Operation and Service Manual supplied with the instrument for additional parts supplied as standard.
PVM620 Micromanometer		Refer to PVM620 Operation and Service Manual supplied with the instrument for additional parts supplied as standard.

**IMPORTANT—
Read Before Using the PANDA for the First Time**

It is **IMPORTANT** that the PANDA be connected to the power supply using a 30 mA residual-current device (RCD) or Ground Fault Circuit Interrupter (GFCI).

It is **IMPORTANT** that the 110V PANDA (yellow power socket) be connected only to 110V to 120V supplies. Connecting it to a higher voltage supply will permanently damage the inverter.

The 220V/240V PANDA (blue power socket) should only be connected to 200V to 240V power supplies.

When storing the PANDA in a vertical position, please ensure that the straps holding the instrument box are in place and tightened first.

The PANDA is designed so that the instrument box and duct carry tube are removable to lighten the load when lifting.

DANGER

Turn the isolation switch to the **OFF** position and wait 10 minutes prior to disconnecting power.

(This page intentionally left blank)

Chapter 2

Preparing PAN300 System for Air Duct Leak Testing

The following procedure should be followed carefully so that safe and accurate leakage testing can be achieved:

Successfully completing a duct leakage test requires certain information be compiled prior to starting the test. Refer to [Appendix B](#) for a discussion of standards relating to duct leakage testing. The list below indicates the information required:

- Type of leakage test to be performed (Positive or negative).
- Leakage standard to be followed.
- Air tightness/leakage class to be achieved
- Amount of ductwork to be tested, such as the complete system or a statistical sample.

1. Select the section of the ductwork to be tested.
2. Calculate the surface area of the ductwork of the section to be tested.
3. Temporarily seal the all openings of the ductwork except one, which will be connected to the PAN300 duct leakage tester.
4. Position the PAN300 unit as close to the remaining opening in the ductwork as possible to minimize the flexible tubing needed. Minimize bends in the flexible tubing to reduce the pressure loss, giving the best performance.
5. Make sure the Fan Control Switch on the Fan Speed Controller is in the **OFF** position and the multi-turn Fan Speed Control potentiometer is fully turned counter-clockwise using the pictures of the VFD in Figure 1 as a reference. Plug the cord into the PANDA unit as shown in Figure 2 and Figure 3. Then connect the other end of the cord to a suitable electrical supply.

CAUTION

Remove the power cord from the PANDA duct leakage tester before tilting it to the vertical position to avoid damaging the cord.

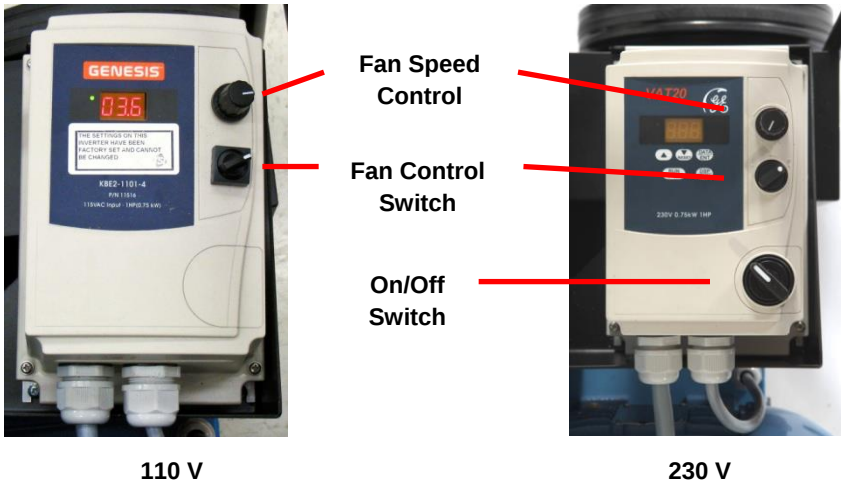


Figure 1. 110V and 230V Fan Speed Controllers

NOTE

The control pad on the Fan Speed Controller has been disabled.




Figure 2. Receptacle for Power Cord



Figure 3. Connected Power Cord

6. Fit the primary duct adapter spigot (black sheet metal with rubber bung) to one end of the 4-in. (100-mm) diameter flexi-tube. Make an air-tight seal using one of the over lock straps and lever-locking cam provided as shown in Figure 4. Adjust the fit of the over lock strap with a screwdriver.



Figure 4. Flex Ductwork Connected to Primary Adapter Spigot. Bung not shown.

7. Securely attach the black primary duct adapter spigot/flexi-tube assembly to the opening on the ductwork to be pressure tested.
8. If the static pressure tap on the black Primary Duct Adapter is open to the duct, connect the 16-ft (5-m) long blue silicone tube to it as shown in Figure 5.

If the static pressure tap on the black Primary Duct Adapter is not open to the duct, drill a 4-mm hole in the duct and insert about 6 inches (10 mm) of the silicone tube into the duct. Seal around the hole with putty.



Figure 5. Connecting Pressure Tubing to Tap on Primary Duct Adapter. Bung not shown.

9. Connect the other end of the 4-in. (100-mm) flexi-tube to the cam lock connector (grey cast aluminum without nozzle). Make an airtight seal using the other over lock strap and lever-locking cam provided. Adjust the fit of the over lock strap with a screwdriver.
10. Determine if you are going to perform a high- or low-flow testing and positive or negative testing. Set-up the duct leakage tester by:

- a. For positive pressure, high-flow testing, remove the low flow nozzle if it is installed. Then, connect the grey cast-aluminum cam lock connector to the outlet side of the blower per Figure 6. Close both cam lock arms at the same time to ensure proper fit.

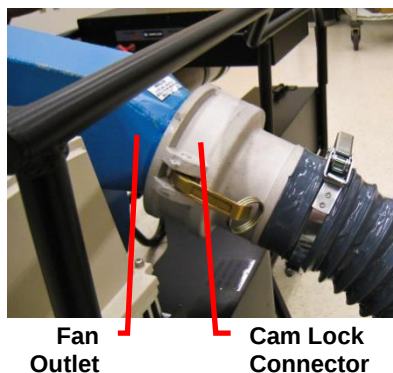


Figure 6. Positive Pressure, High-Flow Set-Up

Connect the free end of the 16-ft (5-m) silicone tube to the pressure tap marked **DUCT PRESSURE P3 (+)** on the black square box.

Finally, verify that the **FLOW GRID MODE** pressure taps on the inlet tubes are connected to the **FLOW GRID** pressure taps, i.e., **P1 (+)** to **P1 (+)** and **P2 (-)** to **P2 (-)**.

- b. For positive pressure, low-flow testing, add the low-flow nozzle to the blower inlet if it is not installed per Figure 7. Then, connect the grey cast-aluminum cam lock connector to the outlet side of the blower per Figure 6. Close both cam lock arms at the same time to ensure proper fit.

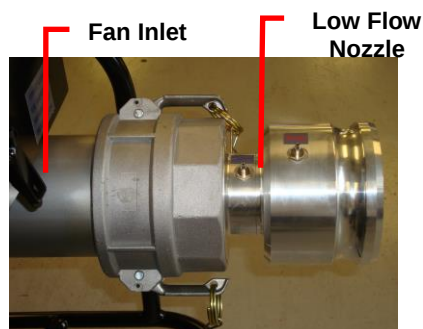


Figure 7. Positive Pressure, Low-Flow Set-Up

Connect the free end of the 16-ft (5-m) silicone tube to the pressure tap marked **DUCT PRESSURE P3 (+)** on the black square box.

- c. For negative pressure, high-flow testing, remove the low flow nozzle if it is installed. Then, connect the grey cast aluminum cam lock connector to the inlet side of the blower per Figure 8. Close both cam lock arms at the same time to ensure proper fit.

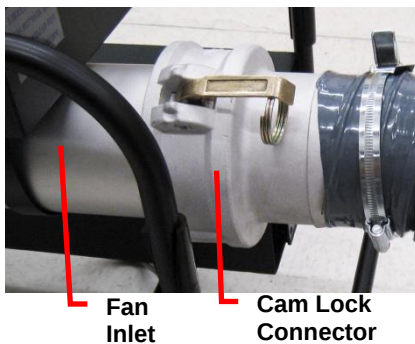


Figure 8. Negative Pressure, High-Flow Set-Up

Connect the free end of the 16-ft (5-m) silicone tube to pressure tap marked **DUCT PRESSURE P4 (-)** on the black square box.

Finally, verify that the **FLOW GRID MODE** pressure taps on the inlet tubes are connected to the **FLOW GRID** pressure taps, i.e., **P1 (+)** to **P1 (+)** and **P2 (-)** to **P2 (-)**.

- d. For negative pressure, low-flow testing, add the low-flow nozzle to the blower inlet if it is not installed. Then, connect the grey cast aluminum cam lock connector to the low-flow nozzle per Figure 9. Close both cam lock arms at the same time to ensure proper fit.

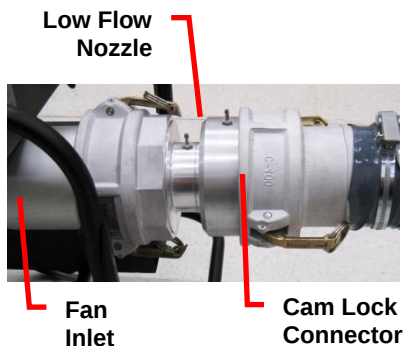


Figure 9. Negative Pressure, Low-Flow Set-Up

Connect the free end of the 16-ft (5-m) silicone tube to pressure tap marked **DUCT PRESSURE P4 (-)** on the black square box.

(This page intentionally left blank)

Chapter 3

Performing a Duct Leakage Test

The PAN300 duct leakage test system includes a Model PVM620 Micromanometer and a Model TA465-P Ventilation Meter. During duct leakage testing, the Model PVM620 Micromanometer measures the duct static pressure while the Model TA465-P Ventilation Meter measures the airflow rate.

Refer to the Operation and Service Manuals for the Model PVM620 Micromanometer and the Model TA465-P Ventilation Meter to use these instruments in other applications. If you do not have the manuals, download them from TSI® Incorporated's website www.tsi.com.

Measuring Duct Static Pressure

1. Turn ON the Model PVM620.
2. Zero the Model PVM620 pressure sensor with both ports open to the atmosphere.
3. Connect the (+) port on the Model PVM620 to **P3 (+)** to measure the duct static pressure (see Figure 6).
4. Leave the (-) port on the Model PVM620 open to the atmosphere.

NOTE

Refer to the Model PVM620 Operation and Service Manual for instructions on using data logging to automatically record the duct static pressure.

Measuring Duct Leakage Flow

1. Turn ON Model TA465-P.
2. Zero the Model TA465-P pressure sensor with both ports open to the atmosphere.
3. Connect the Model TA465-P to the PAN300 by connecting the (+) and (-) ports on the Model TA465-P to the **P1 (+)** and **P2 (+)** ports located inside the black box of the PAN300 as shown in Figure 10.

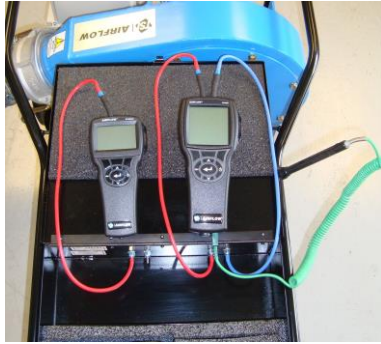


Figure 10. Connecting Instruments to PANDA Tester in High Flow Mode

4. Connect the thermocouple to the Model TA465-P.
5. Insert the thermocouple probe into the blower inlet through the hole marked **TC1** as shown in Figure 11.



Thermocouple
Hole

Figure 11. Thermocouple
Insertion Hole

Turning on the PAN300 Duct Leakage Tester

1. Switch the PANDA unit on.
 - a. For 230V models position the Mains Power switch of the inverter to the **ON** position to power the Inverter speed controller. The Fan motor is not energized.
 - b. 110V models **DO NOT** include a separate power switch. The PANDA unit is turned on when the power cord is plugged in.
2. Position the Fan Control switch to the **RUN** position to energize the fan.
3. Increase the fan to the desired speed by turning the Fan Speed Controller clockwise. To decrease the fan speed, turn the Fan Speed controller counter-clockwise.

Using Leakage Test Application in the Model TA465-P

CAUTION

The Model PVM620 and Model TA465-P meters must be zeroed before entering the Leakage Test Application.

1. Press the **MENU** key to access the menu system on the Model TA465-P.
2. Use the **▲▼** keys to highlight the Applications item.
3. Press the **← (ENTER)** key to access the Applications menu.

MENU
Zero Press
Display Setup
Settings
Flow Setup
Actual/Std Setup
Data Logging
Zero CO
Applications
Calibration
Discover Printer

4. Select **Leakage Test** and press **←** key.

APPLICATIONS
Draft Rate
Heatflow
Turbulence
% Outside Air
Leakage Test

5. Select either the **EN Standard** or **SMACNA** leakage test.

LEAKAGE TEST
EN Standard
SMACNA

Instrument Operation if EN Standard Test Protocol is Selected

1. Enter key parameters:
 - a. Surface Area of ductwork section to be tested.
 - b. Static Pressure of test, as measured by Model PVM620 micromanometer.
 - c. Flow Device as Nozzle or Flow Grid.
 - d. Leakage class as A, B, C, or D. Note that tests with negative pressures must be selected as negative tests, as indicated by -.
 - e. Test Length, or duration of leakage test, usually 5 minutes.
2. Increase the blower speed until the desired static pressure is achieved.
3. When the static pressure has stabilized, select **Run Test** and press **↵**.
4. The display will show the readings on the right. Leakage Factor and Leak Rate will update in real time, while other parameters will remain constant.

If the Leakage Factor and Leak Rate are sufficiently stable, press the **START** soft key or the **↵** key to begin the leak test. Pressing the **ESC** key will exit back to the previous screen.
5. After the leak test is complete, the Model TA465-P will prompt you to press the **SAVE** or **PRINT** soft key. You can also press the **ESC** key here to back out to the previous screen without saving the data.

LEAKAGE TEST

Surface Area
Static Pressure
Flow Device
Tightness Class
Test Length
Run Test

LEAKAGE TEST

Leakage Factor x.xx
Leak Limit x.xx
Leak Rate x.xx
Status OK
Flow Device Flow Grid
Baro Pressure 20.20
Temperature 20°C
Time 9:55
Standard TestXXX
Sample 0
(Sample Saved 1)

After completing leakage testing for a section of duct, you can move on to the next section.

Instrument Operation if SMACNA Test Protocol is Selected

1. Enter key parameters:
 - a. Surface Area of ductwork section to be tested.
 - b. Static Pressure of test, as measured by Model PVM620 micromanometer.
 - c. Flow Device as Nozzle or Flow Grid.
 - d. Leakage class as a number from 1 to 48. Typical values are 3, 6, 12, 24, or 48.
 - e. Test Length, or duration of leakage test.
2. Increase the blower speed until the desired static pressure is achieved.
3. When the static pressure has stabilized, select **Run Test** and press ←.
4. The display will show the readings on the right. Leakage

<u>LEAKAGE TEST</u>	
Surface Area	
Static Pressure	
Flow Device	
Leakage Class	
Test Length	
Run Test	

<u>LEAKAGE TEST</u>	
Leakage Factor	x.xx
Leak Limit	x.xx
Leak Rate	x.xx
Status	OK
Flow Device	Flow Grid
Baro Pressure	20.20
Temperature	20°C
Time	9:55
Standard	TestXXX
	Sample
	0
(Sample Saved 1)	
Stop(Save) Print	

Factor and Leak Rate will update in real time, while other parameters will remain constant.

If the Leak Factor and Leak Rate are sufficiently stable, press the **START** soft key or the ← key to begin the leak test. Pressing the **ESC** key will exit back to the previous screen.

5. After the leak test is complete, the Model TA465-P will prompt you to press the **SAVE** or **PRINT** soft key. You can also press the **ESC** key here to back out to the previous screen without saving the data.

After completing leakage testing for a section of duct, you can move on to the next section.

DANGER

Turn the isolation switch to the **OFF** position and wait 10 minutes prior to disconnecting power.

Troubleshooting Guide

Symptom	Recommended Action
Fan motor will not run.	• Check the power connection. • Circuit Breaker may have tripped.
Static pressure reading (on PVM620) is zero.	• Check the connections.
Static pressure reading (on PVM620) is too low. Required static pressure cannot be achieved with motor speed control settings at the maximum.	• Leakage rate is too high. Check for leaks using soap bubbles or smoke pallets. Alternatively, test a smaller section of the ductwork.
Leak Flow (on TA465-P) shows flashing XXX.XX.	• Check the pressure tube connections to the TA465-P meter. • Leak flow is too low. Use low flow nozzle adapter.

CAUTION

If recommended actions are used and the problem persists
DO NOT service further. Return to TSI® Incorporated for servicing.

Appendix A

Specifications

Pressure Measurement (PVM620)

Range.....	± 3,735 Pa (± 15 in. W.G.)
Resolution	0.1 Pa (0.001 in. W.G.)
Accuracy	1% of reading ± 1 Pa (± 0.005 in. W.G.)
Actual duct static range.....	± 2,500 Pa (± 10 in. W.G.) at Zero Flow

Volume Flow Measurement (TA465-P)

Wilson radial flow grid	High leakage range: 10 to 200 l/s (36 to 720 m ³ /hr, 21 to 424 cfm)
15 mm conical inlet	Low leakage range: 1 to 13 l/s
nozzle adapter	(3.6 to 46.9 m ³ /hr, 2 to 27.5 cfm)
Resolution	0.01 l/s (0.01 m ³ /hr, 0.01 cfm)
Accuracy	± 2.5% of reading ± 0.01 l/s (± 0.04 m ³ /hr, ± 0.02 cfm)

Temperature Measurement (TA465-P)

K Type thermocouple probe	To EN60584 (IEC 584)
---------------------------	----------------------

Barometric Pressure Measurement (TA465-P)

Range.....	690 to 1,241 hPa (517.5 to 930.87 mm Hg, 20.36 to 36.648 in. Hg)
Accuracy	± 2% of reading

Power Requirements

Model PAN331*	220 to 240 V, 1 Phase, 50/60 Hz, 10A
Model PAN331-110*	110 to 120 V, 1 Phase, 50/60 Hz, 16A
Model PAN311**	220 to 240 V, 1 Phase, 50/60 Hz, 10A
Model PAN311-110**	110 to 120 V, 1 Phase, 50/60 Hz, 16A

Weight	71 kg (157 lbs.)
--------------	------------------

Dimensions (L x W x H)	1,130 mm x 660 mm x 510 mm (44.5 in. x 26 in. x 20 in.)
-----------------------------	--


TA465-P and PVM620	See specification sheets for details on individual instruments
--------------------------	--

* Model: instruments included


** Model: instruments NOT included

(Specifications subject to change without notice.)

Panda Fan Performance Graph (metric units)

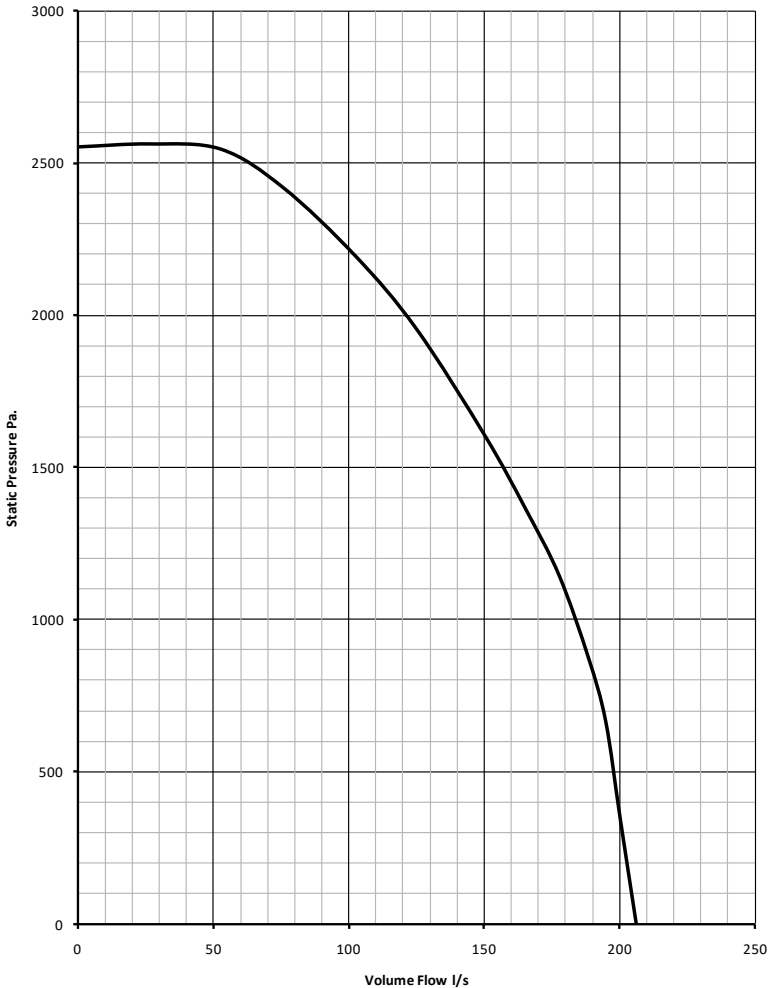

Panda Fan Performance Graph (imperial units)

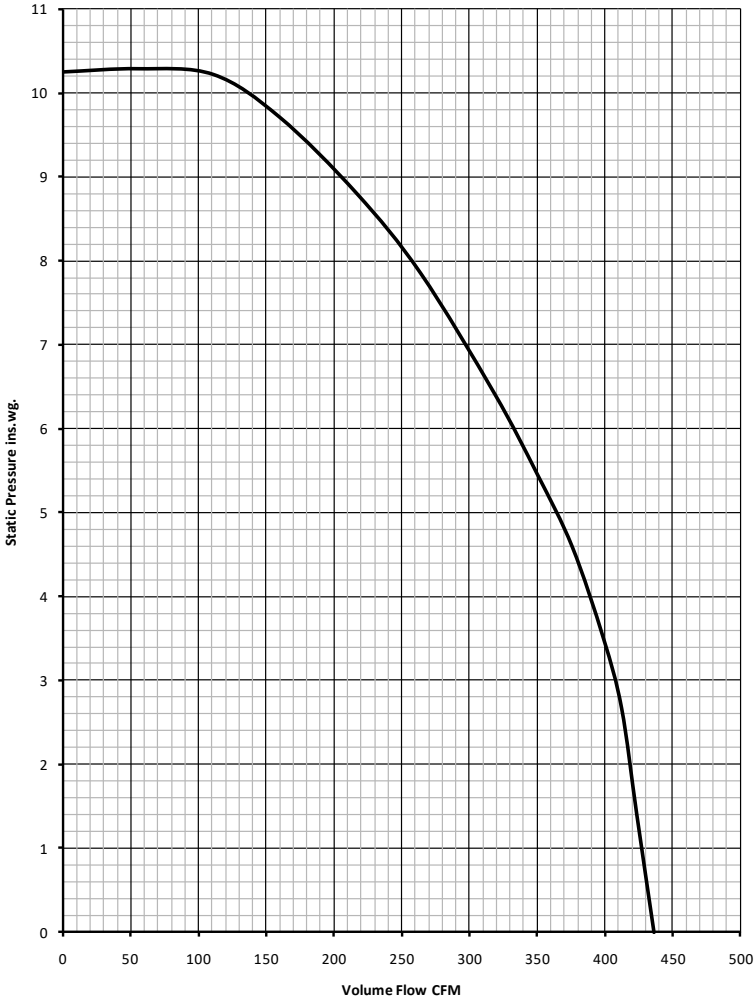

Environmental Requirements

Ambient Air Temperature	-10 to +40°C
Relative Humidity	0–95%, non-condensing
Altitude	2000m or less

Transportation and Storage

Storage Temperature	-10 to +40°C
---------------------------	--------------

**IMPORTANT—
Read Before Using the PANDA for the First Time**

It is **IMPORTANT** that the PANDA be connected to the power supply using a 30 mA residual-current device (RCD) or Ground Fault Circuit Interrupter (GFCI).

It is **IMPORTANT** that the 110V PANDA (yellow power socket) be connected only to 110V to 120V supplies. Connecting it to a higher voltage supply will permanently damage the inverter.

The 220V/240V PANDA (blue power socket) should only be connected to 200V to 240V power supplies.

Appendix B

Leakage Testing Standards Highlights

Different standards are used throughout the world to specify duct air tightness and leakage requirements. The PAN300 duct leakage test system has a duct leakage application to automatically compare the actual leakage flow with the maximum allowed leakage flow for EN and SMACNA standards. Field technicians can also use the duct leakage application to determine actual leakage flow and manually compare it to maximum leakage from another standard. The PAN300 duct leakage test system cannot determine the appropriate leakage classification for a given duct.

Standards Supported

Standard	US- or EU-Based	Description
BS EN 12237:2003	EU	Ventilation for buildings—Ductwork—Strength and leakage of circular sheet metal ducts.
BS EN 1507:2006	EU	Ventilation for buildings—Sheet metal air ducts with rectangular section—Requirements for strength and leakage.
DW/143	EU	HVAC—A practical guide to Ductwork leakage testing.
Eurovent 2/2	EU	Air leakage rate in sheet metal air distribution systems.
SMACNA HVAC Air Duct Leakage Test manual, First edition, 1985	US	Duct construction leakage classification, expected leakage rates for sealed and unsealed ductwork, duct leakage test procedures, recommendations on use of leakage testing, types of test apparatus and test setup and sample leakage analysis.

TSI® has made every effort to accurately reflect the standards referenced. Please refer to the actual standards for more detailed information and to make the best interpretation of each statement.

The scope of the standards listed above includes many items other than duct leakage. This summary, however, is limited to duct leakage testing.

EU Standards

Ductwork classification and maximum air leakage. Note that EN1507, EN12237 Eurovent 2/2 and DW/143 all have the same formula to determine $f_{\max}$, the Air Leakage Limit, although DW/143 uses units of l/s/m² whereas others use m³/s/m².

- EN 1507 (rectangular ductwork)

Air Tightness Class	Air Leakage Limit ($f_{\max}$) m ³ /s/m ²	Static Pressure Limit (p_s) Pa			
		Negative	Positive at pressure class		
			1	2	3
A	$\frac{0.027 * p_t^{0.65}}{1000}$	200	400		
B	$\frac{0.009 * p_t^{0.65}}{1000}$	500	400	1000	2000
C	$\frac{0.003 * p_t^{0.65}}{1000}$	750	400	1000	2000
D*	$\frac{0.001 * p_t^{0.65}}{1000}$	750	400	1000	2000

* Class D ductwork is only for special apparatus

- EN12237 (circular ductwork)

Air Tightness Class	Air leakage limit ($f_{\max}$) m ³ /s/m ²	Static Pressure Limit (p_s) Pa	
		Negative	Positive
A	$\frac{0.027 * p_t^{0.65}}{1000}$	500	500
B	$\frac{0.009 * p_t^{0.65}}{1000}$	750	1000
C	$\frac{0.003 * p_t^{0.65}}{1000}$	750	2000
D*	$\frac{0.001 * p_t^{0.65}}{1000}$	750	2000

* Class D ductwork is only for special apparatus

- Eurovent 2/2 Air Tightness For Installed Duct Testing:

Air Tightness Class	Air leakage limit ($f_{\max}$) $\text{m}^3/\text{s}/\text{m}^2$
A	$\frac{0.027 * p_t^{0.65}}{1000}$
B	$\frac{0.009 * p_t^{0.65}}{1000}$
C	$\frac{0.003 * p_t^{0.65}}{1000}$

- DW/143: A Practical Guide to Ductwork Leakage Testing

Duct Pressure Class	Static Pressure Limit		Maximum Air Velocity m/s	Air leakage limits $\text{l/s}/\text{m}^2$
	Positive Pa	Negative Pa		
Low-pressure – Class A	500	500	10	$0.027 * p_t^{0.65}$
Medium-pressure – Class B	1000	750	20	$0.009 * p_t^{0.65}$
High pressure – Class C	2000	750	40	$0.003 * p_t^{0.65}$

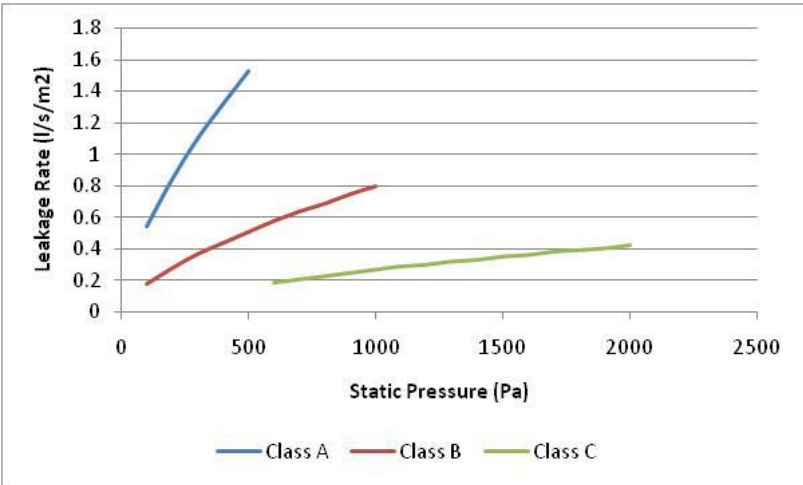


Figure 12. Allowable Air Leakage Rates from DW/143

- The measured leakage flow rates shall be corrected if the temperature and/or barometric pressure are different from standard conditions (+20°C and 101 325 Pa) as follows:

$$q_v = q_{measured} \cdot \frac{293}{273 + t} \cdot \frac{p}{101325}$$

where:

q_v =corrected flow leakage rate

$q_{measured}$ = measured flow leakage rate

t = measured temperature (°C)

p = measured barometric pressure (Pa)

- The test report shall give the following general information of the test performed:
 - Date and place
 - Test personnel and witness
 - Test equipment, including pressuring means and measuring instruments
 - Air temperature and barometric pressure during the test
 - Building and project reference
 - Design of installed ductwork including dimensions, thickness of materials, types of stiffening, length, type of duct/tubes and fittings, assembly method and distance of hangers/supports
 - Required air tightness class and design operating pressure of the installed ductwork
 - Installer of ductwork
 - Manufacturer of the ductwork
 - Measured values of:
 1. Ductwork surface area (A)
 2. Total joint length (L)
 3. Test pressure (p_{test})
 4. Leakage flow rate (q_v) corrected for temperature and barometric pressure
 5. Pressurizing time
 - Calculated values of
 1. Leakage factor (f)
 2. Air leakage limit (f_{max}) according to the formulas given in table above at the measured test pressure (p_{test})
 - Air tightness class achieved

- For tests including several test pressures it is recommended to plot the leakage factors as a function of test pressure in a diagram together with the air leakage limit curve.

US Standards

Ductwork classification and maximum air leakage

Duct Class	½-, 1-, 2-inwg	3-inwg	4-, 6-, 10-inwg
Seal Class	C	B	A
Sealing Applicable	Transverse Joints Only	Transverse Joints and Seams	Joints, Seams and All Wall Penetrations
Leakage Class			
Rectangular Metal	24	12	6
Round Metal	12	6	3

Maximum air leakage is then defined as

$$F = C_L P^{0.65}$$

where: F = Maximum air leakage (cfm/100 ft²)

C_L = Leakage class

P = Pressure (inwg)

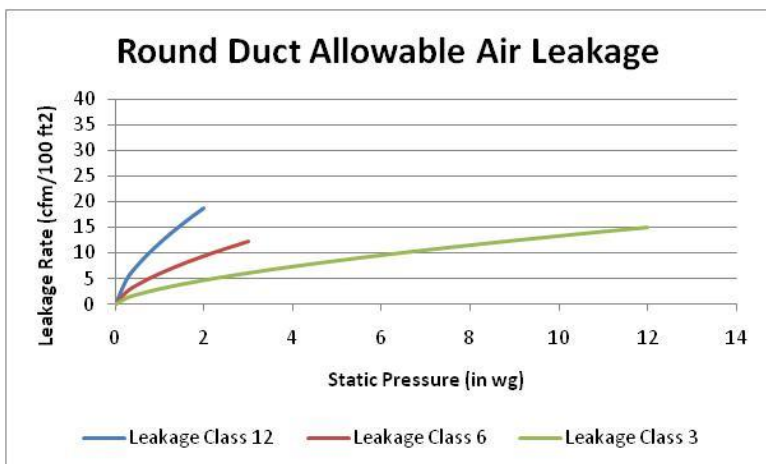


Figure 13. Allowable Air Duct Leakage from Round Ducts, per SMACNA Standard

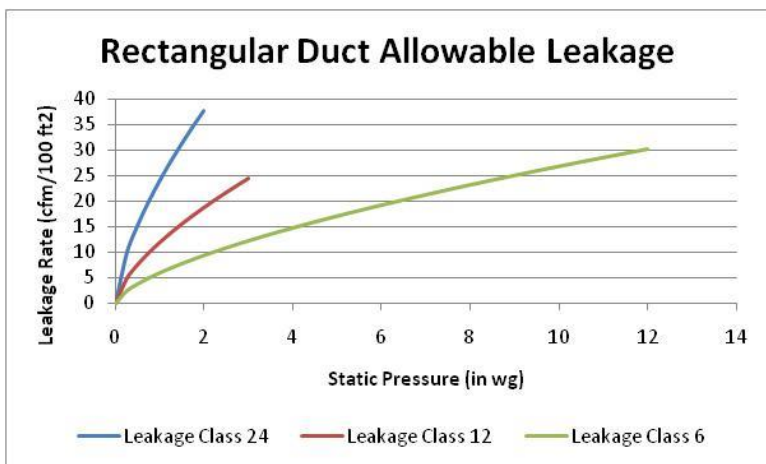


Figure 14. Allowable Air Duct Leakage from Rectangular Ducts, per SMACNA Standard

- The SMACNA standard does not generally require correcting leakage flow rates to standard conditions, unless:
 1. Air temperature <40°F or >100 °F
 2. Elevation <1500 ft above sea level
 3. Duct static pressure <-20 inwg or >+20 inwg


Should one of these conditions not be satisfied, then correcting the leakage to standard conditions may be done using one of these formulas:

1. $ACFM = SCFM * (460 + T) / 530$
where T = actual dry bulb air temperature (°F)
moisture is negligible
pressure between -20 and +20 inwg
 2. $ACFM = SCFM * 0.075 / d$
where d = air density from psychrometric chart
 3. $ACFM = \text{lb dry air/minute} * \text{humid volume (ft}^3/\text{lb dry air)}$
- The SMACNA standard does not specify the information to be reported, but instead defers to project documents. However, the SMACNA standard does include a sample test report that includes:
 - Test date and place
 - Test personnel and witness
 - Building and project reference
 - Duct section tested
 - Specified leakage class, test pressure and duct construction pressure class
 - Measurements of:
 - Ductwork surface area
 - Leakage flow and calculations required to determine leakage flow

(This page intentionally left blank)

Appendix C

Typical Setup

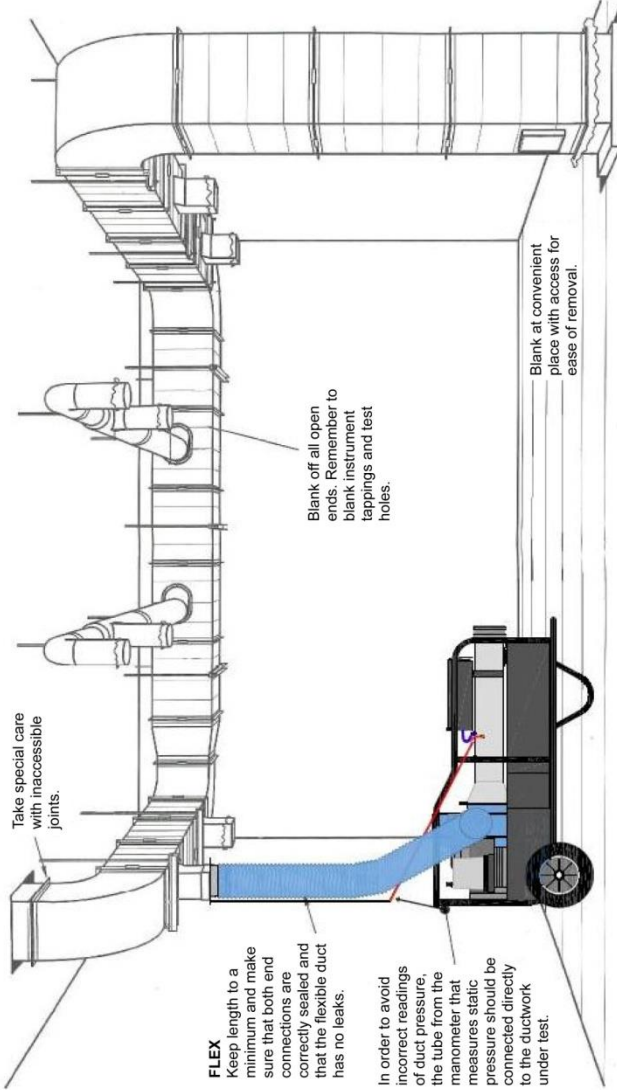

SEQUENCE OF TEST

1. Prepare test sheet.
2. Connect and adjust test rig to correct pressure.
3. Read off leakage rate.
4. Reseal if necessary (allow time to cure).
5. Maintain test for 15 minutes.
6. Switch off and allow to zero.
7. Reapply test pressure and check reading.
8. Record details on test sheet and obtain signature.

WARNING

Take care not to over pressurize system under test.

HOW TO FIND LEAKS

1. **Look** – at blanks, access openings and difficult joints.
2. **Listen** – with test rig running, leaks should be audible.
3. **Feel** – running your hand (particularly if wet) over joints can help locate leaks.
4. **Soap and Water** – paint over joints and look for bubbles.
5. **Smoke Pellet** – placed inside ductwork (obtain permission for use).

(This page intentionally left blank)

Appendix D


Procedure for Using Smoke Pellets in Leakage Testers

As shown in the sketch below, a rubber bung is fitted into the hole in the duct adapter which holds the wire coil.

When a smoke pellet is required to be used, remove the bung and fit a pellet into the wire coil as shown in the sketch.

Light the pellet and immediately plug into the hole in the duct adapter and proceed with the test.

The pellet should emit dense white smoke for up to a minute.

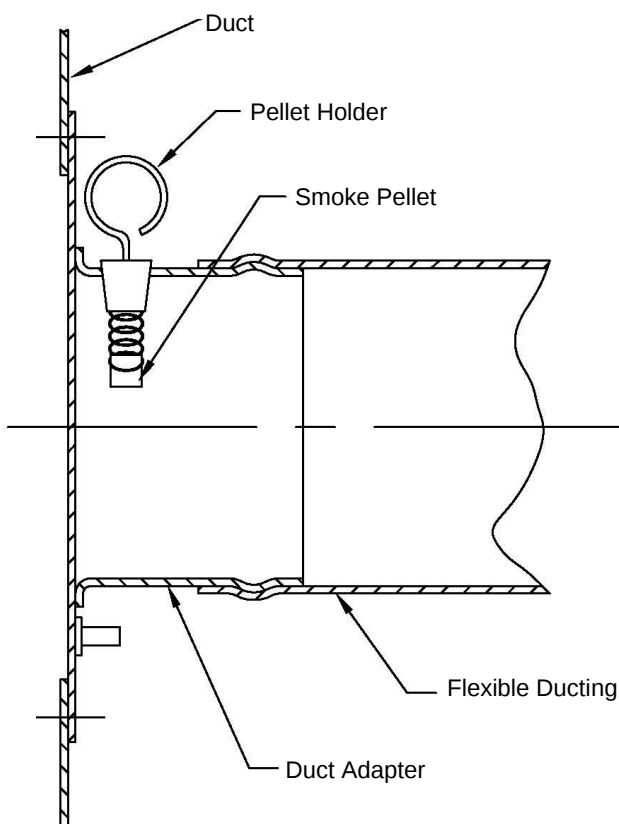

(This page intentionally left blank)



TSI Instruments Ltd.

Visit our website at www.tsi.com for more information.

UK **Tel:** +44 149 4 459200
France **Tel:** +33 1 41 19 21 99

Germany **Tel:** +49 241 523030

P/N 6005447 Rev B

©2021 TSI Incorporated

Printed in U.S.A.

