


Certifier® Air Velocity Calibrator

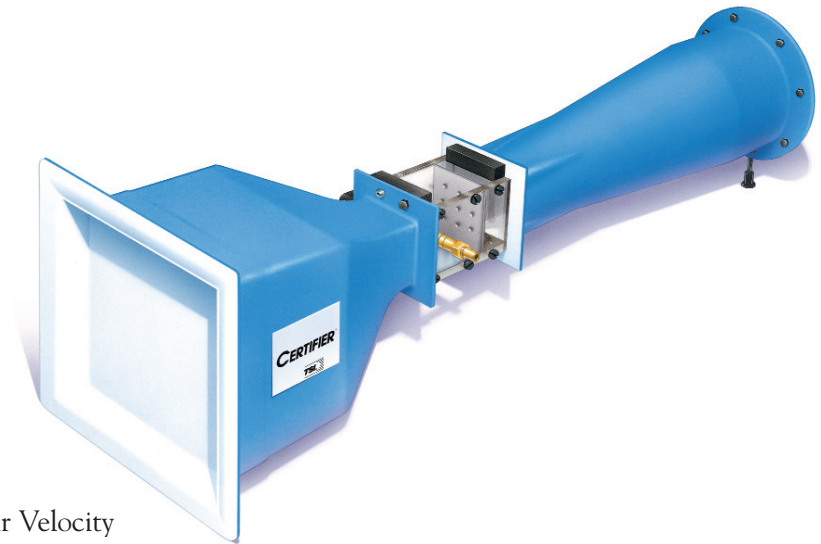

TSI's Model 8392 CERTIFIER® Air Velocity Calibrator gives you reliable and convenient in-house calibrations at a reasonable cost. You can have the confidence of high accuracies over a wide velocity range with the CERTIFIER. It enables you to calibrate your probed air velocity meters or transducers at velocities as low as 30 ft/min (0.15 m/s) and as high as 9000 ft/min (45 m/s) with typical accuracies of ± 1 percent of reading.

The CERTIFIER is ideal whenever frequent, accurate, air velocity calibrations are required. Having a CERTIFIER on site avoids the delays associated with sending the instrument to an outside calibration facility. Calibrations can be performed at your convenience as often as necessary.

The CERTIFIER comes with a TSI Model 8495 TRANSDUCER DISPLAY & MONITOR that will display actual air velocity. Entering a density correction factor automatically converts the velocity to standard conditions. This allows the user to read air velocity directly from the TRANSDUCER DISPLAY & MONITOR instead of reading pressure and then calculating velocity.

The Model 8392 CERTIFIER Air Velocity Calibrator provides a complete system to meet all of your calibration needs. Standard accessories furnished with the system include:

- Model 8495 TRANSDUCER DISPLAY & MONITOR
- MKS Pressure Transducer
- Fittings which accept 0.188 in. (4.8 mm) through 0.625 in. (15.9 mm) diameter probes (other sizes can be accommodated with the proper 1/2 NPT male compression fitting)
- Controller for setting fan speed
- Two nozzle plates for establishing low velocities



Specifications

Model 8392 CERTIFIER Air Velocity Calibrator

Test Section Dimensions: 4 in. × 4 in. (10.2 cm × 10.2 cm)
 Feedthrough Hole: 1/2" NPT
 Overall Dimensions: 57 in. L × 17 in. W × 17 in. H
 (145 cm × 43 cm × 43 cm)
 Weight: 30 lbs (14.6 kg)
 Power: 115 or 230 VAC
 (specify when ordering), 50/60 Hz

MKS Pressure Transducer

Range: 0 to 10 mmHg
 Accuracy: 0.15% of reading
 Power: 115/230 VAC, 50/60 Hz switch selectable

Specifications


Model 8495 Transducer Display & Monitor

Accuracy^(1&2) ±0.25% of reading, ±1 digit of resolution
 Time Constant 1 to 20 seconds in 1 second intervals
 Display 5 digit LED
 Input Power 11-30 VDC or 18-28 VAC, requires 500mA maximum

¹±.02% of reading/°C = .01% of reading /°F away from 25°C.
²±.025% of full scale= effect of EMI per IEC801-3.

Specifications subject to change without notice.
 Specifications in parentheses () indicate metric equivalents.

Nozzle Plate	Velocity Range		Accuracy	Pressure Drop (mmHg)	Typical Turbulence Intensity*
	(ft/min)	(m/s)			
None	1500-9000	7.5-45	1.0% of reading ±15 ft/min (±.075 m/s)	0.25-10.0	0.25%
No. 1	250-1500	1.25-7.5	2.0% of reading ±5 ft/min (±.025 m/s)	0.2-8.5	1.0%
No. 2	30-250	0.15-1.25	2.0% of reading ±2 ft/min (±.01 m/s)	0.11-8.5	1.0%

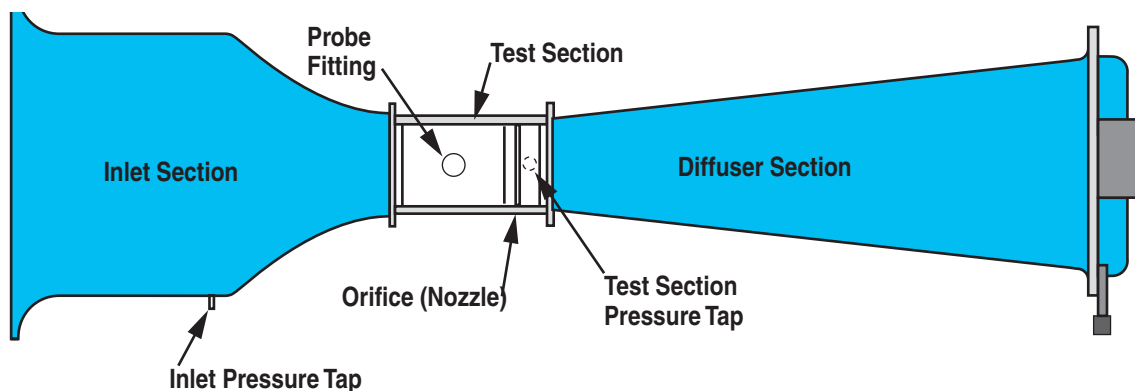

TSI

TSI Incorporated

United States: Tel: 651 490 2811 Toll Free: 1 800 874 2811 Fax: 651 490 3824 E-mail: answers@tsi.com
 Germany: Tel: +49-241 523030 Fax: +49-241 523 0349 E-mail: tsigmbh@tsi.com
 Sweden: Tel: +46-8-595-132 30 Fax: +46-8-595-132 39 E-mail: tsiab@tsi.com
 United Kingdom: Tel: +44-1275-847837 Fax: +44-1275-842437 E-mail: tsiuk@tsi.com

or visit www.tsi.com to find your closest TSI Representative or distributor.

For current information
www.tsi.com

