

nox medical

# noxturnal

MANUAL

English

## Noxturnal Manual

Version 4.1

Latest Revision: December 2020

Copyright © 2020

Nox Medical - All rights reserved

### **Manufactured by:**

Nox Medical ehf

Katrinartuni 2

IS - 105 Reykjavik

Iceland

Website: [www.noxmedical.com](http://www.noxmedical.com)

# nox medical

For distributor information go to:

[www.noxmedical.com](http://www.noxmedical.com)

# C€2797

### **Copyright Notice**

No part of this publication may be reproduced, transmitted, transcribed, stored in a retrieval system, or translated into any language or computer language, in any form, or by any means: electronic, mechanical, magnetic, optical, chemical, manual, or otherwise, without the prior written authorization from Nox Medical.

## Contents

|                                                                       |    |
|-----------------------------------------------------------------------|----|
| Introduction.....                                                     | 6  |
| Intended Use.....                                                     | 6  |
| Contraindications.....                                                | 6  |
| Scope .....                                                           | 6  |
| Warnings and Cautions for Use .....                                   | 6  |
| Noxturnal Description .....                                           | 8  |
| Noxturnal App Description .....                                       | 8  |
| Supported Devices.....                                                | 8  |
| Installing Noxturnal.....                                             | 8  |
| Noxturnal System Requirements.....                                    | 9  |
| Minimum System Requirements .....                                     | 9  |
| Installation Instructions .....                                       | 9  |
| Standard Operation .....                                              | 10 |
| Connecting a Nox Recording Device to Noxturnal.....                   | 11 |
| Upgrading the Recording Device Firmware.....                          | 11 |
| Starting a New Ambulatory Recording .....                             | 12 |
| Recording Types.....                                                  | 16 |
| Device Profiles .....                                                 | 20 |
| Downloading an Ambulatory Recording from a Nox Recording Device ..... | 24 |
| Setup of the Nox Sleep System for Online Recordings.....              | 25 |
| Online System Network Overview .....                                  | 25 |
| Online System Configuration .....                                     | 27 |
| Online Room .....                                                     | 27 |
| Configuration of New Sensors .....                                    | 31 |
| Device Profiles for Online Devices .....                              | 32 |
| Recording Types for Online Devices .....                              | 32 |
| Starting an Online Recording.....                                     | 32 |
| Nox C1 Configuration.....                                             | 35 |

|                                                         |    |
|---------------------------------------------------------|----|
| Nox C1 Access Point Network Configuration.....          | 35 |
| Upgrading Nox C1 Access Point firmware .....            | 36 |
| Activating Nox DC Channel License .....                 | 38 |
| Integration of Video Devices for Online Recordings..... | 39 |
| Setup an Online Room with a Video Device .....          | 39 |
| Video Codecs .....                                      | 39 |
| Video Camera Integration .....                          | 39 |
| Setup a Recording Type with a Video Device .....        | 42 |
| Working with recordings in Noxturnal .....              | 45 |
| Recording Results Page.....                             | 45 |
| Result Page Commands .....                              | 45 |
| Patient Information .....                               | 45 |
| Sleep Parameters.....                                   | 46 |
| Respiratory Indices .....                               | 46 |
| Overall Signal Quality and Single Body Source .....     | 47 |
| Signal Overview and Parameters.....                     | 47 |
| Signals and Events .....                                | 48 |
| Changing the Analysis Periods.....                      | 49 |
| Setting Units .....                                     | 50 |
| Viewing Signals .....                                   | 51 |
| Workspace Menu Button.....                              | 51 |
| Signal Sheets .....                                     | 52 |
| Working with Signals .....                              | 53 |
| Keyboard Navigation .....                               | 54 |
| Working with Events.....                                | 55 |
| Scoring an Event .....                                  | 55 |
| Single Click Scoring .....                              | 55 |
| Deleting an Event.....                                  | 56 |

|                                              |    |
|----------------------------------------------|----|
| Moving an Event .....                        | 56 |
| Resizing an Event .....                      | 56 |
| Navigating Events .....                      | 56 |
| Analysis Protocols .....                     | 57 |
| Working with Scorings .....                  | 58 |
| New Scoring .....                            | 59 |
| Select a Scoring .....                       | 60 |
| Save Scoring .....                           | 60 |
| Clear Scoring .....                          | 60 |
| Revert Scoring .....                         | 60 |
| Delete Selected Scoring .....                | 60 |
| Scoring Keyboard Shortcuts .....             | 60 |
| Noxturnal Reports .....                      | 60 |
| Generating Reports .....                     | 60 |
| Customizing Reports .....                    | 61 |
| Report Parts and Report Fields .....         | 63 |
| Create a New Report Parts .....              | 63 |
| Create a New Report Field .....              | 64 |
| Add Report Parts and Fields to Reports ..... | 65 |
| Report Header and Footer .....               | 65 |
| Exporting Reports .....                      | 67 |
| Printing Reports .....                       | 67 |
| The Recording Library .....                  | 67 |
| Archiving Recordings .....                   | 68 |
| Single Body Source .....                     | 68 |
| Compatible Devices .....                     | 70 |
| Switches, IP CAMERAS AND MICROPHONES .....   | 70 |
| Auxiliary devices supported .....            | 70 |

|                                                  |    |
|--------------------------------------------------|----|
| Regulatory Information .....                     | 71 |
| Performance Testing and Validation Summary ..... | 71 |
| Description of Symbols and Abbreviations.....    | 71 |
| About.....                                       | 73 |
| Appendix.....                                    | 74 |
| Default Derived Signals .....                    | 74 |
| Automatic Analysis Overview .....                | 76 |

## Introduction

Congratulations on choosing the Noxturnal® application software. The Noxturnal software is a modern sleep diagnostics software platform designed for ease of use and operation efficiency. The Noxturnal software is an essential part of the Nox Sleep Assessment Systems. Its main function is to work with physiological signals recorded/received using devices from Nox Medical (see Supported Devices chapter) and their linked devices and accessories. It takes the user through the workflow of configuring recordings, downloading data, analyzing and reporting.

## Intended Use

The Nox Sleep System is used as an aid in the diagnosis of different sleep disorders and for the assessment of sleep.

The Nox Sleep System is used to measure, record, display, organize, analyze, summarize, and retrieve physiological parameters during sleep and wake in patients greater than 2 years of age.

The Nox Sleep System allows the user to decide on the complexity of the study by varying the number and types of physiological signals measured.

The Nox Sleep System allows for generation of user/pre-defined reports based on subject's data.

The user of the Nox Sleep System are medical professionals who have received training in the areas of hospital/clinical procedures, physiological monitoring of human subjects, or sleep disorder investigation.

The intended environments are hospitals, institutions, sleep centers, sleep clinics, or other test environments, including patient's home.

## Contraindications

The Nox Sleep System does not provide any alarms and is not intended to be used for continuous monitoring where failure to operate can cause injuries or death of the patient.

## Scope

This manual covers the use of the Noxturnal software. The use of the Nox devices and their accessories that are needed for the recording of physiological signals are covered in:

- Nox A1 Manual
- Nox C1 Manual
- Nox T3 Manual
- Nox T3s Manual

This manual also includes a short introduction about the Noxturnal App and its features.

## Warnings and Cautions for Use

- ▶ **Warning:** The Nox Sleep Assessment Systems are **NOT CERTIFIED TO BE USED FOR CONTINUOUS MONITORING** where failure to operate can cause injuries or death of the patient.

- ▶ **Warning:** The Nox Sleep Assessment Systems are intended as an aid in diagnosis of sleep disorders. The systems must be used in conjunction with other methods of assessing clinical signs and symptoms.
- ▶ **Note:** Automatic analysis may be less accurate than analysis conducted by trained physician. The result of the automatic analysis/scoring must always be manually verified by the trained physician prior to diagnosis.
- ▶ **Warning:** Derived signals calculated by Noxturnal, especially heart rate and respiratory rate from the underlying electrocardiogram (ECG) and respiratory effort signals, are not validated for patients with diaphragm pacing/phrenic nerve stimulators.
- ▶ **Warning:** The pressure column in the Positive Airway Pressure (PAP) Overview section of the PAP report and the Polysomnography (PSG) PAP report represents the mask pressure of the corresponding device and NOT the Set Pressure of the device.
- ▶ **Caution:** U.S. federal law restricts this device to sale by, or on the order of, a physician.
- ▶ **Warning:** The Nox A1, T3 and T3s Recorders shall under no circumstances be connected to the USB port on the PC while applied to the patient. This could result in electroshock to the patient and serious harm.



- ▶ Please read this manual carefully before use, especially sections marked with an exclamation mark.

## Noxturnal Description

The Noxturnal software interacts with Nox Recording Devices and Nox Access Points. It allows the configuration of the devices as well as: displaying, navigating, organizing, analyzing, reporting, archiving and retrieving physiological signals recorded/received by use of the Nox devices. This section describes the main features of the application and installation instructions.

## Noxturnal App Description

The Noxturnal App is an Android application that is used as a mobile interface to Nox A1 Recorders and Nox C1 Access Points. The app allows the user to perform certain tasks already known in the Noxturnal software with more flexibility and proximity to the patient.

The App features include:

- Configure ambulatory recordings
- Connect to online rooms that have been configured in Noxturnal
- Review signal quality
- Perform impedance check
- Perform bio calibration
- Start and stop recordings
- View status of online recordings (Recording, Standby, Not Prepared)



### NOXTURNAL APP

Scan this QR code with your mobile device for easy access to the app. You can also search for "Noxturnal" in the Google Play Store.



To download the app, scan the QR code above or search for "Noxturnal" in the Google Play Store. The app runs on mobile devices running Android 4.3 or higher.

## Supported Devices

Noxturnal supports the following Nox devices and their linked devices and accessories:

- Nox A1 Recorder
- Nox C1 Access Point
- Nox T3 Recorder
- Nox T3s Recorder

In this manual, a Nox Recorder is used as a collective name for Nox A1, Nox T3 and Nox T3s recorder.

Throughout this manual, a Nox T3 recorder and Nox T3s recorder are collectively referred to as Nox T3 recorders.

## Installing Noxturnal

Before installing the Noxturnal software, review the system requirements for running the software application.

## Noxturnal System Requirements



- ▶ Note: The computer used must comply with the international standard IEC 60950-1 for the safety of information technology equipment.
- ▶ Note: It is recommended that a virus protection be installed on the computer running Noxturnal.

The following table shows the minimum hardware requirements needed to install and operate the software effectively.


### Minimum System Requirements

| Hardware Type         | Minimum Requirements   |
|-----------------------|------------------------|
| Operating System      | Windows 8              |
| Processor             | x64 based Intel or AMD |
| Processor Clock Speed | 1.7 GHz or faster      |
| Memory                | 2 GB or more           |
| Free Hard Drive Space | 4 GB or more           |
| Graphics Resolution   | 1024x768 or higher     |

For online system setup, the same minimum system requirements apply as listed above. It is highly recommended to use a separate computer for each online system. However, for expert users it is possible to run more than one system on a single computer.

### Installation Instructions


- Make sure to be logged onto the system with administrator privileges.
- Browse for a file on the installation CD called **Setup.exe** and run it.
- A wizard opens that guides the user through the installation. Follow the instructions to install the application. If upgrading from Noxturnal 5.x, an upgrade process runs in the background. Upgrading the user application settings. A copy of the settings prior to the upgrade is stored in "[My Documents]\NoxturnalUpgrade".

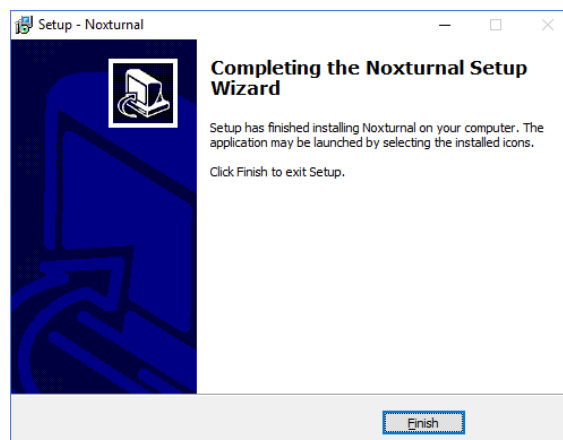

## Standard Operation

To run the Noxturnal application, double-click on the desktop icon or click on the application icon in the Windows start menu. To close the application either click on the **X** in the top right corner, or on the **File** menu choose **Exit**.

When Noxturnal starts up the workspace environment is displayed. If you have a device connected, you will see that in the picture, otherwise no device will be displayed. For the purposes of this document we have a Nox T3 Recorder connected as can be seen on the picture.

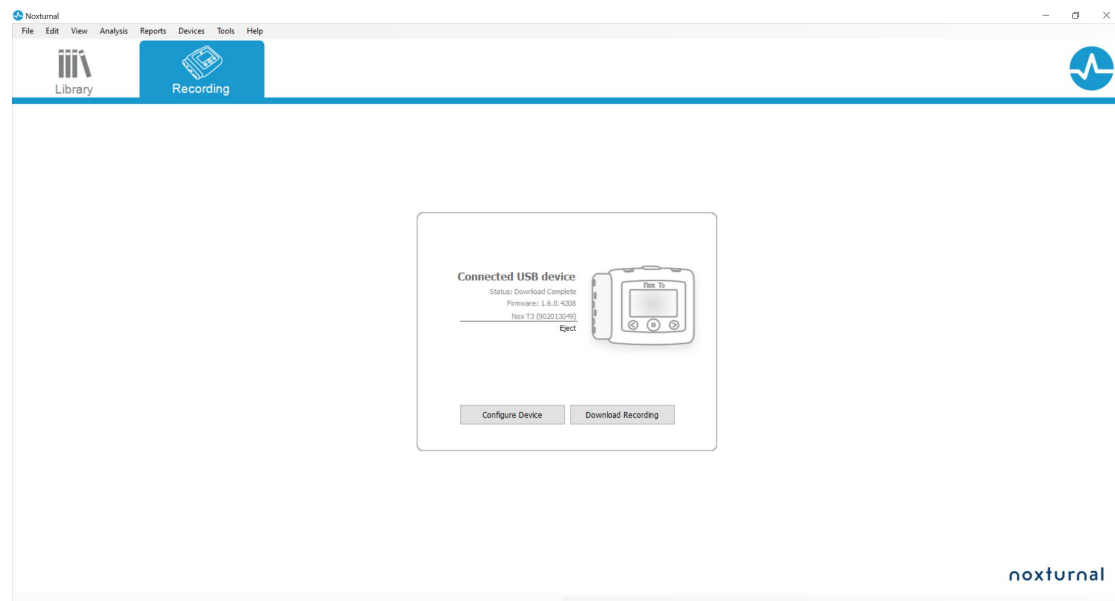

The **Recording** page is where the user works with Nox devices and the data recorded/received by use of those devices. This page guides the user through the most common tasks which are possible to perform in the application. These are:

- **Library:** In the top left corner, you will see this option. This option opens the recording library. The library stores a list of all recordings that have been recorded, downloaded or manually added to the recording library. For more information, refer to the section *The Recording Library*.
- **Configure Device:** To start a new ambulatory recording, select this option. A configuration wizard will guide the user through the configuration process. For more information, refer to the section *Starting a New Ambulatory Recording*.
- **Download Recording:** If a recording device is connected and it contains a recording, the user may download and review the recording. For more information, refer to the section *Downloading an Ambulatory Recording from a Nox Recording Device*.

To configure an online recording an online room needs to be pre-configured and it will appear in the Recording page and be selectable. For instruction on how to configure an online recording refer to the section *Setup of the Nox Sleep System for Online Recordings*.

## Connecting a Nox Recording Device to Noxturnal



- Note: Please note that although it is recommended to eject the recording device before unplugging it from the computer the device can be disconnected without ejecting.

Noxturnal is used to configure and download recorded data from Nox recording devices. To work with a recording device, start by connecting it with a USB cable to the computer. Noxturnal automatically detects the device and displays information about the device. Detection can take 2-4 seconds.

When Noxturnal detects the connected device the following information about the device is displayed: **recording status**, **firmware version** and **device name**.

The tasks performed on the recording device depend on the device status which can be the following:

- **Empty** – The device has not been configured and does not contain any recordings. Click **Configure Device** to configure the device for a new recording. Please note that configuring the device will remove any existing recordings from the device.
- **Ready to Record** – The device has been configured but does not contain any recordings. At this point the user can disconnect the device and initiate the recording process.
- **Ready to Download** – The device contains a recording that has not been downloaded to the computer. Click on the **Download Recording** button to download the recording to the computer.
- **Download Complete** – The device contains a recording that has already been downloaded and has been added to the recording library. At this point the user can either click on **Configure Device** to configure the device for another recording or click on **Download Recording** to download the recording again.


When you are done working with the device click on the **Eject** link and unplug the device from the computer.

## Upgrading the Recording Device Firmware



- Note: After clicking the upgrade firmware notification, you must disconnect the recording device from the computer and reconnect it again for a device firmware upgrade to take place.
- Note: It is always recommended to perform the device firmware upgrade to make sure the Nox recorder is running on the latest firmware version. New firmware versions can include important updates for the operation of the recorder.

If a new version of the device firmware is available for the connected device, Noxturnal will notify the user by displaying a balloon tooltip next to the device. This behavior is device independent and you will see the type of device on this page, depending on which device you have connected. In this picture, we have a Nox T3 Recorder connected.

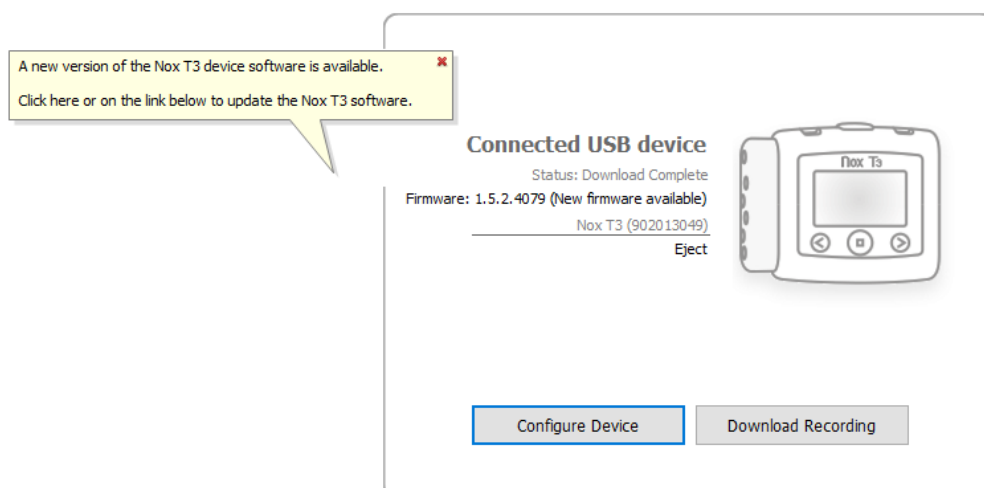

Choose either to ignore this message and continue working, or to upgrade the device firmware, which is always recommended. To upgrade click on the balloon and then follow the instructions presented.

### Starting a New Ambulatory Recording

To prepare a recording device for a new recording, start the Noxturnal application and connect the device to the computer using a USB cable. Noxturnal automatically detects the device and shows information about it on the **Recording** page. Click on the **Configure Device** button on the **Recording** page and a wizard opens which guides the user through the configuration process of the device.

The Configuration Wizard is device dependent. This means that the configuration wizard will vary depending on the type of Nox recording device being configured. However, the key steps are always the same:

1. **Configuration** of the device. Where you select the Recording Type to use (auxiliary devices that may be connected and channels to be recorded).
2. **Schedule Recording** where you can select the time and date for a recording to start or to have a patient start the recording themselves.
3. **Patient Information** where you add the necessary patient information to the recording.

This manual shows the configuration wizard for the Nox T3 Recorder. The first step is to define which Recording Type to use for the recording. The Recording Types have descriptive names to exhibit the recordings they are used for.

See the *Recording Types and Device Profiles* sections for more information on creating and editing recording types and device profiles.

Nox T3 Configuration

**Recording Type**

1 Recording Type 2 Schedule Recording 3 Patient Information

Recording Type:  
Nox BodySleep

Other Devices:

Nonin 3150 BLE Oximeter

BDA: [ : : : : : ]

Pair with Oximeter

Make sure the oximeter is turned on by pressing the button on top of the device.

[See channels:](#)

Next > Finish Cancel

If your Recording Type is set up to record data from an auxiliary Bluetooth device, e.g. pulse oximeter you will see that in the Configuration Wizard. To be able to use auxiliary Bluetooth device it needs to be paired to the Nox recording device. Enter the appropriate Bluetooth device Pin/BDA (Bluetooth Device Address) number in the relevant field in the Configuration Wizard.

For some devices, it is required to pair the device with the oximeter used. After entering the BDA address of the oximeter, click the **Pair with Oximeter** button and wait for the response. Note that the oximeter needs to be turned on by pressing the button of the oximeter when performing this step. Follow the instructions that appear on the screen.

Click **Next** to move on to step two where you schedule the recording time.

- If the **Manually Start Recording** option is checked, the user is responsible for starting/stopping the recording from the Nox recording device. This is done by pressing and holding the **Middle** button on the device until the device display indicates that the recording has started.
- Check the **Start Recording At:** option to schedule a specific recording time. The device will turn itself on and automatically start recording at the specified time. If the user chooses to record for more than one night, each recording will start at the same time each night.
- To stop recording after a specific duration, specify the **Duration** to be either: **7 Hours, 8 Hours, 10 Hours** or enter a customized duration. If **Unspecified** is chosen, then the user is responsible for stopping the recording. This is done by pressing and holding the **Middle** button on the device until the device display indicates that the recording has stopped.

Click **Next** to continue to the third step, the patient information dialog. In this dialog, it is possible to enter detailed information about the patient. The only required field is the patient name or the patient ID.

Nox T3 Configuration

**Patient Information**

1 2 3  
Recording Type Schedule Recording Patient Information

Name  
First: Last: ID:

Gender  
☐ Male  
☐ Female

Date of Birth  
☐ 1. 1.1960  
☒ N/A

Body Metrics  
Height: cm Weight: kg BMI:

Tags  
use ';' to separate multiple tags

Notes

Edit...


Enter Name or ID before Finishing

< Previous Finish Cancel

After having entered the patient information click **Finish** to write the configuration to the device.

If there is a recording on the device, the user will be asked if he wants to erase the recording from the device.

Finally, a confirmation page appears confirming the device has been configured. For Nox T3 Recorders the hookup instructions can be printed by clicking the **Print Hookup Instructions** button. A PDF document containing the hookup diagram is launched and can be printed. If no hookup instructions are available, this option is not displayed.

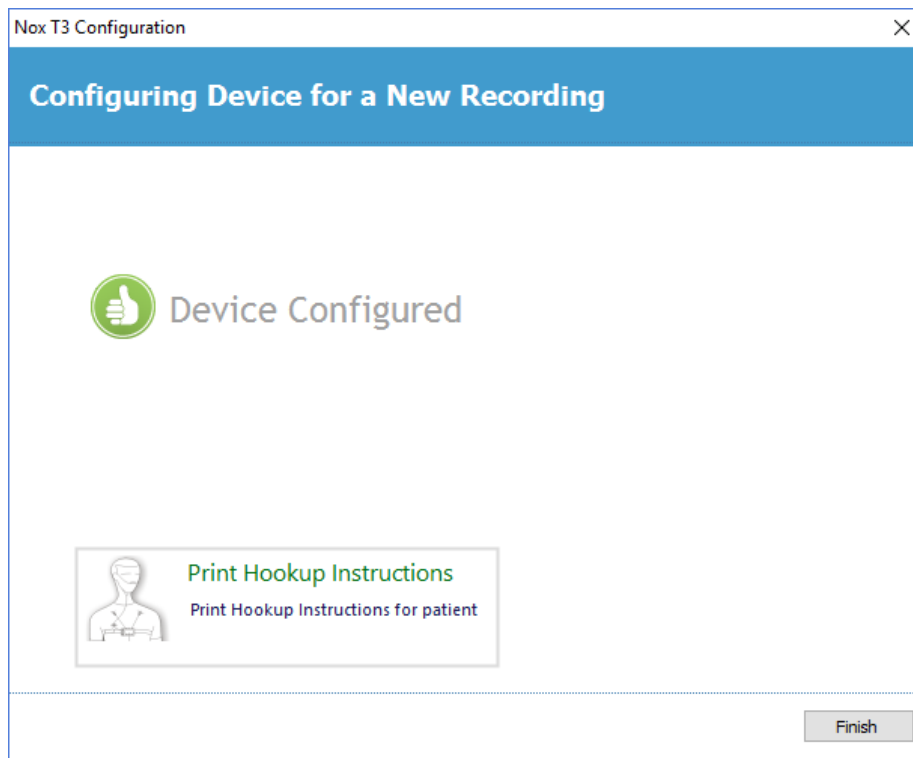


## Recording Types

Noxturnal offers a range of **Recording Types** available for configuration of both ambulatory and online recordings. The Recording Types encompass the device combination used for different types of sleep studies and the device settings. The Recording Types also define the automation for the different recordings, the relevant Workspace Layout, Analysis and Report that are used for the recording. In Noxturnal you can easily create your own Recording Types to control devices and settings used for recordings. Follow these steps in order to create your own Recording Type.


1. Select the Nox recording device you are creating the Recording Type for and if it is intended for ambulatory or online recordings
2. Set up the Recording Type to include Workspace Layout, Analysis, Report and devices and device profiles to be used, as applicable.

The Recording Type Wizard is device dependent. This means that the wizard will vary depending on the type of Nox recording device being configured. However, the key steps are always the same:

From the Noxturnal toolbar navigate to **Devices > Recording Types...**

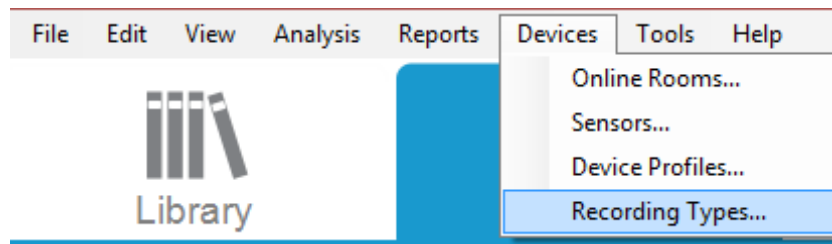


The Recording Types Wizard will open up.

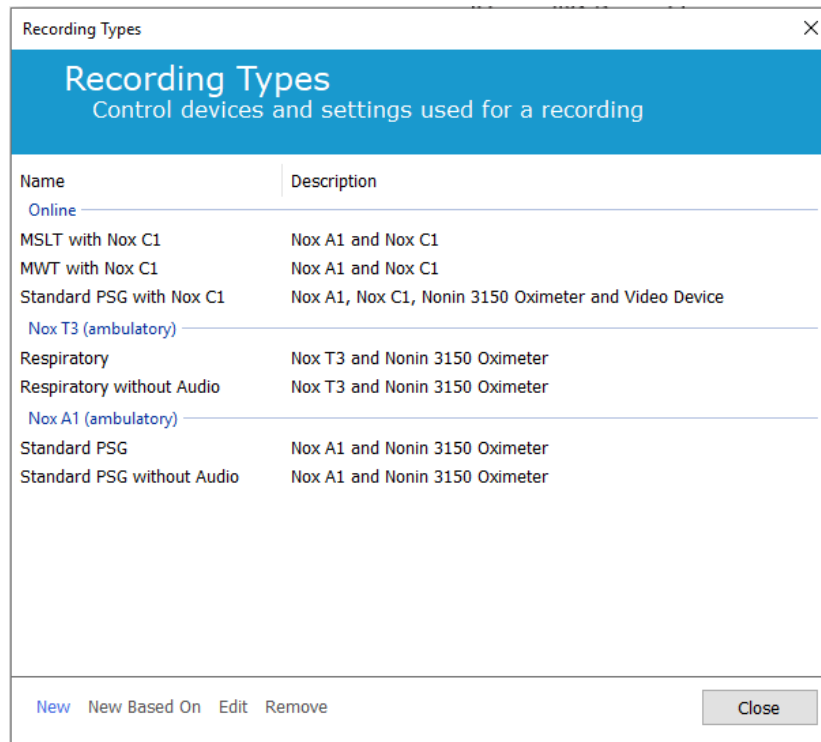


Here you can create a **New** Recording Type, a **New Based On** one of the available Recording Types and **Edit** or **Remove** custom Recording Types. For this example we will create a new Recording Type for the Nox T3 Recorder.


Select the **Nox T3 (ambulatory)** Recording Type from the dropdown list as shown below.

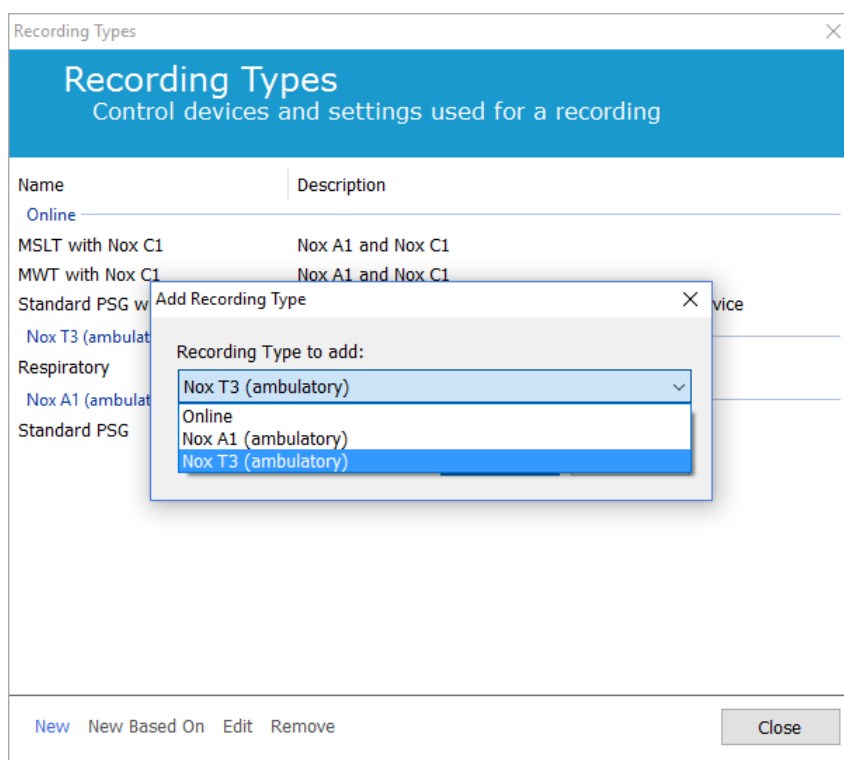

The next step is to set up the Recording Type as applicable. In the following wizard you can set up your Recording Type.

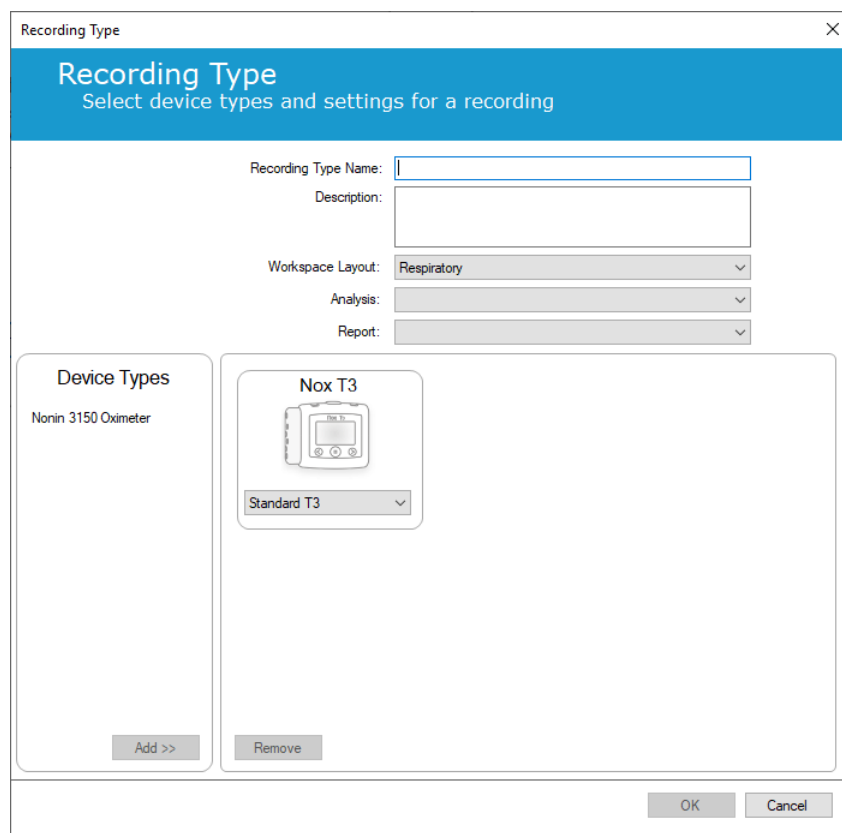


Type in the **Recording Type Name** and **Description** of the recording type. Choose the applicable **Workspace Layout**, **Analysis** and **Report**. You also have the availability to add auxilliary devices. Choose for example the Nonin 3150 (under Device Types) and click **Add>>**.

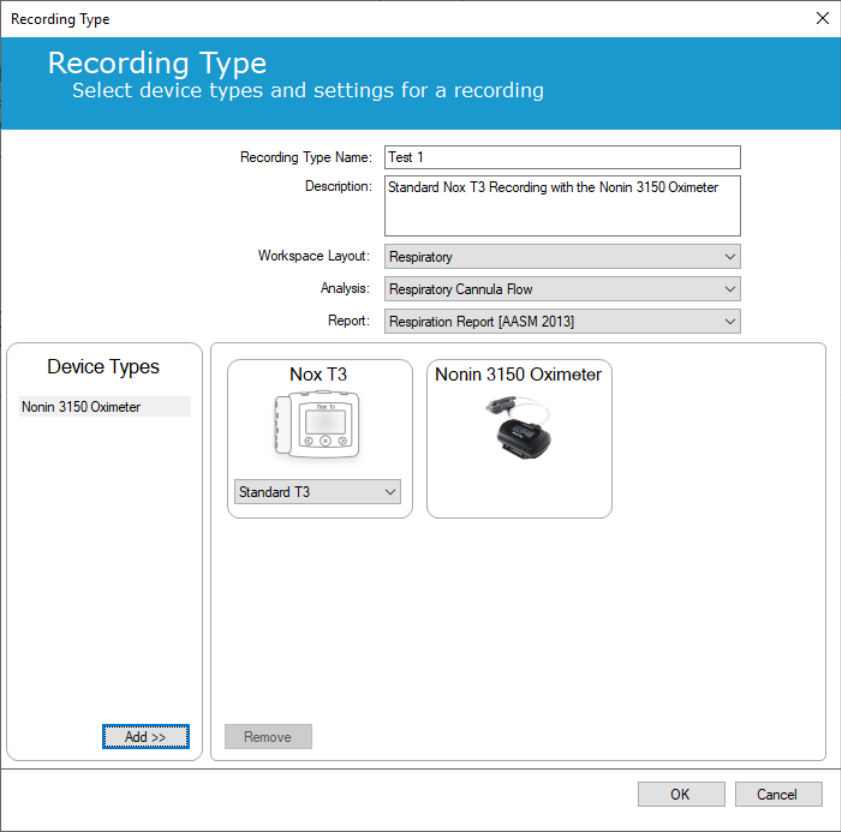

The image shows a software dialog box titled "Recording Type" with a close button (X) in the top right corner. The dialog has a blue header bar with the title and subtitle "Select device types and settings for a recording". Below the header, there are several input fields and dropdown menus. The "Recording Type Name" field contains "Test 1". The "Description" field contains "Standard Nox T3 Recording with the Nonin 3150 Oximeter". Below these are three dropdown menus: "Workspace Layout" set to "Respiratory", "Analysis" set to "Respiratory Cannula Flow", and "Report" set to "Respiration Report [AASM 2013]". At the bottom left, there is a "Device Types" section with a list containing "Nonin 3150 Oximeter" and an "Add >>" button. To the right of this list are two device cards: "Nox T3" with an icon of a device and a "Standard T3" dropdown, and "Nonin 3150 Oximeter" with an icon of a device. Below these cards is a "Remove" button. At the bottom right of the dialog are "OK" and "Cancel" buttons.

Note that it is also possible to choose the applicable Device Profile for this Recording Type directly in the Recording Type wizard, see below.

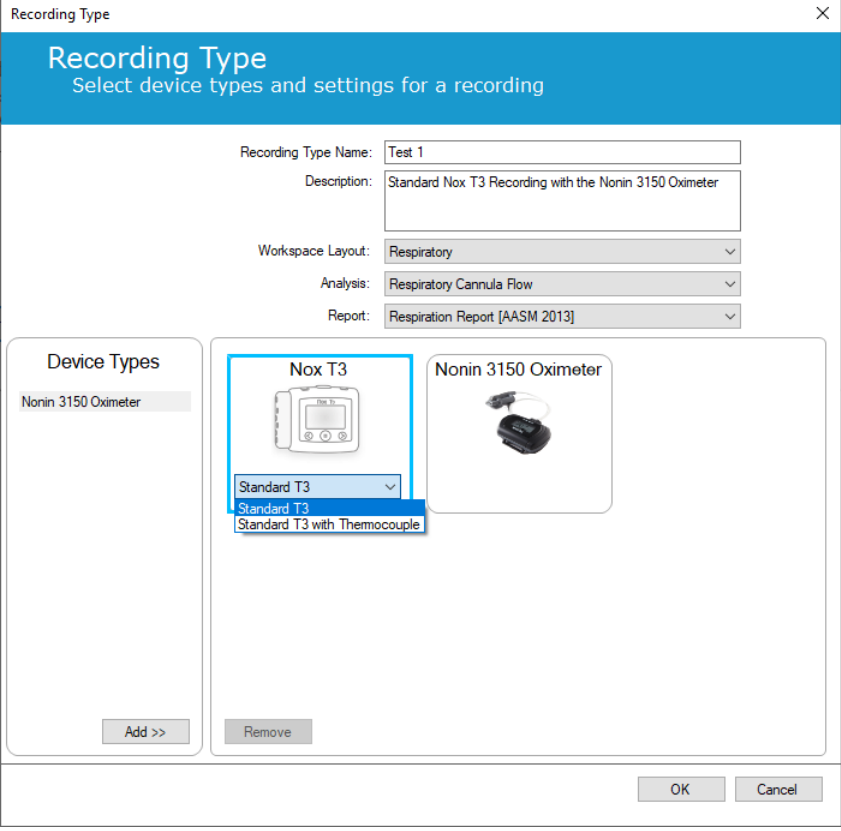

**Recording Type**  
Select device types and settings for a recording

Recording Type Name: Test 1  
Description: Standard Nox T3 Recording with the Nonin 3150 Oximeter

Workspace Layout: Respiratory  
Analysis: Respiratory Cannula Flow  
Report: Respiration Report [AASM 2013]

**Device Types**

Nonin 3150 Oximeter

**Nox T3**

Standard T3  
Standard T3  
Standard T3 with Thermocouple

Nonin 3150 Oximeter

Add >> Remove

OK Cancel

You can also create custom Device Profiles, please follow the instructions in the *Device Profiles* section for further instructions. Once you have created a new Device Profile it will appear in the dropdown list in the Recording Type wizard.

When you have set up your Recording Type click **OK** and your custom Recording Type will be available for configuration.


## Device Profiles




► Note: The Device Profiles wizards vary between Nox recording devices.

The Device Profiles are created for all standard recordings that you might perform with Nox devices. They allow for simple setup during the device configuration process.


From Noxturnal toolbar navigate to **Devices > Device Profiles...**

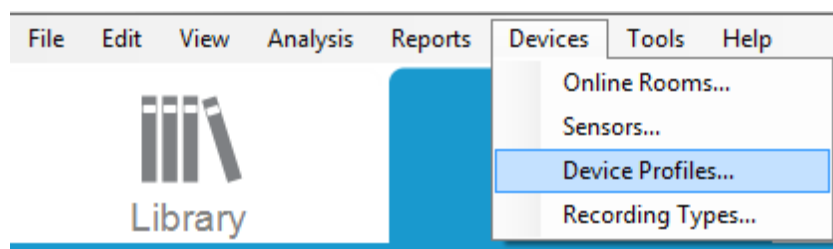


In the Device Profiles wizard, you can see list of the available Device Profiles for the Nox recording devices and the Nox access point.

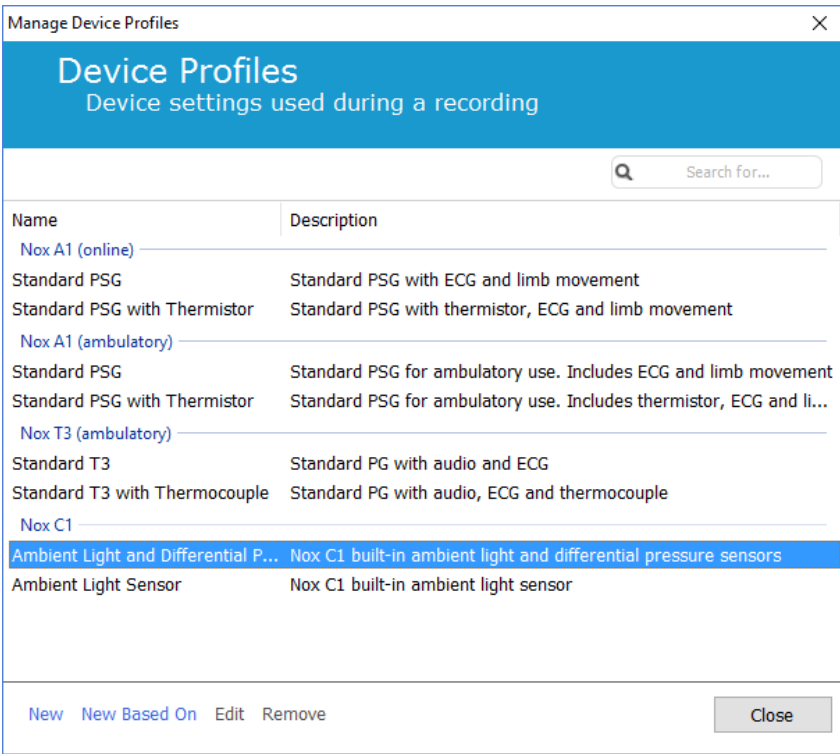

To create a custom device profile, select New or New Based On. You will then need to select for which recording device the template is for or from which of the current device profiles you wish to base your new template on. For this example, we will create a new device profile for the Nox T3 Recorder.

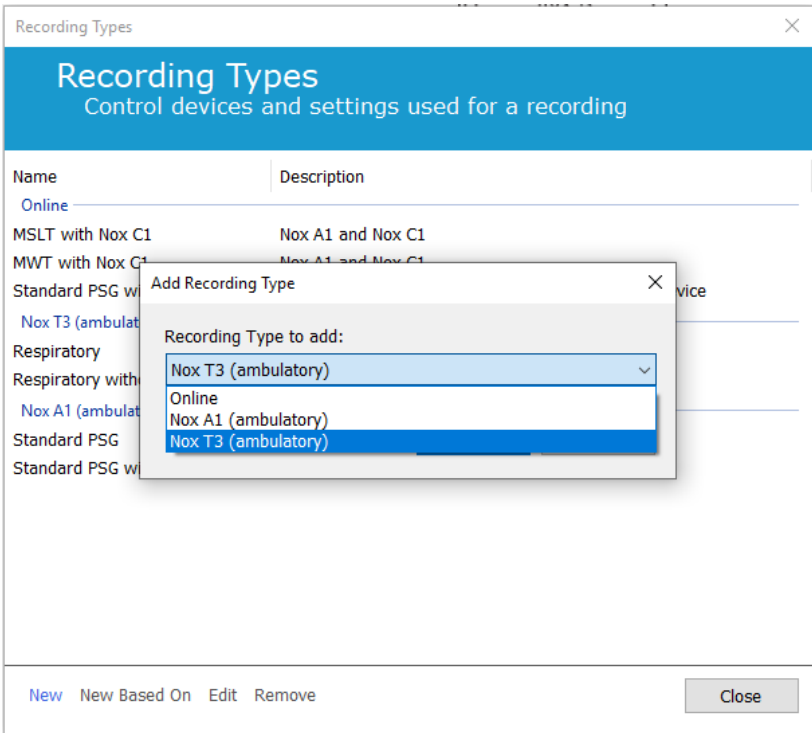

In the Profile Properties Wizard, you can setup the Device Profile. Type in the name (and description if you wish).

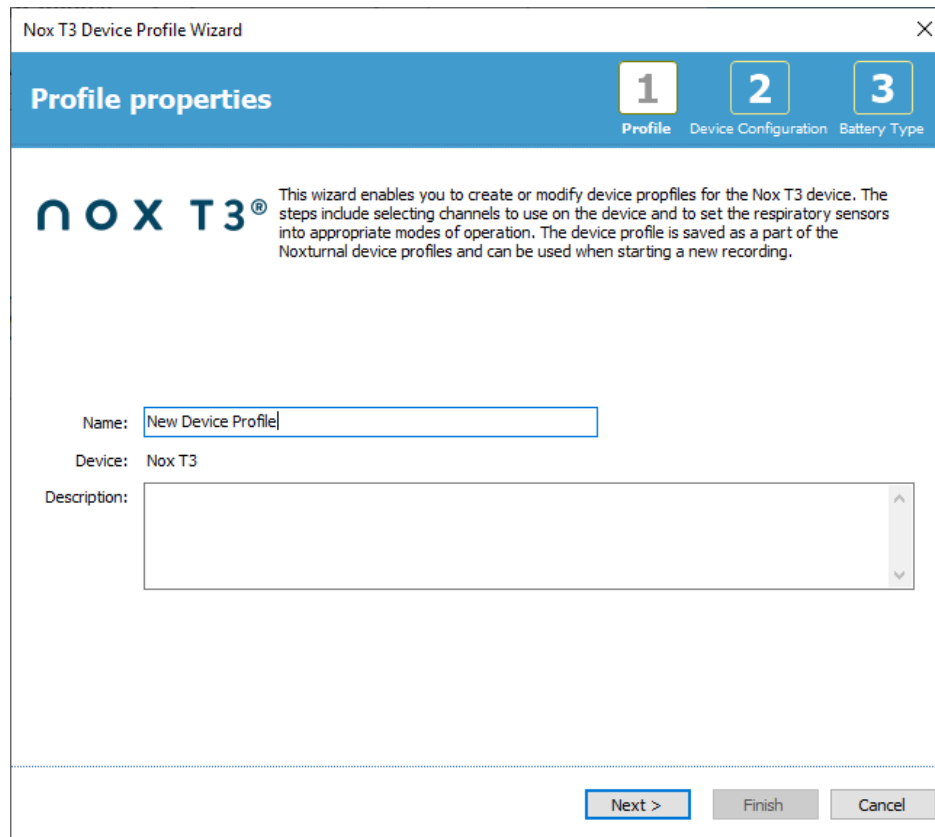

The image shows a screenshot of the 'Nox T3 Device Profile Wizard' window. The title bar reads 'Nox T3 Device Profile Wizard'. The window has a blue header bar with the text 'Profile properties' on the left. On the right of the header bar, there are three numbered steps: '1' (Profile), '2' (Device Configuration), and '3' (Battery Type). Below the header bar, the 'Nox T3' logo is on the left, and a paragraph of text explains the wizard's purpose: 'This wizard enables you to create or modify device profiles for the Nox T3 device. The steps include selecting channels to use on the device and to set the respiratory sensors into appropriate modes of operation. The device profile is saved as a part of the Noxturnal device profiles and can be used when starting a new recording.' Below this text, there are three input fields: 'Name:' with a text box containing 'New Device Profile', 'Device:' with a dropdown menu showing 'Nox T3', and 'Description:' with a large text area. At the bottom right, there are three buttons: 'Next >', 'Finish', and 'Cancel'.


Click **Next** to proceed to the next step.

In the dialog below you can setup the channel configuration for the device. The Configure Device dialog is device dependent. This means that the wizard will vary depending on the type of Nox device being used. When you have setup the channel configuration, click **Next**.

Nox T3 Device Profile Wizard

**Configure Device**

1 Profile 2 **Device Configuration** 3 Battery Type

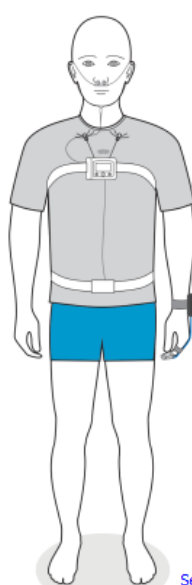

Audio Recording  
☒ Enable Audio Playback

Pressure  
☐ Not Used  
☒ Nasal Flow  
☐ Mask Pressure  
☐ Nasal Flow and Mask Pressure

General purpose channels  
☐ Channel 1: Abdomen Piezo  
☐ Channel 2: Abdomen Piezo

[See channels:](#)

< Previous Next > Finish Cancel

The final step for configuring a Nox recording device is to define the battery type used. Select the applicable battery type and click **Finish**.

Nox T3 Device Profile Wizard

**Battery Type Selection**

1 Profile 2 Device Configuration 3 **Battery Type**

Select battery type that will be used in the recorder:

☐ Alkaline Battery  
☐ Lithium Battery  
☐ Rechargeable Ni-MH Battery

 Please note that it's recommended to use new or fully charged batteries for each new recording. When recording multiple nights the patient might be required to change the battery after each night.

< Previous Finish Cancel

The Device Profile you created will be available from the list of Device Profiles and available for configuration.

### Downloading an Ambulatory Recording from a Nox Recording Device




- ▶ Note: If a download partially fails for any reason, it can lead to inconclusive recording results. The user will be warned when this happens and needs to decide whether the recorded data is complete or not. It is possible to download the data from the device again.
- ▶ Note: The downloaded recording is not deleted from the device until the device is configured for another recording.

To download recorded data from a Nox recording device to the computer, ensure that Noxturnal is running and then connect a device to a USB port on the computer.

Noxturnal automatically detects the device and shows information about it on the **Recording Page**. Detection can take 2-4 seconds.

Click on the **Download Recording** button on the **Recording Page** and Noxturnal will start downloading the recording from the device to the computer. A download progress dialog will appear that displays the steps involved while downloading. The data is first downloaded then the default analysis protocol is run and, if the device was configured to record audio, the audio download starts. It is possible to start working with the data at any time while it is being downloaded by clicking on the **Start Working** link.

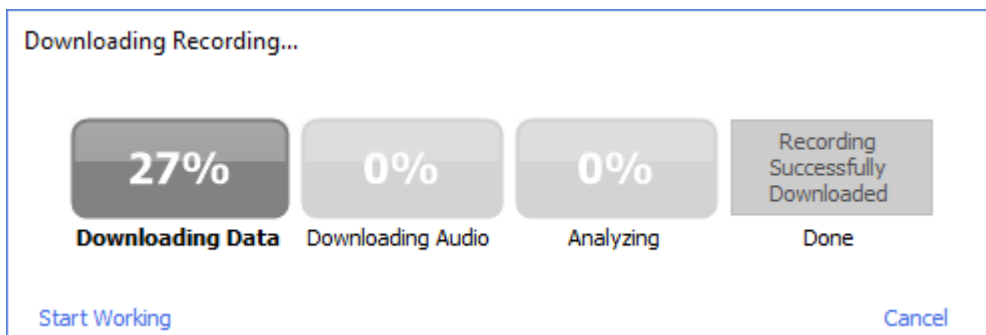

After the download is completed the user is notified and can start working with the whole recording.

Recordings are always downloaded to the default data storage location. It is possible to change the default data storage location on the automation tab in the tools options dialog (**Tools** → **Settings...** → **General**). Downloaded recordings are automatically added to the recording library and can be reviewed any time by going to the recording library and opening it. For more information, refer to section *The Recording Library*.

## Setup of the Nox Sleep System for Online Recordings

### Online System Network Overview

To ensure steady operation of the online functionality for the Nox Sleep System please follow the recommended system setup below.

- It is recommended to use a separate computer for each online system setup. However, it is possible to run more than one online system on a single computer; refer to *Minimum System Requirements* section for details.
- Use a separate local area network (LAN) for each Nox C1 Access Point and a computer running the Noxturnal software.
- Use a separate Nox C1 Access Point for each Nox A1 Recorder to be used.

The table below describes the setup of the control room where the computer with Noxturnal installed is located.


| Control Room |                                                                               |
|--------------|-------------------------------------------------------------------------------|
| Item         | Connection                                                                    |
| PC           | Connected to the same network as the Nox C1 Access Point with a network cable |
| Noxturnal    | Installed on PC                                                               |

The table below describes the setup of the patient room where the patient is sleeping during a sleep study.

| Patient Room                           |                                                                                                                 |                                                                                                                                                                                                                                                                                                                                                                                                                |                                                                                                 |
|----------------------------------------|-----------------------------------------------------------------------------------------------------------------|----------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------|-------------------------------------------------------------------------------------------------|
| Item Name                              | Description                                                                                                     | Function                                                                                                                                                                                                                                                                                                                                                                                                       | Setup/Connection                                                                                |
| Nox C1 Access Point                    | Bluetooth access point with analog and serial inputs and built in light sensor and differential pressure sensor | <ul style="list-style-type: none"> <li>▶ Data transfer received from Nox A1 over Bluetooth connection and forwarded to Noxturnal via Ethernet</li> <li>▶ Commands received from Noxturnal via Ethernet and forwarded to Nox A1 using Bluetooth connection</li> <li>▶ Data transfer received from auxiliary devices connected to analog and/or serial inputs and forwarded to Noxturnal via Ethernet</li> </ul> | Located in the patient room. Connected to the same LAN as the PC running the Noxturnal software |
| Nox A1 Recorder and applicable sensors | Recording device that may be configured for different types of sleep studies                                    | Records physiological signals from built-in and attached sensors                                                                                                                                                                                                                                                                                                                                               | Attached to the patient in the patient room                                                     |

|                           |                                                                                                                                                                                         |                                                                                                                                                             |                                                                                                                                                  |
|---------------------------|-----------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------|-------------------------------------------------------------------------------------------------------------------------------------------------------------|--------------------------------------------------------------------------------------------------------------------------------------------------|
| Medical auxiliary devices | Any medical device that fits the input channel specifications of the Nox C1 Access Point. Medical devices supported by the system to be connected to Nox A1 Recorder via Bluetooth link | Depends on the auxiliary device being used                                                                                                                  | The applicable connection cable connected to the analog input/serial input on the Nox C1 access point. Via Bluetooth link to the Nox A1 Recorder |
| Noxturnal App             | Android App                                                                                                                                                                             | Can be used to connect to Online Rooms, review signal traces and perform bio calibration and impedance check. Can also be used to start and stop recordings | Set the App to Online Mode and connect to the applicable online room                                                                             |

Figure below shows the overview of the online setup for the Nox Sleep System.

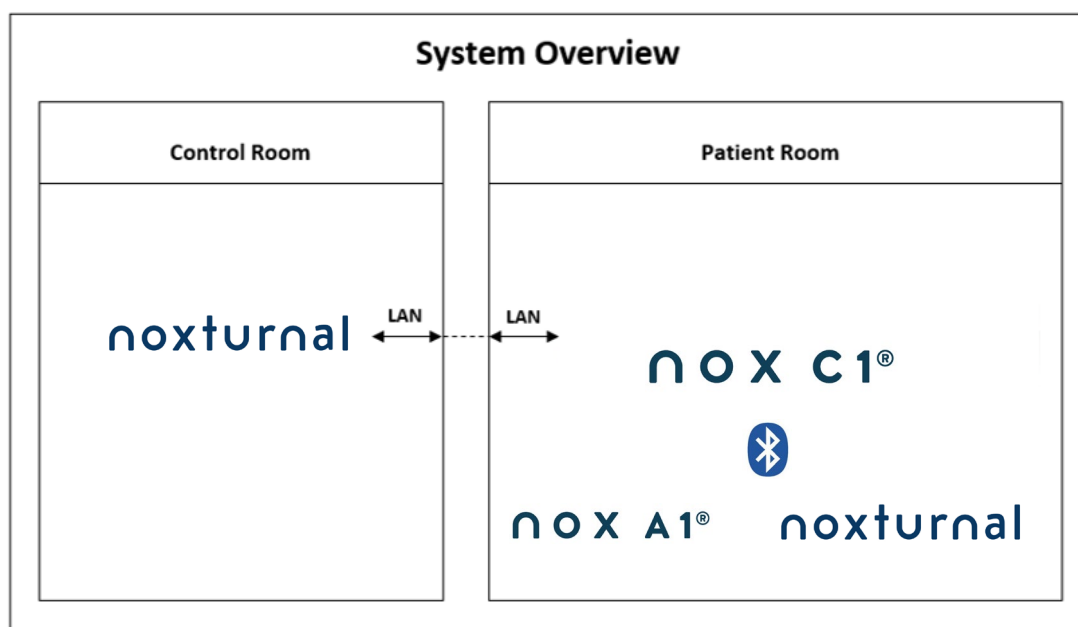

The Nox C1 Access Point is operated by the Noxturnal software.

For further instructions on the Nox C1 Access Point and the Nox A1 Recorder refer to the Nox C1 Manual and the Nox A1 Manual.

Refer to the "Compatible Devices" section regarding the types of Ethernet supported devices and switches that have been validated with the Nox Sleep System.

## Online System Configuration



- Note: To perform online recording with the Nox A1 Recorder you will need a Noxturnal A1 Online Acquisition License to be active on your computer and a Nox C1 Access Point. For further information, please consult with Nox Medical or their sales representatives.

This chapter describes how to setup the Nox Sleep System for online configuration. First make sure that you have setup all the devices and accessories needed, such as the Nox C1 Access Point, Ethernet cables and switch. Detailed information on how to setup your network, including the Nox C1 Access Point, is found in the Nox C1 Manual.

To set up the Nox Sleep System for online configuration you must perform the following steps in Noxturnal, as applicable:

1. Set up **Online Rooms**
2. Configure new **Sensors**
3. Set up **Device Profiles**
4. Set up **Recording Types**


These steps are outlined below. Following these steps will allow you to start your online recording and then start working with the signals in Noxturnal.

### Online Room


---

Setting up an Online Room is part of setting up Noxturnal for online recordings. The Online Room encompasses collection of devices which you normally keep together in a room. These may, for example, be all the devices that you keep in a particular hospital room dedicated for sleep studies.


To add a new room, select **Devices > Online Rooms...** from the Noxturnal toolbar. This will bring up the **Rooms** dialog.

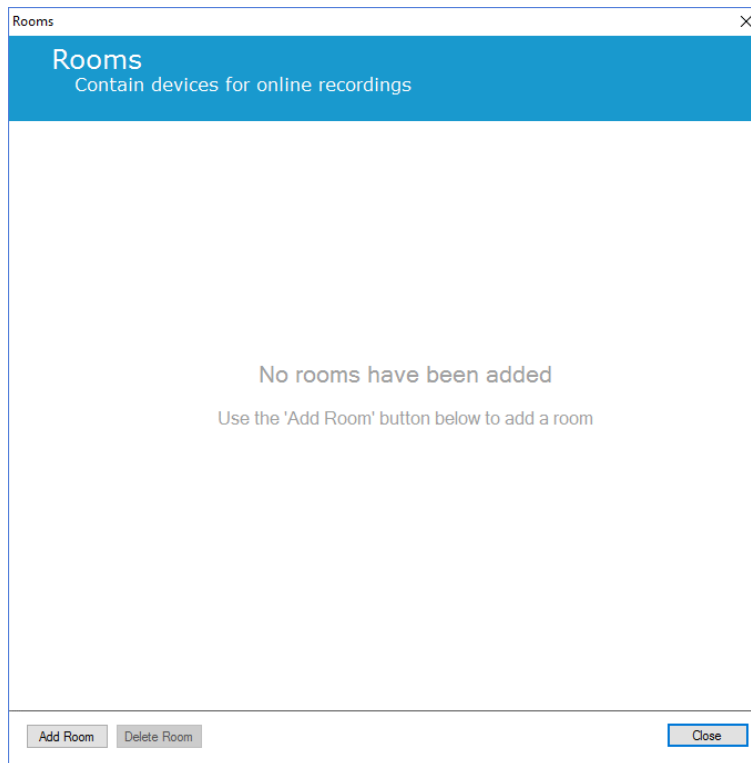

From here you can add a new room or edit an existing one. To add a new room click **Add Room** and in the dialog below you can give the new room a name, by clicking the pencil icon and add devices to your room by clicking **Add Devices**.

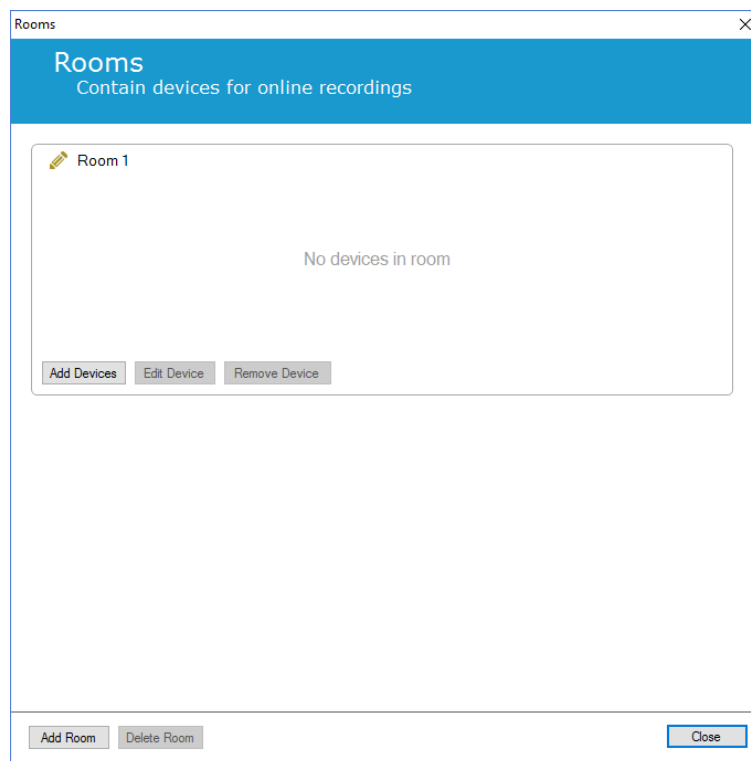

In the **Add Devices** Wizard you can add devices to your room. To add a device, select the applicable device from the **Device Types** list and click **Add >>** or double-click the device from the list. You can scan for connected IP devices on your network by clicking **Scan for IP Devices**.

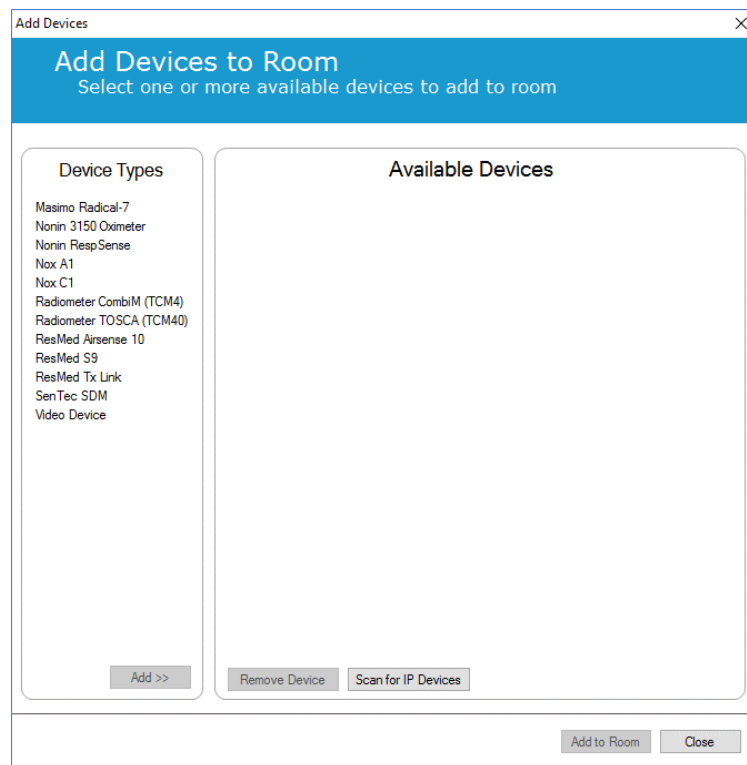

When you add a Nox A1 Recorder you will need to select the applicable Nox C1 Access Point being used in the room and click **Scan** for your Nox A1 Recorder or manually type in the A1 serial number. Remember to have your A1 Recorder turned on for this step. Select your recorder from the list and click **Next**.

Device Properties

12

Select deviceDevice Settings

Nox A1



Enter the 9 digit serial number (found on the A1 device label) or scan for it via Access Point

SNIxxxxxxxxxxId:

GTIN(01): 1569431111XXXX  
PROD DATE(11):YYMMDD  
SERIAL(21):9xxxxxxxxx



☒ Via Serial Number:

☐ Via Access Point:

Nox C1 - 109

Scan

| Device Type | Device Name | Serial Number | BDA |
|-------------|-------------|---------------|-----|
|-------------|-------------|---------------|-----|

Next >

Finish

Cancel

When you have added a selection of devices to collection of available devices you can select the devices to add to your Online Room.

## Add Devices to Room

Select one or more available devices to add to room

### Device Types

- Maximo Radical-7
- Nonin 3150 Oximeter
- Nonin RespSense
- Nox A1
- Nox C1
- Radiometer Combim (TCM4)
- Radiometer TOSCA (TCM40)
- ResMed Airsense 10
- ResMed S3
- ResMed Tx Link
- SenTec SDM
- Video Device

### Available Devices

|                                                                                                                                         |                                                                                                                                                                               |                                                                                                                                              |
|-----------------------------------------------------------------------------------------------------------------------------------------|-------------------------------------------------------------------------------------------------------------------------------------------------------------------------------|----------------------------------------------------------------------------------------------------------------------------------------------|
| <p><b>Video Device</b></p>  <p>IP: 192.168.101.4</p> | <p><b>Nox C1</b></p>  <p>License: DC Licensed<br/>SN: 931010058<br/>IP: 192.168.101.10</p> | <p><b>ResMed Tx Link</b></p>  <p>IP: 192.168.101.15</p> |
| <p><b>Nox A1</b></p>  <p>SN: 972901527</p>           | <p><b>Nonin 3150 Oximeter</b></p>  <p>BDA: 13:15:28:69:42:96</p>                           | <p><b>SenTec SDM</b></p>  <p>C1 Serial Port: 1</p>      |

Add >>


Remove Device

Scan for IP Devices

Add to Room

Close


To select devices to add to your room click the device and a blue bold frame will appear around each selected device. When you have selected the devices to add to the room, click **Add to Room** and your room with this selection of devices will be added.

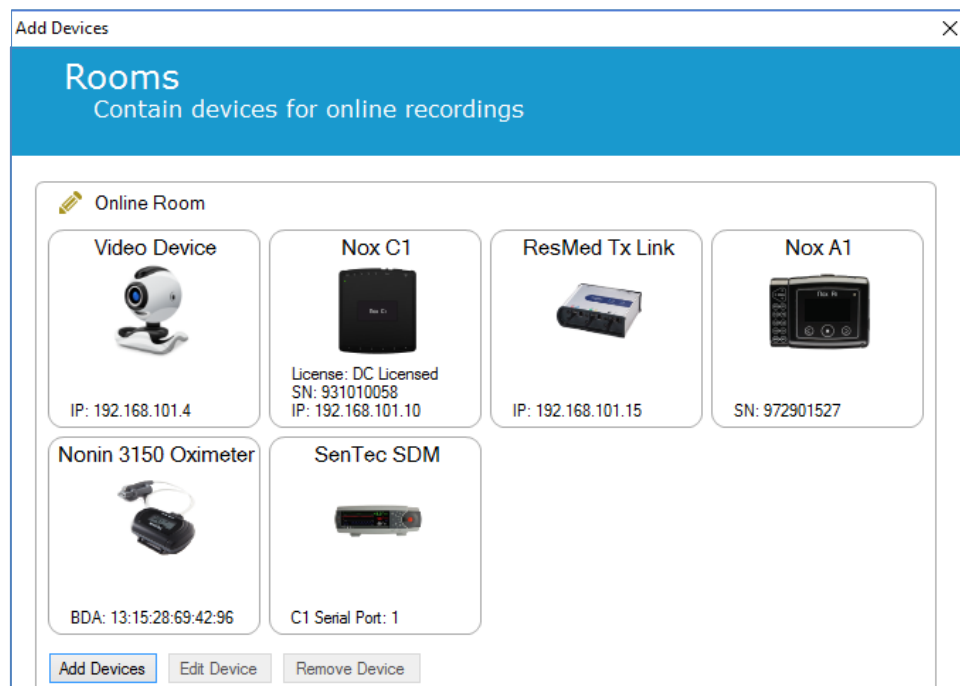

You have now completed the configuration of the online room. You can in the same way as described here above add additional rooms.

## Configuration of New Sensors

If you want to create new sensor configurations, e.g. to use with the Nox C1 Access Point, you can do that by navigating to **Devices > Sensors...** from the Noxturnal Toolbar.

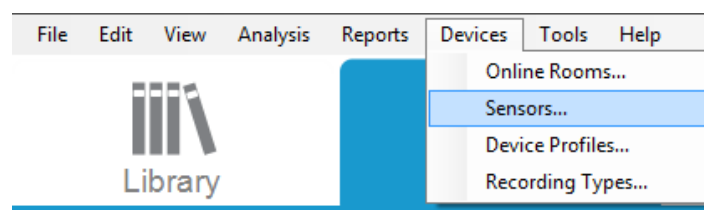

From the **Manage Sensors** Wizard you can create a new sensor and edit/delete existing sensors. To create a new patient or auxiliary device sensor click **New**. Patient sensors are sensors connected to Nox A1, T3 or T3s Recorders and the patient. Auxiliary device sensors are connected to Nox C1 Access Point and an auxiliary device.

**Manage Sensors** [X]

**Sensors**  
Patient and auxiliary sensor configuration

Search:

| Label              | Location               | Unit | Auxiliary | Bipolar | Description                     |
|--------------------|------------------------|------|-----------|---------|---------------------------------|
| <b>Respiratory</b> |                        |      |           |         |                                 |
| Abdomen Piezo      | Piezo.Abdomen          |      | No        | Yes     | Abdomen Piezo sensor            |
| Abdomen RIP        | Inductive.Abdomen      |      | No        | Yes     | Abdomen RIP sensor              |
| Pneumoflow         | Pneumoflow             | V    | No        | Yes     | Differential Pressure           |
| Thermistor         | Thermistor.NasalOral   |      | No        | Yes     |                                 |
| Thermocouple       | Thermocouple.NasalOral |      | No        | Yes     | Thermocouple for nasal and oral |
| Thorax Piezo       | Piezo.Thorax           |      | No        | Yes     | Thorax piezo sensor             |
| Thorax RIP         | Inductive.Thorax       |      | No        | Yes     | Thorax RIP sensor               |
| <b>EMG</b>         |                        |      |           |         |                                 |
| Both Legs          | Leg                    | V    | No        | Yes     | EMG sensor for the sum of both  |
| Bruxism            |                        | V    | No        | Yes     |                                 |
| BruxismLeft        | Left                   | V    | No        | Yes     |                                 |
| BruxismRight       | Right                  | V    | No        | Yes     |                                 |
| Left Leg           | Leg.Left               | V    | No        | Yes     | Left leg EMG sensor             |
| Right Leg          | Leg.Right              | V    | No        | Yes     | Sensor for right leg EMG        |
| Submental          | Chin                   | V    | No        | Yes     | Sensor for submental EMG        |
| <b>FCG</b>         |                        |      |           |         |                                 |

[New](#)
[New Based On](#)
[Edit](#)
[Remove](#)
[Close](#)

You can select whether a new patient sensor or an auxiliary device sensor is to be created. Fill in the applicable fields and click **OK** to save the sensor configuration.

## Device Profiles for Online Devices


For the Nox devices used for online recordings you can set up **Device Profiles**. The Device Profiles encompass the device's channel configuration. Noxturnal offers a range of default Device Profiles and you can also easily setup new Device Profiles. For instructions on how to customize Device Profiles refer to the *Device Profiles* section.

## Recording Types for Online Devices

The final step is to set up **Recording Types**. This is a list of the types of recordings that you will record online in your clinic. Each **Recording Type** brings together a collection of available online device types which would be grouped together. Examples are: **Standard PSG with Nox C1**, would bring together a Nox C1 Access Point, Nox A1 Recorder, Nonin 3150 Oximeter and a Video Camera. For instructions on how to setup new Recording Types refer to the *Recording Types* section.

## Starting an Online Recording

When you have completed the steps above to setup your online configuration an online recording can be started. From the **Recording** page you can start an online recording within the room you have set up. To start the recording either double-click the room icon or click **Configure Recording**.

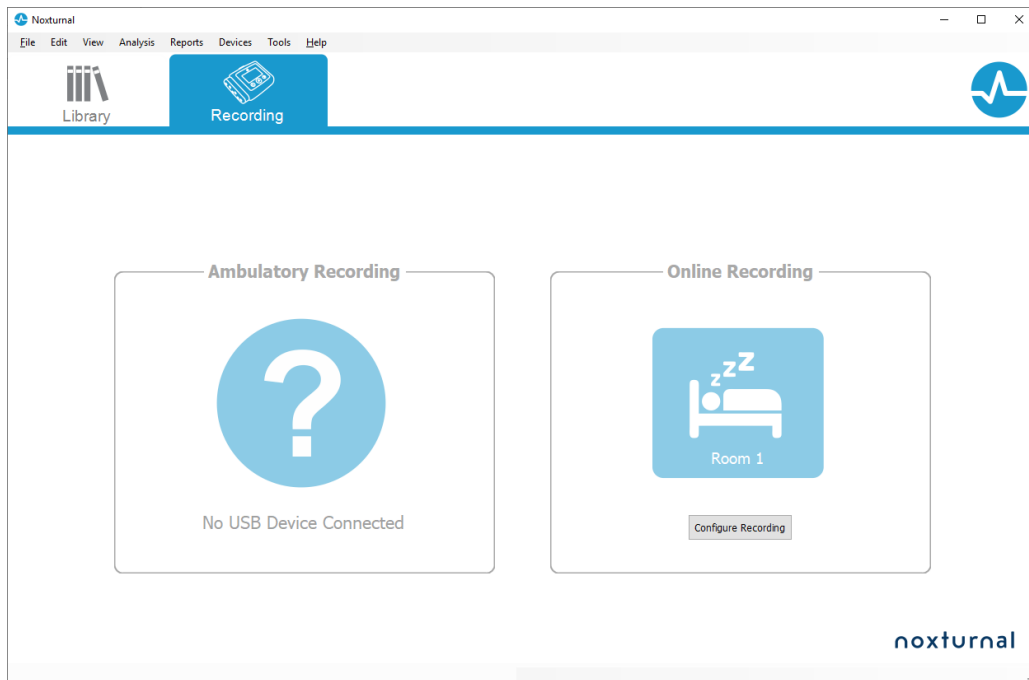

This will bring up the **Start Online Recording** wizard. This wizard will allow you to:

- Select the **Recording Type** which is about to be performed from the dropdown list.
- The selection of **Devices** is dependent on the **Recording Type** selected. All devices available in the online room are listed, however the devices not included in the recording type are greyed out. You can include the disabled devices for the recording by checking the appropriate boxes from the list of devices.
- Select **Device Profile** for some devices, such as the Nox A1 and the Nox C1.

Start Online Recording

**Select Recording Type**

Recording type: 1 Patient: 2

Recording Type: MSLT with Nox C1

**Devices**

|                     |                                                                                              |  |                                     |
|---------------------|----------------------------------------------------------------------------------------------|--|-------------------------------------|
| Nox A1              | Profile: Standard PSG<br>SN: 972901527                                                       |  | <input checked="" type="checkbox"/> |
| Nox C1              | Profile: Ambient Light Sensor<br>IP: 192.168.101.10<br>SN: 931010058<br>License: DC Licensed |  | <input checked="" type="checkbox"/> |
| Nonin 3150 Oximeter | BDA: 13:15:28:69:42:96                                                                       |  | <input checked="" type="checkbox"/> |
| SenTec SDM          | C1 Serial Port: 1                                                                            |  | <input checked="" type="checkbox"/> |
| ResMed Tx Link      | IP: 192.168.101.15                                                                           |  | <input checked="" type="checkbox"/> |

Next > Standby Mode Start Recording Cancel

When you have selected your **Recording Type** and the applicable devices along with their **Device Profiles** you can click **Next** to enter the patient information. The final step is to start the recording and you do that by clicking **Start Recording** or clicking **Standby** within the **Patient Information Wizard**.

#### Start Recording:

You will then see your selected Workspace Layout appear with a status window showing the status of the recording which is starting. Finally, you will see the recorded signals appear in real time and you can start working with them.

#### Standby Mode:

The **Standby Mode** will open your selected workspace with a status window showing you have entered **Standby Mode** that gives you the option to connect to the Online Room for preparing, evaluating, and assisting the patient hook-up and finally start the recording using the **Noxturnal App** or **Start Recording** as is described in the step above.


Online Recording Standby

● **Recording Ready**


Start Recording or Connect via Noxturnal App

Start Recording Cancel Recording


When the user has connected the Noxturnal App to the online room the live traces that start to appear are **NOT** being saved to the recording. It is only a preview as is indicated by the preview status. The signal will start to record as soon as the user hits **Start Recording** either in the Noxturnal App or in the Noxturnal software.



The user can also enter the standby mode any time after the recording has been started if he wants to pause the recording for some period of time by clicking the red rec button on top of the screen.



By clicking the rec button, it will give you the option to either enter standby mode, stop the recording or cancel and continue with the recording.

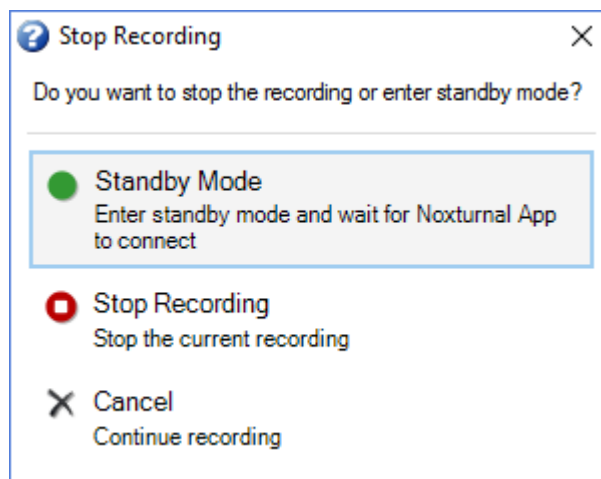

## Nox C1 Configuration

The Nox C1 Access Point is equipped with 12 analog channels suitable for collecting of DC signals from auxiliary devices. The channels are collected on 6 ports, labeled DC IN from 1 to 12 on the top of the device; each analog port yields 2 channels. Auxiliary devices can be connected to the Nox C1 analog inputs. The voltage range allows interfacing signals from -5V to +5V. For further information on the Nox C1 Access Point, refer to the Nox C1 Manual.

### Nox C1 Access Point Network Configuration


The default factory configuration of the Nox C1 Access Point is listed in the table below. The Nox C1 network configuration can be managed through Noxturnal.

| Nox C1 Network Configuration             | Details                                                                   |
|------------------------------------------|---------------------------------------------------------------------------|
| DHCP server                              | DHCP pool: 192.168.101.64-192.168.101.127                                 |
| Static IP address                        | 192.168.101.10                                                            |
| Universal Plug and Play (UPnP) discovery | Networking protocol that permits the Nox C1 to be discovered on a network |

To manage the network configuration of the Nox C1 you can open an Online Room that has been configured (Devices > Online Rooms...) and select the Nox C1 within the room and click **Edit Device**. In the dialog below you can see how you can change the network configuration of the Nox C1.


## Upgrading Nox C1 Access Point firmware

If a new version of the Nox C1 Access Point firmware is available for the connected device, Noxturnal will notify the user by displaying this message when the user starts an online recording.

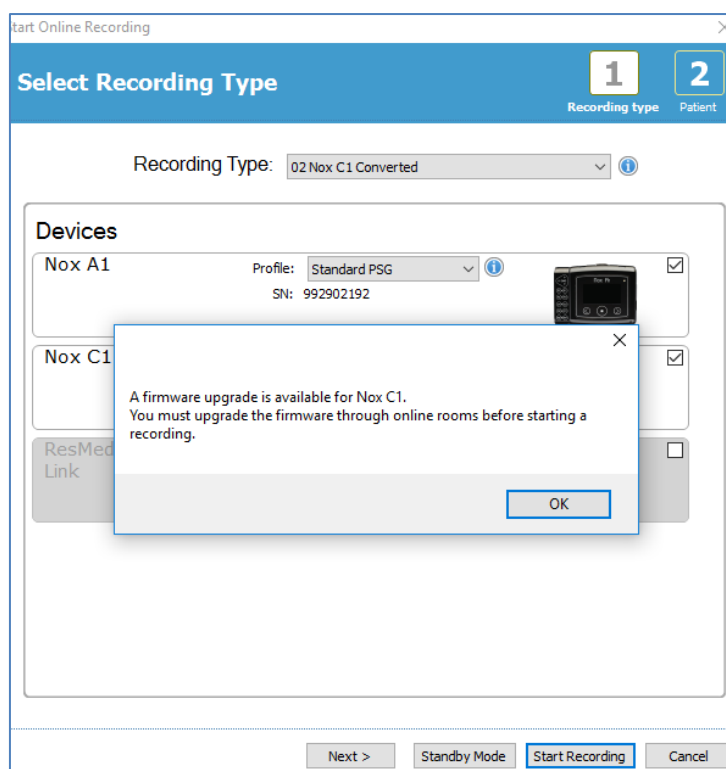

The user can access the firmware upgrade by navigating to the **Devices** tab in the menu bar.

**Devices >> Online Rooms...**

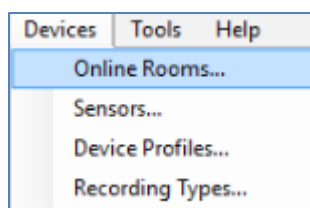

Select the Nox C1 access Point and click **Edit Device**.



In the device properties window select **Upgrade Firmware**.

The firmware upgrade will be indicated with a status bar and when finished will display like this.

## Activating Nox DC Channel License

The DC channels on the Nox C1 Access Point are locked by default. To be able to use the DC channels on the Nox C1 you will need to have a Nox DC Channel license activated. For further information on this, please consult with Nox Medical or their sales representatives.

The license is activated by clicking **Set License** in the **Device Properties** dialog that is shown below and following the instructions on the page.

## Integration of Video Devices for Online Recordings

Noxturnal supports online video recording. To use the digital video support provided by Noxturnal in an online recording you need to configure your system to include a video device.

A video device can be added to your online system configuration and the setup saved for future use. To configure a video device with your system you must:

1. Ensure that you have **video codecs** installed on your computer
2. Ensure that the video device is connected to the same network as the Nox C1 Access Point and the computer running Noxturnal
3. Setup an **Online Room** including the video device
4. Setup a **Recording Type** including the video device and define the video profile
5. Select the Online Room and start an online recording from the Noxturnal **Recording** page

### Setup an Online Room with a Video Device

#### VIDEO CODECS


Noxturnal's support for video is governed by the video codecs that are installed on your computer system. These video codecs are specialized software that enables the compression and decompression of digital video. Noxturnal does not install any codecs but most computer systems have some types of codecs installed. You will require codecs to be installed on your computer system to use video with your Nox Sleep System. Noxturnal will then provide you with access to the features supported by these codecs. You can download the **K-Lite Codec Pack** from the Nox Medical support site: <http://support.noxmedical.com/hc/en-us/articles/207882176>

#### VIDEO CAMERA INTEGRATION


To setup an online recording including a video device follow the steps below.

1. Setup an Online Room in Noxturnal as explained in *Online Room* section (Devices > Online Rooms... from the Noxturnal toolbar).

2. Add a video device to your Online Room by clicking **Add Devices** and select **Video Device** from the **Device Types** list.

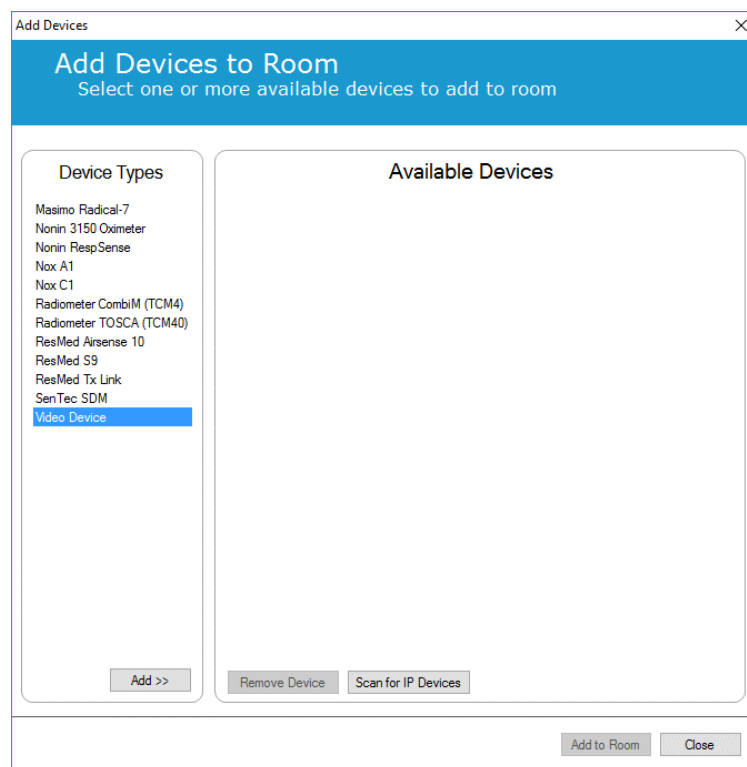

3. You will see the Device Properties dialog shown below. Check the applicable option, depending on the video device being used and click **Next**.

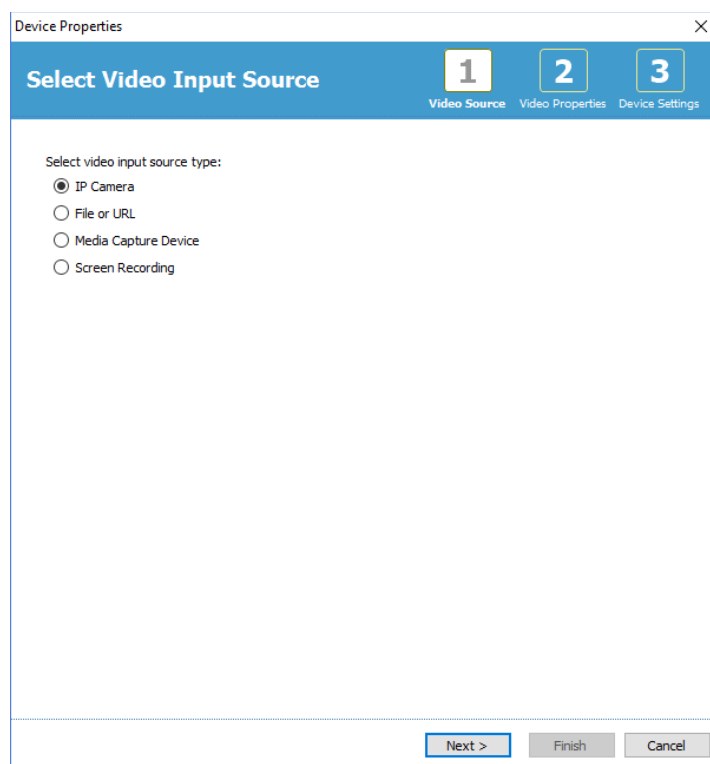


To setup your IP camera click **Find...** and Noxturnal will scan your network and discover video cameras that are connected to your network if they have UPnP (networking protocol that permits IP camera to be discovered on a network) enabled. Noxturnal offers default connection options for some IP cameras (Axis, D-Link cameras, Vivotek and Hikvision). Make sure that when choosing the connection string available in Noxturnal to choose the connection string (URL) per the recording you are performing, if only video is to be recorded, or both video and audio are to be recorded.

If your camera is not automatically discovered by Noxturnal when using the **Find...** action you can always manually add your camera by entering the relevant connection string (URL) and the camera IP address into the **File or URL** field.

If you have a video device that is not supported by the default connection options mentioned above you can always manually add new connection strings (URL) to have them accessible in Noxturnal for future use. To do that browse to **Tools > Settings > Advanced** and select the **Default Settings**. Open the Video Profiles folder and open the *IPCameras* Excel sheet. You can add to the existing list of connection strings a new connection string for your video device and that will become available to use within Noxturnal.

When you have entered the User and Password information for your camera you can click **Start Preview** to see if your camera is correctly set up and working with Noxturnal. If a delay is observed during the preview a delay input can be added to correct the video replay during the analysis. Click **Next** and you can give the camera a unique name and then click **Finish**.

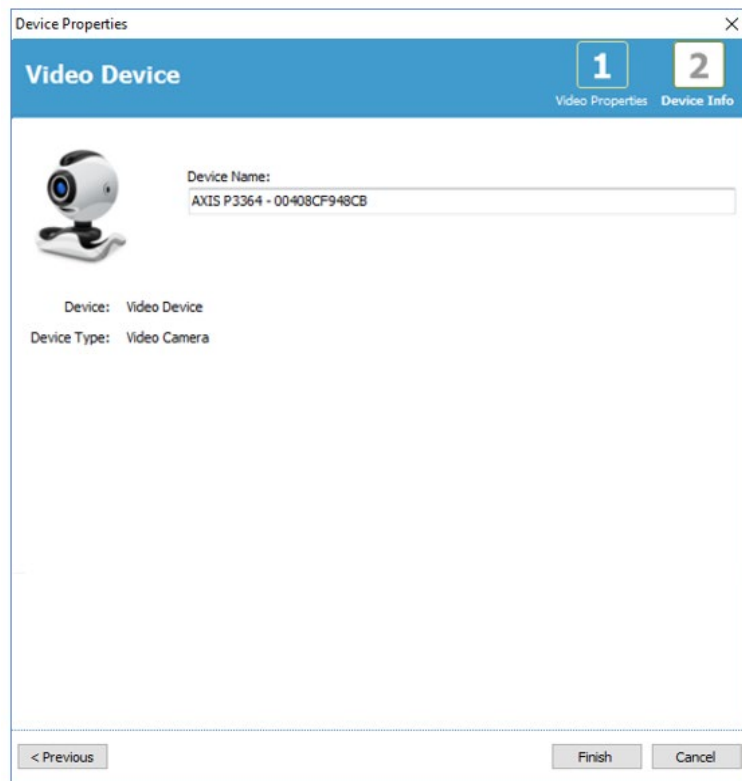


You have now added the video device to your online room.


### Setup a Recording Type with a Video Device

---

Noxturnal offers default Recording Types for online recordings that include video device. You can select one of the default Recording Types and start directly an online recording which includes a video device. You can also set up a custom Recording Type and define the Windows Media Profile to use with Noxturnal when recording and compressing the online video. To do that navigate to **Devices > Recording Types...** from the Noxturnal toolbar. In the Recording Types wizard select **New** and **Online** from the **Recording Type** dropdown list.

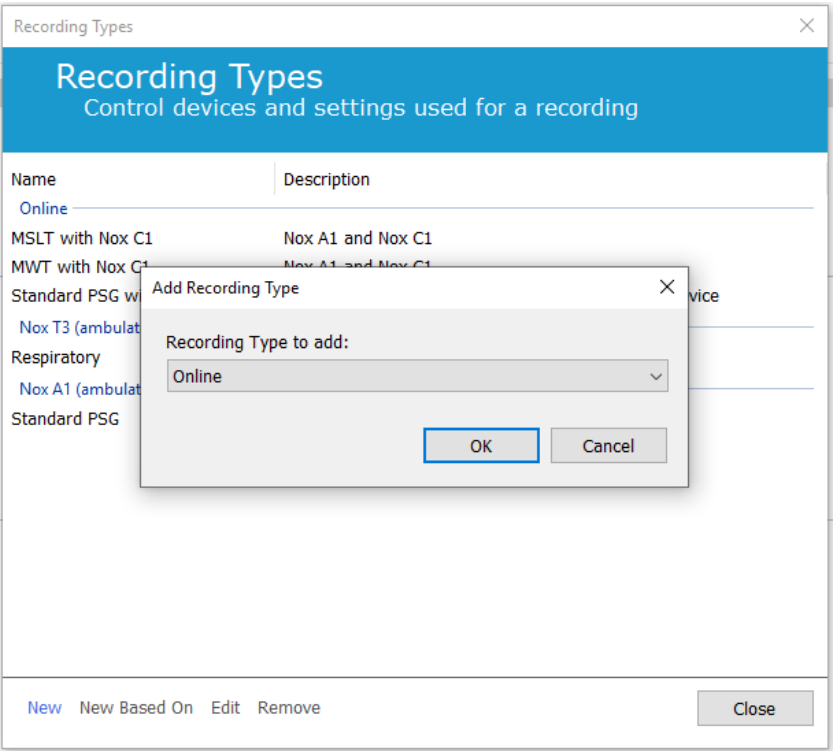


In the Online Recording Type wizard, you can add your video device as other devices. You can select the video profile to be used from the drop-down list, see image below.

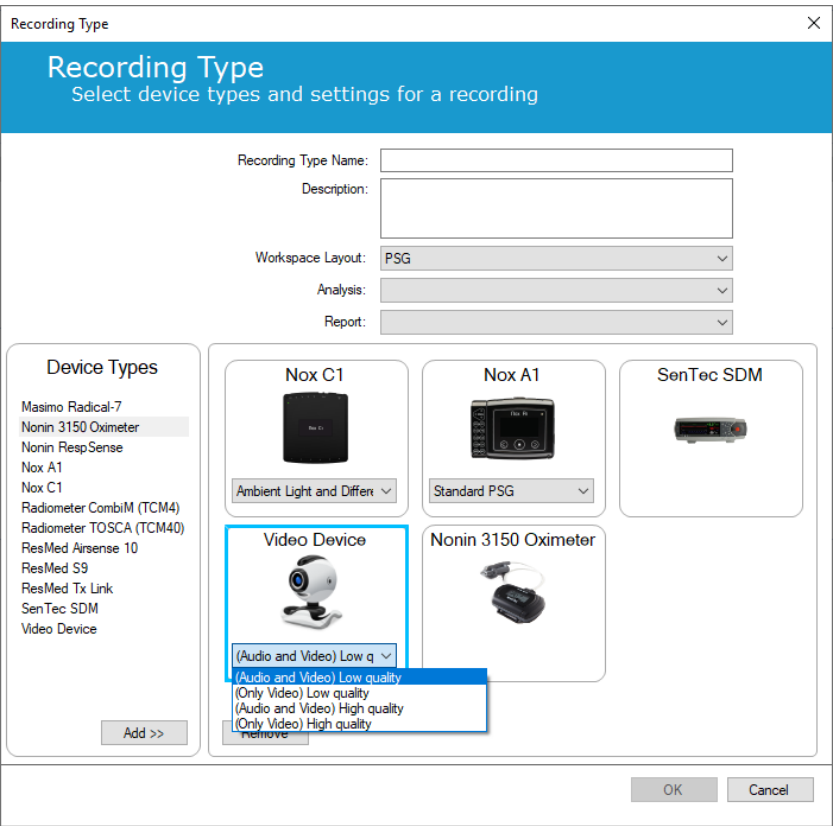

Noxturnal offers selection of default video profiles, however, you can create custom profiles and access them for use in Noxturnal. For further information and instructions on how to do that refer to Nox Medical support site, Windows Media Profiles in Noxturnal.


You have now configured your system to include a video device and you can start an online recording from the Noxturnal **Recording** page by double-clicking the room or click **Configure Recording**.

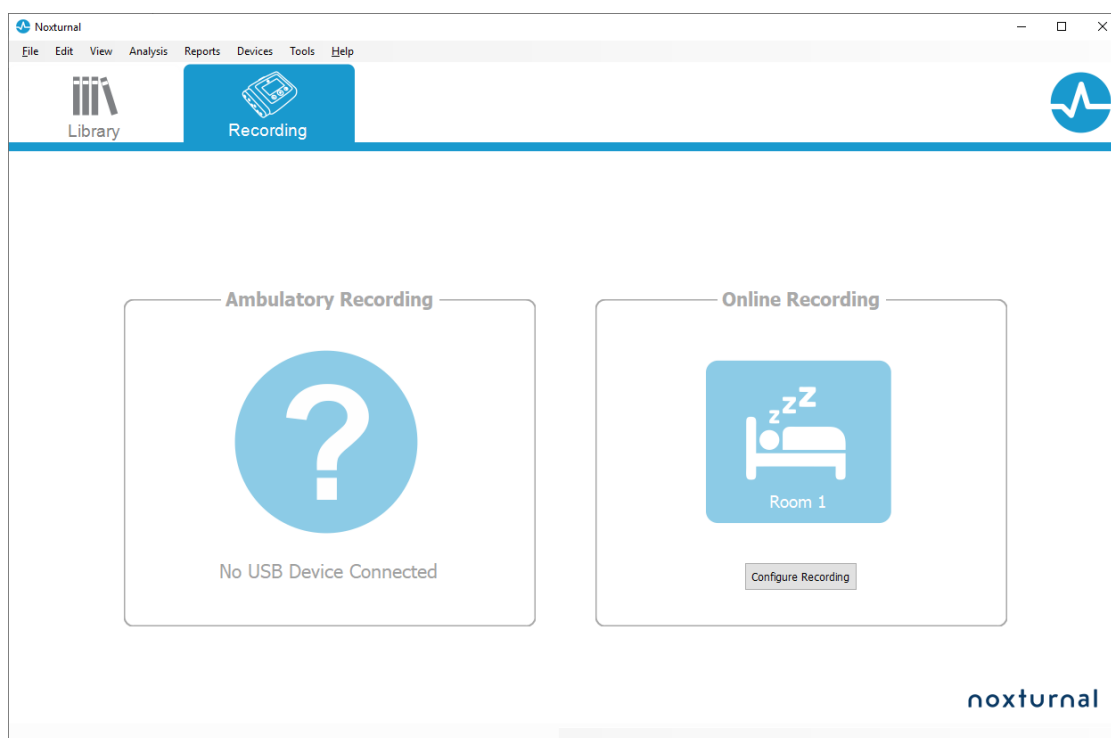

## Working with recordings in Noxturnal

### Recording Results Page

After downloading from a recording device or opening an existing recording in Noxturnal the **Recording Results** page is shown. This page contains an overview of the most common analysis parameters and the recorded signals. The result page is automatically updated when changes are made to the existing scoring or if the automatic analysis is run. When sleep stages are available, such as for recordings done with the Nox A1 Recorder, you will see graphs and information with that information. For the Nox T3 Recorders, you will only see parameters available with those devices.

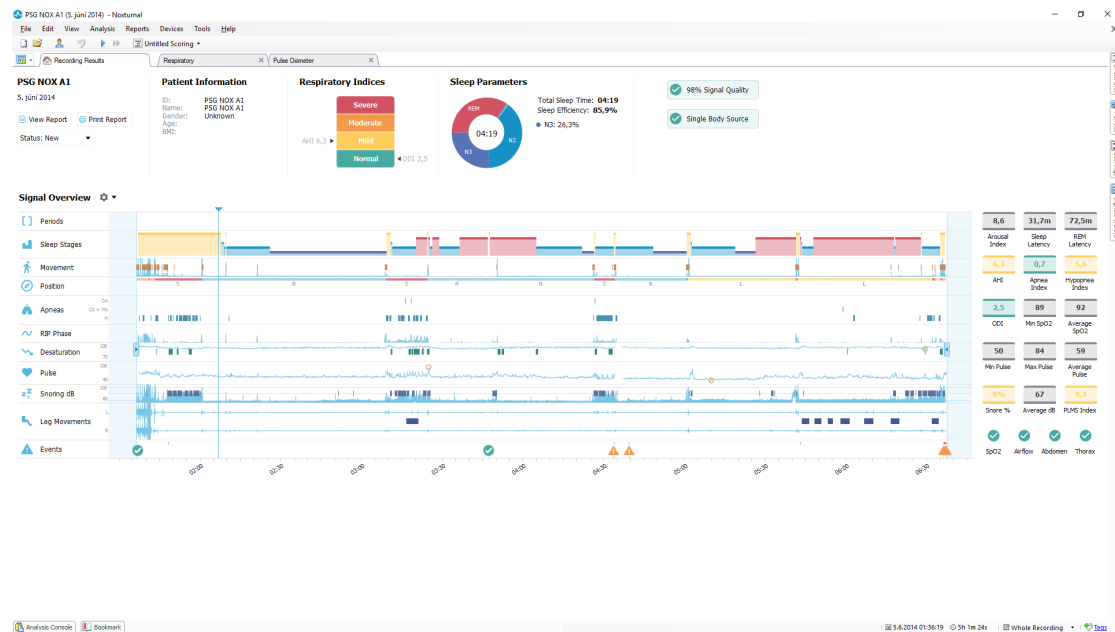

### Result Page Commands

The **Recording Results** page has buttons for the following actions:

- **View Report:** This option creates the default report for the recording, the report defined within the Recording Type (for further information refer to the Recording Types section).
- **Print Report:** This option prints the default Report.
- **Recording Status:** This option allows to set the status of recordings. Downloaded recordings always have the status **New**. If a recording has failed for any reason, the status can be set to **Invalid**. If the recording has been diagnosed, the status can be set to **Scored**. If the recording and the scoring have been reviewed, the status can be set to **Reviewed**. If the recording has been interpreted, the status can be set to **Interpreted**. If a recording has been diagnosed and accepted, the status can be set to **Done**.

### Patient Information


The **Information** panel shows information about the recorded patient. Edit the recording properties and patient information by clicking the patient icon or by pressing the **Ctrl+I** shortcut key.

### Patient Information

ID: PSG NOX A1  
 Name: PSG NOX A1  
 Gender: Unknown  
 Age:  
 BMI:

### Sleep Parameters


The **Sleep Parameters** panel shows a doughnut chart of different sleep stages **if** sleep stage events have been scored.

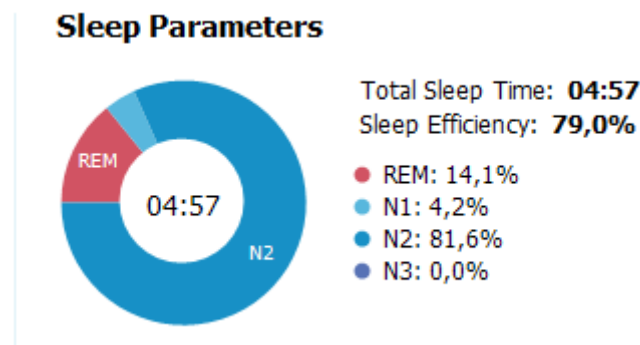

- **Total Sleep Time** is the time the patient spent asleep (based on Hypnogram).
- When **Total Sleep Time** is not available **Est. Total Sleep Time** (Same as AASM term Monitoring Time) is the parameter used. That is the time the patient is lying down during the recording.
- **Sleep Efficiency** ranges from 0-100% where 0% means that the patient was awake the entire night and 100% means that he slept throughout the night. When sleep scoring is not available the software uses movement periods to estimate this parameter.

### Respiratory Indices

The **Respiratory Indices** panel shows the main analysis parameters and their relation to severity. AHI, the Apnea Hypopnea Index, is the number of apneas and hypopneas per hour of sleep and Oxygen Desaturation Index (ODI) is the number of scored oxygen saturation drops per hour of sleep (default automatic analysis scores all desaturations of 3% or higher but this can be customized by the user). The severity goes from *Normal* → *Mild* → *Moderate* → *Severe* and complies with the levels set forth by the AASM. If more than one night has been recorded, then these parameters will show the average values for all nights. Refer to the section *Analysis Protocols* for more information.

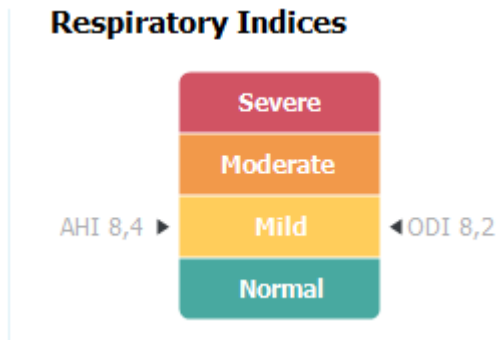

## Overall Signal Quality and Single Body Source

Overall **Signal Quality** is determined from the monitoring of signal quality of the following signals: oximeter, airflow, abdominal or thoracic respiratory effort signals. The lowest signal quality of those signals is displayed for the overall **Signal Quality** on the Recording Results Page and is represented from 0-100%.

The **Single Body Source** result indicates whether the oximeter and RIP belt signals are originated from the same subject. For further information about this result, refer to the section *Single Body Source*.



## Signal Overview and Parameters

The **Signal Overview** panel is a top down reviewing tool where recording results can efficiently be reviewed and edited. The overview panel is split up into analysis parameters on the right and signal overview on the left.



The analysis parameters show a summary of the most common analysis parameters for a single night. If more than one night has been recorded, then each night is represented within its own panel. You can also select the period to view with the period menu located in the lower right corner of the application. Each parameter is color coded based on its severity ranging from green to red (*Normal* → *Mild* → *Moderate* → *Severe*).

- **Arousal Index** is the number of arousals per hour during sleep time.
- **Sleep Latency** is the duration in minutes from Lights out (Analysis Start Time) until the first epoch of scored sleep.
- **REM Latency** is the duration in minutes from the first occurrence of sleep until the first occurrence of REM.
- Respiration is represented by indices. Indices are a method to represent analysis parameters in a standardized way.
  - Apnea Hypopnea Index (**AHI**)
  - **Apnea Index** (AI)
  - **Hypopnea Index** (HI)
  - Oxygen Desaturation Index (**ODI**) represents a number of oxygen desaturation events per hour of **Total Sleep Time** or alternatively **Est. Total Sleep Time**.
  - **Snore Percentage** is the proportion of sleep time spent in snore episodes (marked as **Snore Trains**)
  - **Average dB** is the average dB levels during snore train periods.
- **Signal Quality** is determined from the monitoring of signal quality of the following signals: SpO<sub>2</sub>, airflow, abdominal or thoracic respiratory effort signals. The signal quality of those signals is and is represented from 0-100%.

## Signals and Events


---

The signals and events plot in the signal overview panel give an overview of the whole night.

- Signals in the overview can include:
  - **Spectrogram** for the channel displayed on the screen (Right click the Spectrogram to change the channel)
  - **Sleep Stages/Hypnogram** shows the sleep stages throughout the night
  - **Arousals** shows the arousals throughout the night
  - **Movement**
  - **Position**
  - **Apneas/RIP Phase** (phase between abdomen and thoracic respiratory effort signals)
  - **Oxygen Desaturation** (SpO<sub>2</sub>)
  - **Pulse**
  - Audio Volume (**Snoring dB**)
  - **Leg Movements** (optional)
- Events shown in the overview include apneas and hypopneas, oxygen saturation drops, snoring episodes and artifacts.


## Changing the Analysis Periods

If a recording starts before all sensors have been attached or if the patient removes the sensors before the recording ends, it is possible to adjust the interval being analyzed by moving the Analysis Start 1 and Analysis Stop markers 3 to the appropriate location within the recording. All the analysis parameters are updated accordingly when these adjustments are made.

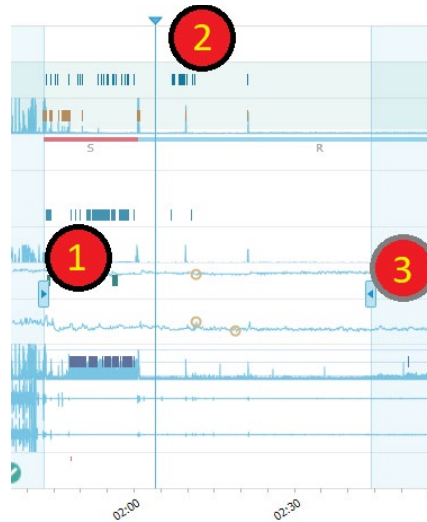

To navigate into the recording use the synchronization marker 2. All signal sheets such as the **PSG**, **Respiratory** and **Pulse Oximeter** sheets are synchronized accordingly. If an interesting event is located in the overview, drag the synchronization marker over that area and browse into the relevant signal sheet to view the raw signals.

Event periods can be added directly from the **Signal Overview** panel. To add an event period, locate the mouse pointer to the **Periods** panel and mouse click. The **Event** period menu will be available as shown below.

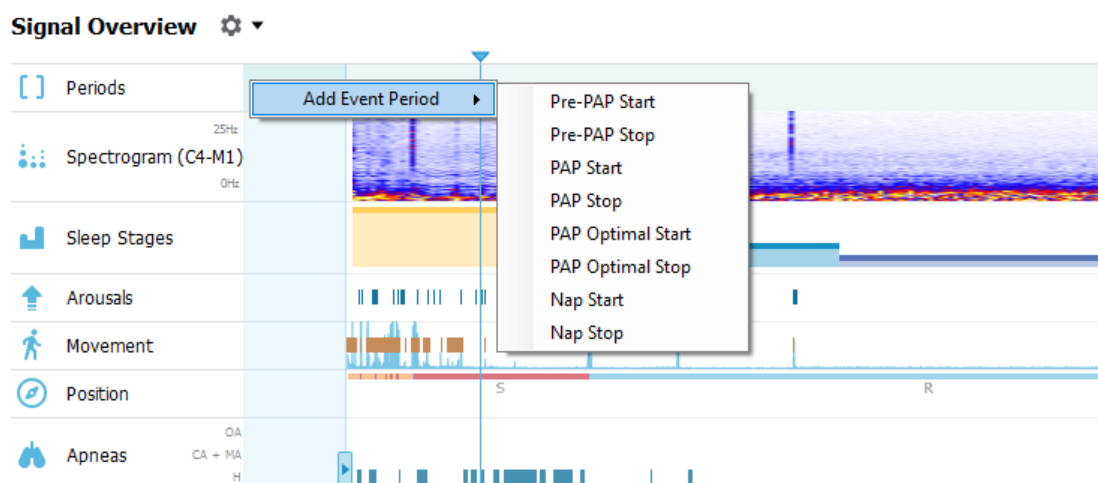

Exclusion of invalid data can be performed in Signal Overview panel. To exclude invalid data from the recording locate the mouse pointer on of the signals, left mouse click and select an area by dragging


left/right. Release the mouse button and the menu showed below will be available. The 'Invalid Data' events will be excluded from the report calculations.

## Signal Overview



## Setting Units


To change the unit system used to represent units such as height and weight navigate to **Tools > Settings...** from the Noxturnal toolbar. On the **General** property page locate the **System Units** drop-down list and select the applicable field to be edited.

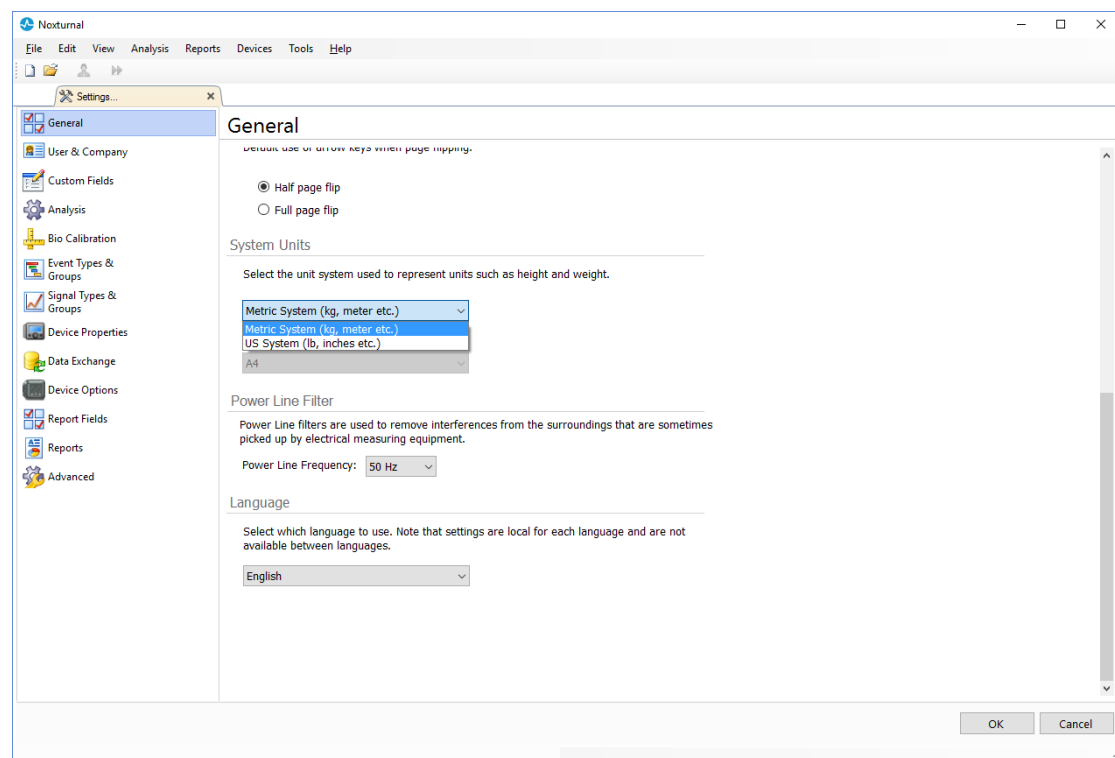


## Viewing Signals

### Workspace Menu Button


The **Workspace Menu Button**  allows you to apply different Workspace Layouts and signal sheets to manage the way you want to see your recordings. The Workspace Layouts include a selection of signal sheets and signal sheet properties. Noxturnal offers a range of default Workspace Layouts (Respiratory and PSG layouts) and signal sheets. You can also setup custom Workspace Layouts and Signal Sheets. You can save all changes to your workspace layout for future use. This means that you can change settings on traces and setup your work environment as you see fit.

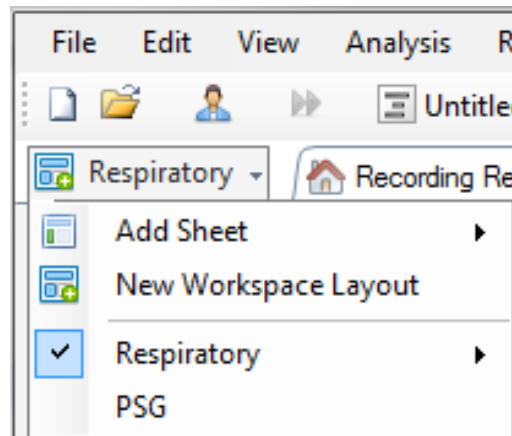

You can use the Workspace Menu button to **Add Sheet**, create a **New Workspace Layout**, using a default layout to base it from or even **Revert Layout** after making changes.

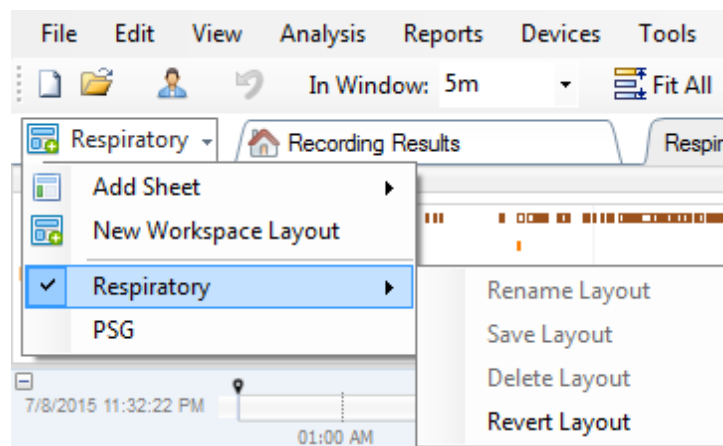


To save a customized signal sheet you right click on the signal sheet tab and select **Save Sheet Layout As...** When you have saved the customized signal sheet you can always **Update Saved Layout** if additional changes are made. For further information on signal sheets refer to the *Signal Sheets* section.

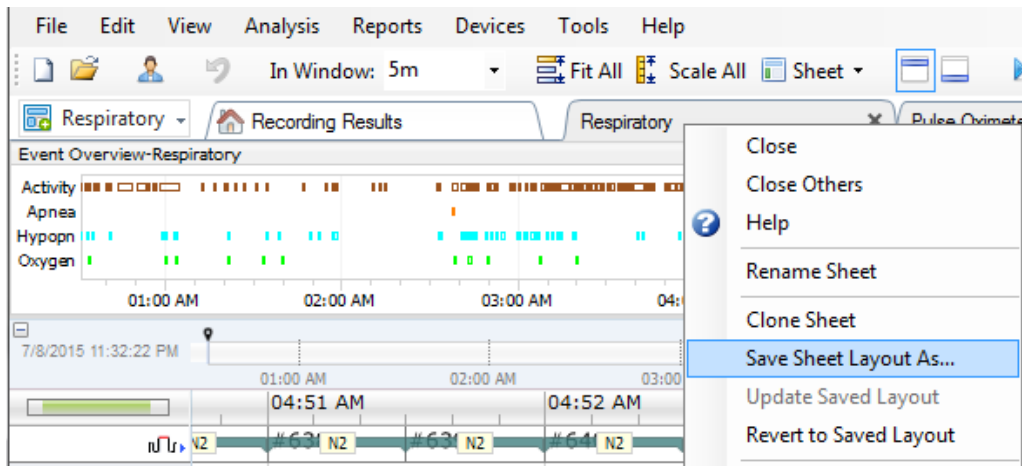


## Signal Sheets

A signal sheet shows one or more signals in a tab window in the workspace. Noxturnal comes with predefined signal sheets such as the **Respiratory** sheet, **PSG** sheet, and the **Pulse Oximeter** sheet.


To add or remove signals in a signal sheet navigate the mouse to the **Signals and Data** task window located to the right of the workspace. When the mouse cursor is over this tab the **Signals and Data** task window will slide out. A list of all signals available is listed in this task window. A checkbox next to the signal determines if the signal is displayed in the sheet or not. Check/Uncheck the box to add or remove the signal from the sheet. See the **Signals & Data** tab here below.

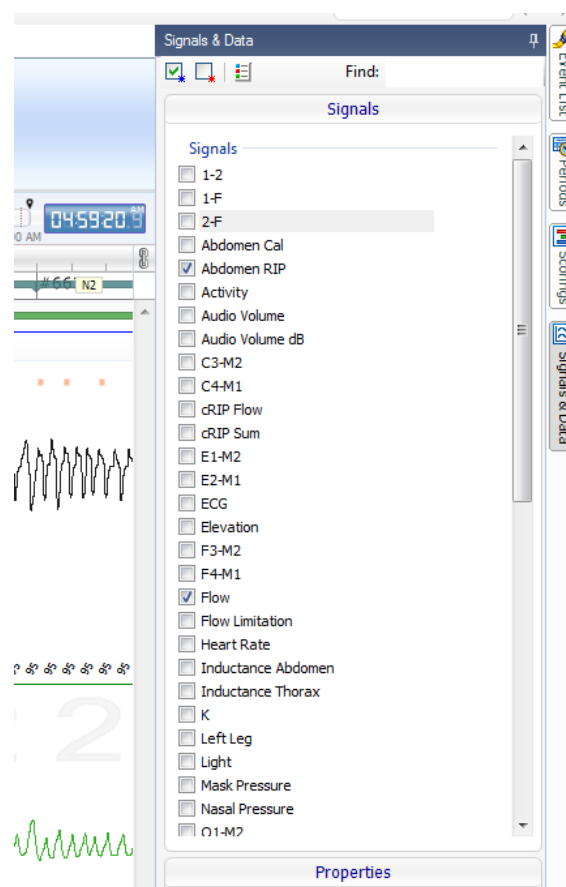

## Working with Signals

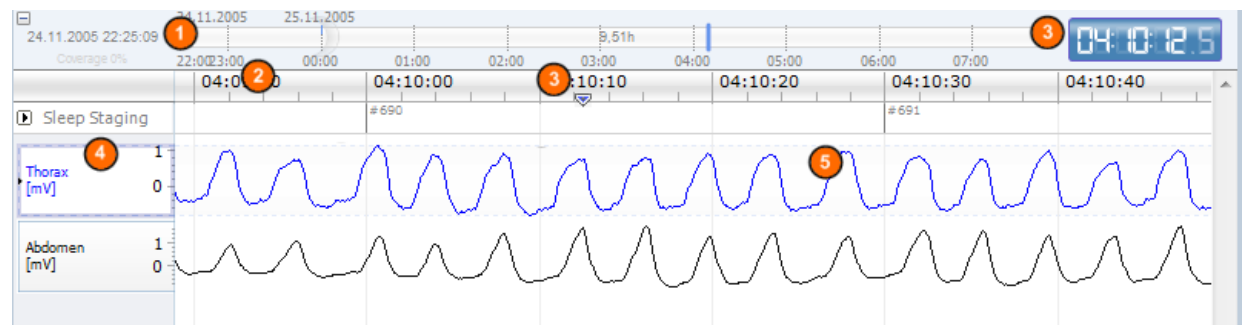

- 1 The navigation bar allows to quickly navigate to any time in the recording. The blue line indicates where the user is located in the recording. Click on any location in the bar to jump to that time.
- 2 Time axis displays the recording time and the time period in the window. Right-click on the time axis to change the interval in the window. Stretch/compress the time axis with the mouse to change time interval in the window.
- 3 The synchronization marker located on the time axis is used to synchronize with other signal sheets and views. The clock on the right side of the navigation bar shows the time of the marker position. The synchronization marker can be dragged and moved in time.
- 4 Signal value axis shows the name of the corresponding plotted signal and the value axis scale. The axis can be stretched/compressed with the mouse. To change the properties of the value axis, double-click on the axis and a dialog will appear where the properties can be changed.
- 5 Signal plot in a pane. Signals can be adjusted in many ways. Resize the signal pane or move the signal pane around by using the mouse. To change the properties of the signal, double-click on the signal and a dialog will appear where the signal properties can be changed. To access all actions for an individual signal trace right click the signal trace and the following menu will be available.

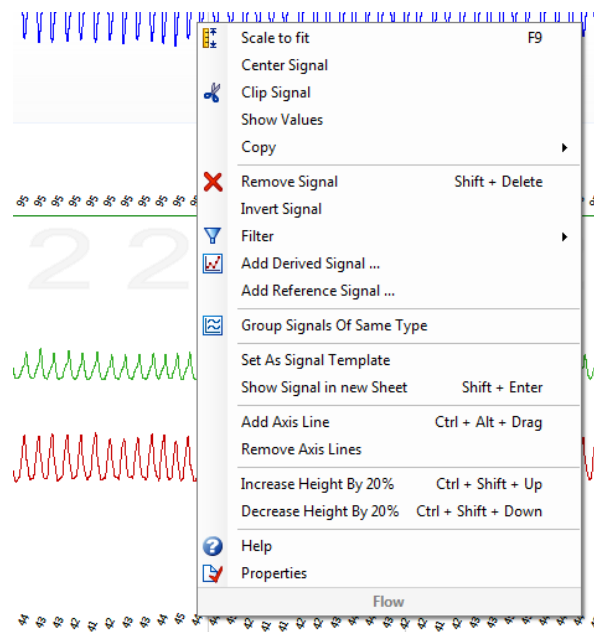

## Keyboard Navigation

---

Navigate and manipulate the signal sheet by pressing the following shortcut keys:

### Navigation:

- Right key = By default - Half page flip forward, user configurable
- Left key = By default - Half page flip backward, user configurable
- Ctrl + Right key = By default - Full page flip forward, user configurable
- Ctrl + Left key = By default - Full page flip backward, user configurable
- Page Down key = Page flip forward
- Page Up key = Page flip backward
- Home key = Start of recording
- End key = End of recording
- Shift + Right key = Increases time span in window
- Shift + Left key = Decreases Time span in window
- Shift + Ctrl + Left key = Jump to previous data session
- Shift + Ctrl + Right key = Jump to next data session
- - key = Zoom out of selection
- + key = Zoom into selection
- Mouse wheel = Scroll forward/backward
- Mouse wheel + Ctrl key = Scroll up and down

### Active Signal:

- Shift + Up = Increase signal scaling
- Shift + Down = Decrease signal scaling
- Ctrl + Up = Shift signal up
- Ctrl + Down = Shift signal down
- Shift + Return = Show active signal in new sheet
- Shift + Delete = Remove active signal from sheet
- Up key = Select signal above
- Down key = Select signal below
- Ctrl + F = Find events
- F9 = Auto scale signal

### Signal Sheet:

- Space = Play/Pause recording playback
- Ctrl + W = Auto scale signals
- Ctrl + A = Arrange signals

### Events:

- Tab = Next event, if searching then next search result
- Shift + Tab = Previous event, if searching then previous search result
- Delete = Delete selected events, or delete events overlapping selection
- Return = Deselect all events
- Esc = Clear all selections


## Working with Events

Events are used to identify areas of interest in a signal. An event has a start and stop time and a type used to classify it. Events can either be manually added to a signal or scored by the automatic analysis to flag areas of interest. Events can be modified or removed.

### Scoring an Event

To score an event go to a sheet containing signals; locate an area on a signal of interest.


- 1 With the left mouse button, highlight an area to score the event on.
- 2 Press the shortcut key for that event. Shortcut key can be assigned to an event type from **Setting -> Event Types & Groups -> Edit -> Behavior**.

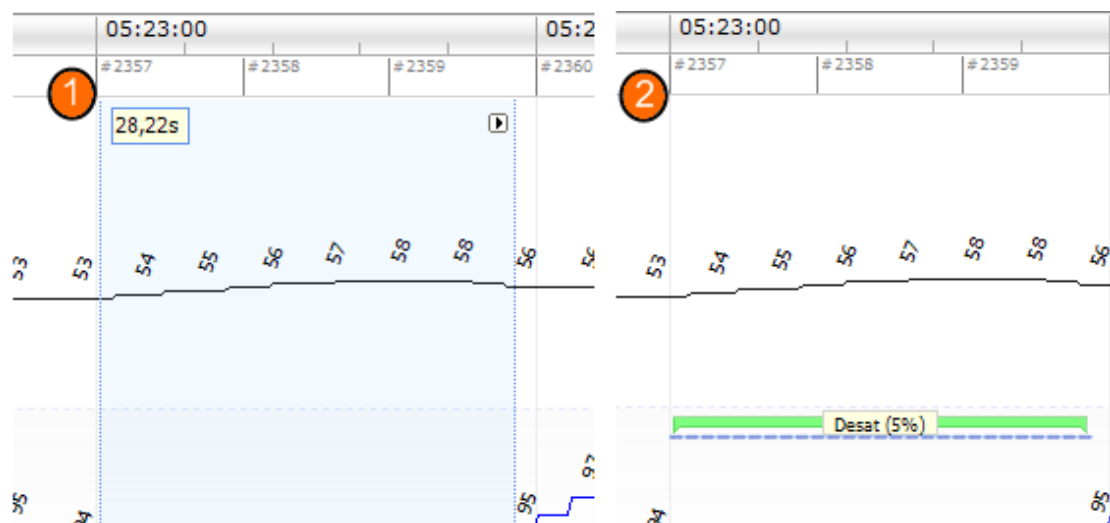

An alternative method for scoring an event is to highlight an area with the left mouse button, as before, but then right-click on the area and select an event from the list.

### Single Click Scoring

Noxturnal offers the option to use **Single Click Scoring**. To activate the single click scoring action click the  icon located in the Noxturnal toolbar.

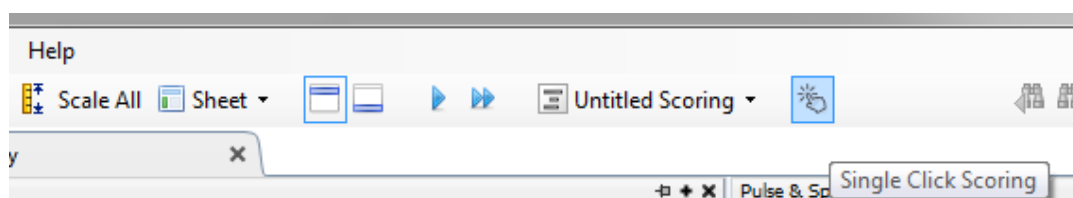

Within the applicable signal sheet manually score an event on the relevant signal trace, for instructions on how to manually score an event refer to the *Scoring an Event* section above. When you have scored the first event the single click scoring feature will enable you to continue scoring the same event type with only single mouse click as you browse through the recording.

## Deleting an Event

---

There are several ways to delete existing events:

- Select an event by left-clicking it and then press the **Delete** key.
- Right-click on an event and select **Remove Event**.
- Select an area with the mouse that intersects with the events to delete and press the **Delete** key.

## Moving an Event

---

To move an event to a different location, select the event by holding down the left mouse button and then drag the event to the desired location. Events can be dragged between signals as well as to a different time period.

## Resizing an Event

---

To resize an event, move the mouse cursor over the left or right boundary of an event. The mouse cursor should change to an icon of an arrow pointing right and left. Once the icon has changed to an arrow, left-click and drag the event to the desired duration.

## Navigating Events

---


There are several ways to navigate scored events in the recording:

- Jump between the events that have been scored on a signal by clicking on the signal and pressing the **Tab** key which jumps to the next event in time. To jump to the previous event in time press the **Shift + Tab** key.
- In the top right corner of the workspace there is a search text box which allows you to search for any events that have been scored. Clicking on the textbox shows a dropdown list of all event types that have been scored. To search for events of some type click on the event type in the list. This shows the next event in time with that type. Click on the navigation buttons in the drop-down list to navigate the events.
- Select **View > Event Overview** from the Noxturnal toolbar to bring up an overview window that shows all the events in a plot that have been scored in the recording. To navigate to a specific event, click on it in the overview plot.


## Analysis Protocols

An **Analysis Protocol** is a set of detectors that can be run on the recording to detect and mark various events within the recorded signals. The available analysis protocols, including the default protocols, are listed under the **Analysis** menu. To run an analysis protocol on the recording, select the applicable analysis from the **Analysis** menu and click on it.

Noxturnal offers a range of default analysis protocols and you can also create a new analysis protocol which uses customized settings and/or detectors. To setup a customized analysis protocol go to **Analysis > Manage Protocols** from the Noxturnal toolbar. You can **Edit** and **Rename** an existing protocol or create a **New based on** an existing protocol.

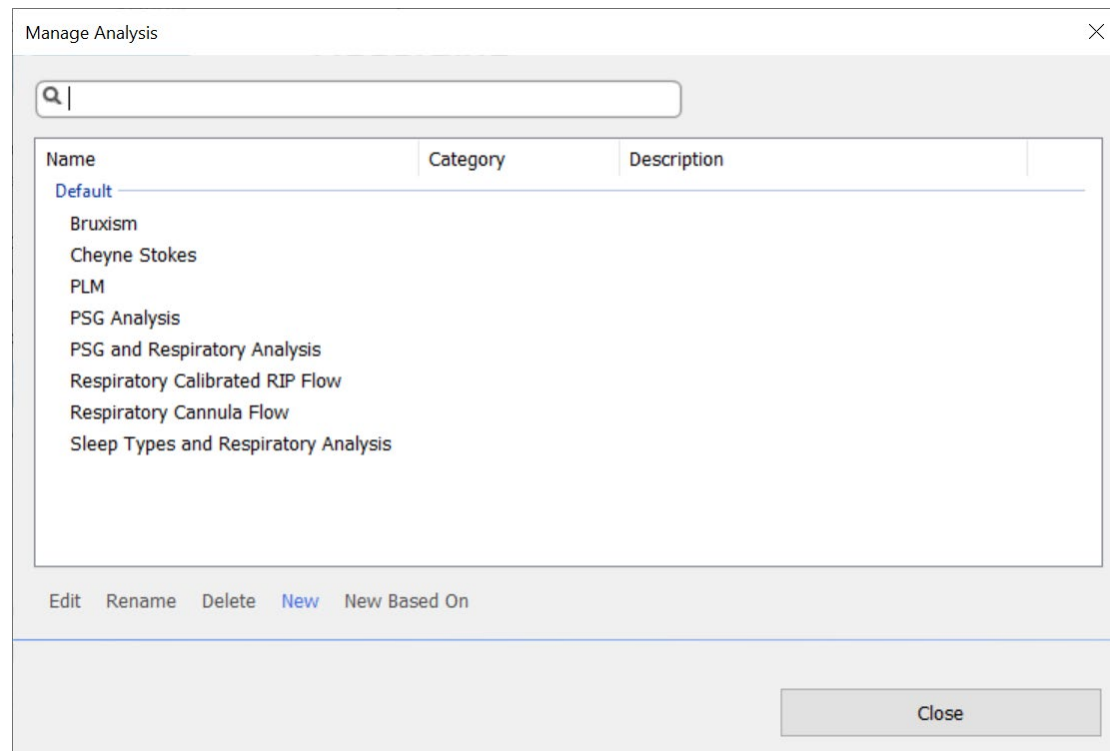

For this example, we will create a new analysis protocol. Select **New** in the **Manage Analysis dialog**. A new **Analysis Protocol** sheet will open up where the new protocol can be defined. A protocol is a collection of detectors and the function of a detector is to locate areas of interest within a signal and score the areas with events.

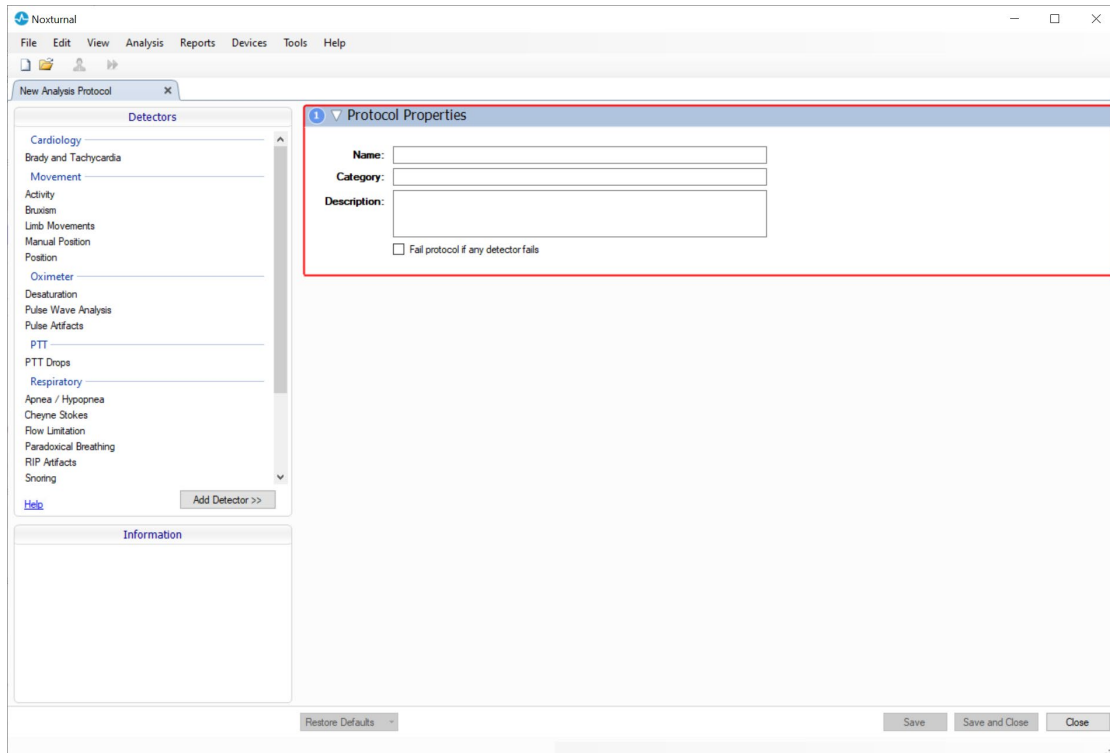


To add a detector to the protocol, choose detector from list of **Detectors** and select **Add Detector >>** **General Properties** and the **Input Signal** can be edited.


When you have setup your analysis protocol click **Save and Close** and the protocol will be added to the list of available analysis.

## Working with Scorings

A scoring is a collection of events that are scored on signals in the recording. The actions for working with scorings are located in the **Scoring Button** in the Noxturnal toolbar. The actions taken while working with scorings are listed in the sections below.

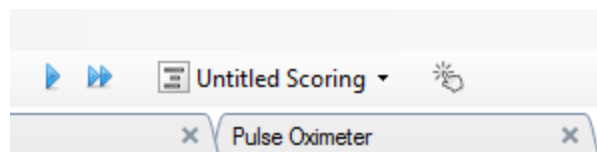

If you have included an **Analysis protocol** in the **Recording Type** configured for the recording then when downloading from a Nox recording device, Noxturnal automatically uses the default analysis protocol to analyze the recording. For online studies you need to close down the recording when completed and when reopened from the recording library the defined default analysis will analyze the data. The automatic analyzing of the data creates a new scoring called **Untitled Scoring**, see screenshot above. In the **Scoring Button** you always see the **Selected Scoring** which is used for the reporting and recording overview features. You may easily create new scorings by using the features of the **Scoring Button**, for example if you make modifications to the automatic scoring, you can easily save that as a new scoring with the applicable name.

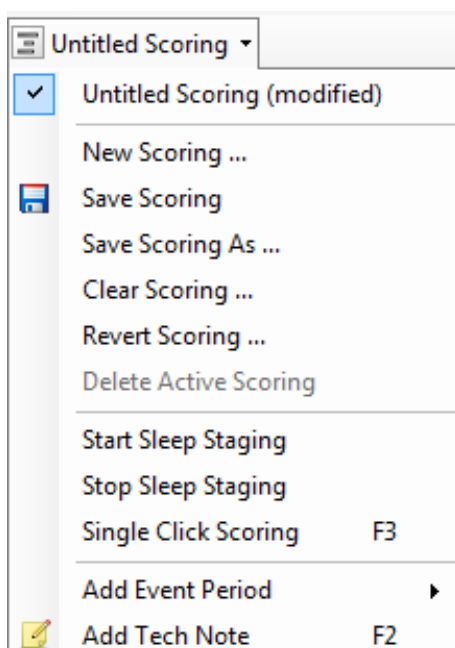


From the **Scoring Button** you can also **Add Event Period** or **Add Tech Note** to the recording.

## New Scoring

---

When using devices that record EEG, you can use the sleep staging features of Noxturnal. Noxturnal offers an automatic sleep stager with the system to assist the manual scorer. Also, a manual sleep staging without using the automatic sleep stager first, is possible.

To perform manual sleep staging click the **Scoring Button** and select a **New Scoring**.

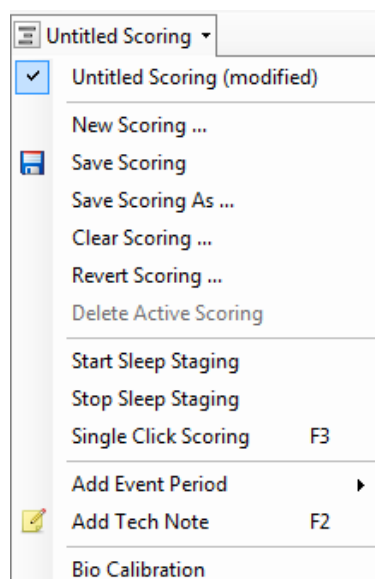

After that, to start sleep staging you can select the **Start Sleep Staging** action from the menu in the **Scoring Button**. The number pad on your keyboard is used for the default sleep staging hotkeys. You can change the scoring hotkeys as explained below.

The **Scoring Button** is also where you can start your **Bio Calibration**.

## Select a Scoring

---

Multiple scorings can be associated with a single recording. All available scorings are listed in the scorings panel. Select the active scoring by clicking on it.

## Save Scoring

---

Save the active scoring by clicking on the **Save Scoring** option. The user will be prompted for a name for the saved scoring. The saved scoring will be added to the list of scorings.

## Clear Scoring

---

If a scoring is active, this action will clear it. If the active scoring has local modifications, the user will be prompted on whether he wants to save his local modifications.

## Revert Scoring

---

If a scoring has local, unsaved modifications, these modifications can be reverted. This means that the scoring will be returned to the state it was in when it was loaded.

## Delete Selected Scoring

---

A saved scoring can be deleted by selecting it from the scoring list and clicking on the **Delete Selected Scoring** option. A prompt will come up, asking whether it is OK to delete the scoring.

## Scoring Keyboard Shortcuts

---

A shortcut key is used to score events quickly. Shortcut key can be assigned to an event type from **Setting -> Event Types & Groups -> Edit -> Behavior**.

As a general rule events should only have a single keyboard character as a shortcut, but a combination of **Ctrl**, **Shift** and **Alt** plus a keyboard character is supported.

## Noxturnal Reports




- ▶ Note: Report results are fixed and are not updated when the analysis of the recording changes.
- ▶ Note: If changes are made to the analysis another report can be generated or the existing report refreshed.

Noxturnal offers a range of default reports that can be accessed by clicking the **Reports** menu from the Noxturnal toolbar.

## Generating Reports

Report can be generated by clicking the View Report button on the Recording Results page or choose a report from the Reports menu in Noxturnal toolbar.

When you have generated a report in the report system, you can easily modify the report by using the **Edit** button which is visible in the toolbar when viewing reports.




The Edit button launches the **Edit Mode** which allows you to edit the report in the same way as you would use Microsoft Word®. All changes that you make are immediately visible to you. You can also add new indices and even pre-defined report parts when interpreting a study. To stop **Edit Mode**, press the **Edit** button again. Changes that are made in the **Edit** mode are not saved as part of the report template.


## Customizing Reports

Noxturnal offers a powerful custom report system that includes Microsoft Word® like editing capabilities. Reports in Noxturnal can easily be customized. To create a custom report template, follow the steps below.

1. From the Noxturnal Toolbar select **Reports -> Manage Reports...**
2. In the Manage Reports dialog select one of the options **Edit**, **New** or **New Based On** depending on your preferences.

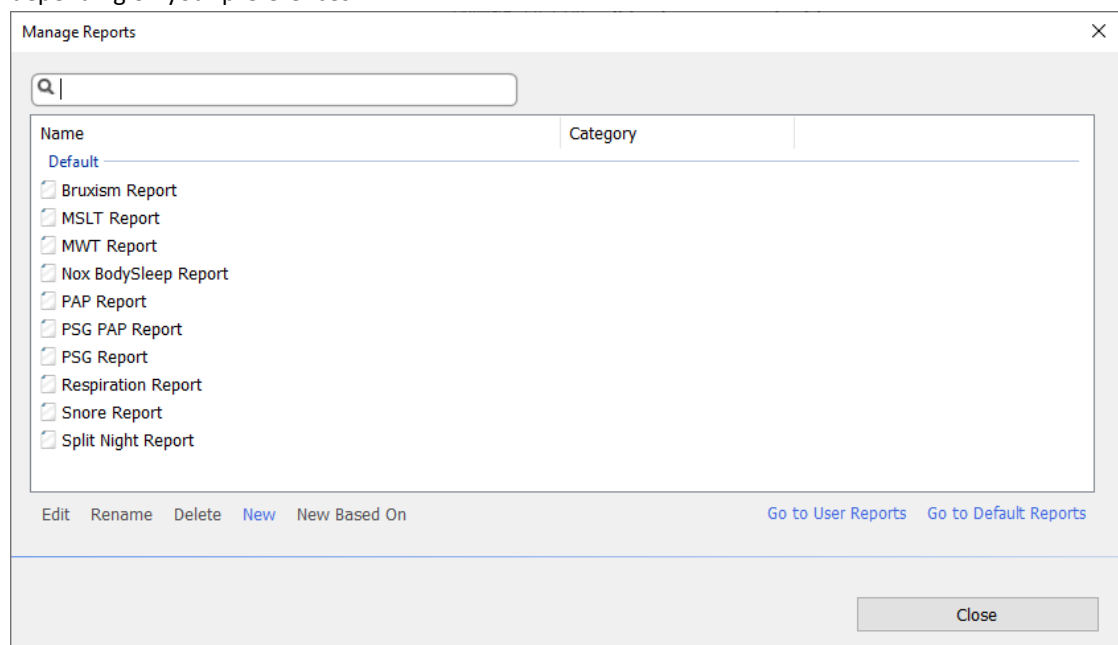

3. For this example, we will create a new custom report based on the default **PSG Report**. Select the **PSG Report** from the list of available reports and click **New Based On**.
4. You will see the following dialog where you can give the new report template a name and then select **Create**.

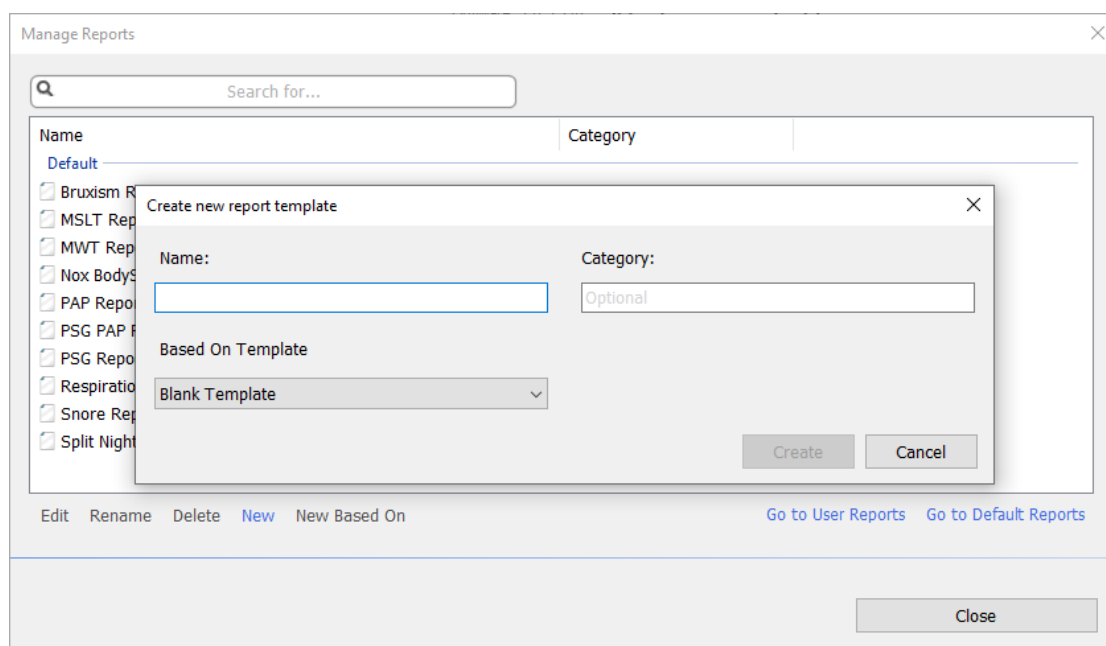

A new sheet opens up with the default chosen report and in this window you can edit it. On the right side of the screen you can find a collection of **Fields** and **Report Parts** that you can use for your report. For further information on Report Parts and Fields refer to the *Report*

Parts and Report Fields section below.

**PSG Report**

|                            |               |               |
|----------------------------|---------------|---------------|
| <b>Patient Information</b> |               |               |
| Full Name: -               | Patient ID: - | Patient ID: - |
| Height: -                  | Weight: -     | BMI: -        |
| Date of Birth: -           | Age: -        | Gender: -     |

|                              |                                     |
|------------------------------|-------------------------------------|
| <b>Recording Information</b> |                                     |
| Recording Date: -            | Analysis Duration (TRT): - m        |
| Recording Tags: -            | Analysis Start Time (Lights out): - |
| Device Type: -               | Analysis Stop Time (Lights on): -   |

|                                          |                         |
|------------------------------------------|-------------------------|
| <b>Summary</b>                           |                         |
| Total Sleep Time (TST): - m              | Sleep Latency (SL): - m |
| Sleep Efficiency (TST/TRT*100): - %      | REM Latency: - m        |
| Wake After Sleep Onset (TRT-SL-TST): - m |                         |

AHI: Color Coded AHI ODI: Color Coded ODI Snore %: Color Coded Snoring Label Index PLMS Index: Color Coded PLMS Index

|                             |            |          |
|-----------------------------|------------|----------|
| <b>Sleep Parameters</b>     |            |          |
| Sleep Stages Doughnut Chart |            |          |
|                             | Percentage | Duration |
| REM:                        | - %        | - m      |
| N1:                         | - %        | - m      |
| N2:                         | - %        | - m      |
| N3:                         | - %        | - m      |

**Fields Report Parts**

Field

- Arousals
- All Arousals Count TST
- All Arousals Count Wake
- All Arousals Index TST
- Arousal Count Non-Supine TST
- Arousal Count REM TST
- Arousal Count Supine TST
- Arousal Count TST
- Arousal Count Wake
- Arousal Index Non-Supine TST
- Arousal Index REM TST
- Arousal Index Supine TST
- Arousal Index TST
- Bruxism Arousal Count REM TST
- Bruxism Arousal Count Supine TST
- Bruxism Arousal Count TST
- Bruxism Arousal Count Wake
- Bruxism Arousal Index REM TST
- Bruxism Arousal Index Supine TST
- Bruxism Arousal Index TST
- LM Arousal Count Non-Supine TST
- LM Arousal Count REM TST
- LM Arousal Count Supine TST
- LM Arousal Count TST
- LM Arousal Count Wake
- LM Arousal Index Non-Supine TST
- LM Arousal Index REM TST
- LM Arousal Index Supine TST
- LM Arousal Index TST
- LM Arousal Index Wake

Description

New Based On Edit New Delete

Note: In the report template you can hover over the fields (-) with the mouse to see the parameter's details. See figure below.

|                                          |                         |
|------------------------------------------|-------------------------|
| <b>Summary</b>                           |                         |
| Total Sleep Time (TST): - m              | Sleep Latency (SL): - m |
| Sleep Efficiency (TST/TRT*100): - %      | REM Latency: - m        |
| Wake After Sleep Onset (TRT-SL-TST): - m |                         |

REM Latency  
Duration to the first REM events in Analysis in minutes


## REPORT PARTS AND REPORT FIELDS

Each report part represents a section of your report such as Oximetry Saturation, PLM Details etc. Report parts and fields can be created in Noxturnal and you can save report parts from default reports to have available when creating reports from scratch.

## CREATE A NEW REPORT PARTS

You can create new report parts and save for later use. To do that select the applicable report part in the report template (or any custom created text/table) and drag and drop it to the list of **Report**

**Parts.** Give the report part a name and select the category. The new report part you created will be added to the list of **Report Parts**.

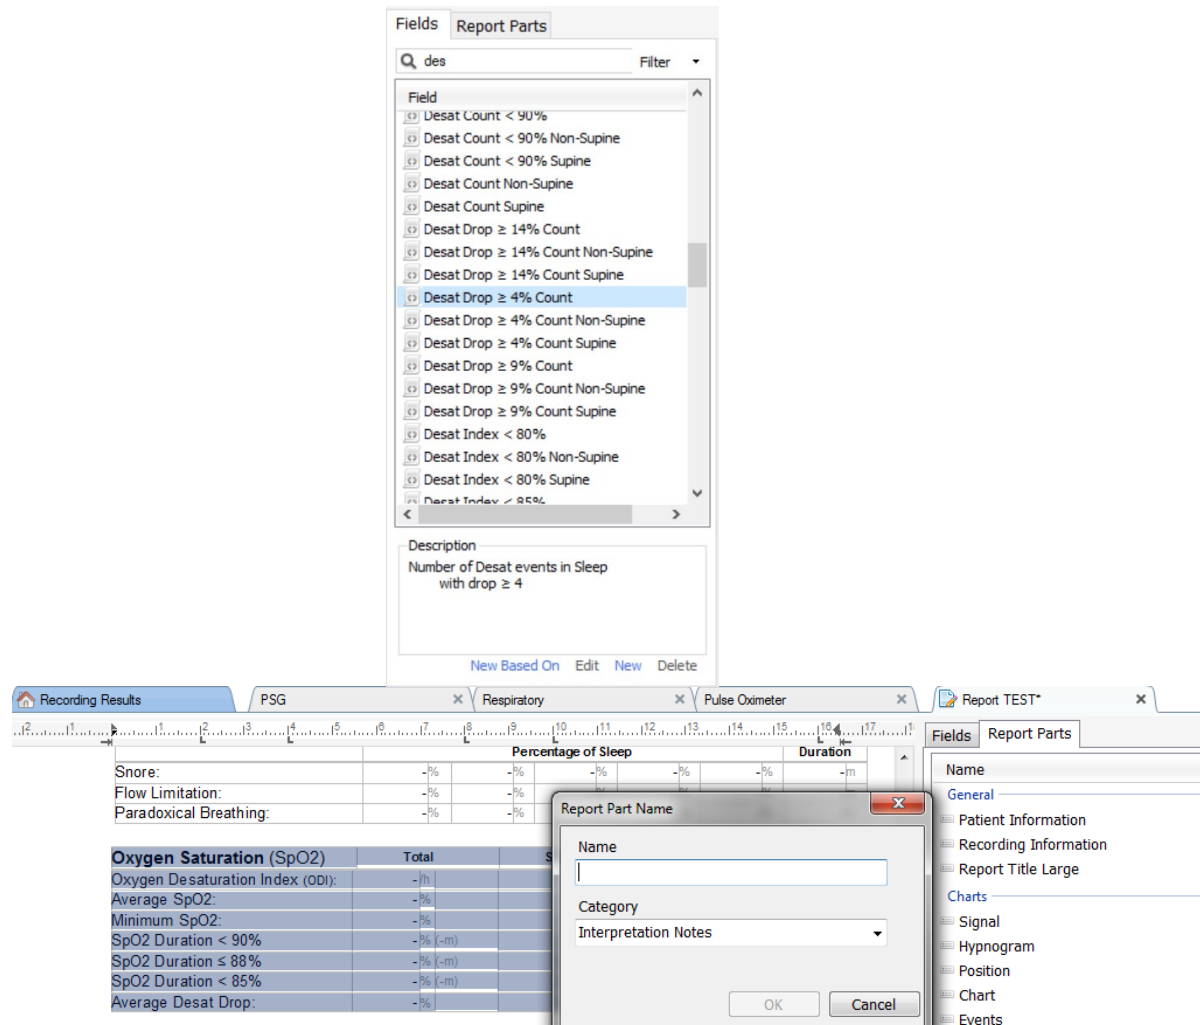

## CREATE A NEW REPORT FIELD

You can create new report fields and save for later use. To do that follow the steps below.

1. For this example, we will select the default field available in Noxturnal **Desat Drop ≥ 4% Count** as a base for our custom field. Select the **Desat Drop ≥ 4% Count** and click **New Based On**.

2. In the Edit Report Field dialog give the new field a name and edit the properties of the new field as required.

Name:

Category: Oximetry

Number of events ▼

Number of [Desat](#) events in [Sleep](#) with drop ≥ [3](#)

An example of this type of field is the number of Desats

Conditions

```
stats(named:Sleep).AsReference().Markers[Types(MarkerType:oxygensaturation-drop), Epoch:PeakToPeak:GreaterOrEqual(3)].Periods.Count
```

Save Cancel

For this example, we will change the desaturation drop to  $\geq 3$  and give the new field a descriptive name **Desat Drop  $\geq 3\%$  Count**. If the conditions are to be changed click **Conditions** to see all available conditions.

## ADD REPORT PARTS AND FIELDS TO REPORTS

To add **Report Parts** and **Fields** to your report set the mouse point to the preferred location in the report and double-click the desired report part from the list on the right side. Another way to add a Report Part and Field to a report is to drag and drop the desired report part/field into your report.

## REPORT HEADER AND FOOTER

To customize the report header and footer follow the steps below.

1. From the Noxturnal toolbar select **Tools -> Settings -> User & Company** and you will see the following wizard where you can enter user and company information.

**User & Company**

**User Information**

User name, initials and email address are used to personalize reports and the user interface.

Name:  Initials:

E-Mail:

**Company Information**

The company information is used in reports and in the user interface.

Name:  Web Site:


Address:  E-Mail:

OK Cancel


Analysis Console | Bookmark | 5.6.2014 01:36:19 | 5h 1m 24s | Whole Recording | Data

Fill in the fields shown above the applicable information. You can insert the information entered into your report using the corresponding Report Fields.

- To insert the information into the header/footer of your report place the mouse pointer within the upper part of the report, **right click** and select the option to **Edit Header/Footer**.

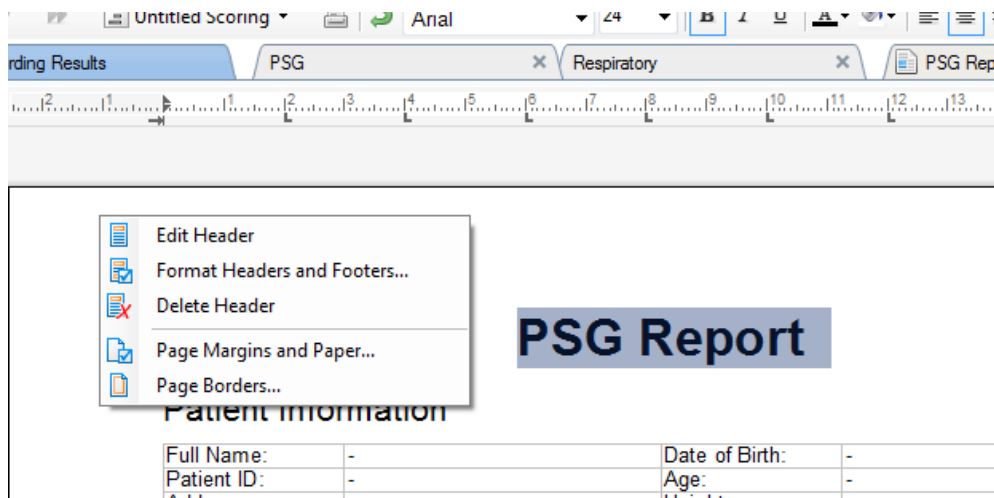

- Add the applicable fields from the list of available fields into the header section.
- To add logo to your report header, click **Format -> Insert Image...** as shown below.

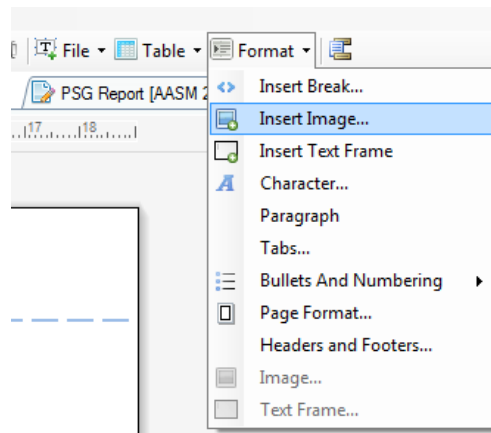


5. To add a page numbering to your report, go the bottom of the report page **right click** and select **Edit Footer**. **Right click** within the **footer** area and select **Insert > Page Number**.

When you have completed setting up your report template select **Save**. Your report will be added to the **Report** list available from the Noxturnal toolbar.

## Exporting Reports


To export a report, click **Export** from the report toolbar.



This will open a new dialog to specify the file format and the file name. Click the **Save** button when done and the report will be saved to the disk in the specified file format.

## Printing Reports

After a report has been generated the user can print the report. To print a report, select the **Print** option from the report toolbar.



A dialog will open where the printing options can be changed. Click the **Print** button to print.

## The Recording Library

The recording library shows and manages all the recordings that have been downloaded from the Nox recording devices and online studies. When recordings are opened or downloaded in Noxturnal they are automatically added to the recording library. It is also possible to acquire licenses to open EDF files, EDF+ files, Embla files and Somnostar files in Noxturnal, and the corresponding recordings will be added automatically to the recording library.

To open a recording, select it from the recording library list and double-click.

## Archiving Recordings

---

Recordings in the recording library can be archived to a different location or to a permanent storage. To archive a recording select one or more recordings in the library and click on the **Archive Recording...** button on the recording information panel. A dialog will appear guiding the user through the archiving process.

## Single Body Source

The Single Body Source algorithm is a patent pending algorithm in Noxturnal that determines if the same subject wore the recording device and the associated sensors during the recording period.

The algorithm can return one of three results. The results and their meanings are listed below.

- **Not analyzed:** The algorithm has not been run for the recording.
- **Approved:** A single body source can be verified for the recording.
- **Inconclusive:** A single body source cannot be verified for the recording.

A variety of factors can result in an **Inconclusive** result, including the following:

- The recording does not contain the necessary signals (a pulse waveform signal from the oximeter and at least one RIP signal)
- The necessary signals are noisy or include prominent artifacts
- The sensors were not placed on the subject
- The sensors were placed incorrectly on the patient or were displaced during sleep
- The oximeter and the RIP belts were worn by separate subjects
- The recording is too short (at least 15 minutes of concurrently recorded pulse waveform and RIP signals are necessary)
- The cardiac artifact in the RIP signals (caused by the emission of blood from the heart to the arteries and the resulting torso movement) is too small

The Single Body Source algorithm can be run either as a tool (by clicking **Tools -> Single Body Source**) or as an analysis detector, which can be included in a custom analysis protocol. The tool is run automatically after recordings are downloaded from a recording device.

The Single Body Source result is displayed on the **Recording Results** page under the **Signal Overview** section for each night and is also available as a report field for inclusion in custom reports. The result is indicated with one of the following symbols:

### Not analyzed



A grey circle

### Approved



A white check mark on a green circle

### Inconclusive



A white question mark on a  
yellow circle

The automatic calculation of the Single Body Source algorithm for downloaded recordings and display of the Single Body Source result can be turned on and off in **Tools -> Settings... -> Advanced -> Single Body Source**.

## Compatible Devices

The following table lists Ethernet supported devices and switches that have been validated with the Nox Sleep Assessment Systems. Noxturnal can receive, synchronize, display, and store signals from Ethernet supported devices when they are connected to the same network.

### SWITCHES, IP CAMERAS AND MICROPHONES

| Type                                 | Catalog Number |
|--------------------------------------|----------------|
| Trendnet PoE Switch                  | NA             |
| Axis T8351, microphone 3.5 mm        | NA             |
| Axis P3374, internet protocol camera | NA             |

### AUXILIARY DEVICES SUPPORTED

| Type               | Catalog Number |
|--------------------|----------------|
| SenTec SDM         | NA             |
| Resmed TxLink      | NA             |
| Resmed Airsense™10 | NA             |
| Resmed S9™         | NA             |
| Resmed Aircurve    | NA             |

Regulatory Information

Performance Testing and Validation Summary

The Nox Sleep Assessment Systems have been tested and verified in various phases to include internal testing, verification, and validation as well as external testing to assure product safety, effectiveness, and reliability. The design was verified and validated, including clinical evaluation, throughout the design process, according to requirement specifications and intended use.

Nox Medical holds an ISO 13485:2016 (MDSAP) certified Quality Management System which complies with the requirements of the Medical Device Directive (MDD - Council Directive 93/42/EEC as amended by Directive 2007/47/EC); Canada – Medical Devices Regulations – Part 1 – SOR 98/282; Australia – Therapeutic Goods (Medical Devices) Regulations, 2002, Schedule 3 Part 1 (excluding Part 1.6) – Full Quality Assurance Procedure; Japan – MHLW Ministerial Ordinance 169, Article 4 to Article 68; PMD Act and USA – 21 CFR 820, 21 CFR 803, 21 CFR 806, 21 CFR 807 – Subparts A to D.

Description of Symbols and Abbreviations

|                                                                                     |                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                               |
|-------------------------------------------------------------------------------------|---------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------|
| PG                                                                                  | ▶ Polygraphy                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                  |
| PSG                                                                                 | ▶ Polysomnography                                                                                                                                                                                                                                                                                                                                                                                                                                                                                             |
| CE2797                                                                              | ▶ CE marking indicating conformance to the applicable EU regulations.                                                                                                                                                                                                                                                                                                                                                                                                                                         |
| (01)15694311110255(8012)VVvvr<br>r(11)YYMMDD(10)ZZZZZZ                              | ▶ Unique Device Identifier (UDI): the Application Identifier (01) indicates the device identifier (DI) (i.e. “15694311110255”), the Application Identifier (8012) indicates the software version (i.e. “VVvvr”), the Application Identifier (11) indicates the production date/date of manufacture (i.e. “YYMMDD”, with “YY” the last two digits of the production year, “MM” the production month and “DD” the production day), and the Application Identifier (10) indicates the lot number (i.e. “ZZZZZZ”) |
|  | ▶ Unique Device Identifier (UDI) presented in data matrix format on Noxturnal CD                                                                                                                                                                                                                                                                                                                                                                                                                              |
|  | ▶ Manufacturer information                                                                                                                                                                                                                                                                                                                                                                                                                                                                                    |
|  | ▶ Date of manufacture                                                                                                                                                                                                                                                                                                                                                                                                                                                                                         |
|  | ▶ Batch code / Lot number                                                                                                                                                                                                                                                                                                                                                                                                                                                                                     |

**REF**

▶ Catalogue number / Reference number

## About

This manual and associated translations are provided in electronic format according to Commission Regulation (EU) No 207/2012 of 9 March 2012 on electronic instructions for use of medical devices. They are also available in electronic format on Nox Medical's website: [www.noxmedical.com](http://www.noxmedical.com).

Electronic versions are provided as PDF documents and a PDF reader is required to open the documents. PDF readers are commonly available at no cost for users. Refer to the applicable system and hardware requirements for the PDF reader that is used.

Hard copies can be requested at no additional cost by emailing [support@noxmedical.com](mailto:support@noxmedical.com). The hard copy will be sent within 7 calendar days.

## Appendix

### Default Derived Signals

Noxturnal calculates default derived signals from the recorded source signals. Derived signals are statistical or direct transforms of any given signal and are described in the table below.

| Derived Signal          | Source Signal              | Description                                                                                                                                                                                                                                                                                                                                                                                                                                                                         |
|-------------------------|----------------------------|-------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------|
| Activity                | Gravity X and Gravity Y    | Indication on patient activity/movements. The Activity signal is calculated from raw gravity signals (X and Y axis) measured by 3-dimensional accelerometer in the Nox recorders. The measured gravity signal is differentiated with respect to time and scaled by the correct scaling factor to create the derived activity signal.                                                                                                                                                |
| Audio Volume [dB]       | Audio Volume               | An Audio Volume signal in logarithmic scale (with units of decibels) is automatically calculated from the raw Audio Volume signal, which is in linear scale. The transform used to calculate the signal is $V_{dB} = 20 \log(x/P_0)$ , where $V_{dB}$ is the volume in decibels, $P$ is the raw audio volume signal (which is a pressure signal with units of Pa) and $P_0$ is the reference sound pressure, which has a value of $P_0 = 20 \text{ uPa}$ in the Noxturnal software. |
| Calibrated RIP Abdomen  | RIP Abdomen                | The Calibrated RIP Abdomen Signal is calculated by scaling each value of the RIP Abdomen signal with the corresponding RIP K signal (derived signal). The flow signal will be automatically created if both: RIP Abdomen and RIP K signal exist.                                                                                                                                                                                                                                    |
| Calibrated RIP Flow     | RIP Thorax                 | The calibrated RIP flow is calculated from a derivative of the sum of the RIP Thorax and calibrated RIP Abdomen signals (derived) and has the unit [V/s].                                                                                                                                                                                                                                                                                                                           |
| Calibrated RIP Sum      | RIP Abdomen and RIP Thorax | The Calibrated RIP Sum signal is calculated by adding the RIP Thorax signal with the RIP Abdomen signal after the latter has been scaled with the RIP K signal.                                                                                                                                                                                                                                                                                                                     |
| Cannula Flow            | Cannula Pressure           | The Cannula Flow signal is a qualitative signal derived from the raw nasal Cannula Pressure signal and has the unit [cmH <sub>2</sub> O]. The nasal Cannula Pressure signal is low-pass filtered at 3 Hz and then the cannula flow signal is derived from a non-linear transformation.                                                                                                                                                                                              |
| Cannula Snore           | Cannula Pressure           | The snoring signal (Cannula Snore) is derived by high-pass filtering a raw nasal Cannula Pressure or airflow signal.                                                                                                                                                                                                                                                                                                                                                                |
| Cheyne Stokes breathing | Cannula Pressure           | The Cheyne Stokes Breathing signal is derived by using a mathematical formula to detect the form of the inhalation and exhalation.                                                                                                                                                                                                                                                                                                                                                  |
| Flow Limitation         | Cannula Pressure           | The Flow Limitation signal is derived by using a mathematical formula for calculating the flatness of an inhalation.                                                                                                                                                                                                                                                                                                                                                                |

| Derived Signal         | Source Signal              | Description                                                                                                                                                                                                                                                                                                                                                               |
|------------------------|----------------------------|---------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------|
| Heart Rate             | ECG                        | An R wave detection algorithm is run to detect each heart beat in the ECG signal. The instantaneous heart rate is the reciprocal of the intervals between successive heart beats. The heart rate signal has the unit [bpm] (beats per minute).                                                                                                                            |
| Position               | Gravity X and Gravity Y    | Indication of patient posture to discriminate between upright, supine, prone, left, and right position. The Position signal is created from Gravity X and Gravity Y and is the angle of the rotation of the body. It ranges from -180° to 180° and is 0° if the patient is facing directly upwards.                                                                       |
| Pulse Wave Amplitude   | Plethysmograph             | Pulse Waveform Amplitude (PWA) is a signal that shows the peak to peak value of a pulse waveform (the photoplethysmography signal from the oximeter) using a sample and hold method for the duration of the wave. The unit is [k].                                                                                                                                        |
| RIP Sum                | RIP Abdomen and RIP Thorax | The RIP Sum [V] is calculated as the sum of the RIP Abdomen and RIP Thorax signals.                                                                                                                                                                                                                                                                                       |
| RIP Flow               | RIP Abdomen and RIP Thorax | The belt flow is calculated from a derivative of the sum of the RIP Abdomen and RIP Thorax signals and has the unit [V/s].                                                                                                                                                                                                                                                |
| RIP K                  | RIP Abdomen and RIP Thorax | To get a more accurate estimate of the actual respiratory flow from the RIP Abdomen and Thorax signals, the RIP Abdomen signal needs to be scaled using a calibration factor. This calibration factor is stored as the derived signal K. The K is found by seeking the optimal value giving the best correlation between the derived RIP flow and a reference pneumoflow. |
| RIP Phase              | RIP Abdomen and RIP Thorax | The phase difference between the RIP Abdomen and RIP Thorax belts. The phase signal ranges from 0-180°. The RIP Phase is shown as a signal synchronized with RIP Abdomen and RIP Thorax belts.                                                                                                                                                                            |
| Reference EEG          | EEG Signals                | The reference EEG signal is an average of two or more EEG input signals.                                                                                                                                                                                                                                                                                                  |
| Respiratory Rate       | RIP Abdomen and RIP Thorax | The respiratory rate signal is derived from the RIP Sum signal (derived signal). The respiratory rate is displayed as respirations per minute or [rpm].                                                                                                                                                                                                                   |
| Set Pressure           | Mask Pressure              | The Set Pressure signal is created from the Mask Pressure signal. It shows the most common Mask Pressure over a 5 second interval.                                                                                                                                                                                                                                        |
| TcCO <sub>2</sub> [Pa] | TcCO <sub>2</sub>          | The signal received from a transcutaneous CO <sub>2</sub> device has the unit [torr]. The new TcCO <sub>2</sub> signal which has the unit [Pa] is calculated, using the scaling factor 133.3 Pa/torr.                                                                                                                                                                     |

## Automatic Analysis Overview

Clinical performance testing was conducted for the automatic analysis implemented in Noxturnal to demonstrate safety and effectiveness. The clinical performance testing consisted of retrospectively analyzing pre-existing clinical data from sleep studies that had already been collected and manually scored as part of routine clinical care. All scorers were qualified polysomnographic technologists and followed the American Academy of Sleep Medicine (AASM) scoring guidelines. The study protocol consisted of exporting the reported indices/events from the pre-existing manual scoring and then running the automatic analysis in Noxturnal on the same clinical data. The results of the automatic scoring were exported and compared to the results of the manually scored data. The overall conclusion of the clinical performance testing is that the Noxturnal's automatic analysis tools are found to be acceptable as a scoring aid in the clinical routine for the clinical purpose as specified for each analysis in the table below.

The table below lists the automatic analysis implemented in Noxturnal, gives a short overview how the algorithm works, what signals are analyzed, describes the criteria used for scoring, and what indices/event/parameters are calculated/scored.

Furthermore, the table includes information on the clinical purposes and limitations, the clinical conditions being analyzed, safety endpoints specified for each analysis and the type of clinical data sets used for validation.

| Name, Purpose, Indices, Events                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                   | Clinical Condition                                                                                                                                                                                    | Overview                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                    |
|------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------|-------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------|-----------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------|
| <p><b><u>Bruxism Analysis</u></b></p> <p>The <u>clinical purpose</u> is to improve the efficiency of scoring EMG data that is consistent with potential bruxism-related events by labeling mandibular movements as measured by masseter EMG for review and confirmation by a trained healthcare professional.</p> <p><u>Limitations:</u> The analysis is known to overestimate the number of bruxism events and on average 42% of automatically scored events may have to be removed manually. The automatic analysis results should always be reviewed by a</p> | <p>Jaw contractions during sleep. Jaw contractions (possible bruxism-related events) are classified either as tonic (sustained clenching contractions) or phasic (repetitive brief contractions).</p> | <p>The algorithm uses a masseter EMG signal and the activity signal. Periods of temporarily increased masseter muscle activity are found and scored as bursts. If the scored bursts fit the pattern of tonic or phasic bruxism episodes they are scored as such as defined by the AASM guidelines. By default, bruxism episodes are disregarded if they occur concurrently with patient movement, which is characterized by an increase in the activity signal.</p> <p><u>Clinical data set:</u> The automatic analysis was validated on clinical sleep recordings from an adult general population seeking medical attention with regards to their sleep disorders. The sleep recordings were scored by a certified technician as a part of standard clinical routine.</p> |

| Name, Purpose, Indices, Events                                                                                                                                                                                                                                                                                                                                                                                                                                                                            | Clinical Condition                                                                                                                                                                                                                                                                                                                               | Overview                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                       |
|-----------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------|--------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------|--------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------|
| <p>certified technician or a physician prior to diagnosis.</p> <p><u>Index scored:</u> Bruxism Episode Index (BEI) - number of bruxism episodes per hour of sleep</p>                                                                                                                                                                                                                                                                                                                                     |                                                                                                                                                                                                                                                                                                                                                  | <p><u>Primary safety endpoint:</u> The analysis was considered to be safe if it detects at least 90% of oromandibular movements considered by a human expert to be bruxism events with 95% confidence.</p> <p><u>Result:</u> The sensitivity of the analysis was 95.7% (95% CI 93.2% - 97.4%), specificity was 61.0% (95% CI 58.9% - 63.0%), PPV was 34.6% (95% CI 32.0% - 37.3%), NPV was 98.5% (95% CI 97.7% - 99.1%).</p>                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                   |
| <p><b><u>PLM Analysis</u></b></p> <p>The <u>clinical purpose</u> is to improve the efficiency of scoring periodic limb movement events.</p> <p><u>Limitations:</u> The automatic analysis results should always be reviewed by a certified technician or a physician prior to diagnosis.</p> <p><u>Indices scored:</u></p> <p>Limb Movement Index (LMI) - number of limb movements per hour of sleep</p> <p>Periodic Limb Movement Index (PLMS) - number of periodic limb movements per hour of sleep</p> | <p><u>Limb Movements during sleep:</u> Periods, during sleep, lasting 0.5-10 seconds where the muscle tone in a limb, typically measured on the tibialis muscle, is increased from baseline.</p> <p><u>Periodic Limb Movements during sleep:</u> Period, during sleep, containing at least 4 limb movement events separated by 5-90 seconds.</p> | <p>The Limb Movement algorithm uses left leg and right leg EMG signals to identify periods where muscle tone is increased. Additionally, the activity signal is used to detect patient activity.</p> <p>The PLM analysis locates events of high muscular activity or kinetic activity and identifies as LM (limb movement) events. These are subsequently used to determine if any PLM (periodic limb movement) events are present. The analysis follows the guidelines set forth by the AASM.</p> <p><u>Clinical data set:</u> The automatic analysis was validated on clinical sleep recordings from an adult general population seeking medical attention with regards to their sleep disorders. The sleep recordings were scored by a certified technician as a part of standard clinical routine.</p> <p><u>Primary safety endpoint:</u> The analysis was determined to be safe based on the safety hypothesis of having all criteria below met for the PLMI index.</p> <ul style="list-style-type: none"> <li>• Interclass correlation (ICC) must exceed 0.61</li> </ul> |

| Name, Purpose, Indices, Events                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                            | Clinical Condition                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                       | Overview                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                     |
|---------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------|----------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------|------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------|
|                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                           |                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                          | <ul style="list-style-type: none"> <li>• Pearson correlation coefficient (PCC) must match or exceed <math>r = 0.65</math></li> <li>• The absolute bias must not exceed 5.7</li> </ul> <p><u>Result:</u> ICC is 0.98, Pearson correlation coefficient is 0.94 and absolute bias is 0.29 for the Periodic Limb Movement Index</p>                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                              |
| <p><b><u>Respiratory Flow Analysis (calibrated RIP, Cannula)</u></b><sup>1</sup></p> <p>1) The <u>clinical purpose</u> is to improve the efficiency of scoring Apneas, Hypopneas (using calibrated RIP, cannula) and desaturation events from oximeter.</p> <p><u>Limitations:</u> The results should always be reviewed by a certified technician or a physician prior to diagnosis.</p> <p><u>Indices scored:</u></p> <p>Apnea Hypopnea Index (AHI) - number of apneas and hypopneas per hour of sleep</p> <p>Apnea Index (AI) - number of apneas per hour of sleep</p> | <p><u>Apneas during sleep:</u><br/>Periods lasting 10 seconds or longer where a patient stops breathing.</p> <p><u>Hypopneas during sleep:</u><br/>Periods lasting 10 seconds or longer where a patient's breathing is severely reduced.</p> <p><u>Oxygen desaturation during sleep:</u> Periods where the oxygen saturation of a patient's arterial blood falls below the baseline by 3% or more.</p> <p><u>Central Apneas during sleep:</u> Periods lasting 10 seconds or longer where a patient stops breathing and respiratory effort is absent.</p> | <p>The <u>Apnea / Hypopnea (AHI) algorithm</u> uses as applicable the respiratory cannula flow or respiratory calibrated RIP flow signal depending on the analysis run and can utilize scored events in the EEG to score hypopneas. The scored EEG events are arousals during sleep scored manually. The algorithm also uses an SpO2 signal measured by an oximeter to find desaturation events which are used to score hypopneas, but the algorithm does not score the desaturation events.</p> <p>The AHI algorithm determines if a patient is breathing normally, if breathing is severely reduced resulting in a hypopnea, or if a patient is not breathing resulting in an apnea. If breathing is severely reduced the algorithm looks if there is an arousal or a drop-in blood oxygen saturation associated with the reduction in breathing to score an hypopnea.</p> |

<sup>1</sup> Includes AHI and ODI Algorithm and Apnea Classification Algorithm

| Name, Purpose, Indices, Events                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                              | Clinical Condition                                                                                                                                                                             | Overview                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                    |
|---------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------|------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------|-----------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------|
| <p>Hypopnea Index (HI) - number of hypopneas per hour of sleep</p> <p>Oxygen Desaturation Index (ODI) - number of oxygen desaturation events per hour of sleep.</p> <p>2) The <u>clinical purpose</u> is to improve the efficiency of classifying apneas into central apneas, mixed apneas or neither.</p> <p><u>Limitations:</u> The results should always be reviewed by a certified technician or a physician prior to diagnosis.</p> <p><u>Indices scored:</u></p> <p>Central Apnea Index (CAI) - number of central apneas and hypopneas per hour of sleep</p> <p>Mixed Apnea Index (MAI) - number of mixed apneas per hour of sleep</p> <p>Central Mixed Apnea Index (CMAI) - number of central and mixed apneas per hour of sleep</p> | <p><u>Mixed Apneas during sleep:</u> Periods lasting 10 seconds or longer where a patient stops breathing. Respiratory effort is absent at the start of the period but present at the end.</p> | <p>The <u>Desaturation (ODI) algorithm</u> uses an SpO2 signal measured by an oximeter to determine if there is a drop of 3% or more in blood oxygen saturation.</p> <p>The analyses follows the guidelines set forth by the AASM.</p> <p>The <u>Apnea Classification algorithm</u> uses a respiratory flow signal, with the addition of the abdomen and thoracic respiratory Inductance plethysmography (RIP) signals.</p> <p>The Apnea Classification algorithm classifies scored apneas as central or mixed if respiratory effort is absent during the apnea, or neither.</p> <p>The analysis follows the guidelines set forth by the AASM.</p> <p><u>Clinical data set:</u> The automatic analyses were validated on clinical sleep recordings from an adult general population seeking medical attention with regards to their sleep disorders. The sleep recordings were scored by a certified technician as part of standard clinical routine.</p> <p><u>Primary safety endpoints:</u> The automatic respiratory flow analysis was determined to be safe if it met the safety endpoint of having a 95% confidence in not classifying patients with an AHI below 5 as having an AHI greater than or equal to 15 or having a 95% confidence in not classifying patients with an AHI greater than or equal to 15 as having an AHI below 5.</p> <p>Two co-primary endpoints are used for AHI. Cohens Kappa to match or exceed 0.66 and Pearson correlation matches or exceeds <math>r = 0.96</math> for the cannula.</p> |

| Name, Purpose, Indices, Events                                                                                                                                                                                                                                                                                                                                                                                                                           | Clinical Condition                                                                                                                                                               | Overview                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                |
|----------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------|----------------------------------------------------------------------------------------------------------------------------------------------------------------------------------|---------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------|
|                                                                                                                                                                                                                                                                                                                                                                                                                                                          |                                                                                                                                                                                  | <p>Cohen's Kappa of 0.66 to be within the 95% confidence interval and Pearson correlation matches or exceeds <math>r=0.72</math> for the cRIP.</p> <p>The criteria for ODI is that Intra-Class Correlation (ICC) matches or exceeds 0.93</p> <p>The automatic apnea classification analysis was deemed to be safe if it met the acceptance criteria of an ICC comparable with what has been reported in scientific literature of Central Apnea Index (CAI 0.46).</p> <p><u>Result:</u> The analysis is safe since the odds of misclassifying between severity groups is less than the acceptable 5%. Cohens Kappa is 0.78 and Pearson's <math>r = 0.96</math> for the cannula. Cohen's Kappa is 0.62 (95% CI 0.56 – 0.66) and Pearson's <math>r = 0.79</math> for the cRIP. The ICC for ODI was 0.95. The ICC was 0.91 for the Central Apnea Index.</p> |
| <p><b><u>Sleep Staging Analysis</u></b></p> <p>The <u>clinical purpose</u> is to improve the efficiency of scoring sleep stages with the intent of estimating total sleep time.</p> <p><u>Limitations:</u> The automatic analysis results should always be reviewed by a certified technician or a physician prior to diagnosis.</p> <p><u>The following events are scored:</u> Sleep stage W (Wake), Stage N1, Stage N2, Stage N3 and Stage R (REM)</p> | <p>The pattern of sleep stages is used to analyze how the individual sleeps and <u>determine any abnormalities in the sleep profile that might indicate sleep disorders.</u></p> | <p>The algorithm uses electroencephalography (EEG) signals, electrooculogram (EOG) signals, activity signal and submental electromyography (EMG) signal to provide pre-scoring of sleep stages according to the AASM manual.</p> <p>The algorithm is implemented with an artificial neural network. Various features are calculated from the EEG, the EOG, the activity signal and the submental EMG and fed into the neural network, which returns sleep stages for 30 second epochs, to simulate the way sleep stages are scored by human scorers.</p> <p><u>Clinical data set:</u> The automatic analysis was validated on clinical sleep</p>                                                                                                                                                                                                        |

| Name, Purpose, Indices, Events                                                                                                                                                                                                                                                                                                                                                                                        | Clinical Condition                                                                                                                                                                                                                                                                                                                                               | Overview                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                     |
|-----------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------|------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------|------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------|
|                                                                                                                                                                                                                                                                                                                                                                                                                       |                                                                                                                                                                                                                                                                                                                                                                  | <p>recordings from an adult general population seeking medical attention with regards to their sleep disorders. The sleep recordings were scored by a certified technician as a part of standard clinical routine.</p> <p><u>Primary Safety endpoint:</u> The analysis was determined to be safe if it met the safety endpoint of having an average agreement of at least 60% when scoring wake epochs. Co-primary endpoint is that Cohen's kappa statistics matches or exceeds 0.63</p> <p><u>Results:</u> The Cohen's Kappa was calculated resulting in <math>\kappa=0.68</math>. The accuracy of predicting the sleep stages resulted in N1 (9.7%), N2 (86.7%), N3 (84.7%), Wake (66.7%), and REM (84.1%)</p>                                                             |
| <p><b><u>Arousal Analysis</u></b></p> <p>The <u>Clinical Purpose</u> is to improve the efficiency of arousal scoring with the intent of improving the scoring of hypopneas.</p> <p><u>Limitations:</u> The automatic analysis results should always be reviewed by a certified technician or a physician prior to diagnosis.</p> <p><u>The following events are scored:</u> Arousals detected in the EEG signals.</p> | <p><u>Arousals in sleep:</u></p> <p>Abrupt shift of EEG frequency that lasts 3 – 10 seconds after 10 seconds of stable sleep. Resulting arousal index is used to detect any abnormalities in the sleep profile that might indicate sleep disorders. Arousals are considered when detecting hypopneas and thus are related to the Apnea Hypopnea Index (AHI).</p> | <p>The algorithm uses electroencephalography (EEG) signals, electrooculogram (EOG) signals, activity signal and submental electromyography (EMG) signal to provide pre-scoring of arousals according to the AASM manual.</p> <p>The algorithm uses AdaBoost classifier, which returns arousal events if detected the way arousals are scored by human scorers.</p> <p><u>Primary Safety Endpoint:</u> The automatic arousal analysis was determined to be safe if the likelihood of misclassifying between healthy subjects (AHI &lt;5) and moderate to severe (AHI <math>\geq 15</math>) was less than 5%.</p> <p><u>Clinical Condition:</u> The automatic arousal analysis was validated on clinical sleep recordings from an adult general population seeking medical</p> |

| Name, Purpose, Indices, Events                                                                                                                                                                                                                                                                                                                                                                                                                               | Clinical Condition                                                                                                                                                                                                                          | Overview                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                 |
|--------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------|---------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------|--------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------|
|                                                                                                                                                                                                                                                                                                                                                                                                                                                              |                                                                                                                                                                                                                                             | <p>attention with regards to their sleep disorders. The sleep recordings were scored by a certified technician as a part of standard clinical routine.</p> <p><u>Results:</u> The automatic arousal scoring is effective since it is very unlikely to cause a patient to be misclassified from healthy (AHI &lt; 5) to sick (AHI ≥15) and vice versa. The analysis passed that criteria with a p-value &lt; 0.03 and is therefore considered safe and effective.</p>                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                     |
| <p><b>Nox BodySleep Analysis</b></p> <p>The <u>Clinical Purpose</u> is to get more accurate estimate of sleep time during a home sleep study by correctly classifying wake in a home sleep study.</p> <p><u>Limitations:</u> The automatic analysis results should always be reviewed by a certified technician or a physician prior to diagnosis.</p> <p><u>The following events are scored:</u> Sleep state Wake, Sleep state NREM and Sleep state REM</p> | <p>Sleep time is used as a metric when calculating AHI (Apnea-Hypopnea index) during sleep and can also be used to evaluated duration of sleep to determine any abnormalities in the sleep profile that might indicate sleep disorders.</p> | <p>The “Nox BodySleep” is an Artificial Intelligence (AI) method intended to classify 30-second epochs into the states of REM sleep, NREM sleep and Wake. It uses respiratory inductance plethysmography (RIP) signals and actigraphy to measure the impact of brain state change on the body and estimates sleep states from those signals.</p> <p>Body Sleep does not rely on electrooculogram (EOG), electromyogram (EMG), or electroencephalogram (EEG) signals typically used to determine sleep stages. Instead, it uses algorithms to interpret how the body reacts to changes in brain state. For instance, in the transition from wake to sleep, movement decreases, along with the heart rate, respiratory rate, blood oxygen levels and blood pressure. The autonomic nervous system is responsible for these changes. Using very sensitive detection of multiple physiological signals, we can use algorithms to interpret the autonomic changes in body functions that occur with brain state changes. Body Sleep algorithms were specifically designed</p> |

| Name, Purpose, Indices, Events | Clinical Condition | Overview                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                          |
|--------------------------------|--------------------|---------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------|
|                                |                    | <p>to reliably predict changes in autonomic function that correlate with Wake, REM and NREM sleep.</p> <p><u>Clinical Data Set:</u> A retrospective analysis of polysomnography data collected with the Nox Sleep System from patients undergoing a routine clinical sleep study in the case of suspected sleep disorders. The sleep recordings were scored by a certified technician as a part of standard clinical routine.</p> <p><u>Primary Safety Endpoints:</u> The primary endpoint chosen is the sensitivity to sleep state classification, resulting from the comparison of manual and automatic scorings by the analysis. The endpoint is considered successful if the sensitivity to the wake state is statistically significantly over 0.5.</p> <p>A secondary study endpoint is the agreement between manual scoring and automatic scoring as evaluated with Cohens Kappa (<math>\kappa</math>). The endpoint is considered successful if <math>\kappa &gt; 0.50</math></p> <p><u>Results:</u> The sensitivity to wake observed was 0.566 with a p-value of <math>1.1e-16</math>. The corresponding 95% confidence interval is (0.559, 0.574).</p> <p>The Cohens Kappa was 0.57.</p> <p>The results show that the analysis performance exceeds the safety and efficacy criteria.</p> |