

Thermo Scientific Pierce Protein Assay Technical Handbook

Version 2



Table of Contents

Total Protein Assays

Quick Technical Summaries 1

Introduction 4

Selection of the Protein Assay	4
Selection of a Protein Standard	5
Standard Preparation	6
Standards for Total Protein Assay	7
Compatible and Incompatible Substances	9
Compatible Substances Table	10
Time Considerations	12
Calculation of Results	12

Thermo Scientific Pierce 660nm Protein Assay 13

Overview	13
Highlights	13
Typical Response Curves	14

BCA-based Protein Assays 15

Chemistry of the BCA Protein Assay	15
Advantages of the BCA Protein Assay	16
Disadvantages of the BCA Protein Assay	17
BCA Protein Assay – Reducing Agent Compatible	18
BCA Protein Assay	19
Micro BCA Protein Assay	20

Coomassie Dye-based Protein Assays (Bradford Assays) 21

Chemistry of Coomassie-based Protein Assays	21
Advantages of Coomassie-based Protein Assays	21
Disadvantages of Coomassie-based Protein Assays	21
General Characteristics of Coomassie-based Protein Assays	22
Coomassie Plus (Bradford) Protein Assay	23
Coomassie (Bradford) Protein Assay	24

Removal of Interfering Substances 25

Thermo Scientific Compat-Able Protein Assays	26
--	----

Modified Lowry Protein Assay 27

Chemistry of the Modified Lowry Protein Assay	27
Advantages of the Modified Lowry Protein Assay	28
Disadvantages of the Modified Lowry Protein Assay	28
General Characteristics of the Modified Lowry Protein Assay	28
Modified Lowry Protein Assay Reagent	29

Amine Detection 30

OPA Fluorescent Protein Assay	30
Fluoraldehyde o-Phthalaldehyde	31

Specialty Assays

Histidine-tagged Proteins 32

Thermo Scientific HisProbe-HRP Kits	32
-------------------------------------	----

Antibodies 33

IgG and IgM Assays	33
--------------------	----

Proteases 35

Protease Assays	35
-----------------	----

Glycoproteins 36

Glycoprotein Carbohydrate Estimation Assay	36
--	----

Phosphoproteins 37

Phosphoprotein Phosphate Estimation Assay	37
---	----

Peroxides 38

Quantitative Peroxide Assay	38
-----------------------------	----

Spectrophotometers 39

BioMate 3S UV-Visible Spectrophotometer	39
Evolution 260 Bio UV-Visible Spectrophotometer	39
Evolution 300 UV-Visible Spectrophotometer	40
Evolution Array UV-Visible Spectrophotometer	40

Quick Technical Summaries – Thermo Scientific Protein Assays

Working Range (sample volume)*	Characteristics/Advantages	Applications	Disadvantages	Interfering Substances
Pierce® 660nm Protein Assay				
Standard Protocol: 25-2,000µg/mL (65µL)	Compatible with reducing agents, chelating agents and detergents	Ideal for measuring total protein concentration in samples containing both reducing agents and detergents	Use reagent with IDCR (Ionic Detergent Compatibility Reagent) with samples containing ionic detergents like SDS	High levels of ionic detergents require the addition of the Ionic Detergent Compatibility Reagent (IDCR).
Microplate Protocol: 50-2,000µg/mL (10µL)	Faster and easier to perform than BCA or Coomassie (Bradford) Assays Excellent linearity of color development within the detection range Less protein-to-protein variability than the Coomassie (Bradford) Assay Reaches a stable end point Compatible with Laemmli sample buffer containing bromophenol blue when using Compatibility Buffer	Used for quick, yet accurate estimation of protein	Greater protein-to-protein variability than the BCA Assay	
The BCA Protein Assay - Reducing Agent Compatible				
Standard Protocol: 125-2,000µg/mL (25µL)	Compatible with up to 5mM DTT, 35mM 2-Mercaptoethanol or 10mM TCEP	Allows the use of the superior BCA Assay in situations in which it is normally unable to be read	Requires heating for color development	Compatible with all reducing agents and detergents found at concentrations routinely used in protein sample buffers
Microplate Protocol: 125-2,000µg/mL (9µL)	No protein precipitation involved Sample volume only 9µL (microplate protocol) Compatible with most detergents Significantly less (14-23%) protein:protein variation than Bradford-based methods	No precipitation step means no worries about difficult-to-solubilize proteins		
The BCA Protein Assay				
Standard Protocol: 20-2,000µg/mL (50µL)	Two stable reagents used to make one working reagent	Adaptable for use with microplates	Not compatible with thiols/reducing agents	Reducing sugars and reducing agents
Enhanced Standard Protocol: 5-250µg/mL (50µL)	Working reagent stable for one week at room temperature Compatible with detergents	Determine the amount of IgG coated on plates Measure the amount of protein covalently bound to affinity supports	Requires heating for color development Not a true end-point assay	Thiols Copper chelating agents Ascorbic acid and uric acid
Microplate Protocol: 20-2,000µg/mL (25µL)	Simple, easy to perform Less protein:protein variation than Coomassie dye methods Works with peptides (three amino acids or larger) Flexible incubation protocols allow customization of reagent sensitivity and working range	Determine copper levels using a reagent formulated with BCA Reagent A ⁴		Tyrosine, cysteine and tryptophan 50mM Imidazole, 0.1M Tris, 1.0M glycine
The Micro BCA Protein Assay				
Standard Protocol: 60°C for 60 minutes 0.5-20µg/mL (0.5mL)	Three stable reagents used to make one working reagent	Suitable for determining protein concentration in very dilute aqueous solutions	More substances interfere at lower concentrations than with BCA Assay because the sample volume-to-reagent volume ratio is 1:1	Reducing sugars and reducing agents
Microplate Protocol: 37°C for 120 minutes 2-40µg/mL (150µL)	Working reagent stable for 24 hours at room temperature Compatible with most detergents Simple, easy to perform Less protein:protein variation than BCA, Coomassie dye or Lowry Methods Works with peptides (three amino acids or larger) Linear color response to increasing protein concentration	Adaptable for use with microplates ¹	60°C water bath is needed	Thiols Copper chelating agents Ascorbic acid and uric acid Tyrosine, cysteine and tryptophan 50mM Imidazole, 0.1M Tris, 1.0M glycine

* Sample volume per 1mL total assay volume for measurement in 1cm cuvette (Standard Protocol). Sample volume per 200-300µL total volume for measurement in 96-well microplate.

Quick Technical Summaries – Thermo Scientific Protein Assays

Working Range (sample volume)*	Characteristics/Advantages	Applications	Disadvantages	Interfering Substances
The Modified Lowry Protein Assay				
Standard Protocol: 1-1,500µg/mL	Two-reagent system – shelf life of at least one year	Lowry method is the most cited protein assay in the literature	Timed addition of Folin reagent adds complexity	Detergents (cause precipitation)
Microplate Protocol: 10-1,500µg/mL (40µL)	Two-step incubation requires precise sequential timing of samples Color response read at 750nm Works with peptides (three amino acids or larger) Protein:protein variation similar to that seen with BCA Method Many authors have reported ways to deal with substances that interfere	Adaptable for use with microplates	Longer total assay time Practical limit of about 20 samples per run	Thiols, disulfides Copper chelating reagents Carbohydrates including hexoseamines and their <i>N</i> -actyl derivatives Glycerol, Tris, Tricine, K ⁺ ions
Coomassie Plus (Bradford) Assay				
Linear Range: IgG: 125-1,500µg/mL BSA: 125-1,000µg/mL	Simple/fast protocols Total preparation and assay time < 30 minutes	Standard assay ⁸ Micro assay ^{9,10,11}	Less linear color response in the micro assay	Detergents ¹⁸
Standard Protocol: Sample-to-Reagent Ratio: 1:30 Typical Working Range: 100-1,500µg/mL (35µL)	One reagent system; stable for 12 months Ready-to-use formulation — no dilution or filtration needed Nearly immediate color development at room temperature	Microplate format assay ¹² Assay of protein solutions containing reducing agents ¹³ Quantitation of immobilized protein ¹⁴	Effect of interfering substances more pronounced in the micro assay Protein dye complex has tendency to adhere to glass (easily removed with MeOH) ¹⁷	
Microplate Protocol: Sample-to-Reagent Ratio: 1:1 Typical Working Range: 1-25µg/mL (150µL)	Linear color response in standard assay (more accurate results) Color response sensitive to changes in pH Temperature dependence of color response Compatible with buffer salts, metal ions, reducing agents, chelating agents Low-odor formulation	Protein in permeabilized cells ¹⁵ NaCNBH ₃ determination ¹⁶	Protein must be > 3,000 Da	
Coomassie (Bradford) Protein Assay				
Standard Protocol: Sample-to-Reagent Ratio: 1:50 100-1,500µg/mL (20µL)	Simple-to-perform protocols One-reagent system, stable for 12 months Ready-to-use formulation	Standard assay ⁸ Micro assay ^{9,10,11} Microplate format assay ¹⁹	Nonlinear color response More protein standard concentrations required to cover working range	Detergents ¹⁸
Microplate Protocol: Sample-to-Reagent Ratio: 1:1 1-25µg/mL (150µL)	No dilution or filtration needed Fast, nearly immediate color development at room temperature Total preparation and assay time < 30 minutes Typical protein:protein variation expected for a Coomassie dye-based reagent Color response sensitive to pH Temperature-dependent color response Compatible with buffer salts, metal ions, reducing agents, chelating agents	Assay of protein solutions containing reducing agents Cell line lysates ²⁰ Protein recovery studies	Micro assay has potential for interference Protein must be > 3,000 Da	

* Sample volume per 1mL total assay volume for measurement in 1cm cuvette (Standard Protocol). Sample volume per 200-300µL total volume for measurement in 96-well microplate.

Quick Technical Summaries – References

Working Range	Characteristics/Advantages	Benefits
Pre-Diluted Protein Assay Standard Sets		
Working Range: 125-2,000µg/mL	Ready to use 3.5mL each of seven standard curve data points within the working range Stable and sterile filtered 15-35 standard test tube assays or 175-350 microplate assays	No dilution series preparation Dramatically improved speed to result General utility standards for BCA, Bradford and Lowry Assay methods More reliable quantitation Standard set is treated as you would treat the sample Unparalleled convenience Economical for microplate format assays

References

1. Redinbaugh, M.G. and Turley, R.B. (1986). Adaptation of the bicinchoninic acid protein assay for use with microtiter plates and sucrose gradient fractions. *Anal. Biochem.* **153**, 267-271.
2. Sorensen, K. and Brodbeck, U. (1986). A sensitive protein assay using microtiter plates. *J. Immunol. Meth.* **95**, 291-293.
3. Stich, T.M. (1990). Determination of protein covalently bound to agarose supports using bicinchoninic acid. *Anal. Biochem.* **191**, 343-346.
4. Brenner, A.J. and Harris, E.D. (1995). A quantitative test for copper using bicinchoninic acid. *Anal. Biochem.* **226**, 80-84.
5. Akins, R.E. and Tuan, R.S. (1992). Measurement of protein in 20 seconds using a microwave BCA assay. *Biotechniques.* **12**(4), 496-499.
6. Brown, R.E., et al. (1989). Protein measurement using bicinchoninic acid: elimination of interfering substances. *Anal. Biochem.* **180**, 136-139.
7. Peterson, G.L. (1983). Meth. in Enzymol. Hirs, C.H.W. and Timasheff, S.N., eds. *San Diego: Academic Press*, **91**, pp. 95-119.
8. Bradford, M.M. (1976). A rapid and sensitive method for the quantitation of microgram quantities of protein utilizing the principle of protein-dye binding. *Anal. Biochem.* **72**, 248-254.
9. Pande, S.V. and Murthy, S.R. (1994). A modified micro-Bradford procedure for elimination of interference from sodium dodecyl sulfate, other detergents and lipids. *Anal. Biochem.* **220**, 424-426.
10. Brogdon, W.G. and Dickinson, C.M. (1983). A microassay system for measuring esterase activity and protein concentration in small samples and in high pressure liquid chromatography eluate fractions. *Anal. Biochem.* **131**, 499-503.
11. Simpson, I.A. and Sonne, O. (1982). A simple, rapid and sensitive method for measuring protein concentration in subcellular membrane fractions prepared by sucrose density ultracentrifugation. *Anal. Biochem.* **119**, 424-427.
12. Redinbaugh, M.G. and Campbell, W.H. (1985). Adaptation of the dye-binding protein assay to microtiter plates. *Anal. Biochem.* **147**, 144-147.
13. Ribin, R.W. and Warren, R.W. (1977). Quantitation of microgram amounts of protein in SDS-mercaptoethanol-Tris electrophoresis sample buffer. *Anal. Biochem.* **83**, 773-777.
14. Bonde, M., Pontoppidan, H. and Pepper, D.S. (1992). Direct dye binding — a quantitative assay for solid-phase immobilized protein. *Anal. Biochem.* **200**, 195-198.
15. Alves Cordeiro, C.A. and Freire, A.P. (1994). Protein determination in permeabilized yeast cells using the Coomassie Brilliant Blue Dye Binding Assay. *Anal. Biochem.* **223**, 321-323.
16. Sorensen, K. (1994). Coomassie Protein Assay Reagent used for quantitative determination of sodium cyanoborohydride (NaCNBH₃). *Anal. Biochem.* **218**, 231-233.
17. Gadd, K.G. (1981). Protein estimation in spinal fluid using Coomassie blue reagent. *Med. Lab. Sci.* **38**, 61-63.
18. Friedenauer, D. and Berlet, H.H. (1989). Sensitivity and variability of the Bradford protein assay in the presence of detergents. *Anal. Biochem.* **178**, 263-268.
19. Splittgerber, A.G. and Sohl, J. (1989). Nonlinearity in protein assays by the Coomassie blue dye-binding method. *Anal. Biochem.* **179**(1), 198-201.
20. Tsukada, T., et al. (1987). Identification of a region in the human vasoactive intestinal polypeptide gene responsible for regulation by cyclic AMP. *J. Biol. Chem.* **262**(18), 8743-8747.



Introduction

Protein quantitation is often necessary prior to handling protein samples for isolation and characterization. It is a required step before submitting protein samples for chromatographic, electrophoretic and immunochemical separation or analyses.

The most common methods for the colorimetric detection and quantitation of total protein can be divided into two groups based upon the chemistry involved. Protein assay reagents involve either protein-dye binding chemistry (Coomassie/Bradford) or protein-copper chelation chemistry. We offer numerous colorimetric assays for detection and quantitation of total protein. They are all well-characterized, robust assays that provide consistent, reliable results. Collectively, they represent the state-of-the-art for colorimetric detection and quantitation of total protein.

Selection of the Protein Assay

When it is necessary to determine the total protein concentration in a sample, one of the first issues to consider is the selection of a protein assay method. The choice among available protein assays usually is based upon the compatibility of the method with the samples to be assayed. The objective is to select a method that requires the least manipulation or pre-treatment of the samples containing substances that may interfere with the assay.

Table 1. Thermo Scientific Pierce Protein Assay Reagents and their working ranges.

Reagent	Protocol Used	Estimated Working Range
Pierce 600nm Protein Assay	Standard tube	25-2,000µg/mL
	Standard microplate	50-2,000µg/mL
Coomassie (Bradford) Protein Assay	Standard tube or microplate	100-1,500µg/mL
	Micro tube or microplate	1-25µg/mL
Coomassie Plus (Bradford) Assay	Standard tube or microplate	100-1,500µg/mL
	Micro tube or microplate	1-25µg/mL
BCA Protein Assay – Reducing Agent Compatible	Standard tube or microplate	125-2,000µg/mL
BCA Protein Assay	Standard tube or microplate	20-2,000µg/mL
	Enhanced tube	5-250µg/mL
Micro BCA Protein Assay	Standard tube	0.5-20µg/mL
	Standard microplate	2-40µg/mL
Modified Lowry Protein Assay	Standard protocol	1-1,500µg/mL
	Standard microplate	10-1,500µg/mL

Each method has its advantages and disadvantages (see pages 1-3). Because no one reagent can be considered to be the ideal or best protein assay method, most researchers have more than one type of protein assay reagent available in their labs.

If the samples contain reducing agents or copper chelating reagents, either of the ready-to-use liquid Coomassie dye reagents (Coomassie [Bradford] Protein Assay or the Coomassie Plus Assay) would be excellent choices.

Thermo Scientific Total Protein Assays

The Modified Lowry Protein Assay offers all of the advantages of the original reagent introduced by Oliver Lowry in 1951 in a single, stable and ready-to-use reagent.

If the samples to be analyzed contain one or more detergents (at concentrations up to 5%), the BCA Protein Assay is the best choice. If the protein concentration in the detergent-containing samples is expected to be very low ($< 20\mu\text{g/mL}$), the Micro BCA Protein Assay may be the best choice. If the total protein concentration in the samples is high ($> 2,000\mu\text{g/mL}$), sample dilution can often be used to overcome any problems with known interfering substances.

Sometimes the sample contains substances that make it incompatible with any of the protein assay methods. The preferred method of dealing with interfering substances is to simply remove them. We offer several methods for performing this function, including dialysis, desalting, chemical blocking and protein precipitation followed by resolubilization. This handbook focuses on the last two methods. Chemical blocking involves treating the sample with something that prevents the interfering substance from causing a problem. Protein precipitation causes the protein to fall out of solution, at which time the interfering buffer can be removed and the protein resolubilized. The chemical treatment method, like that used in the BCA Protein Assay – Reducing Agent Compatible, or the Pierce 660nm Protein Assay is generally preferred because, unlike protein precipitation, resolubilization of potentially hydrophobic proteins is not involved.

Selection of a Protein Standard

Selection of a protein standard is potentially the greatest source of error in any protein assay. Of course, the best choice for a standard is a highly purified version of the predominant protein found in the samples. This is not always possible or necessary. In some cases, all that is needed is a rough estimate of the total protein concentration in the sample. For example, in the early stages of purifying a protein, identifying which fractions contain the most protein may be all that is required. If a highly purified version of the protein of interest is not available or if it is too expensive to use as the standard, the alternative is to choose a protein that will produce a very similar color response curve with the selected protein assay method. For general protein assay work, bovine serum albumin (BSA) works well for a protein standard because it is widely available in high purity and is relatively inexpensive. Although it is a mixture containing several immunoglobulins, bovine gamma globulin (BGG) also is a good choice for a standard when determining the concentration of antibodies, because BGG produces a color response curve that is very similar to that of immunoglobulin G (IgG).

For greatest accuracy in estimating total protein concentration in unknown samples, it is essential to include a standard curve each time the assay is performed. This is particularly true for the protein assay methods that produce nonlinear standard curves. Determination of the number of standards and replicates used to define the standard curve depends upon the degree of nonlinearity in the standard curve and the degree of accuracy required. In general, fewer points are needed to construct a standard curve if the color response is linear. Typically, standard curves are constructed using at least two replicates for each point on the curve.

Thermo Scientific Total Protein Assays

Preparation of Standards

Use this information as a guide to prepare a set of protein standards. Dilute the contents of one Albumin Standard (BSA) ampule into several clean vials, preferably using the same diluent as the sample(s). Each 1mL ampule of 2.0mg/mL Albumin Standard is

Preparation of Diluted Albumin (BSA) Standards for BCA Assay, BCA Reducing Agent-Compatible Assay and Pierce 660nm Assay.

Dilution Scheme for Standard Test Tube Protocol and Microplate Procedure
(Working Range = 20-2,000µg/mL)

Vial	Volume of Diluent	Volume and Source of BSA	Final BSA Concentration
A	0	300µL of stock	2,000µg/mL
B	125µL	375µL of stock	1,500µg/mL
C	325µL	325µL of stock	1,000µg/mL
D	175µL	175µL of vial B dilution	750µg/mL
E	325µL	325µL of vial C dilution	500µg/mL
F	325µL	325µL of vial E dilution	250µg/mL
G	325µL	325µL of vial F dilution	125µg/mL
H	400µL	100µL of vial G dilution	25µg/mL
I	400µL	0	0µg/mL = Blank

Dilution Scheme for Enhanced Test Tube Protocol
(Working Range = 5-250µg/mL)

Vial	Volume of Diluent	Volume and Source of BSA	Final BSA Concentration
A	700µL	100µL of stock	250µg/mL
B	400µL	400µL of vial A dilution	125µg/mL
C	450µL	300µL of vial B dilution	50µg/mL
D	400µL	400µL of vial C dilution	25µg/mL
E	400µL	100µL of vial D dilution	5µg/mL
F	400µL	0	0µg/mL = Blank

Preparation of Diluted Albumin (BSA) Standards for Micro BCA Assay.

Vial	Volume of Diluent	Volume and Source of BSA	Final BSA Concentration
A	.45mL	0.5µL of stock	200µg/mL
B	8.0mL	2.0µL of vial A dilution	40µg/mL
C	4.0mL	4.0µL of vial B dilution	20µg/mL
D	4.0mL	4.0µL of vial C dilution	10µg/mL
E	4.0mL	4.0µL of vial D dilution	5µg/mL
F	4.0mL	4.0µL of vial E dilution	2.5µg/mL
G	4.8mL	3.2µL of vial F dilution	1µg/mL
H	4.0mL	4.0µL of vial G dilution	0.5µg/mL
I	8.0mL	0	0µg/mL = Blank

sufficient to prepare a set of diluted standards for either working range suggested. There will be sufficient volume for three replications of each diluted standard.

Preparation of Protein Standards for Coomassie Plus (Bradford) Assay and Coomassie (Bradford) Assay.

Dilution Scheme for Standard Test Tube and Microplate Protocols
(Working Range = 100-1,500µg/mL)

Vial	Volume of Diluent	Volume and Source of BSA	Final BSA Concentration
A	0	300µL of stock	2,000µg/mL
B	125µL	375µL of stock	1,500µg/mL
C	325µL	325µL of stock	1,000µg/mL
D	175µL	175µL of vial B dilution	750µg/mL
E	325µL	325µL of vial C dilution	500µg/mL
F	325µL	325µL of vial E dilution	250µg/mL
G	325µL	325µL of vial F dilution	125µg/mL
H	400µL	100µL of vial G dilution	25µg/mL
I	400µL	0	0µg/mL = Blank

Dilution Scheme for Micro Test Tube or Microplate Protocols
(Working Range = 1-25µg/mL)

Vial	Volume of Diluent	Volume and Source of BSA	Final BSA Concentration
A	2,370µL	30µL of stock	25µg/mL
B	4,950µL	50µL of stock	20µg/mL
C	3,970µL	30µL of stock	15µg/mL
D	2,500µL	2,500µL of vial B dilution	10µg/mL
E	2,000µL	2,000µL of vial D dilution	5µg/mL
F	1,500µL	1,500µL of vial E dilution	2.5µg/mL
G	5,000µL	0	0µg/mL = Blank

Preparation of Diluted Albumin (BSA) for Modified Lowry Assay.

Dilution Scheme for Test Tube and Microplate Procedure
(Working Range = 1-1,500µg/mL)

Vial	Volume of Diluent	Volume and Source of BSA	Final BSA Concentration
A	250µL	750µL of stock	200µg/mL
B	625 µ	625µL of stock	40µg/mL
C	310 µ	310µL of vial A dilution	20µg/mL
D	625µL	625µL of vial B dilution	10µg/mL
E	625µL	625µL of vial D dilution	5µg/mL
F	625µL	625µL of vial E dilution	2.5µg/mL
G	800µL	200µL of vial F dilution	1µg/mL
H	800µL	200µL of vial G dilution	0.5µg/mL
I	800µL	200µL of vial H dilution	0µg/mL = Blank
J	1,000µL	0	0µg/mL = Blank

Standards for Total Protein Assay

Bovine Serum Albumin Standard

The Thermo Scientific Pierce BSA Standard ... the most relied-upon albumin standard for total protein determination measurements.



Ordering Information

Product	Description	Pkg. Size
23208	Bovine Serum Albumin Standard Pre-Diluted Set Contains: Bovine Albumin in 0.9% NaCl solution containing sodium azide	7 x 3.5mL
23209	Albumin Standard Ampules, 2mg/mL Contains: Bovine Albumin in 0.9% NaCl solution containing sodium azide	10 x 1mL
23210	Albumin Standard, 2mg/mL Contains: Bovine Albumin in 0.9% NaCl solution containing sodium azide	50mL

Bovine Gamma Globulin Standard

Easy-to-use, 2mg/mL BGG solution. Ampuled to preserve product integrity. An excellent choice for IgG total protein determination. Recommended for Coomassie (Bradford) Assays.

Ordering Information

Product	Description	Pkg. Size
23212	Bovine Gamma Globulin Standard, 2mg/mL Contains: Bovine Gamma Globulin Fraction II in 0.9% NaCl solution containing sodium azide	10 x 1mL

Additional Thermo Scientific Pierce Mammalian Gamma Globulins for Standards:

Product	Description	Pkg. Size
31878	Mouse Gamma Globulin	10mg
31887	Rabbit Gamma Globulin	10mg
31885	Rat Gamma Globulin	10mg
31871	Goat Gamma Globulin	10mg
31879	Human Gamma Globulin	10mg

Thermo Scientific Total Protein Assays

Pre-Diluted BSA and BGG Protein Assay Standard Sets

Construct a standard curve for most protein assay methods as fast as you can pipette.



Highlights:

- Stable and sterile filtered
- Ideal for BCA and Bradford-based protein assays
- Standard curve range: 125-2,000µg/mL
- Seven data points within the range
- Sufficient materials to prepare 15-35 standard tube protocol curves or 175-350 standard microplate protocol curves running duplicate data points
- Convenient – no need to prepare a diluted standard series for each determination
- Consistent – no need to worry about variability in dilutions from day to day or person to person
- More reliable protein quantitation because of the assured accuracy of the concentrations of each standard
- Dramatically improved speed to result, especially with Bradford-based protein assays

Sample Preparation

Before a sample is analyzed for total protein content, it must be solubilized, usually in a buffered aqueous solution. The entire process is usually performed in the cold, with additional precautions taken to inhibit microbial growth or to avoid casual contamination of the sample by foreign debris such as hair, skin or body oils.

When working with tissues, cells or solids, the first step of the solubilization process is usually disruption of the sample's cellular structure by grinding and/or sonication or by the use of specially designed reagents (e.g., Thermo Scientific Pierce Cell Lysis Reagents) containing surfactants to lyse the cells. This is done in aqueous buffer containing one or more surfactants to aid the

solubilization of the membrane-bound proteins, biocides (antimicrobial agents) and protease inhibitors. After filtration or centrifugation to remove the cellular debris, additional steps such as sterile filtration, removal of lipids or further purification of the protein of interest from the other sample components may be necessary.

Nonprotein substances in the sample that are expected to interfere in the chosen protein assay method may be removed by dialysis with Thermo Scientific Slide-A-Lyzer Dialysis Cassettes or Thermo Scientific SnakeSkin Dialysis Tubing, gel filtration with Thermo Scientific Desalting Columns or D Detergent Removing Gel, or precipitation as in the Compat-Able™ Protein Assays or SDS-Out Reagent.

Protein:protein Variation

Each protein in a sample is unique and can demonstrate that individuality in protein assays as variation in the color response. Such protein:protein variation refers to differences in the amount of color (absorbance) obtained when the same mass of various proteins is assayed concurrently by the same method. These differences in color response relate to differences in amino acid sequence, isoelectric point (pI), secondary structure and the presence of certain side chains or prosthetic groups.

Table 2 (page 9) shows the relative degree of protein:protein variation that can be expected with our different protein assay reagents. This differential may be a consideration in selecting a protein assay method, especially if the relative color response ratio of the protein in the samples is unknown. As expected, protein assay methods that share the same basic chemistry show similar protein:protein variation. These data make it obvious why the largest source of error for protein assays is the choice of protein for the standard curve.

Ordering Information

Product	Description	Pkg. Size
23208	Pre-Diluted Protein Assay Standards: Bovine Serum Albumin (BSA) Set Diluted in 0.9% saline and preserved with 0.05% sodium azide Includes: 7 x 3.5mL of standardized BSA solutions each at a specific concentration along a range from 125-2,000µg/mL	Kit
23213	Pre-Diluted Protein Assay Standards: Bovine Gamma Globulin Fraction II (BGG) Set Diluted in 0.9% saline and preserved with 0.05% sodium azide Includes: 7 x 3.5mL of standardized BGG solutions each at a specific concentration along a range from 125-2,000µg/mL	Kit

Total Protein Assays

For each of the six methods presented here, a group of 14 proteins was assayed using the standard protocol in a single run. The net (blank corrected) average absorbance for each protein was calculated. The net absorbance for each protein is expressed as a ratio to the net absorbance for BSA. If a protein has a ratio of 0.80, it means that the protein produces 80% of the color obtained for an equivalent mass of BSA. All of the proteins tested using the standard tube protocol with the BCA Protein Assay, the Modified Lowry Protein Assay, the Coomassie (Bradford) Assay and the Coomassie Plus (Bradford) Assay were at a concentration of 1,000µg/mL.

Compatible and Incompatible Substances

An extensive list of substances that have been tested for compatibility with each protein assay reagent can be found in the instruction booklet that accompanies each assay product. A copy can also be obtained from our web site.

In summary, the Coomassie (Bradford) and the Coomassie Plus (Bradford) Assays will tolerate the presence of most buffer salts, reducing substances and chelating agents, but they will not tolerate the presence of detergents (except in very low concentrations) in the sample. Strong acids or bases, and even some strong buffers, may interfere if they alter the pH of the reagent.

The Modified Lowry Protein Assay is sensitive to the presence of reducing substances, chelating agents and strong acids or strong bases in the sample. In addition, the reagent will be precipitated by the presence of detergents and potassium ions in the sample.

The BCA Protein Assay is tolerant of most detergents but is sensitive to the presence of reducing substances, chelating agents and strong acids or strong bases in the sample. In general, the Micro BCA Protein Assay is more sensitive to the same substances that interfere with the BCA Protein Assay because less dilution of the sample is used.

Table 2. Protein:protein variation.

	Pierce 660nm Assay Ratio	BCA Ratio	Micro BCA Ratio	Modified Lowry Ratio	Coomassie (Bradford) Ratio	Coomassie Plus Ratio	Bio-Rad (Bradford) Ratio
1. Albumin, bovine serum	1.00	1.00	1.00	1.00	1.00	1.0	1.00
2. Aldolase, rabbit muscle	0.83	0.85	0.80	0.76	0.76	0.74	0.97
3. α-Chymotrypsinogen	x	1.14	0.99	0.48	0.48	0.52	0.41
4. Cytochrome C, horse heart	1.22	0.83	1.11	1.07	1.07	1.03	0.48
5. Gamma Globulin, bovine	0.51	1.11	0.95	0.56	0.56	0.58	0.58
6. IgG, bovine	x	1.21	1.12	0.58	0.58	0.63	0.65
7. IgG, human	0.57	1.09	1.03	0.63	0.63	0.66	0.70
8. IgG, mouse	0.48	1.18	1.23	0.59	0.59	0.62	0.60
9. IgG, rabbit	0.38	1.12	1.12	0.37	0.37	0.43	0.53
10. IgG, sheep	x	1.17	1.14	0.53	0.53	0.57	0.53
11. Insulin, bov. pancreas	0.81	1.08	1.22	0.60	0.60	0.67	0.14
12. Myoglobin, horse heart	1.18	0.74	0.92	1.09	1.19	1.15	0.89
13. Ovalbumin	0.54	0.93	1.08	0.32	0.32	0.68	0.27
14. Transferrin, human	0.80	0.89	0.98	0.84	0.84	0.90	0.95
Avg. ratio	0.7364	1.02	1.05	0.68	0.68	0.73	0.60
S.D.	0.2725	0.15	0.12	0.26	0.26	0.21	0.28
CV	37%	14.7%	11.4%	38.2%	38.2%	28.8%	46%

1. All of the proteins were tested using the standard tube protocol with the Micro BCA Protein Assay at a protein concentration of 10µg/mL.

This table is a useful guideline to estimate the protein:protein variation in color response that can be expected with each method. It does not tell the whole story. However, because the comparisons were made using a single protein concentration, it is not apparent that the color response ratio also varies with changes in protein concentration.

Thermo Scientific Total Protein Assays

Substances Compatible with Thermo Scientific Pierce Protein Assays

Concentrations listed refer to the actual concentration in the protein sample. A blank indicates that the material is incompatible with the assay; n/a indicates the substance has not been tested in that respective assay.

Test Compound	Microplate ^{††}						
	660nm	BCA	Micro BCA	BCA-RAC	Coomassie Plus	Coomassie	Modified Lowry
2-D sample buffer [†]	neet [†]	n/a	n/a	n/a	n/a	n/a	n/a
2-Mercaptoethanol	1M	0.01%	1mM	25mM (35)	1M	1M	1mM
ACES, pH 7.8	50mM	25mM	10mM	∅	100mM	100mM	n/a
Acetone	50%	10%	1%	∅	10%	10%	10%
Acetonitrile	50%	10%	1%	30%	10%	10%	10%
Ammonium sulfate	125mM	1.5M	∅	∅	1M	1M	∅
Aprotinin	2mM	10mg/L	1mg/L	∅	10mg/L	10mg/L	10mg/L
Ascorbic acid	500mM	∅	∅	n/a	50mM	50mM	1mM
Asparagine	40mM	1mM	n/a	∅	10mM	10mM	5mM
Bicine	>1M	20mM	2mM	1mM	100mM	100mM	n/a
Bis-Tris pH 6.5	50mM	33mM	0.2mM	16.5mM	100mM	100mM	n/a
Borate (50mM) pH 8.5	neet	neet	1:4	∅	neet	neet	n/a
B-PER [®] Reagent	1:2	neet	n/a	1:3	1:2	1:2	n/a
B-PER Reagent II	1:2	n/a	n/a	1:4	1:4	n/a	n/a
B-PER Reagent PBS	1:2	n/a	n/a	1:4	n/a	n/a	n/a
Brij [®] -35	5%	5%	5%	0.63%	0.062%	0.125%	0.031%
Brij-56	n/a	1%	1%	n/a	0.031%	0.031%	0.062%
Brij-58	5%	1%	1%	0.50%	0.016%	0.031%	0.062%
Bromophenol blue (in 50mM NaOH)	0.031%	∅	∅	∅	∅	∅	∅
Calcium chloride (in TBS pH 7.2)	40mM	10mM	10mM	1mM	10mM	10mM	n/a
Cesium bicarbonate	100mM	100mM	100mM	∅	100mM	100mM	50mM
Cetylpyridinium chloride	2.5% [†]	n/a	n/a	n/a	n/a	n/a	n/a
CHAPS	5%	5%	1%	10% (10)	5%	5%	0.062%
CHAPSO	4%	5%	5%	∅	5%	5%	0.031%
CHES	>500mM	100mM	100mM	50mM	100mM	100mM	n/a
Cobalt chloride (in TBS pH 7.2)	20mM	0.8mM	∅	0.4mM	10mM	10mM	n/a
CTAB	2.5% [†]	n/a	n/a	n/a	n/a	n/a	n/a
Cysteine	350mM	∅	∅	2.5mM	10mM	10mM	1mM
Dithioerythritol (DTE)	25mM	1mM	∅	2.5mM	1mM	1mM	∅
Dithiothreitol (DTT)	500mM	1mM	∅	5mM (5)	5mM	5mM	∅
DMF	50%	10%	1%	5%	10%	10%	10%
DMSO	50%	10%	1%	0.25%	10%	10%	10%
DTAB	2% [†]	n/a	n/a	n/a	n/a	n/a	n/a
EDTA	20mM	10mM	0.5mM	5mM (20)	100mM	100mM	1mM
EGTA	20mM	∅	∅	5mM (10)	2mM	2mM	1mM
EPPS pH 8.0	200mM	100mM	100mM	∅	100mM	100mM	n/a
Ethanol	50%	10%	1%	∅	10%	10%	10%
Ferric chloride (in TBS pH 7.2)	5mM	10mM	0.5mM	5mM	10mM	10mM	n/a
Glucose	500mM	10mM	1mM	∅	1mM	1mM	100mM
Glutathione (reduced)	100mM	n/a	n/a	10mM	n/a	n/a	n/a
Glycerol (fresh)	50%	10%	1%	5%	10%	10%	10%
Glycine-HCl pH 2.8	100mM	100mM	n/a	50mM	100mM	100mM	100mM
Guanidine-HCl	2.5M	4M	4M	1.5M (2)	3.5M	3.5M	n/a
HEPES pH 7.5	100mM	100mM	100mM	200mM (200)	100mM	100mM	1mM
Hydrides (Na ₂ BH ₄ or NaCNBH ₃)	∅	∅	∅	n/a	n/a	n/a	n/a
Hydrochloric acid (HCl)	125mM	100mM	10mM	∅	100mM	100mM	100mM
Imidazole pH 7.0	200mM	50mM	12.5mM	30mM (50)	200mM	200mM	25mM
I-PER [®] Reagent	1:4	neet	n/a	n/a	n/a	n/a	n/a
Laemmli SDS sample buffer [†]	neet [†]	∅	∅	∅	∅	∅	∅
Leupeptin	80µM	10mg/L	10mg/L	∅	10mg/L	10mg/L	10mg/L
Mannitol	100mM	n/a	n/a	n/a	n/a	n/a	n/a
Melibiose	500mM	∅	n/a	n/a	100mM	100mM	25mM
Mem-PER [®] Reagent	neet	neet	neet	1:2	neet	n/a	n/a
MES-buffered saline pH 4.7 [†]	neet	neet	1:4	∅	neet	neet	n/a
MES pH 6.1	125mM	100mM	100mM	100mM (100)	100mM	100mM	125mM
Methanol	50%	10%	1%	0.5%	10%	10%	10%
Magnesium chloride	>1M	n/a	n/a	100mM	n/a	n/a	n/a
Modified Dulbecco's PBS [†]	neet	neet	neet	neet	neet	neet	n/a
MOPS pH 7.2	125mM	100mM	100mM	200mM	100mM	100mM	n/a
M-PER [®] Reagent	1:2	neet	n/a	1:2	neet	n/a	n/a
N-Acetylglucosamine	100mM	10mM	∅	∅	100mM	100mM	n/a
Na acetate pH 4.8	100mM	200mM	200mM	∅	180mM	180mM	200mM
Na azide	0.125%	0.2%	0.20%	0.01%	0.5%	0.5%	0.2%
Na bicarbonate	100mM	100mM	100mM	∅	100mM	100mM	100mM
Na carb-bicarbonate pH 9.4 [†]	1:3	neet	neet	neet	neet	neet	n/a

Test Compound	Microplate ^{††}						
	660nm	BCA	Micro BCA	BCA-RAC	Coomassie Plus	Coomassie	Modified Lowry
Na chloride	1.25M	1M	1M	150mM	5M	5M	1M
Na citrate pH 4.8	12.5mM	200mM	5mM	50mM	200mM	200mM	n/a
Na citrate-carbonate pH 9 [‡]	∅	1:8	1:600	∅	neet	neet	n/a
Na citrate-MOPS pH 7.5 [‡]	1:16	1:8	1:600	neet	n/a	neet	n/a
Na deoxycholate (DOC)	0.25%	5%	5%	n/a	0.4%	0.05%	n/a
Na hydroxide (NaOH)	125mM	100mM	50mM	∅	100mM	100mM	100mM
Na phosphate	500mM	100mM	100mM	100mM	100mM	100mM	100mM
NE-PER [®] Reagent (CER)	neet	neet	n/a	1:2	1:4	n/a	n/a
NE-PER Reagent (NER)	neet	neet	n/a	1:4	neet	n/a	n/a
Nickel chloride (in TBS pH 7.2)	10mM	10mM	0.2mM	∅	10mM	10mM	n/a
NP-40	5%	5%	5%	∅	0.5%	0.5%	0.016%
Octyl beta-glucoside	5%	5%	0.1%	2.5% (10)	0.5%	0.5%	0.031%
Octylthioglucoside	10%	5%	5%	7%	3%	3%	n/a
Na-orthovanadate (in PBS pH 7.2)	50mM	1mM	1mM	0.5mM	1mM	1mM	n/a
Phenol Red	0.5mg/mL	∅	∅	3.125µg/mL	0.5mg/mL	0.5mg/mL	n/a
Phosphate-buffered saline (PBS) [‡]	neet	neet	neet	neet	neet	neet	n/a
PIPES pH 6.8	100mM	100mM	100mM	25mM	100mM	100mM	n/a
PMSF in isopropanol	1mM	1mM	1mM	0.125mM	1mM	1mM	1mM
Potassium thiocyanate	250mM	3M	n/a	∅	3M	3M	100mM
P-PER [®] Reagent	1:2	∅	n/a	1:2	∅	∅	∅
RIPA buffer [‡]	neet	neet	1:10	1:2	1:40	1:10	n/a
SDS	0.01%, 5% †	5%	5%	5% (10)	0.016%	0.125%	1%
Sodium compounds	(see Na)	(see Na)	(see Na)	(see Na)	(see Na)	(see Na)	(see Na)
Span [®] 20	n/a	1%	1%	n/a	0.5%	0.5%	0.25%
Sucrose	50%	40%	4%	40% (40)	10%	10%	7.5%
TCEP	40mM	n/a	n/a	10mM (10)	n/a	n/a	n/a
Thimerosal	0.25%	0.01%	∅	0.03%	0.01%	0.01%	0.01%
Thiourea	2M	n/a	n/a	n/a	n/a	n/a	n/a
TLCK	5mg/mL	0.1mg/L	0.1mg/L	∅	0.1mg/mL	0.1mg/L	0.01mg/L
TPCK	4mg/mL	0.1mg/L	0.1mg/L	∅	0.1mg/mL	0.1mg/L	0.1mg/L
T-PER Reagent	1:2	1:2	n/a	n/a	neet	n/a	n/a
Tricine pH 8.0	500mM	25mM	2.5mM	0.5mM	100mM	100mM	n/a
Triethanolamine pH 7.8	100mM	25mM	0.5mM	25mM	100mM	100mM	n/a
Tris-buffered saline (TBS) [‡]	neet	neet	1:10	neet	neet	neet	n/a
Tris-glycine pH 8.0 [‡]	neet	1:3	1:10	∅	neet	neet	n/a
Tris-glycine-SDS pH 8.3 [‡]	neet †	neet	neet	∅	1:4	1:2	n/a
Tris-HCl pH 8.0	250mM	250mM	50mM	35mM (50)	2M	2M	10mM
Tris-HEPES-SDS [‡]	neet †	n/a	n/a	n/a	n/a	n/a	n/a
Triton [®] X-100	1%	5%	5%	7% (10)	0.062%	0.125%	0.031%
Triton X-114	0.50%	1%	0.05%	2% (2)	0.062%	0.125%	0.031%
Triton X-305	9%	1%	1%	1%	0.125%	0.5%	0.031%
Triton X-405	5%	1%	1%	∅	0.025%	0.5%	0.031%
Tween [®] 20	10%	5%	5%	10% (10)	0.031%	0.062%	0.062%
Tween 60	5%	5%	0.5%	5%	0.025%	0.1%	n/a
Tween 80	5%	5%	5%	2.5%	0.016%	0.062%	0.031%
Urea	8M	3M	3M	3M (4)	3M	3M	3M
Y-PER [®] Reagent	∅	neet	n/a	n/a	n/a	n/a	n/a
Y-PER Plus Reagent	1:2	neet	n/a	n/a	neet	n/a	n/a
Zinc chloride (in TBS pH 7.2)	10mM	10mM	0.5mM	∅	10mM	10mM	n/a
Zwittergent [®] 3-14	0.05%	1%	∅	2% (2)	0.025%	0.025%	n/a

Compounds are listed alphabetically using common names or abbreviations, except sodium compounds which are alphabetized under "Na"; Dilutions are expressed as "neet" (= undiluted) or in the form of a ratio, where "1:2" means 2-fold dilution; n/a Denotes that the compound was not tested in this assay; ∅ Denotes compounds that were not compatible at the lowest concentration tested; † Value when the 660nm Assay is run using the ionic detergent compatibility reagent (IDCR, Part No. 22663); †† Selected values for the regular BCA-RAC Kit are given in parentheses in the column for the Microplate BCA-RAC.

‡ Compound (buffer) whose formulation is described more fully in the following table:

Part No.	Buffer	Formulation
–	2-D sample buffer	(8M urea, 4% CHAPS) or (7M urea, 2M thiourea, 4% CHAPS)
–	Laemmli SDS sample buffer	65mM Tris-HCl, 10% glycerol, 2% SDS, 0.025% bromophenol blue
28390	MES-buffered saline pH 4.7	0.1M MES, 150mM NaCl pH 4.7
28374	Modified Dulbecco's PBS	8mM sodium phosphate, 2mM potassium phosphate, 0.14M NaCl, 10mM KCl, pH 7.4
28382	Na carb-bicarb pH 9.4	0.2M sodium carbonate-bicarbonate pH 9.4
28388	Na citrate-carbonate pH 9	0.6M sodium citrate, 0.1M sodium-carbonate pH 9
28386	Na citrate-MOPS pH 7.5	0.6M sodium citrate 0.1M MOPS pH 7.5
28372	Phosphate-buffered saline (PBS)	100mM sodium phosphate, 150mM NaCl pH 7.2
89900	RIPA Buffer	50mM Tris, 150mM NaCl, 0.5% DOC, 1% NP40, 0.1% SDS pH 8.0
28379	Tris-buffered saline (TBS)	25mM Tris, 150mM NaCl pH 7.6
28380	Tris-glycine pH 8.0	25mM Tris, 192mM glycine pH 8.0
28378	Tris-glycine-SDS pH 8.3	25mM Tris, 192mM glycine, 0.1% SDS pH 8.3
28398	Tris-HEPES-SDS	100mM Tris, 100mM HEPES, 3mM SDS

Thermo Scientific Total Protein Assays

Time Considerations

The amount of time required to complete a total protein assay will vary for the different colorimetric, total protein assay methods presented. To compare the amount of time required to perform each assay, all seven assays were performed using 20 samples and eight standards (including the blank). Each sample or standard was assayed in duplicate using the standard tube protocol (triplicate using the plate). The estimates include times for both incubation(s) and handling:

- Preparing (diluting) the standard protein in the diluent buffer (10 minutes)
- Organizing the run and labeling the tubes (5 minutes)
- Pipetting the samples and reagents (10 minutes for 56 tubes, 1 minute per plate)
- Mixing or incubating the tubes or plates (varies)
- Measuring the color produced (15 minutes for 56 tubes or 1 minute per plate)
- Graphing the standard curve, calculating, recording and reporting the results (30 minutes)

Table 3. Times required to assay 20 samples and 8 standards using the test tube procedure; handling times are considerably less using the microplate procedure.

Method	Product #	Incubation Time	Total Assay Time
Pierce 600nm Protein Assay	23250	5 minutes	75 minutes
Coomassie Plus (Bradford) Assay	23236	10 minutes	80 minutes
Coomassie (Bradford) Assay	23200	10 minutes	80 minutes
BCA Assay	23225	30 minutes	100 minutes
Modified Lowry Assay	23240	10 minutes and 30 minutes	110 minutes
BCA Protein Assay – Reducing Agent Compatible	23250	45 minutes	115 minutes
Micro BCA Assay	23235	60 minutes	130 minutes

Calculation of Results

When calculating protein concentrations manually, it is best to use point-to-point interpolation. This is especially important if the standard curve is nonlinear. Point-to-point interpolation refers to a method of calculating the results for each sample using the equation for a linear regression line obtained from just two points on the standard curve. The first point is the standard that has an absorbance just below that of the sample and the second point is the standard that has an absorbance just above that of the sample. In this way, the concentration of each sample is calculated from the most appropriate section of the whole standard curve. Determine the average total protein concentration for each sample from the average of its replicates. If multiple dilutions of each sample have been assayed, average the results for the dilutions that fall within the most linear portion of the working range.

When analyzing results with a computer, use a quadratic curve fit for the nonlinear standard curve to calculate the protein concentration of the samples. If the standard curve is linear, or if the absorbance readings for your samples fall within the linear portion of the standard curve, the total protein concentrations of the samples can be estimated using the linear regression equation.

Most software programs allow one to construct and print a graph of the standard curve, calculate the protein concentration for each sample, and display statistics for the replicates. Typically, the statistics displayed will include the mean absorbance readings (or the average of the calculated protein concentrations), the standard deviation (SD) and the coefficient of variation (CV) for each standard or sample. If multiple dilutions of each sample have been assayed, average the results for the dilutions that fall in the most linear portion of the working range.

References

- Krohn, R.I. (2002). The colorimetric detection and quantitation of total protein, *Current Protocols in Cell Biology*, **A3.H.1-A.3H.28**, John Wiley & Sons, Inc.
Krohn, R.I. (2001). The colorimetric determination of total protein, *Current Protocols in Food Analytical Chemistry*, **B1.1.1-B1.1.27**, John Wiley & Sons, Inc.

Thermo Scientific Pierce 660nm Protein Assay

Thermo Scientific Pierce 660nm Protein Assays

Rapid, reproducible and colorimetric.

Accurate protein concentration measurements are required to study many biochemical processes. Although there are several methods for quantifying proteins, colorimetric or chromogenic methods remain popular because of their relative simplicity and speed. The most commonly used dye-binding protein assay is the Bradford assay,¹ which is based on coomassie dye binding to proteins. The Bradford assay, however, is prone to inaccuracy from its typical non-linear standard curves. Moreover, the assay is not compatible with samples containing detergents at commonly used concentrations. The Pierce 660nm Protein Assay is highly reproducible, rapid and more linear than the Bradford method. Furthermore, it is compatible with commonly used detergents and reducing agents.

Highlights:

- **Accurate results** – standard curves are more linear than the Bradford method
- **Versatile** – compatible with commonly used detergents and reducing agents and with samples lysed in Laemmli sample buffer
- **Fast** – single reagent with a simple mix-and-read assay
- **Flexible** – available in test tube and microplate formats
- **Economical** – use small volumes of valuable samples: 10 μ L in microplate and 100 μ L in standard procedures
- **Convenient** – room temperature storage means no waiting for the reagent to warm-up before use

Every protein assay has limitations depending on the application and the specific protein sample analyzed. The most useful features to consider when choosing a protein assay are sensitivity (lower detection limit), compatibility with common substances in samples (e.g., detergents, reducing agents, chaotropic agents, inhibitors, salts and buffers), standard curve linearity and protein-to-protein variation. Current methods for the colorimetric determination of protein concentration in solution include the Coomassie Blue G-250 dye-binding assay,¹ Biuret method,² the Lowry method,³ the bicinchoninic acid (BCA) assay⁴ and colloidal gold protein assay.⁵

The Pierce 660nm Protein Assay is based on the binding of a proprietary dye-metal complex to protein in acidic conditions that causes a shift in the dye's absorption maximum, which is measured at 660nm. To demonstrate the effect of protein binding to the dye-metal complex, we performed spectral analysis of the dye with and without metal and in the presence and absence of BSA. The absorption maximum of the dye-metal complex shifts proportionally upon binding to BSA (Figure 1).

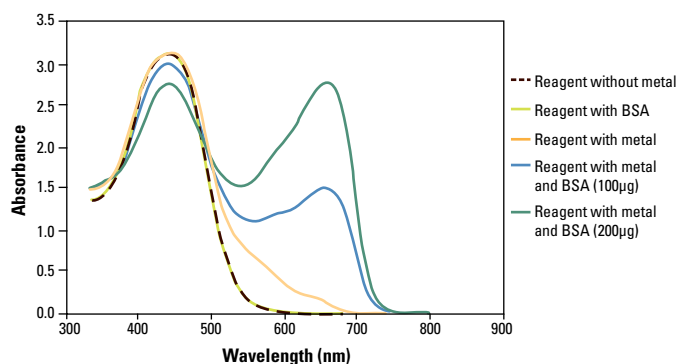


Figure 1. The absorption maximum of the reagent-metal complex shifts proportionally upon binding to BSA. The absorption spectra were recorded for the Thermo Scientific Pierce 660nm Protein Assay Reagent from 340 to 800nm using a Varian Cary[®] Spectrophotometer. The assay reagent is a proprietary dye-metal complex that binds to protein in acidic conditions, which shifts the dye's absorption maximum.

The dye-metal complex is reddish-brown that changes to green upon protein binding. The color produced in the assay is stable and increases in proportion to a broad range of increasing protein concentrations. The color change is produced by deprotonation of the dye at low pH facilitated by protein-binding interactions through positively charged amino acid groups and the negatively charged deprotonated dye-metal complex.

The linear detection ranges for BSA are 25-2,000 μ g/mL for the test tube assay and 50-2,000 μ g/mL for the microplate assay. The linear range for BGG is 50-2,000 μ g/mL for both the test tube and microplate assays (Figures 2 and 3). The assay has a moderate protein-to-protein variation of 37% and is more linear compared with the Bradford assay and, thus, produces more accurate results (Figure 4). The Pierce 660nm Protein Assay color development is significantly greater with BSA than with most other proteins, including BGG. Therefore, BSA is a suitable standard if the sample contains primarily albumin, or if the protein being assayed has a similar response to the dye as BSA. For a color response that is typical of globulins, BGG is an appropriate standard protein.

The Pierce 660nm Protein Assay is compatible with high concentrations of most detergents, reducing agents and other commonly used reagents. Additionally, by simply adding Ionic Detergent Compatibility Reagent (IDCR) to the assay reagent, the assay is compatible with samples containing Laemmli SDS sample buffer with bromophenol blue and many common ionic detergents. IDCR completely dissolves by thorough mixing and does not have any affect on the assay. In conclusion, the Pierce 660nm Protein Assay is a detergent- and reducing agent-compatible protein assay that is linear over wide range of concentrations. The simple mix-and-read format is easy to use, providing researchers a fast method for accurate protein quantitation.

Pierce 660nm Protein Assay

Methods:

Spectral Analysis: The absorption spectra from 340 to 800nm were recorded using a Varian Cary Spectrophotometer of the following component combinations: the Pierce 660nm Protein Assay Reagent alone and in the presence of the transition metal; 100µg of bovine serum albumin (BSA) and reagent with and without metal; and 200µg of BSA with the reagent and metal.

Typical Response Curves

Test Tube Procedure: To each test tube containing 0.1mL of BSA or BGG standard replicate (25, 50, 125, 250, 500, 750, 1000, 1500 and 2000µg/mL) in saline, 1.5mL of the Pierce 660nm Protein Assay Reagent was added, mixed well and incubated at room temperature for 5 minutes. The absorbance of all samples and controls was measured at 660nm. The average absorbance for the blank replicates (control) was subtracted from the absorbance for individual standard replicates. A standard curve was generated by plotting the average blank-corrected 660nm measurement for each standard versus its concentration. For a comparison study, the standard Bio-Rad Bradford Assay was performed as per manufacturer's directions.

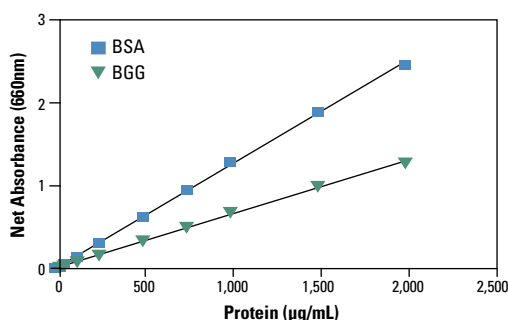


Figure 2. Typical color response curves using the test tube procedure. The linear detection ranges are 25-2,000µg/mL for bovine serum albumin (BSA) and 50-2,000µg/mL for bovine gamma globulin (BGG). The average absorbance for the blank replicates (control) was subtracted from the absorbance for individual standard replicates.

Microplate Procedure: To each well containing 0.01mL of BSA or BGG standard replicate (25, 50, 125, 250, 500, 750, 1000, 1500 and 2000µg/mL) in saline, 0.15mL of the Pierce 660nm Protein Assay Reagent was added. The plate was covered with sealing tape, mixed for one minute on a plate shaker and incubated at room temperature for five minutes. The plate reader was set to 660nm and using the control as a blank, the absorbance of all samples was measured. A standard curve was generated by plotting the average blank-corrected 660nm measurement for each standard versus its concentration.

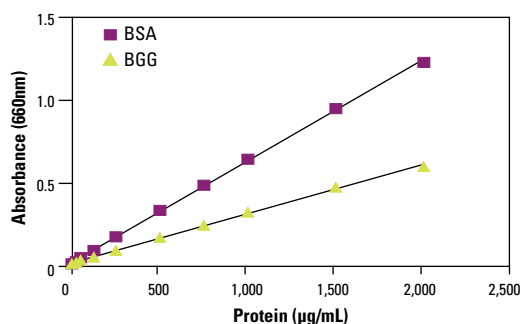


Figure 3. Typical color response curves using the microplate procedure. The linear detection range is 50-2,000µg/mL for bovine serum albumin (BSA) and bovine gamma globulin (BGG). The average absorbance for the blank replicates (control) was subtracted from the absorbance for individual standard replicates.

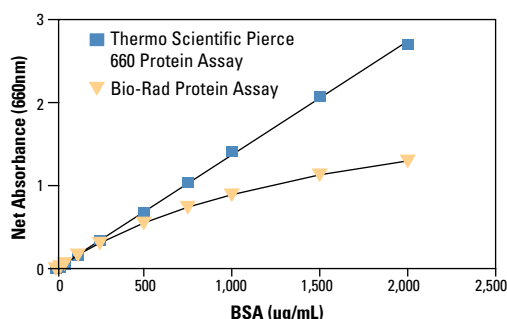


Figure 4. Performance comparison of Bradford Protein Assay versus the Thermo Scientific Pierce 660nm Protein Assay. Assays were performed according to the standard test-tube procedure using 100µL of BSA. The Pierce 660nm Protein Assay has a greater linear range of 25-2,000µg/mL, compared with the Bradford Assay, which has a linear range of only 125-1,000µg/mL.

References

- Bradford, M.M. (1976). A rapid and sensitive method for the quantitation of microgram quantities of protein utilizing the principle of protein-dye binding. *Anal. Biochem.* **72**, 248-254.
- Gornall, A.G. (1949). Determination of serum proteins by means of the biuret reaction. *J. Biol. Chem.* **177**, 751-766.
- Lowry, O.H. (1951). Protein measurement with Folin-Phenol reagent. *J. Biol. Chem.* **193**, 265-275.
- Smith, P.K., et al. (1985). Measurement of protein using bicinchoninic acid. *Anal. Biochem.* **150**, 76-85.
- Stoscheck, C.M. (1987). Protein assay sensitive at nanogram levels. *Anal. Biochem.* **160**, 301-305.

Ordering Information

Product	Description	Pkg. Size
22660	Pierce 660nm Protein Assay Reagent Sufficient reagent for 500 standard assays and 5,000 microplate assays.	750mL
22662	Pierce 660nm Protein Assay Kit Sufficient reagent to perform 300 standard assays and 3,000 microplate assays. Contains: Pierce 660nm Protein Assay Reagent Pre-Diluted Protein Assay Standards, Bovine Serum Albumin (BSA) Set 3.5mL each of 125- 2,000mg/mL BSA	Kit 450mL
22663	Ionic Detergent Compatibility Reagent Sufficient for treating 100mL Pierce 660nm Protein Assay Reagent. 5 pouches, 1 gram each	5 x 1g

BCA-based Protein Assays

Bicinchoninic Acid (BCA)-based Protein Assays

In 1985, Paul K. Smith, *et al.* introduced the BCA Protein Assay. Since then it has become the most popular method for colorimetric detection and quantitation of total protein. The BCA Protein Assay has a unique advantage over the Modified Lowry Protein Assay and any of the Coomassie dye-based assays – it is compatible with samples that contain up to 5% surfactants (detergents).


Briefly, the sample is added to the tube or plate containing the prepared BCA Working Reagent and after a 30-minute incubation at 37°C and cooling to room temperature, the resultant purple color is measured at 562nm. The protocol is similar for the Micro BCA Protein Assay, except the ratio of sample volume to working reagent is different and the tubes are incubated for 60 minutes at 60°C.

Chemistry of BCA-based Protein Assays

The BCA Protein Assay combines the well-known reduction of Cu^{2+} to Cu^{1+} by protein in an alkaline medium with the highly sensitive and selective colorimetric detection of the cuprous cation (Cu^{1+}) by bicinchoninic acid (Figure 1). The first step is the chelation of copper with protein in an alkaline environment to form a blue colored complex. In this reaction, known as the biuret reaction, peptides containing three or more amino acid residues form a colored chelate complex with cupric ions in an alkaline environment containing sodium potassium tartrate. This became known as the biuret reaction because a similar complex forms with the organic compound biuret ($\text{NH}_2\text{-CO-NH-CO-NH}_2$) and the cupric ion. Biuret, a product of excess urea and heat, reacts with copper to form a light blue tetradentate complex (Figure 2). Single amino acids and dipeptides do not give the biuret reaction, but tripeptides and larger polypeptides or proteins will react to produce the light blue to violet complex that absorbs light at 540nm. One cupric ion forms a colored coordination complex with four to six nearby peptides bonds.

The intensity of the color produced is proportional to the number of peptide bonds participating in the reaction. Thus, the biuret reaction is the basis for a simple and rapid colorimetric reagent of the same name for quantitatively determining total protein concentration. Since the working range for the biuret assay is from 5 to 160mg/mL, the biuret assay is used in clinical laboratories for the quantitation of total protein in serum.

Step 1.



Step 2.

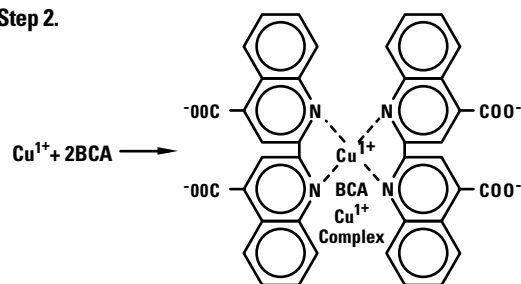


Figure 1. Reaction schematic for the bicinchoninic acid (BCA)-containing protein assay.

BCA-based Protein Assays

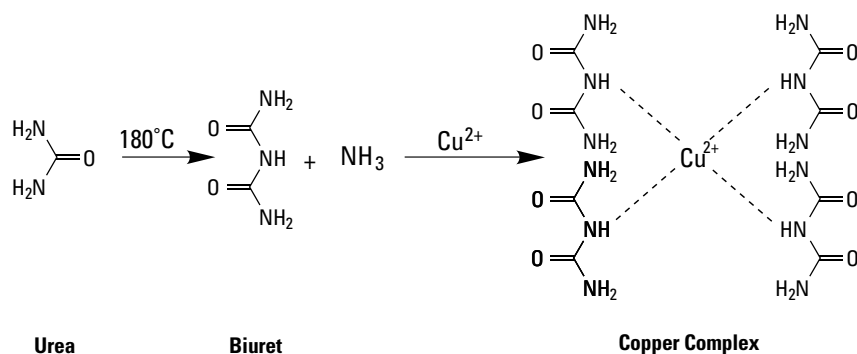


Figure 2. Biuret reaction schematic.

In the second step of the color development reaction, BCA Reagent, a highly sensitive and selective colorimetric detection reagent reacts with the cuprous cation (Cu^{1+}) that was formed in step 1. The purple colored reaction product is formed by the chelation of two molecules of BCA Reagent with one cuprous ion (Figure 1). The BCA/Copper Complex is water-soluble and exhibits a strong linear absorbance at 562nm with increasing protein concentrations. The purple color may be measured at any wavelength between 550-570nm with minimal (less than 10%) loss of signal. The BCA Reagent is approximately 100 times more sensitive (lower limit of detection) than the biuret reagent. The reaction that leads to BCA Color Formation as a result of the reduction of Cu^{2+} is also strongly influenced by the presence of any of four amino acid residues (cysteine or cystine, tyrosine, and tryptophan) in the amino acid sequence of the protein. Unlike the Coomassie dye-binding methods that require a minimum mass of protein to be present for the dye to bind, the presence of only a single amino acid residue in the sample may result in the formation of a colored BCA- Cu^{1+} Chelate. This is true for any of the four amino acids cited above. Studies performed with di- and tripeptides indicate that the total amount of color produced is greater than can be accounted for by the color produced with each BCA Reagent-reactive amino acid. Therefore, the peptide backbone must contribute to the reduction of copper as well.

The rate of BCA Color Formation is dependent on the incubation temperature, the types of protein present in the sample and the relative amounts of reactive amino acids contained in the proteins. The recommended protocols do not result in end-point determinations, the incubation periods were chosen to yield maximal color response in a reasonable time frame.

Advantages of the BCA Protein Assay

The primary advantage of the BCA Protein Assay is that most surfactants (even if present in the sample at concentrations up to 5%) are compatible. The protein:protein variation in the amount of color produced with the BCA Protein Assay is relatively low, similar to that observed for the Modified Lowry Protein Assay (Table 2, page 9).

The BCA Protein Assay produces a linear response curve ($r^2 > 0.95$) and is available in two formulations based upon the dynamic range needed to detect the protein concentration of an unknown sample. The BCA Assay is less complicated to perform than the Lowry Protein Assay for both formulations. The standard BCA Protein Assay (Figure 3) detects protein concentrations from 20 to 2,000 $\mu\text{g}/\text{mL}$ and is provided with Reagent A (carbonate buffer containing BCA Reagent) and Reagent B (cupric sulfate solution). A working solution (WS) is prepared by mixing 50 parts of BCA Reagent A with 1 part of BCA Reagent B (50:1, Reagent A:B). The working solution is an apple green color that turns purple after 30 minutes at 37°C in the presence of protein. The ratio of sample to WS used is 1:20. The Micro BCA Protein Assay (Figure 4) is more sensitive and has a narrower dynamic range of 0.1-25 $\mu\text{g}/\text{mL}$. To prepare the Micro BCA WS, three reagents (A, B and C) are mixed together at a ratio of 25 parts Micro Reagent A to 24 parts Micro Reagent B and 1 part Micro Reagent C. The Micro BCA WS is mixed with the sample or standard at a 1:1 volume ratio. The purple color response is read at 562nm after 1 hour at 60°C.

Since the color reaction is not a true end-point reaction, considerable protocol flexibility is allowed with the BCA Protein Assay. By increasing the incubation temperature, the sensitivity of the assay can be increased. When using the enhanced tube protocol (incubating at 60°C for 30 minutes), the working range for the assay shifts to 5-250 $\mu\text{g}/\text{mL}$ and the minimum detection level becomes 5 $\mu\text{g}/\text{mL}$.

Both BCA Protein Assay formulations have less protein:protein variability than the Coomassie-based assays. The color response obtained for a seven point standard curve with the standard BCA Protein Assay using BSA or BGG standards shows less than a 20% variation between these two proteins (Figure 3). The Coomassie assay demonstrates >30% variation in the signal generated between BSA and BGG (Table 2, page 9). There is even less variation (<12%) when comparing these protein standards with the Micro BCA Protein Assay (Figure 4). In general, the BCA Protein Assay provides one of the most accurate measurements of protein concentration in biological samples, is detergent-compatible and simple to perform.

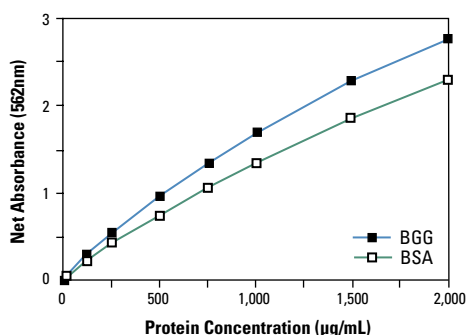


Figure 3. Color response curves obtained with the Thermo Scientific BCA Protein Assay using bovine serum albumin (BSA) and bovine gamma globulin (BGG). The standard tube protocol was performed and the color was measured at 562nm.

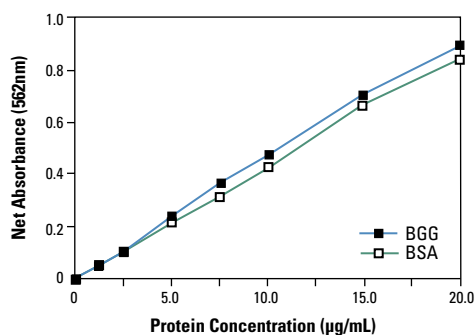


Figure 4. Color response curves obtained with the Thermo Scientific Micro BCA Protein Assay using bovine serum albumin (BSA) and bovine gamma globulin (BGG). The standard tube protocol was performed and the color was measured at 562nm.

Disadvantages of the BCA Protein Assay

Substances that reduce copper will also produce color in the BCA Assay, thus interfering with the accuracy of the protein quantitation. Reagents that chelate the copper also interfere by reducing the amount of BCA color produced with protein. Certain single amino acids (cysteine or cystine, tyrosine and tryptophan) will also produce color and interfere in BCA Assays.

BCA-based Protein Assays

BCA Protein Assay – Reducing Agent Compatible

The Thermo Scientific Pierce BCA Assay is always compatible with more detergents, buffers/salts and solvents than any other colorimetric protein assay. Now it's compatible with reducing agents at concentrations routinely used in protein sample buffers!



The BCA Assay provides one of the most accurate measurements of protein concentration in biological samples available. Although the BCA Assay is compatible with more detergents, buffers/salts and solvents than any colorimetric protein assay, the presence of disulfide reducing agents, including dithiothreitol (DTT) and 2-mercaptoethanol interferes with the assay. The BCA Protein Assay Kit – Reducing Agent Compatible (Product # 23250) provides all the advantages of the original BCA Assay as well as compatibility with reducing agents at concentrations routinely used in protein sample buffers (Figures 1 and 2).

Highlights:

- Compatible with up to 5mM DTT, 35mM 2-mercaptoethanol or 10mM TCEP
- No protein precipitation required
- Linear working range: 125-2,000µg/mL
- Sample volume: 25µL
- Compatible with most ionic and nonionic detergents
- Significantly less protein:protein variation than coomassie (Bradford)-based methods
- Colorimetric method; measure at 562nm
- Easy-to-use protocol (Figure 2)

Reference

Smith, P.K., *et al.* (1985). Measurement of protein using bicinchoninic acid. *Anal. Biochem.* **150**, 76-85.

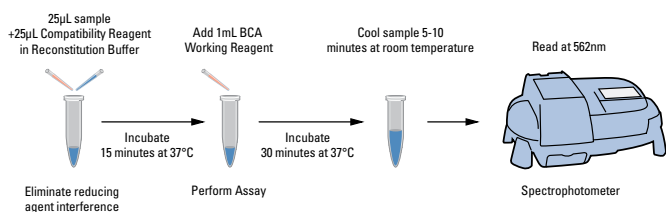


Figure 2. Thermo Scientific Pierce BCA Protein Assay – Reducing Agent Compatible protocol.

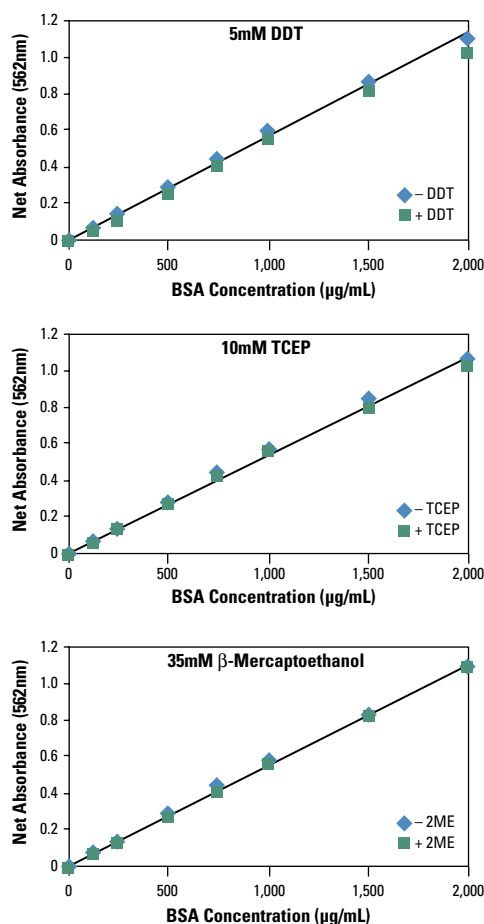


Figure 1. Thermo Scientific Pierce BCA Protein Assay – Reducing Agent Compatible produces a linear standard curve in the presence of reducing agents. Color response curves for BSA after treatment with Reducing Agent Compatible Reagent in the presence and absence of 5mM DTT, 35mM β-mercaptoethanol and 10mM TCEP.

Ordering Information

Product	Description	Pkg. Size
23250	BCA Protein Assay Kit – Reducing Agent Compatible Sufficient reagents to perform 250 standard tube assays. Includes: BCA Reagent A BCA Reagent B Compatibility Reagent Reconstitution Buffer Albumin Standard (2mg/mL)	750mL 250mL 25mL 10 x 20mg 15mL 10 x 1mL ampules
23252	Microplate BCA Protein Assay Kit – Reducing Agent Compatible Sufficient reagents for 1,000 microplate assays. Includes: BCA Reagent A BCA Reagent B Compatibility Reagent Reconstitution Buffer Albumin Standard (2mg/mL)	Kit 250mL 25mL 48 x 10mg 15mL 10 x 1mL ampules 20/pkg.
	96-Well Microplates	

The Original BCA Protein Assay

Used in more labs than any other detergent-compatible formulation.



Highlights:


- Colorimetric method; read at 562nm
- Compatible with most ionic and nonionic detergents
- Four times faster and easier than the classical Lowry method
- All reagents stable at room temperature for two years
- Working reagent stable for 24 hours
- Linear working range for BSA from 20 to 2,000µg/mL
- Minimum detection level of 5µg/mL with the enhanced protocol
- Convenient microplate or cuvette format
- Less protein:protein variation than dye-binding methods

Ordering Information

Product	Description	Pkg. Size
23225	BCA Protein Assay Kit Sufficient reagents to perform 500 standard tube assays or 5,000 microplate assays. Includes: Reagent A Reagent B Albumin Standard (2mg/mL)	Kit 2 x 50mg 25mL 10 x 1mL ampules
23227	BCA Protein Assay Kit Sufficient reagents to perform 250 standard tube assays or 2,500 microplate assays. Includes: Reagent A Reagent B Albumin Standard (2mg/mL)	Kit 1 x 500mL 25mL 10 x 1mL ampules
23221	BCA Protein Assay Reagent A Contains: BCA and tartrate in an alkaline carbonate buffer	250mL
23223	BCA Protein Assay Reagent A Contains: BCA and tartrate in an alkaline carbonate buffer	1,000mL
23222	BCA Protein Assay Reagent A Contains: BCA and tartrate in an alkaline carbonate buffer	3.75 liter
23224	BCA Protein Assay Reagent B Contains: 4% CuSO ₄ •5H ₂ O	25mL
23230	BCA Protein Assay Reagent A Recrystallized purified powder	25g
23228	BCA Protein Assay Reagent A Contains: BCA and tartrate in an alkaline carbonate buffer	500mL

References

- Smith, P.K., *et al.* (1985). *Anal. Biochem.* **150**, 76-85.
 Sorensen, K. (1992). *BioTechniques* **12**(2), 235-236.
 Ju, T., *et al.* (2002). *J. Biol. Chem.* **277**, 178-186.
 Shibuya, T., *et al.* (1989). *J. Tokyo Mid. College* **47**(4), 677-682.
 Hinson, D.L. and Webber, R.J. (1988). *BioTechniques* **6**(1), 14, 16, 19.
 Akins, R.E. and Tuan, R.S. (1992). *BioTechniques* **12**(4), 469-499.
 Tyllianakis, P.E., *et al.* (1994). *Anal. Biochem.* **219**(2), 335-340.
 Gates, R.E. (1991). *Anal. Biochem.* **196**(2), 290-295.
 Stich, T.M. (1990). *Anal. Biochem.* **191**, 343-346.
 Tuszynski, G.P. and Murphy, A. (1990). *Anal. Biochem.* **184**(1), 189-191.

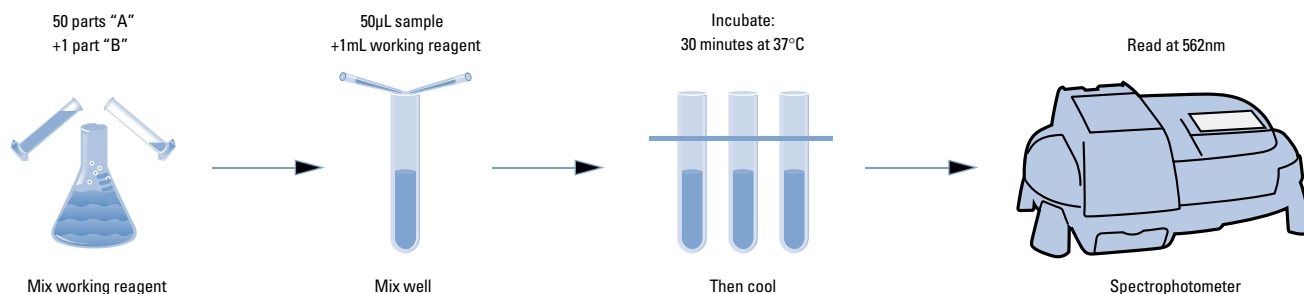

Thermo Scientific Pierce BCA Protein Assay protocol.

BCA-based Protein Assays

Micro BCA Protein Assay

Most sensitive BCA formulation measuring dilute protein solutions from 0.5 to 20 μ g/mL.

Highlights:


- Colorimetric method; read at 562nm
- Compatible with most ionic and nonionic detergents
- A very sensitive reagent for dilute protein samples
- Linear working range for BSA: 0.5-20 μ g/mL
- Less protein:protein variation than dye-binding methods
- All kit reagents stable at room temperature for two years
- Working reagent is stable for 24 hours
- Convenient microplate or cuvette format

References

- Smith, P.K., *et al.* (1985). *Anal. Biochem.* **150**(1), 76-85.
Kang, D.E., *et al.* (2002). *Cell* **110**, 751-762.
Rawadi, G., *et al.* (1999). *J. Immunol.* **162**, 2193-2203.
Blum, D., *et al.* (2002). *J. Neurosci.* **22**, 9122-9133.
Paratcha, G., *et al.* (2003). *Cell* **113**, 867-879.

Ordering Information

Product	Description	Pkg. Size
23235	Micro BCA Protein Assay Kit Sufficient reagents to perform 480 standard tube assays or 3,200 microplate assays. Includes: Micro Reagent A (MA) (Sodium carbonate, sodium bicarbonate, and sodium tartrate in 0.2 N NaOH) Micro Reagent B (MB) (4% BCA in water) Micro Reagent C (MC) (4% cupric sulfate pentahydrate in water) Albumin Standard Ampules (2mg/mL)	Kit 240mL 240mL 12mL
23231	Micro BCA Reagent A (MA)	240mL
23232	Micro BCA Reagent B (MB)	240mL
23234	Micro BCA Reagent C (MC)	12mL
23209	Albumin Standard Ampules, 2mg/mL Contains: Bovine Albumin Fraction V in 0.9% NaCl solution containing sodium azide	Kit

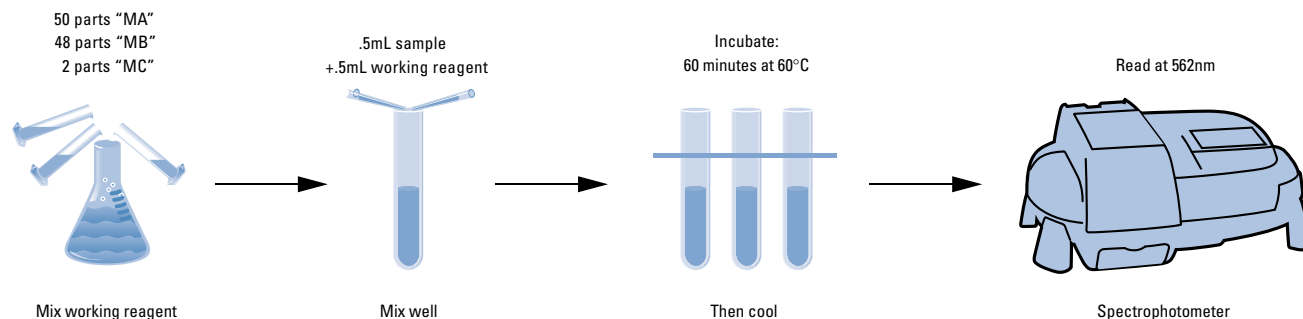

Thermo Scientific Pierce Micro BCA Protein Assay protocol.

Coomassie Dye-based Protein Assays

Coomassie Dye-based Protein Assays (Bradford Assays)

Use of Coomassie G-250 Dye in a colorimetric reagent for the detection and quantitation of total protein was first described by Dr. Marion Bradford in 1976. Both the Coomassie (Bradford) Protein Assay Kit (Product # 23200) and the Coomassie Plus (Bradford) Assay Kit (Product # 23236) are modifications of the reagent first reported by Dr. Bradford.

Chemistry of Coomassie-based Protein Assays

In the acidic environment of the reagent, protein binds to the Coomassie dye. This results in a spectral shift from the reddish/brown form of the dye (absorbance maximum at 465nm) to the blue form of the dye (absorbance maximum at 610nm) (Figure 1). The difference between the two forms of the dye is greatest at 595nm, so that is the optimal wavelength to measure the blue color from the Coomassie dye-protein complex. If desired, the blue color can be measured at any wavelength between 575nm

and 615nm. At the two extremes (575nm and 615nm) there is a loss of about 10% in the measured amount of color (absorbance) compared to that obtained at 595nm.

Development of color in Coomassie dye-based protein assays has been associated with the presence of certain basic amino acids (primarily arginine, lysine and histidine) in the protein. Van der Waals forces and hydrophobic interactions also participate in the binding of the dye by protein. The number of Coomassie dye ligands bound to each protein molecule is approximately proportional to the number of positive charges found on the protein. Free amino acids, peptides and low molecular weight proteins do not produce color with Coomassie dye reagents. In general, the mass of a peptide or protein must be at least 3,000 daltons to be assayed with this reagent. In some applications this can be an advantage. The Coomassie (Bradford) Protein Assay has been used to measure "high molecular weight proteins" during fermentation in the beer brewing industry.

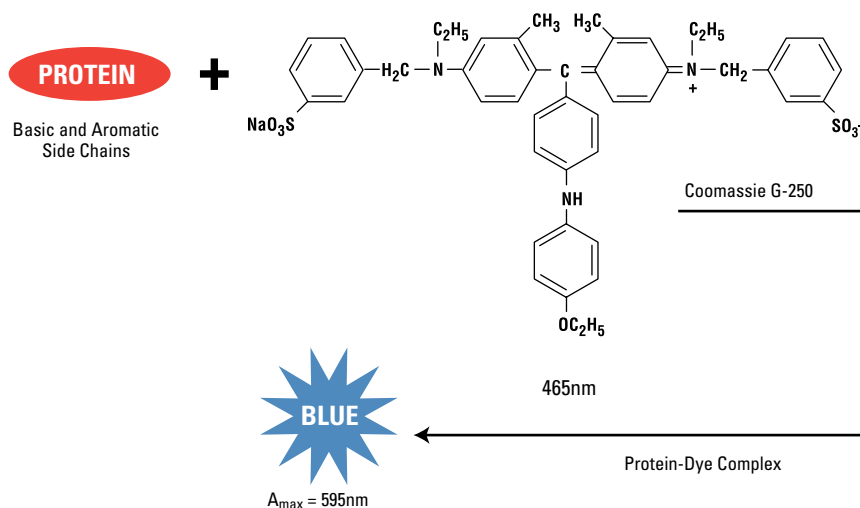


Figure 1. Reaction schematic for the Coomassie dye-based protein assays (the Coomassie [Bradford] Protein Assay and the Coomassie Plus [Bradford] Assay).

Advantages of Coomassie-based Protein Assays

Coomassie dye-binding assays are the fastest and easiest to perform of all protein assays. The assay is performed at room temperature and no special equipment is required. Briefly, for either the Coomassie (Bradford) Protein Assay or the Coomassie Plus Assay, the sample is added to the tube containing reagent and the resultant blue color is measured at 595nm following a short room-temperature incubation. The Coomassie dye-containing protein assays are compatible with most salts, solvents, buffers, thiols, reducing substances and metal chelating agents encountered in protein samples.

Disadvantages of Coomassie-based Protein Assays

The main disadvantage of Coomassie-based protein assays is their incompatibility with surfactants at concentrations routinely used to solubilize membrane proteins. In general, the presence of a surfactant in the sample, even at low concentrations, causes precipitation of the reagent. Since the Coomassie dye reagent is highly acidic, a small number of proteins cannot be assayed with this reagent due to their poor solubility in the acidic reagent. Also, Coomassie reagents result in about twice as much protein:protein variation as copper chelation based assay reagents (Table 2, page 9). In addition, Coomassie dye stains the glass or quartz cuvettes used to hold the solution in the spectrophotometer while the color intensity is being measured. (Cuvettes can be cleaned with strong detergent solutions and/or methanol washes, but use of disposable polystyrene cuvettes eliminates the need to clean cuvettes.)

Coomassie Dye-based Protein Assays

General Characteristics of Coomassie-based Protein Assays (Bradford Assays)

Coomassie-based protein assays share a number of characteristics. The Coomassie (Bradford) Protein Assay produces a non-linear standard curve. The Coomassie Plus (Bradford) Assay has the unique advantage of producing a linear standard curve over part of its total working range. When using bovine serum albumin (BSA) as the standard, the Coomassie Plus Assay is linear from 125 to 1,000 $\mu\text{g/mL}$. When using bovine gamma globulin (BGG) as the standard, the Coomassie Plus Assay is linear from 125 to 1,500 $\mu\text{g/mL}$. The complete working range of the Coomassie Plus Assay covers the concentration range from 125 to 1,000 $\mu\text{g/mL}$ for the tube protocol and from 1 to 25 $\mu\text{g/mL}$ for the micro protocol (Figures 2-3).

Coomassie dye-based protein assays must be refrigerated for long-term storage. If ready-to-use liquid Coomassie dye reagents will be used within one month, they may be stored at ambient temperature (18-26°C). Coomassie protein assay reagent that has been left at room temperature for several months will

have a lower color response, especially at the high end of the working range. Coomassie protein assay reagents that have been stored refrigerated must be warmed to room temperature before use. Using either cold plates or cold liquid Coomassie dye reagent will result in low absorbance values.

The ready-to-use liquid Coomassie dye reagents must be mixed gently by inversion just before use. The dye in these liquid reagents spontaneously forms loose aggregates upon standing. These aggregates may become visible after the reagent has been standing for as little as 60 minutes. Gentle mixing of the reagent by inversion of the bottle will uniformly disperse the dye. After binding to protein, the dye also forms protein-dye aggregates. Fortunately, these protein-dye aggregates can be dispersed easily by mixing the reaction tube. This is common to all liquid Coomassie dye reagents. Since these aggregates form relatively quickly, it is also best to routinely mix (vortex for 2-3 seconds) each tube or plate just before measuring the color.

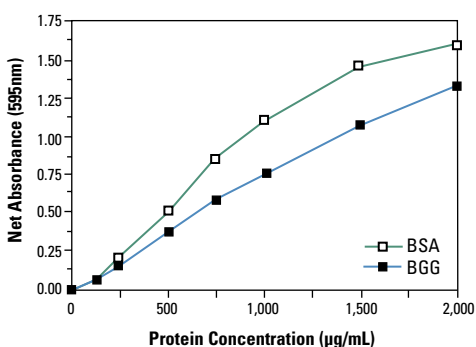


Figure 2. Color response curves obtained with Thermo Scientific Pierce Coomassie Plus (Bradford) Assay using bovine serum albumin (BSA) and bovine gamma globulin (BGG). The standard tube protocol was performed and the color was measured at 595nm.

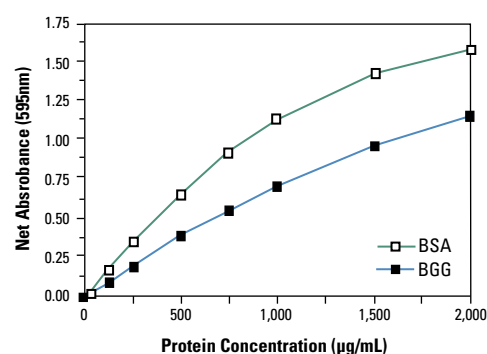


Figure 3. Color response curves obtained with Thermo Scientific Pierce Coomassie (Bradford) Protein Assay using bovine serum albumin (BSA) and bovine gamma globulin (BGG). The standard tube protocol was performed and the color was measured at 595nm.

Coomassie Plus (Bradford) Protein Assay

As fast as the original Coomassie Assay, with increased accuracy ... the high-performance Bradford reagent.

- **Easier, quicker preparation**

Working reagent is ready to use. No tedious dilution, no filtration of a dye concentrate and no mess to clean up.

- **Lower cost per assay**

Just 23¢ per sample with the standard protocol, and less than 5¢ per sample with the microplate protocol.

- **Faster assay**


Total assay time is less than 10 minutes!

- **More accurate results**

Substantially increased linearity of response, and only half the expected protein:protein variation of other commercial formulations.

Highlights:

- Detects protein concentrations from 1 to 1,500 µg/mL
- Ready-to-use dye-binding reagent formulation
- Fast (almost immediate) color development read at 595nm
- Compatible with reducing sugars, reducing substances and thiols
- Refrigerated reagent is stable for up to two years
- Superior linear response over the range of 125-1,500 µg/mL
- Convenient microplate or cuvette format
- Micro protocol useful for protein concentrations from 1 to 25 µg/mL

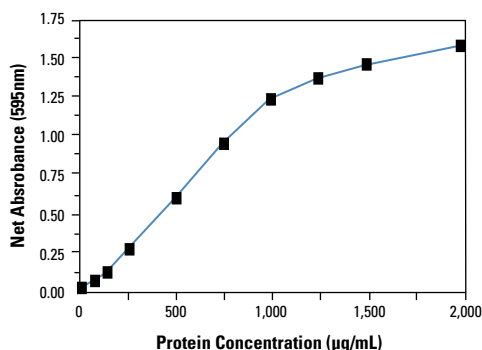

Typical color response curve for BSA using the Thermo Scientific Pierce Coomassie Plus (Bradford) Protein Assay Reagent.

References


Bradford, M. (1976). *Anal. Biochem.* **72**, 248-254.
 Glover, B.P. and McHenry, C.S. (2001). *Cell* **105**, 925-934.
 Kagan, A., et al. (2000). *J. Biol. Chem.* **275**, 11241-11248.
 Goel, R., et al. (2002). *J. Biol. Chem.* **277**, 18640-18648.

Ordering Information

Product	Description	Pkg. Size
23236	Coomassie Plus (Bradford) Assay Kit Sufficient reagents to perform 630 standard assays or 3,160 microplate assays. Includes: Coomassie Plus Protein Assay Reagent Albumin Standard (2mg/mL)	Kit 950mL 10 x 1mL ampules
23238	Coomassie Plus (Bradford) Reagent Sufficient reagents to perform 200 standard assays or 1,000 microplate assays. Albumin Standard not included.	300mL

Related Products

Product	Description	Pkg. Size
23239	Coomassie Plus Compat-Able Protein Assay Kit	Kit

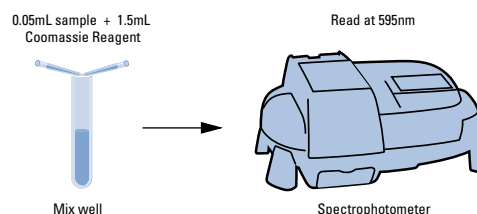

Thermo Scientific Pierce Coomassie Plus (Bradford) Assay protocol.

The protocol is simple, fast and very easy to perform.

Compatible Substances

Reagents compatible with Coomassie Plus Assay using the standard protocol. Interferences may be observed at the stated concentration when using the Micro Assay Procedure.

Ammonium Sulfate	1.0M	2-Mercaptoethanol	1.0M
Azide	0.5%	MES	100mM
Brij-56	0.03%	NaCl	5.0M
Brij-35	0.06%	NaOH	0.1M
Brij-58	0.016%	NP-40	0.5%
CHAPS	5.0%	SDS	0.016%
CHAPSO	5.0%	Sucrose	10.0%
Citrate	200mM	Tris	2.0M
EDTA	100mM	Triton X-100	0.06%
Glucose	1.0M	Triton X-114	0.06%
Glycine	0.1M	Triton X-405	0.25%
Guanidine•HCl	3.5M	Tween-20	0.03%
HCl	0.1M	Tween-80	0.016%
KSCN	3.0M	Urea	3.0M

Coomassie Dye-based Protein Assays


Coomassie (Bradford) Protein Assay

The Bradford method workhorse ... ready-to-use, allowing total protein determination in seconds!


This ready-to-use formulation more closely resembles in performance, the reagent published by Bradford.¹ It demonstrates the typical assay characteristics known for Coomassie dye-based formulations.²

Highlights:

- Ready-to-use dye-binding reagent formulation
- Fast (almost immediate) color development; read at 595nm
- Compatible with reducing substances and chelating agents
- Refrigerated reagent is stable for 12 months
- Determine protein concentration from 100 to 1,500µg/mL
- Micro method for the range of 1 to 25µg/mL
- Convenient microplate or cuvette format

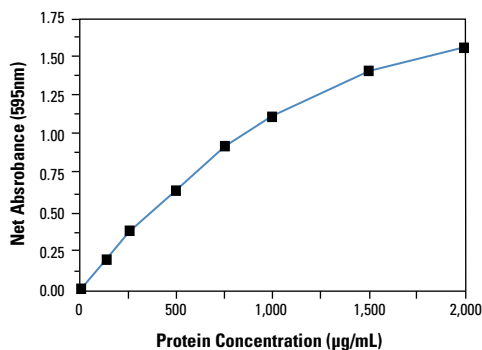

Thermo Scientific Pierce Coomassie (Bradford) Protein Assay Reagent: typical color response curve for BSA.

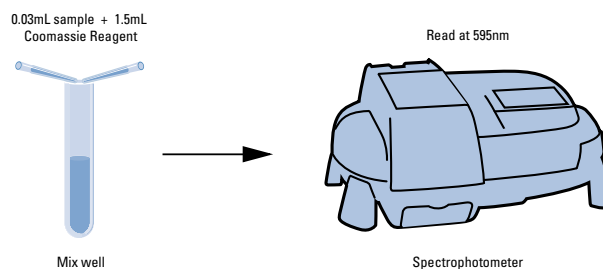

Thermo Scientific Pierce Coomassie (Bradford) Protein Assay protocol.

Ordering Information

Product	Description	Pkg. Size
23200	Coomassie (Bradford) Protein Assay Kit (Ready-to-use Coomassie Blue G-250 based reagent) <i>Sufficient reagents to perform 630 standard tube assays or 3,800 microplate assays.</i> Includes: Coomassie Protein Assay Reagent Albumin Standard Ampules (2mg/mL)	Kit 950mL 10 x 1mL

References

1. Bradford, M. (1976). *Anal. Biochem.* **72**, 248-254.
2. VanKley, H. and Hale, S.M. (1977). *Anal. Biochem.* **81**, 485-487.
- Messenger, M.M., et al. (2002). *J. Biol Chem.* **277**, 23054-23064.

Removal of Interfering Substances

Removing Interfering Substances

Virtually every protein detection method known exhibits sensitivity to the presence of particular reagents in the protein sample. Proteins are typically found in solutions that contain detergents, buffer salts, denaturants, reducing agents, chaotropic agents and/or anti-microbial preservatives. These additives may affect the results of an assay. When a component of a protein solution artificially increases or decreases the signal of any assay, the component is considered to be an interfering substance.

Interfering substances can affect the protein assay in the following ways:

- They can suppress the response of an assay
- They can enhance the response of an assay
- They can result in an elevated background reading

A small amount of interference from many common substances can be compensated for in the blank designed for a specific assay. To compensate for the interference, the protein samples for the standard curve must be diluted in the same buffer as the protein being assayed.

Often, interfering substances can overwhelm the assay, making it difficult or impossible to perform. The two most popular assay methods, Lowry- or Bradford-based assays, are both strongly affected by various components found in standard sample buffers. Lowry-based methods are incompatible with reducing and chelating agents; DTT, β -mercaptoethanol, cysteine, EDTA and some sugars while Bradford-based methods are incompatible with most detergents. Unfortunately, many common sample buffers contain both reducing agents and detergents, Laemmli buffer for example.

In these situations, the interfering substance can be removed by a variety of means, of which gel filtration and dialysis are the most common. However both of these methods are time-consuming and can result in diluted protein samples.

The Compat-Able Protein Assay Preparation Set (page 26) was developed to solve this problem. The Compat-Able Reagents render potentially interfering substances virtually invisible to either a Lowry- or Bradford-based assay. These unique reagents dispose of any possible interfering substances in your sample by selectively precipitating out the protein, allowing the non-protein sample components to be removed easily. Precipitated protein is recovered in water or an assay-compatible buffer and then assayed by any method.

In one round of treatment, Compat-Able Reagents can remove most any interfering substance, including but not limited to:

- Laemmli buffer
- 3.0M Tris
- 20% glycerol
- 4% SDS
- 3.6M magnesium chloride
- 1.25M sodium chloride
- 350mM dithiothreitol (DTT)
- 5% Triton X-100
- 5% Tween-20
- 125mM sodium citrate
- 200mM glucose
- 200mM sodium acetate
- 5% β -mercaptoethanol
- 200mM EDTA
- 1.0M imidazole

If concentrations of these or other interfering components exceed this level, more than one round of pre-treatment can be performed.

Removal of Interfering Substances

Compat-Able Protein Assays

Excellent choice for use with samples prepared for 1-D or 2-D electrophoresis.

These Thermo Scientific Kits pair BCA and Coomassie Plus (Bradford) Assays, recognized around the world as the best detergent- and reducing agent-compatible assays (respectively) for total protein analysis, with a great sample preparation reagent. These unique reagents dispose of any interfering substances in your sample by selectively precipitating the protein, allowing the nonprotein components to be removed easily. Precipitated protein is recovered in water and assayed with the BCA Protein Assay or Coomassie Plus Assay.


Highlights:

- Removes interfering substances prior to any downstream application
- Ready-to-use sample preparation reagents save time and effort
- Four-step protocol takes less than 10 minutes to complete
- Room temperature-stable sample preparation reagents can be stored on your bench top so they won't get lost in the cold room or hidden in the lab refrigerator
- Precipitates protein out of solution, leaving potentially interfering substances to be decanted away without dialysis or gel filtration, saving time and avoiding sample loss or dilution
- Easily adaptable to pre-treatment of many samples at one time
- Adaptable to both a test tube and microcentrifuge tube sample preparation protocol, to allow for 50 μ L or 100 μ L sample volumes
- Sample prep reagents are available with the BCA or Coomassie Assays or sold separately



Ordering Information

Product	Description	Pkg. Size
23229	BCA Compat-Able Protein Assay Kit Contains one each of the following: Product # 23227, BCA Protein Assay Kit <i>Sufficient reagents to perform 250 standard tube assays or 2,500 microplate assays.</i> BCA Reagent A BCA Reagent B BSA Standards (2mg/mL) Product # 23215, Compat-Able Protein Assay Preparation Reagent Set (see description below)	Kit 2 x 250mL 25mL 10 x 1mL
23239	Coomassie Plus Compat-Able Protein Assay Reagent Kit Contains one each of the following: Product # 23236, Coomassie Plus Protein Assay Reagent Kit <i>Sufficient materials for 630 standard assays, 950 microassays or 3,160 microplate assays.</i> Coomassie Plus Reagent Formulation BSA Standards (2mg/mL) Product # 23215, Compat-Able Protein Assay Preparation Reagent Set (see description below)	Kit 950mL 10 x 1mL
23215	Compat-Able Protein Assay Preparation Reagent Set <i>Two-reagent set with sufficient material to pre-treat up to 500 samples prior to total protein assay.</i> Compat-Able Protein Assay Preparation Reagent 1 Compat-Able Protein Assay Preparation Reagent 2	Kit 250mL 250mL

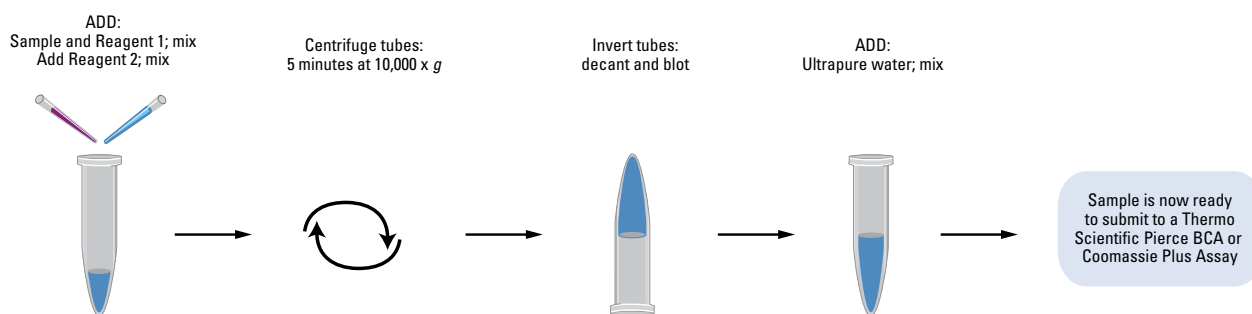

Thermo Scientific Compat-Able Protein Assay protocol. Make almost any protein sample compatible with the Thermo Scientific Pierce BCA or Coomassie Plus (Bradford) Assays in four simple steps.

Modified Lowry Protein Assay

Modified Lowry Protein Assay

Although the mechanism of color formation for the Modified Lowry Protein Assay is similar to that of the BCA Protein Assay, there are several significant differences between the two.

In 1951 Oliver H. Lowry introduced this colorimetric total protein assay method. It offered a significant improvement over previous protein assays and his paper became one of the most cited references in the life science literature. The Modified Lowry Protein Assay uses a stable reagent that replaces two unstable reagents described by Dr. Lowry. The Modified Lowry assay is easy to perform because the incubations are done at room temperature and the assay is sensitive enough to allow the detection of total protein in the low microgram per milliliter range. Essentially, the Modified Lowry protein assay is an enhanced biuret assay involving copper chelation chemistry.

Chemistry of the Modified Lowry Protein Assay

Although the mechanism of color formation for the Modified Lowry Protein Assay is similar to that of the BCA Protein Assay, there are several significant differences between the two. The exact mechanism of color formation in the Modified Lowry Protein Assay remains poorly understood. It is known that the color-producing reaction with protein occurs in two distinct steps. As seen in Figure 1, protein is first reacted with alkaline cupric sulfate in the presence of tartrate during a 10-minute incubation at room temperature. During this incubation, a tetradentate copper complex forms from four peptide bonds and one atom of copper. The tetradentate copper complex is light

blue in color (this is the “biuret reaction”). Following the incubation, Folin phenol reagent is added. It is believed that the color enhancement occurs when the tetradentate copper complex transfers electrons to the phosphomolybdic/phosphotungstic acid complex (the Folin phenol reagent).

The reduced phosphomolybdic/phosphotungstic acid complex produced by this reaction is intensely blue in color. The Folin phenol reagent loses its reactivity almost immediately upon addition to the alkaline working reagent/sample solution. The blue color continues to intensify during a 30-minute room temperature incubation. It has been suggested by Lowry, *et al.* and by Legler, *et al.* that during the 30-minute incubation, a rearrangement of the initial unstable blue complex leads to the stable final blue colored complex that has higher absorbance.

For small peptides, the amount of color increases with the size of the peptide. The presence of any of five amino acid residues (tyrosine, tryptophan, cysteine, histidine and asparagine) in the peptide or protein backbone further enhances the amount of color produced because they contribute additional reducing equivalents to further reduce the phosphomolybdic/phosphotungstic acid complex. With the exception of tyrosine and tryptophan, free amino acids will not produce a colored product with the Modified Lowry Reagent; however, most dipeptides can be detected. In the absence of any of the five amino acids listed above in the peptide backbone, proteins containing proline residues have a lower color response with the Modified Lowry Reagent due to the amino acid interfering with complex formation.

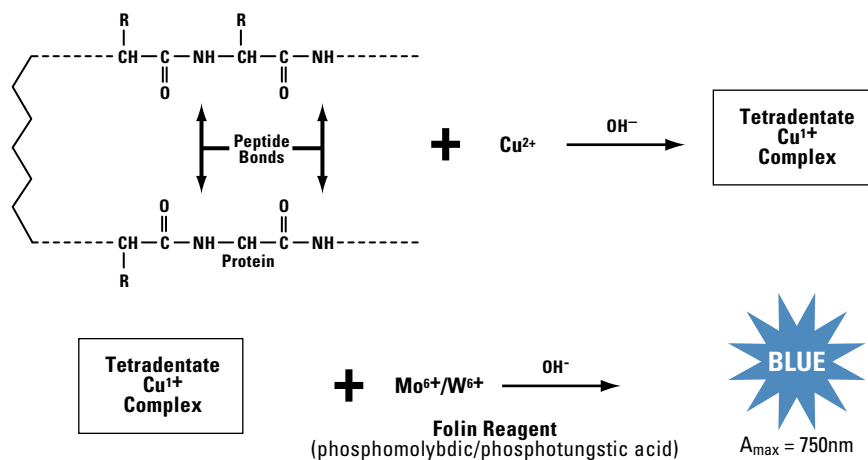


Figure 1. Reaction schematic for the Modified Lowry Protein Assay.

Modified Lowry Protein Assay

Advantages of the Modified Lowry Protein Assay

The final blue color is optimally measured at 750nm, but it can be measured at any wavelength between 650nm and 750nm with little loss of color intensity. It is best to measure the color at 750nm because few other substances absorb light at that wavelength. The amount of light absorbed at 750nm is directly proportional to the amount of protein in the sample, but the color response curve produced is nonlinear. The sensitivity of the Modified Lowry Protein Assay is greatly enhanced over that of the biuret reagent. The working range of the method extends from 5 to 2,000mg/mL.

The Modified Lowry Protein Assay demonstrates less protein:protein variability than Coomassie-based assays. When comparing the standard curve responses between BSA and BGG, there is less than a 15% variation in the signal generated with these two standard proteins (Figure 2). The Coomassie Protein Assay demonstrates > 30% variation in the signal generated between BSA and BGG (Table 2, page 9).

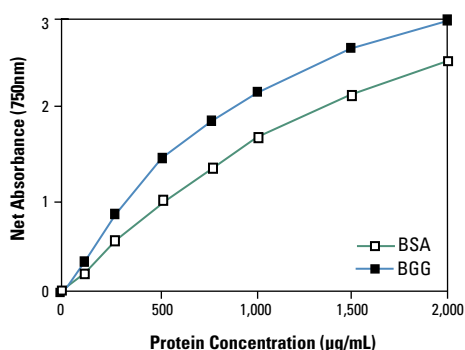


Figure 2. Color response curves obtained with the Thermo Scientific Pierce Modified Lowry Protein Assay Reagent using bovine serum albumin (BSA) and bovine gamma globulin (BGG). The standard tube protocol was performed and the color was measured at 750nm.

Disadvantages of the Modified Lowry Protein Assay

The Modified Lowry Protein Assay will form precipitates in the presence of detergents or potassium ions. The problem of precipitation caused by the presence of potassium ions in the sample can sometimes be overcome by centrifuging the tube and measuring the color in the supernatant. Most surfactants will cause precipitation of the reagent even at very low concentrations. One exception is sodium dodecyl sulfate (SDS), which is compatible with the reagent at concentrations up to 1% in the sample. Chelating agents interfere by binding copper and preventing formation of the copper peptide bond complex. Reducing agents and free thiols also interfere by reducing the phosphotungstate-phosphomolybdate complex, immediately forming an intensely blue colored product upon their addition to the Modified Lowry Protein Assay Reagent.

General Characteristics of the Modified Lowry Protein Assay

The Modified Lowry Protein Assay Reagent must be refrigerated for long-term storage. If the entire bottle of reagent will be used within one month, it may be stored at room temperature (18-26°C). Reagent that has been left at room temperature for more than one month may produce lower color response, especially at the higher end of the working range. If the reagent has been stored refrigerated, it must be warmed to room temperature before use. Using cold Modified Lowry Protein Assay Reagent will result in low absorbance values.


The protocol requires that the Folin phenol reagent be added to each tube precisely at the end of the 10-minute incubation. At the alkaline pH of the Lowry reagent, the Folin phenol reagent is almost immediately inactivated. Therefore, it is best to add the Folin phenol reagent at the precise time while simultaneously mixing each tube. Because this is somewhat cumbersome, some practice is required to obtain consistent results. This also limits the total number of samples that can be assayed in a single run. If a 10-second interval between tubes is used, the maximum number of tubes that can be assayed within 10 minutes is 60 (10 seconds/tube x 60 tubes = 600 seconds or 10 minutes).

Modified Lowry Protein Assay Reagent

All the accuracy of the Lowry, but modified so it's ready-to-use and stable for at least one year!

Highlights:

- The most widely cited colorimetric method; read at 750nm
- Ready-to-use reagent for the loyal Lowry method user
- Preformulated cupric sulfate-tartrate reagent stable for one year at room temperature
- Linear results from 1 to 1,500µg/mL for BSA
- Adaptable to microplates
- Less protein:protein variation than dye-binding methods

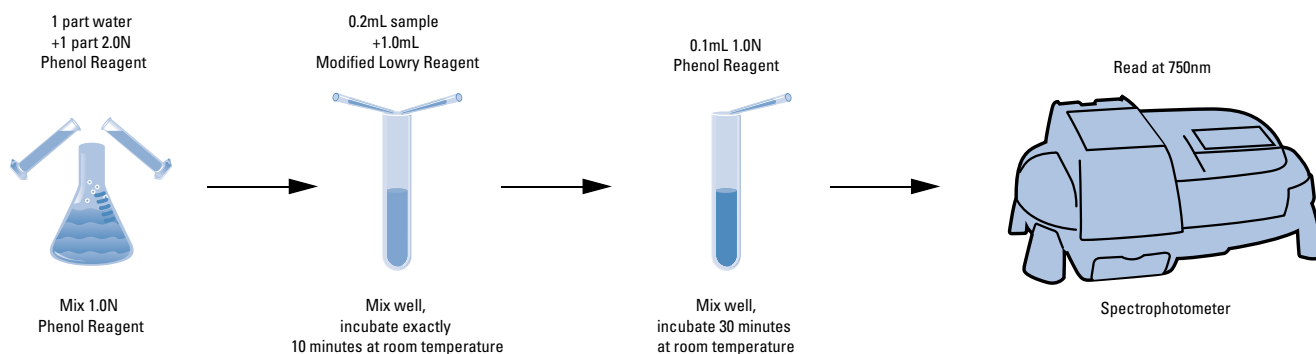

Thermo Scientific Pierce Modified Lowry Protein Assay Reagent protocol.

Ordering Information

Product	Description	Pkg. Size
23240	Modified Lowry Protein Assay Kit Sufficient reagents to perform 480 standard tube assays or 2,400 microplate assays. Includes: Modified Lowry Protein Assay Reagent 2 N Folin-Ciocalteu Phenol Reagent Albumin Standard Ampules (2mg/mL)	Kit 480mL 50mL 10 x 1mL

References

- Lowry, O.H., *et al.* (1951). *J. Biol. Chem.* **193**, 76-85.
Temel, R.E., *et al.* (2003). *J. Biol. Chem.* **278**, 4792-4799.

Total Protein Assays – Amine Detection


o-Phthalaldehyde [OPA] Fluorescent Protein Assay

The Thermo Scientific Pierce Fluoraldehyde Protein/Peptide Assay is an *o*-phthalaldehyde-based reagent developed to detect minute amounts of protein and peptides. Fluoraldehyde reactions are complete in less than one minute with sensitivity down to 50ng/mL. While some solutions interfere with protein/peptide measurement at 280nm, our Fluoraldehyde Assay is compatible with many substances that interfere with other protein assays, such as detergents and reducing agents. Amine-containing buffers must be avoided, however, when performing assays using this chemistry.

In the standard assay mode, the fluoraldehyde ready-to-use formulation can measure protein concentration in the range of 10 to 500µg/mL, while the micro-assay working range is 50ng/mL to 25µg/mL.

Our Fluoraldehyde Protein/Peptide Assay Reagent requires only 200µL of sample for use in a microplate assay, saving valuable sample and time. Fluoraldehyde assays require an excitation wavelength of 360nm and emission wavelength of 455nm.

OPA will react only with primary amines. When reacted with primary amines in the presence of mercaptoethanol, OPA yields an intense blue colored fluorescent product that has a maximum wavelength of excitation of 340nm and emission at 455nm.^{1,2} Wavelengths from 330-375nm have been used for excitation and 436-490nm for measuring emission. Protein concentrations as low

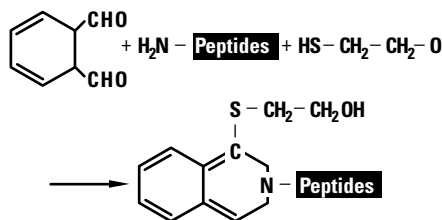


The reaction of *o*-Phthalaldehyde with a primary amine on a peptide in the presence of 2-mercaptoethanol to form a fluorescently labeled peptide.

Fluoraldehyde *o*-Phthalaldehyde Crystals

An easy, economical way to detect amino acids in pre- and post-column chromatographic effluents.

Highlights:



Fluoraldehyde
o-Phthalaldehyde
M.W. 134.13

- Stable in aqueous solution
- Highly sensitive, low background
- Rapid analysis, no heating required

as 50ng/mL can be measured with an OPA assay. The inherent sensitivity and speed of OPA, along with its broad linear range, makes it a useful protein and peptide assay reagent.

OPA is ideal for assaying peptides that do not contain tyrosine residues, or for other applications in which absorbance at 280nm cannot be used. Proteins and peptides tested yield linear results over a wide range of concentrations using both standard and microassay protocols.

There is considerable protein:protein and peptide:peptide variation with the OPA assay; therefore, it is best to use a purified sample of the particular protein or peptide as the standard. When this is not possible, the next best option is to use a protein or peptide that gives a response similar to the sample. Alternatively, a commonly accepted standard protein such as bovine serum albumin can be used.

Reducing agents and metal chelators do not interfere with an OPA-based assay, provided they are included in the blanks and standards. In addition, most detergents do not interfere. Any common sample buffers and constituents are also compatible, but primary amines such as Tris or glycine buffers will interfere with OPA and must be avoided. Acetylated and other primary amine-blocked peptides will not give a response with OPA.

References

1. Ogden, G. and Foldi, P. (1987). *LC•GC* **5**(1), 28-38.
2. Roth, M. (1971). *Anal. Chem.* **43**, 880-882.

Ordering Information


Product	Description	Pkg. Size
26015	Fluoraldehyde <i>o</i> -Phthalaldehyde Crystals	5g

References

- Lindroth, P. and Mopper, K. (1979). *Anal. Chem.* **51**, 1667-1674.
Lee, K.S. and Drescher, D.G. (1979). *J. Biol. Chem.* **254**, 6248-6251.
Van Eijk, H.M., et al. (1988). *Clin. Chem.* **34**, 2510-2513.
Graser, T.A., et al. (1985). *Anal. Biochem.* **151**, 142-152.
Cooper, J.D., et al. (1984). *Anal. Biochem.* **142**, 98-102.
Krishnamurti, C.R., et al. (1984). *J. Chromatogr.* **315**, 321-331.
Jones, B.N., et al. (1983). *J. Chromatogr.* **266**, 471-482.
Lee, H., et al. (1979). *Anal. Biochem.* **96**, 298-307.
Chen, R.F., et al. (1979). *Biochem. Biophys. Acta* **576**, 440-455.
Jones, B.N., et al. (1981). *J. Liq. Chrom.* **4**, 565-586.

Fluoraldehyde *o*-Phthalaldehyde Reagent Solution

Excellent sensitivity – an ideal choice when working with limited amounts of purified protein or peptides.



Fluoraldehyde *o*-Phthalaldehyde Reagent Solution

M.W. 134.13
 λ_{ex} = 340nm
 λ_{em} = 455nm

Thermo Scientific Pierce Fluoraldehyde Reagent Solution contains a stabilized, highly purified preparation of *o*-phthalaldehyde, Brij-35 Detergent and mercaptoethanol in a specially formulated borate buffer. It is a highly sensitive, ready-to-use reagent solution that exhibits excellent linear response (Figure 1) and offers outstanding shelf life (Figure 2). In addition, when compared to other *o*-phthalaldehyde detection reagents, our solution exhibits decreased background over time and a high signal:noise ratio.

Highlights:

- A ready-to-use, highly sensitive fluorescent pre- or post-column reagent for amino acid detection and quantitation
- Provides an accurate measure of both composition and absolute protein/peptide content
- Ready-to-use with no processing needed
- Reacts with all primary amine-containing analytes
- High sensitivity; low background

Application Note:

For even greater sensitivity, use a combination of OPA with Fmoc-Chloride with automated pre-column derivatization, detecting both primary and secondary amines. With this application, primary amino acids are first derivatized with OPA, while non-reacted secondary amino acids are then reacted with Fmoc-Chloride, resulting in extraordinary amino acid detection sensitivity and accuracy.^{1,2}

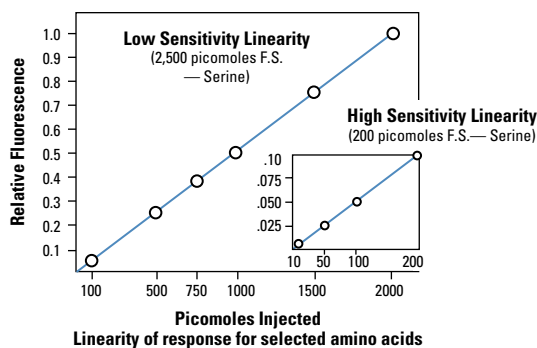


Figure 1. Excellent linear response. Thermo Scientific Pierce Fluoraldehyde Reagent Solution shows excellent linear response, whether in the 2,500 or 200 picomole range.

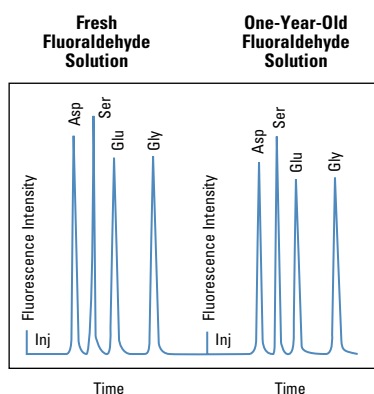


Figure 2. Outstanding shelf life. Comparison of fluorescence response of selected amino acids after reaction with recently prepared and one-year-old Thermo Scientific Pierce Fluoraldehyde Reagent Solutions.

Ordering Information

Product	Description	Pkg. Size
26025	Fluoraldehyde <i>o</i> -Phthalaldehyde Reagent Solution	945mL

References

1. Godel, H., et al. (1992). *LC-GC International* **5**, 44-49.
2. Schuster, R. (1988). *J. Chromatogr.* **431**, 271-284.
- Jones, B.N. and Gilligan, J.P. (1983). *American Biotechnology Laboratory*, Dec. Issue, 46-51.
- Benson, J.R. and Woo, D.J. (1984). *J. Chromatogr. Sci.* **22**, 386-399.

Specialty Assays – Histidine-tagged Proteins


Histidine-tagged Protein Detection

Thermo Scientific HisProbe-HRP Western blotting probe takes advantage of the affinity of histidine for the Ni²⁺ cation.

HisProbe-HRP is a nickel (Ni²⁺)-activated derivative of horse-radish peroxidase (HRP). This product has been optimized for direct detection of recombinant histidine-tagged proteins and other histidine-rich proteins. The active ligand is a tridentate chelator that allows Ni²⁺ to be bound in active form for subsequent interaction and detection of target molecules. The active chelator has similar binding capabilities to that reported for iminodiacetic acid, which has long been used for immobilized metal affinity chromatography (IMAC).

Highlights:


- Yields lower background than anti-histidine antibodies
- Pierce HRP is a high-activity enzyme
- Stripping and reprobing is possible
- HisProbe-HRP (Ni²⁺) can be used for detection of histidine-tagged proteins

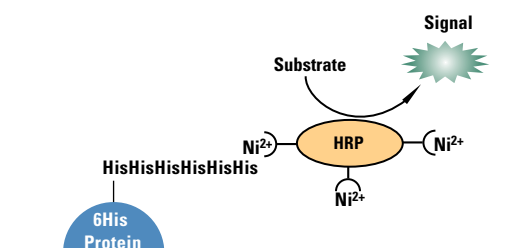

Detection of histidine-tagged fusion proteins with Thermo Scientific HisProbe-HRP.

Ordering Information

Product	Description	Pkg. Size
15165	HisProbe-HRP	1mg
15168	SuperSignal® West Pico HisProbe Kit	Kit
	Includes: HisProbe-HRP	2mg
	SuperSignal West Pico Chemiluminescent Substrate	500mL
	BSA in TBS (10X)	1 x 125mL
	BupH™ Tris Buffered Saline Packs	10 x 500mL
	Surfact-Amps® 20 (10%)	6 x 10 ampules

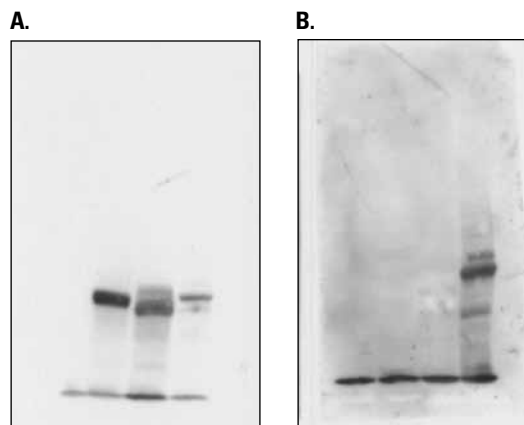

Panel A using Thermo Scientific HisProbe-HRP shows high specific binding and low background.

Panel B using anti-polyHis failed to recognize two of the three fusion proteins.

References

- Adler, J. and Bibi, E. (2004). Determinants of substrate recognition by the *Escherichia coli* multidrug transporter MdfA identified on both sides of the membrane. *J. Biol. Chem.* **279**, 8957-8965.
- Adler, J. and Bibi, E. (2005). Promiscuity in the geometry of electrostatic interactions between the *Escherichia coli* multidrug resistance transporter MdfA and cationic substrates. *J. Biol. Chem.* **280**, 2721-2729.
- Boulant, S., et al. (2003). Unusual multiple recoding events leading to alternative forms of hepatitis C virus core protein from genotype 1b. *J. Biol. Chem.* **278**, 45785-45792.
- Kanaya, E., et al. (2001). Zinc release from the CH₂C₆ zinc finger domain of filamentous flower protein from *Arabidopsis thaliana* induces self-assembly. *J. Biol. Chem.* **276**, 7383-7390.
- Robalino, J., et al. (2004). Two zebrafish eIF4E family members are differentially expressed and functionally divergent. *J. Biol. Chem.* **279**, 10532-10541.
- Robichon, C., et al. (2005). Depletion of apolipoprotein N-acyltransferase causes mislocalization of outer membrane lipoproteins in *Escherichia coli*. *J. Biol. Chem.* **280**, 974-983.
- Segawa, H., et al. (2005). Reconstitution of GDP-mannose transport activity with purified *Leishmania* LPG2 protein in liposomes. *J. Biol. Chem.* **280**, 2028-2035.
- Sundberg-Smith, L., et al. (2005). Adhesion stimulates direct PAK1/ERK2 association and leads to ERK-dependent PAK1 Thr212 phosphorylation. *J. Biol. Chem.* **280**, 2055-2064.
- Wagner, C., et al. (2005). Dimerization of NO-sensitive guanylyl cyclase requires the $\alpha 1$ N terminus. *J. Biol. Chem.* **280**, 17687-17693.
- Wann, E., et al. (2000). The fibronectin-binding MSCRAMM FnbpA of *Staphylococcus aureus* is a bifunctional protein that also binds to fibrinogen. *J. Biol. Chem.* **275**, 13863-13871.

Specialty Assays – Antibodies

Easy-Titer IgG and IgM Assay Kits

Simply the fastest, easiest way to quantitate antibodies ... ever!

It is no longer necessary to wait or to rely on inaccurate and insensitive UV or colorimetric IgG determination methods. It is not necessary to struggle with the inadequacies of methods that titrate antibody activity. It is even possible to avoid the tedious, time-consuming ELISA approach to determine antibody titer. Thermo Scientific Easy-Titer IgG Assay Kits make it possible to detect IgG in less time and with greater specificity and sensitivity than ever before.


Our Easy-Titer[®] Assay Kits do not cross-react with antibodies from other species such as bovine antibodies present in the media used to culture antibody-producing hybridoma cells. This remarkable specificity allows the measurement of human IgG concentrations from a variety of sample types such as culture supernatants, ascites or body fluids without first purifying the antibody from other contaminants.

Highlights:


- Easy-to-use particle-based antibody titer determination kit
- Start of assay to recovery of result in less than one hour
- Four times faster than classical ELISA-based protocols
- Convenient design – perform the assay in a 96-well plate and measure the result in a microplate reader
- Measures antibodies from culture supernatants ascites or body fluids
- Measures humanized antibodies and chimeras with intact Fc regions
- No cross-reactivity with Ig from other species




1. Suspend beads




2. Pipette 20 μ L beads




3. Pipette 20 μ L sample



4. Incubate on plate mixer; 5 minutes at room temperature




5. Add Blocking Buffer



6. Mix for 5 minutes on plate mixer



7. Read at 405/340nm



8. Plot Standard Curve; determine concentration of Human IgG or Human IgM

Thermo Scientific Easy-Titer IgG and IgM Assay Kit protocol. A simple assay makes for an easy-to-perform assay protocol. Easy-Titer IgG Assay Kits feature a simple procedure that reduces hands-on time and requires fewer steps that lead to more reproducible results. The entire process can be completed easily in about 30 minutes.

Specialty Assays – Antibodies

Performance Specifications:

Specificity

- Against all IgG subclasses (human, mouse or rabbit)

Sensitivity


- Detection limit: 15ng/mL
- Detection range (standard curve): 15 to 300ng/mL

Coefficient of Variation (intra- and interassay): < 5%

Reaction time: 10 minutes


- Read results at 340nm or 405nm

Standard curve calculations are compatible with software supplied for use with microplate readers.

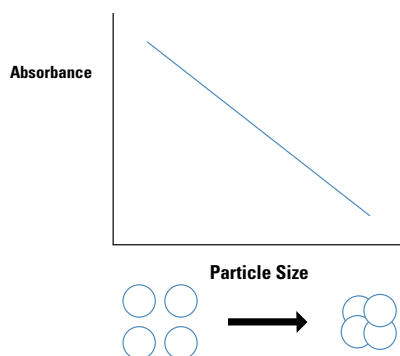

How the assay works:

- Monodisperse beads sensitized with a specific antibody absorb at 340 and 405nm
- The beads agglutinate in the presence of human IgG or IgM
- Larger diameter clusters form that absorb less efficiently at 340 and 405nm
- This decrease in absorbance is proportional to antibody concentration

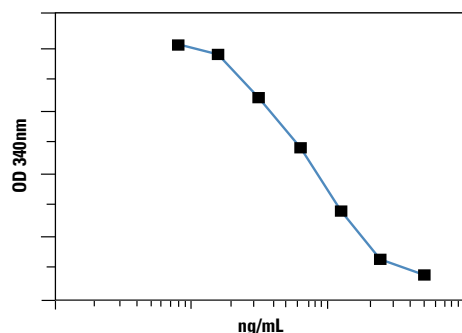

Typical standard curve for Thermo Scientific Easy-Titer Kit. The unknown concentration of IgG is easily determined on a standard curve constructed with serial dilutions of a standard sample.

Ordering Information

Product	Description	Pkg. Size
23310	Easy-Titer Human IgG Assay Kit* Sufficient reagents for 96 tests (87 determinations and one standard curve). Includes: Goat Anti-Human IgG	Kit 2mL
	Sensitized Polystyrene Beads [Monodispersed, polystyrene IgG (Fc) sensitized beads are supplied suspended in a phosphate buffer, pH 7.4 and stabilized with BSA and 0.1% sodium azide] Easy-Titer Dilution Buffer Easy-Titer Blocking Buffer	30mL 15mL
23315	Easy-Titer Human IgG Assay Kit* Includes: Goat Anti-Human IgG	Kit 2mL
	Sensitized Beads Easy-Titer Dilution Buffer Easy-Titer Blocking Buffer	30mL 15mL
23300	Easy-Titer Mouse IgG Assay Kit* Includes: Goat Anti-Mouse IgG	Kit 2mL
	Sensitized Beads Easy-Titer Dilution Buffer Easy-Titer Blocking Buffer	30mL 15mL
23305	Easy-Titer Rabbit IgG Assay Kit* Includes: Goat Anti-Rabbit IgG	Kit 2mL
	Sensitized Beads Easy-Titer Dilution Buffer Easy-Titer Blocking Buffer	30mL 15mL
23325	Easy-Titer Human IgG Assay Kit* Includes: Goat Anti-Human IgG	Kit 2mL

* Note: An IgG or IgM Standard is not included in these kits. Select the appropriate standard from the Related Products listed below.

Related Products

IgG Standards for Easy-Titer Kits

Product	Description	Pkg. Size
31154	Human IgG, Whole Molecule	10mg
31146	Human IgM, Whole Molecule	2mg
31204	Mouse IgG, Whole Molecule	5mg
31235	Rabbit IgG, Whole Molecule	10mg

Microplate Accessories

Product	Description	Pkg. Size
15041	96-Well Plates Corner Notch	100 plates
15031	8-Well Strip Plates Corner Notch Includes one strip well ejector per package.	100 plates
23325	Easy-Titer Human IgG (Gamma Chain) Assay Kit	Kit

Reference

Brown, M.A., et al. (2000). *J. Biol. Chem.* **275**, 19795-19802.

Specialty Assays – Proteases

Protease Assay Kits – Colorimetric and Fluorometric

Detects protease as low as 2ng/mL in less than one hour!


Thermo Scientific Pierce Protease Assay Kits are an ideal choice for performing routine assays necessary during the isolation of proteases, or for identifying the presence of contaminating proteases in protein samples. These protease assays are also ideal for studying pH or temperature vs. activity profiles of purified proteases.

Highlights:

- No corrosive precipitants used
- Entire assay can be run in microplates
- 1,000 times more sensitive, three times faster and uses half the sample of unmodified casein-based protease assays
- Total elapsed time to result – less than one hour
- Measure multiple samples simultaneously in ELISA plate readers
- Time/temperature/pH easily manipulated to optimize sensitivity

The colorimetric Protease Assay Kit uses fully succinylated casein as substrate for this assay. Hydrolysis of this readily soluble casein substrate in the presence of protease results in the release of peptide fragments with free aminoterminal groups. Evidence of protease activity is obtained by reaction of these peptides with trinitrobenzene sulfonic acid (TNBSA), followed by measurement of the absorbance increase that is due to the formation of yellow colored TNB-peptide adducts. A standard protease is provided, allowing you to determine the concentration of protease in samples undergoing analysis.

Our Fluorescent Protease Assay Kit is based on a FITC-labeled casein. This sensitive assay can be used in either FRET or FP modes.

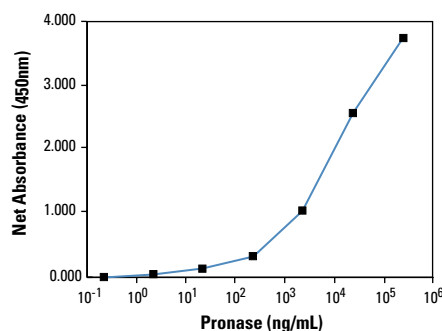

Sensitivity of the colorimetric Thermo Scientific Pierce Protease Assay.

Ordering Information

Product	Description	Pkg. Size
23263	Protease Assay Kit	Kit
	Sufficient material for 250 assays	
	Includes: Succinylated Casein (supplied as a lyophilized salt-free powder)	5 x 10mg
	2,4,6-Trinitrobenzene sulfonic acid (TNBSA)	2mL
	TPCK Trypsin standard (40 BAEE units/mg)	50mg
	BupH Borate Buffer Pack (makes 500mL)	1 pack
23266	Fluorescent Protease Assay Kit	Kit
	Sufficient material for at least 1,000 assays in a 96-well format.	
	Includes: FITC-Casein, Lyophilized	2.5mg
	TPCK Trypsin	50mg
	BupH Tris Buffered Saline	1 pack
23267	FITC-Casein	2.5mg (1,000 assays)

Reference

Rao, S.K., et al. (1997). *Anal. Biochem.* **250**(2), 222-227.

Specialty Assays – Glycoproteins

Glycoprotein Carbohydrate Estimation Kit

Direct approach to the estimation of carbohydrate content in proteins with Thermo Scientific Glycoprotein Carbohydrate Estimation Kit.



Highlights:

- Enables quick and easy identification of an unknown protein sample as a glycoprotein
- Estimates the percent carbohydrate content of a glycoprotein when run against a set of glycoprotein standards with known carbohydrate content
- Complementary to electrophoresis, Western blotting and ELISA-based procedures often used to detect glycoprotein
- Determines carbohydrate content in three easy steps: (1) oxidize, (2) react and (3) read
- Entire assay performed in less than 75 minutes
- All you need is this kit, a microplate and a plate reader to determine carbohydrate content


Ordering Information

Product	Description	Pkg. Size
23260	Glycoprotein Carbohydrate Estimation Kit Sufficient reagents for 250 microplate assays or 60 standard test tube assays. Includes: Sodium meta-Periodate Glycoprotein Detection Reagent Glycoprotein Assay Buffer Negative Controls: Lysozyme and BSA Positive Controls: Ovalbumin Apo-Transferrin Fetuin α_1 -Acid Glycoprotein	Kit 500mg 500mg 250mL 2.5mg each 2.5mg 2.5mg 0.25mg 0.25mg
23259	Fluorescent Protease Assay Kit Sufficient material for at least 1,000 assays in a 96-well format. Includes: Negative Controls: Lysozyme and BSA Positive Controls: Ovalbumin Apo-Transferrin Fetuin α_1 -Acid Glycoprotein	Set 2.5mg each 2.5mg 2.5mg 0.25mg 0.25mg
23262	Glycoprotein Detection Agent	1 g


Assay Principle

The protein sample under analysis is oxidized and reacted with the exclusive Glycoprotein Detection Reagent. The resulting colored complex is read at 550nm. From the absorbance of the resulting complex at 550nm the approximate percentage of carbohydrate in the glycoprotein under analysis can be estimated.


1. Add 50 μ L of protein standard or sample to each well.




2. Add 25 μ L of 10mM Sodium *meta*-Periodate in assay buffer.




3. Mix and incubate for 10 minutes at room temperature (RT).



4. Add 150 μ L of a 0.5% solution of Thermo Scientific Glycoprotein Detection Reagent in 1.0M NaOH.



5. Mix and incubate at RT for 60 minutes.



6. Read the plate in a microplate reader at 550nm. Interpolate the results of the unknown with the results of the standard proteins.



The Thermo Scientific Phosphoprotein Phosphate Estimation Assay microplate protocol.

Specialty Assays – Phosphoproteins

Phosphoprotein Phosphate Estimation Kit

Get some basic questions about your target protein answered without having to perform a Western blot.

The novel protein characterization tool, that gives today's protein analyst the ability to quickly and reliably determine whether a purified target protein is phosphorylated and, if so, the extent of phosphorylation compared to a phosphoprotein of known phosphorus content. This easy-to-perform assay is specific for estimating phosphoserine or phosphothreonine post-translational modifications and has been adapted to both a tube and convenient microplate format. The Thermo Scientific Phosphoprotein Phosphate Estimation Assay provides answers that a traditional Western blot simply cannot, and you can get answers about five times faster, too.

Unique advantage of the assay chemistry

The specificity of this assay toward seryl and threonyl phosphate ester modifications can indirectly "detect" a phosphotyrosine modification should the result of the assay be negative. A negative result on a pure protein preparation can suggest that the protein is not phosphorylated or that the protein is, in fact, phosphorylated, but modified by way of the tyrosyl side chains. Further Western blot analysis can verify which conclusion is correct.

In addition, the Phosphoprotein Phosphate Estimation Assay Kit can also be used to determine the amount of a purified known phosphoprotein in a sample. A standard curve can be constructed using a purified preparation of the known protein.


Highlights:

- Easy-to-prepare working reagent
- Colorimetric detection
- Use as qualitative or semi-quantitative assay
- Test tube or microplate assay option
- Estimate extent of phosphoserine/phosphothreonine modification
- Calculate the moles of phosphate (phosphorus) per mole of purified protein
- Use as quantitative assay for known pure phosphoproteins
- Results in about one hour
- Room temperature stability of kit components – saves refrigerator and freezer space


Assay Principle

The Phosphoprotein Phosphate Estimation Assay is based on the alkaline hydrolysis of phosphate from seryl and threonyl residues in phosphoprotein and the quantification of the released phosphate by the use of malachite green and ammonium molybdate.


3 parts Malachite Green Solution + 1 part Ammonium Molybdate Solution




1. Mix the Phosphate Reagent Working Solution.




2. Add 50µL of protein sample and diluted standards to each well.




3. Add 50µL of 2N NaOH per well. Mix the plate for 30 seconds.




4. Incubate in a 65°C incubator for 30 minutes.



5. Add 50µL of 4.7N HCl per well. Mix for 30 seconds.



6. Add 50µL of Phosphate Reagent per well. Mix for 30 seconds.



7. Incubate for 30 minutes at room temperature.



8. Read the plate in a microplate reader at 650nm. Plot the results of the unknown against the results of the standard protein provided. Calculate the approximate number of phosphorylation sites.

The Thermo Scientific Phosphoprotein Phosphate Estimation Assay microplate protocol.

Ordering Information

Product	Description	Pkg. Size
23270	Phosphoprotein Phosphate Estimation Kit Sufficient reagents for 20 x 96-well microplate assays or 500 test tube assays. Includes: Ammonium Molybdate Solution Malachite Green Solution Phosvitin Positive Control BupH Tris Buffered Saline	Kit 25mL 75mL 1mg 1 pack

Related Products

Product	Description	Pkg. Size
24550	GelCode® Phosphoprotein Staining Kit	Kit

Specialty Assays – Peroxidases

Quantitative Peroxide Assay Kits

Quickly measure peroxide contamination in various biological samples.

Highlights:

- Fast and easy to use
- Peroxidase independent
- No lipid extraction necessary
- Spectrophotometric analysis
- No heating required

Thermo Scientific Pierce Quantitative Peroxide Assays are the simplest assays for detecting the presence of peroxides in both aqueous and lipid-containing laboratory reagents. The basis of these assays is the complexing of ferric ion (Fe^{2+}) by H_2O_2 in the presence of xylenol orange. Peroxides in the sample oxidize Fe^{2+} to Fe^{3+} , and the Fe^{3+} will form a colored complex with xylenol orange that can be read at 560nm.

The presence of hydrogen peroxide (H_2O_2) can now be detected to monitor any peroxide contamination that may be harmful to biological samples. When performed on a routine basis, our Quantitative Peroxide Assay can prevent inadvertent introduction of peroxides into your valuable samples. If the effects of peroxide cannot be avoided in a particular system, these assays will help you assess the risk to your sample.

References

- Coutant, F., et al. (2002). *J. Immunol.* **169**, 688-1695.
Goyer, A., et al. (2002). *Eur. J. Biochem.* **269**, 272-282.
Requena, J. (2001). *Proc. Nat. Acad. Sci., U.S.A.* **98**, 69-74.

Comparison of Assay Protocols for Lipid Peroxide Content

Thermo Scientific Pierce Quantitative Peroxidase Assay

1. Mix one volume of Reagent A with 100 volumes of Reagent C to prepare Working Reagent.
2. Add 950 μL of Working Reagent to 50 μL of sample.
3. Incubate at room temperature for 30 minutes.
4. Read at 560nm (or 595nm for ELISA plate readers).

Total Time: 35 Minutes

Ordering Information

Product	Description	Pkg. Size
23280	Quantitative Peroxide Assay Kit <i>Aqueous compatible formulation.</i> Includes: Reagent A (25mM Ammonium Ferrous Sulfate) Reagent B (125 μM Xylenol Orange in water with Sorbitol)	Kit 2 x 50mL
23285	Quantitative Peroxide Assay Kit <i>Lipid-compatible formulation.</i> Includes: Reagent A (25mM Ammonium Ferrous Sulfate) Reagent B (125 μM Xylenol Orange in methanol with BHT)	Kit 4 x 25mL

Thiobarbituric Acid Assay

1. Mix 0.1mL sample, 0.4mL H_2O and 0.2mL 7% SDS.
2. Stir gently and add 2mL 0.1 N HCl.
3. Add 0.3mL 10% phosphotungstic acid.
4. Incubate 5 minutes at room temperature.
5. Add 1mL 0.67% thiobarbituric acid (TBA) and acetic acid.
6. Heat 45 minutes at 95°C.
7. Cool in ice bath.
8. Add 5mL butanol.
9. Vortex and centrifuge for 15 minutes.
10. Determine lipid peroxide concentration in butanol layer by fluorescence at 515nm excitation and 553nm emission.

Total Time: 80-90 Minute

Spectrophotometers

Thermo Scientific family of UV-visible spectrophotometers

For more information on the complete line of Thermo Scientific UV-visible Spectrophotometers, visit www.thermoscientific.com/uv-vis

BioMate 3S UV-Visible Spectrophotometer

Accurate and convenient life science measurements.



The Thermo Scientific BioMate 3S UV-Visible spectrophotometer is the ideal life science instrument providing exceptional performance at an affordable price. For your routine analysis, assays, or SOPs, count on the BioMate™ 3S system for accurate and reliable data. The xenon lamp provides fast, instant-on measurements with no warm-up time and is guaranteed for three years of continuous use. The efficient optical design delivers maximum performance with 1.8 nm bandwidth for optimal signal-to-noise performance.

Feature-rich and easy-to-use embedded software has advanced functionality for demanding samples, yet is simple and straightforward for routine analysis. Built-in life science methods are aligned with the most up-to-date protocols for protein and nucleic acid assays. Quantitative analysis, wavelength scanning, fixed wavelength measurements, kinetics, and other more advanced calculations are easy to setup and run. USB connectivity for data storage, printing and computer control makes the BioMate 3S spectrophotometer an excellent choice for a fast-paced laboratory environment.

Evolution 260 Bio UV-Visible Spectrophotometer

Performance and versatility to advance your research.




The innovative Thermo Scientific Evolution 260 Bio UV-Vis spectrophotometer will keep you ahead in the quickly changing life science research field. With the choice of integrated or computer software control, the Evolution™ 260 Bio system is always up-to-date and ready for the next challenge. Powerful software, a high-performance spectrophotometer, and an extensive line of accessories combine for a complete solution that helps to move you from samples to answers faster. Thermo Scientific INSIGHT software, included with the Evolution 260 Bio spectrophotometer, offers pre-programmed assay methods for increased accuracy and convenience.

Designed with research, routine analysis, and core laboratory facilities in mind, the Evolution 260 Bio instrument is at home in a multi-user laboratory or as a dedicated analyzer for research-level analysis. The Evolution 260 Bio is one instrument that can satisfy all the needs of your routine to research life science lab.

Evolution 300 UV-Visible Spectrophotometer

Superior performance for demanding applications.

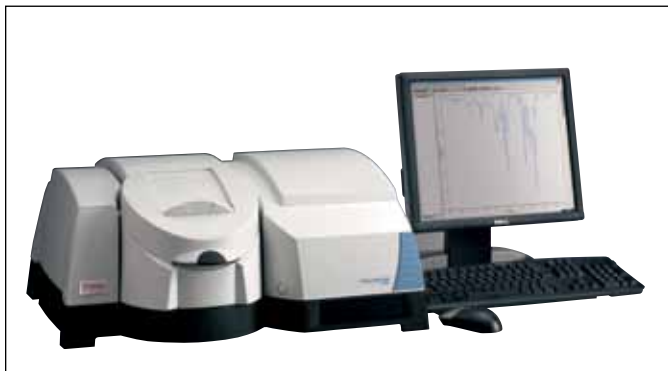

The Thermo Scientific Evolution 300 spectrophotometer is the natural fit for any multi-user, life-science research laboratory. From performing fast or routine assays, such as protein quantification, to performing more advanced studies, such as kinetics or thermal denaturation/renaturation assays, the Evolution™ 300 system offers the ideal configuration for your life science laboratory.

This high-performance, double-beam instrument features a long lifetime xenon lamp - eliminating the need to replace lamps. Powerful accessories and low cost of ownership make the Evolution 300 system a versatile and affordable addition to your research lab.

Evolution Array UV-Visible Spectrophotometer

Samples to answers in an instant.



Fast data acquisition and superb reliability make the Thermo Scientific Evolution Array spectrophotometer the cornerstone of your complete analytical environment. Instant full-spectrum analysis, room light immunity, and a complete line of accessories deliver simplicity and capability that is second to none. Photodiode array technology allows you to acquire full spectrum UV-visible data almost instantaneously for increased efficiency and throughput in the lab. Full spectrum data gives the most complete information for thermal denaturation and kinetics of protein interaction and structure analysis.

The Evolution Array system can be configured with a wide range of accessories for temperature control of samples and automation-making it one of the most powerful and versatile UV-Vis spectrophotometers on the market.

Protein Assay Selection Guide Poster

The updated Thermo Scientific Pierce Protein Assay Selection Guide Poster (Product # 1601652) measures 32 5/8" x 24 3/8" (~83 cm x 62 cm) and provides an overview of all of our protein assays, including the recently introduced BCA, Reducing Agent Compatible and Pierce 660nm Protein Assay. The poster outlines each protein assay's advantages, applications, standard assay protocol, precautions, reaction schemes, typical standard curves, detection range and interfering substance information. If your lab performs protein assays, you'll want to have this poster on your wall.




Protein Purification Technical Handbook

This 81-page handbook provides protocols and technical and product information to help maximize results for protein purification. It also includes background and troubleshooting advice for covalent coupling of affinity ligands to chromatography supports, avidin:biotin-binding, affinity purification of antibodies, IP and co-IP, affinity procedures for contaminant removal, and related procedures.




Electrophoresis Technical Handbook

This 44-page reference guide provides information to improve the speed, convenience and sensitivity of your protein gel electrophoresis and staining applications. The handbook covers all aspects of electrophoresis – from sample and gel preparation to choice of molecular weight markers. In addition, it contains an extensive section on protein gel-staining techniques and products.

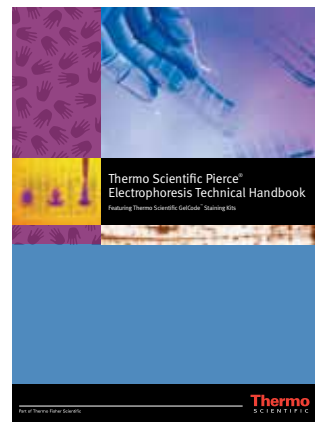

Cell Lysis Technical Handbook

This handbook provides protocols and technical and product information to help maximize results for Protein/Gene Expression studies. The handbook provides background, helpful hints and troubleshooting advice for cell lysis, protein purification, cell fractionation, protease inhibitors and protein refolding. The handbook is an essential resource for any laboratory studying Protein/ Gene Expression.

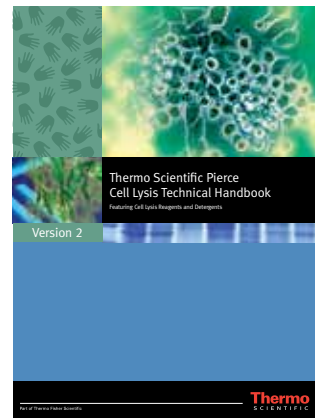

To request a copy of any of these pieces, visit www.thermoscientific.com/pierce or contact your local office or distributor.

Brij[®], Span[®] and Tween[®] are registered trademarks of ICI Americas.
Triton[®] is a registered trademark of Rohm & Haas.
Lubrol[®] is a registered trademark of Imperial Chemical Industries PLC.
Zwittergent[®] is a registered trademark of Calbiochem-Novabiochem Corp.
Cary[®] is a registered trademark of Varian Inc.
Tandem Mass Tag, TMT, TMTzero, TMTsixplex and TMTduplex are trademarks of Proteome Sciences plc.



Contact Information

**Belgium and Europe,
the Middle East
and Africa Distributors**
Tel: +32 53 85 71 84

France
Tel: 0 800 50 82 15

The Netherlands
Tel: 076 50 31 880

Germany
Tel: 0228 9125650

United Kingdom
Tel: 0800 252 185

Switzerland
Tel: 0800 56 31 40

Email: perbio.euromarketing@thermofisher.com
www.thermoscientific.com/perbio

United States
Tel: 815-968-0747 or 800-874-3723
Customer Assistance E-mail:
Pierce.CS@thermofisher.com
www.thermoscientific.com/pierce



© 2010 Thermo Fisher Scientific Inc. All rights reserved.
These products are supplied for laboratory or manufacturing
applications only. Unless indicated otherwise on the inside
back cover, all trademarks are property of Thermo Fisher
Scientific Inc. and its subsidiaries.

1602063 12/10 Printed in the U.S.

