



MDM300 Sampling System User's Manual



97232 Issue 1.4
October 2016

Please fill out the form(s) below for each instrument that has been purchased.

Use this information when contacting Michell Instruments for service purposes.

Instrument	
Code	
Serial Number	
Invoice Date	
Location of Instrument	
Tag No	

Instrument	
Code	
Serial Number	
Invoice Date	
Location of Instrument	
Tag No	

Instrument	
Code	
Serial Number	
Invoice Date	
Location of Instrument	
Tag No	



MDM300 Sampling System

For Michell Instruments' contact information please go to
www.michell.com

© 2016 Michell Instruments

This document is the property of Michell Instruments Ltd. and may not be copied or otherwise reproduced, communicated in any way to third parties, nor stored in any Data Processing System without the express written authorization of Michell Instruments Ltd.

Contents

Safety	v
Electrical Safety	v
Pressure Safety	v
Toxic Materials	v
Repair and Maintenance	v
Calibration	v
Safety Conformity	v
Abbreviations	vi
Warnings	vi
1 INTRODUCTION	1
2 INSTALLATION	2
2.1 Safety	2
2.2 Unpacking the Instrument	2
2.3 Environmental Requirements	2
2.4 Preparing the Sampling System for Operation	3
2.5 Controls, Indicators and Connectors	5
3 OPERATION	6
3.1 Sample Gas Connection	6
3.2 Operating Procedure	6
3.3 Sampling Hints	7
4 MAINTENANCE	10
4.1 General Maintenance Guidelines	10
4.2 Filter Element Replacement	10

Figures

<i>Figure 1</i>	<i>Panel-Mount Sampling System and Flight Case</i>	<i>1</i>
<i>Figure 2</i>	<i>Gas Port Adaptors</i>	<i>3</i>
<i>Figure 3</i>	<i>MDM300 Positioning</i>	<i>3</i>
<i>Figure 4</i>	<i>MDM300 Inlet and Outlet Port Connection</i>	<i>4</i>
<i>Figure 5</i>	<i>Mounting Posts</i>	<i>4</i>
<i>Figure 6</i>	<i>Port Connection Tightening</i>	<i>4</i>
<i>Figure 7</i>	<i>Controls, Indicators and Connectors</i>	<i>5</i>
<i>Figure 8</i>	<i>Sample Line Connection to GAS IN Port</i>	<i>6</i>
<i>Figure 9</i>	<i>Filter Element Removal</i>	<i>10</i>
<i>Figure 10</i>	<i>Glycol Absorption Cartridge Removal</i>	<i>11</i>

Tables

Table 1	Controls, Indicators and Connectors.....	5
---------	--	---

Appendices

Appendix A	Technical Specifications.....	13
Appendix B	Quality, Recycling & Warranty Information.....	15
	B.1 Pressure Equipment Directive (PED) 97/23/EC	15
	B.2 Recycling Policy	15
	B.3 WEEE Compliance.....	15
	B.4 RoHS2 Compliance	16
	B.5 Warranty.....	16
	B.6 REACH Compliance	17
	B.7 Calibration Facilities	17
	B.8 Return Policy	18
	B.9 Manufacturing Quality	18
Appendix C	Return Document & Decontamination Declaration.....	20

Safety

The manufacturer has designed this equipment to be safe when operated using the procedures detailed in this manual. The user must not use this equipment for any other purpose than that stated. Do not subject the equipment to conditions outside of the specified operating limits.

This manual contains operating and safety instructions, which must be followed to ensure the safe operation and to maintain the equipment in a safe condition. The safety instructions are either warnings or cautions issued to protect the user and the equipment from injury or damage. Use competent personnel using good engineering practice for all procedures in this manual.

Electrical Safety

The instrument is designed to be completely safe when used with options and accessories supplied by the manufacturer for use with the instrument.

Pressure Safety

DO NOT permit pressures greater than the safe working pressure to be applied to the instrument. The specified safe working pressure will be as follows (refer to Appendix A - Technical Specifications):

Low pressure:	20 barg (290 psig)
Medium pressure:	110 barg (1595 psig)
High pressure:	340 barg (4931 psig)



WARNING
The flowmeter should never be pressurized.
Always expand a pressurized sample to atmospheric pressure
before it enters the flow meter.

Toxic Materials

The use of hazardous materials in the construction of this instrument has been minimized. During normal operation it is not possible for the user to come into contact with any hazardous substance which might be employed in the construction of the instrument. Care should, however, be exercised during maintenance and the disposal of certain parts.

Repair and Maintenance

The instrument must be maintained either by the manufacturer or an accredited service agent. Refer to www.michell.com for details of Michell Instruments' worldwide offices contact information

Calibration

The recommended calibration interval for the MDM300 Hygrometer is 12 months. The instrument should be returned to the manufacturer, Michell Instruments, or one of their accredited service agents for recalibration.

Safety Conformity

This product meets the essential protection requirements of the relevant EU directives. Further details of applied standards may be found in the product specification.

Abbreviations

The following abbreviations are used in this manual:

AC	alternating current
barg	pressure unit (=100 kP or 0.987 atm) gauge
°C	degrees Celsius
°F	degrees Fahrenheit
NI/min	liters per minute
kg	kilogram(s)
lb	pound(s)
mm	millimeters
"	inch(es)
psig	pounds per square inch gauge
scfh	standard cubic feet per hour

Warnings

The following general warning listed below is applicable to this instrument. It is repeated in the text in the appropriate locations.



Where this hazard warning symbol appears in the following sections, it is used to indicate areas where potentially hazardous operations need to be carried out.

1 INTRODUCTION

The MDM300 panel-mount sampling system offers a complete package for conditioning of a sample, prior to measurement with an MDM300 or MDM300 I.S.

It is contained within an optional flight case which allows easy transport of everything required to make the measurements. The anti-static construction of the case makes it suitable for use in hazardous areas.



Figure 1 *Panel-Mount Sampling System and Flight Case*

2 INSTALLATION

2.1 Safety



It is essential that the installation of the electrical and gas supplies to this instrument be undertaken by qualified personnel.

2.2 Unpacking the Instrument

The shipping box will contain the following:

- MDM300 Panel-Mount Sampling System
 - Flight case (optional)
 - 2.5mm Allen key
 - 2 x 2.5mm hex bolts
 - 2 x 1/8" NPT to 1/8" Swagelok® adaptors
1. Open the box. If a flight case was ordered, the sampling system will be packaged within it.
 2. Remove the sampling panel (or flight case, if ordered) from the box, along with the fittings.
 3. Save all packing materials in case it is necessary to return the instrument.

2.3 Environmental Requirements

Refer to the user's manual for information on acceptable environmental conditions in which to operate the MDM300.

2.4 Preparing the Sampling System for Operation

To prepare the system for operation, it is necessary to install the MDM300 into the sampling system as follows:

- Wrap PTFE tape (not supplied), around the ends of the 1/8" NPT to 1/8" Swagelok® tube fittings and install into the orifice adaptors fitted to the MDM300. **Ensure that the orifice port adaptors in the MDM300 are both large bore type** (see relevant user's manual for more details).

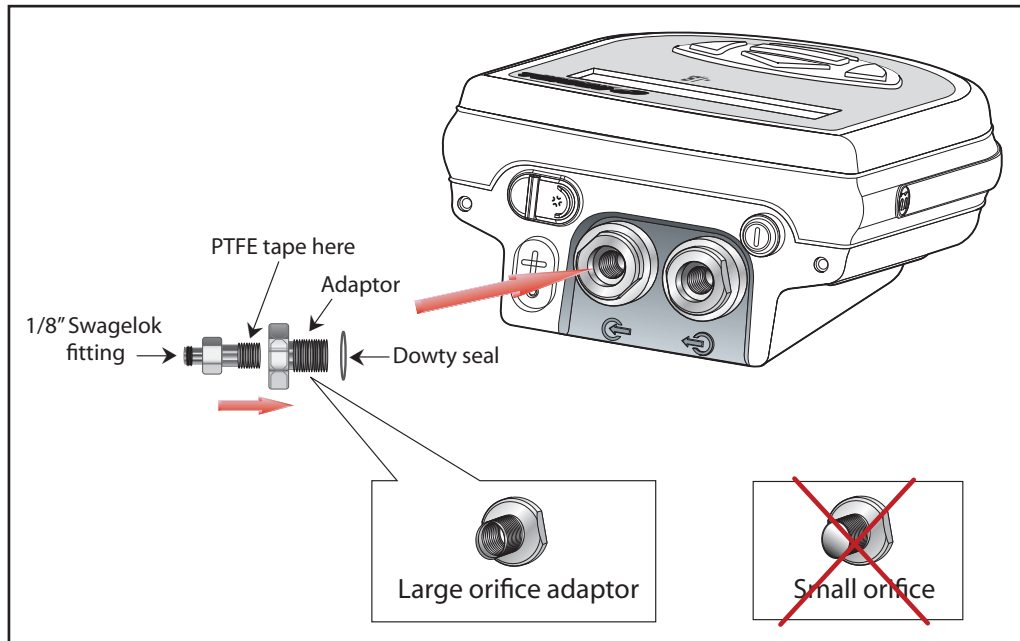


Figure 2 Gas Port Adaptors

- Locate the MDM300 in the position shown below.

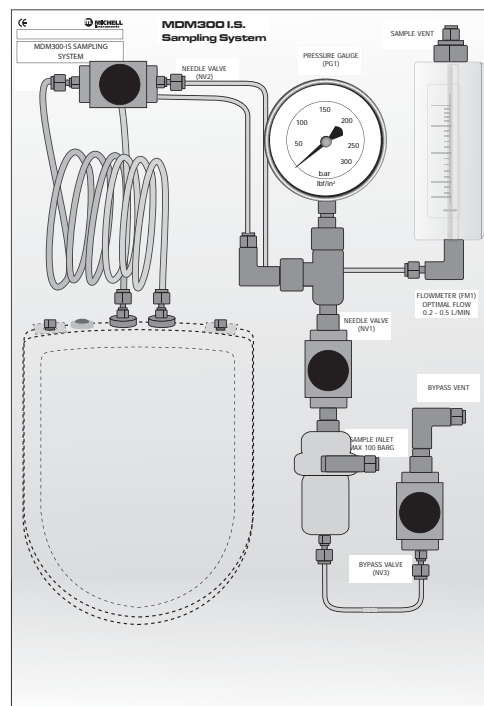


Figure 3 MDM300 Positioning

6. Connect the coiled tubes to the inlet and outlet of the MDM300. Ensure that the 1/8" Swagelok® nuts are finger tight.

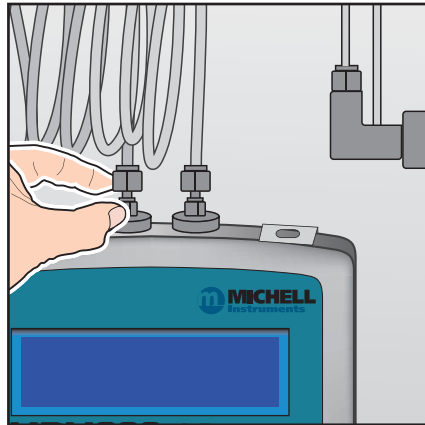


Figure 4 MDM300 Inlet and Outlet Port Connection

7. Secure the instrument to the mounting posts using the supplied 2.5mm hex bolts and allen key.

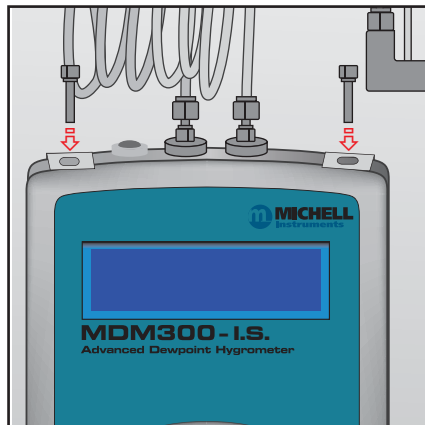


Figure 5 Mounting Posts

8. Use a wrench/spanner to finish tightening the 1/8" Swagelok® nuts on the inlet/outlet to ensure there are no leaks. The body of the 1/8" NPT to 1/8" Swagelok® adaptor should be held securely with another wrench/spanner while the nuts are tightened to prevent any movement.

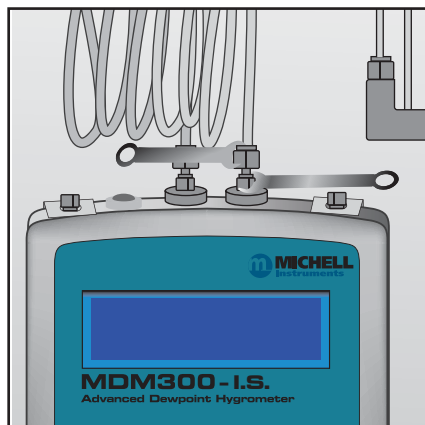


Figure 6 Port Connection Tightening

2.5 Controls, Indicators and Connectors

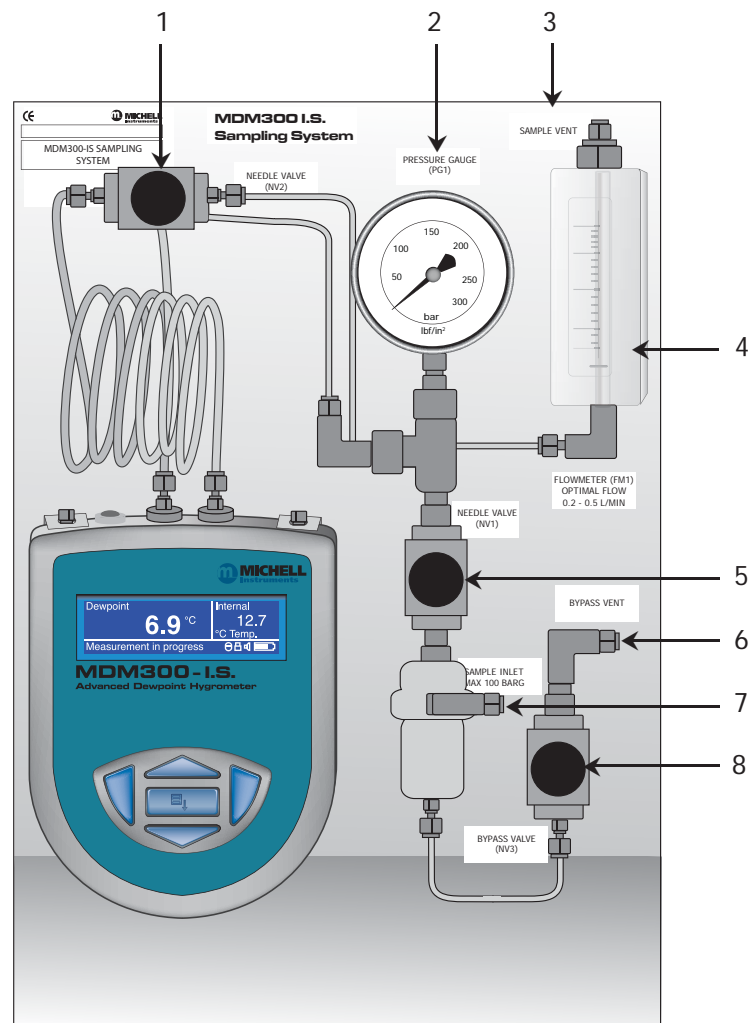


Figure 7 Controls, Indicators and Connectors

1	Outlet Metering Valve	Used to regulate sample flow for system pressure measurements Should be fully open for system pressure measurements
2	Pressure Gauge	Gauge showing the sample pressure across the sensor cell
3	Sample Vent	Fitted with either a silencer or Swagelok® tube fitting to enable a vent line to be connected
4	Flow Meter	For flow indication
5	Inlet Metering Valve	Used to regulate sample flow for atmospheric pressure measurements Should be fully open for system pressure measurements
6	Bypass Port	Outlet from the bypass path Can optionally be connected to a vent line during operation
7	Sample Inlet	For connection to the sample gas line Refer to Section 3.1 for more information on making connections to the system
8	Bypass Metering Valve	Used for regulating the flow rate through the bypass path

Table 1 Controls, Indicators and Connectors

3 OPERATION

3.1 Sample Gas Connection

Gas is introduced to the system by connecting the sample take-off line to the GAS IN port, as shown in *Figure 8*.

If required, connect a vent line to the BYPASS port, and to the flowmeter vent (if fitted).

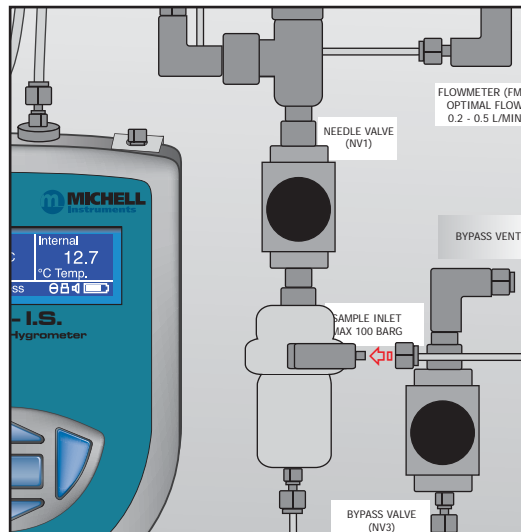


Figure 8 Sample Line Connection to GAS IN Port


3.2 Operating Procedure

1. Connect an instrument to the sample gas as detailed in Section 3.1.
2. Fully open the isolation valve.
3. Refer to the Operation Guide section in the relevant MDM300 user's manual for condition specific instructions on operation.
4. Depending on the sample pressure it may be necessary to use the bypass flow control to overcome sample flow control difficulties.

3.3 Sampling Hints

Measurement of moisture content is a complex subject, but does not need to be difficult. This section aims to explain the common mistakes made in measurement situations, the causes of the problem, and how to avoid them. Mistakes and bad practices can cause the measurement to vary from the expectation; therefore a good sampling technique is crucial for accurate and reliable results.

Transpiration and Sampling Materials

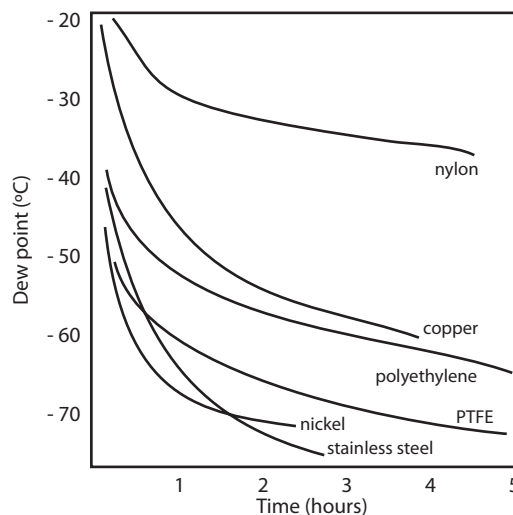

All materials are permeable to water vapor, as the water molecule is extremely small compared to the structure of solids, even when compared to the crystalline structure of metals. The graph to the right shows the dew point inside tubing of different materials when purged with very dry gas, where the exterior of the tubing is in the ambient environment.

Many materials contain moisture as part of their structure, particularly organic materials (natural or synthetic), salts (or anything which contains them) and anything which has small pores. It is important to ensure that the materials used are suitable for the application.

If the partial water vapor pressure exerted on the outside of a compressed air line is higher than on the inside, the atmospheric water vapor will naturally push through the porous medium causing water to migrate into the pressurized air line. This effect is called transpiration.

Adsorption and Desorption

Adsorption is the adhesion of atoms, ions, or molecules from a gas, liquid, or dissolved solid to the surface of a material, creating a film. The rate of adsorption is increased at higher pressures and lower temperatures.

Desorption is the release of a substance from or through the surface of a material. In constant environmental conditions, an adsorbed substance will remain on a surface almost indefinitely. However, as the temperature rises, so does the likelihood of desorption occurring.

In practical terms, as the temperature of the environment fluctuates, water molecules are adsorbed and desorbed from the internal surfaces of the sample tubing, causing small fluctuations in the measured dew point.

Sample Tubing Length

The sample point should always be as close to the critical measurement point as possible, in order to obtain a truly representative measurement. The length of the sample line to the sensor or instrument should be as short as possible. Interconnection points and valves trap moisture, so using the simplest sampling arrangement possible will reduce the time it takes for the sample system to dry out when purged with dry gas.

Over a long tubing run, water will inevitably migrate into any line, and the effects of adsorption and desorption will become more apparent. It is clear from the graph shown above that the best materials to resist transpiration are stainless steel and PTFE.

Trapped Moisture


Dead volumes (areas which are not in a direct flow path) in sample lines, hold onto water molecules which are slowly released into the passing gas; this results in increased purge and response times, and wetter than expected readings. Hygroscopic materials in filters, valves (e.g. rubber from pressure regulators) or any other parts of the system can also trap moisture.

Sample Conditioning

Sample conditioning is often necessary to avoid exposure of sensitive measuring components to liquids and other contaminants which may cause damage or affect the accuracy over time, depending on the measurement technology.

Particulate filters are used for removing dirt, rust, scale and any other solids that may be in a sample stream. For protection against liquids, a coalescing filter should be used. The membrane filter is a more expensive but highly effective alternative to a coalescing filter. It provides protection from liquid droplets, and can even stop flow to the analyzer completely when a large slug of liquid is encountered.

Condensation and Leaks

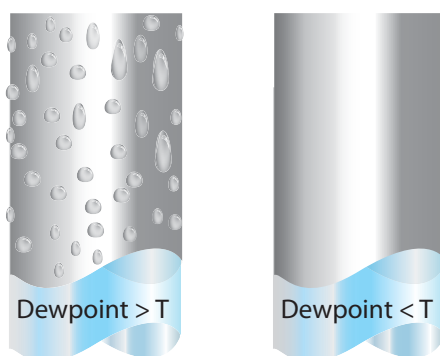

Maintaining the temperature of the sample system tubing above the dew point of the sample is vital to prevent condensation. Any condensation invalidates the sampling process as it changes the water vapor content of the gas being measured. Condensed liquid can alter the humidity elsewhere by dripping or running to other locations where it may re-evaporate.

The integrity of all connections is also an important consideration, especially when sampling low dew points at an elevated pressure. If a small leak occurs in a high pressure line, gas will leak out but vortices at the leak point and a negative vapor pressure differential will also allow water vapor to contaminate the flow.

Flow Rates

Theoretically flow rate has no direct effect on the measured moisture content, but in practice it can have unanticipated effects on response speed and accuracy. The optimal flow rate varies depending on the measurement technology.

MDM300 I.S. flow rate	0.2 to 0.5 NI/min (0.5 to 1 scfh)
MDM300 flow rate	0.2 to 1.2 NI/min (0.5 to 1.2 scfh)



WARNING
The flowmeter should never be pressurized.
Always expand a pressurized sample to atmospheric pressure before it enters the flow meter.

An inadequate flow rate can:

- Accentuate adsorption and desorption effects on the gas passing through the sampling system.
- Allow pockets of wet gas to remain undisturbed in a complex sampling system, which will then gradually be released into the sample flow.
- Increase the chance of contamination from back diffusion: ambient air that is wetter than the sample can flow from the exhaust back into the system. A longer exhaust (sometimes called a pigtail) can also help alleviate this problem.

An excessively high flow rate can:

- Introduce back pressure, causing slower response times and unpredictable effects on equipment such as humidity generators.
- Result in a reduction in heating capabilities of the sensor tile during the initialization period. This is most apparent with gases that have a high thermal conductivity such as hydrogen and helium.

4 MAINTENANCE

4.1 General Maintenance Guidelines

Routine maintenance of the system is confined to filter element replacement and regular recalibration of the MDM300 or MDM300 I.S. sensor. For specific details on replacing filter elements, please see Section 4.2.

In most applications, annual recalibration ensures that the stated accuracy of the MDM300 Advanced Dew-Point Hygrometer is maintained. The exchange sensor scheme is the most efficient method of providing accurate annual recalibration with minimum downtime.

Please contact Michell Instruments for more details.

Prior to recalibration being necessary, an exchange sensor can be ordered from Michell Instruments or any authorized dealer. Once the sensor and calibration certificate has been received it can be fitted and the original sensor returned to Michell Instruments.

For more details of recalibration of the MDM300 please see the relevant user's manual.

4.2 Filter Element Replacement

Frequency of filter element replacement is primarily dependent upon the quantity of contaminants present in the sample gas. If the gas is heavily laden with particulates or liquids it is recommended to inspect the filter element on a regular basis initially, and increase the time between inspections if the filter is found to be in good condition.

It is imperative that all filters are replaced before they become saturated. If a filter element becomes saturated with contaminants there is a possibility that the performance of the filter will be reduced, and contamination of the MDM300 sensor could occur.



Before attempting to replace the filter always disconnect the Sampling System from the sample gas and ensure that the system is depressurized.

To replace a particulate or coalescing filter element, proceed as follows:

1. Disconnect the U-shaped section of Swagelok® tubing from the filter drain.

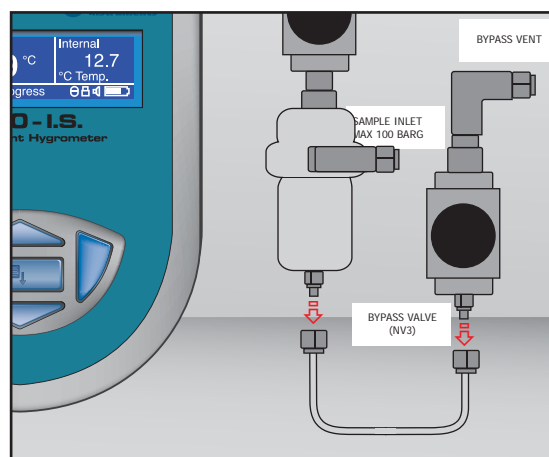


Figure 9 Filter Element Removal

2. Unscrew and remove the filter bowl and then the filter element. **NOTE: the filter bowl is sealed with an O-ring.**
3. Discard the old used filter element and replace with a new filter element

Order codes:

MDM300-SAM-PAR - particulate element

MDM300-SAM-COA - coalescing element

4. Replace the filter bowl, ensuring the O-ring is correctly seated and reconnect the tube to the drain port. **NOTE: Tighten both securely.**

To replace the glycol absorption cartridge, proceed as follows:

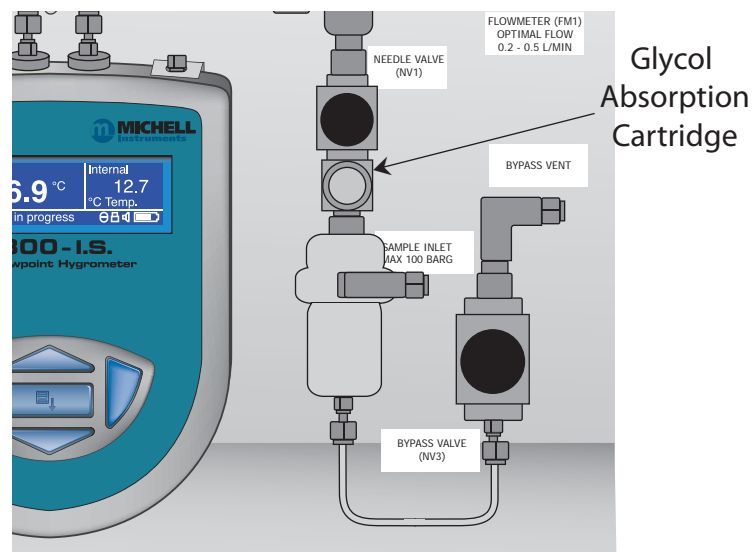


Figure 10 Glycol Absorption Cartridge Removal

1. Loosen union bonnet nut with open end spanner/wrench. Support body to minimize strain on pipe or tubing.
2. Unscrew union nut and remove assembly. **NOTE: Union nut, bonnet, spring and retaining ring remain together as an assembly.**
3. Gently tap filter element on side to break loose from tapered seating area.
4. Insert new glycol absorption cartridge. Tap lightly to reseat in tapered bore.

Order code: MDM300-SAM-PNL-GLY

5. Inspect gasket and mating surfaces on bonnet and body. Clean as required. Replacement of the gasket is recommended.

Appendix A

Technical Specifications

Appendix A Technical Specifications

Enclosure	
Dimensions	300 x 400 x 150mm (11.81 x 15.75 x 5.91") (w x h x d)
Materials	ABS (anti-static)
Ingress Protection	IP67 / NEMA4
Sampling System	
Pressure Range	Low pressure: 20 barg (290 psig) Medium pressure: 110 barg (1595 psig) High pressure: 340 barg (4931 psig)
Flow Rate	MDM300 0.2 to 1.2 NI/min (0.4 to 2.54 scfh) MDM300 I.S. 0.2 to 0.5 NI/min (0.4 to 1.1 scfh)
Gas Wetted Materials	316 stainless steel
Gas Connections	Depending on model: Legris quick release - accepts 6mm O/D PTFE (LOW PRESSURE VERSION ONLY) 1/8" Swagelok® 6mm Swagelok®
Components	
Valves	Inlet isolation valve, 2 x sample flow control valves, Bypass flow control valve
Filtration	Options of: Particulate Coalescing Coalescing + Mini Glysob
Pressure Gauge	Depending on model: Low pressure: 0 to 25 barg (0 to 362 psig) Medium pressure: 0 to 137 barg (0 to 1987 psig) High pressure: 0 to 413 barg (0 to 5990 psig)
Vent	Atmospheric pressure only - DO NOT pressurize vent Options of: Silencer 1/8" Swagelok® 6mm Swagelok®

Appendix B

Quality, Recycling & Warranty Information

Appendix B Quality, Recycling & Warranty Information

B.1 Pressure Equipment Directive (PED) 97/23/EC

The above Directive has been implemented in United Kingdom Law by the Pressure Equipment Regulations 1999.

The Regulations require that all pressure equipment and assemblies within the scope of the Pressure Equipment Directive must be safe when placed on the market or put into service.

Michell Instruments' products have been assessed and, as referenced against the Classification Charts detailed in Annex II of the Directive, do not fall into the requirements for CE marking compliance with the Pressure Equipment Directive.

Article 3, paragraph 3 states that any product containing a pressurized fluid that does not qualify for compliance should, nevertheless, be constructed with Sound Engineering Practice (SEP).

Michell Instruments attests here that its products have been designed, manufactured & tested to assure safe operation, and in accordance with Sound Engineering Practices.

B.2 Recycling Policy



Michell Instruments is concerned with the protection of the environment. It is our commitment to reduce and eliminate from our operations, wherever possible, the use of substances which may be harmful to the environment. Similarly, we are increasingly using recyclable and/or recycled material in our business and products wherever it is practical to do so.

To protect natural resources and to promote material reuse, please separate batteries from other types of waste and recycle responsibly. If batteries are not properly disposed of, these substances can cause harm to human health and the environment.

The product that you have purchased may contain recyclable and/or recycled parts and we will be happy to provide you with information on these components if required. For further information please see the following sections.

B.3 WEEE Compliance

Directive 2012/19/EU 4 July 2012 on Waste Electronic and Electrical Equipment (WEEE)

The Waste Electronic and Electrical Equipment (WEEE) Directive places rules upon European manufacturers of electrical and electronic equipment. The directives' aim is to reduce the impact that electronic devices have on the environment.

Michell Instruments is in full compliance with the WEEE Directive and is registered with an approved recycler (Registration No. WEE/JB0235YW) and treats the requirement of the directive and the protection of the environment with the utmost importance. All Michell Instruments' products are appropriately marked indicating their requirement for recycling.

It may be required to return certain instruments for treatment at the end of their working life.

Feb 2013

B.4 RoHS2 Compliance

Directive 2011/65/EU of the European Parliament and of the Council of 8 June 2011

The Restriction of Hazardous Substances (RoHS) Directive places rules upon European manufacturers of electrical and electronic equipment. The directives' aim is to reduce the impact that electronic devices have on the environment.

According to the EC Directive 2002/95/EC, Michell Instruments' products qualify as Category 9, Control and Monitoring Equipment. Under the 2002/95/EC Directive, Category 9 products are exempt from compliance with the Directive.

However, the careful design of all Michell Instruments' products takes into consideration the requirements of the Directive and, wherever possible, compliance is achieved. All future products will be developed entirely using compliant materials. Furthermore, Michell Instruments is taking active steps to remove non-compliant materials and components from existing products wherever these may occur. Presently, none of the non-compliant materials are known to occur in Michell Instruments' products.

The new Directive 2011/65/EU (RoHS2) entered into force on 21 July 2011 and required all Member States to transpose the provisions into their respective national laws by 2 January 2013.

Under the provisions of the RoHS2 EU Directive 2011/65/EU (Article 3, [24]) defines 'Control and Monitoring Equipment' specifically as 'monitoring and control instruments designed exclusively for industrial or professional use'.

RoHS2 EU Directive 2011/65/EU states the closing date for compliance of any Control and Monitoring Equipment product sold into the EU market place as 22nd July 2017.

However, the careful design policy of all Michell Instruments' products continues to attain compliance in the shortest practical timescales and strives to ensure that less than 0.1% of total mass per product, of all non-compliant materials, appear within them. Michell Instruments continues to monitor suppliers and material sources to ensure that compliance of goods provided is maintained.

January 2013

B.5 Warranty

Unless otherwise agreed, the Supplier warrants that, as from the date of delivery for a period of 12 months, the goods and all their component parts, where applicable, are free from any defects in design, workmanship, construction or materials.

The Supplier warrants that the services undertaken shall be performed using reasonable skill and care, and be of a quality conforming to generally accepted industry standards and practices.

Except as expressly stated, all warranties whether express or implied, by operation of law or otherwise, are hereby excluded in relation to the goods and services to be provided by the Supplier.

All warranty services are provided on a return to base basis. Any transportation costs for the return of a warranty claim shall reside with the Customer.

B.6 REACH Compliance

Regulation (EC) No. 1907/2006

Registration, Evaluation, Authorisation and Restriction of Chemicals (REACH)

Michell Instruments is a manufacturer of moisture measurement and gas analysis instrumentation and is a 'downstream' user of chemicals, as described by the EU Council Directive 76/769/EEC. The products we supply are not raw chemical products (goods).

Under normal and reasonably foreseeable circumstances of application, the goods supplied to you shall not contain or release any prohibited chemicals. No listed SVHC (Substances of Very High Concern) appear within products manufactured by Michell Instruments. Therefore the 0.1% mass per product, or total usage of 1 tonne/year, will never be exceeded. For these reasons we are neither required by obligation for registration nor for the creation of material safety data sheets (MSDS) for our products.

Our continued review of the SVHC Candidate List and latest additions is to ensure we remain compliant.

Michell Instruments maintains a hazardous material register in which MSDS data sheets are collated, and we will check that our suppliers will comply to REACH requirements for all materials and substances we use in the processes of our manufacturing.

In the unlikely event that any chemicals of concern appear in our products in quantities greater than 0.1% of total mass per product we will immediately inform you by correspondence according to the REACH Article 33 requirements. Our current appraisal is, however, that we do not expect or foresee such an incidence.

January 2013

B.7 Calibration Facilities

Michell Instruments' calibration facilities are among the most sophisticated in the world and have been recognized for their excellence.

Traceability to the National Physical Laboratory (NPL) UK is achieved through our UKAS Accreditation (Number 0179). This covers dew point over the range -90 to +90°C (-130 to +194°F) and also Relative Humidity.

Dew-point calibrations are also traceable to the National Institute for Standards & Technology (NIST) USA over the range -75 to +20°C (-103 to +68°F).

NOTE: Standard traceable calibration certificates for instruments and sensors are not issued under our UKAS accreditation. UKAS certificates are usually to special order and are clearly identified.

B.8 Return Policy

If a Michell Instruments' product malfunctions within the warranty period, the following procedure must be completed:

1. Notify a Michell Instruments' distributor, giving full details of the problem, the model variant and the serial number of the product.
2. If the nature of the problem indicates the need for factory service then the instrument should be returned to Michell Instruments, carriage prepaid, preferably in the original packaging, with a full description of the fault and the customer contact information.
3. Upon receipt, Michell Instruments will evaluate the product to determine the cause of the malfunction. Then, one of the following courses of action will be taken:
 - If the fault is covered under the terms of the warranty, the instrument will be repaired at no cost to the owner and returned.
 - If Michell Instruments determines that the fault is not covered under the terms of the warranty, or if the warranty has expired, an estimate for the cost of the repairs, at standard rates, will be provided. Upon receipt of the owner's approval to proceed, the product will be repaired and returned.

B.9 Manufacturing Quality

Michell Instruments is registered with the British Standards Institute for Quality Assurance to:

BS EN ISO 9001: 2008

Rigorous procedures are performed at every stage of production to ensure that the materials of construction, manufacturing, calibration and final test procedures meet the requirements laid down by our BSI approved Quality System.

Please contact Michell Instruments (www.michell.com) if the product does not arrive in perfect working order.

Appendix C

Return Document & Decontamination Declaration

Appendix C Return Document & Decontamination Declaration

Decontamination Certificate

IMPORTANT NOTE: Please complete this form prior to this instrument, or any components, leaving your site and being returned to us, or, where applicable, prior to any work being carried out by a Michell engineer at your site.

Instrument			Serial Number	
Warranty Repair?	YES	NO	Original PO #	
Company Name			Contact Name	
Address				
Telephone #			E-mail address	
Reason for Return /Description of Fault:				
Has this equipment been exposed (internally or externally) to any of the following? Please circle (YES/NO) as applicable and provide details below				
Biohazards			YES	NO
Biological agents			YES	NO
Hazardous chemicals			YES	NO
Radioactive substances			YES	NO
Other hazards			YES	NO
Please provide details of any hazardous materials used with this equipment as indicated above (use continuation sheet if necessary)				
Your method of cleaning/decontamination				
Has the equipment been cleaned and decontaminated?			YES	NOT NECESSARY
Michell Instruments will not accept instruments that have been exposed to toxins, radio-activity or bio-hazardous materials. For most applications involving solvents, acidic, basic, flammable or toxic gases a simple purge with dry gas (dew point <-30°C) over 24 hours should be sufficient to decontaminate the unit prior to return. Work will not be carried out on any unit that does not have a completed decontamination declaration.				
Decontamination Declaration				
I declare that the information above is true and complete to the best of my knowledge, and it is safe for Michell personnel to service or repair the returned instrument.				
Name (Print)			Position	
Signature			Date	



<http://www.michell.com>